

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082021\
 Data File : PP038759.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Aug 2021 22:56
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 02:31:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 18 04:51:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.883	3.868	948533	596573	23.503	24.894
2)	SA Decachlor...	10.867	9.127	635999	621953	25.850	25.536
Target Compounds							
20)	L4 AR-1242-5	7.174	6.001f	17085	26847	23.896	43.369 #
24)	L5 AR-1248-4	7.119f	0.000	143676	0	116.350	N.D. #
25)	L5 AR-1248-5	7.174	6.001f	17085	26847	13.973	29.735 #
26)	L6 AR-1254-1	7.119	6.001f	143676	26847	125.919	20.443 #
28)	L6 AR-1254-3	7.744f	0.000	94076	0	52.406	N.D. #
29)	L6 AR-1254-4	8.014	0.000	29872	0	23.151	N.D. #
32)	L7 AR-1260-2	8.159	0.000	9951	0	6.782	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082021\
Data File : PP038759.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Aug 2021 22:56
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 02:31:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 18 04:51:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

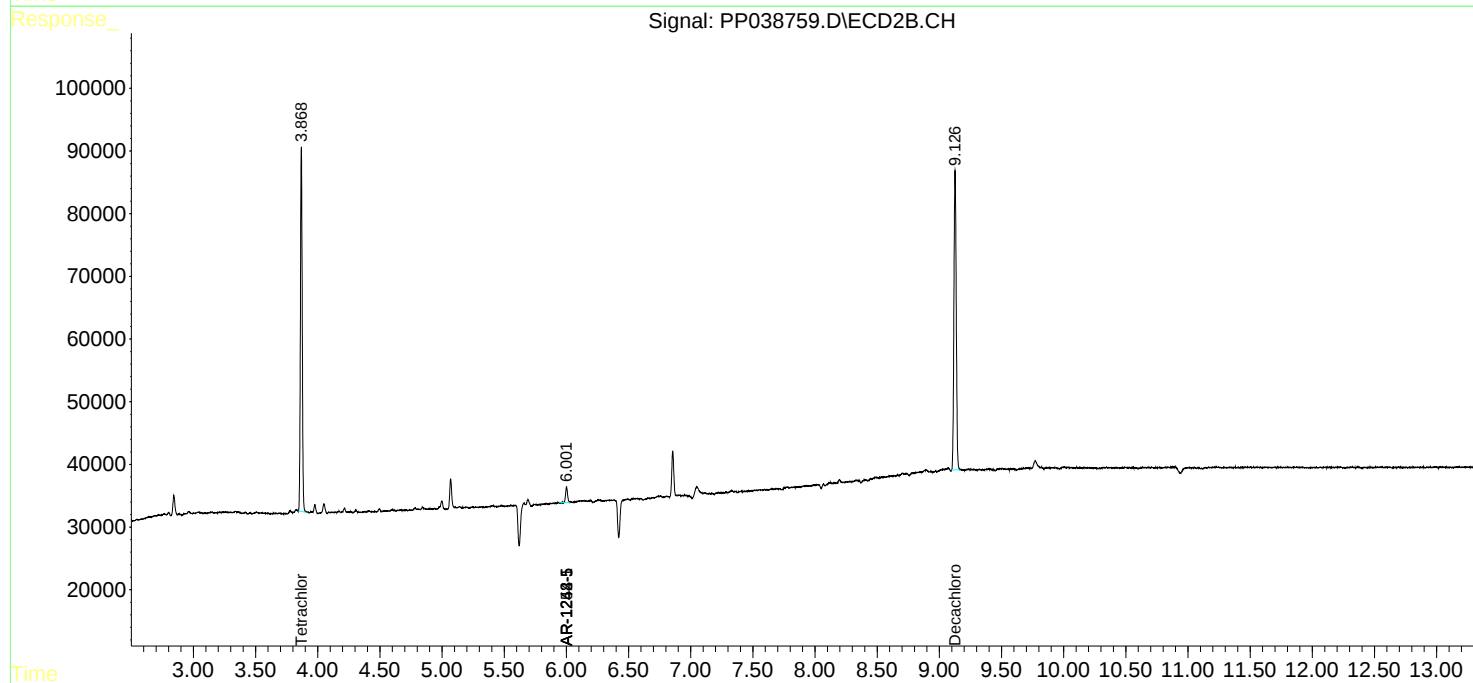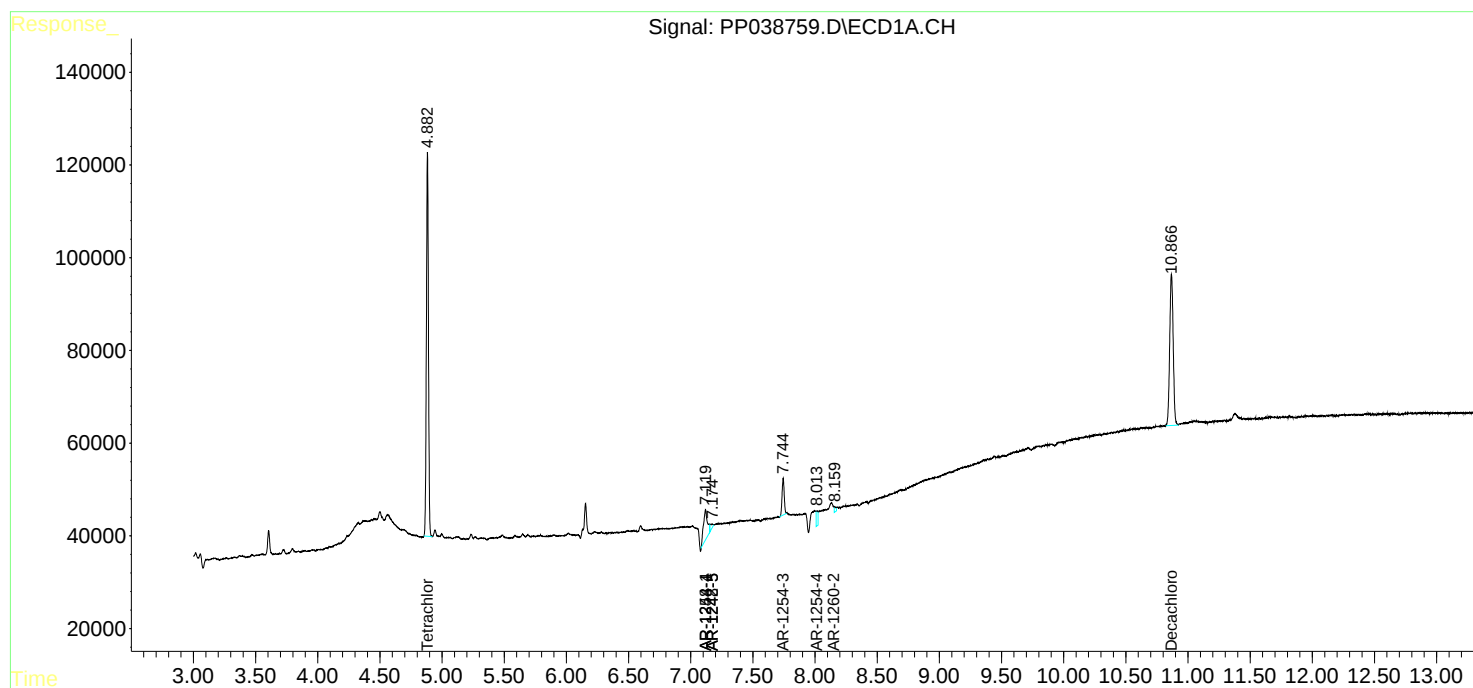


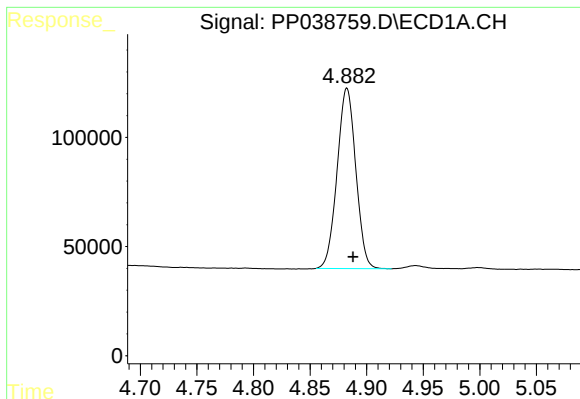

#1 Tetrachloro-m-xylene


R.T.: 4.883 min
Delta R.T.: -0.005 min
Response: 948533
Conc: 23.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

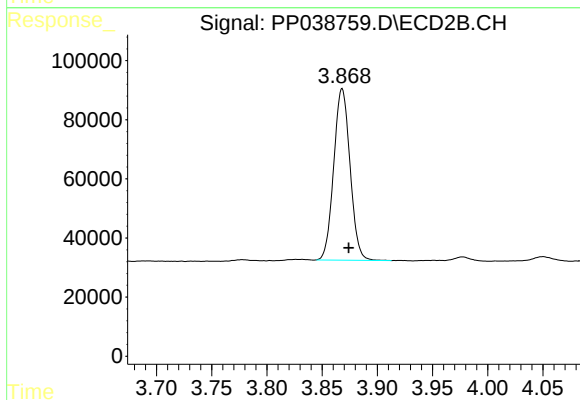


#1 Tetrachloro-m-xylene

R.T.: 3.868 min
Delta R.T.: -0.006 min
Response: 596573
Conc: 24.89 ng/ml

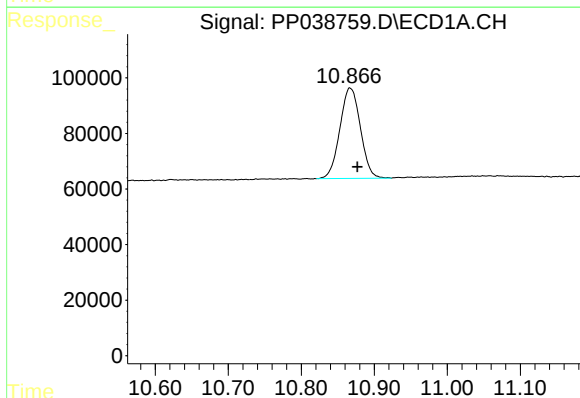


#2 Decachlorobiphenyl

R.T.: 10.867 min
Delta R.T.: -0.010 min
Response: 635999
Conc: 25.85 ng/ml

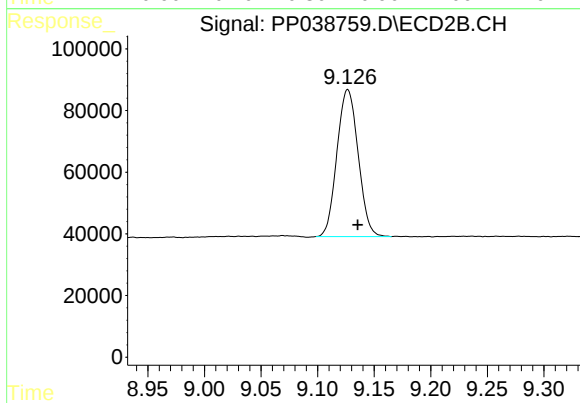

#2 Decachlorobiphenyl


R.T.: 9.127 min
Delta R.T.: -0.009 min
Response: 621953
Conc: 25.54 ng/ml

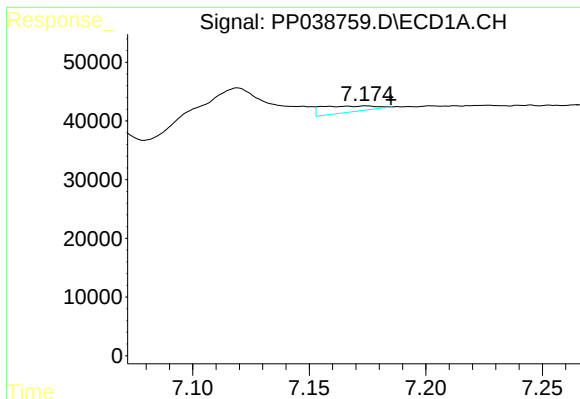

#20 AR-1242-5


R.T.: 7.174 min
Delta R.T.: -0.011 min
Response: 17085
Conc: 23.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

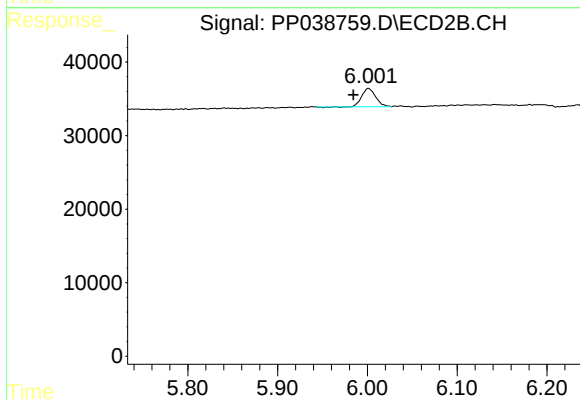


#20 AR-1242-5

R.T.: 6.001 min
Delta R.T.: 0.017 min
Response: 26847
Conc: 43.37 ng/ml

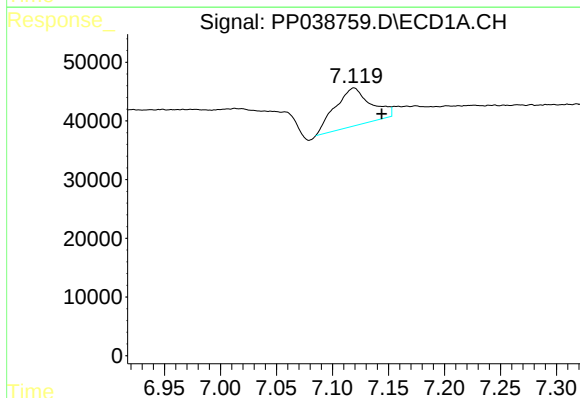


#24 AR-1248-4

R.T.: 7.119 min
Delta R.T.: -0.025 min
Response: 143676
Conc: 116.35 ng/ml

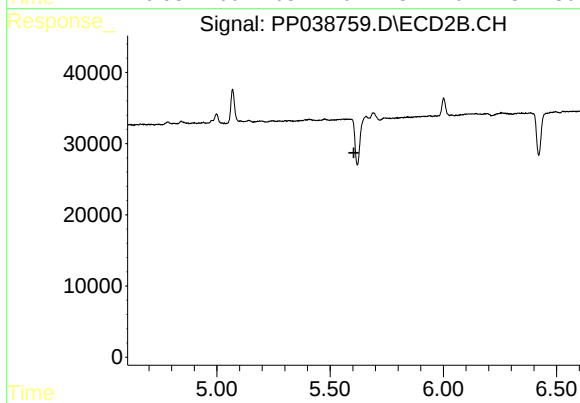

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.605 min
Response: 0
Conc: N.D.

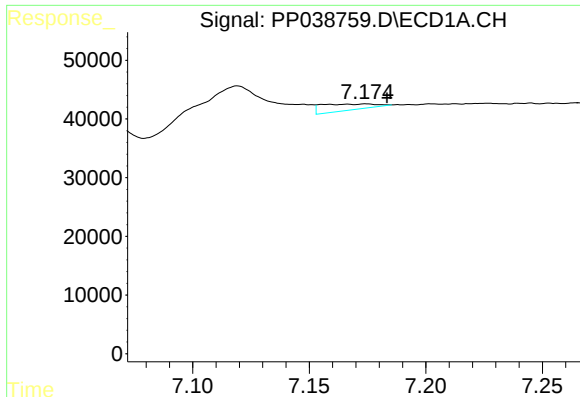

#25 AR-1248-5


R.T.: 7.174 min
Delta R.T.: -0.009 min
Response: 17085
Conc: 13.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

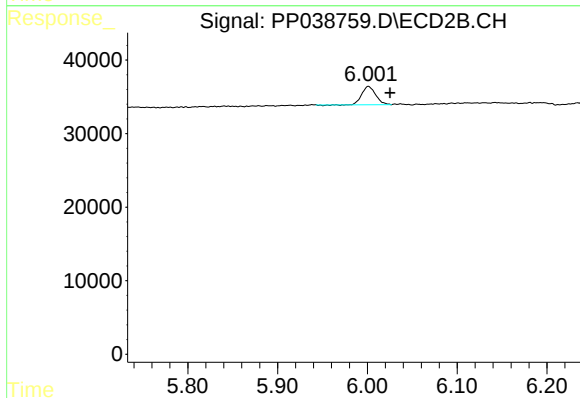


#25 AR-1248-5

R.T.: 6.001 min
Delta R.T.: -0.024 min
Response: 26847
Conc: 29.73 ng/ml

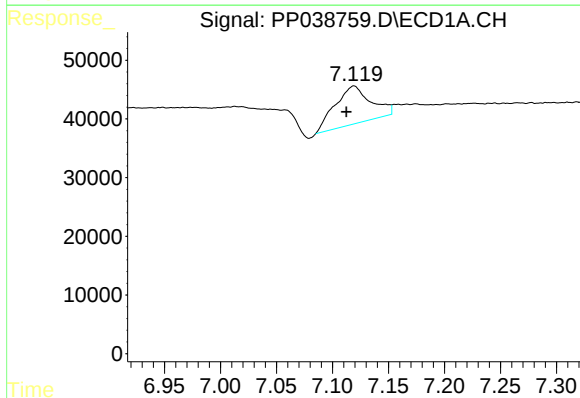


#26 AR-1254-1

R.T.: 7.119 min
Delta R.T.: 0.007 min
Response: 143676
Conc: 125.92 ng/ml

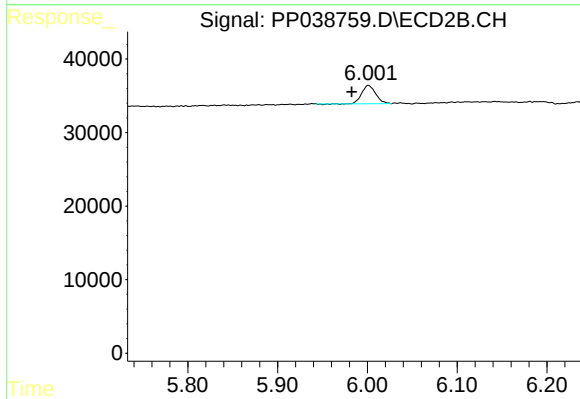

#26 AR-1254-1


R.T.: 6.001 min
Delta R.T.: 0.019 min
Response: 26847
Conc: 20.44 ng/ml

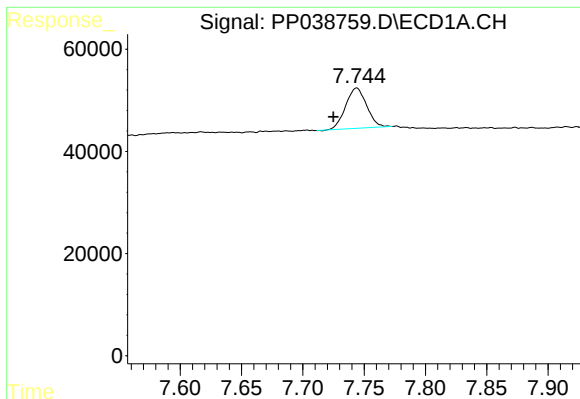

#28 AR-1254-3


R.T.: 7.744 min
Delta R.T.: 0.019 min
Response: 94076
Conc: 52.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

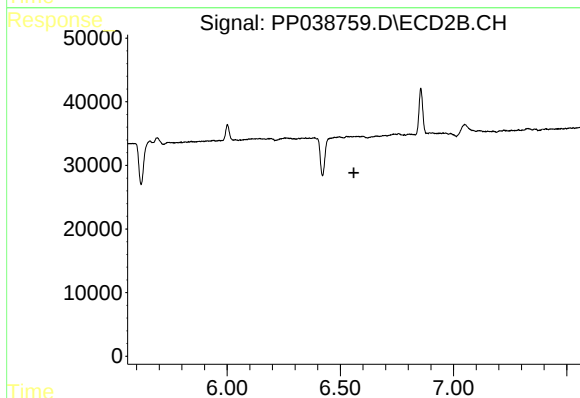


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.560 min
Response: 0
Conc: N.D.

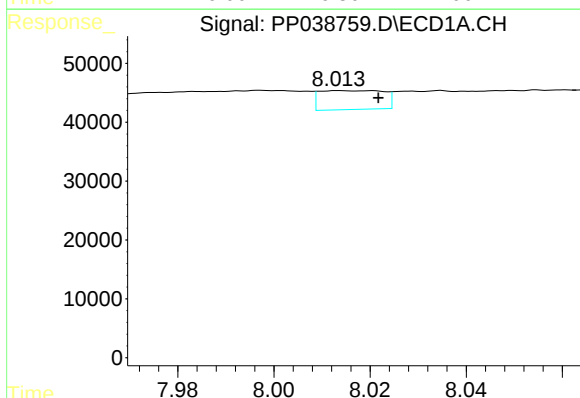


#29 AR-1254-4

R.T.: 8.014 min
Delta R.T.: -0.008 min
Response: 29872
Conc: 23.15 ng/ml

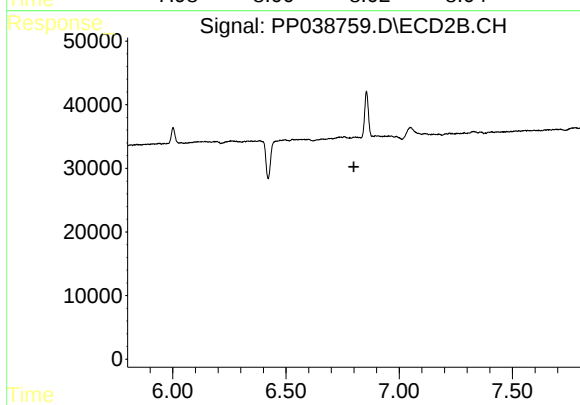

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.800 min
Response: 0
Conc: N.D.

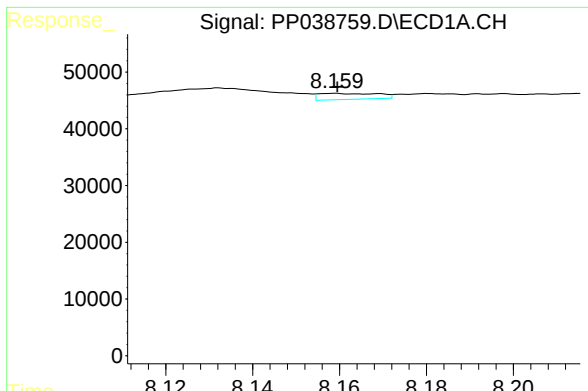

#32 AR-1260-2

R.T.: 8.159 min
Delta R.T.: 0.000 min
Response: 9951
Conc: 6.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

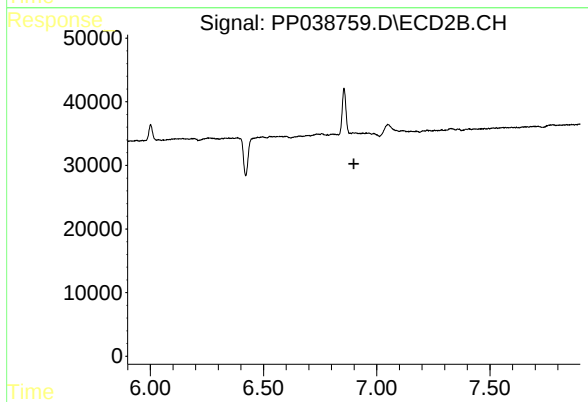

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.899 min
Response: 0
Conc: N.D.