

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082021\
 Data File : PP038746.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Aug 2021 19:15
 Operator : AJ\MA
 Sample : M3467-13
 Misc :
 ALS Vial : 83 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SAMPLE-2-(161.00)

Manual Integrations
 APPROVED

mohammad
 8/23/2021 2:21:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 05:48:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 18 04:51:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.883	3.869	938188	589389	23.247	24.595
2) SA Decachlor...	10.869	9.128	503717	497407	20.473m	20.423m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082021\
Data File : PP038746.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Aug 2021 19:15
Operator : AJ\MA
Sample : M3467-13
Misc :
ALS Vial : 83 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SAMPLE-2-(161.00)


Manual Integrations
APPROVED

mohammad
8/23/2021 2:21:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 05:48:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 18 04:51:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

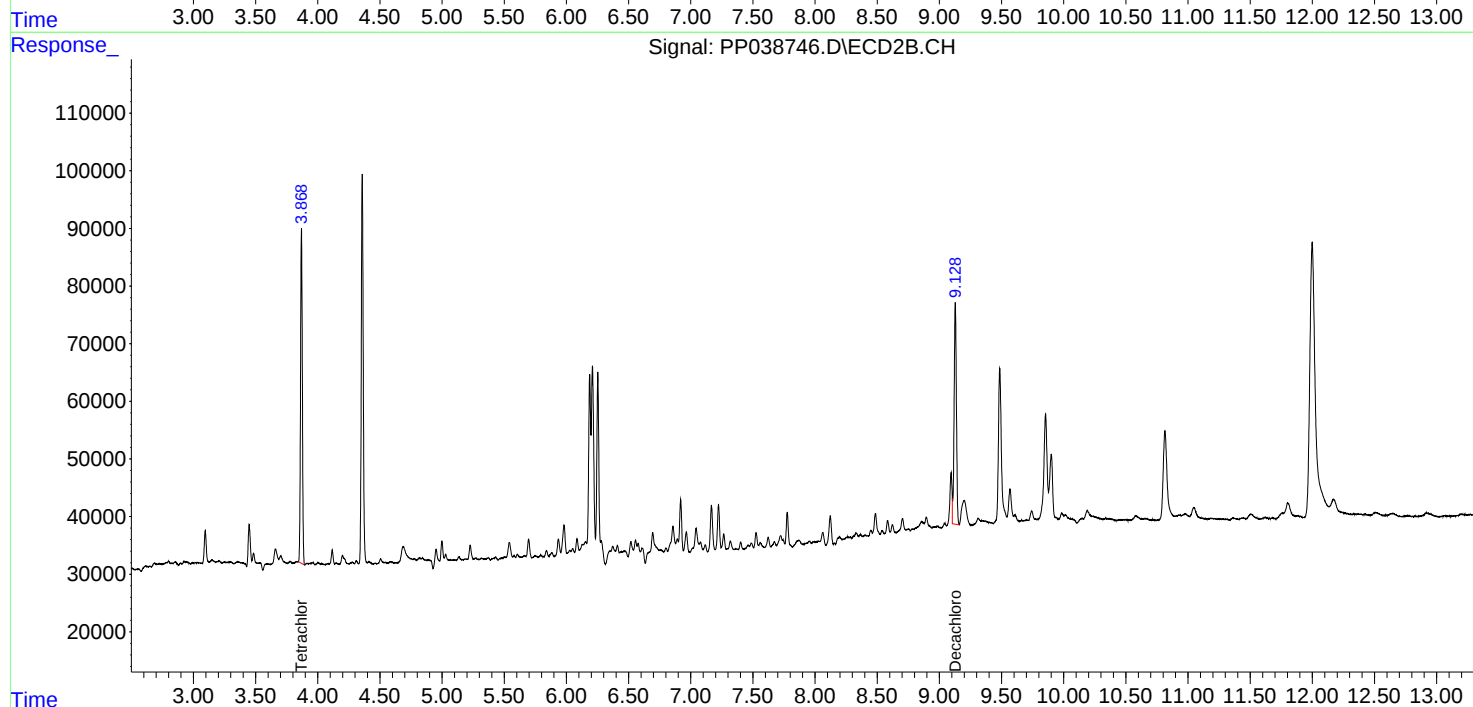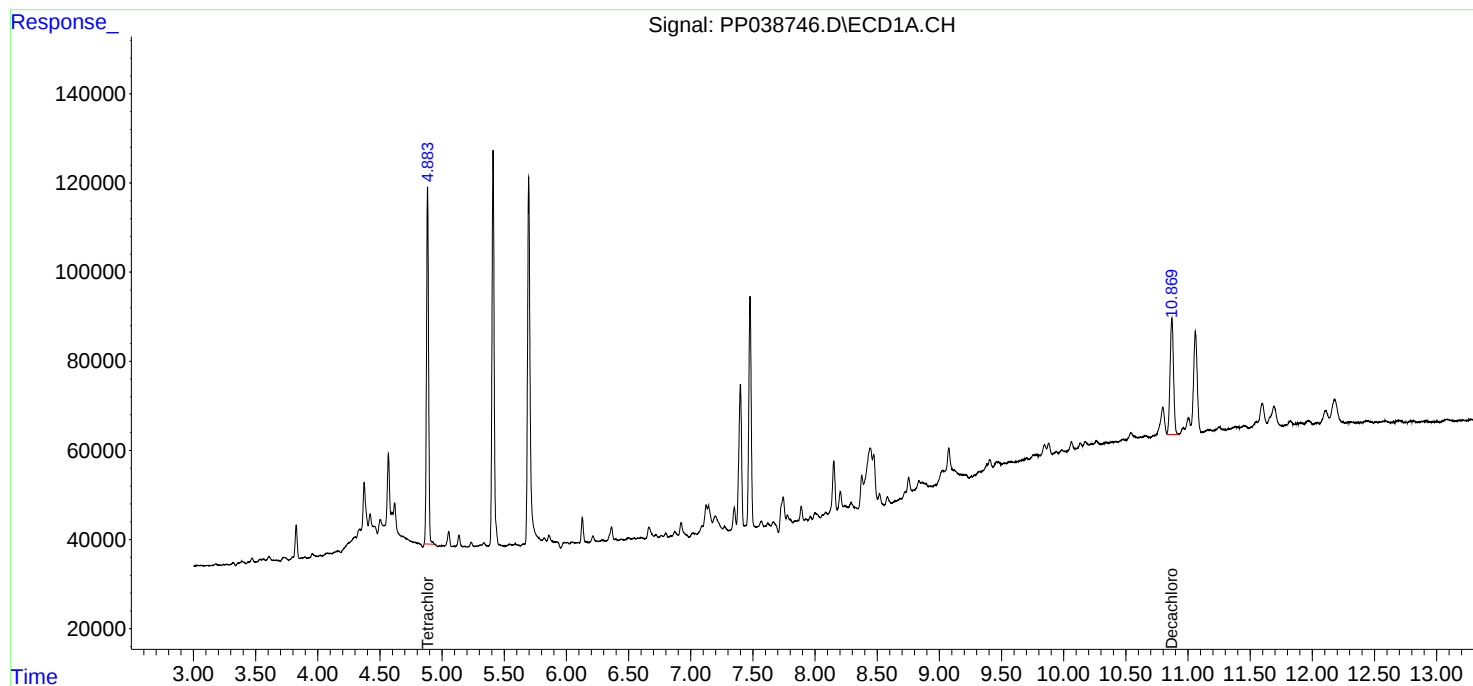

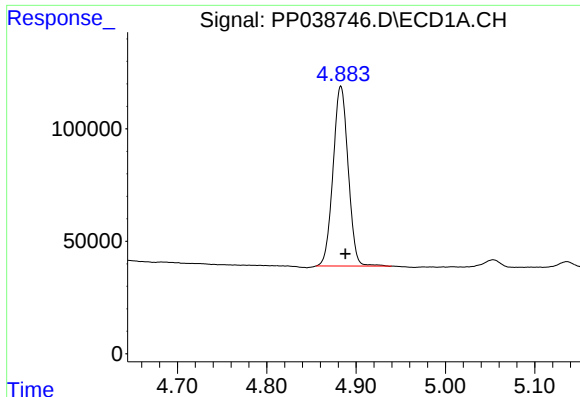


#1 Tetrachloro-m-xylene

R.T.: 4.883 min
Delta R.T.: -0.005 min
Response: 938188
Conc: 23.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
SAMPLE-2-(161.00)


Manual Integrations
APPROVED

mohammad
8/23/2021 2:21:09 PM

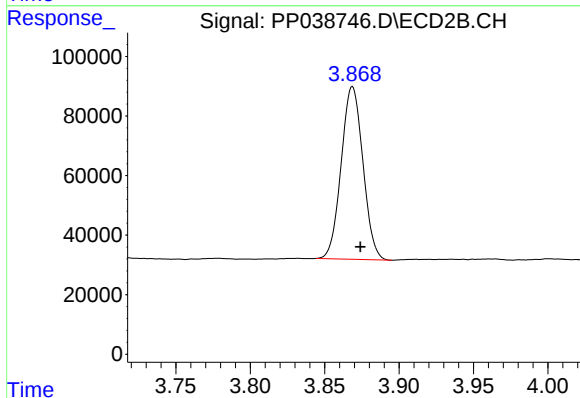


#1 Tetrachloro-m-xylene

R.T.: 3.869 min
Delta R.T.: -0.005 min
Response: 589389
Conc: 24.59 ng/ml

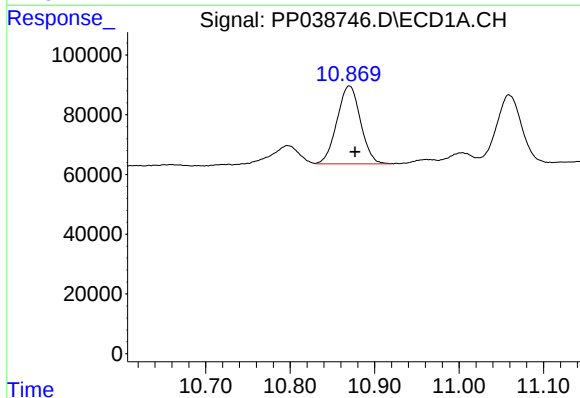

#2 Decachlorobiphenyl

R.T.: 10.869 min
Delta R.T.: -0.007 min
Response: 503717
Conc: 20.47 ng/ml m

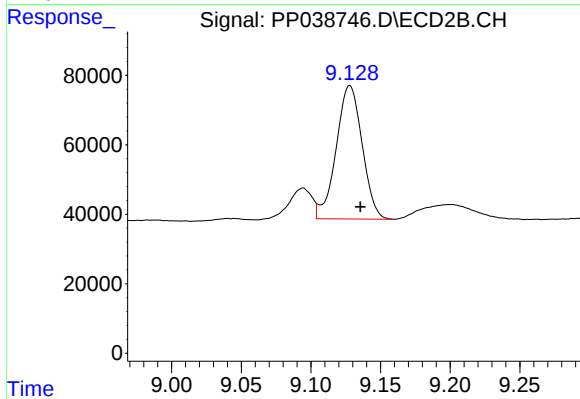

#2 Decachlorobiphenyl

R.T.: 9.128 min
Delta R.T.: -0.008 min
Response: 497407
Conc: 20.42 ng/ml m