

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082021\
 Data File : PP038748.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Aug 2021 19:49
 Operator : AJ\MA
 Sample : M3467-17
 Misc :
 ALS Vial : 85 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SAMPLE-4-(177.00)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 02:27:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 18 04:51:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.883	3.869	645117	406410	15.985	16.959
2)	SA Decachlor...	10.868	9.128	247518	250384	10.060	10.280

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082021\
Data File : PP038748.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Aug 2021 19:49
Operator : AJ\MA
Sample : M3467-17
Misc :
ALS Vial : 85 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SAMPLE-4-(177.00)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 02:27:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 18 04:51:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

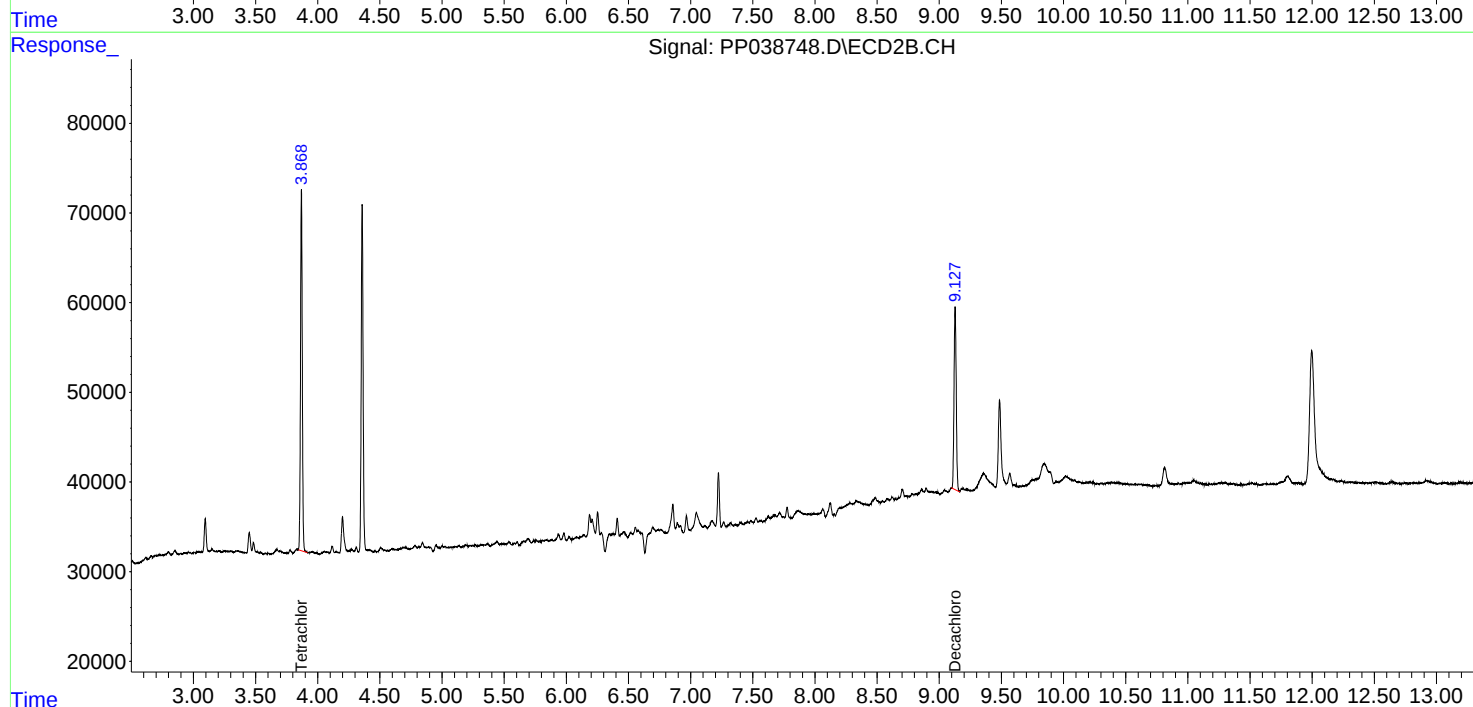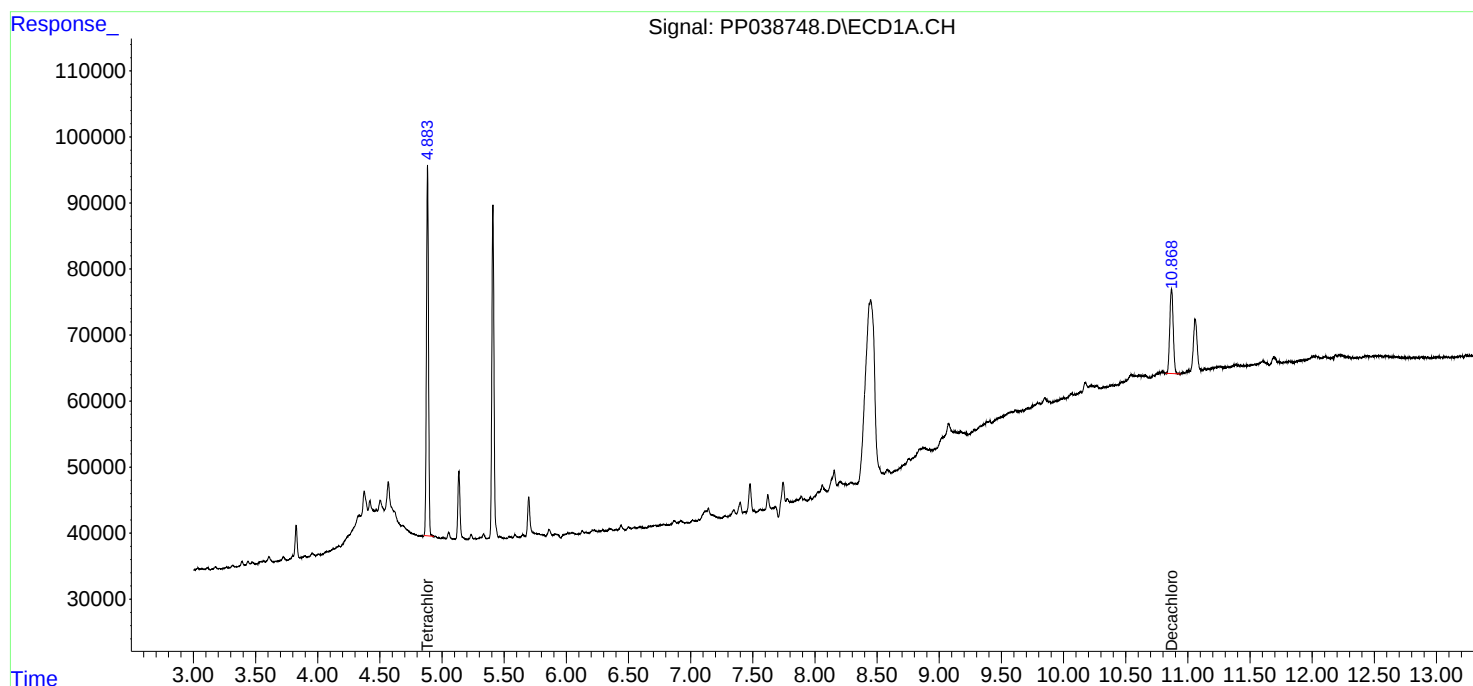


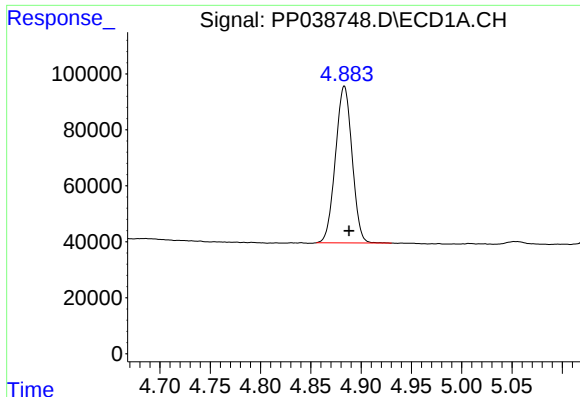

#1 Tetrachloro-m-xylene


R.T.: 4.883 min
Delta R.T.: -0.005 min
Response: 645117
Conc: 15.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
SAMPLE-4-(177.00)

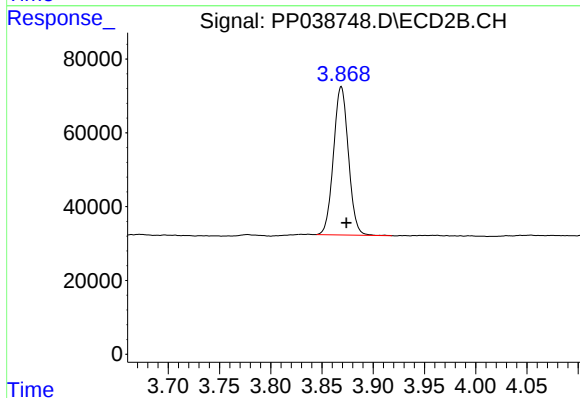


#1 Tetrachloro-m-xylene

R.T.: 3.869 min
Delta R.T.: -0.005 min
Response: 406410
Conc: 16.96 ng/ml

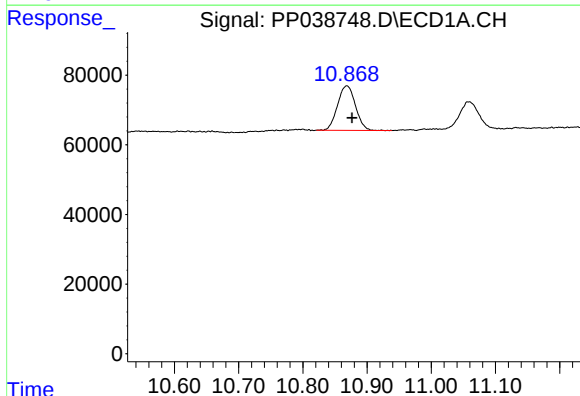

#2 Decachlorobiphenyl

R.T.: 10.868 min
Delta R.T.: -0.008 min
Response: 247518
Conc: 10.06 ng/ml

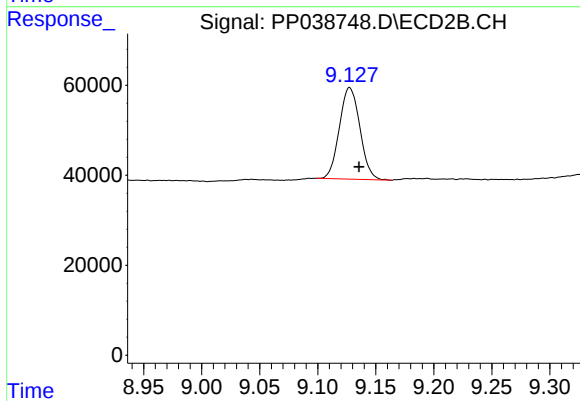

#2 Decachlorobiphenyl

R.T.: 9.128 min
Delta R.T.: -0.008 min
Response: 250384
Conc: 10.28 ng/ml