

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
 Data File : PP066710.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2024 00:50
 Operator : YP\AJ
 Sample : P3390-07
 Misc : AR1660 LOD 25 PPB
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 05:53:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 21 05:19:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.703	3.978	24068663	20425402	16.254	15.622
2)	SA Decachlor...	10.622	9.142	14121234	12422484	16.092	14.912
Target Compounds							
3)	L1 AR-1016-1	5.877	5.085	960643	824799	22.540	20.575
4)	L1 AR-1016-2	5.900	5.105	1403270	1200525	20.976	20.146
5)	L1 AR-1016-3	5.962	5.287	941073	627438	22.234	20.990
6)	L1 AR-1016-4	6.061	5.325	610342	666568	18.706	25.436 #
7)	L1 AR-1016-5	6.357	5.546	704147	699427	22.203	21.539
9)	L2 AR-1221-2	5.012	4.288	377723	362537	30.461	30.889
10)	L2 AR-1221-3	5.075	4.359	502918	547720	13.253	15.029
11)	L3 AR-1232-1	5.075	4.359	502918	547720	15.814	17.873
12)	L3 AR-1232-2	5.608	5.105	910648	1200525	52.575	44.494
13)	L3 AR-1232-3	5.900	5.287	1403270	627438	46.484	46.785
14)	L3 AR-1232-4	6.061	5.371	610342	731976	41.441	56.944 #
15)	L3 AR-1232-5	6.149	5.546	673752	699427	56.759	50.504
16)	L4 AR-1242-1	5.877	5.085	960643	824799	29.790	26.883
17)	L4 AR-1242-2	5.900	5.105	1403270	1200525	27.728	26.495
18)	L4 AR-1242-3	5.962	5.287	941073	627438	29.782	26.861
19)	L4 AR-1242-4	6.061	5.371	610342	731976	24.630	29.089
20)	L4 AR-1242-5	6.803	5.904	307363	788823	12.232	27.887 #
21)	L5 AR-1248-1	5.877	5.085	960643	824799	37.586	34.067
22)	L5 AR-1248-2	6.149	5.325	673752	666568	16.768	18.456
23)	L5 AR-1248-3	6.357	5.371	704147	731976	16.149	19.606
24)	L5 AR-1248-4	6.737f	5.546	932777	699427	21.115	15.852
25)	L5 AR-1248-5	6.803	5.942	307363	110572	6.705	2.927 #
26)	L6 AR-1254-1	6.737	5.904	932777	788823	18.895	13.168 #
27)	L6 AR-1254-2	6.952	6.054	1354061	529192	18.559	9.902 #
28)	L6 AR-1254-3	7.323	6.478	319572	1056633	4.574	13.363 #
29)	L6 AR-1254-4	0.000	6.726f	0	452219	N.D.	11.186 #
30)	L6 AR-1254-5	8.024	7.118	3720673	1233196	56.122	19.186 #
31)	L7 AR-1260-1	7.485	6.597	1233039	1391609	22.003	23.544
32)	L7 AR-1260-2	7.740	6.785	1371684	1556959	21.546	22.850
33)	L7 AR-1260-3	8.102	6.944	1352736	1507892	30.418	23.208
34)	L7 AR-1260-4	8.339	7.421	2068788	1168589	39.197	25.948 #
35)	L7 AR-1260-5	8.675	7.661	1806619	1890450	20.310	19.590
36)	L8 AR-1262-1	8.024	7.118	3720673	1233196	82.406	38.580 #
37)	L8 AR-1262-2	8.675	7.421	1806619	1168589	16.544	18.741
38)	L8 AR-1262-3	9.025	7.948	1129814	308656	15.914	6.898 #
39)	L8 AR-1262-4	9.107	8.013	692794	1325696	11.871	15.990 #
40)	L8 AR-1262-5	9.811	8.538	446795	491792	13.382	15.531
41)	L9 AR-1268-1	9.025f	7.948	1129814	308656	9.015	2.465 #
42)	L9 AR-1268-2	9.107	8.013	692794	1325696	6.281	11.447 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
 Data File : PP066710.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2024 00:50
 Operator : YP\AJ
 Sample : P3390-07
 Misc : AR1660 LOD 25 PPB
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 05:53:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 21 05:19:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	8.253f	0	150646	N.D.	1.512 #
44) L9	AR-1268-4	9.811	8.538	446795	491792	14.663	14.533
45) L9	AR-1268-5	10.259	8.865	231440	231571	0.812	0.797



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
Data File : PP066710.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2024 00:50
Operator : YP\AJ
Sample : P3390-07
Misc : AR1660 LOD 25 PPB
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 05:53:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 21 05:19:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

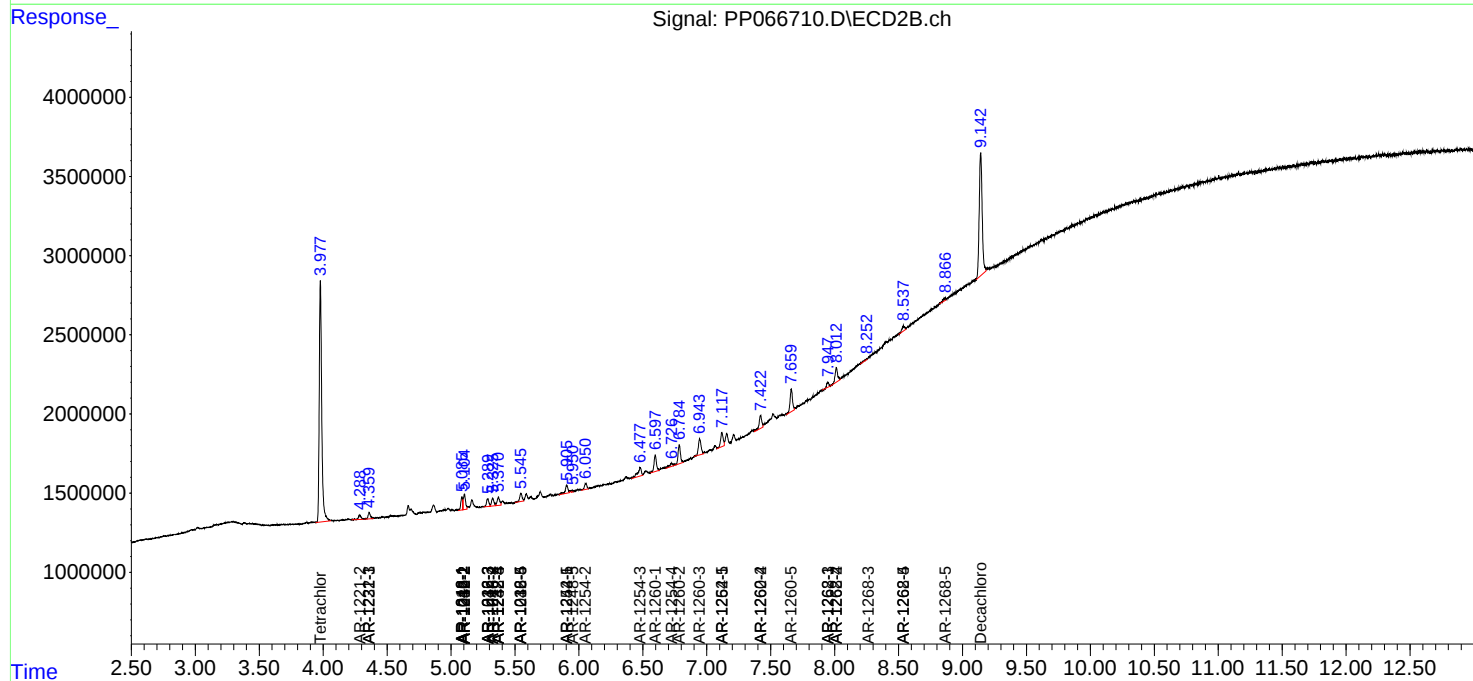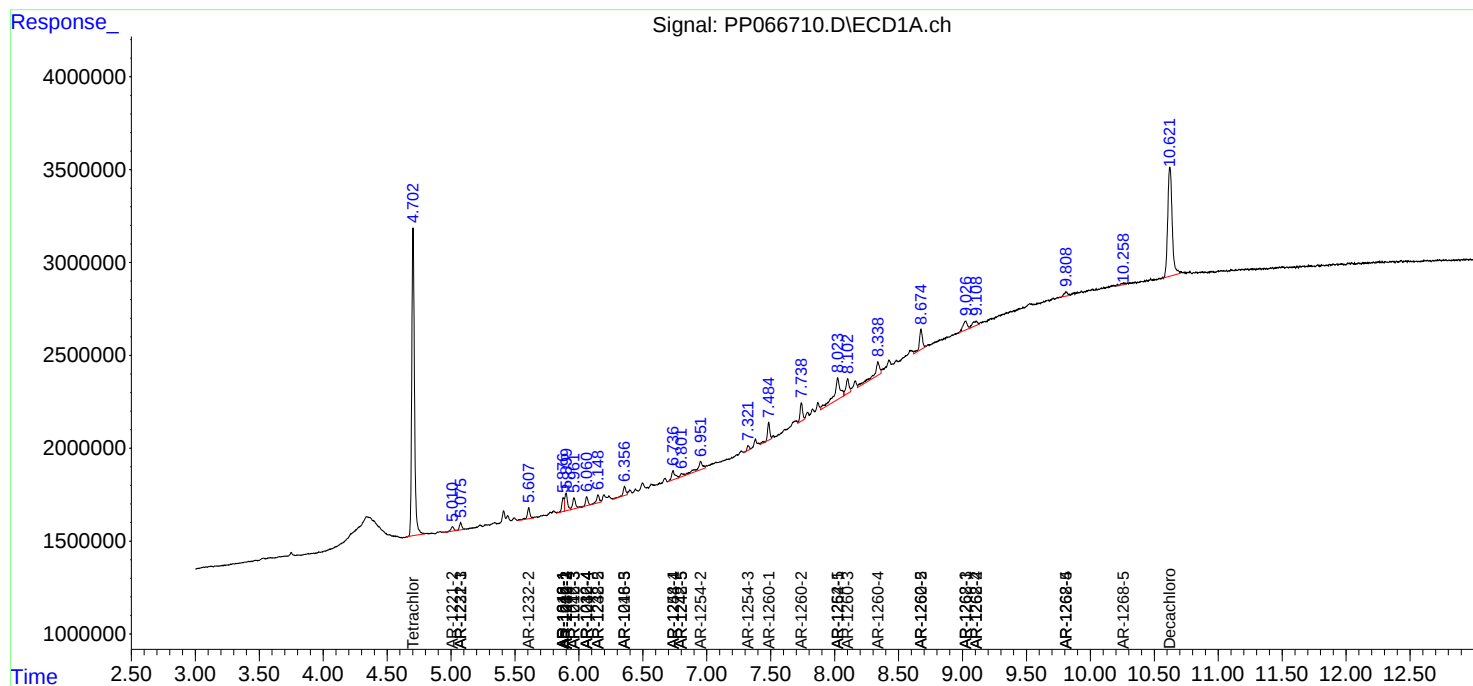


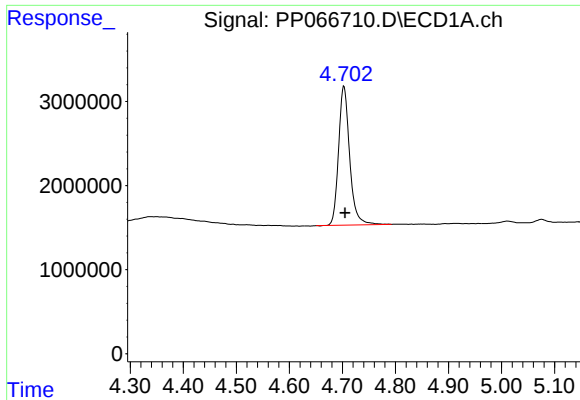

#1 Tetrachloro-m-xylene


R.T.: 4.703 min
Delta R.T.: -0.002 min
Response: 24068663
Conc: 16.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

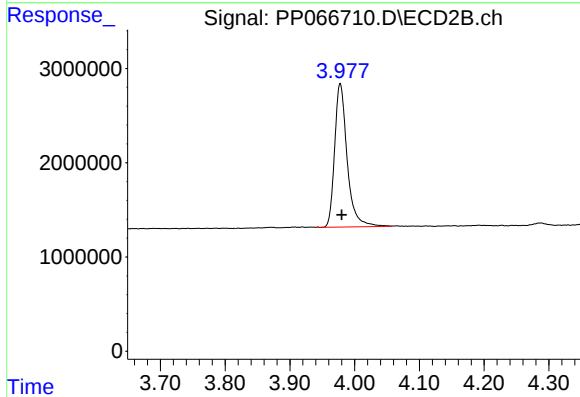


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.002 min
Response: 20425402
Conc: 15.62 ng/ml

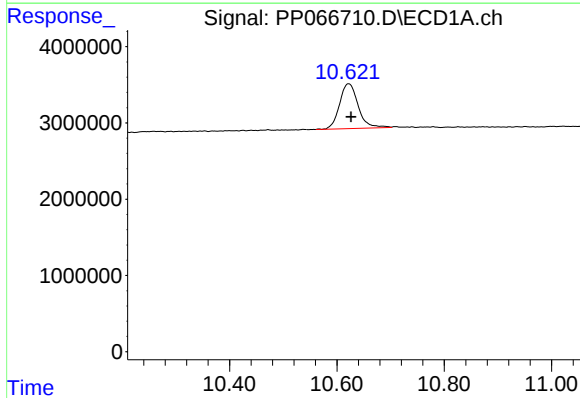


#2 Decachlorobiphenyl

R.T.: 10.622 min
Delta R.T.: -0.004 min
Response: 14121234
Conc: 16.09 ng/ml

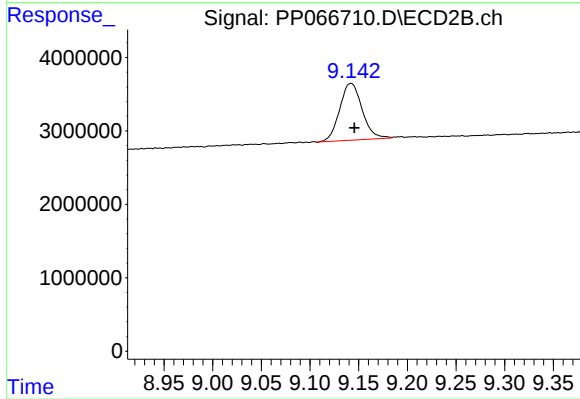

#2 Decachlorobiphenyl


R.T.: 9.142 min
Delta R.T.: -0.003 min
Response: 12422484
Conc: 14.91 ng/ml

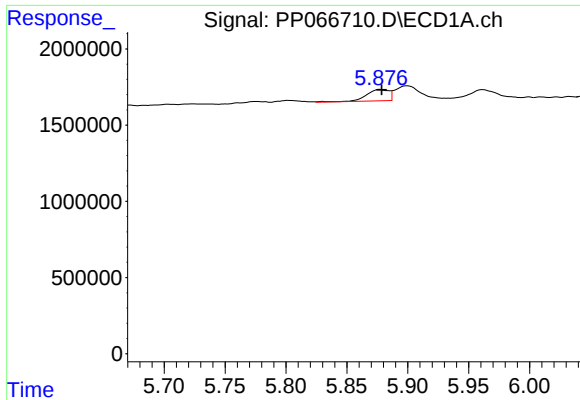

#3 AR-1016-1


R.T.: 5.877 min
Delta R.T.: -0.001 min
Response: 960643
Conc: 22.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

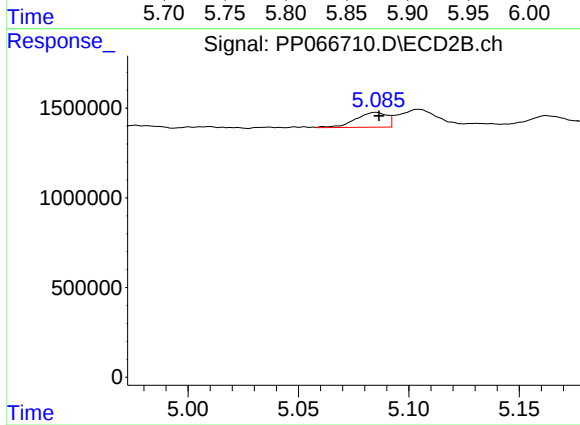


#3 AR-1016-1

R.T.: 5.085 min
Delta R.T.: -0.002 min
Response: 824799
Conc: 20.57 ng/ml

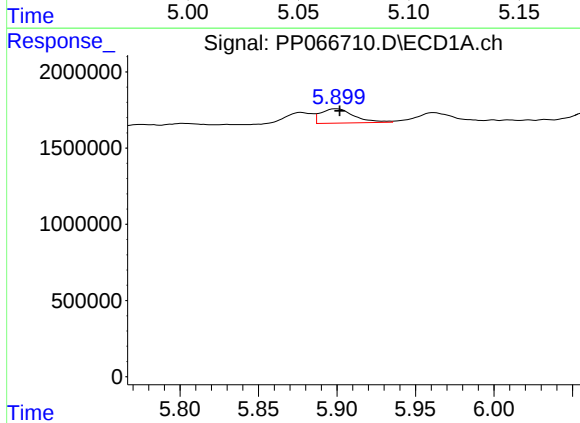


#4 AR-1016-2

R.T.: 5.900 min
Delta R.T.: -0.002 min
Response: 1403270
Conc: 20.98 ng/ml

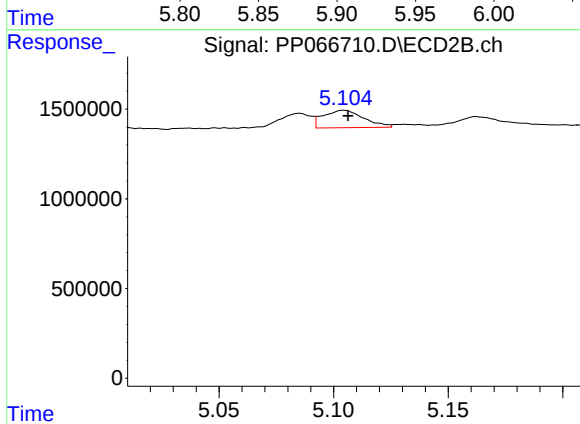

#4 AR-1016-2


R.T.: 5.105 min
Delta R.T.: -0.002 min
Response: 1200525
Conc: 20.15 ng/ml

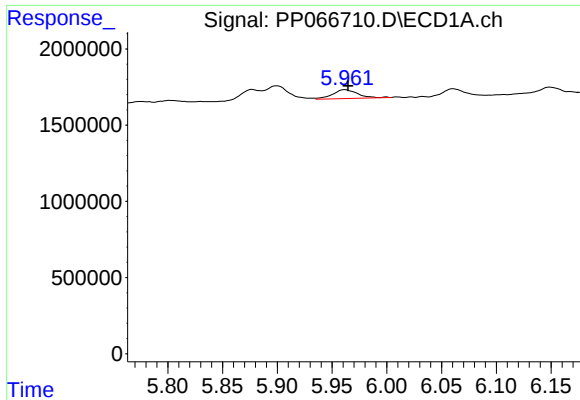

#5 AR-1016-3


R.T.: 5.962 min
Delta R.T.: -0.003 min
Response: 941073
Conc: 22.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

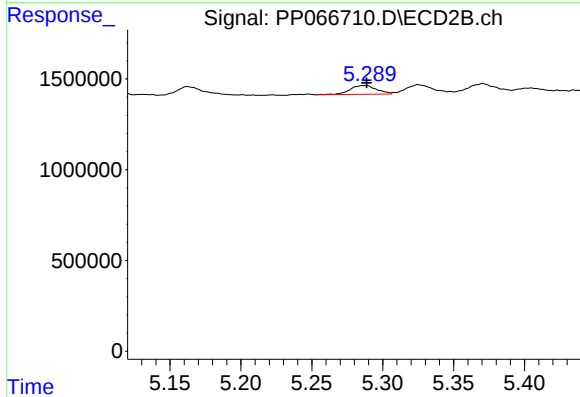


#5 AR-1016-3

R.T.: 5.287 min
Delta R.T.: -0.001 min
Response: 627438
Conc: 20.99 ng/ml

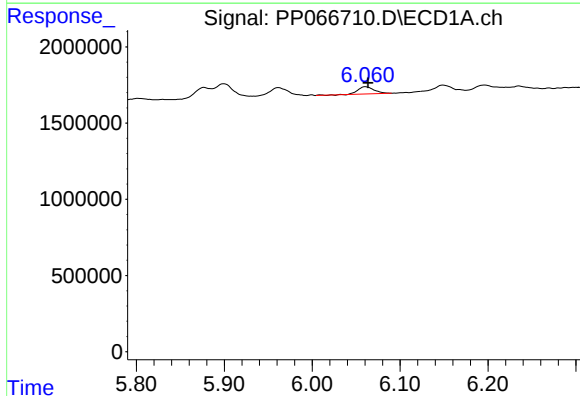


#6 AR-1016-4

R.T.: 6.061 min
Delta R.T.: -0.002 min
Response: 610342
Conc: 18.71 ng/ml

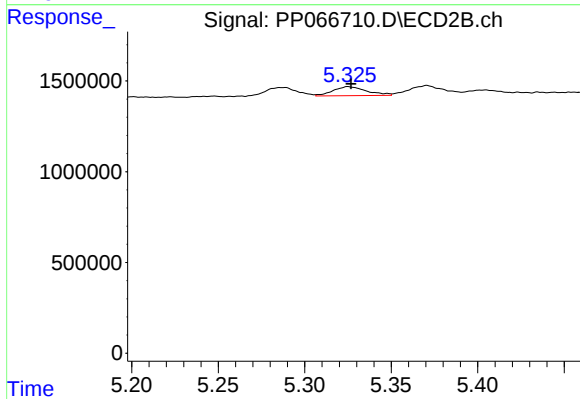

#6 AR-1016-4


R.T.: 5.325 min
Delta R.T.: -0.002 min
Response: 666568
Conc: 25.44 ng/ml

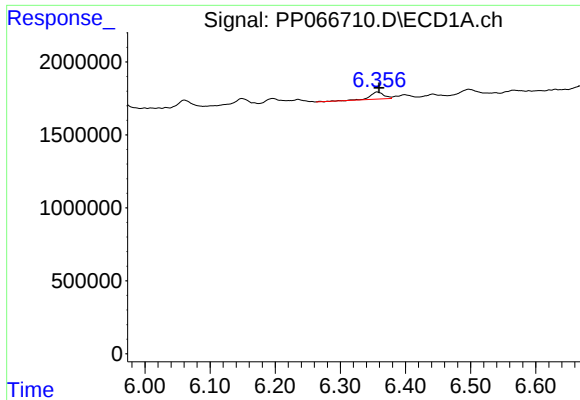

#7 AR-1016-5


R.T.: 6.357 min
Delta R.T.: -0.002 min
Response: 704147
Conc: 22.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

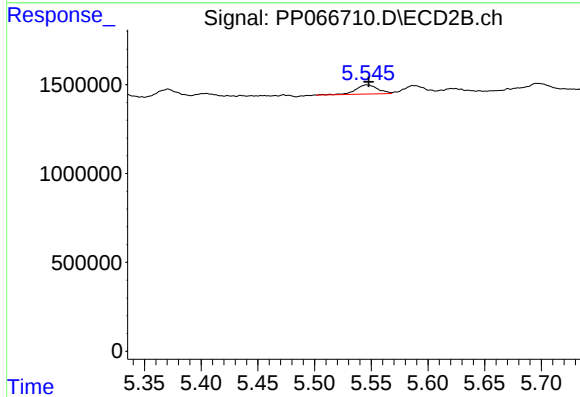


#7 AR-1016-5

R.T.: 5.546 min
Delta R.T.: -0.001 min
Response: 699427
Conc: 21.54 ng/ml

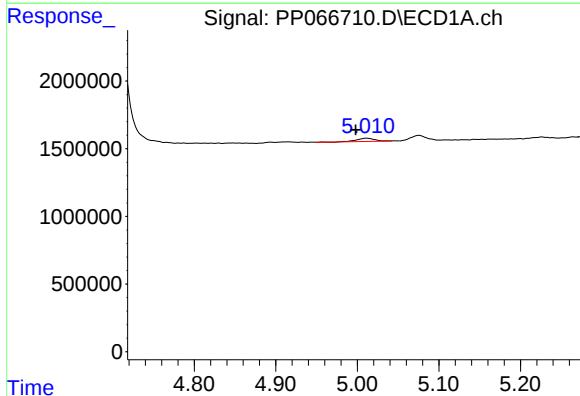


#9 AR-1221-2

R.T.: 5.012 min
Delta R.T.: 0.014 min
Response: 377723
Conc: 30.46 ng/ml

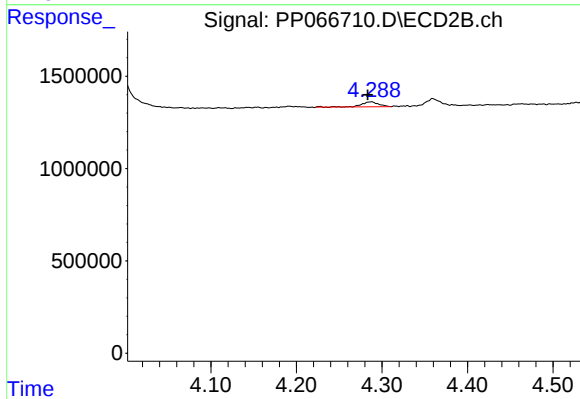

#9 AR-1221-2


R.T.: 4.288 min
Delta R.T.: 0.004 min
Response: 362537
Conc: 30.89 ng/ml

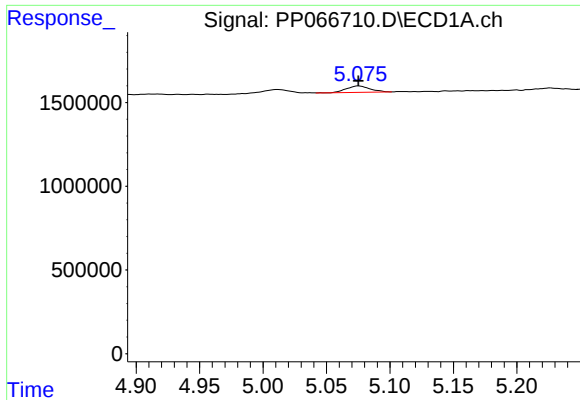

#10 AR-1221-3


R.T.: 5.075 min
Delta R.T.: 0.000 min
Response: 502918
Conc: 13.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

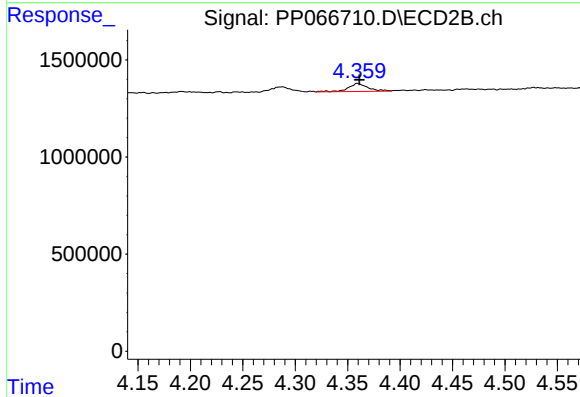


#10 AR-1221-3

R.T.: 4.359 min
Delta R.T.: -0.002 min
Response: 547720
Conc: 15.03 ng/ml

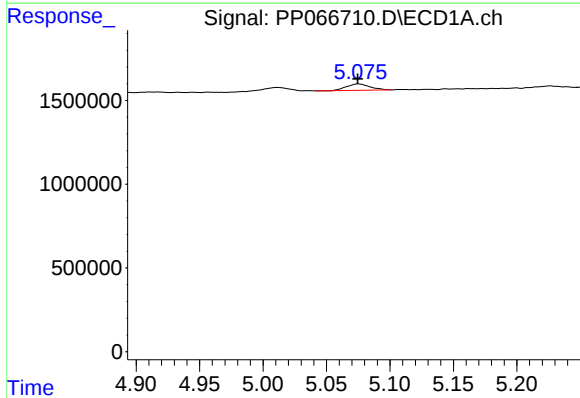


#11 AR-1232-1

R.T.: 5.075 min
Delta R.T.: 0.000 min
Response: 502918
Conc: 15.81 ng/ml

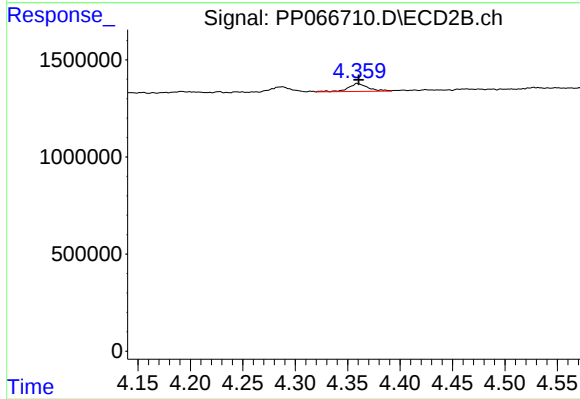

#11 AR-1232-1


R.T.: 4.359 min
Delta R.T.: -0.001 min
Response: 547720
Conc: 17.87 ng/ml

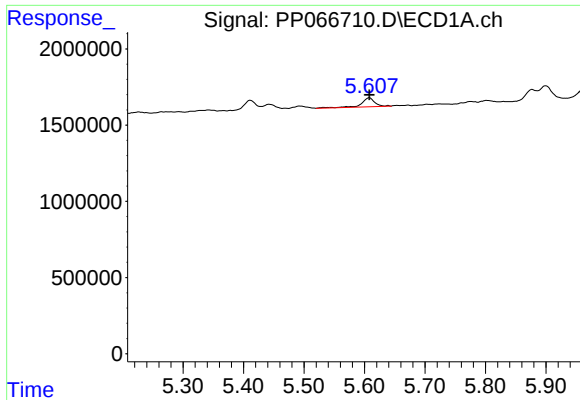

#12 AR-1232-2


R.T.: 5.608 min
Delta R.T.: 0.000 min
Response: 910648
Conc: 52.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

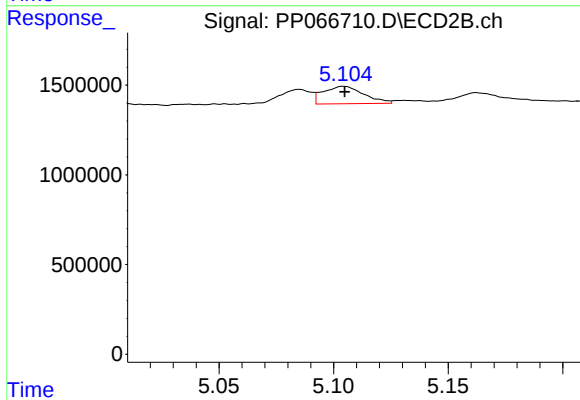


#12 AR-1232-2

R.T.: 5.105 min
Delta R.T.: 0.000 min
Response: 1200525
Conc: 44.49 ng/ml

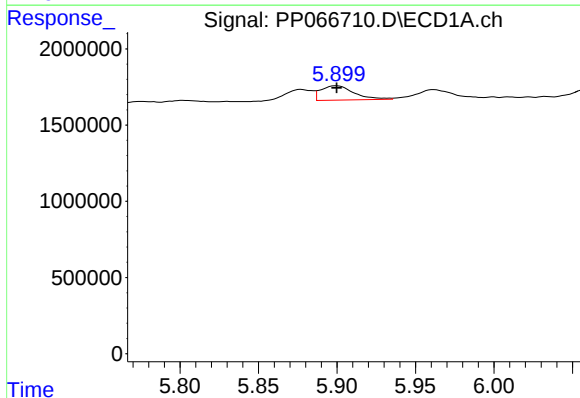


#13 AR-1232-3

R.T.: 5.900 min
Delta R.T.: 0.000 min
Response: 1403270
Conc: 46.48 ng/ml

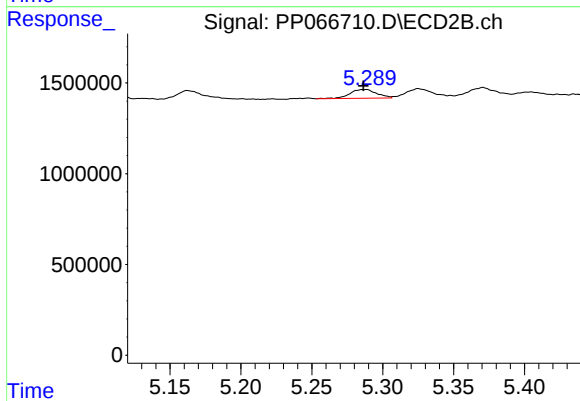

#13 AR-1232-3


R.T.: 5.287 min
Delta R.T.: 0.000 min
Response: 627438
Conc: 46.78 ng/ml

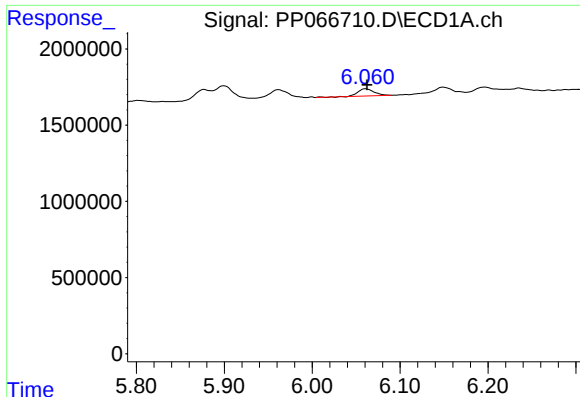

#14 AR-1232-4


R.T.: 6.061 min
Delta R.T.: -0.002 min
Response: 610342
Conc: 41.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

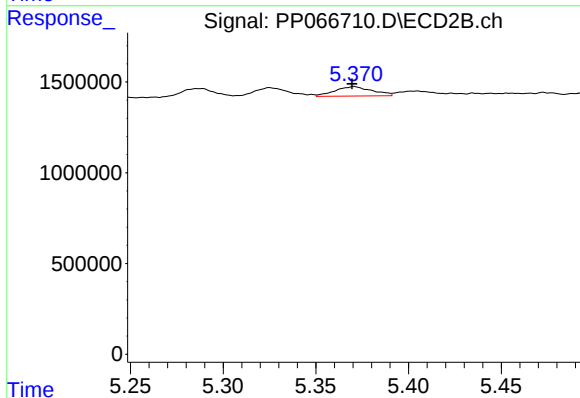


#14 AR-1232-4

R.T.: 5.371 min
Delta R.T.: 0.001 min
Response: 731976
Conc: 56.94 ng/ml

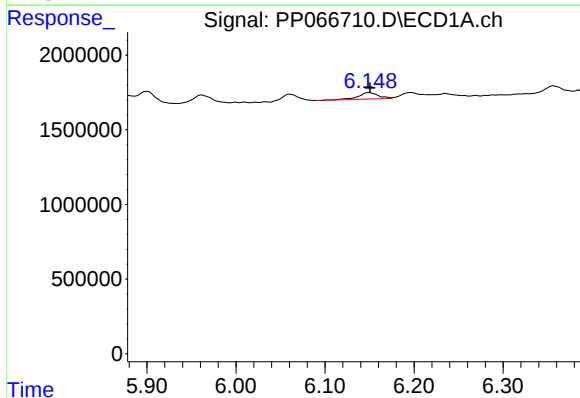


#15 AR-1232-5

R.T.: 6.149 min
Delta R.T.: -0.001 min
Response: 673752
Conc: 56.76 ng/ml

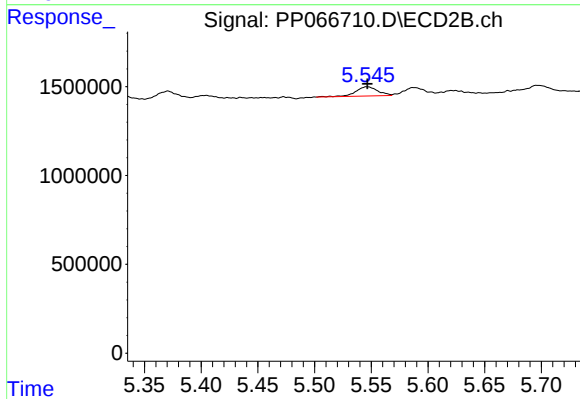

#15 AR-1232-5


R.T.: 5.546 min
Delta R.T.: 0.000 min
Response: 699427
Conc: 50.50 ng/ml

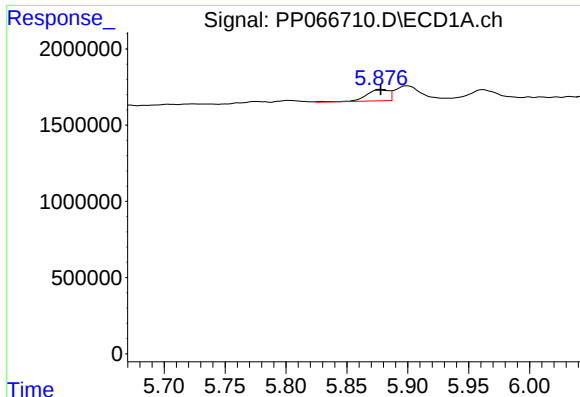

#16 AR-1242-1


R.T.: 5.877 min
Delta R.T.: 0.000 min
Response: 960643
Conc: 29.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

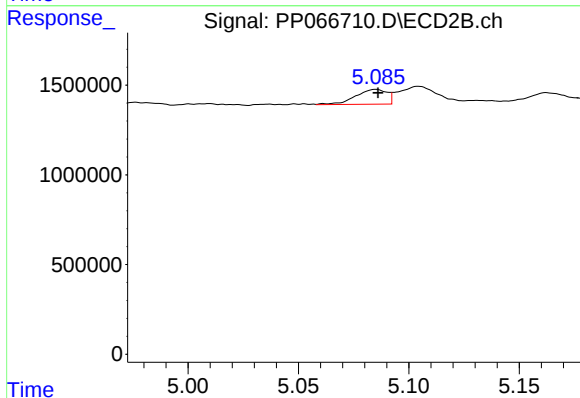


#16 AR-1242-1

R.T.: 5.085 min
Delta R.T.: -0.001 min
Response: 824799
Conc: 26.88 ng/ml

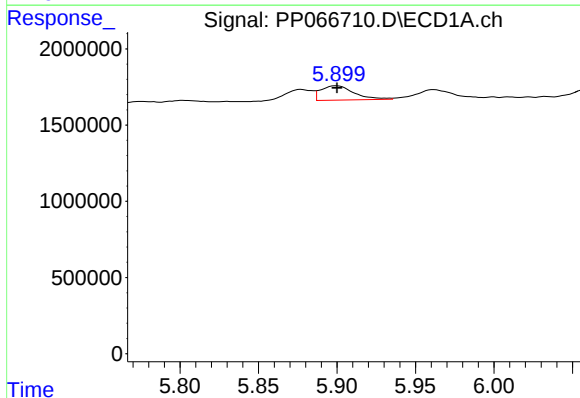


#17 AR-1242-2

R.T.: 5.900 min
Delta R.T.: 0.000 min
Response: 1403270
Conc: 27.73 ng/ml

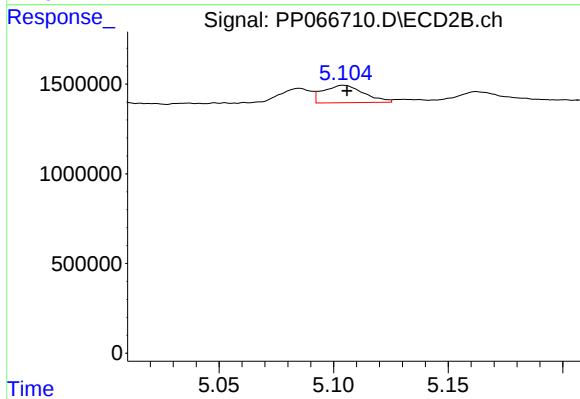

#17 AR-1242-2


R.T.: 5.105 min
Delta R.T.: -0.001 min
Response: 1200525
Conc: 26.49 ng/ml

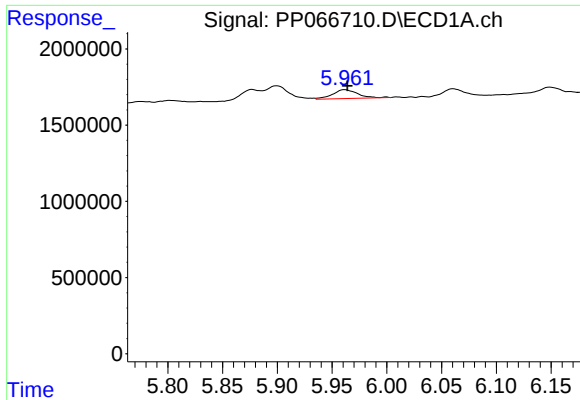

#18 AR-1242-3


R.T.: 5.962 min
Delta R.T.: -0.002 min
Response: 941073
Conc: 29.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

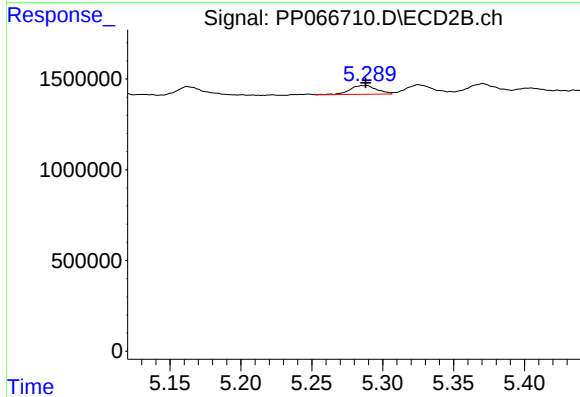


#18 AR-1242-3

R.T.: 5.287 min
Delta R.T.: 0.000 min
Response: 627438
Conc: 26.86 ng/ml

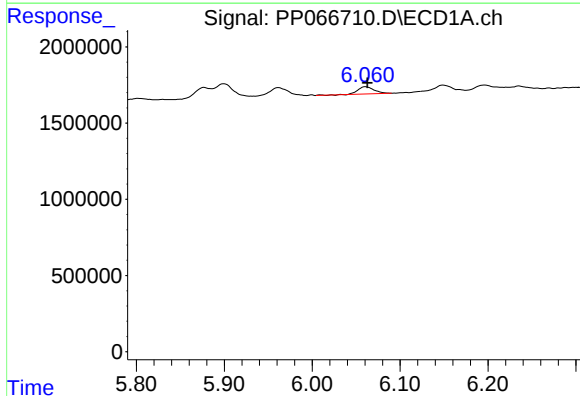


#19 AR-1242-4

R.T.: 6.061 min
Delta R.T.: -0.002 min
Response: 610342
Conc: 24.63 ng/ml

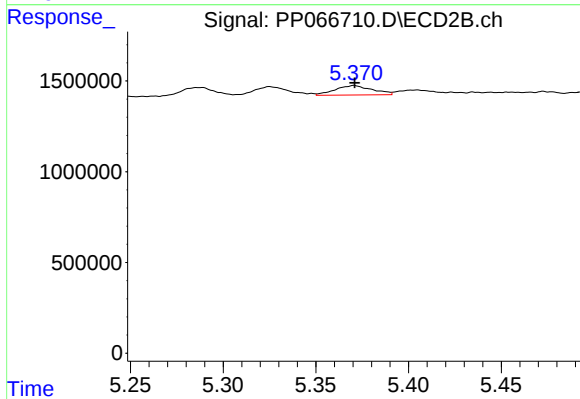

#19 AR-1242-4


R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 731976
Conc: 29.09 ng/ml

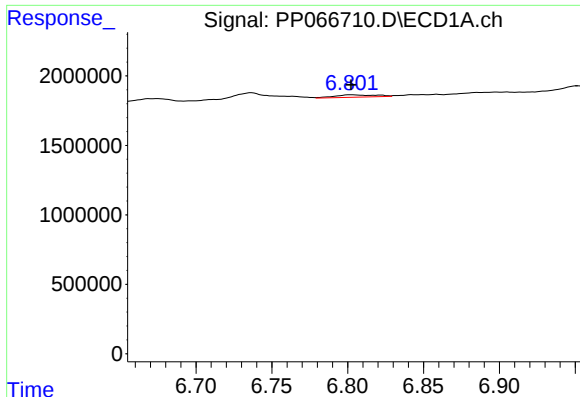

#20 AR-1242-5


R.T.: 6.803 min
Delta R.T.: 0.000 min
Response: 307363
Conc: 12.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

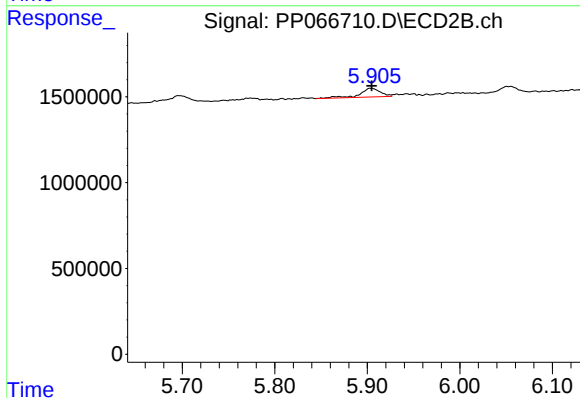


#20 AR-1242-5

R.T.: 5.904 min
Delta R.T.: 0.000 min
Response: 788823
Conc: 27.89 ng/ml

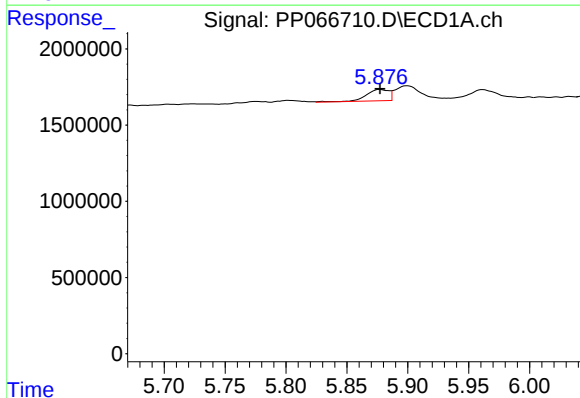


#21 AR-1248-1

R.T.: 5.877 min
Delta R.T.: 0.000 min
Response: 960643
Conc: 37.59 ng/ml

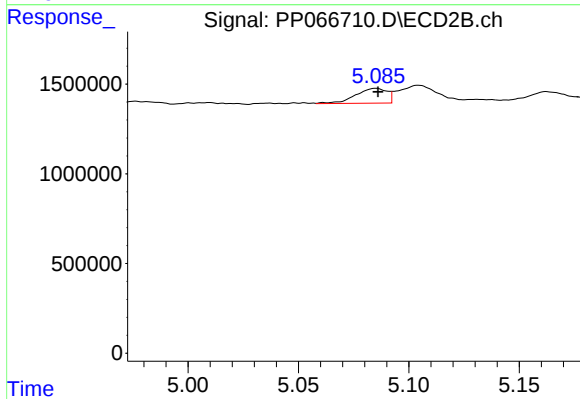

#21 AR-1248-1


R.T.: 5.085 min
Delta R.T.: -0.001 min
Response: 824799
Conc: 34.07 ng/ml

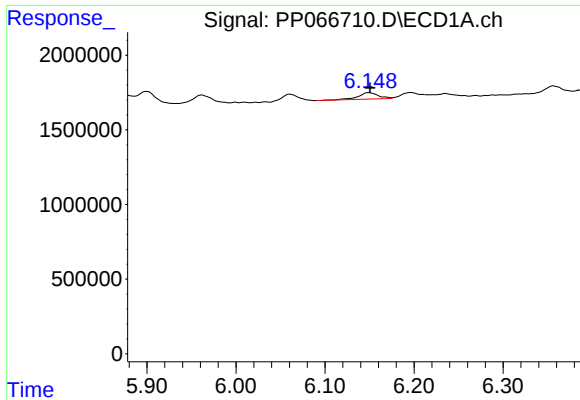

#22 AR-1248-2


R.T.: 6.149 min
Delta R.T.: -0.001 min
Response: 673752
Conc: 16.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

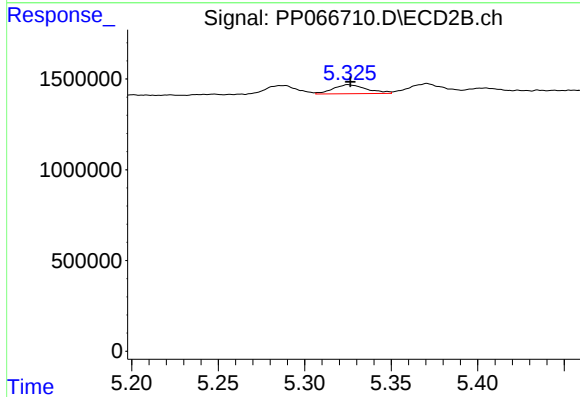


#22 AR-1248-2

R.T.: 5.325 min
Delta R.T.: -0.001 min
Response: 666568
Conc: 18.46 ng/ml

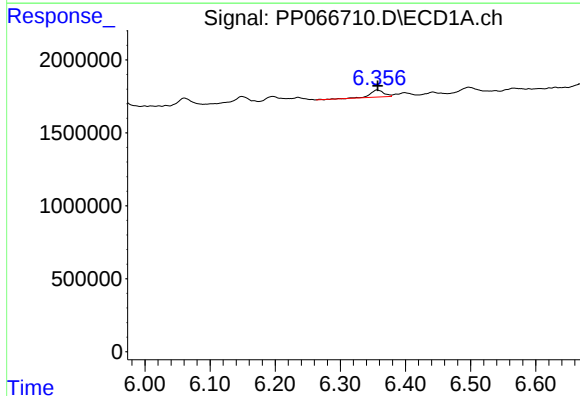


#23 AR-1248-3

R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 704147
Conc: 16.15 ng/ml

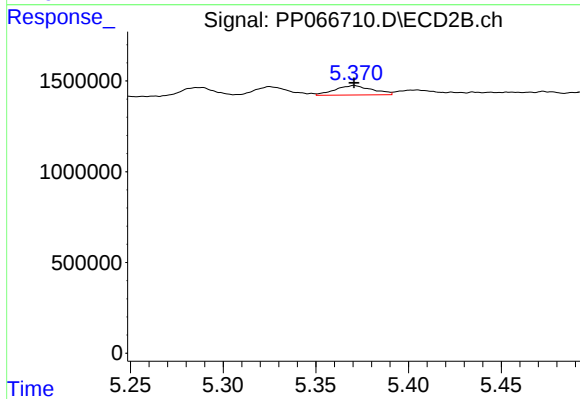

#23 AR-1248-3


R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 731976
Conc: 19.61 ng/ml

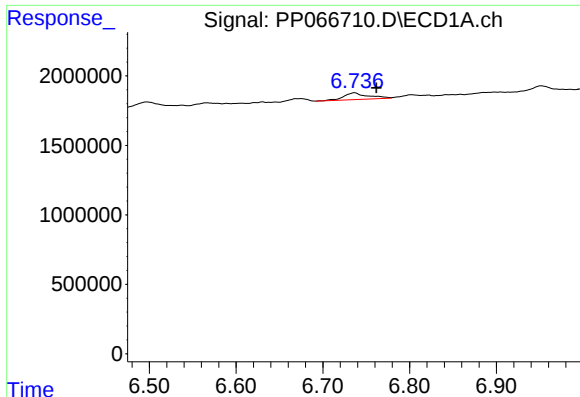

#24 AR-1248-4


R.T.: 6.737 min
Delta R.T.: -0.025 min
Response: 932777
Conc: 21.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

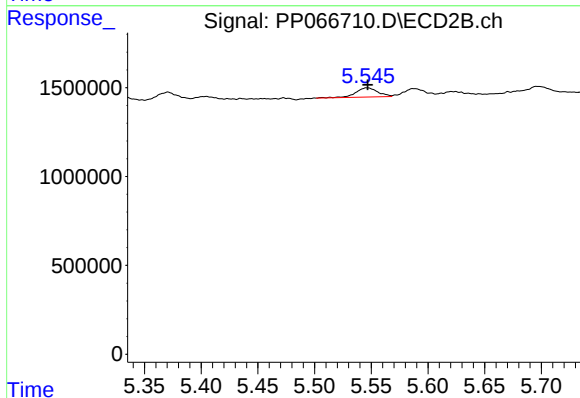


#24 AR-1248-4

R.T.: 5.546 min
Delta R.T.: 0.000 min
Response: 699427
Conc: 15.85 ng/ml

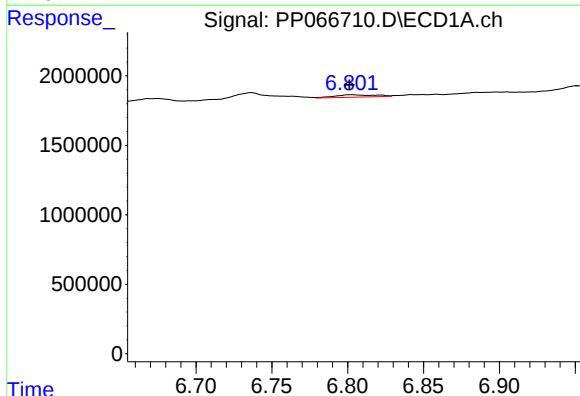


#25 AR-1248-5

R.T.: 6.803 min
Delta R.T.: 0.002 min
Response: 307363
Conc: 6.70 ng/ml

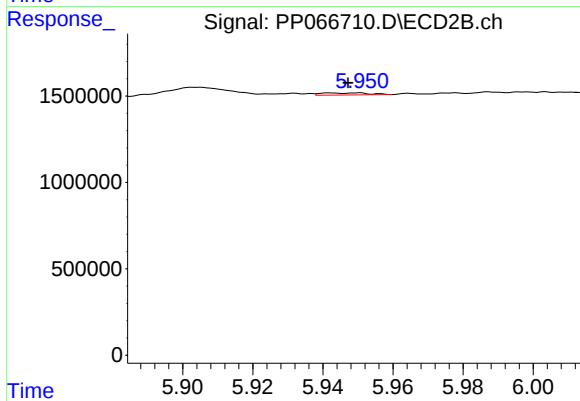

#25 AR-1248-5


R.T.: 5.942 min
Delta R.T.: -0.005 min
Response: 110572
Conc: 2.93 ng/ml

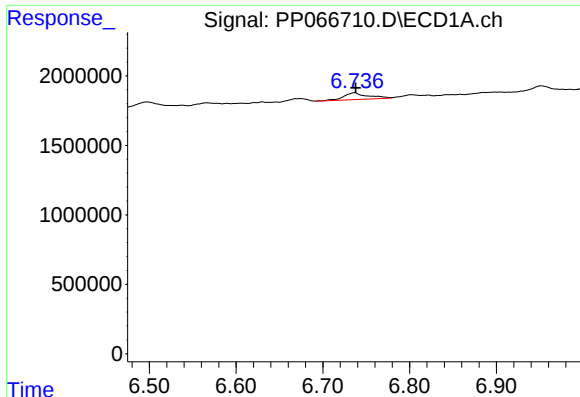

#26 AR-1254-1


R.T.: 6.737 min
Delta R.T.: -0.002 min
Response: 932777
Conc: 18.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

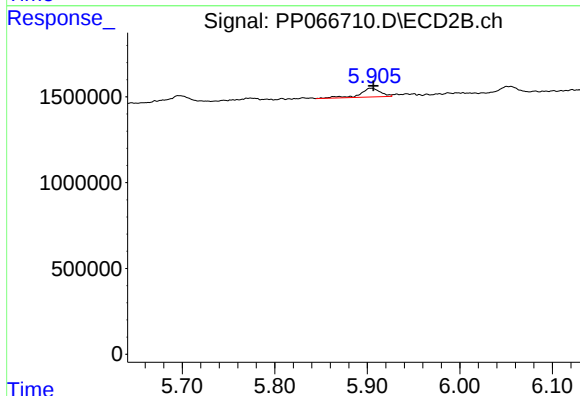


#26 AR-1254-1

R.T.: 5.904 min
Delta R.T.: -0.003 min
Response: 788823
Conc: 13.17 ng/ml

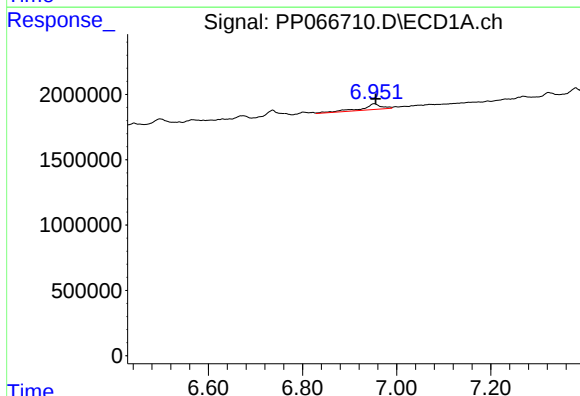


#27 AR-1254-2

R.T.: 6.952 min
Delta R.T.: -0.003 min
Response: 1354061
Conc: 18.56 ng/ml

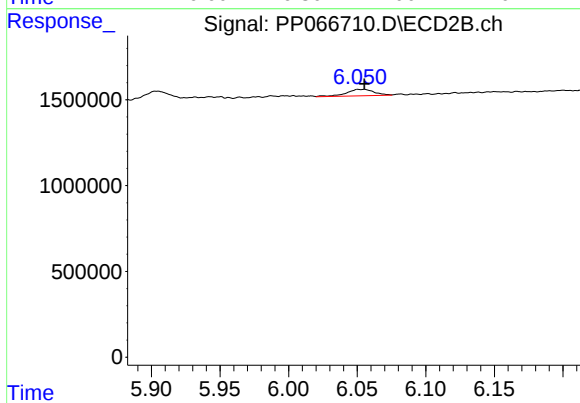

#27 AR-1254-2


R.T.: 6.054 min
Delta R.T.: -0.001 min
Response: 529192
Conc: 9.90 ng/ml

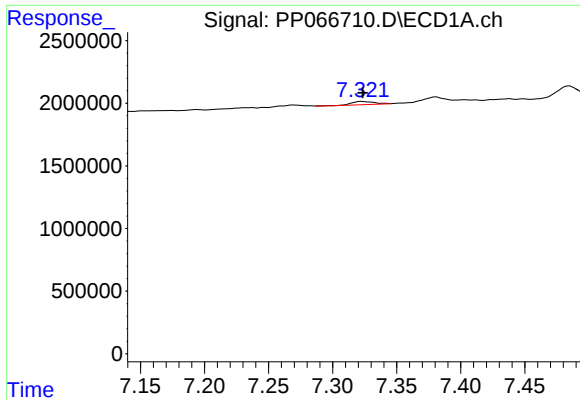

#28 AR-1254-3


R.T.: 7.323 min
Delta R.T.: 0.000 min
Response: 319572
Conc: 4.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

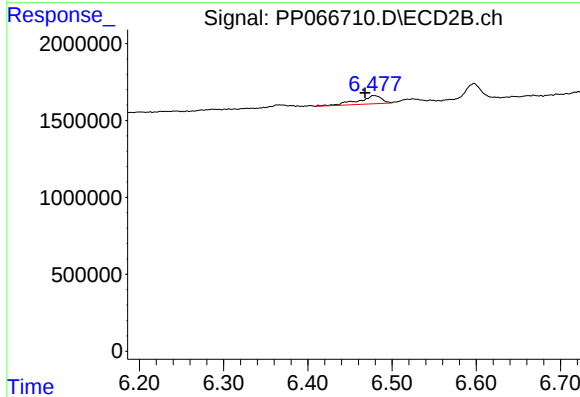


#28 AR-1254-3

R.T.: 6.478 min
Delta R.T.: 0.010 min
Response: 1056633
Conc: 13.36 ng/ml

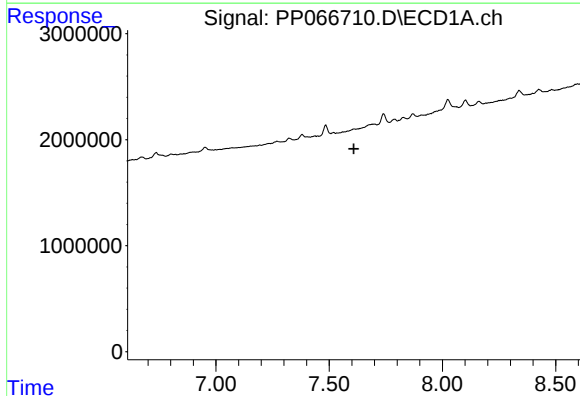


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.609 min
Response: 0
Conc: N.D.

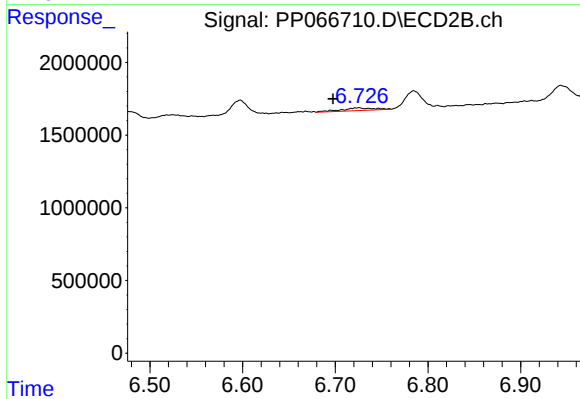

#29 AR-1254-4


R.T.: 6.726 min
Delta R.T.: 0.028 min
Response: 452219
Conc: 11.19 ng/ml

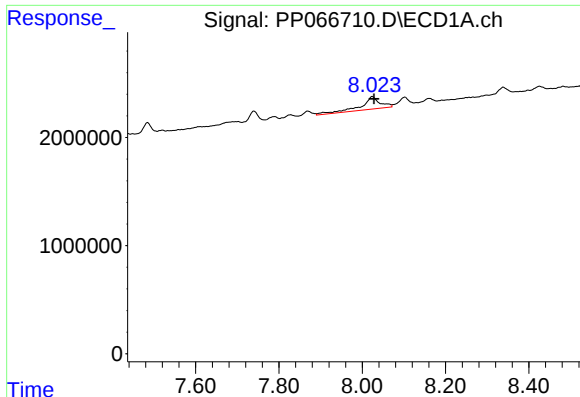

#30 AR-1254-5


R.T.: 8.024 min
Delta R.T.: -0.004 min
Response: 3720673
Conc: 56.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

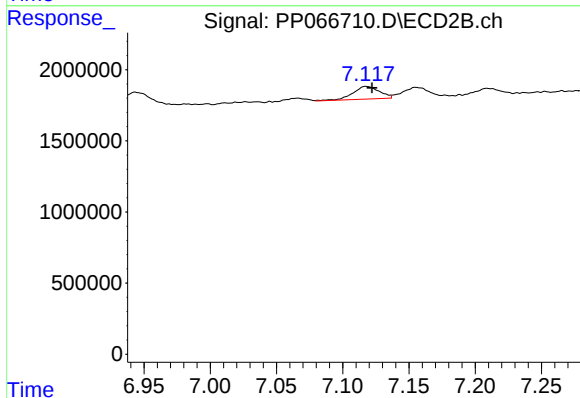


#30 AR-1254-5

R.T.: 7.118 min
Delta R.T.: -0.004 min
Response: 1233196
Conc: 19.19 ng/ml

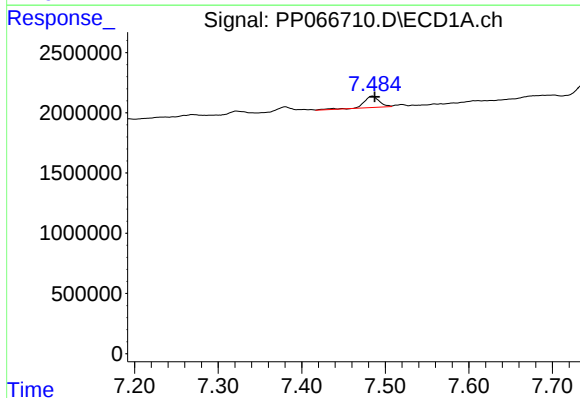


#31 AR-1260-1

R.T.: 7.485 min
Delta R.T.: -0.003 min
Response: 1233039
Conc: 22.00 ng/ml

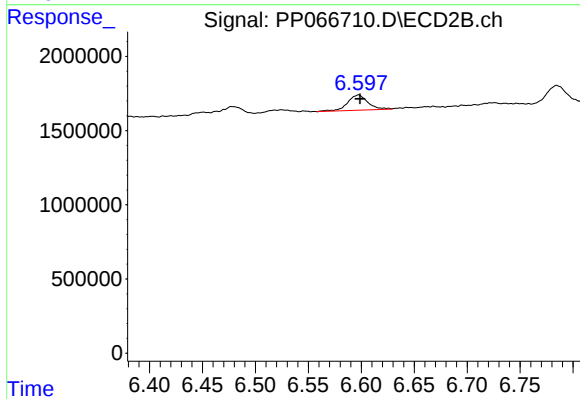

#31 AR-1260-1


R.T.: 6.597 min
Delta R.T.: -0.001 min
Response: 1391609
Conc: 23.54 ng/ml

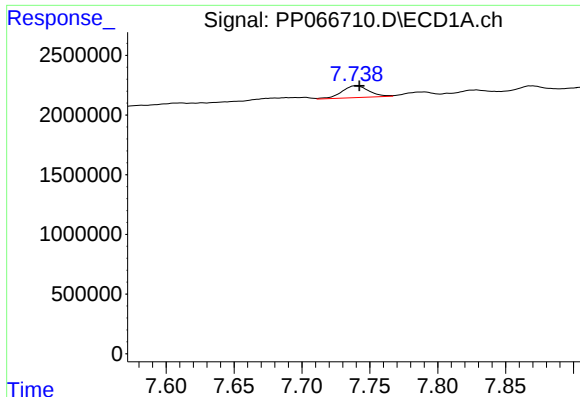

#32 AR-1260-2


R.T.: 7.740 min
Delta R.T.: -0.002 min
Response: 1371684
Conc: 21.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

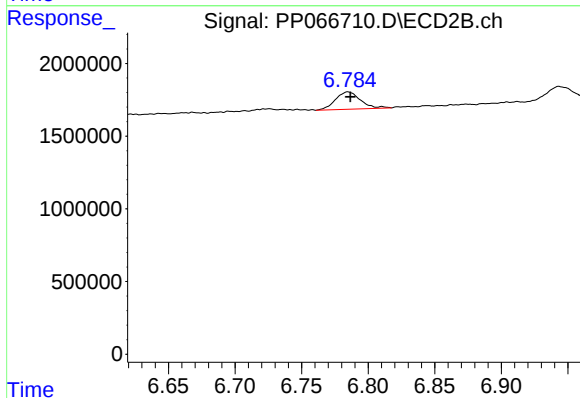


#32 AR-1260-2

R.T.: 6.785 min
Delta R.T.: -0.002 min
Response: 1556959
Conc: 22.85 ng/ml

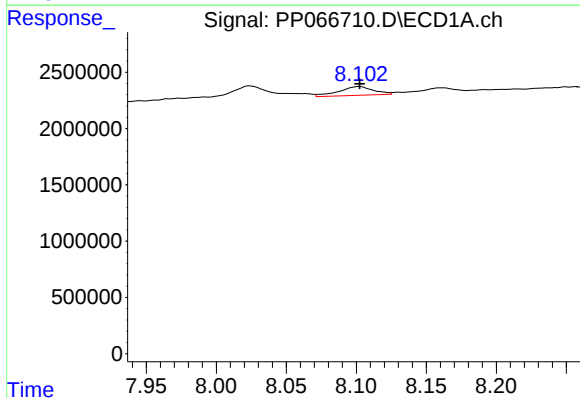


#33 AR-1260-3

R.T.: 8.102 min
Delta R.T.: 0.000 min
Response: 1352736
Conc: 30.42 ng/ml

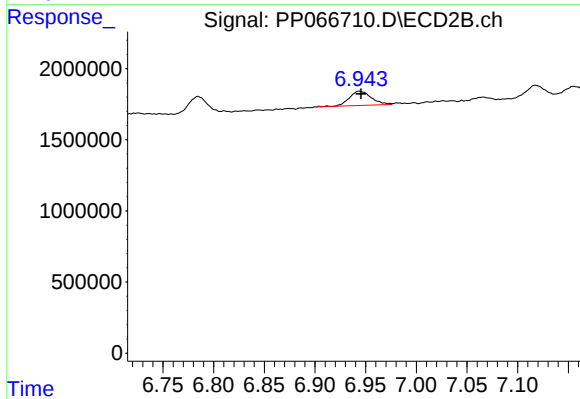

#33 AR-1260-3


R.T.: 6.944 min
Delta R.T.: -0.002 min
Response: 1507892
Conc: 23.21 ng/ml

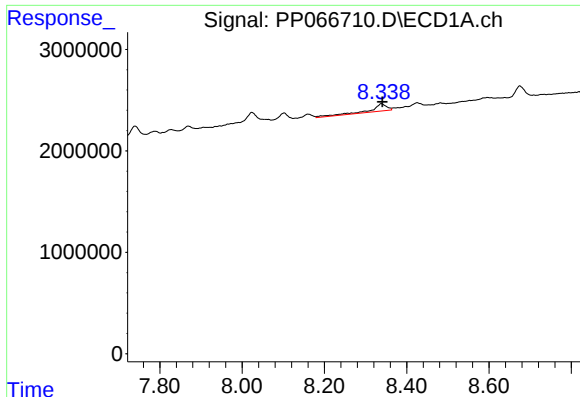

#34 AR-1260-4


R.T.: 8.339 min
Delta R.T.: -0.002 min
Response: 2068788
Conc: 39.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

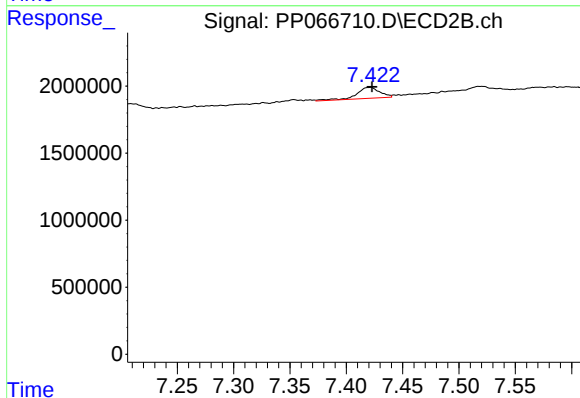


#34 AR-1260-4

R.T.: 7.421 min
Delta R.T.: -0.002 min
Response: 1168589
Conc: 25.95 ng/ml

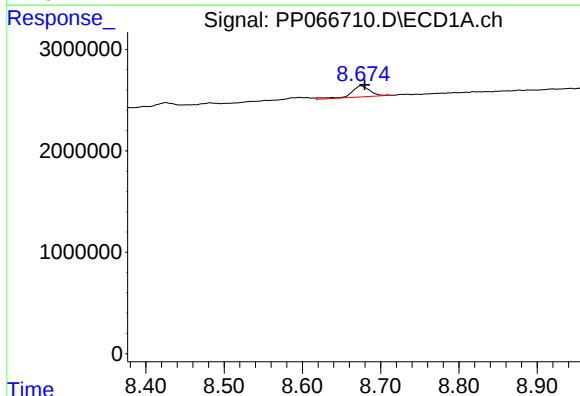


#35 AR-1260-5

R.T.: 8.675 min
Delta R.T.: -0.004 min
Response: 1806619
Conc: 20.31 ng/ml

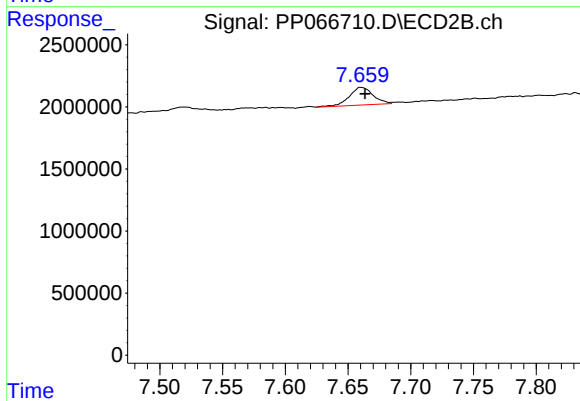

#35 AR-1260-5


R.T.: 7.661 min
Delta R.T.: -0.003 min
Response: 1890450
Conc: 19.59 ng/ml

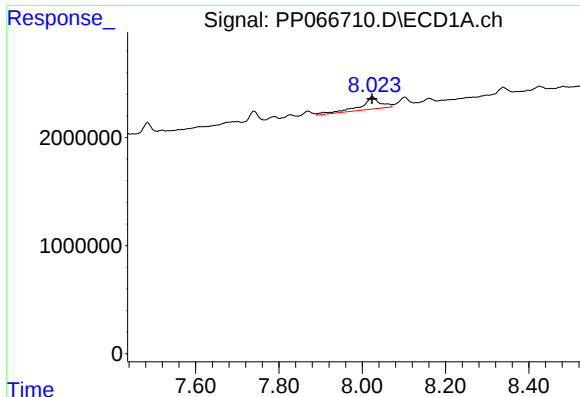

#36 AR-1262-1


R.T.: 8.024 min
Delta R.T.: 0.000 min
Response: 3720673
Conc: 82.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

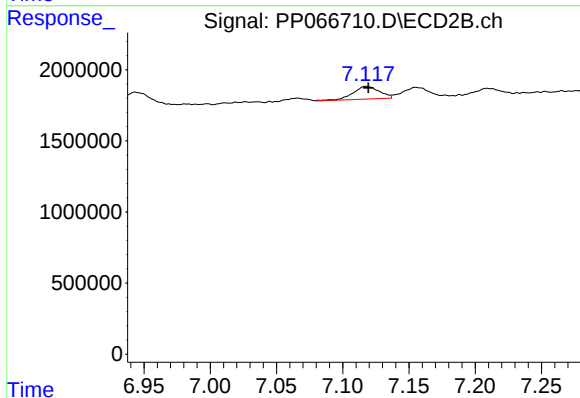


#36 AR-1262-1

R.T.: 7.118 min
Delta R.T.: -0.002 min
Response: 1233196
Conc: 38.58 ng/ml

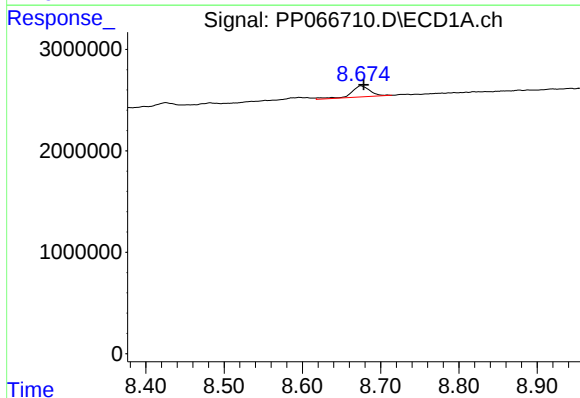


#37 AR-1262-2

R.T.: 8.675 min
Delta R.T.: -0.003 min
Response: 1806619
Conc: 16.54 ng/ml

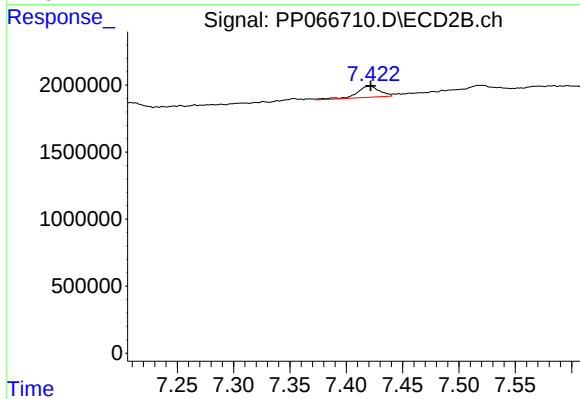

#37 AR-1262-2


R.T.: 7.421 min
Delta R.T.: 0.000 min
Response: 1168589
Conc: 18.74 ng/ml

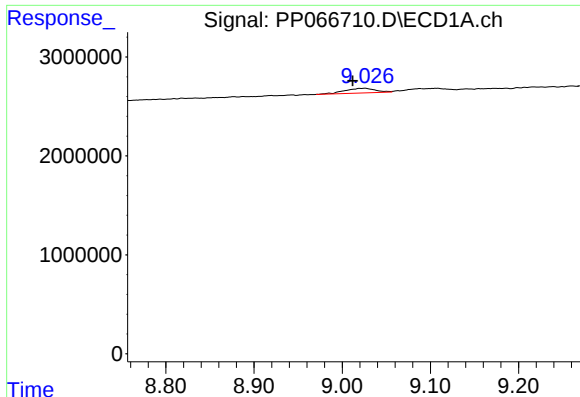

#38 AR-1262-3


R.T.: 9.025 min
Delta R.T.: 0.013 min
Response: 1129814
Conc: 15.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

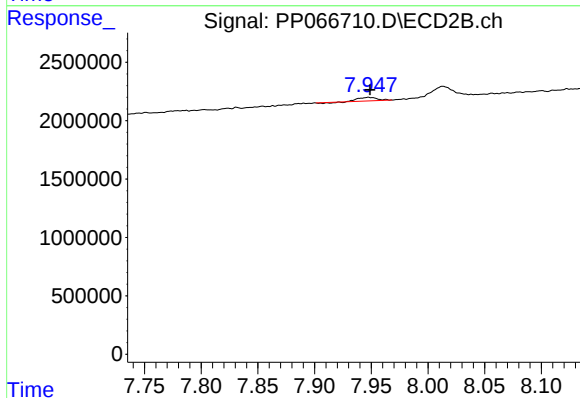


#38 AR-1262-3

R.T.: 7.948 min
Delta R.T.: -0.001 min
Response: 308656
Conc: 6.90 ng/ml

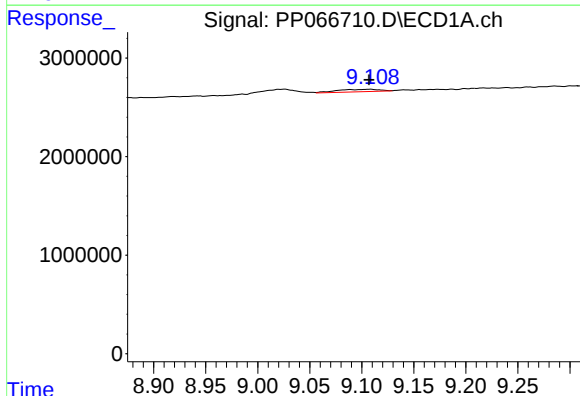


#39 AR-1262-4

R.T.: 9.107 min
Delta R.T.: 0.000 min
Response: 692794
Conc: 11.87 ng/ml

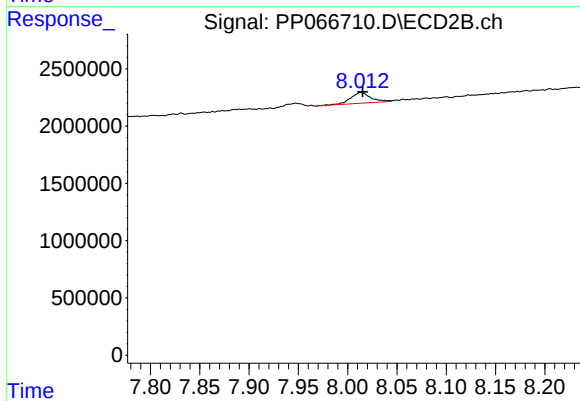

#39 AR-1262-4


R.T.: 8.013 min
Delta R.T.: -0.002 min
Response: 1325696
Conc: 15.99 ng/ml

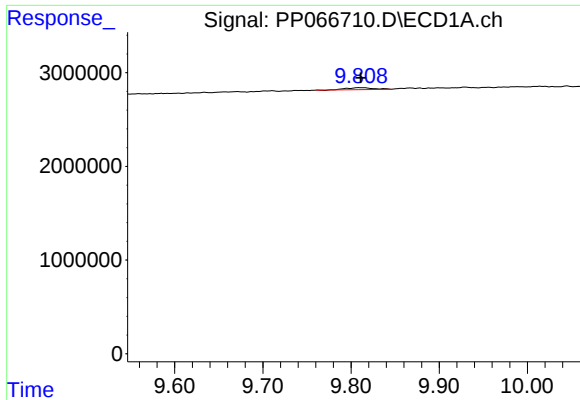

#40 AR-1262-5


R.T.: 9.811 min
Delta R.T.: 0.000 min
Response: 446795
Conc: 13.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

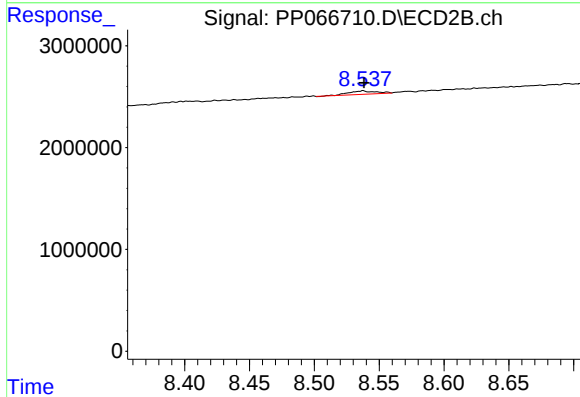


#40 AR-1262-5

R.T.: 8.538 min
Delta R.T.: 0.000 min
Response: 491792
Conc: 15.53 ng/ml

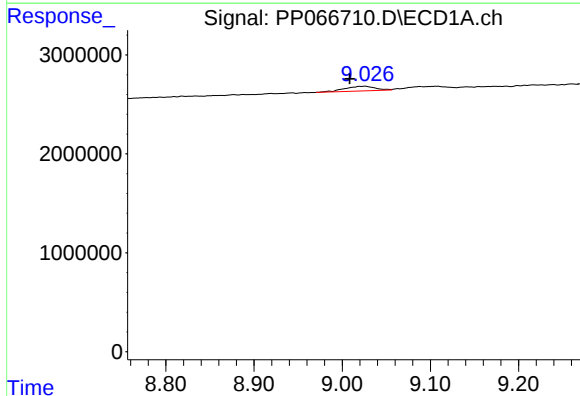


#41 AR-1268-1

R.T.: 9.025 min
Delta R.T.: 0.016 min
Response: 1129814
Conc: 9.01 ng/ml

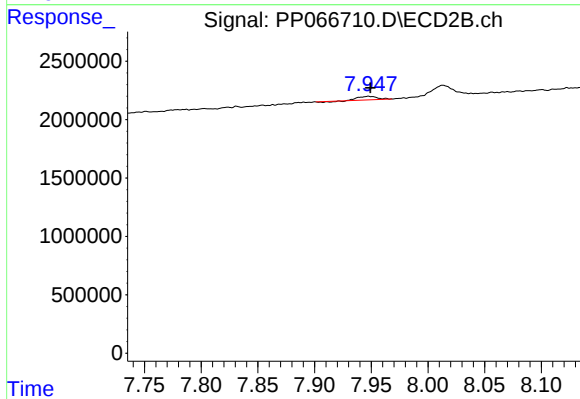

#41 AR-1268-1


R.T.: 7.948 min
Delta R.T.: -0.001 min
Response: 308656
Conc: 2.47 ng/ml

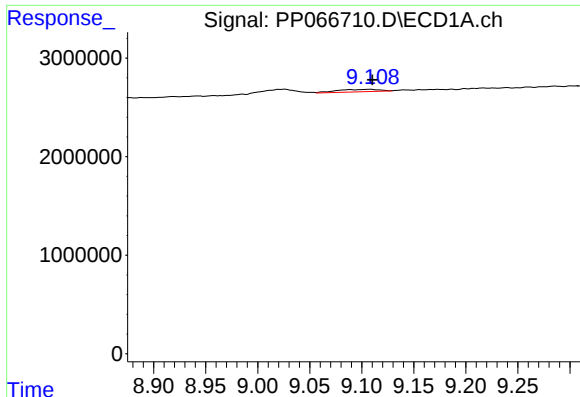

#42 AR-1268-2


R.T.: 9.107 min
Delta R.T.: -0.003 min
Response: 692794
Conc: 6.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

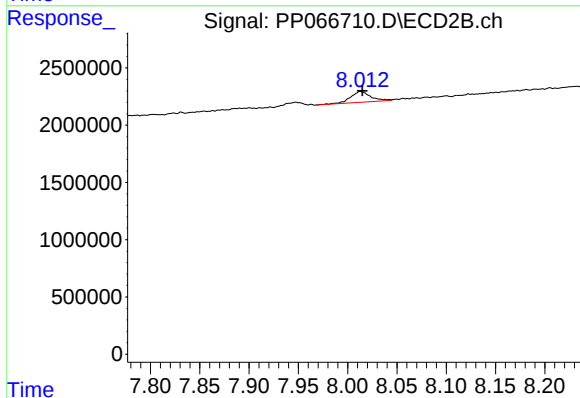


#42 AR-1268-2

R.T.: 8.013 min
Delta R.T.: -0.002 min
Response: 1325696
Conc: 11.45 ng/ml

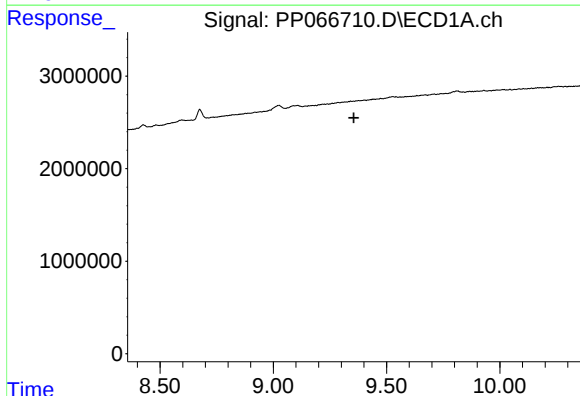


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 9.356 min
Response: 0
Conc: N.D.

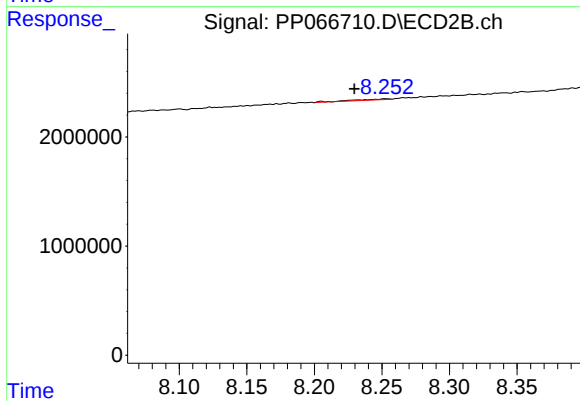

#43 AR-1268-3


R.T.: 8.253 min
Delta R.T.: 0.023 min
Response: 150646
Conc: 1.51 ng/ml

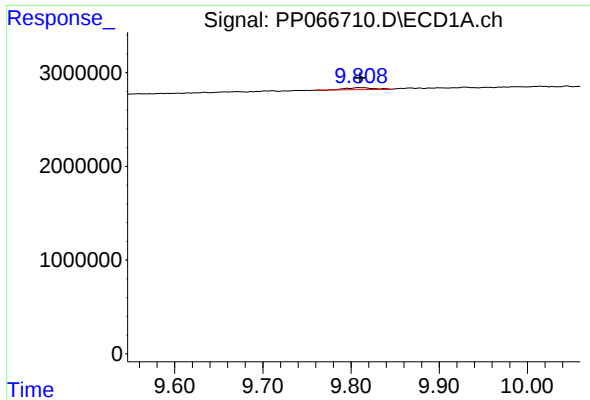

#44 AR-1268-4


R.T.: 9.811 min
Delta R.T.: 0.000 min
Response: 446795
Conc: 14.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

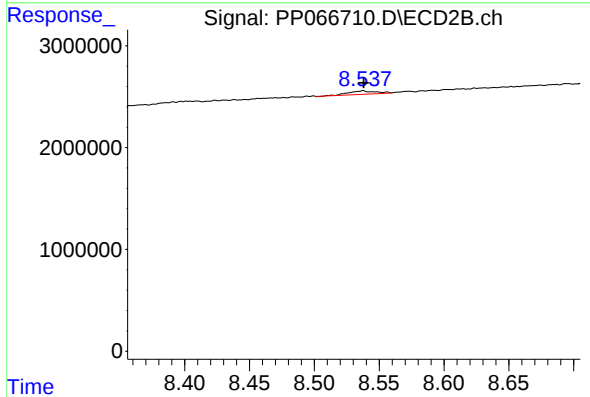


#44 AR-1268-4

R.T.: 8.538 min
Delta R.T.: 0.000 min
Response: 491792
Conc: 14.53 ng/ml

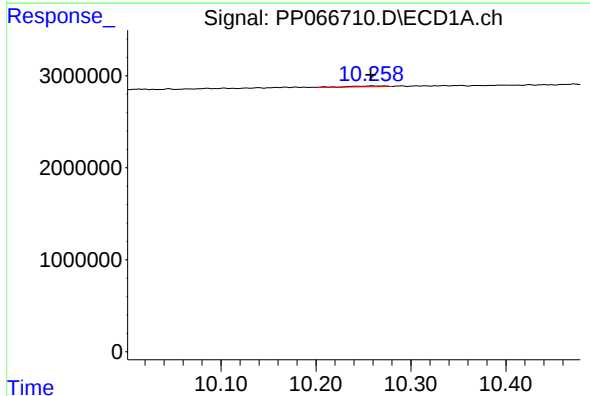

#45 AR-1268-5

R.T.: 10.259 min
Delta R.T.: 0.001 min
Response: 231440
Conc: 0.81 ng/ml

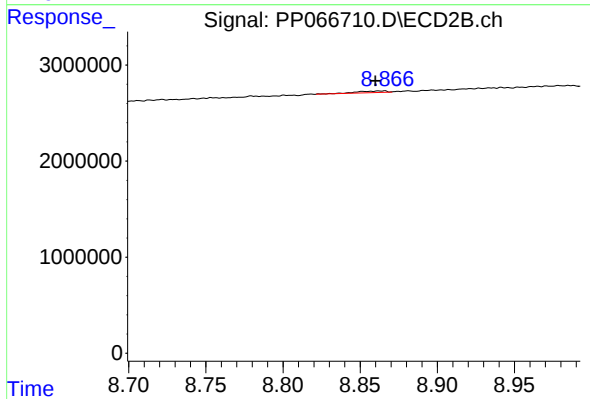

#45 AR-1268-5

R.T.: 8.865 min
Delta R.T.: 0.005 min
Response: 231571
Conc: 0.80 ng/ml