

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
 Data File : PP066712.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2024 01:24
 Operator : YP\AJ
 Sample : P3390-07
 Misc : AR1232 LOD 25 PPB
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 05:54:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 21 05:19:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.702	3.979	24593429	20429368	16.608	15.625
2)	SA Decachlor...	10.621	9.144	14238685	12640764	16.225	15.174
Target Compounds							
3)	L1 AR-1016-1	5.875	5.086	439755	337798	10.318	8.426
4)	L1 AR-1016-2	5.896	5.106	694011	602705	10.374	10.114
5)	L1 AR-1016-3	5.961	5.287	598996	232329	14.152	7.772 #
6)	L1 AR-1016-4	6.062	5.327	309938	311249	9.499	11.877 #
7)	L1 AR-1016-5	6.355	5.552	280055	325846	8.830	10.035
8)	L2 AR-1221-1	4.911	4.196	313799	133336	18.543	8.789 #
9)	L2 AR-1221-2	5.008	4.286	532769	428264	42.965	36.489
10)	L2 AR-1221-3	5.074	4.361	700937	596863	18.471	16.378
11)	L3 AR-1232-1	5.074	4.361	700937	596863	22.040	19.477
12)	L3 AR-1232-2	5.607	5.106	370946	602705	21.416	22.337
13)	L3 AR-1232-3	5.896	5.287	694011	232329	22.990	17.324
14)	L3 AR-1232-4	6.062	5.371	309938	287750	21.044	22.385
15)	L3 AR-1232-5	6.148	5.552	332445	325846	28.006	23.529
16)	L4 AR-1242-1	5.875	5.086	439755	337798	13.637	11.010
17)	L4 AR-1242-2	5.896	5.106	694011	602705	13.713	13.301
18)	L4 AR-1242-3	5.961	5.287	598996	232329	18.956	9.946 #
19)	L4 AR-1242-4	6.062	5.371	309938	287750	12.507	11.435
20)	L4 AR-1242-5	6.800	5.906	415442	320080	16.533	11.316 #
21)	L5 AR-1248-1	5.875	5.086	439755	337798	17.206	13.952
22)	L5 AR-1248-2	6.148	5.327	332445	311249	8.274	8.618
23)	L5 AR-1248-3	6.355	5.371	280055	287750	6.423	7.707
24)	L5 AR-1248-4	6.759	5.552	320122	325846	7.246	7.385
25)	L5 AR-1248-5	6.800	5.949	415442	329838	9.062	8.732
26)	L6 AR-1254-1	6.735	5.906	329004	320080	6.664	5.343
27)	L6 AR-1254-2	6.962	6.055	522776	187359	7.165	3.506 #
28)	L6 AR-1254-3	7.326	6.466	240058	453278	3.436	5.732 #
29)	L6 AR-1254-4	7.607	0.000	84554	0	1.899	N.D. #
30)	L6 AR-1254-5	8.021	0.000	1598328	0	24.109	N.D. #
31)	L7 AR-1260-1	0.000	6.613	0	179117	N.D.	3.030 #
32)	L7 AR-1260-2	7.742	6.783	264525	180452	4.155	2.648 #
33)	L7 AR-1260-3	8.104	6.957	181662	411260	4.085	6.330 #
34)	L7 AR-1260-4	8.352	0.000	1636848	0	31.013	N.D. #
35)	L7 AR-1260-5	8.693	7.659	692844	134332	7.789	1.392 #
36)	L8 AR-1262-1	8.021	0.000	1598328	0	35.400	N.D. #
37)	L8 AR-1262-2	8.693	0.000	692844	0	6.345	N.D. #
38)	L8 AR-1262-3	9.005	0.000	60853	0	0.857	N.D. #
39)	L8 AR-1262-4	9.110	0.000	27604	0	0.473	N.D. #
41)	L9 AR-1268-1	9.005	0.000	60853	0	0.486	N.D. #
42)	L9 AR-1268-2	9.110	0.000	27604	0	0.250	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
Data File : PP066712.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2024 01:24
Operator : YP\AJ
Sample : P3390-07
Misc : AR1232 LOD 25 PPB
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 05:54:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 21 05:19:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43)	L9 AR-1268-3	9.357	8.257f	137203	57395	1.383	0.576 #
45)	L9 AR-1268-5	0.000	8.864	0	134468	N.D.	0.463 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
Data File : PP066712.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2024 01:24
Operator : YP\AJ
Sample : P3390-07
Misc : AR1232 LOD 25 PPB
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 05:54:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 21 05:19:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

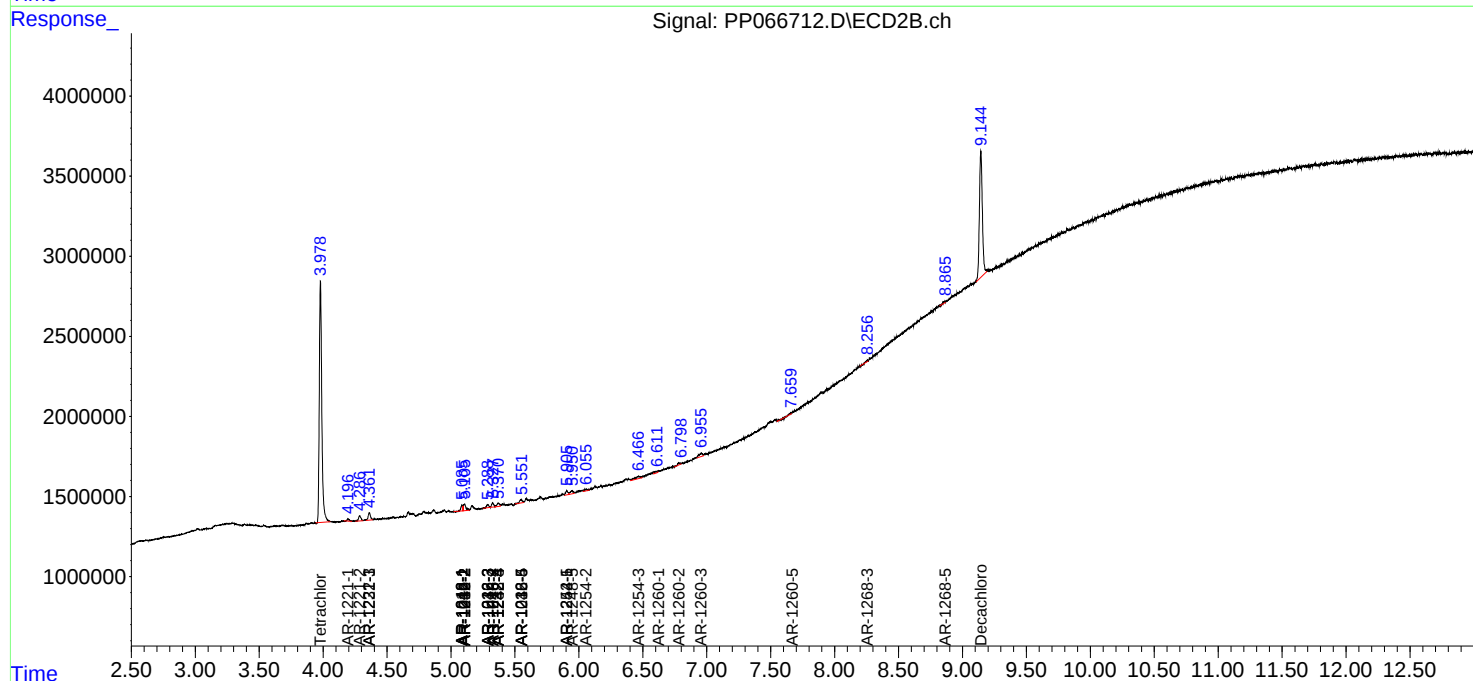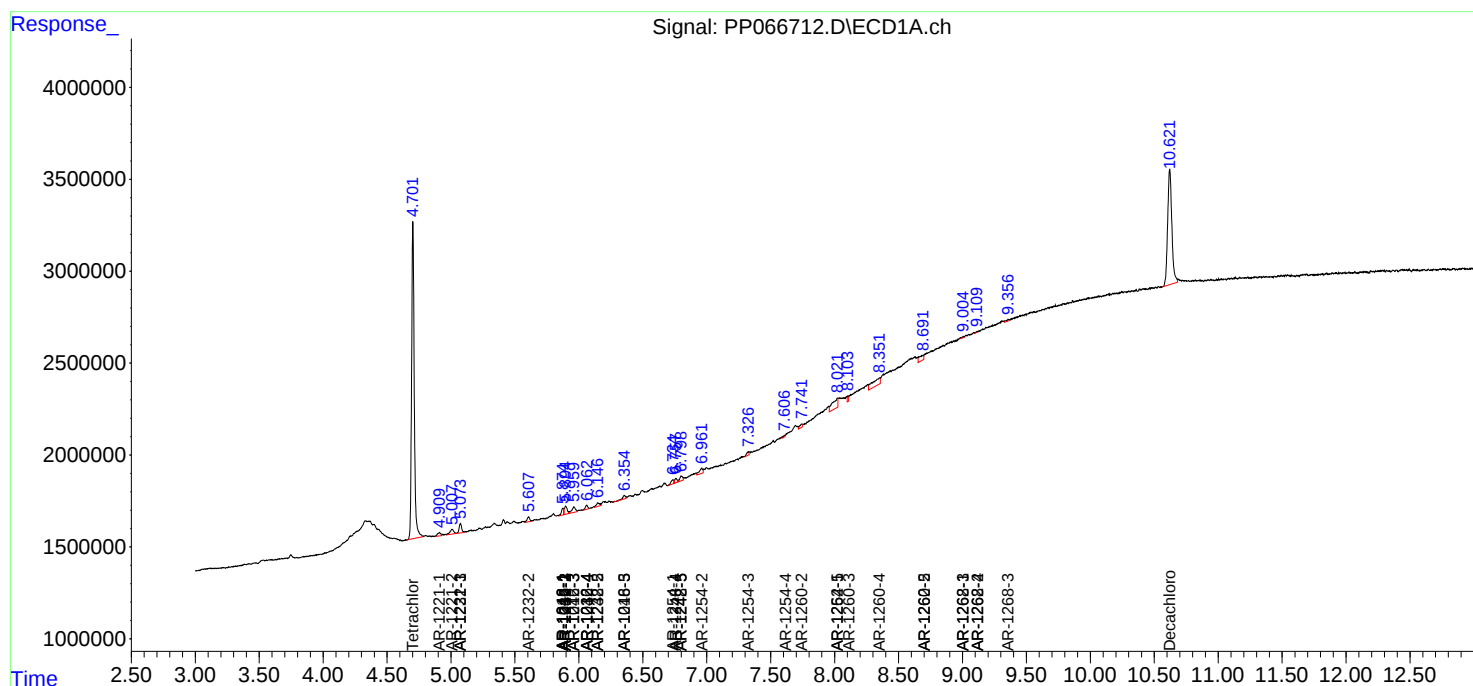


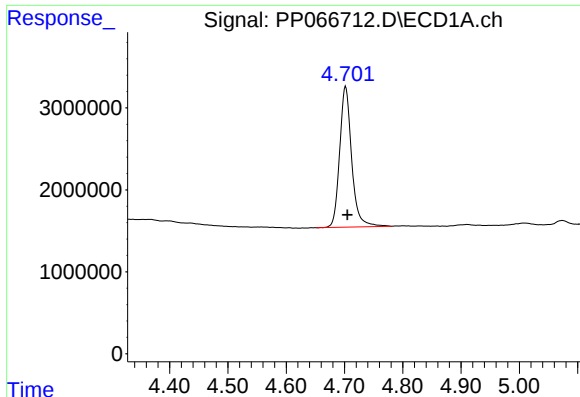

#1 Tetrachloro-m-xylene


R.T.: 4.702 min
Delta R.T.: -0.003 min
Response: 24593429
Conc: 16.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

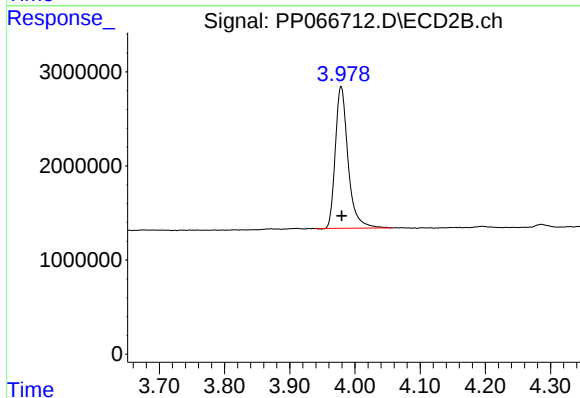


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.001 min
Response: 20429368
Conc: 15.62 ng/ml

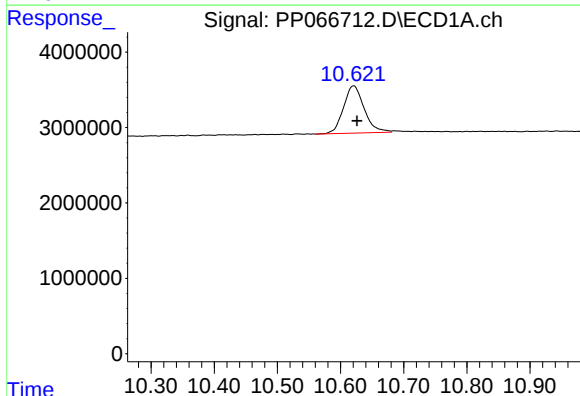


#2 Decachlorobiphenyl

R.T.: 10.621 min
Delta R.T.: -0.005 min
Response: 14238685
Conc: 16.23 ng/ml

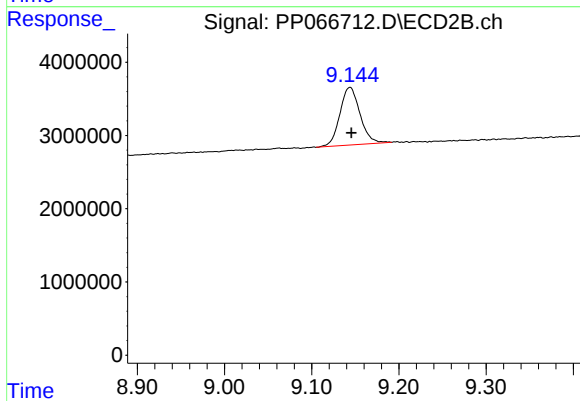

#2 Decachlorobiphenyl


R.T.: 9.144 min
Delta R.T.: -0.002 min
Response: 12640764
Conc: 15.17 ng/ml

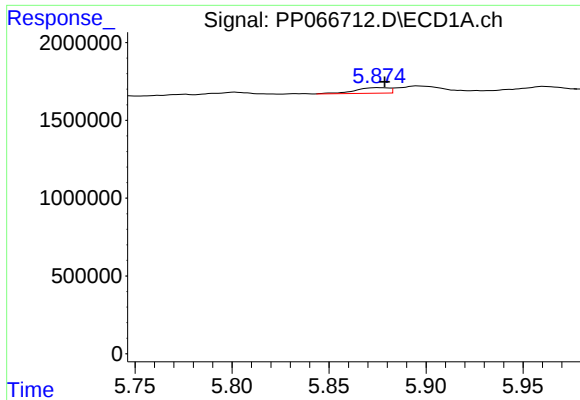

#3 AR-1016-1


R.T.: 5.875 min
Delta R.T.: -0.003 min
Response: 439755
Conc: 10.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

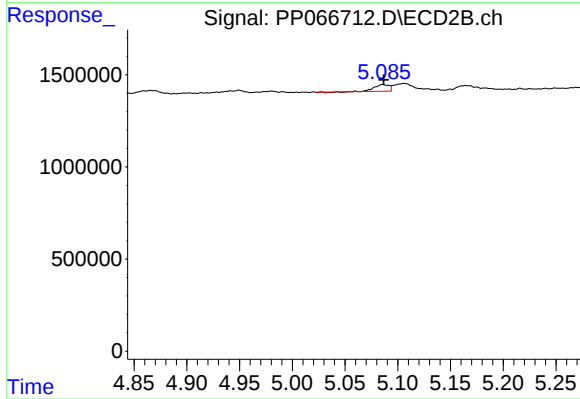


#3 AR-1016-1

R.T.: 5.086 min
Delta R.T.: 0.000 min
Response: 337798
Conc: 8.43 ng/ml

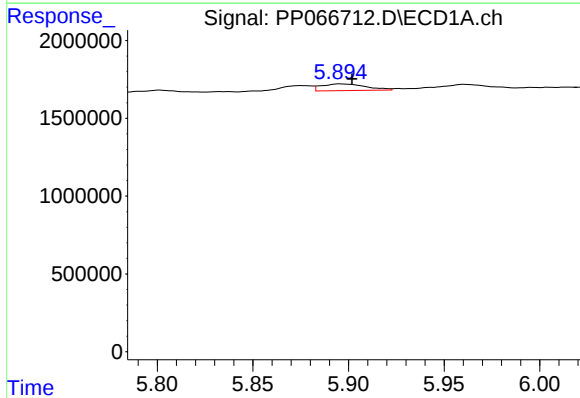


#4 AR-1016-2

R.T.: 5.896 min
Delta R.T.: -0.006 min
Response: 694011
Conc: 10.37 ng/ml

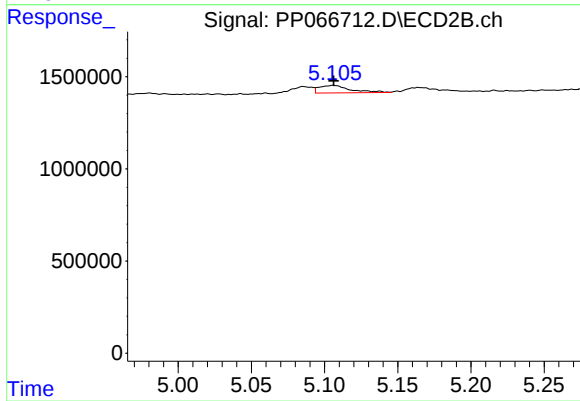

#4 AR-1016-2


R.T.: 5.106 min
Delta R.T.: 0.000 min
Response: 602705
Conc: 10.11 ng/ml

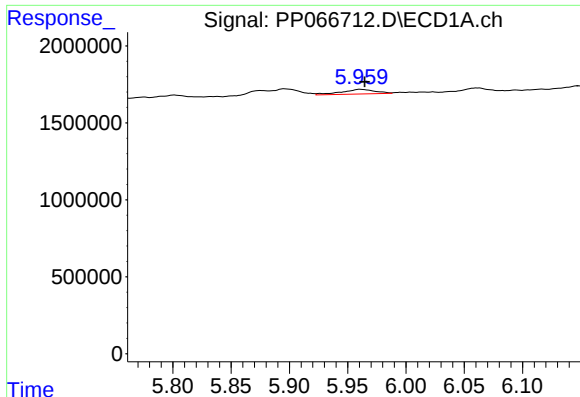

#5 AR-1016-3


R.T.: 5.961 min
Delta R.T.: -0.004 min
Response: 598996
Conc: 14.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

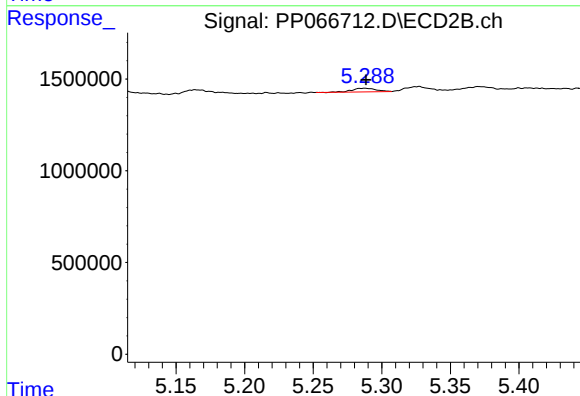


#5 AR-1016-3

R.T.: 5.287 min
Delta R.T.: -0.001 min
Response: 232329
Conc: 7.77 ng/ml

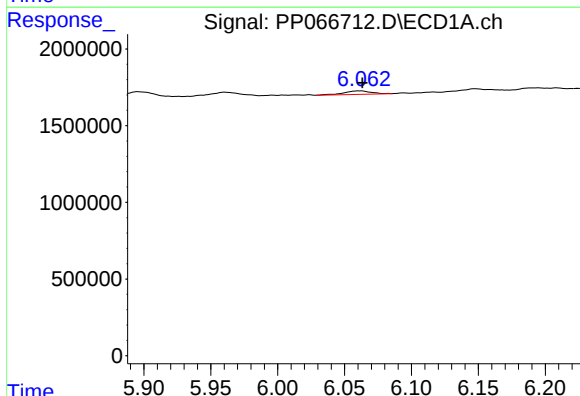


#6 AR-1016-4

R.T.: 6.062 min
Delta R.T.: -0.001 min
Response: 309938
Conc: 9.50 ng/ml

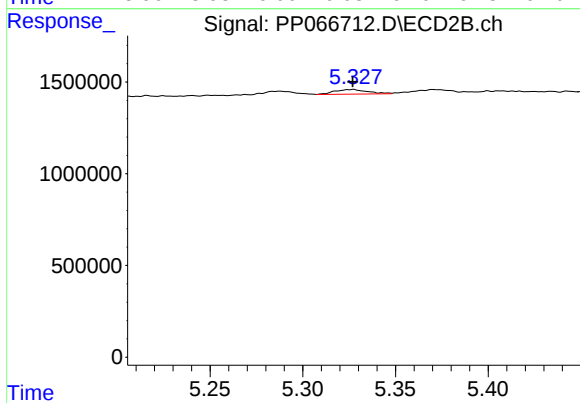

#6 AR-1016-4


R.T.: 5.327 min
Delta R.T.: 0.000 min
Response: 311249
Conc: 11.88 ng/ml

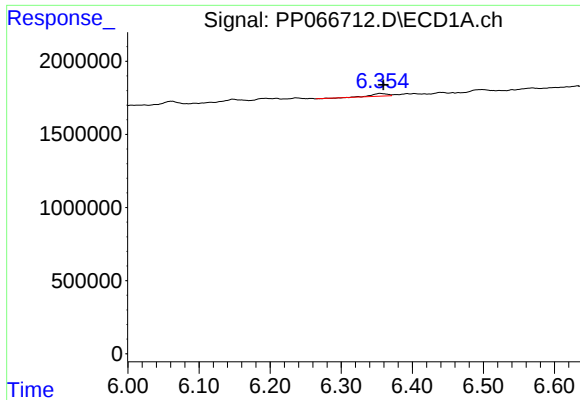

#7 AR-1016-5


R.T.: 6.355 min
Delta R.T.: -0.004 min
Response: 280055
Conc: 8.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

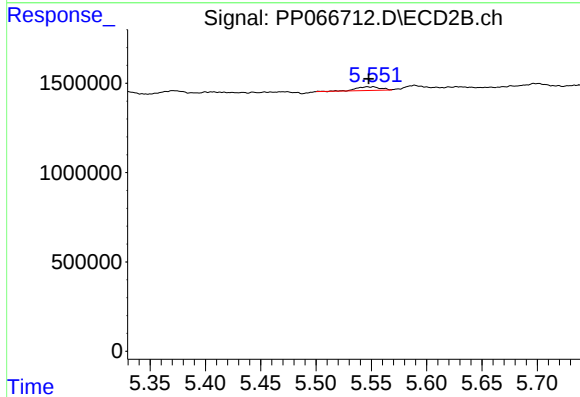


#7 AR-1016-5

R.T.: 5.552 min
Delta R.T.: 0.004 min
Response: 325846
Conc: 10.03 ng/ml

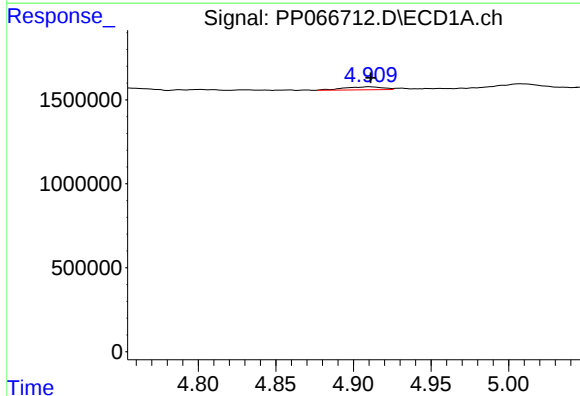


#8 AR-1221-1

R.T.: 4.911 min
Delta R.T.: 0.000 min
Response: 313799
Conc: 18.54 ng/ml

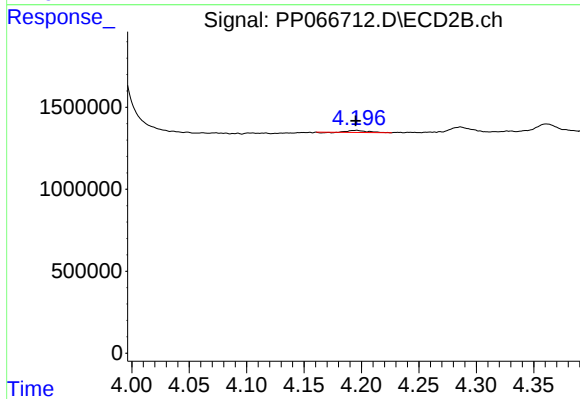

#8 AR-1221-1


R.T.: 4.196 min
Delta R.T.: 0.000 min
Response: 133336
Conc: 8.79 ng/ml

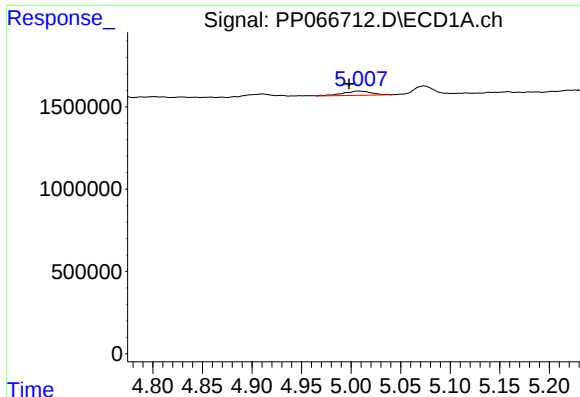

#9 AR-1221-2


R.T.: 5.008 min
Delta R.T.: 0.010 min
Response: 532769
Conc: 42.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

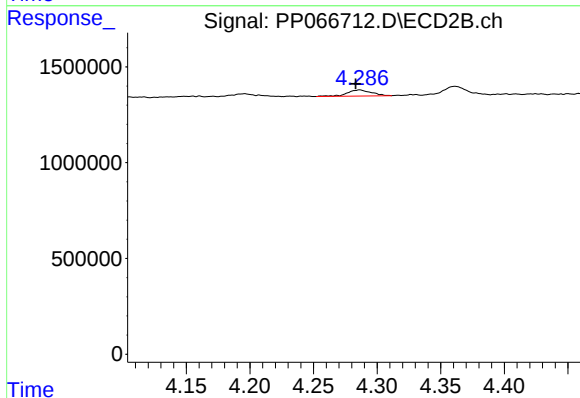


#9 AR-1221-2

R.T.: 4.286 min
Delta R.T.: 0.003 min
Response: 428264
Conc: 36.49 ng/ml

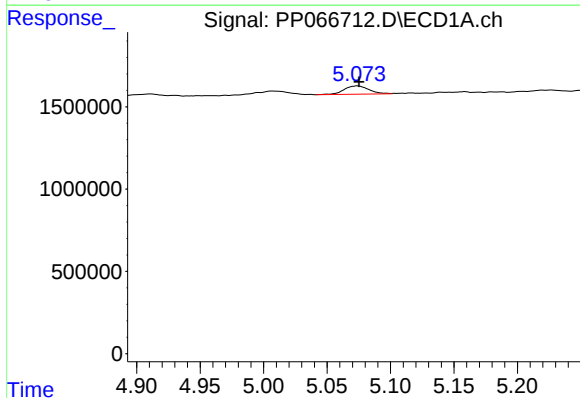


#10 AR-1221-3

R.T.: 5.074 min
Delta R.T.: -0.001 min
Response: 700937
Conc: 18.47 ng/ml

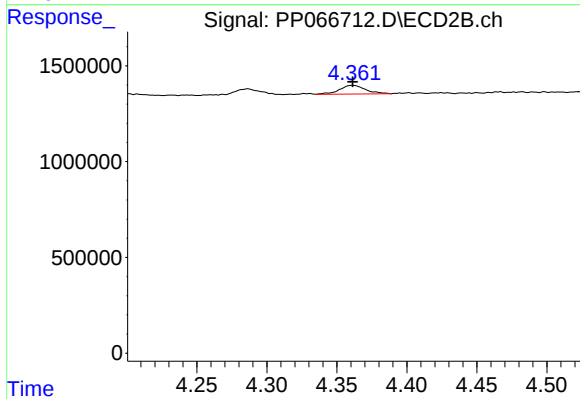

#10 AR-1221-3


R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 596863
Conc: 16.38 ng/ml

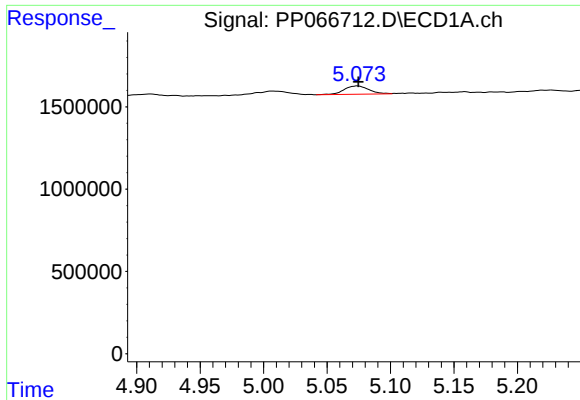

#11 AR-1232-1


R.T.: 5.074 min
Delta R.T.: 0.000 min
Response: 700937
Conc: 22.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

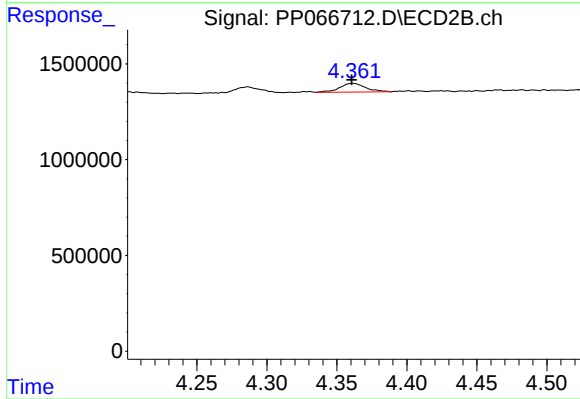


#11 AR-1232-1

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 596863
Conc: 19.48 ng/ml

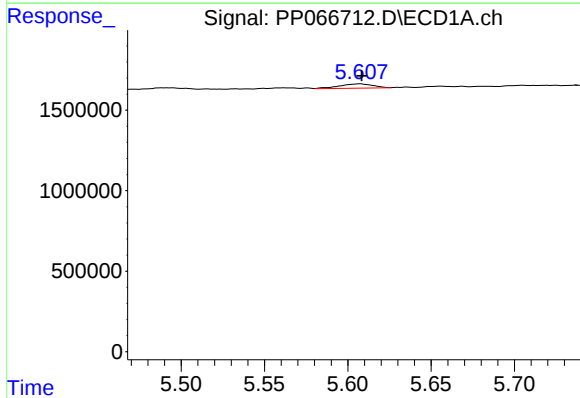


#12 AR-1232-2

R.T.: 5.607 min
Delta R.T.: -0.001 min
Response: 370946
Conc: 21.42 ng/ml

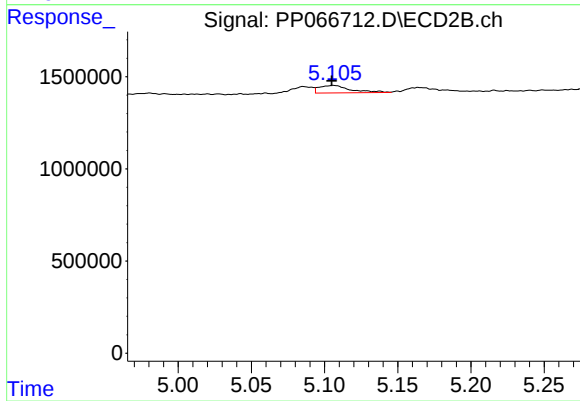

#12 AR-1232-2


R.T.: 5.106 min
Delta R.T.: 0.001 min
Response: 602705
Conc: 22.34 ng/ml

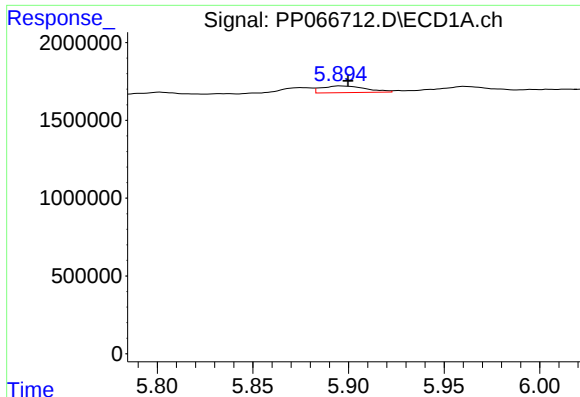

#13 AR-1232-3


R.T.: 5.896 min
Delta R.T.: -0.004 min
Response: 694011
Conc: 22.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

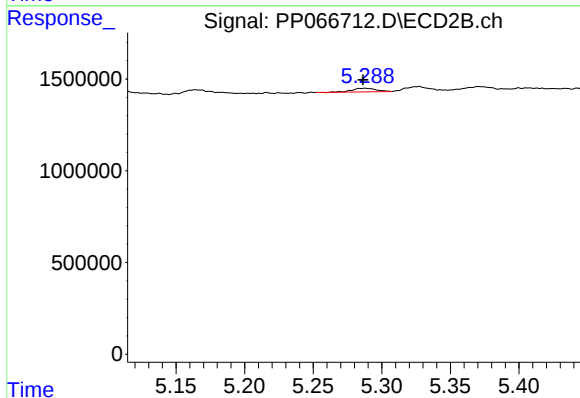


#13 AR-1232-3

R.T.: 5.287 min
Delta R.T.: 0.001 min
Response: 232329
Conc: 17.32 ng/ml

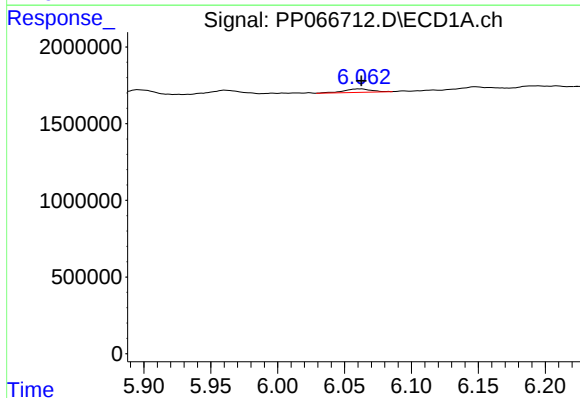


#14 AR-1232-4

R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 309938
Conc: 21.04 ng/ml

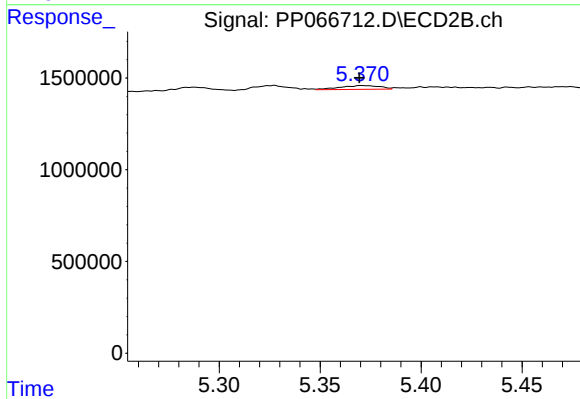

#14 AR-1232-4


R.T.: 5.371 min
Delta R.T.: 0.002 min
Response: 287750
Conc: 22.39 ng/ml

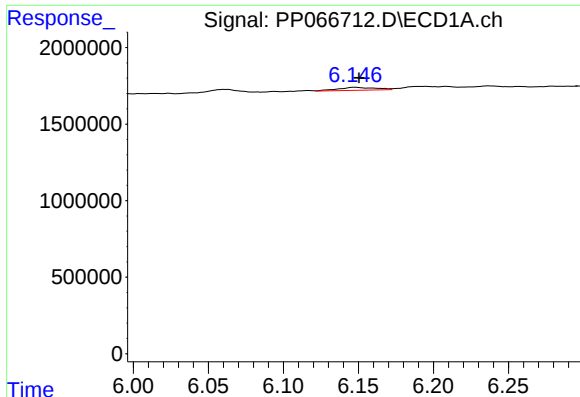

#15 AR-1232-5


R.T.: 6.148 min
Delta R.T.: -0.003 min
Response: 332445
Conc: 28.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

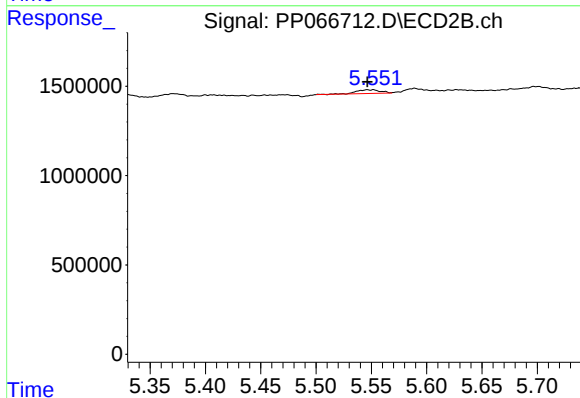


#15 AR-1232-5

R.T.: 5.552 min
Delta R.T.: 0.005 min
Response: 325846
Conc: 23.53 ng/ml

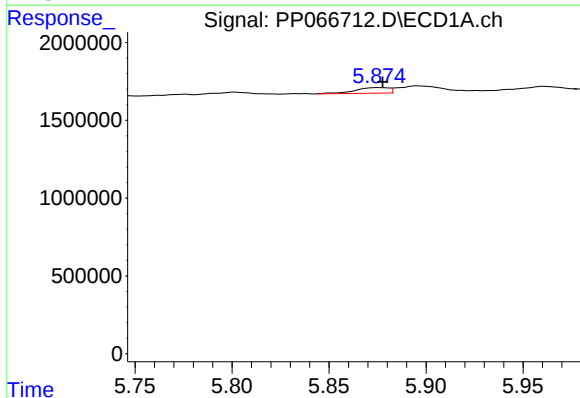


#16 AR-1242-1

R.T.: 5.875 min
Delta R.T.: -0.002 min
Response: 439755
Conc: 13.64 ng/ml

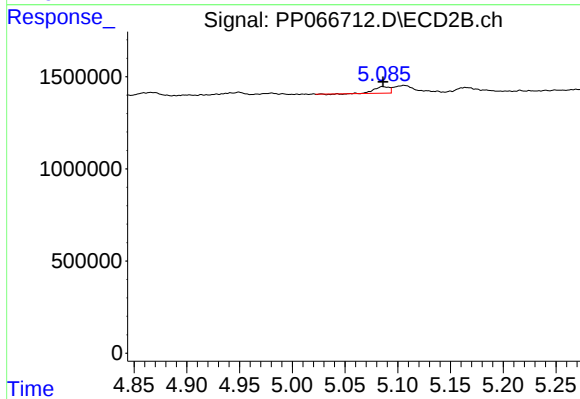

#16 AR-1242-1


R.T.: 5.086 min
Delta R.T.: 0.000 min
Response: 337798
Conc: 11.01 ng/ml

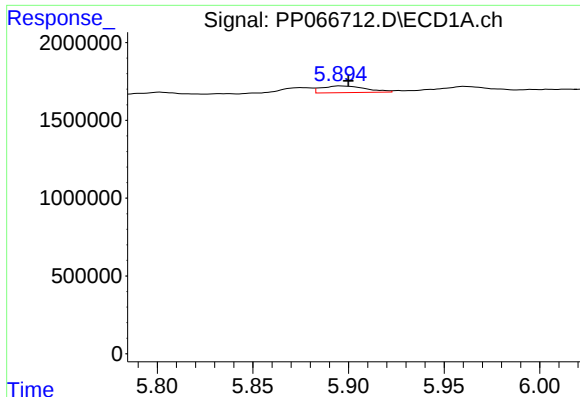

#17 AR-1242-2


R.T.: 5.896 min
Delta R.T.: -0.004 min
Response: 694011
Conc: 13.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

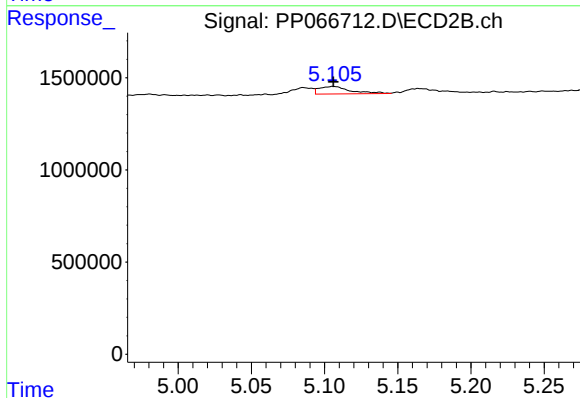


#17 AR-1242-2

R.T.: 5.106 min
Delta R.T.: 0.000 min
Response: 602705
Conc: 13.30 ng/ml

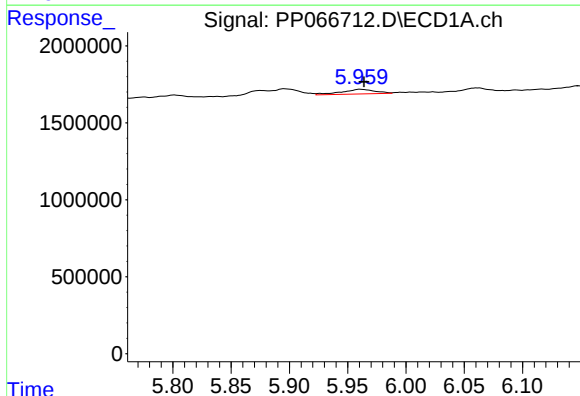


#18 AR-1242-3

R.T.: 5.961 min
Delta R.T.: -0.003 min
Response: 598996
Conc: 18.96 ng/ml

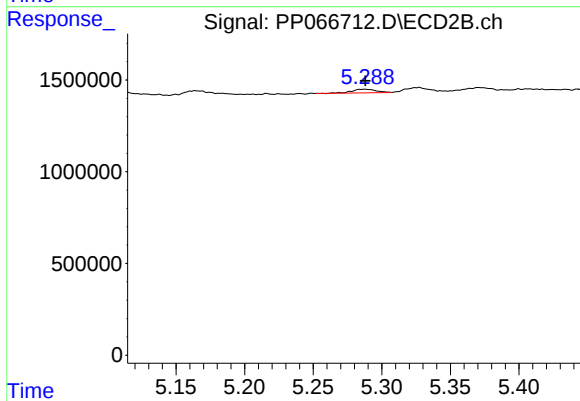

#18 AR-1242-3


R.T.: 5.287 min
Delta R.T.: 0.000 min
Response: 232329
Conc: 9.95 ng/ml

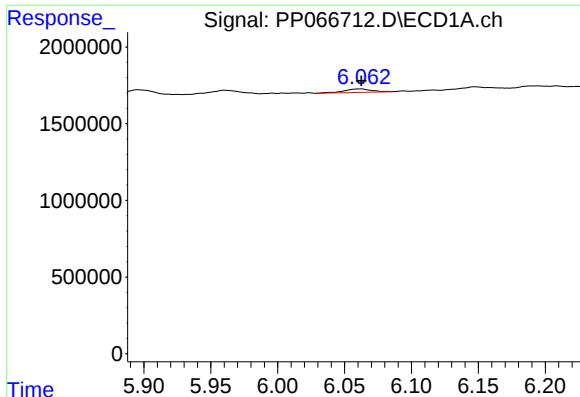

#19 AR-1242-4


R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 309938
Conc: 12.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

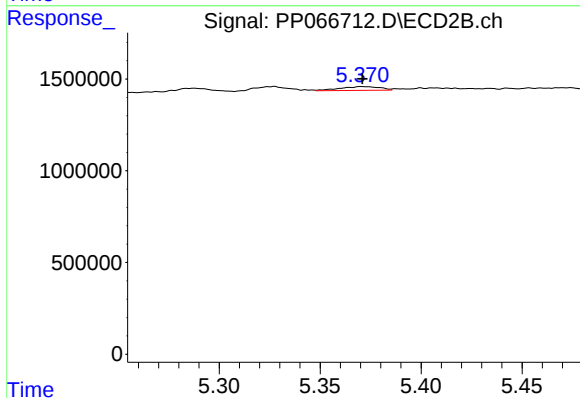


#19 AR-1242-4

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 287750
Conc: 11.44 ng/ml

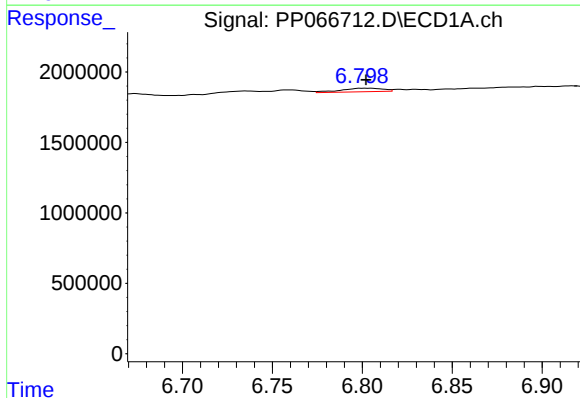


#20 AR-1242-5

R.T.: 6.800 min
Delta R.T.: -0.002 min
Response: 415442
Conc: 16.53 ng/ml

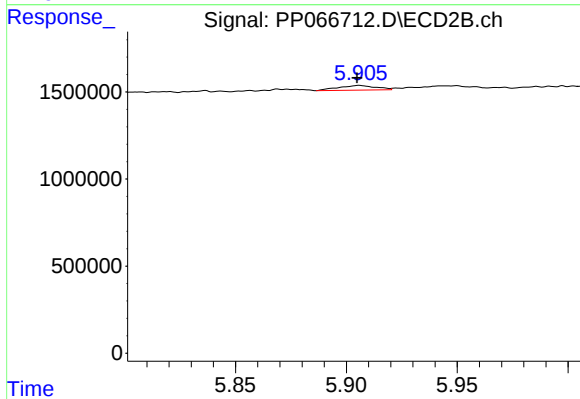

#20 AR-1242-5


R.T.: 5.906 min
Delta R.T.: 0.001 min
Response: 320080
Conc: 11.32 ng/ml

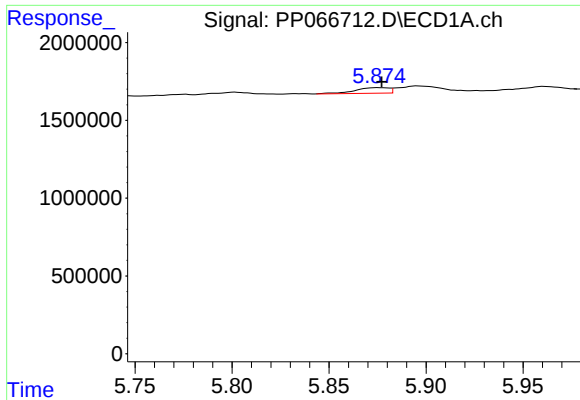

#21 AR-1248-1


R.T.: 5.875 min
Delta R.T.: -0.002 min
Response: 439755
Conc: 17.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

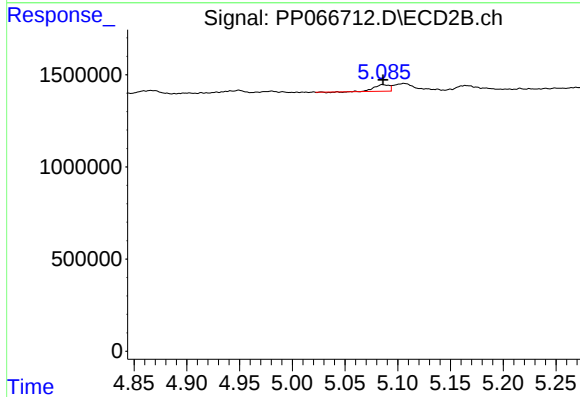


#21 AR-1248-1

R.T.: 5.086 min
Delta R.T.: 0.000 min
Response: 337798
Conc: 13.95 ng/ml

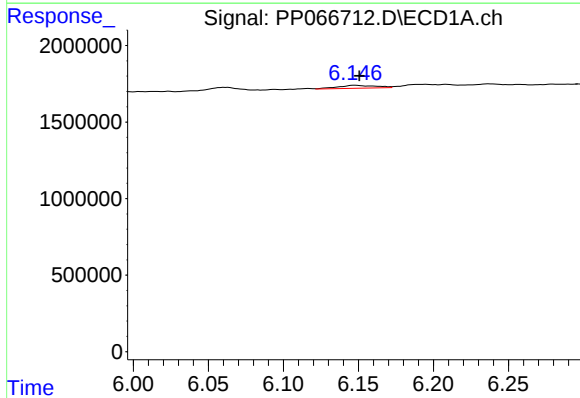


#22 AR-1248-2

R.T.: 6.148 min
Delta R.T.: -0.003 min
Response: 332445
Conc: 8.27 ng/ml

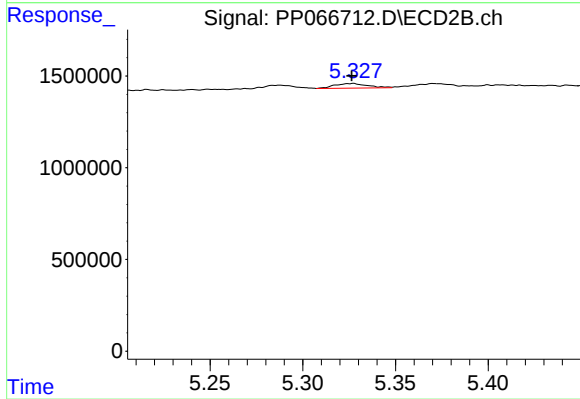

#22 AR-1248-2


R.T.: 5.327 min
Delta R.T.: 0.000 min
Response: 311249
Conc: 8.62 ng/ml

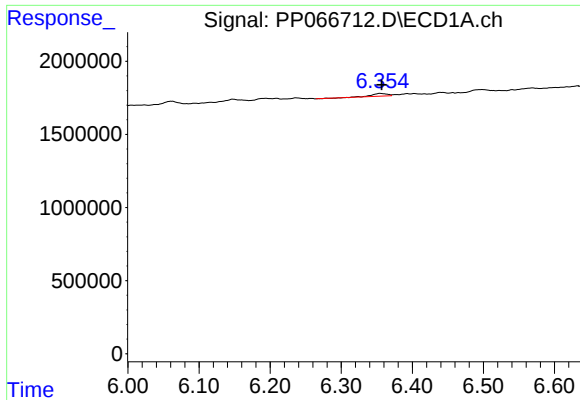

#23 AR-1248-3


R.T.: 6.355 min
Delta R.T.: -0.002 min
Response: 280055
Conc: 6.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

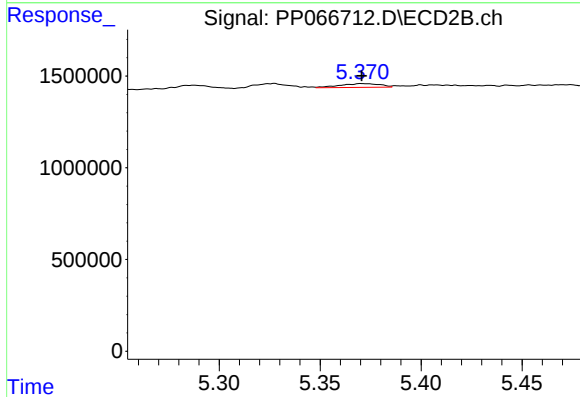


#23 AR-1248-3

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 287750
Conc: 7.71 ng/ml

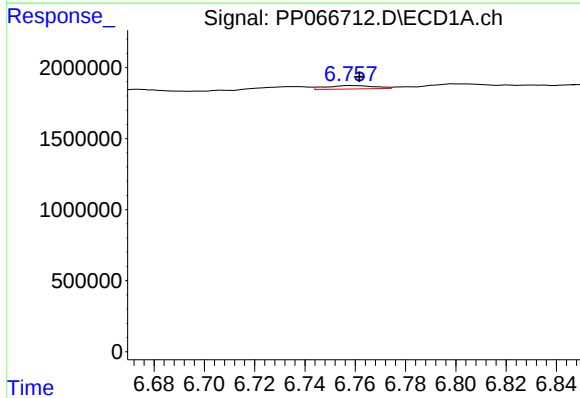


#24 AR-1248-4

R.T.: 6.759 min
Delta R.T.: -0.003 min
Response: 320122
Conc: 7.25 ng/ml

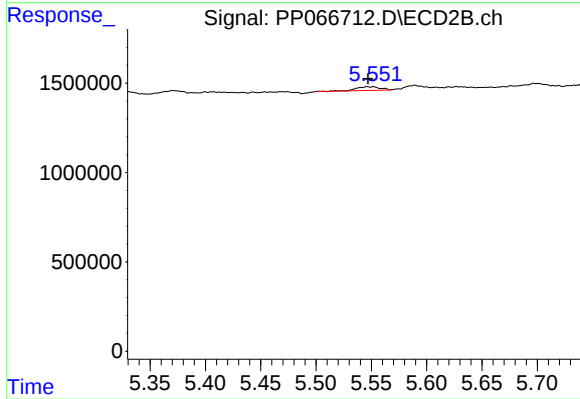

#24 AR-1248-4


R.T.: 5.552 min
Delta R.T.: 0.005 min
Response: 325846
Conc: 7.38 ng/ml

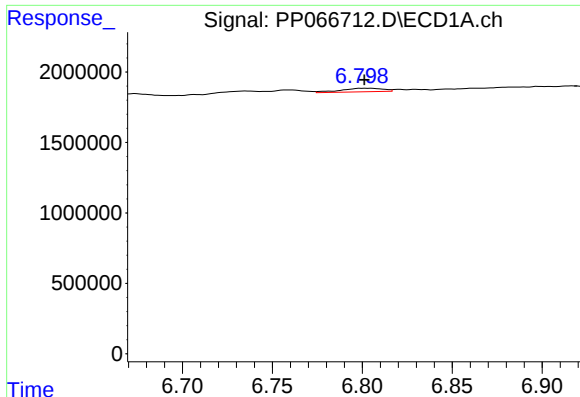

#25 AR-1248-5


R.T.: 6.800 min
Delta R.T.: -0.001 min
Response: 415442
Conc: 9.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

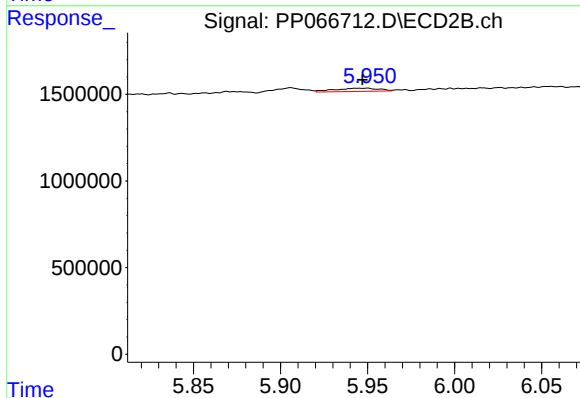


#25 AR-1248-5

R.T.: 5.949 min
Delta R.T.: 0.002 min
Response: 329838
Conc: 8.73 ng/ml

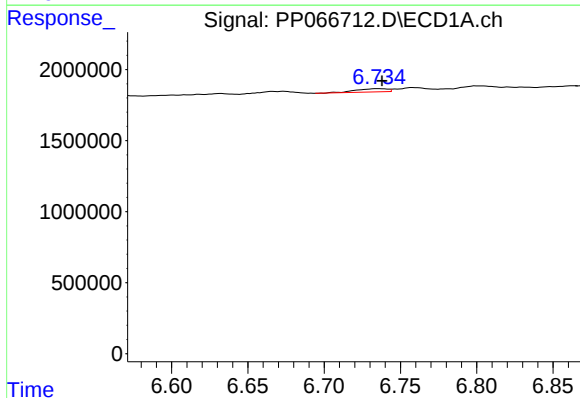


#26 AR-1254-1

R.T.: 6.735 min
Delta R.T.: -0.003 min
Response: 329004
Conc: 6.66 ng/ml

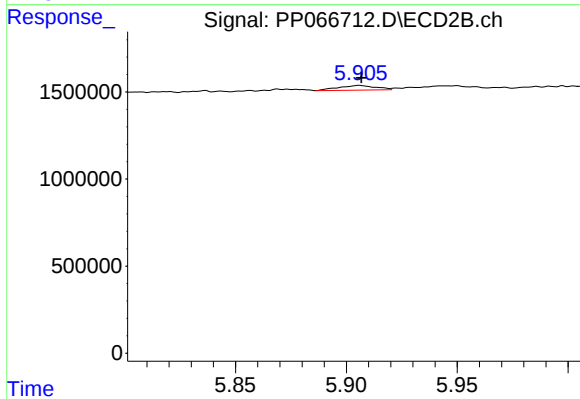

#26 AR-1254-1


R.T.: 5.906 min
Delta R.T.: 0.000 min
Response: 320080
Conc: 5.34 ng/ml

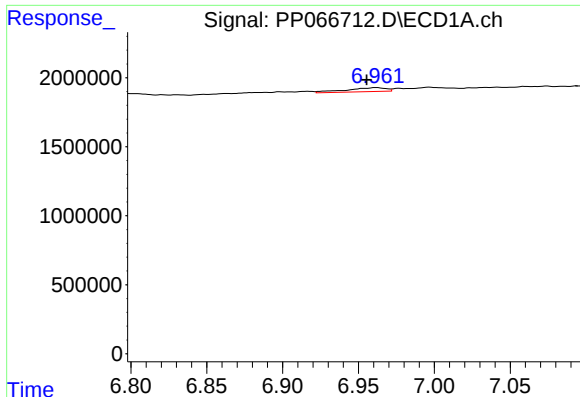

#27 AR-1254-2


R.T.: 6.962 min
Delta R.T.: 0.006 min
Response: 522776
Conc: 7.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

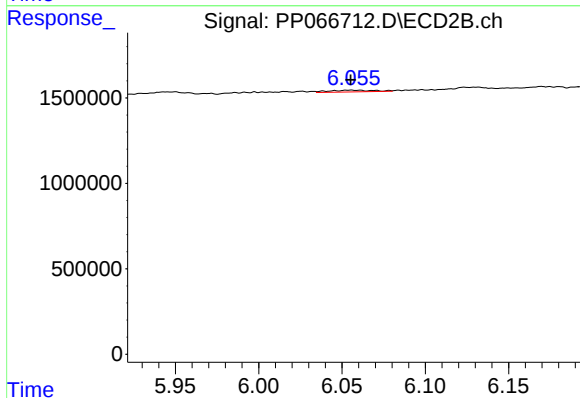


#27 AR-1254-2

R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 187359
Conc: 3.51 ng/ml

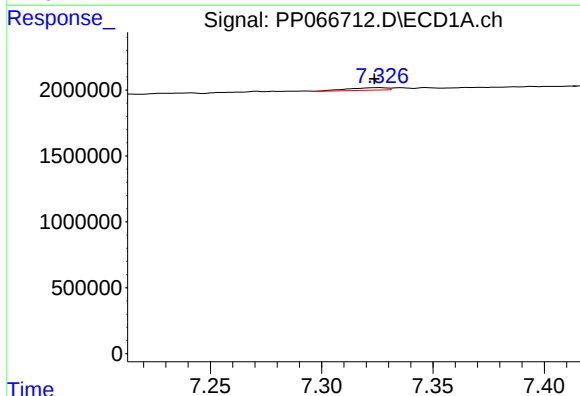


#28 AR-1254-3

R.T.: 7.326 min
Delta R.T.: 0.002 min
Response: 240058
Conc: 3.44 ng/ml

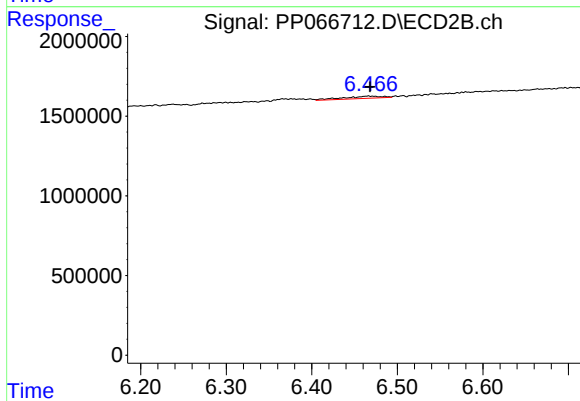

#28 AR-1254-3


R.T.: 6.466 min
Delta R.T.: -0.002 min
Response: 453278
Conc: 5.73 ng/ml

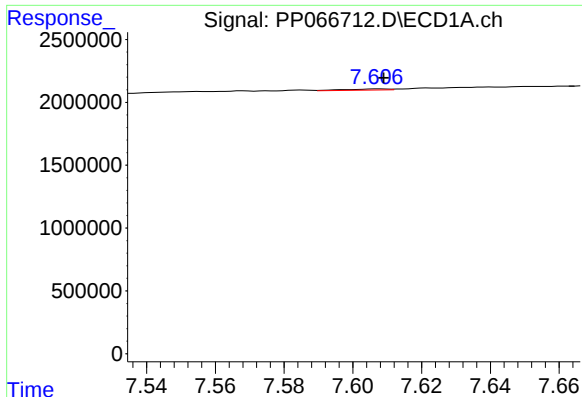

#29 AR-1254-4


R.T.: 7.607 min
Delta R.T.: -0.002 min
Response: 84554
Conc: 1.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

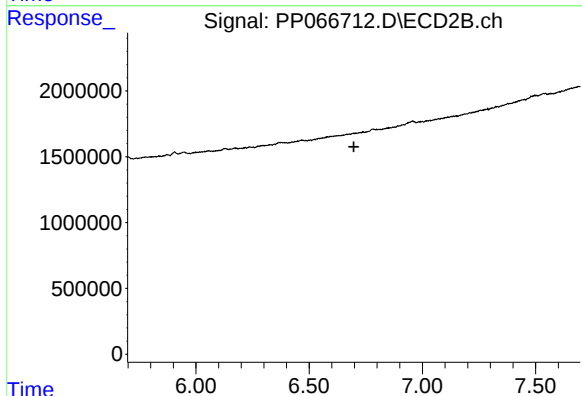


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.697 min
Response: 0
Conc: N.D.

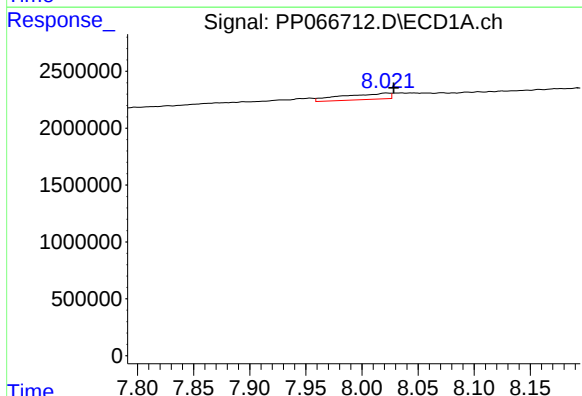


#30 AR-1254-5

R.T.: 8.021 min
Delta R.T.: -0.007 min
Response: 1598328
Conc: 24.11 ng/ml

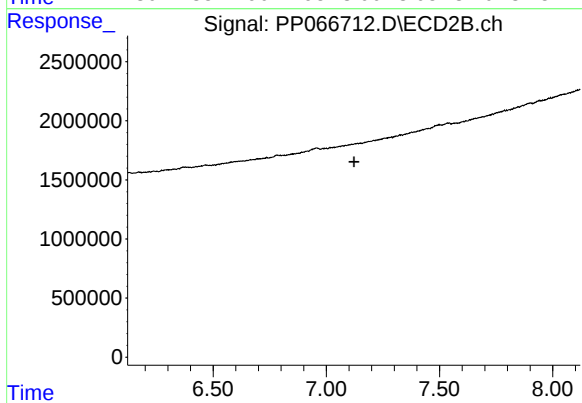

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.122 min
Response: 0
Conc: N.D.

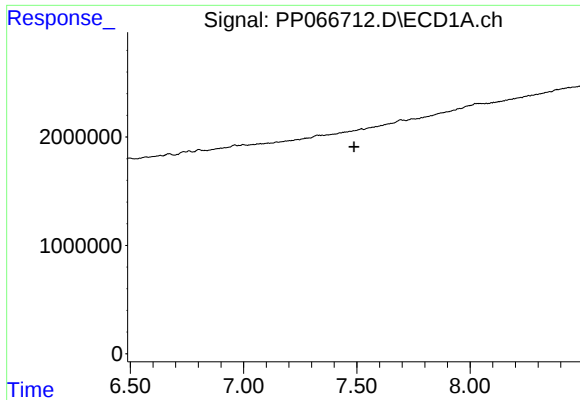

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

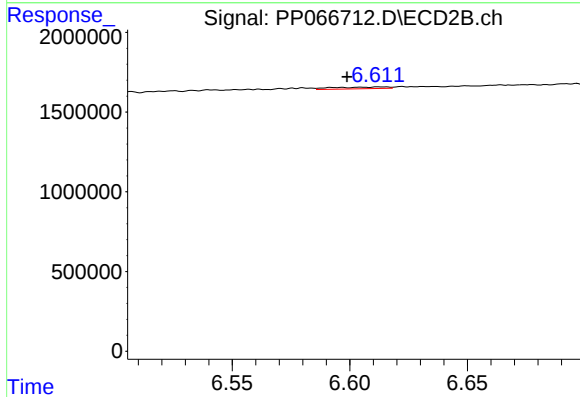


#31 AR-1260-1

R.T.: 6.613 min
Delta R.T.: 0.014 min
Response: 179117
Conc: 3.03 ng/ml

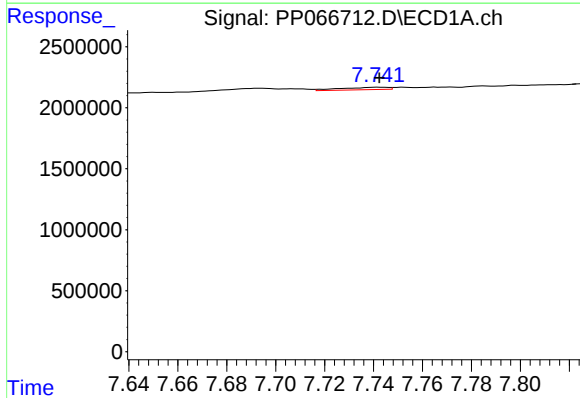


#32 AR-1260-2

R.T.: 7.742 min
Delta R.T.: 0.000 min
Response: 264525
Conc: 4.16 ng/ml

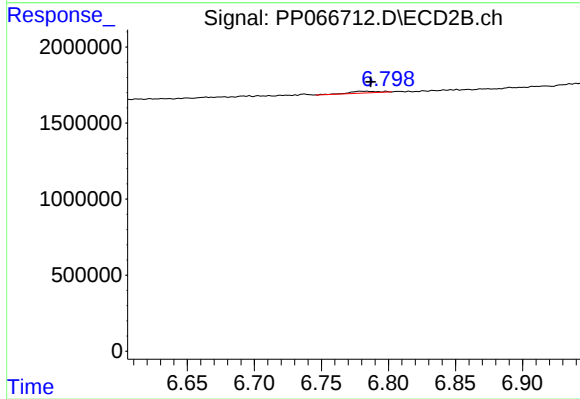

#32 AR-1260-2


R.T.: 6.783 min
Delta R.T.: -0.004 min
Response: 180452
Conc: 2.65 ng/ml

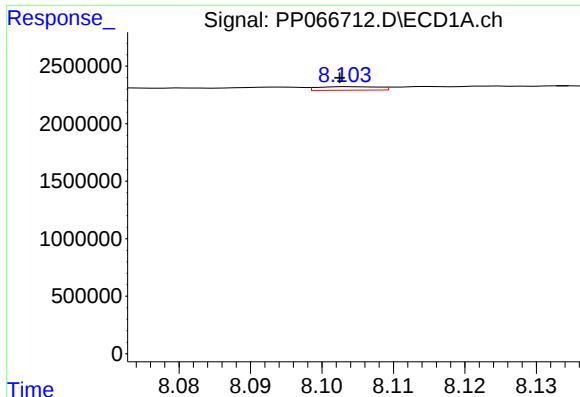

#33 AR-1260-3


R.T.: 8.104 min
Delta R.T.: 0.002 min
Response: 181662
Conc: 4.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

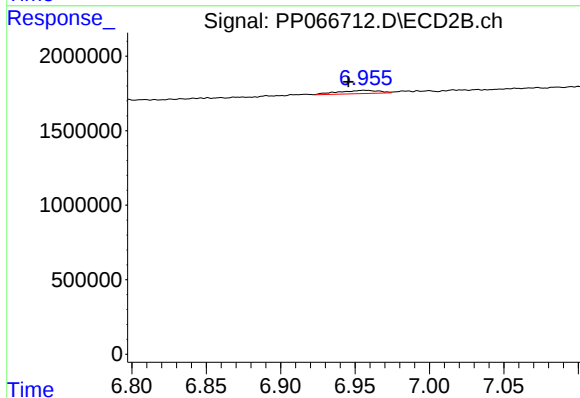


#33 AR-1260-3

R.T.: 6.957 min
Delta R.T.: 0.011 min
Response: 411260
Conc: 6.33 ng/ml

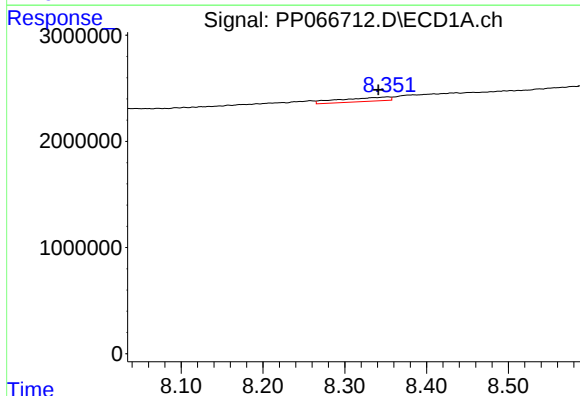


#34 AR-1260-4

R.T.: 8.352 min
Delta R.T.: 0.011 min
Response: 1636848
Conc: 31.01 ng/ml

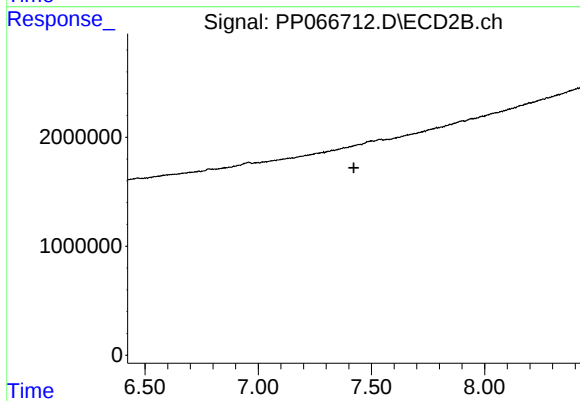

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.423 min
Response: 0
Conc: N.D.

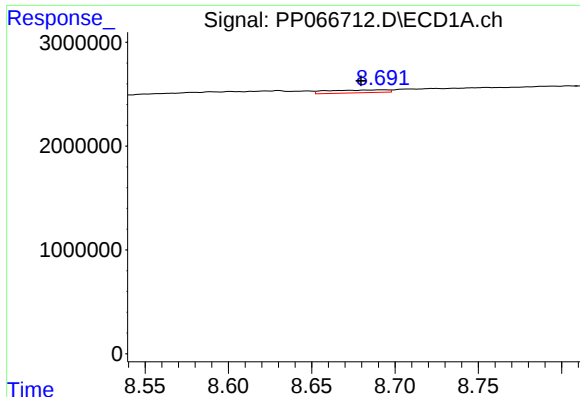

#35 AR-1260-5


R.T.: 8.693 min
Delta R.T.: 0.013 min
Response: 692844
Conc: 7.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

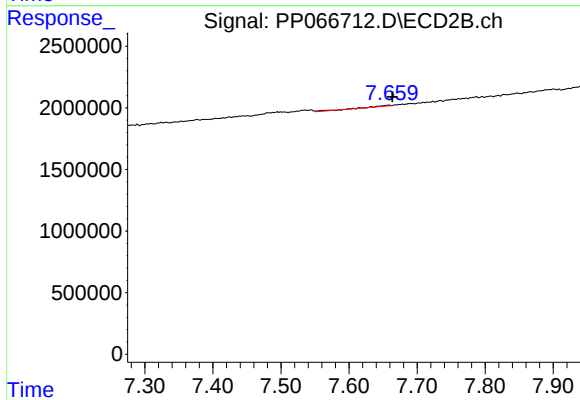


#35 AR-1260-5

R.T.: 7.659 min
Delta R.T.: -0.005 min
Response: 134332
Conc: 1.39 ng/ml

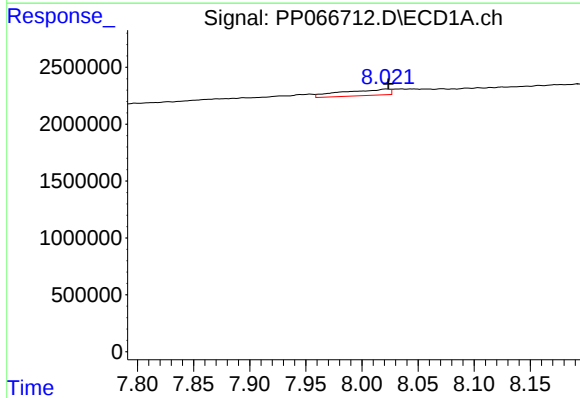


#36 AR-1262-1

R.T.: 8.021 min
Delta R.T.: -0.002 min
Response: 1598328
Conc: 35.40 ng/ml

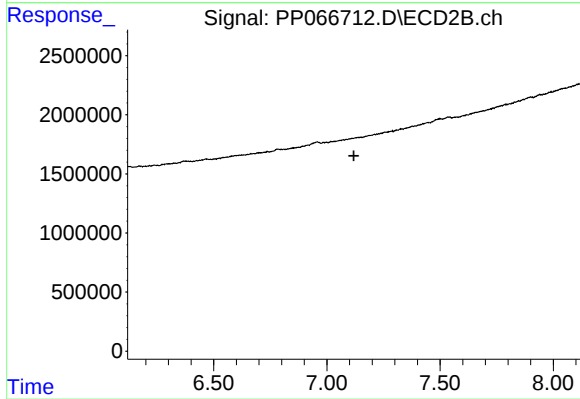

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.119 min
Response: 0
Conc: N.D.

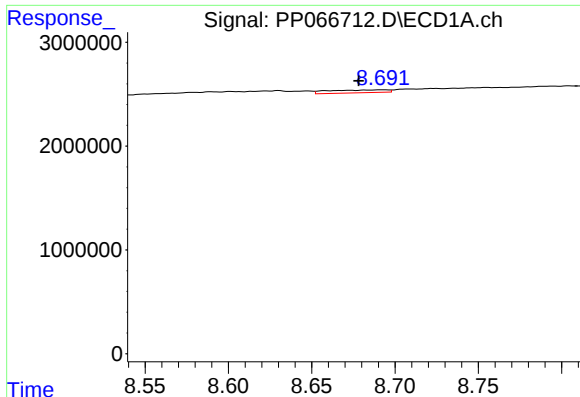

#37 AR-1262-2


R.T.: 8.693 min
Delta R.T.: 0.014 min
Response: 692844
Conc: 6.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

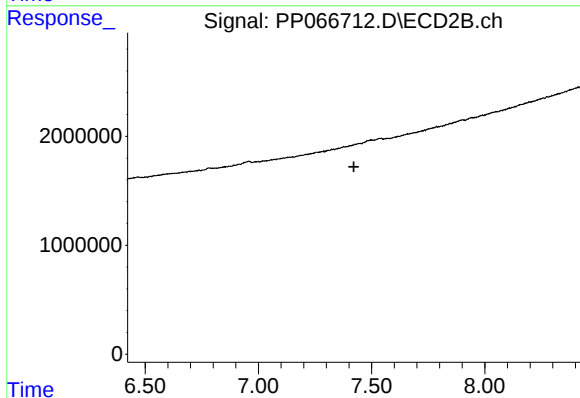


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.422 min
Response: 0
Conc: N.D.

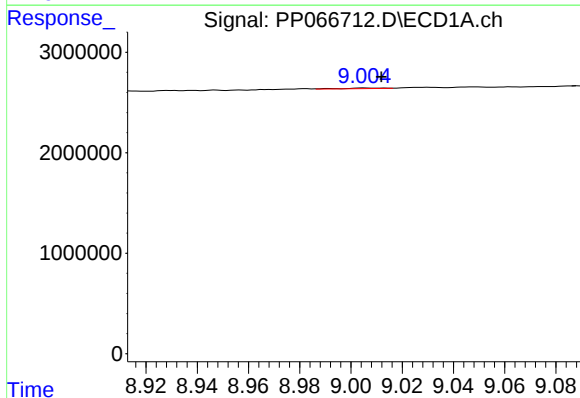


#38 AR-1262-3

R.T.: 9.005 min
Delta R.T.: -0.007 min
Response: 60853
Conc: 0.86 ng/ml

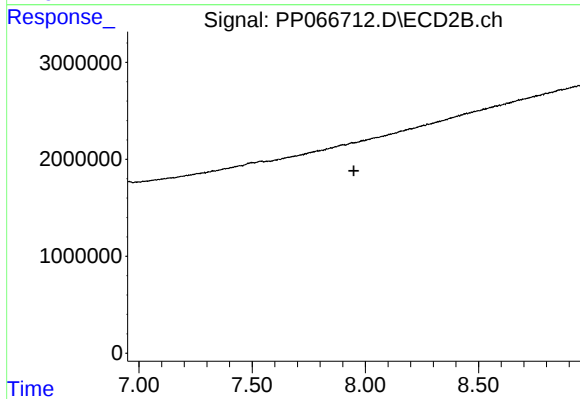

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 7.949 min
Response: 0
Conc: N.D.

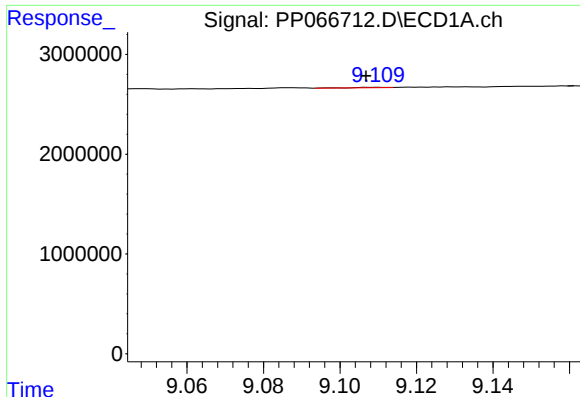

#39 AR-1262-4


R.T.: 9.110 min
Delta R.T.: 0.003 min
Response: 27604
Conc: 0.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

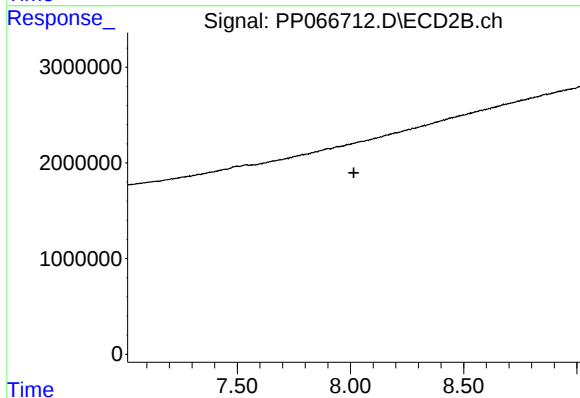


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.015 min
Response: 0
Conc: N.D.

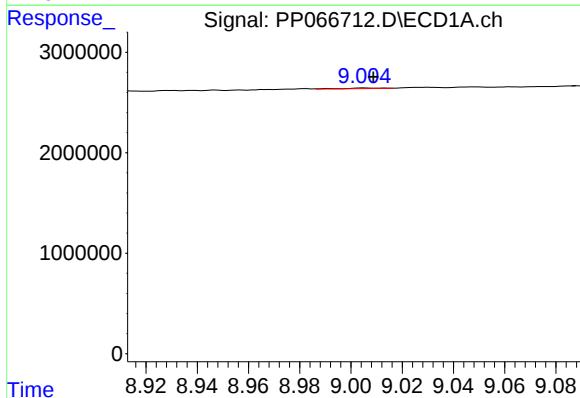


#41 AR-1268-1

R.T.: 9.005 min
Delta R.T.: -0.004 min
Response: 60853
Conc: 0.49 ng/ml

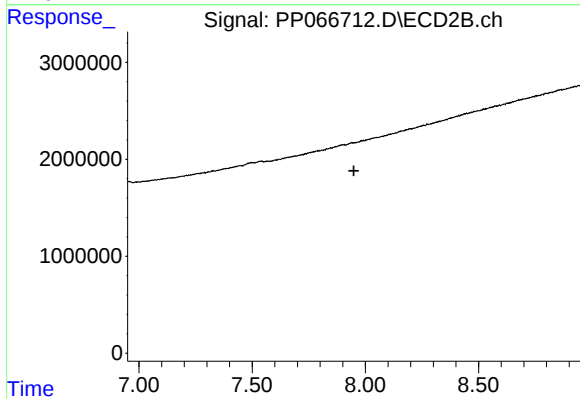

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 7.949 min
Response: 0
Conc: N.D.

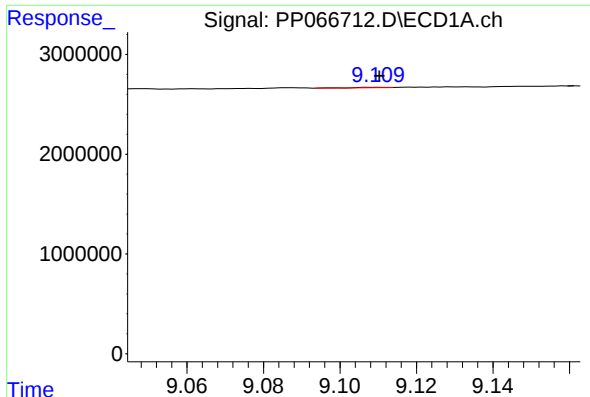

#42 AR-1268-2


R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 27604
Conc: 0.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

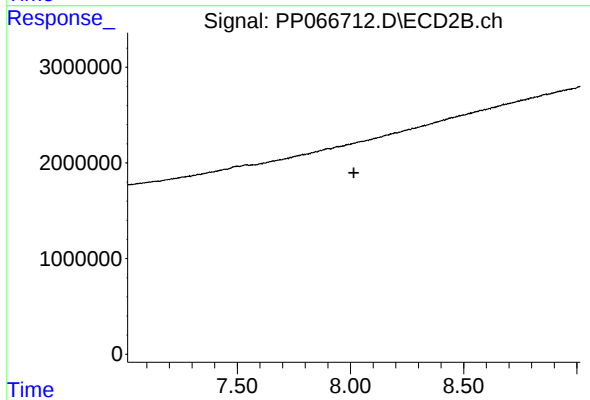


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.015 min
Response: 0
Conc: N.D.

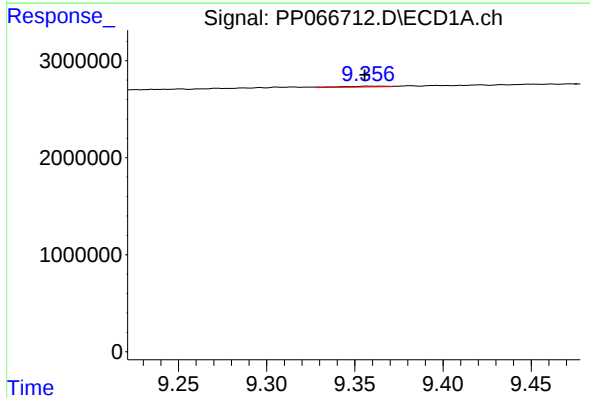


#43 AR-1268-3

R.T.: 9.357 min
Delta R.T.: 0.001 min
Response: 137203
Conc: 1.38 ng/ml

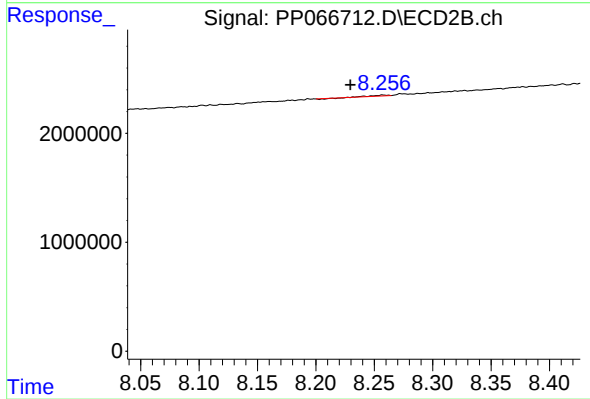

#43 AR-1268-3


R.T.: 8.257 min
Delta R.T.: 0.028 min
Response: 57395
Conc: 0.58 ng/ml

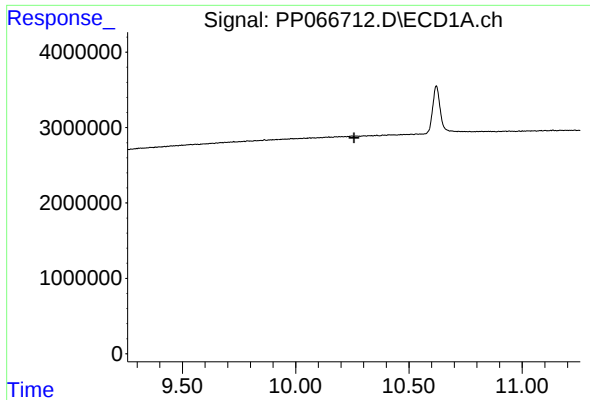

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

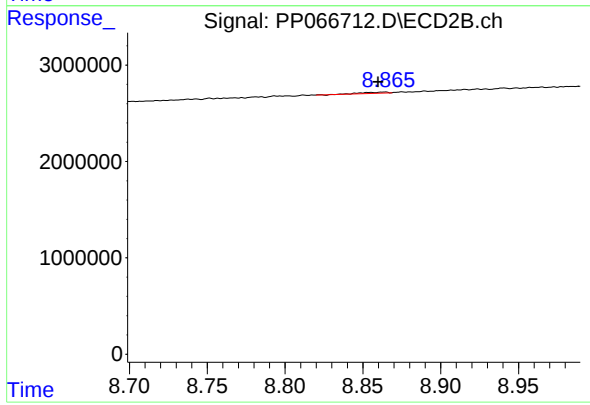

#45 AR-1268-5

R.T.: 8.864 min
Delta R.T.: 0.004 min
Response: 134468
Conc: 0.46 ng/ml