

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
 Data File : PP066713.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2024 01:41
 Operator : YP\AJ
 Sample : P3390-07
 Misc : AR1242 LOD 25 PPB
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 05:54:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 21 05:19:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.702	3.978	22790096	19217655	15.391	14.698
2)	SA Decachlor...	10.620	9.143	13337883	11724224	15.199	14.074
Target Compounds							
3)	L1 AR-1016-1	5.876	5.085	774231	645018	18.166	16.090
4)	L1 AR-1016-2	5.901	5.105	1032026	897020	15.427	15.053
5)	L1 AR-1016-3	5.963	5.287	826265	396496	19.521	13.264 #
6)	L1 AR-1016-4	6.061	5.325	556374	480838	17.052	18.348
7)	L1 AR-1016-5	6.356	5.546	609688	590901	19.224	18.197
9)	L2 AR-1221-2	5.010	4.286	381739	329314	30.785	28.058
10)	L2 AR-1221-3	5.074	4.361	463378	470449	12.211	12.909
11)	L3 AR-1232-1	5.074	4.361	463378	470449	14.570	15.352
12)	L3 AR-1232-2	5.607	5.105	620680	897020	35.834	33.245
13)	L3 AR-1232-3	5.901	5.287	1032026	396496	34.187	29.565
14)	L3 AR-1232-4	6.061	5.370	556374	515517	37.777	40.105
15)	L3 AR-1232-5	6.149	5.546	593494	590901	49.998	42.668
16)	L4 AR-1242-1	5.876	5.085	774231	645018	24.009	21.023
17)	L4 AR-1242-2	5.901	5.105	1032026	897020	20.392	19.797
18)	L4 AR-1242-3	5.963	5.287	826265	396496	26.149	16.974 #
19)	L4 AR-1242-4	6.061	5.370	556374	515517	22.452	20.487
20)	L4 AR-1242-5	6.799	5.903	612414	536574	24.372	18.969
21)	L5 AR-1248-1	5.876	5.085	774231	645018	30.293	26.641
22)	L5 AR-1248-2	6.149	5.325	593494	480838	14.771	13.313
23)	L5 AR-1248-3	6.356	5.370	609688	515517	13.983	13.808
24)	L5 AR-1248-4	6.762	5.546	462374	590901	10.467	13.392 #
25)	L5 AR-1248-5	6.799	5.947	612414	542772	13.359	14.369
26)	L6 AR-1254-1	6.735	5.903	505822	536574	10.246	8.957
27)	L6 AR-1254-2	6.960	6.054	888964	468196	12.184	8.761 #
28)	L6 AR-1254-3	7.326	6.467	249596	356820	3.572	4.513 #
29)	L6 AR-1254-4	7.608	6.697	222282	395091	4.993	9.773 #
30)	L6 AR-1254-5	8.029	7.145f	728753	647681	10.992	10.077
31)	L7 AR-1260-1	7.467f	0.000	21572	0	0.385	N.D. #
32)	L7 AR-1260-2	7.753	0.000	300409	0	4.719	N.D. #
33)	L7 AR-1260-3	8.101	6.963	489782	371439	11.013	5.717 #
35)	L7 AR-1260-5	8.687	0.000	760637	0	8.551	N.D. #
36)	L8 AR-1262-1	8.029	7.145f	728753	647681	16.140	20.263 #
37)	L8 AR-1262-2	8.687	0.000	760637	0	6.966	N.D. #
38)	L8 AR-1262-3	9.036f	0.000	74131	0	1.044	N.D. #
39)	L8 AR-1262-4	9.123f	0.000	116128	0	1.990	N.D. #
40)	L8 AR-1262-5	9.840f	0.000	19191	0	0.575	N.D. #
41)	L9 AR-1268-1	9.036f	0.000	74131	0	0.591	N.D. #
42)	L9 AR-1268-2	9.123	0.000	116128	0	1.053	N.D. #
43)	L9 AR-1268-3	9.347	0.000	9819	0	0.099	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
Data File : PP066713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2024 01:41
Operator : YP\AJ
Sample : P3390-07
Misc : AR1242 LOD 25 PPB
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 05:54:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 21 05:19:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	9.840f	0.000	19191	0	0.630	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
Data File : PP066713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2024 01:41
Operator : YP\AJ
Sample : P3390-07
Misc : AR1242 LOD 25 PPB
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 05:54:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 21 05:19:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

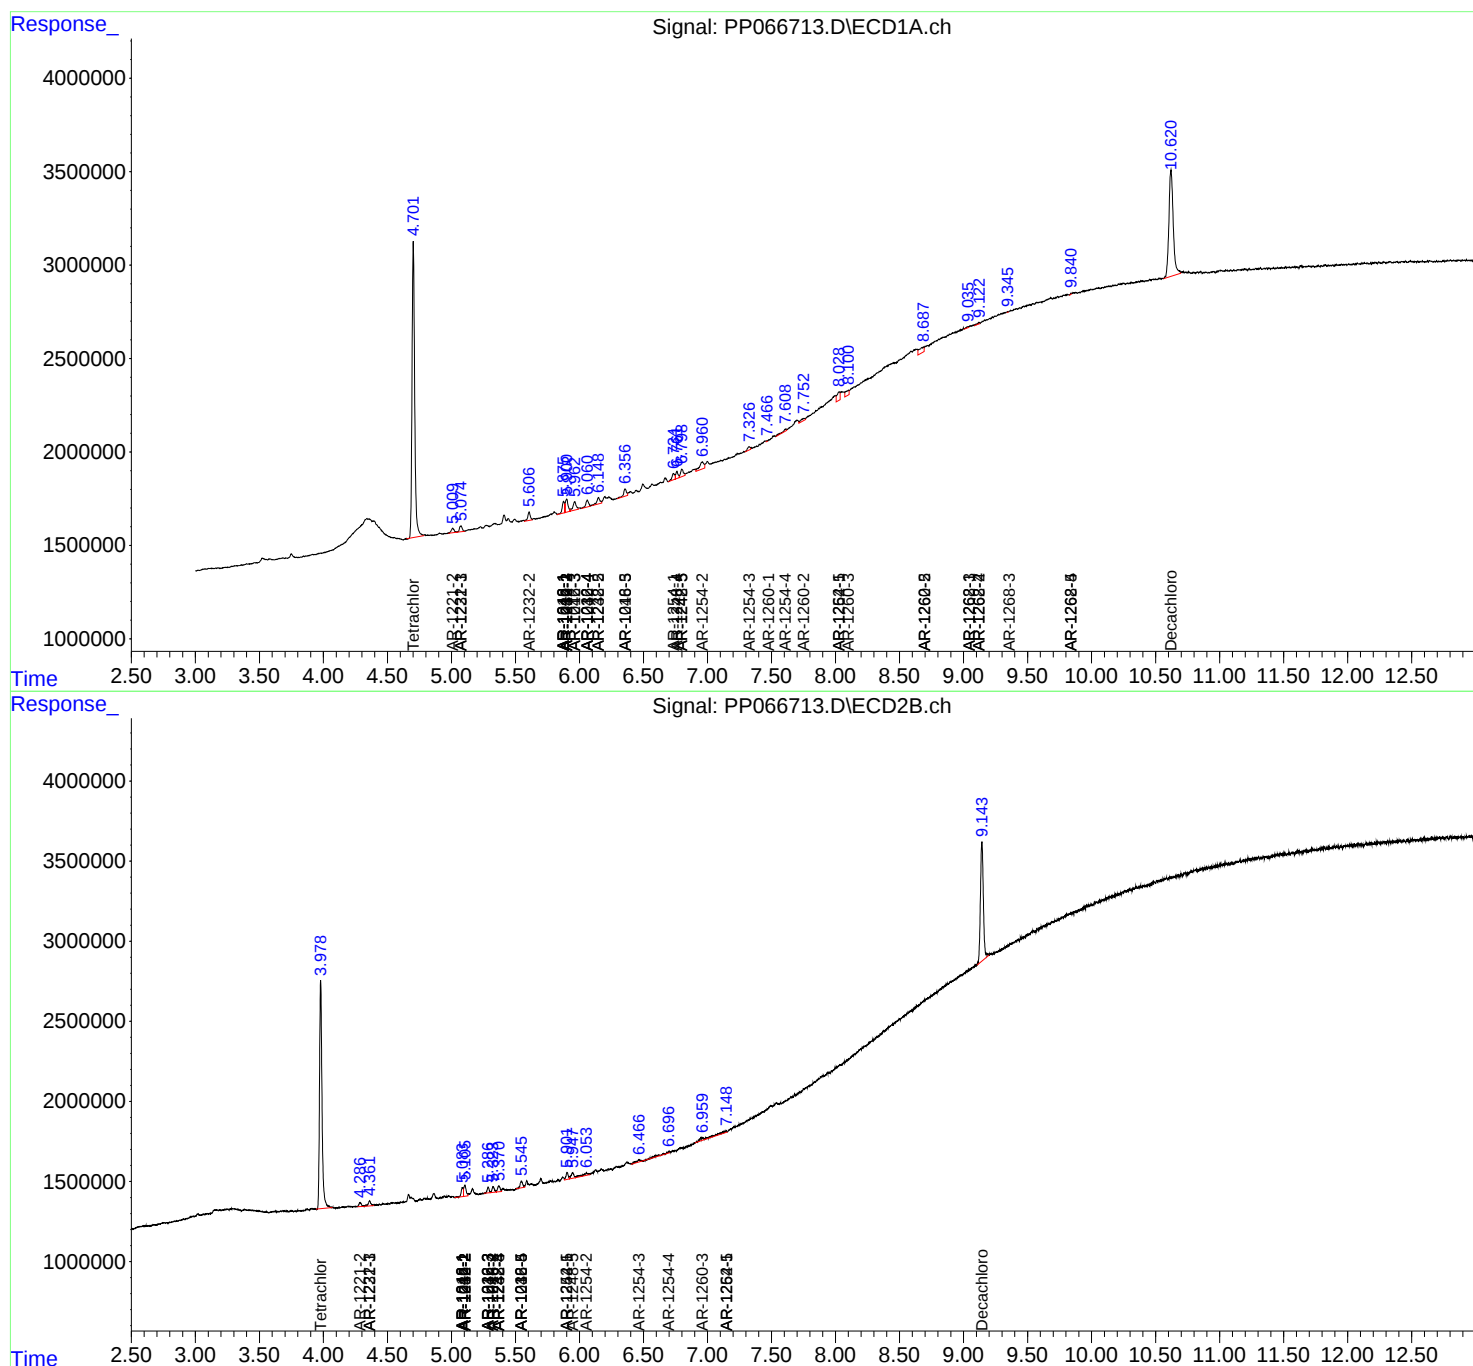


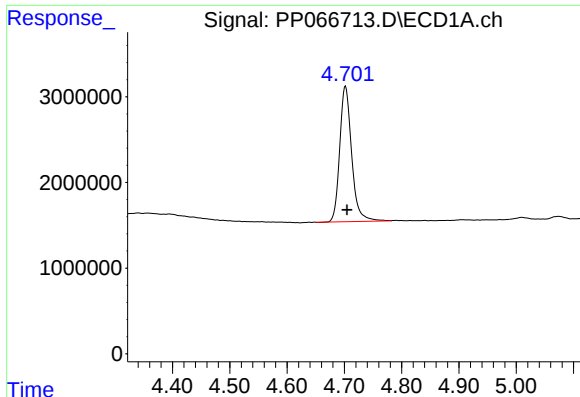

#1 Tetrachloro-m-xylene


R.T.: 4.702 min
Delta R.T.: -0.003 min
Response: 22790096
Conc: 15.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

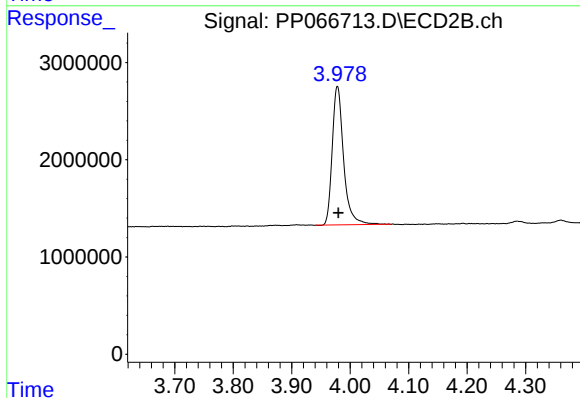


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.002 min
Response: 19217655
Conc: 14.70 ng/ml

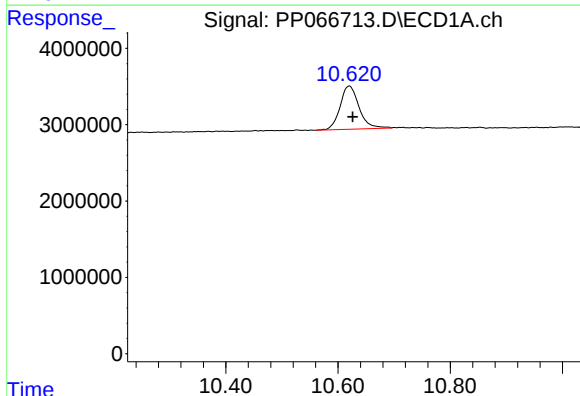


#2 Decachlorobiphenyl

R.T.: 10.620 min
Delta R.T.: -0.006 min
Response: 13337883
Conc: 15.20 ng/ml

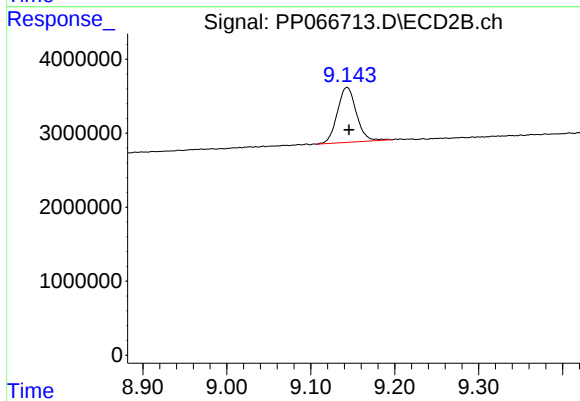

#2 Decachlorobiphenyl


R.T.: 9.143 min
Delta R.T.: -0.002 min
Response: 11724224
Conc: 14.07 ng/ml

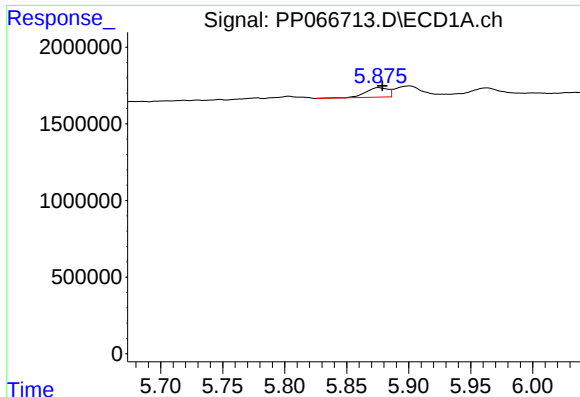

#3 AR-1016-1


R.T.: 5.876 min
Delta R.T.: -0.003 min
Response: 774231
Conc: 18.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

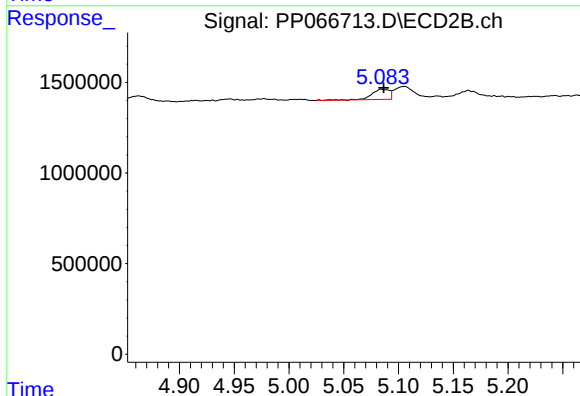


#3 AR-1016-1

R.T.: 5.085 min
Delta R.T.: -0.002 min
Response: 645018
Conc: 16.09 ng/ml

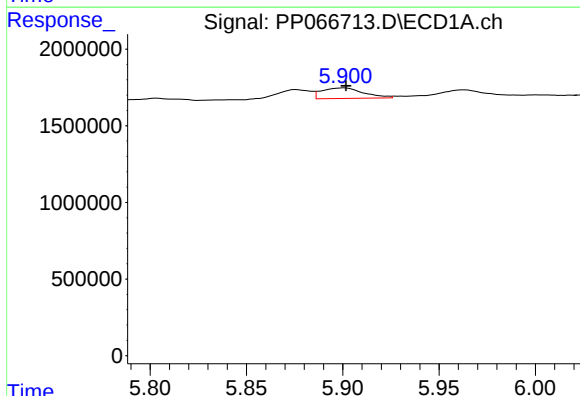


#4 AR-1016-2

R.T.: 5.901 min
Delta R.T.: 0.000 min
Response: 1032026
Conc: 15.43 ng/ml

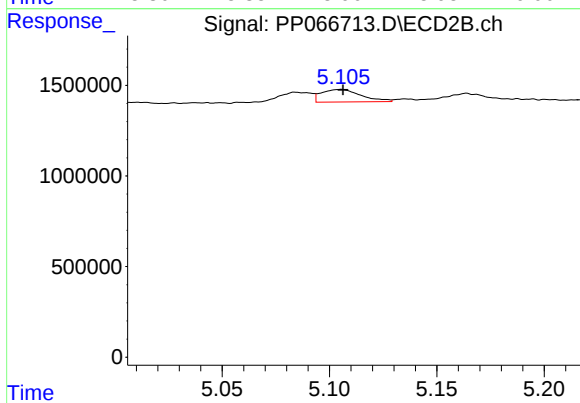

#4 AR-1016-2


R.T.: 5.105 min
Delta R.T.: -0.001 min
Response: 897020
Conc: 15.05 ng/ml

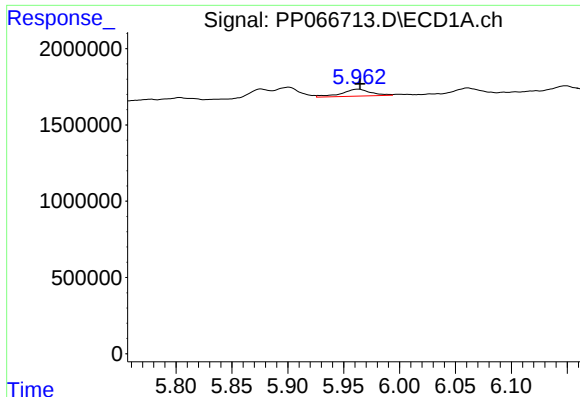

#5 AR-1016-3


R.T.: 5.963 min
Delta R.T.: -0.002 min
Response: 826265
Conc: 19.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

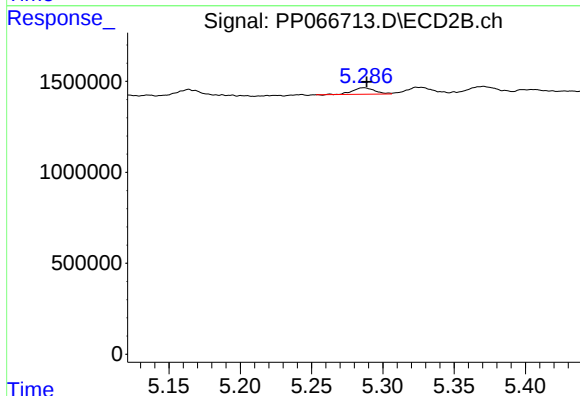


#5 AR-1016-3

R.T.: 5.287 min
Delta R.T.: -0.002 min
Response: 396496
Conc: 13.26 ng/ml

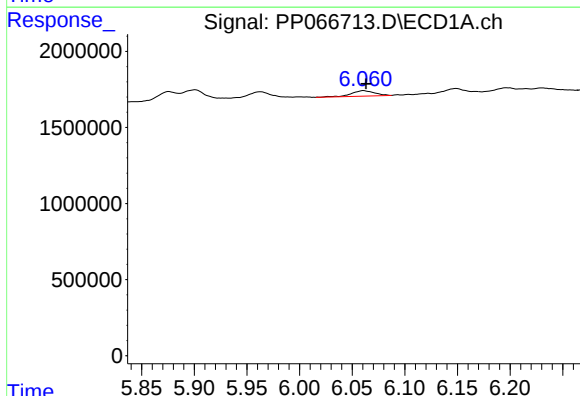


#6 AR-1016-4

R.T.: 6.061 min
Delta R.T.: -0.002 min
Response: 556374
Conc: 17.05 ng/ml

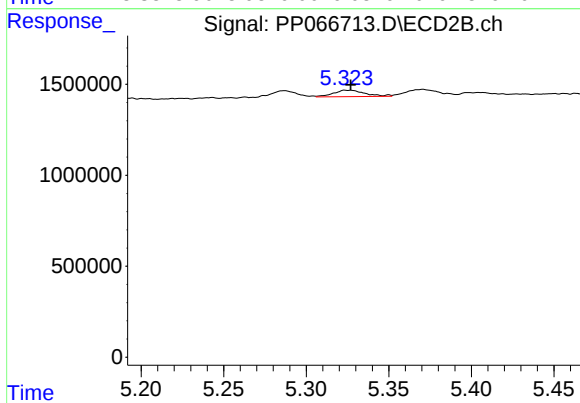

#6 AR-1016-4


R.T.: 5.325 min
Delta R.T.: -0.002 min
Response: 480838
Conc: 18.35 ng/ml

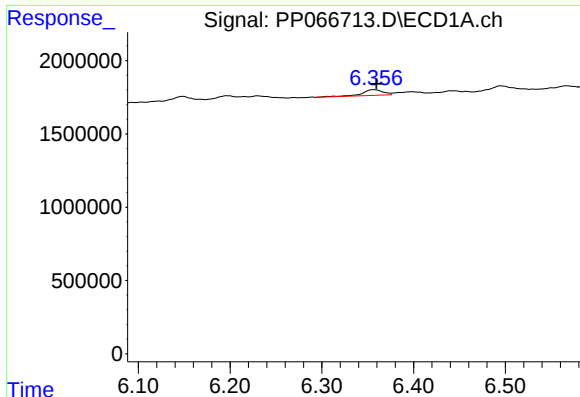

#7 AR-1016-5


R.T.: 6.356 min
Delta R.T.: -0.003 min
Response: 609688
Conc: 19.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

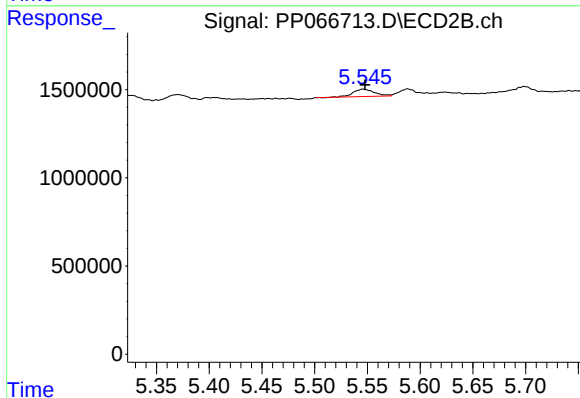


#7 AR-1016-5

R.T.: 5.546 min
Delta R.T.: -0.001 min
Response: 590901
Conc: 18.20 ng/ml

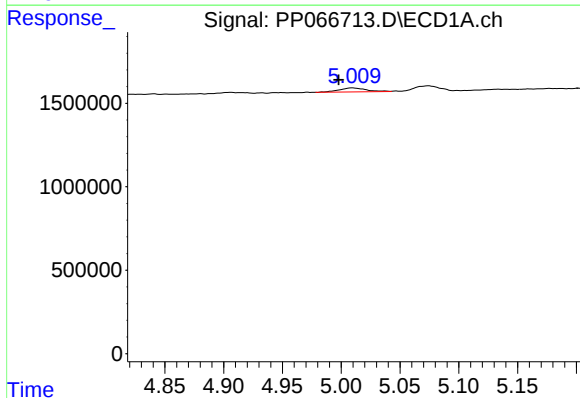


#9 AR-1221-2

R.T.: 5.010 min
Delta R.T.: 0.012 min
Response: 381739
Conc: 30.79 ng/ml

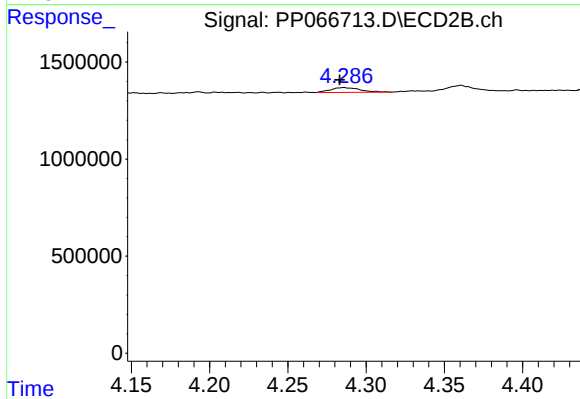

#9 AR-1221-2


R.T.: 4.286 min
Delta R.T.: 0.003 min
Response: 329314
Conc: 28.06 ng/ml

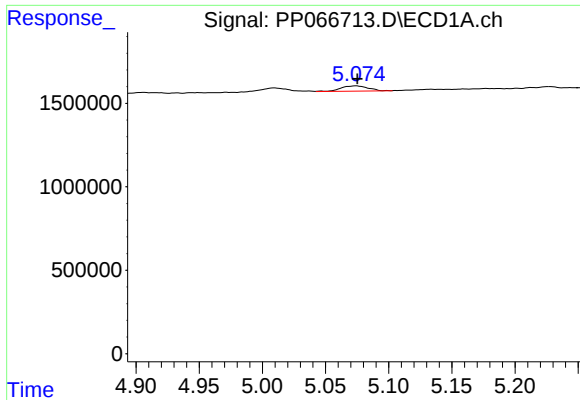

#10 AR-1221-3


R.T.: 5.074 min
Delta R.T.: 0.000 min
Response: 463378
Conc: 12.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

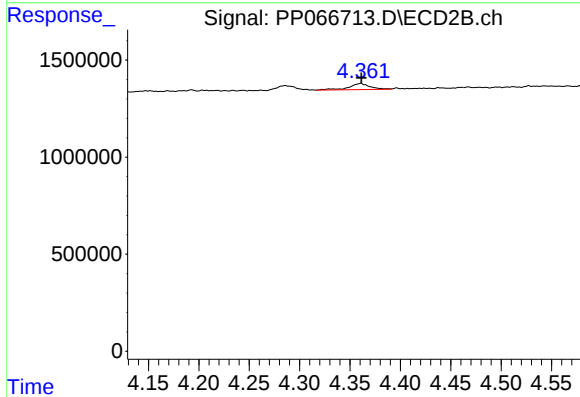


#10 AR-1221-3

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 470449
Conc: 12.91 ng/ml

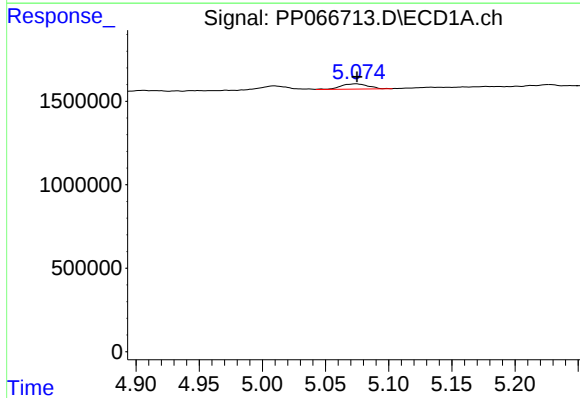


#11 AR-1232-1

R.T.: 5.074 min
Delta R.T.: 0.000 min
Response: 463378
Conc: 14.57 ng/ml

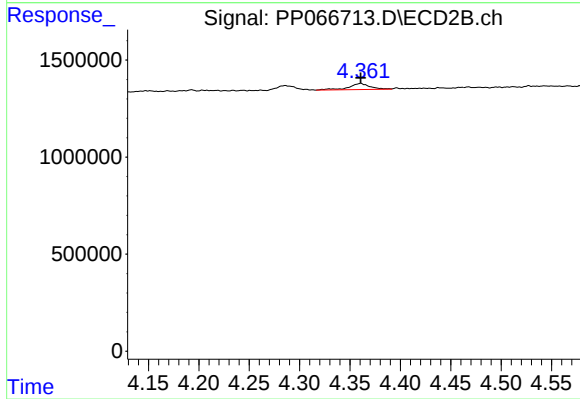

#11 AR-1232-1


R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 470449
Conc: 15.35 ng/ml

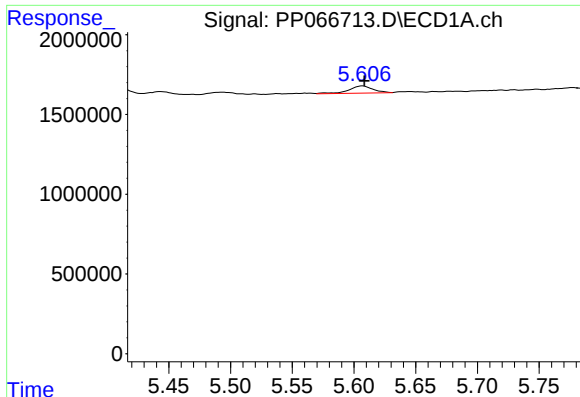

#12 AR-1232-2


R.T.: 5.607 min
Delta R.T.: -0.002 min
Response: 620680
Conc: 35.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

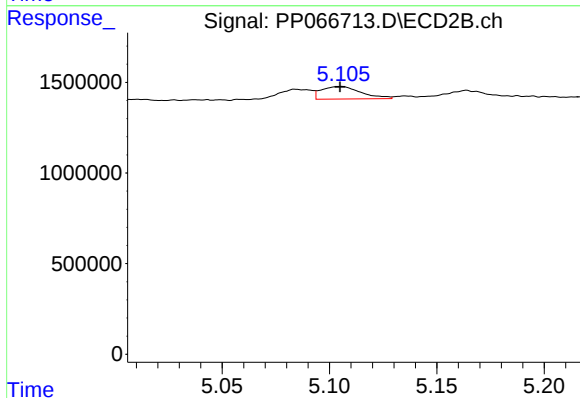


#12 AR-1232-2

R.T.: 5.105 min
Delta R.T.: 0.000 min
Response: 897020
Conc: 33.25 ng/ml

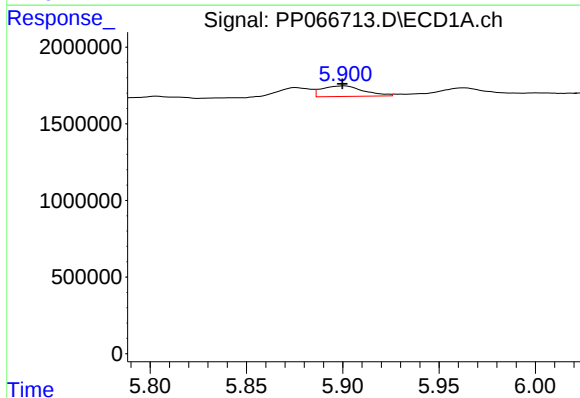


#13 AR-1232-3

R.T.: 5.901 min
Delta R.T.: 0.001 min
Response: 1032026
Conc: 34.19 ng/ml

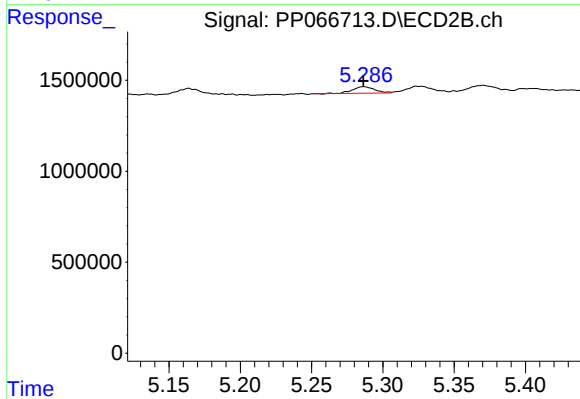

#13 AR-1232-3


R.T.: 5.287 min
Delta R.T.: 0.000 min
Response: 396496
Conc: 29.56 ng/ml

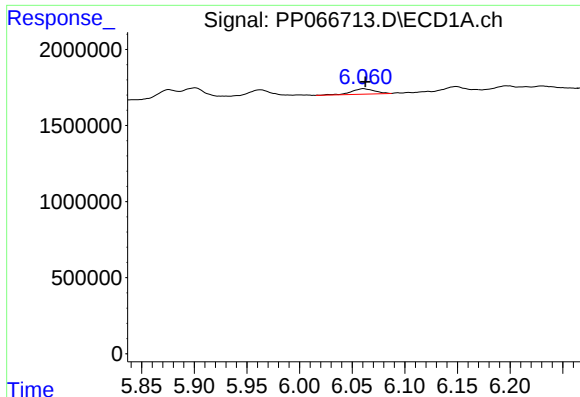

#14 AR-1232-4


R.T.: 6.061 min
Delta R.T.: -0.002 min
Response: 556374
Conc: 37.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

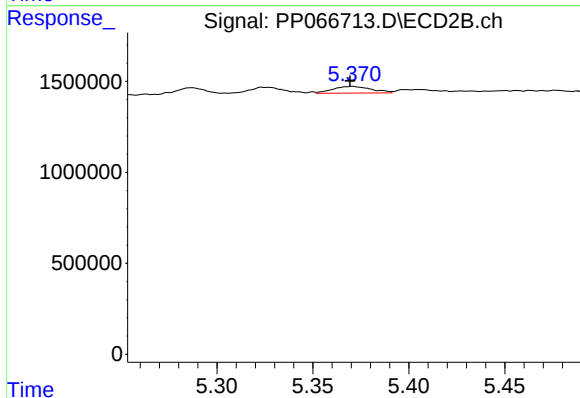


#14 AR-1232-4

R.T.: 5.370 min
Delta R.T.: 0.001 min
Response: 515517
Conc: 40.10 ng/ml

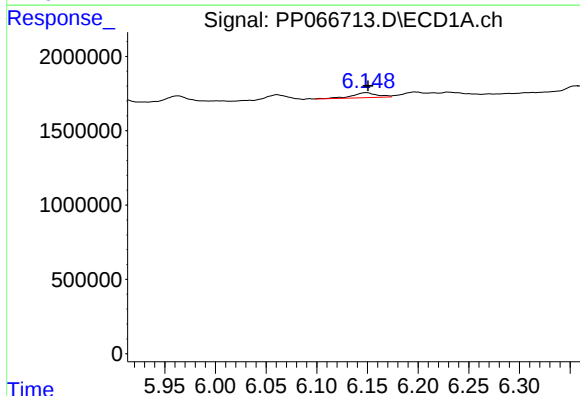


#15 AR-1232-5

R.T.: 6.149 min
Delta R.T.: -0.002 min
Response: 593494
Conc: 50.00 ng/ml

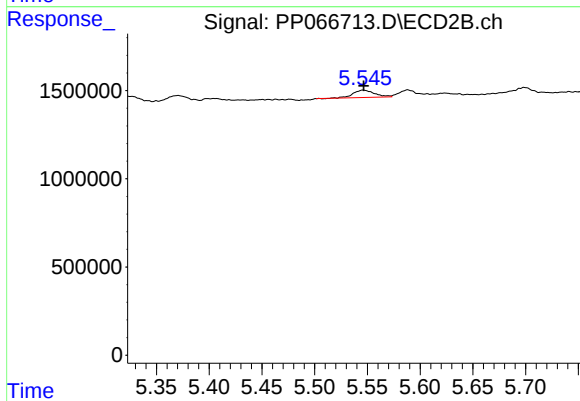

#15 AR-1232-5


R.T.: 5.546 min
Delta R.T.: 0.000 min
Response: 590901
Conc: 42.67 ng/ml

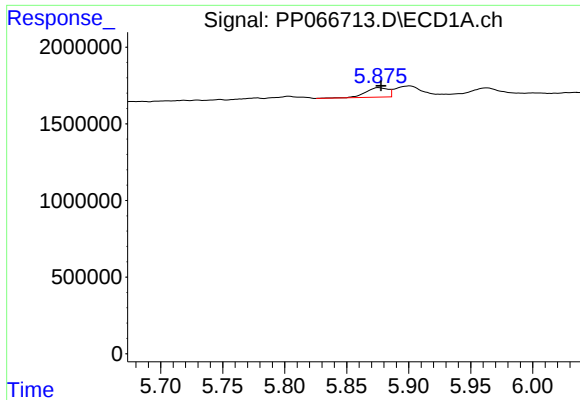

#16 AR-1242-1


R.T.: 5.876 min
Delta R.T.: -0.002 min
Response: 774231
Conc: 24.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

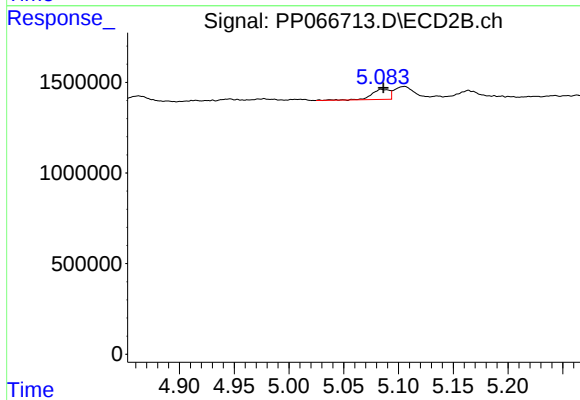


#16 AR-1242-1

R.T.: 5.085 min
Delta R.T.: -0.001 min
Response: 645018
Conc: 21.02 ng/ml

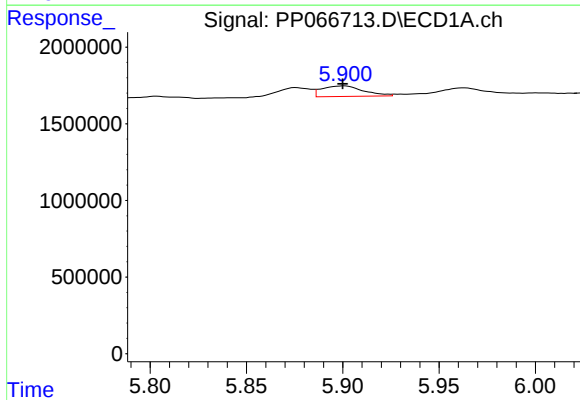


#17 AR-1242-2

R.T.: 5.901 min
Delta R.T.: 0.000 min
Response: 1032026
Conc: 20.39 ng/ml

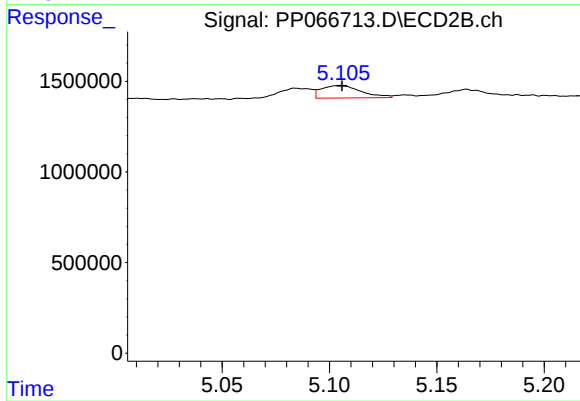

#17 AR-1242-2


R.T.: 5.105 min
Delta R.T.: 0.000 min
Response: 897020
Conc: 19.80 ng/ml

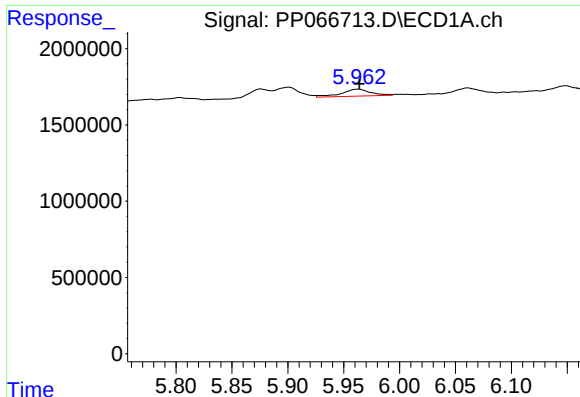

#18 AR-1242-3


R.T.: 5.963 min
Delta R.T.: -0.001 min
Response: 826265
Conc: 26.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

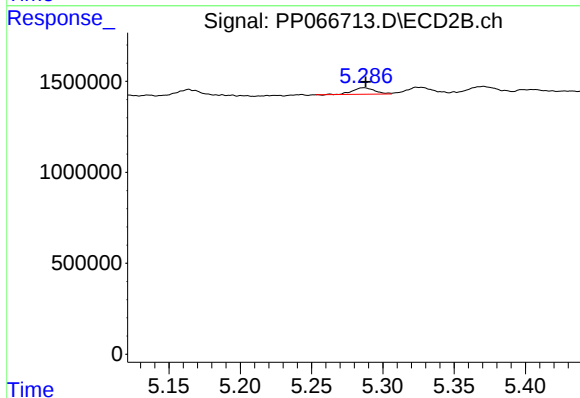


#18 AR-1242-3

R.T.: 5.287 min
Delta R.T.: -0.001 min
Response: 396496
Conc: 16.97 ng/ml

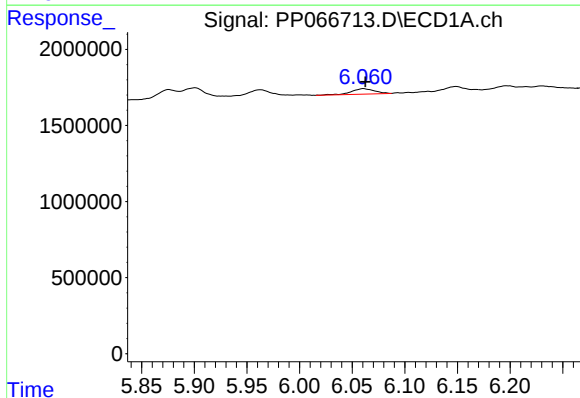


#19 AR-1242-4

R.T.: 6.061 min
Delta R.T.: -0.002 min
Response: 556374
Conc: 22.45 ng/ml

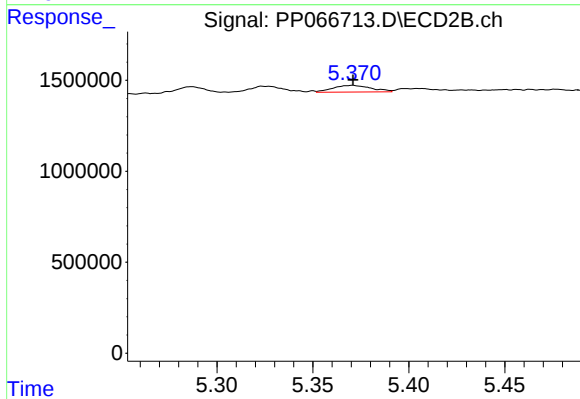

#19 AR-1242-4


R.T.: 5.370 min
Delta R.T.: 0.000 min
Response: 515517
Conc: 20.49 ng/ml

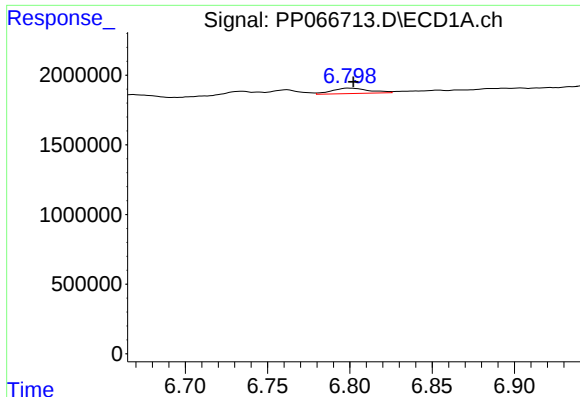

#20 AR-1242-5


R.T.: 6.799 min
Delta R.T.: -0.003 min
Response: 612414
Conc: 24.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

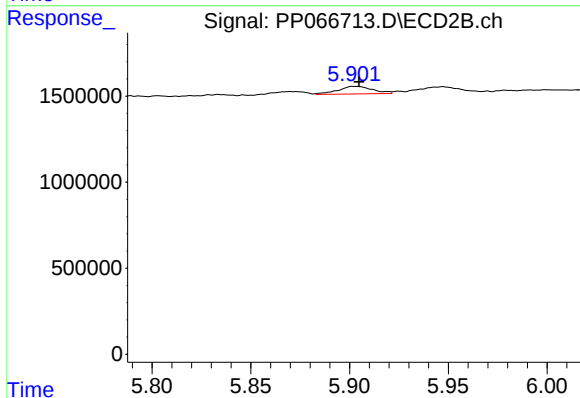


#20 AR-1242-5

R.T.: 5.903 min
Delta R.T.: -0.002 min
Response: 536574
Conc: 18.97 ng/ml

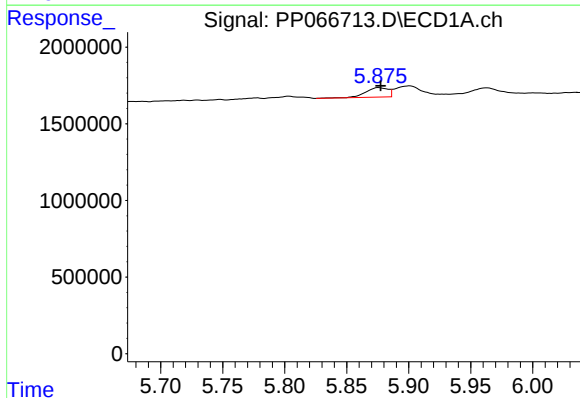


#21 AR-1248-1

R.T.: 5.876 min
Delta R.T.: -0.001 min
Response: 774231
Conc: 30.29 ng/ml

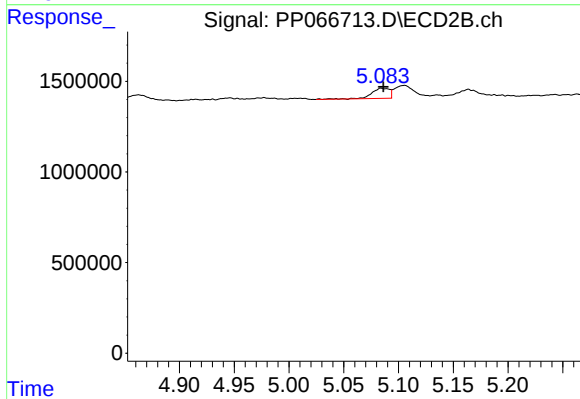

#21 AR-1248-1


R.T.: 5.085 min
Delta R.T.: -0.001 min
Response: 645018
Conc: 26.64 ng/ml

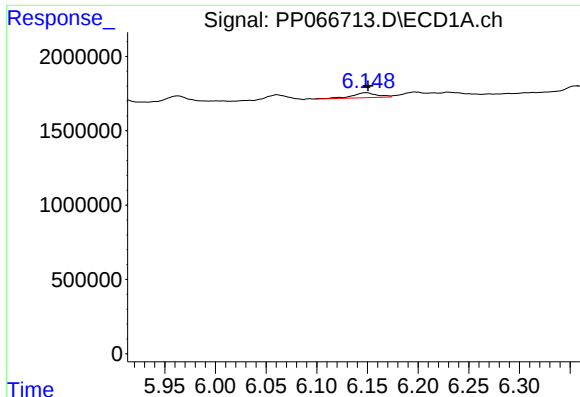

#22 AR-1248-2


R.T.: 6.149 min
Delta R.T.: -0.002 min
Response: 593494
Conc: 14.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

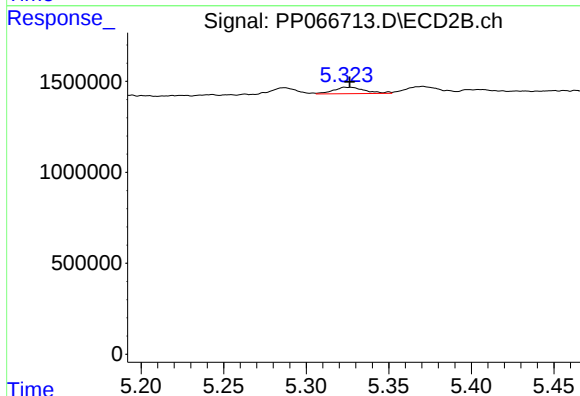


#22 AR-1248-2

R.T.: 5.325 min
Delta R.T.: -0.001 min
Response: 480838
Conc: 13.31 ng/ml

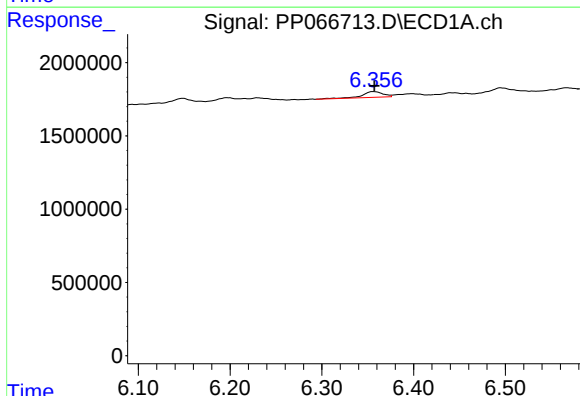


#23 AR-1248-3

R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 609688
Conc: 13.98 ng/ml

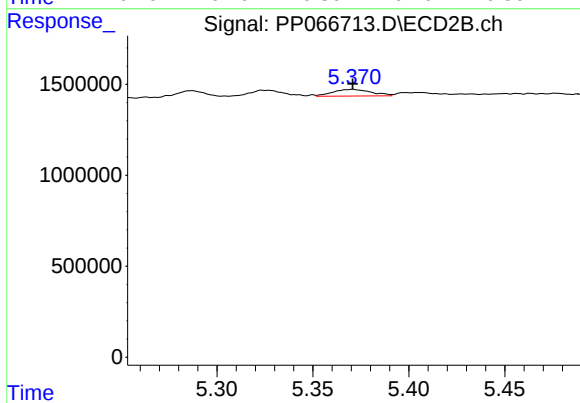

#23 AR-1248-3


R.T.: 5.370 min
Delta R.T.: 0.000 min
Response: 515517
Conc: 13.81 ng/ml

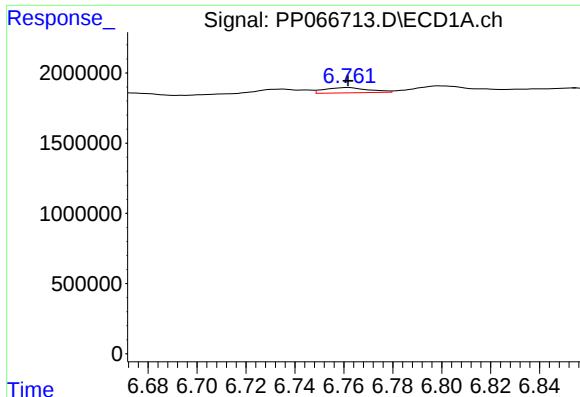

#24 AR-1248-4


R.T.: 6.762 min
Delta R.T.: 0.000 min
Response: 462374
Conc: 10.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

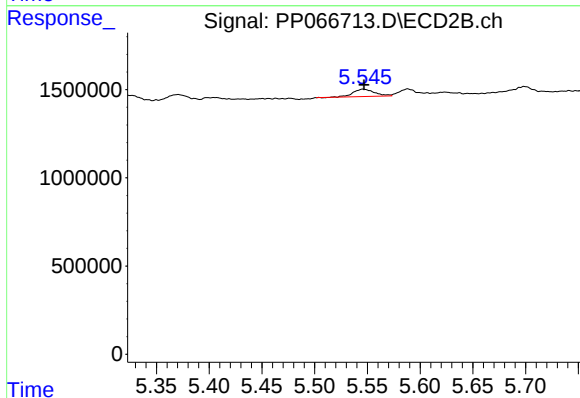


#24 AR-1248-4

R.T.: 5.546 min
Delta R.T.: 0.000 min
Response: 590901
Conc: 13.39 ng/ml

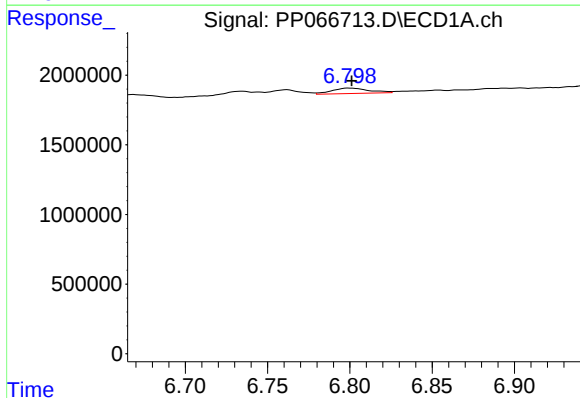


#25 AR-1248-5

R.T.: 6.799 min
Delta R.T.: -0.002 min
Response: 612414
Conc: 13.36 ng/ml

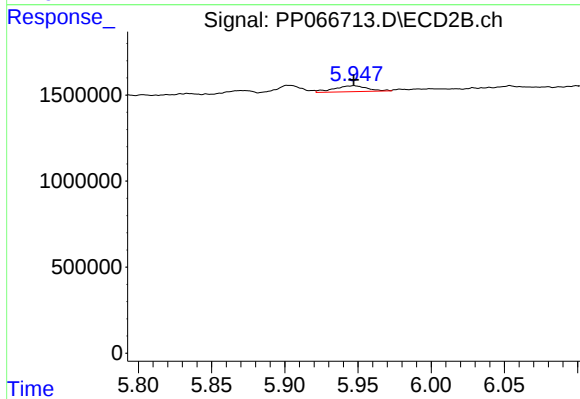

#25 AR-1248-5


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 542772
Conc: 14.37 ng/ml

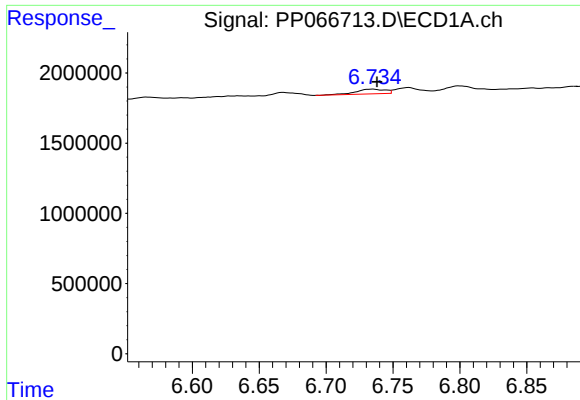

#26 AR-1254-1


R.T.: 6.735 min
Delta R.T.: -0.003 min
Response: 505822
Conc: 10.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

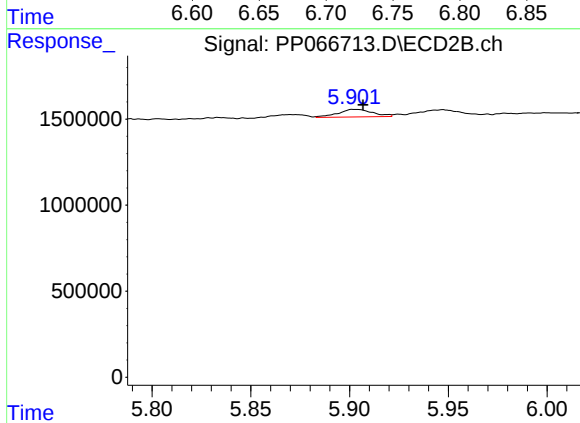


#26 AR-1254-1

R.T.: 5.903 min
Delta R.T.: -0.004 min
Response: 536574
Conc: 8.96 ng/ml

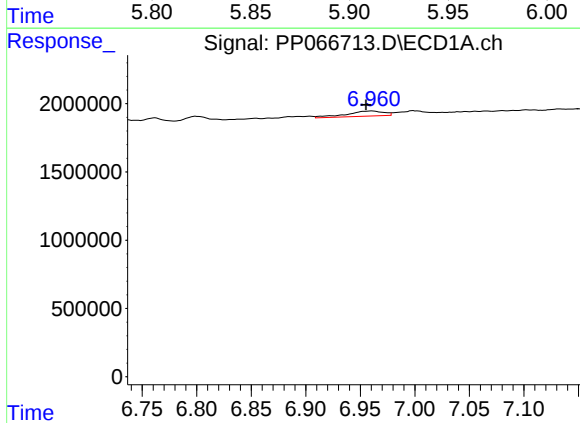


#27 AR-1254-2

R.T.: 6.960 min
Delta R.T.: 0.005 min
Response: 888964
Conc: 12.18 ng/ml

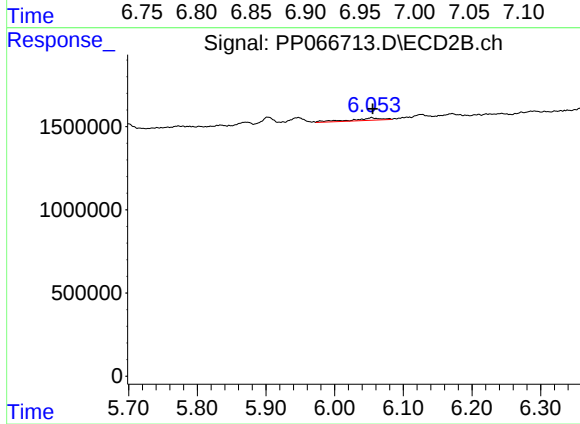

#27 AR-1254-2


R.T.: 6.054 min
Delta R.T.: -0.001 min
Response: 468196
Conc: 8.76 ng/ml

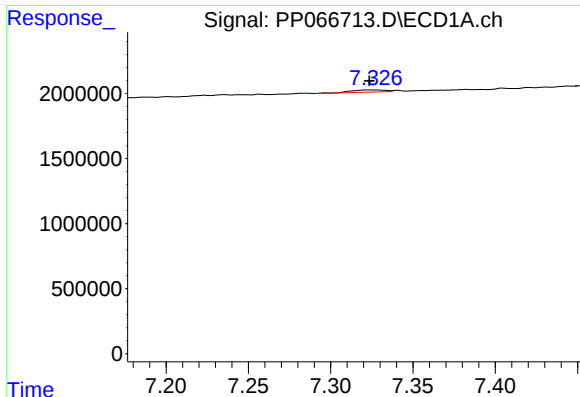

#28 AR-1254-3


R.T.: 7.326 min
Delta R.T.: 0.003 min
Response: 249596
Conc: 3.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

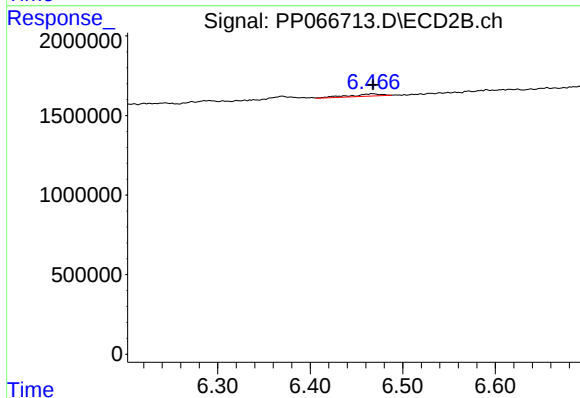


#28 AR-1254-3

R.T.: 6.467 min
Delta R.T.: 0.000 min
Response: 356820
Conc: 4.51 ng/ml

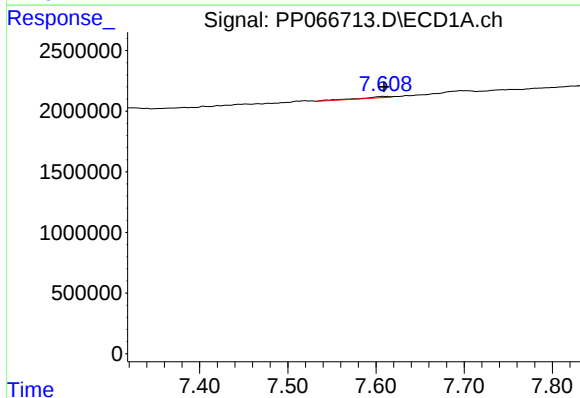


#29 AR-1254-4

R.T.: 7.608 min
Delta R.T.: 0.000 min
Response: 222282
Conc: 4.99 ng/ml

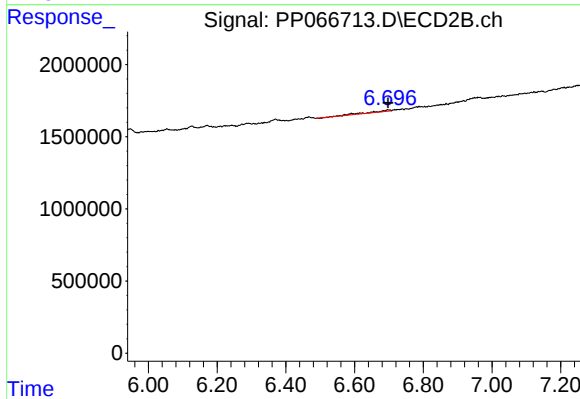

#29 AR-1254-4


R.T.: 6.697 min
Delta R.T.: 0.000 min
Response: 395091
Conc: 9.77 ng/ml

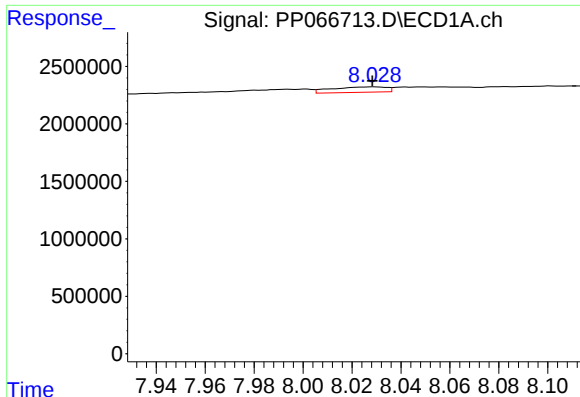

#30 AR-1254-5


R.T.: 8.029 min
Delta R.T.: 0.000 min
Response: 728753
Conc: 10.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

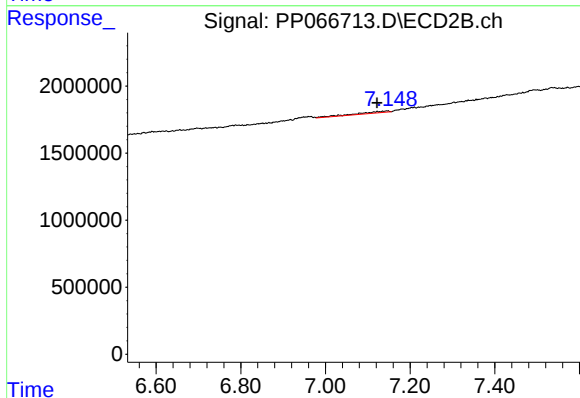


#30 AR-1254-5

R.T.: 7.145 min
Delta R.T.: 0.023 min
Response: 647681
Conc: 10.08 ng/ml

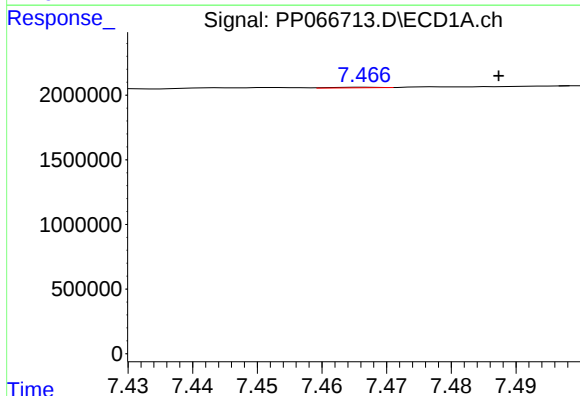


#31 AR-1260-1

R.T.: 7.467 min
Delta R.T.: -0.021 min
Response: 21572
Conc: 0.38 ng/ml

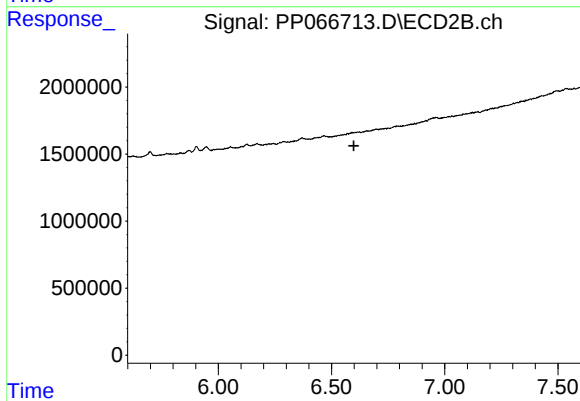

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.599 min
Response: 0
Conc: N.D.

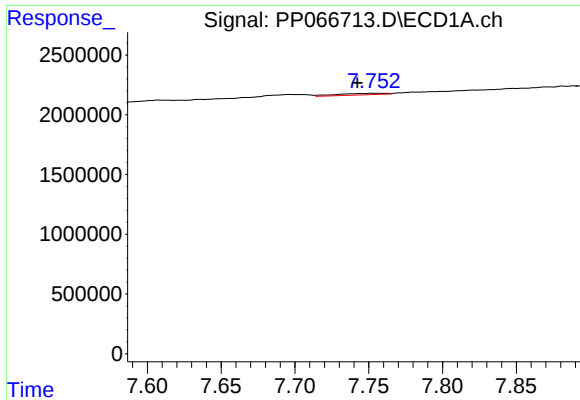

#32 AR-1260-2


R.T.: 7.753 min
Delta R.T.: 0.011 min
Response: 300409
Conc: 4.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

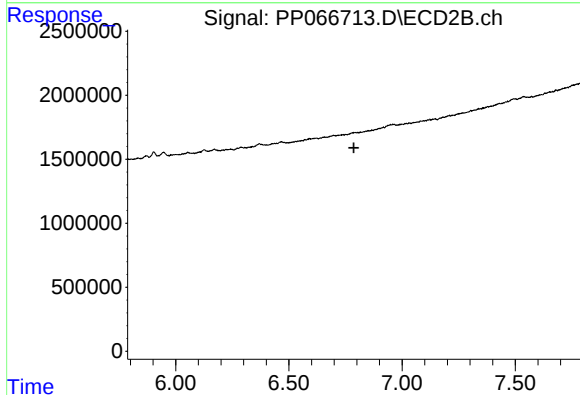


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.787 min
Response: 0
Conc: N.D.

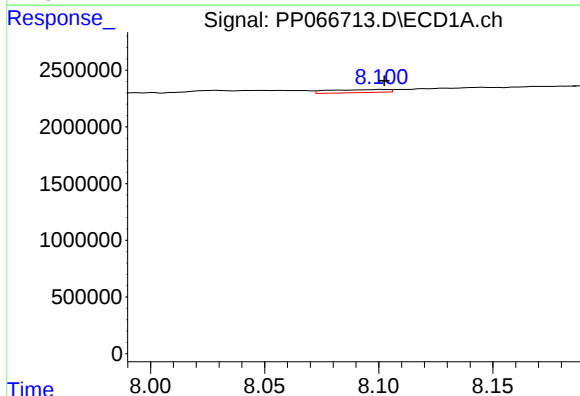


#33 AR-1260-3

R.T.: 8.101 min
Delta R.T.: -0.001 min
Response: 489782
Conc: 11.01 ng/ml

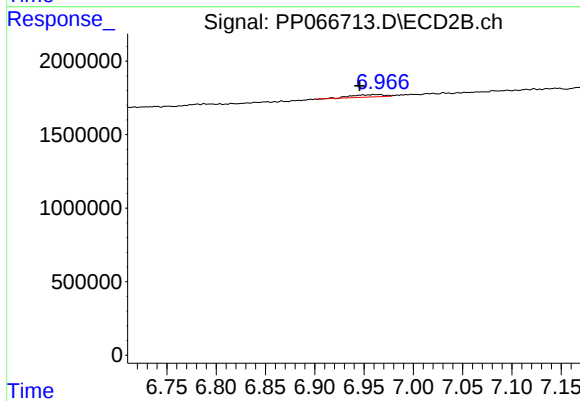

#33 AR-1260-3


R.T.: 6.963 min
Delta R.T.: 0.017 min
Response: 371439
Conc: 5.72 ng/ml

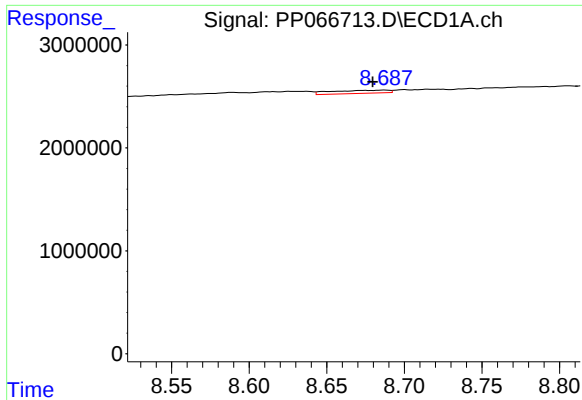

#35 AR-1260-5


R.T.: 8.687 min
Delta R.T.: 0.008 min
Response: 760637
Conc: 8.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

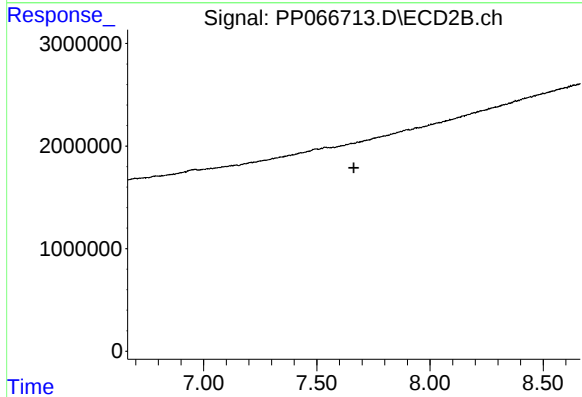


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.664 min
Response: 0
Conc: N.D.

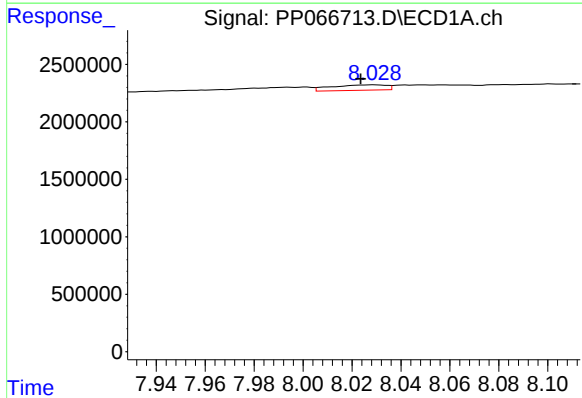


#36 AR-1262-1

R.T.: 8.029 min
Delta R.T.: 0.005 min
Response: 728753
Conc: 16.14 ng/ml

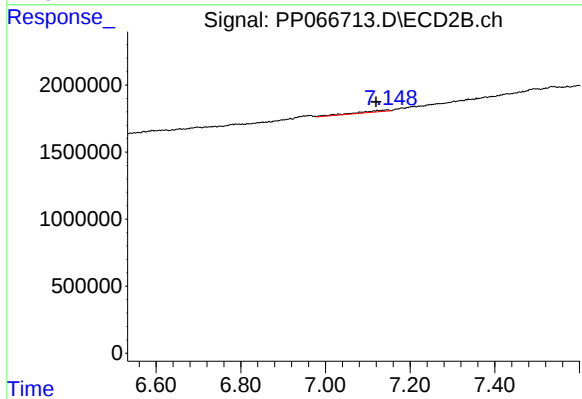

#36 AR-1262-1


R.T.: 7.145 min
Delta R.T.: 0.026 min
Response: 647681
Conc: 20.26 ng/ml

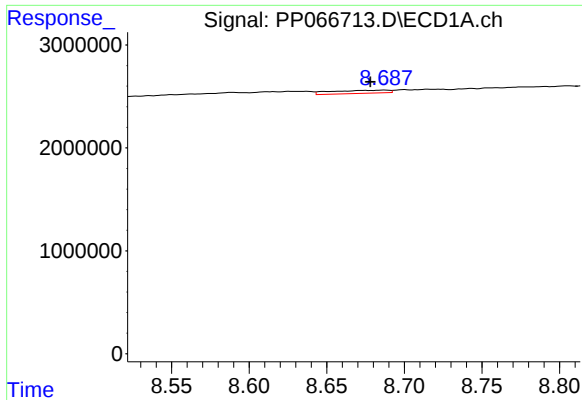

#37 AR-1262-2


R.T.: 8.687 min
Delta R.T.: 0.009 min
Response: 760637
Conc: 6.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

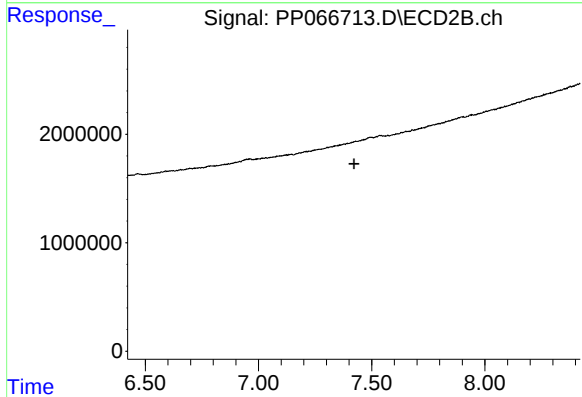


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.422 min
Response: 0
Conc: N.D.

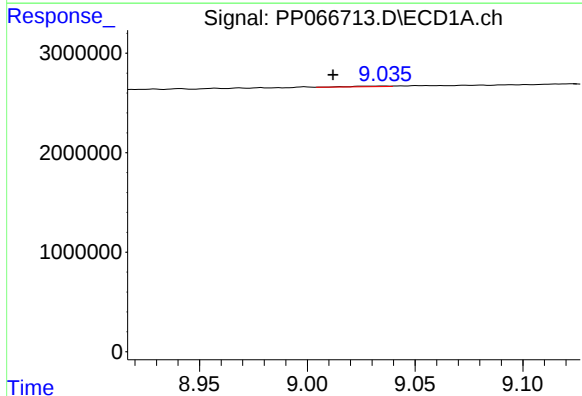


#38 AR-1262-3

R.T.: 9.036 min
Delta R.T.: 0.024 min
Response: 74131
Conc: 1.04 ng/ml

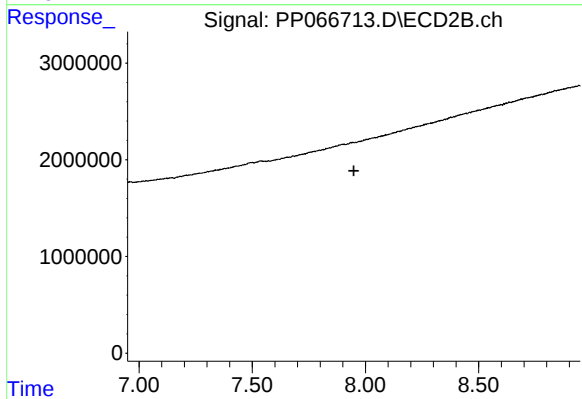

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 7.949 min
Response: 0
Conc: N.D.

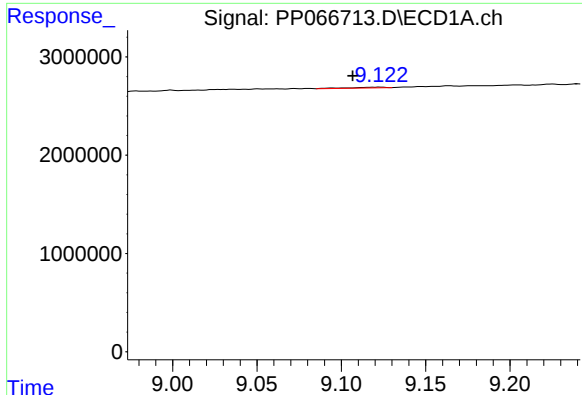

#39 AR-1262-4


R.T.: 9.123 min
Delta R.T.: 0.016 min
Response: 116128
Conc: 1.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

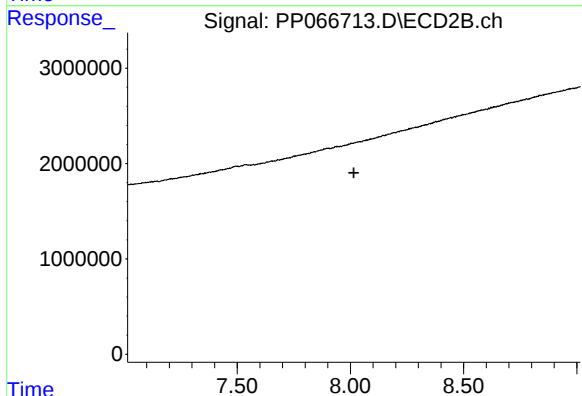


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.015 min
Response: 0
Conc: N.D.

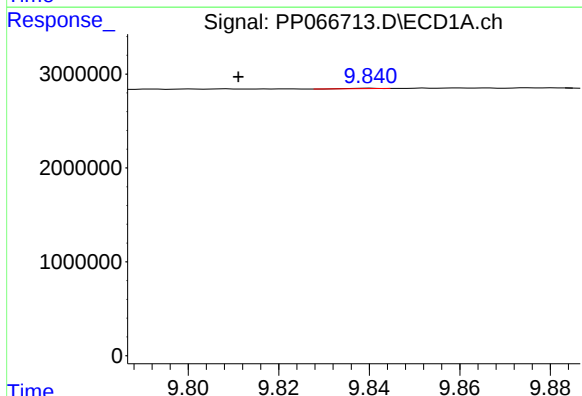


#40 AR-1262-5

R.T.: 9.840 min
Delta R.T.: 0.029 min
Response: 19191
Conc: 0.57 ng/ml

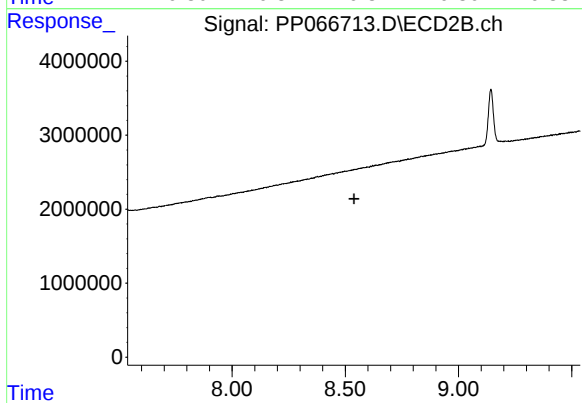

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.538 min
Response: 0
Conc: N.D.

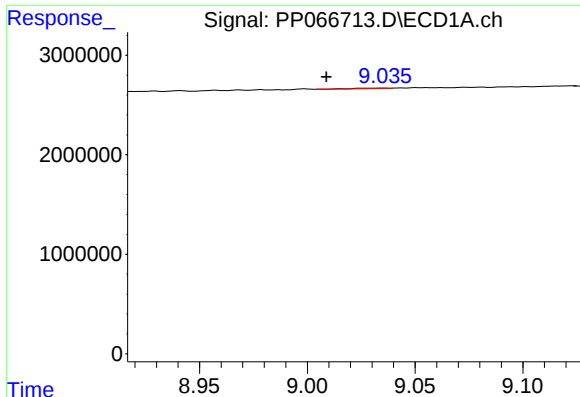

#41 AR-1268-1


R.T.: 9.036 min
Delta R.T.: 0.027 min
Response: 74131
Conc: 0.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

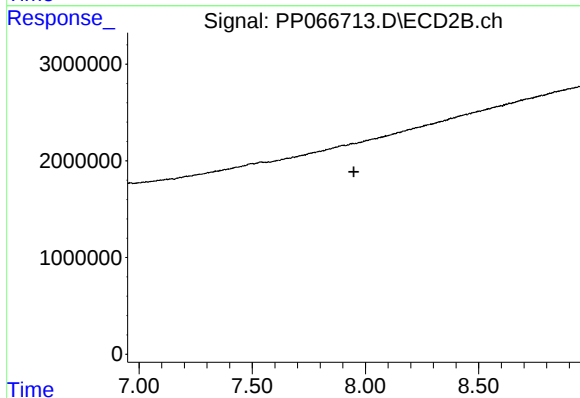


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.949 min
Response: 0
Conc: N.D.

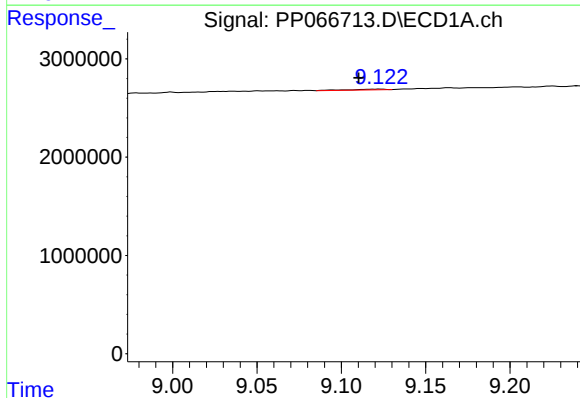


#42 AR-1268-2

R.T.: 9.123 min
Delta R.T.: 0.013 min
Response: 116128
Conc: 1.05 ng/ml

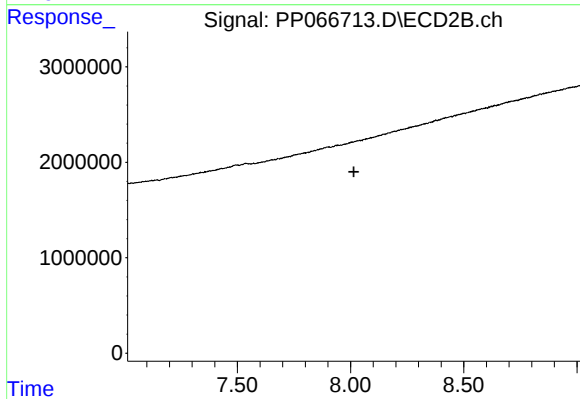

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.015 min
Response: 0
Conc: N.D.

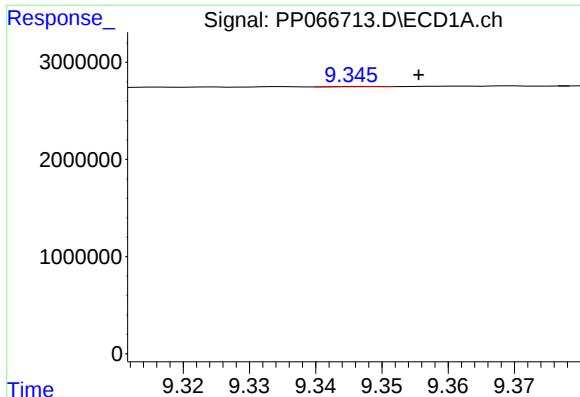

#43 AR-1268-3


R.T.: 9.347 min
Delta R.T.: -0.009 min
Response: 9819
Conc: 0.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

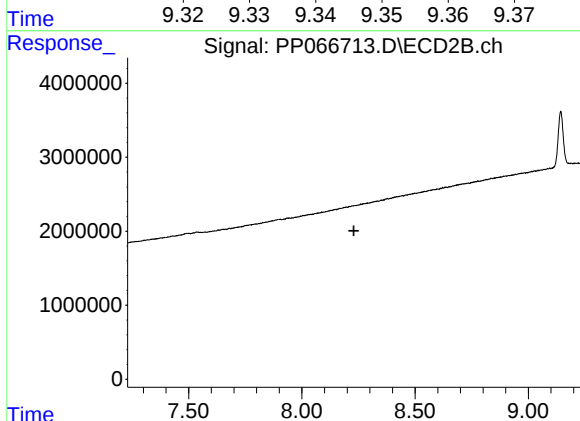


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.230 min
Response: 0
Conc: N.D.

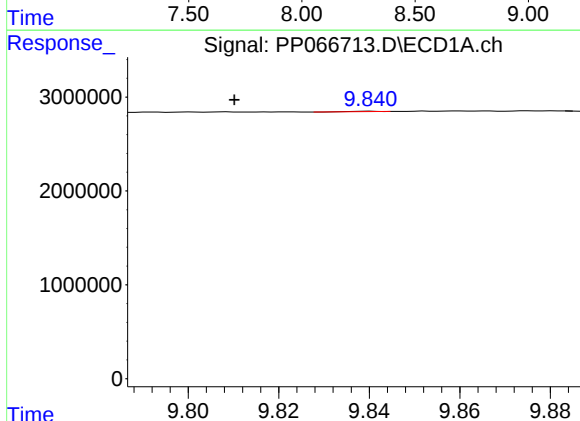

#44 AR-1268-4

R.T.: 9.840 min
Delta R.T.: 0.030 min
Response: 19191
Conc: 0.63 ng/ml

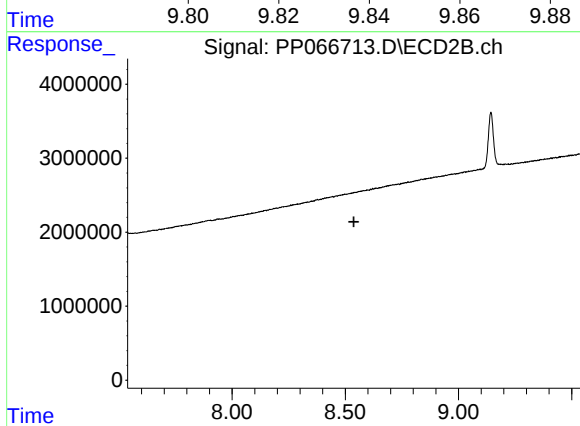

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.538 min
Response: 0
Conc: N.D.