

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
 Data File : PP066714.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2024 01:57
 Operator : YP\AJ
 Sample : P3390-07
 Misc : AR1248 LOD 25 PPB
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 05:55:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 21 05:19:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.702	3.979	24253424	20257177	16.379	15.493
2)	SA Decachlor...	10.621	9.143	14144894	12338848	16.119	14.812
Target Compounds							
3)	L1 AR-1016-1	5.876	5.086	569917	552986	13.372	13.794
4)	L1 AR-1016-2	5.899	5.104	800731	510780	11.969	8.571 #
5)	L1 AR-1016-3	5.963	5.287	492606	271686	11.638	9.089
6)	L1 AR-1016-4	6.059	5.327	456840	843751	14.002	32.197 #
7)	L1 AR-1016-5	6.357	5.548	1169075	932924	36.862	28.730
9)	L2 AR-1221-2	5.012	4.289	343110	371601	27.670	31.661
12)	L3 AR-1232-2	5.608	5.104	328859	510780	18.986	18.930
13)	L3 AR-1232-3	5.899	5.287	800731	271686	26.525	20.258
14)	L3 AR-1232-4	6.059	5.371	456840	857926	31.018	66.742 #
15)	L3 AR-1232-5	6.150	5.548	1054718	932924	88.853	67.364
16)	L4 AR-1242-1	5.876	5.086	569917	552986	17.673	18.024
17)	L4 AR-1242-2	5.899	5.104	800731	510780	15.822	11.273 #
18)	L4 AR-1242-3	5.963	5.287	492606	271686	15.589	11.631 #
19)	L4 AR-1242-4	6.059	5.371	456840	857926	18.436	34.094 #
20)	L4 AR-1242-5	6.800	5.904	1091862	1211680	43.452	42.836
21)	L5 AR-1248-1	5.876	5.086	569917	552986	22.299	22.840
22)	L5 AR-1248-2	6.150	5.327	1054718	843751	26.249	23.362
23)	L5 AR-1248-3	6.357	5.371	1169075	857926	26.812	22.979
24)	L5 AR-1248-4	6.760	5.548	967016	932924	21.890	21.144
25)	L5 AR-1248-5	6.800	5.947	1091862	855838	23.817	22.656
26)	L6 AR-1254-1	6.734	5.904	874349	1211680	17.711	20.226
27)	L6 AR-1254-2	6.956	6.056	1239256	472864	16.986	8.848 #
28)	L6 AR-1254-3	7.320	6.468	501014	585599	7.171	7.406
29)	L6 AR-1254-4	7.608	6.699	255287	332209	5.734	8.217 #
30)	L6 AR-1254-5	8.029	7.133	962716	376071	14.521	5.851 #
31)	L7 AR-1260-1	7.488	6.614	45860	570708	0.818	9.656 #
32)	L7 AR-1260-2	7.748	6.806f	312102	335883	4.902	4.929
33)	L7 AR-1260-3	8.101	6.958	148369	500393	3.336	7.701 #
34)	L7 AR-1260-4	0.000	7.444f	0	1132667	N.D.	25.150 #
35)	L7 AR-1260-5	8.670	7.629f	506347	109559	5.692	1.135 #
36)	L8 AR-1262-1	8.029	7.133	962716	376071	21.322	11.765 #
37)	L8 AR-1262-2	8.670	7.444f	506347	1132667	4.637	18.165 #
38)	L8 AR-1262-3	9.009	7.949	19950	34200	0.281	0.764 #
39)	L8 AR-1262-4	9.114	0.000	92683	0	1.588	N.D. #
40)	L8 AR-1262-5	9.838f	8.549	25106	98306	0.752	3.104 #
41)	L9 AR-1268-1	9.009	7.949	19950	34200	0.159	0.273 #
42)	L9 AR-1268-2	9.114	0.000	92683	0	0.840	N.D. #
43)	L9 AR-1268-3	9.357	0.000	114636	0	1.155	N.D. #
44)	L9 AR-1268-4	9.838f	8.549	25106	98306	0.824	2.905 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
Data File : PP066714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2024 01:57
Operator : YP\AJ
Sample : P3390-07
Misc : AR1248 LOD 25 PPB
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 05:55:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 21 05:19:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
45) L9	AR-1268-5	10.273f	8.854	94231	87222	0.330	0.300



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
Data File : PP066714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2024 01:57
Operator : YP\AJ
Sample : P3390-07
Misc : AR1248 LOD 25 PPB
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 05:55:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 21 05:19:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

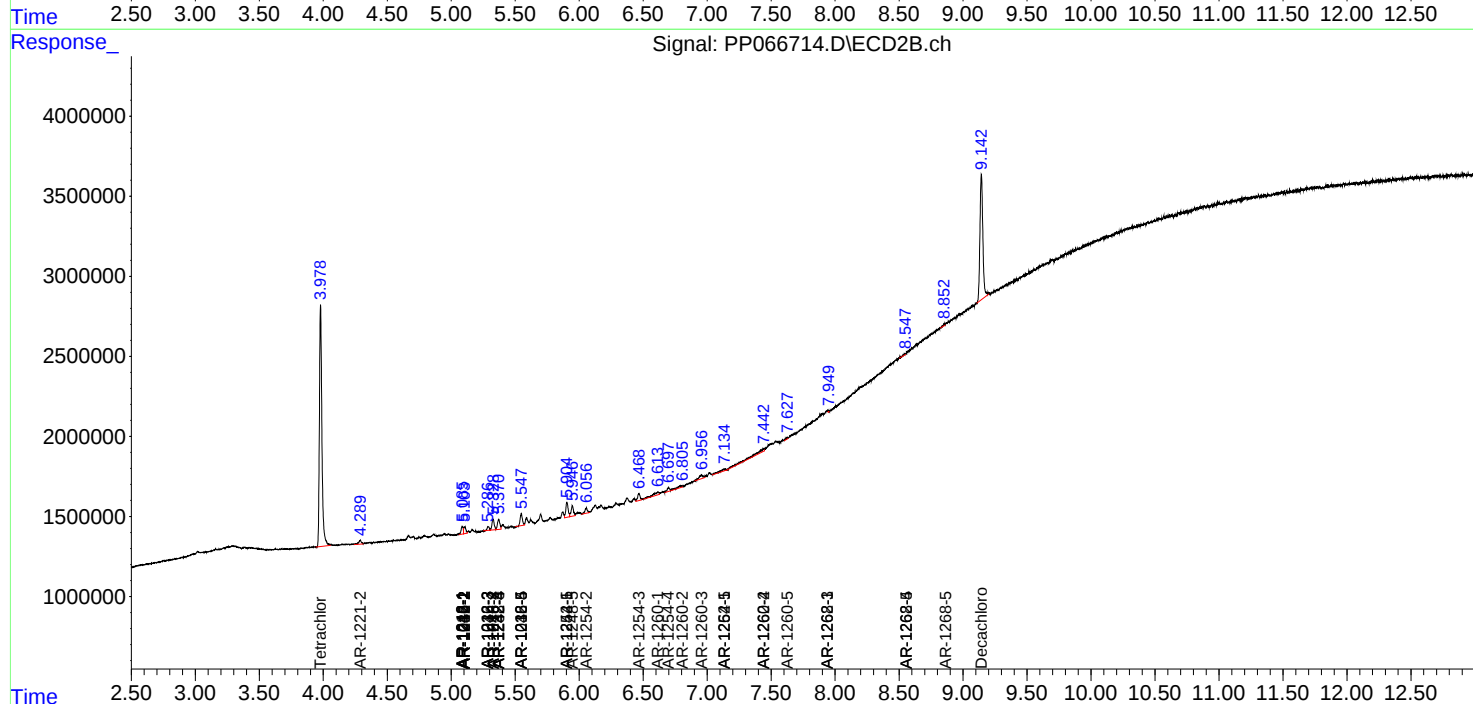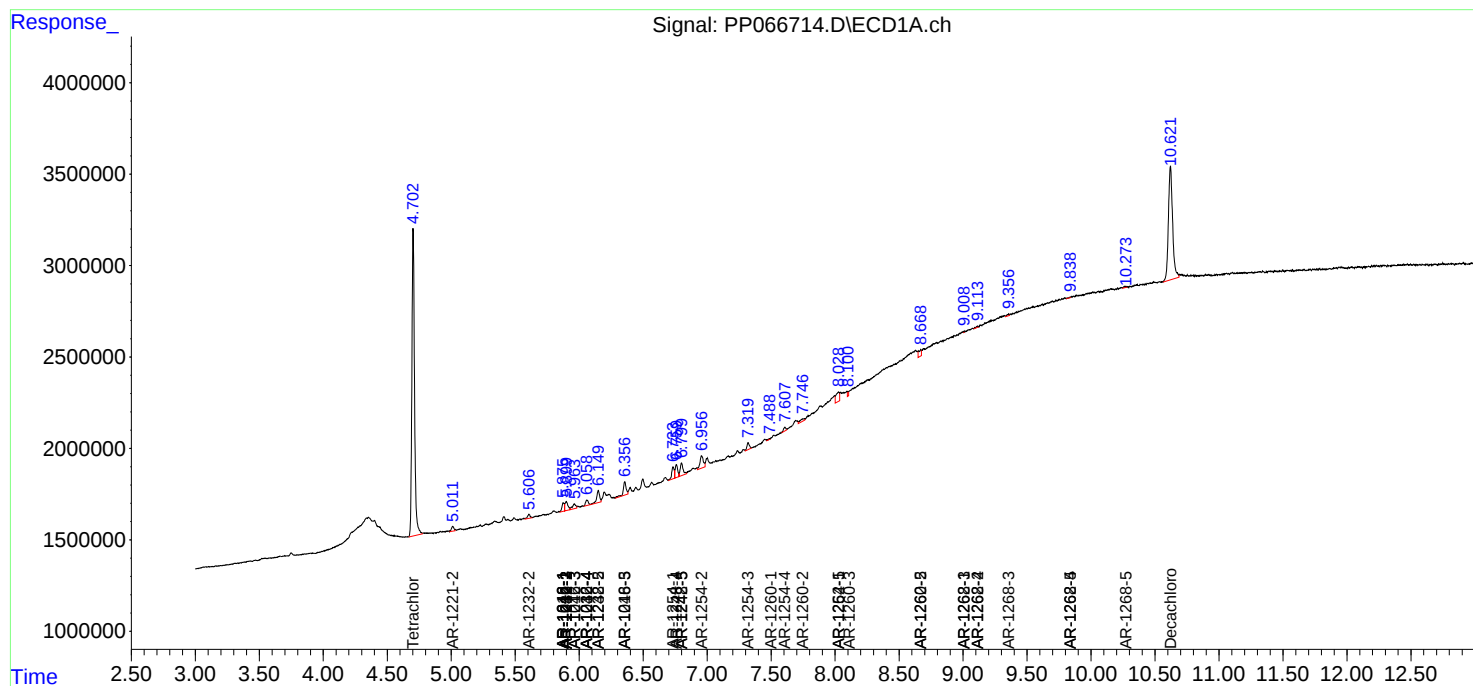


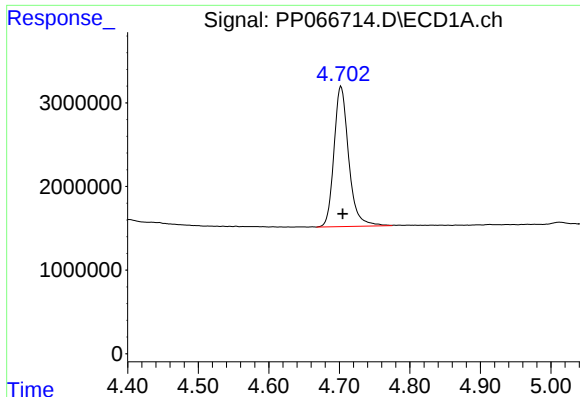

#1 Tetrachloro-m-xylene


R.T.: 4.702 min
Delta R.T.: -0.003 min
Response: 24253424
Conc: 16.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

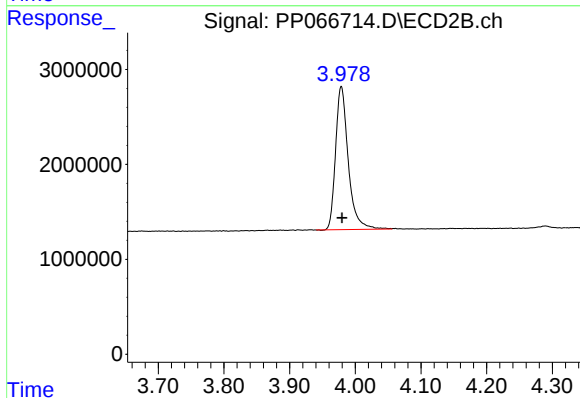


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.001 min
Response: 20257177
Conc: 15.49 ng/ml

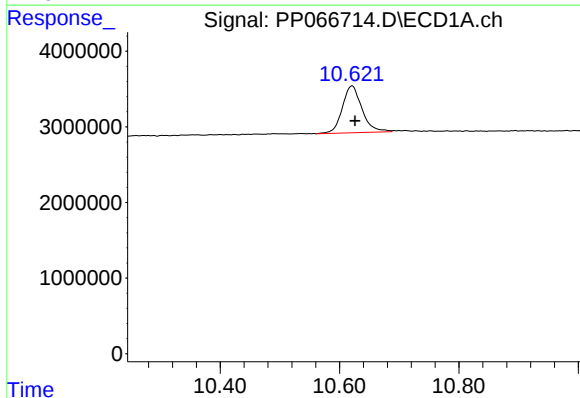


#2 Decachlorobiphenyl

R.T.: 10.621 min
Delta R.T.: -0.005 min
Response: 14144894
Conc: 16.12 ng/ml

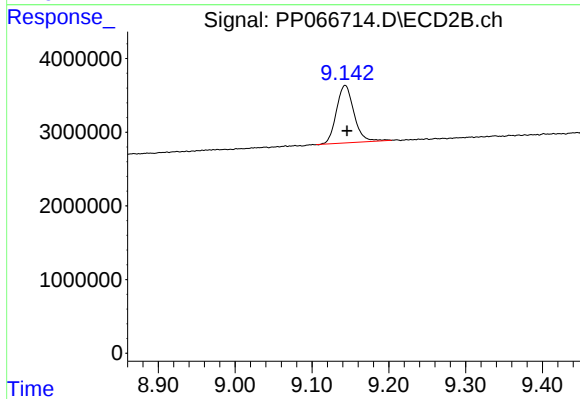

#2 Decachlorobiphenyl


R.T.: 9.143 min
Delta R.T.: -0.002 min
Response: 12338848
Conc: 14.81 ng/ml

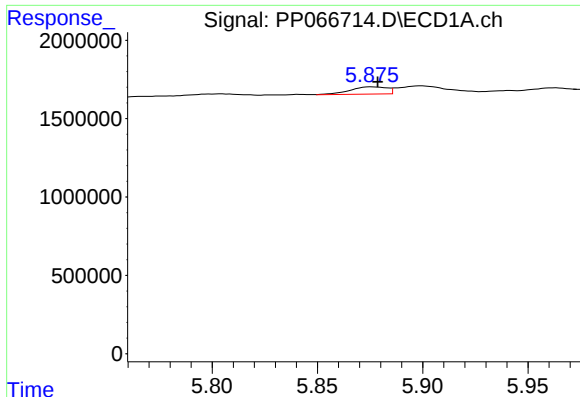

#3 AR-1016-1


R.T.: 5.876 min
Delta R.T.: -0.003 min
Response: 569917
Conc: 13.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

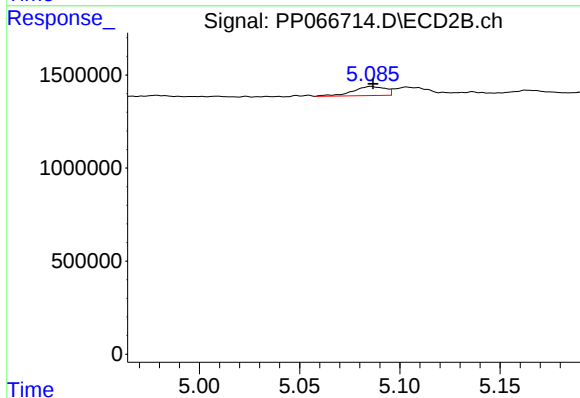


#3 AR-1016-1

R.T.: 5.086 min
Delta R.T.: 0.000 min
Response: 552986
Conc: 13.79 ng/ml

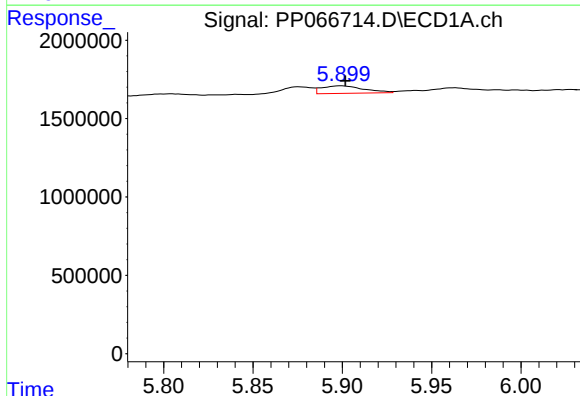


#4 AR-1016-2

R.T.: 5.899 min
Delta R.T.: -0.002 min
Response: 800731
Conc: 11.97 ng/ml

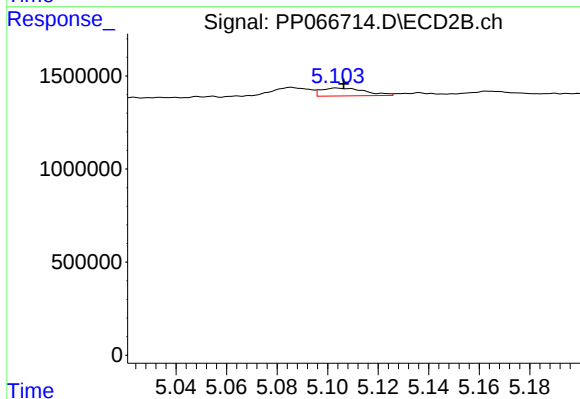

#4 AR-1016-2


R.T.: 5.104 min
Delta R.T.: -0.003 min
Response: 510780
Conc: 8.57 ng/ml

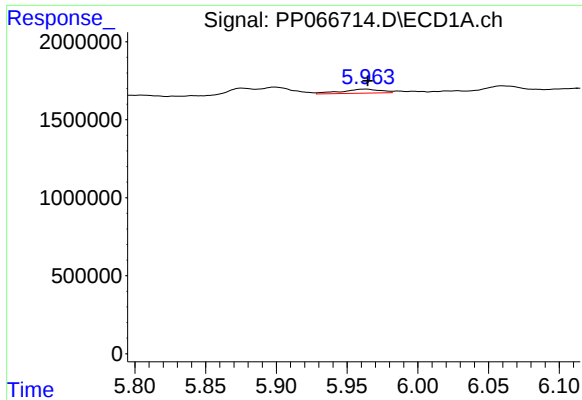

#5 AR-1016-3


R.T.: 5.963 min
Delta R.T.: -0.002 min
Response: 492606
Conc: 11.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

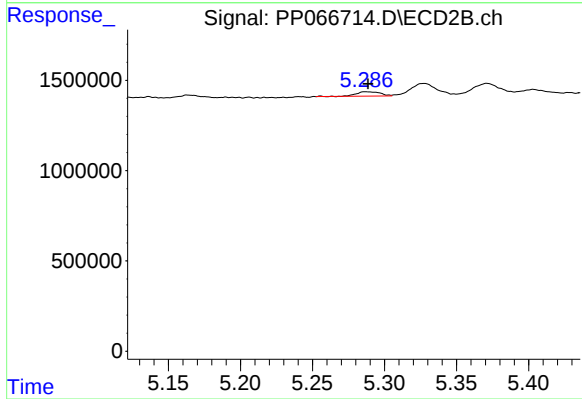


#5 AR-1016-3

R.T.: 5.287 min
Delta R.T.: -0.002 min
Response: 271686
Conc: 9.09 ng/ml

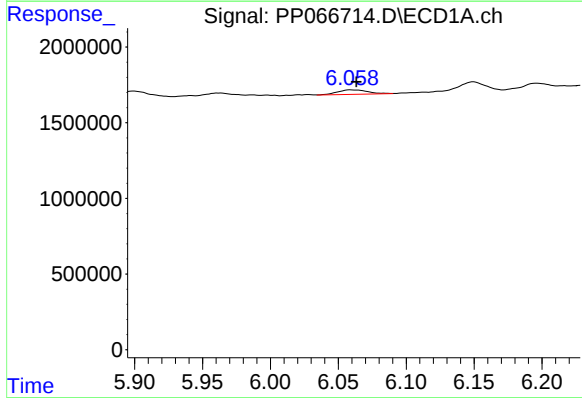


#6 AR-1016-4

R.T.: 6.059 min
Delta R.T.: -0.004 min
Response: 456840
Conc: 14.00 ng/ml

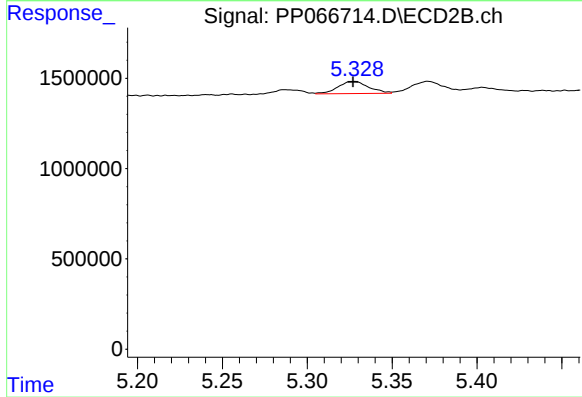

#6 AR-1016-4


R.T.: 5.327 min
Delta R.T.: 0.000 min
Response: 843751
Conc: 32.20 ng/ml

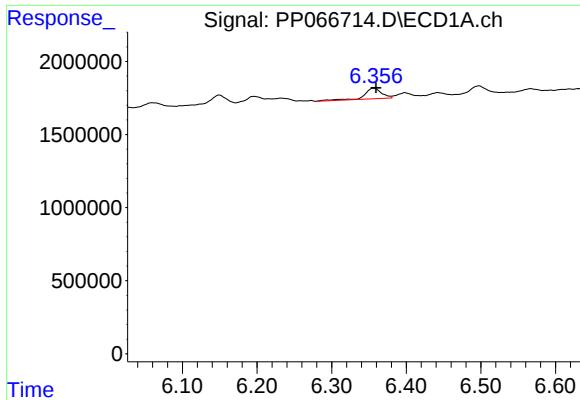

#7 AR-1016-5


R.T.: 6.357 min
Delta R.T.: -0.003 min
Response: 1169075
Conc: 36.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

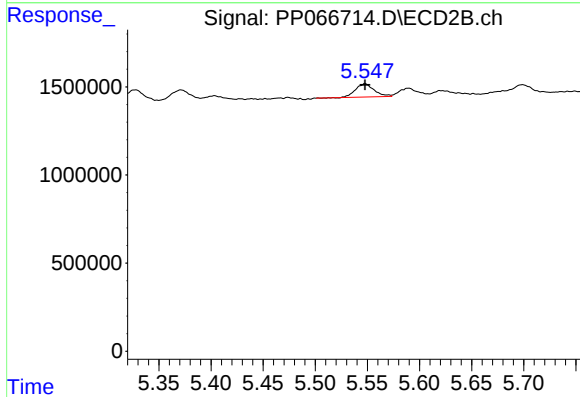


#7 AR-1016-5

R.T.: 5.548 min
Delta R.T.: 0.000 min
Response: 932924
Conc: 28.73 ng/ml

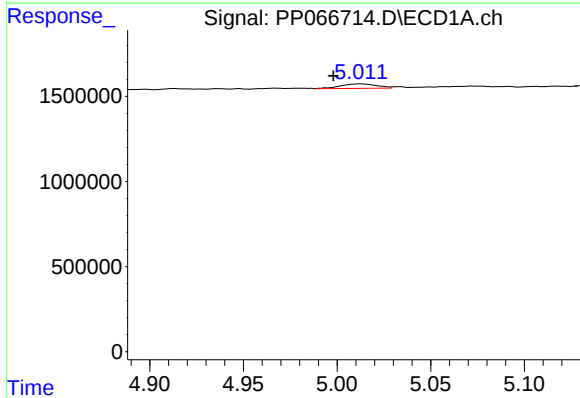


#9 AR-1221-2

R.T.: 5.012 min
Delta R.T.: 0.014 min
Response: 343110
Conc: 27.67 ng/ml

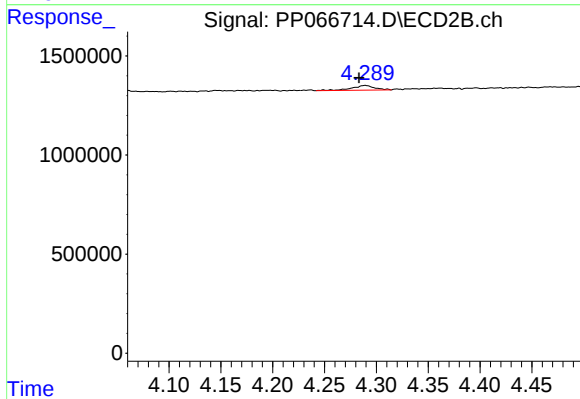

#9 AR-1221-2


R.T.: 4.289 min
Delta R.T.: 0.006 min
Response: 371601
Conc: 31.66 ng/ml

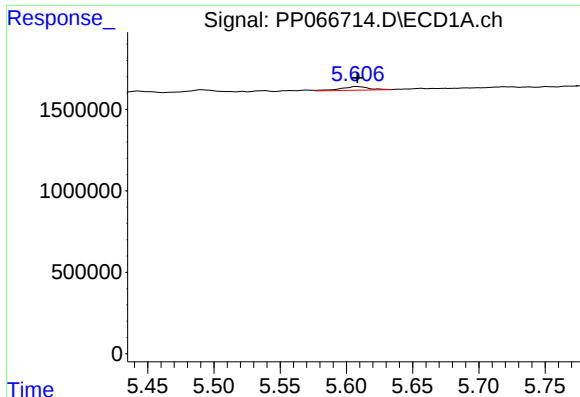

#12 AR-1232-2


R.T.: 5.608 min
Delta R.T.: 0.000 min
Response: 328859
Conc: 18.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

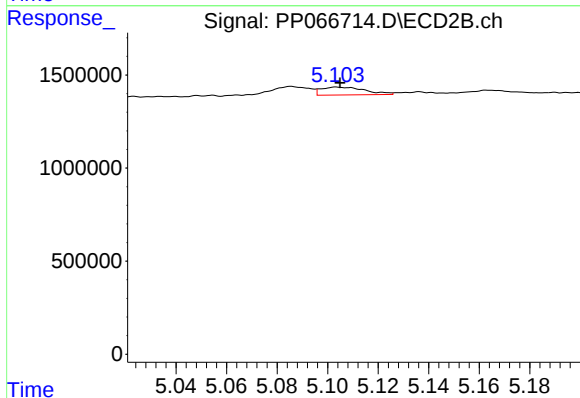


#12 AR-1232-2

R.T.: 5.104 min
Delta R.T.: -0.001 min
Response: 510780
Conc: 18.93 ng/ml

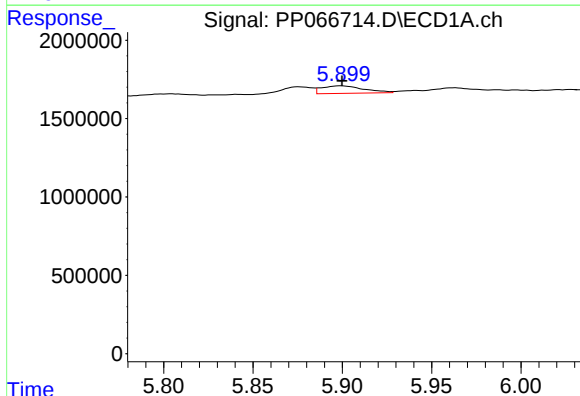


#13 AR-1232-3

R.T.: 5.899 min
Delta R.T.: 0.000 min
Response: 800731
Conc: 26.52 ng/ml

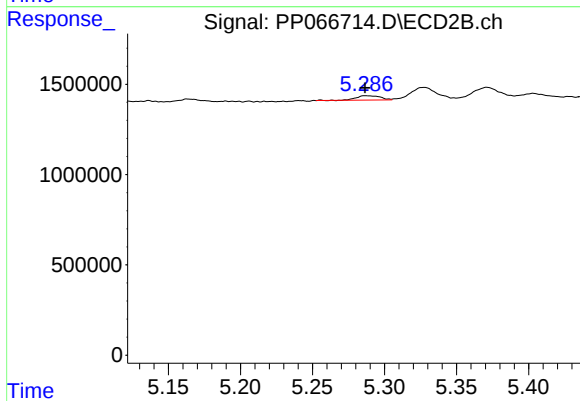

#13 AR-1232-3


R.T.: 5.287 min
Delta R.T.: 0.000 min
Response: 271686
Conc: 20.26 ng/ml

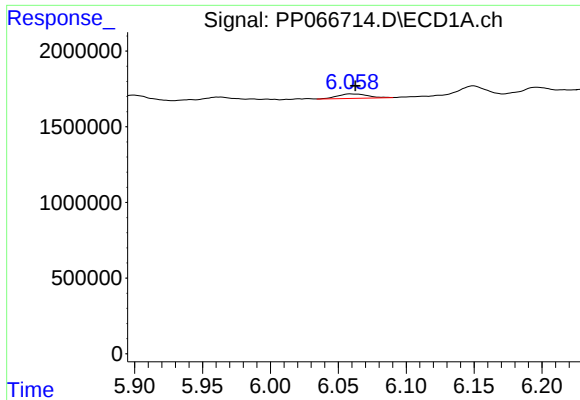

#14 AR-1232-4


R.T.: 6.059 min
Delta R.T.: -0.003 min
Response: 456840
Conc: 31.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

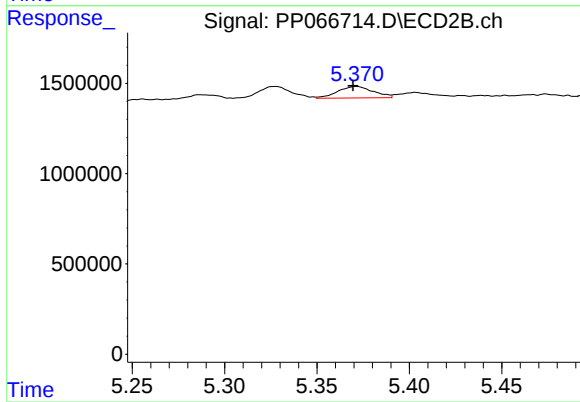


#14 AR-1232-4

R.T.: 5.371 min
Delta R.T.: 0.002 min
Response: 857926
Conc: 66.74 ng/ml

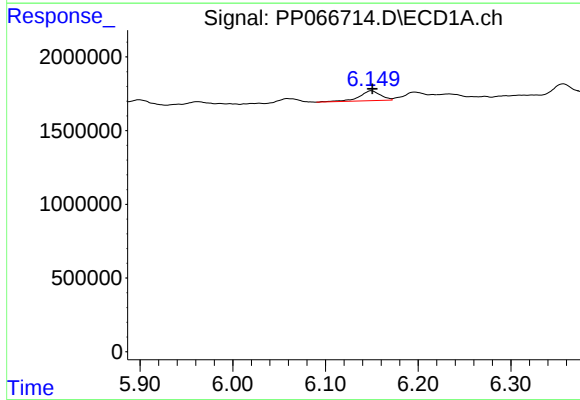


#15 AR-1232-5

R.T.: 6.150 min
Delta R.T.: 0.000 min
Response: 1054718
Conc: 88.85 ng/ml

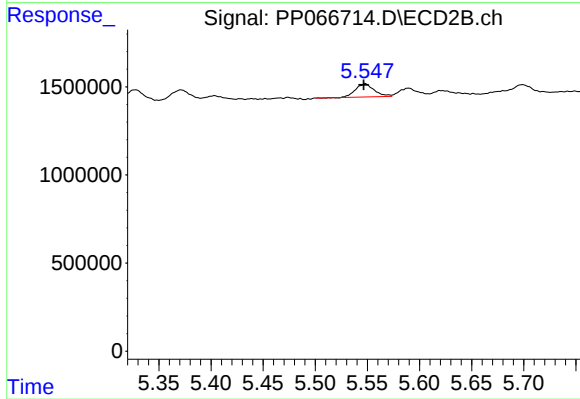

#15 AR-1232-5


R.T.: 5.548 min
Delta R.T.: 0.001 min
Response: 932924
Conc: 67.36 ng/ml

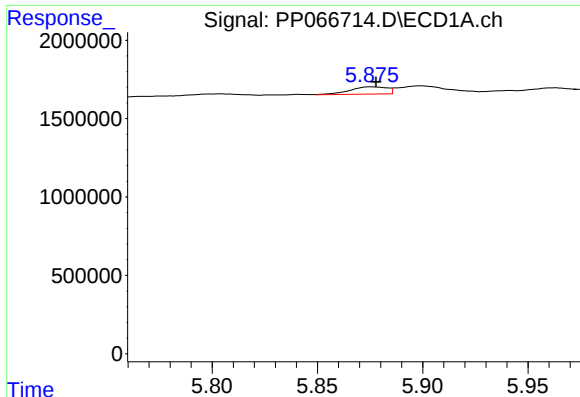

#16 AR-1242-1


R.T.: 5.876 min
Delta R.T.: -0.002 min
Response: 569917
Conc: 17.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

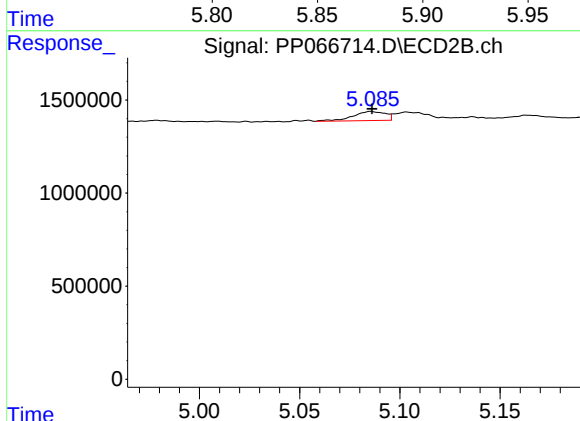


#16 AR-1242-1

R.T.: 5.086 min
Delta R.T.: 0.000 min
Response: 552986
Conc: 18.02 ng/ml

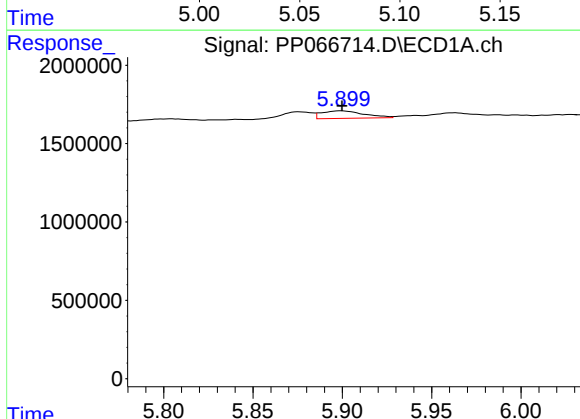


#17 AR-1242-2

R.T.: 5.899 min
Delta R.T.: 0.000 min
Response: 800731
Conc: 15.82 ng/ml

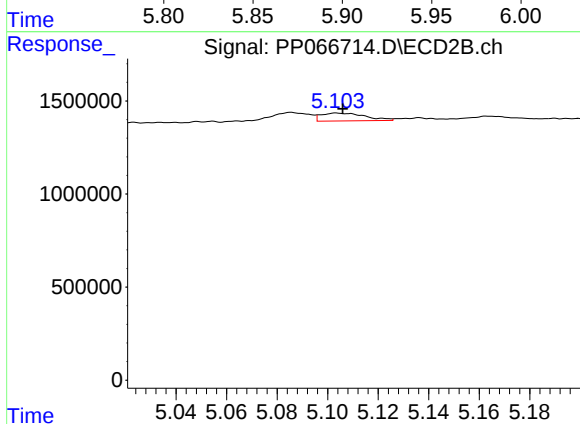

#17 AR-1242-2


R.T.: 5.104 min
Delta R.T.: -0.002 min
Response: 510780
Conc: 11.27 ng/ml

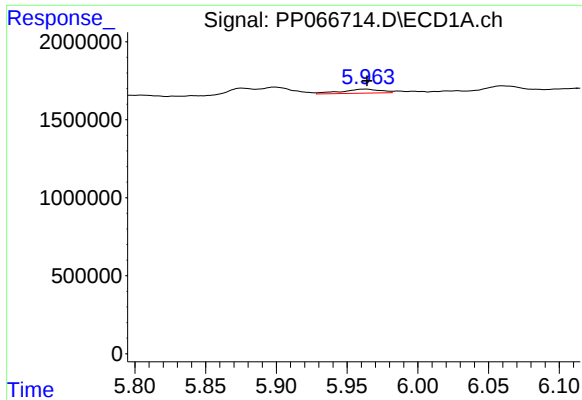

#18 AR-1242-3


R.T.: 5.963 min
Delta R.T.: 0.000 min
Response: 492606
Conc: 15.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

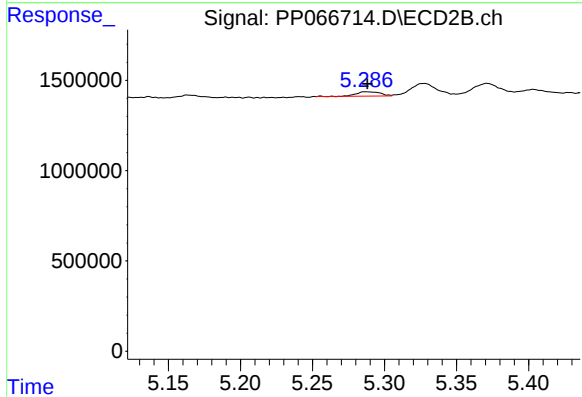


#18 AR-1242-3

R.T.: 5.287 min
Delta R.T.: 0.000 min
Response: 271686
Conc: 11.63 ng/ml

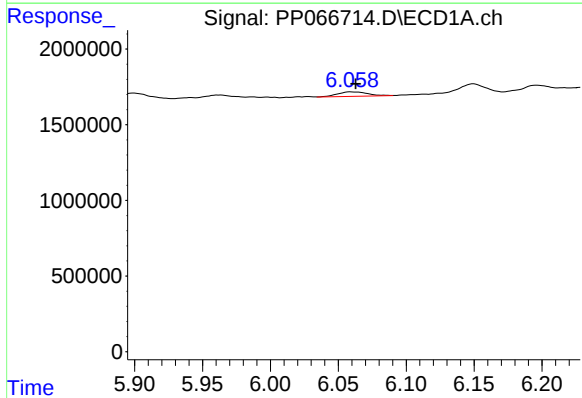


#19 AR-1242-4

R.T.: 6.059 min
Delta R.T.: -0.003 min
Response: 456840
Conc: 18.44 ng/ml

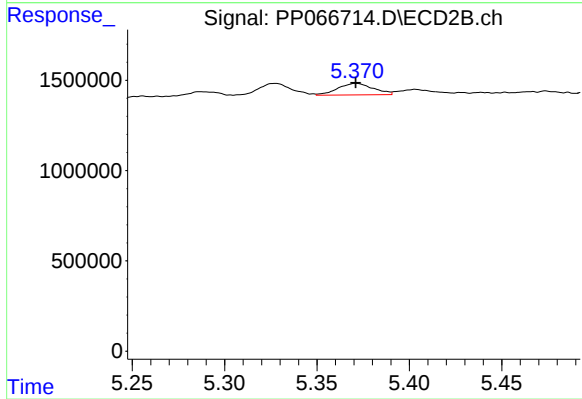

#19 AR-1242-4


R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 857926
Conc: 34.09 ng/ml

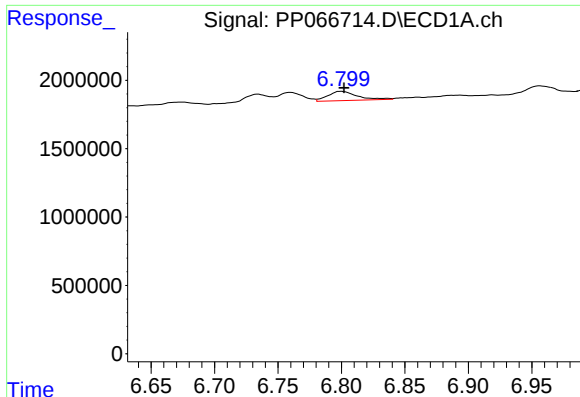

#20 AR-1242-5


R.T.: 6.800 min
Delta R.T.: -0.002 min
Response: 1091862
Conc: 43.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

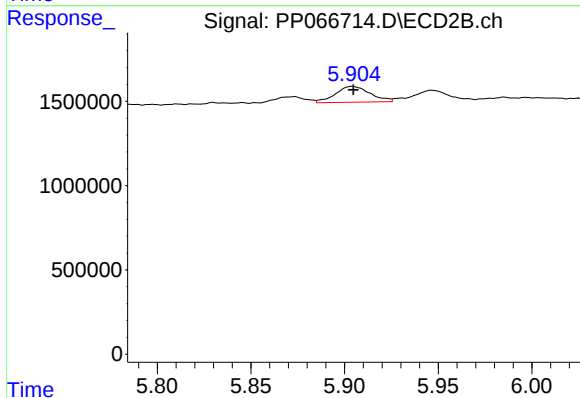


#20 AR-1242-5

R.T.: 5.904 min
Delta R.T.: 0.000 min
Response: 1211680
Conc: 42.84 ng/ml

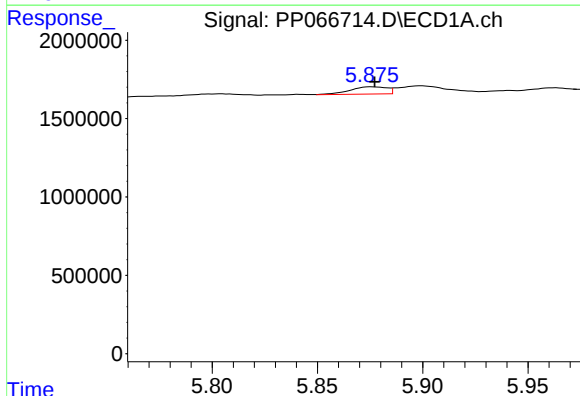


#21 AR-1248-1

R.T.: 5.876 min
Delta R.T.: -0.002 min
Response: 569917
Conc: 22.30 ng/ml

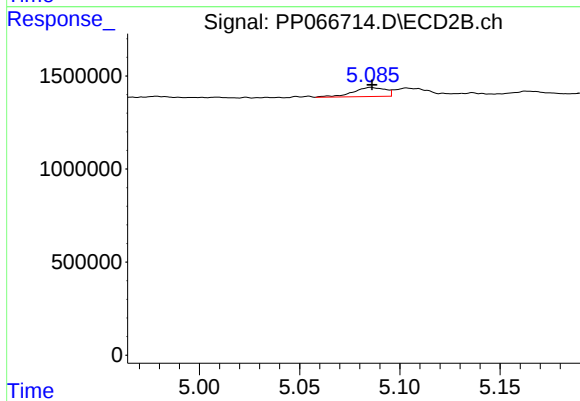

#21 AR-1248-1


R.T.: 5.086 min
Delta R.T.: 0.000 min
Response: 552986
Conc: 22.84 ng/ml

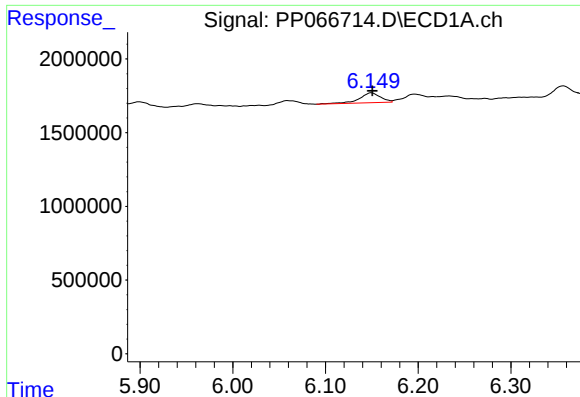

#22 AR-1248-2


R.T.: 6.150 min
Delta R.T.: 0.000 min
Response: 1054718
Conc: 26.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

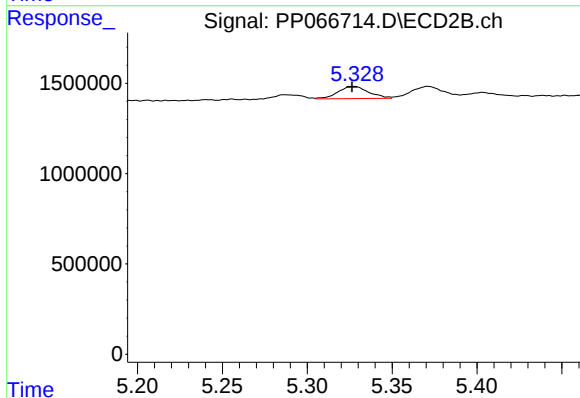


#22 AR-1248-2

R.T.: 5.327 min
Delta R.T.: 0.000 min
Response: 843751
Conc: 23.36 ng/ml

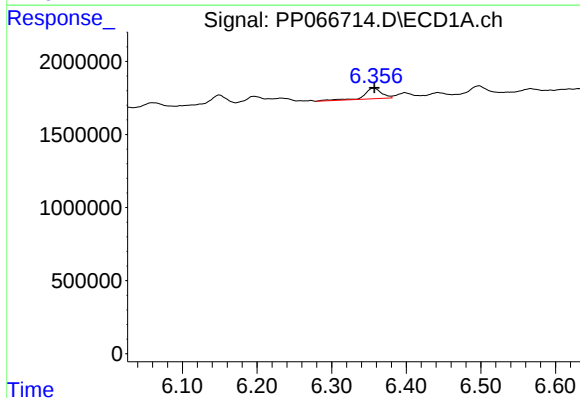


#23 AR-1248-3

R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 1169075
Conc: 26.81 ng/ml

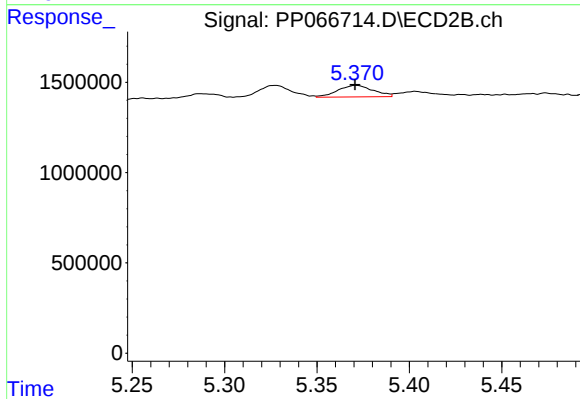

#23 AR-1248-3


R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 857926
Conc: 22.98 ng/ml

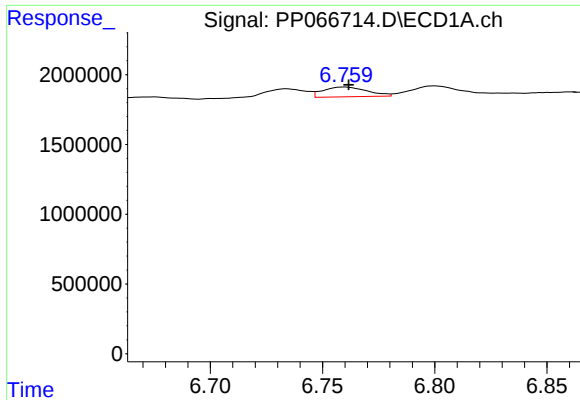

#24 AR-1248-4


R.T.: 6.760 min
Delta R.T.: -0.002 min
Response: 967016
Conc: 21.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

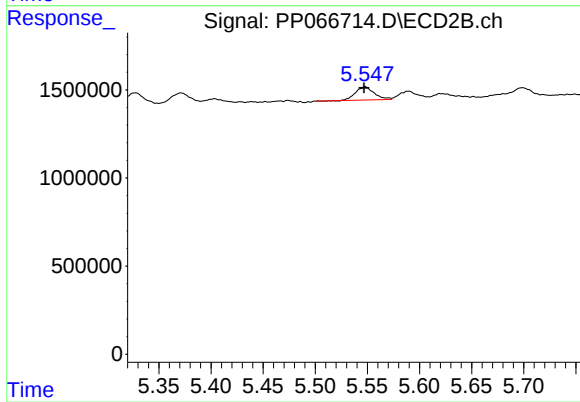


#24 AR-1248-4

R.T.: 5.548 min
Delta R.T.: 0.000 min
Response: 932924
Conc: 21.14 ng/ml

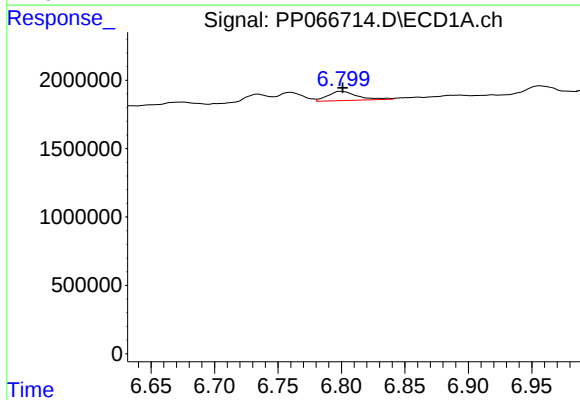


#25 AR-1248-5

R.T.: 6.800 min
Delta R.T.: -0.001 min
Response: 1091862
Conc: 23.82 ng/ml

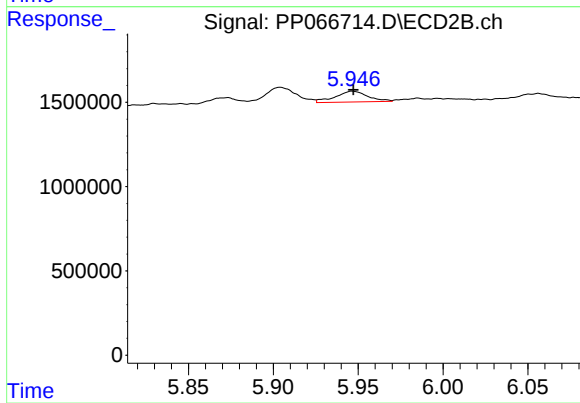

#25 AR-1248-5


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 855838
Conc: 22.66 ng/ml

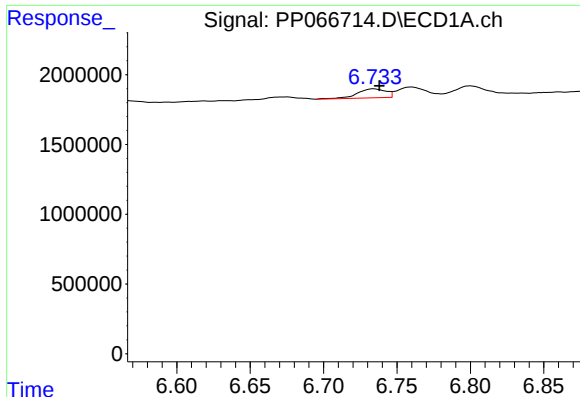

#26 AR-1254-1


R.T.: 6.734 min
Delta R.T.: -0.004 min
Response: 874349
Conc: 17.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

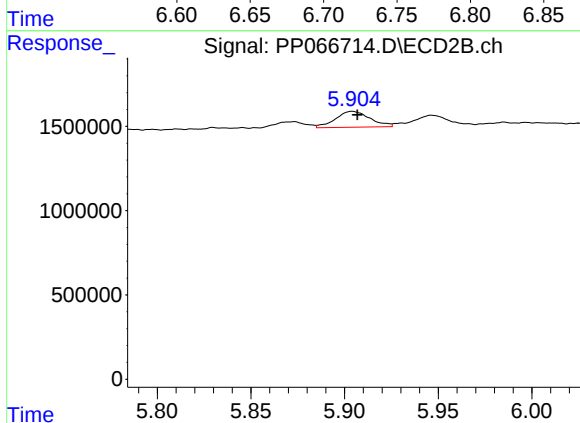


#26 AR-1254-1

R.T.: 5.904 min
Delta R.T.: -0.003 min
Response: 1211680
Conc: 20.23 ng/ml

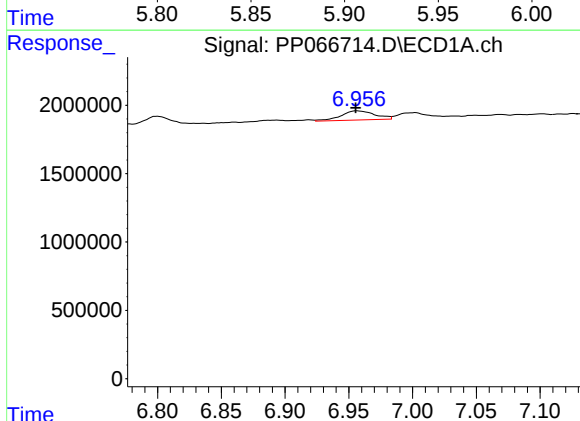


#27 AR-1254-2

R.T.: 6.956 min
Delta R.T.: 0.001 min
Response: 1239256
Conc: 16.99 ng/ml

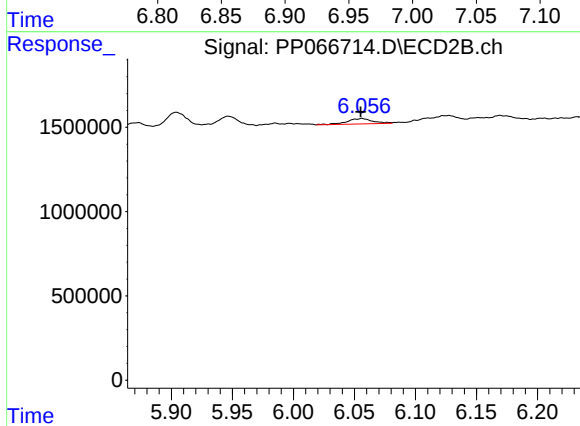

#27 AR-1254-2


R.T.: 6.056 min
Delta R.T.: 0.001 min
Response: 472864
Conc: 8.85 ng/ml

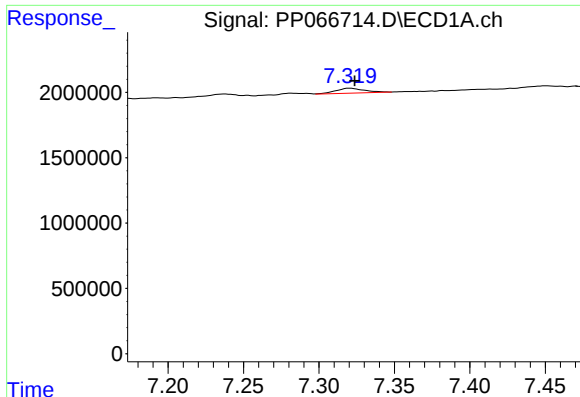

#28 AR-1254-3


R.T.: 7.320 min
Delta R.T.: -0.003 min
Response: 501014
Conc: 7.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

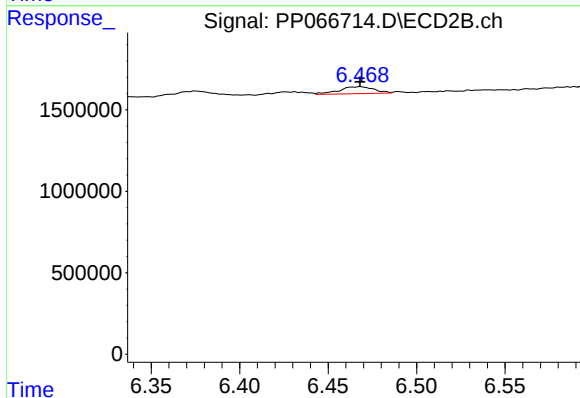


#28 AR-1254-3

R.T.: 6.468 min
Delta R.T.: 0.000 min
Response: 585599
Conc: 7.41 ng/ml

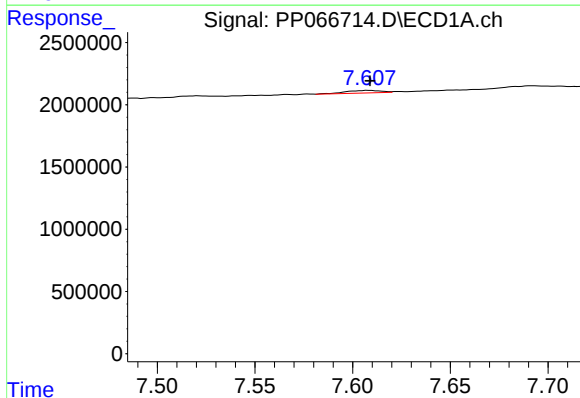


#29 AR-1254-4

R.T.: 7.608 min
Delta R.T.: 0.000 min
Response: 255287
Conc: 5.73 ng/ml

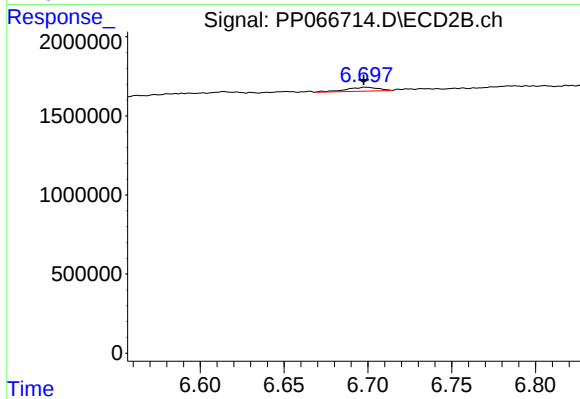

#29 AR-1254-4


R.T.: 6.699 min
Delta R.T.: 0.002 min
Response: 332209
Conc: 8.22 ng/ml

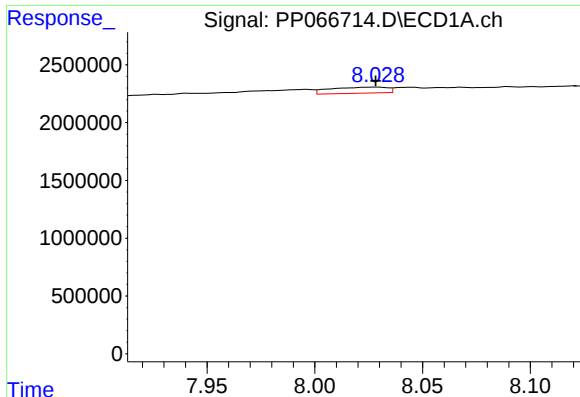

#30 AR-1254-5


R.T.: 8.029 min
Delta R.T.: 0.000 min
Response: 962716
Conc: 14.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

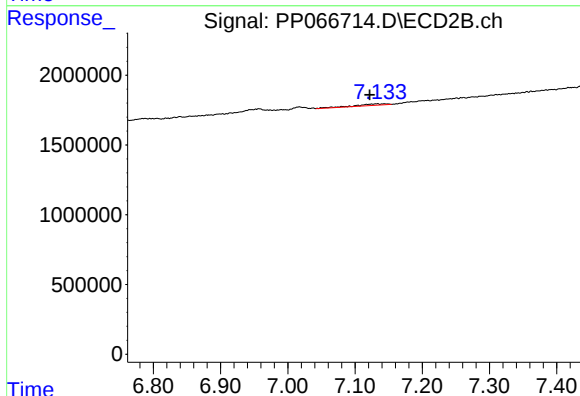


#30 AR-1254-5

R.T.: 7.133 min
Delta R.T.: 0.011 min
Response: 376071
Conc: 5.85 ng/ml

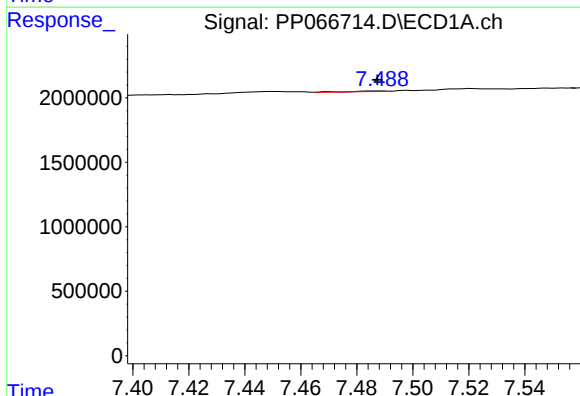


#31 AR-1260-1

R.T.: 7.488 min
Delta R.T.: 0.001 min
Response: 45860
Conc: 0.82 ng/ml

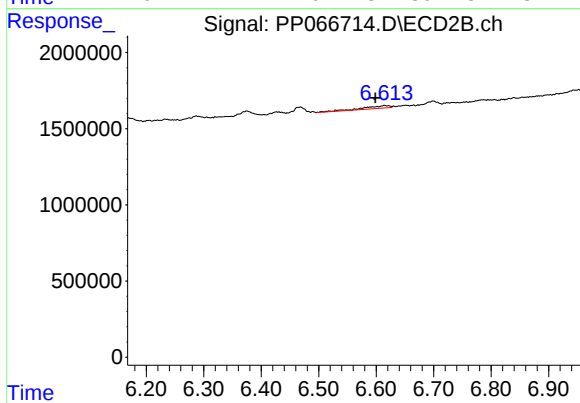

#31 AR-1260-1


R.T.: 6.614 min
Delta R.T.: 0.015 min
Response: 570708
Conc: 9.66 ng/ml

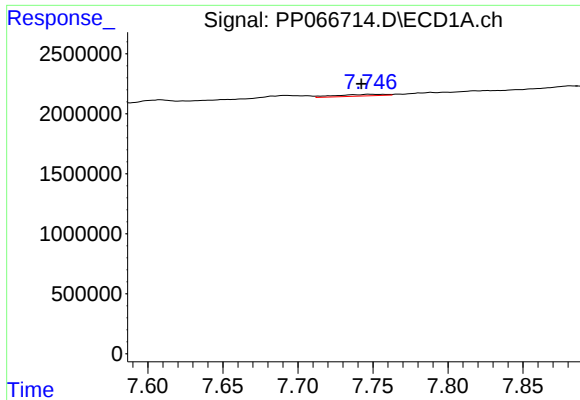

#32 AR-1260-2


R.T.: 7.748 min
Delta R.T.: 0.006 min
Response: 312102
Conc: 4.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

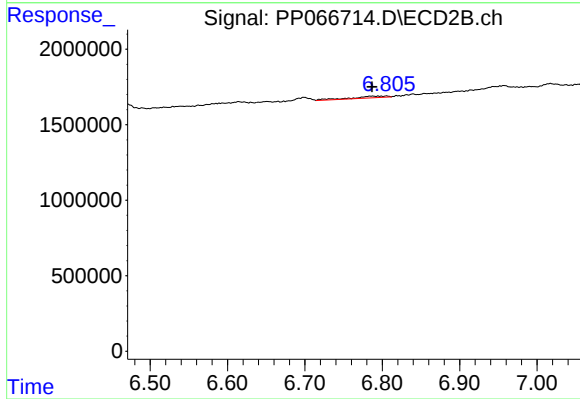


#32 AR-1260-2

R.T.: 6.806 min
Delta R.T.: 0.019 min
Response: 335883
Conc: 4.93 ng/ml

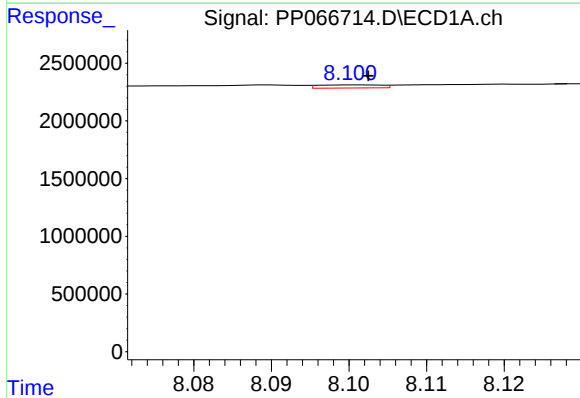


#33 AR-1260-3

R.T.: 8.101 min
Delta R.T.: -0.001 min
Response: 148369
Conc: 3.34 ng/ml

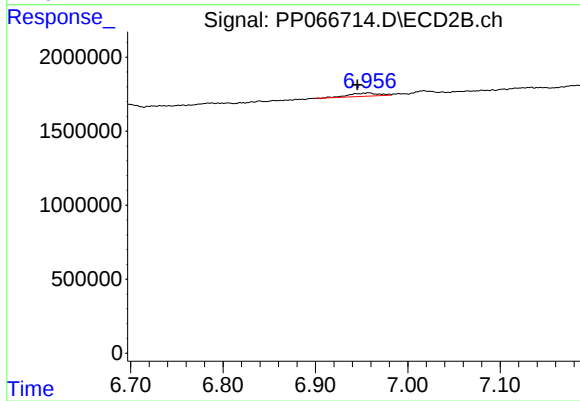

#33 AR-1260-3


R.T.: 6.958 min
Delta R.T.: 0.012 min
Response: 500393
Conc: 7.70 ng/ml

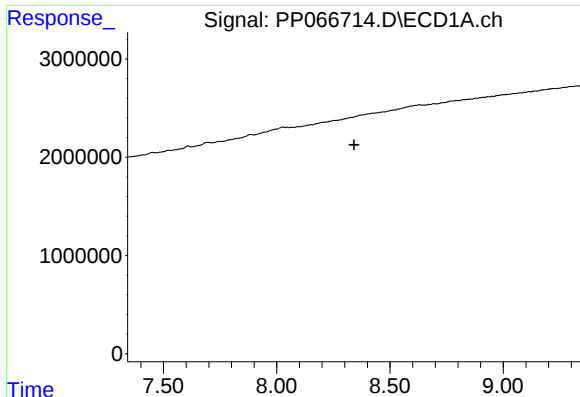

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 8.341 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

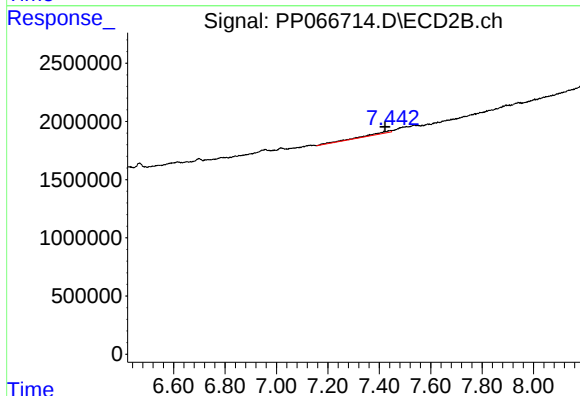


#34 AR-1260-4

R.T.: 7.444 min
Delta R.T.: 0.021 min
Response: 1132667
Conc: 25.15 ng/ml

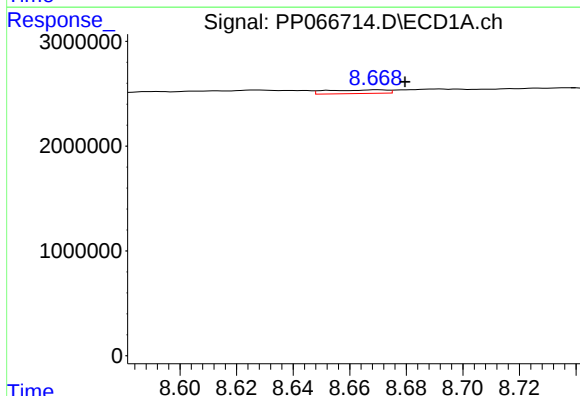


#35 AR-1260-5

R.T.: 8.670 min
Delta R.T.: -0.010 min
Response: 506347
Conc: 5.69 ng/ml

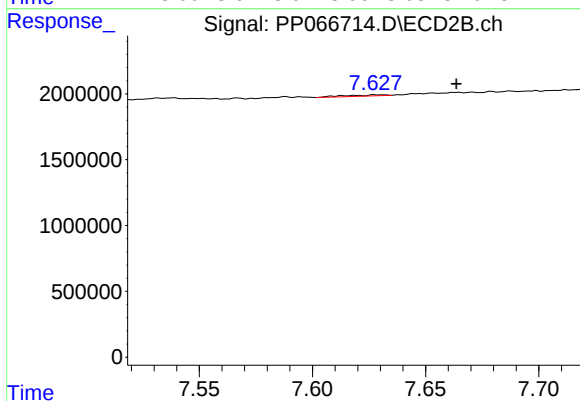

#35 AR-1260-5


R.T.: 7.629 min
Delta R.T.: -0.035 min
Response: 109559
Conc: 1.14 ng/ml

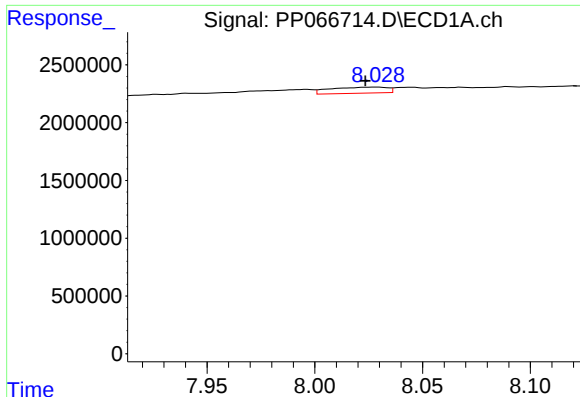

#36 AR-1262-1


R.T.: 8.029 min
Delta R.T.: 0.005 min
Response: 962716
Conc: 21.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

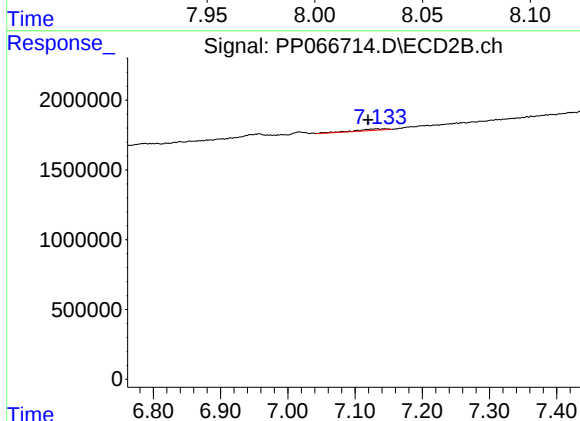


#36 AR-1262-1

R.T.: 7.133 min
Delta R.T.: 0.014 min
Response: 376071
Conc: 11.77 ng/ml

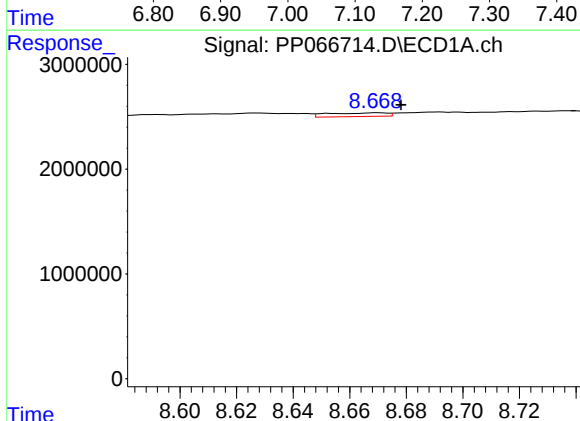


#37 AR-1262-2

R.T.: 8.670 min
Delta R.T.: -0.009 min
Response: 506347
Conc: 4.64 ng/ml

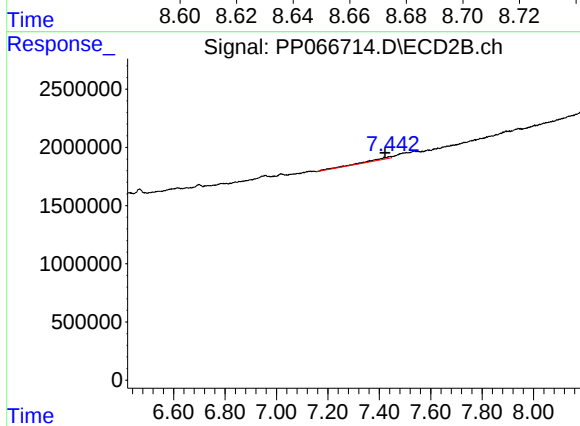

#37 AR-1262-2


R.T.: 7.444 min
Delta R.T.: 0.022 min
Response: 1132667
Conc: 18.17 ng/ml

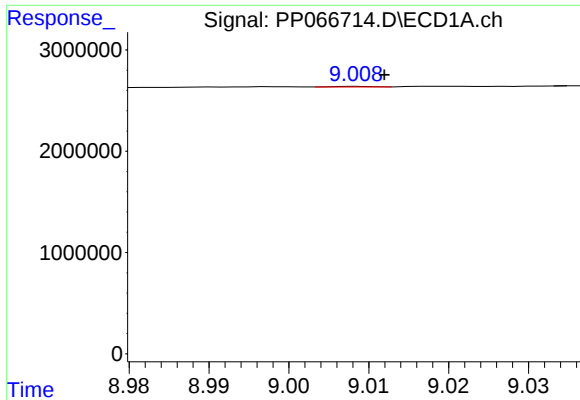

#38 AR-1262-3


R.T.: 9.009 min
Delta R.T.: -0.003 min
Response: 19950
Conc: 0.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

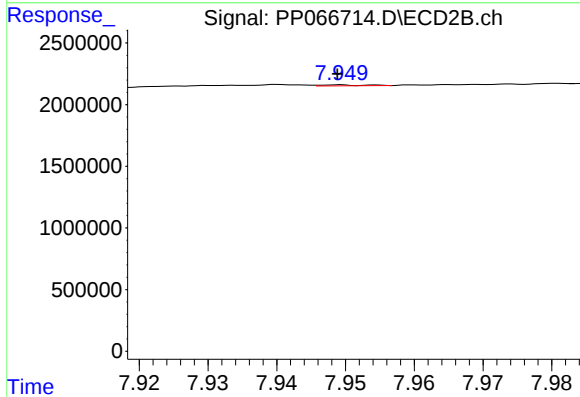


#38 AR-1262-3

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 34200
Conc: 0.76 ng/ml

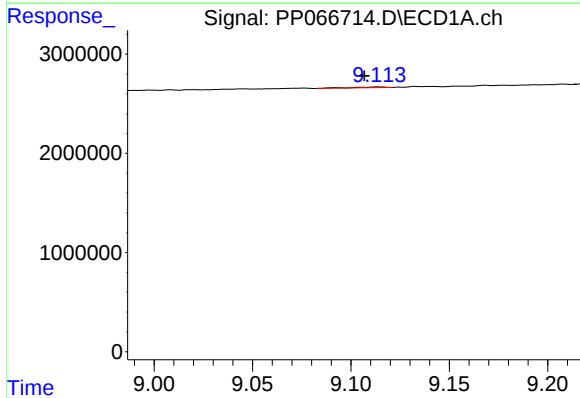


#39 AR-1262-4

R.T.: 9.114 min
Delta R.T.: 0.007 min
Response: 92683
Conc: 1.59 ng/ml

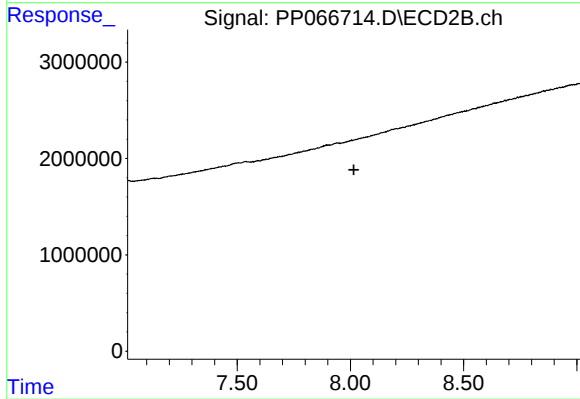

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.015 min
Response: 0
Conc: N.D.

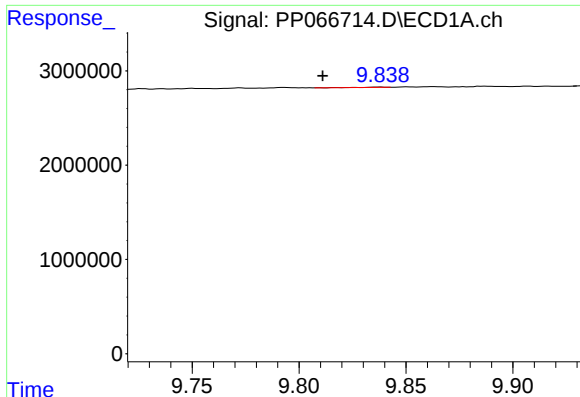

#40 AR-1262-5


R.T.: 9.838 min
Delta R.T.: 0.027 min
Response: 25106
Conc: 0.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

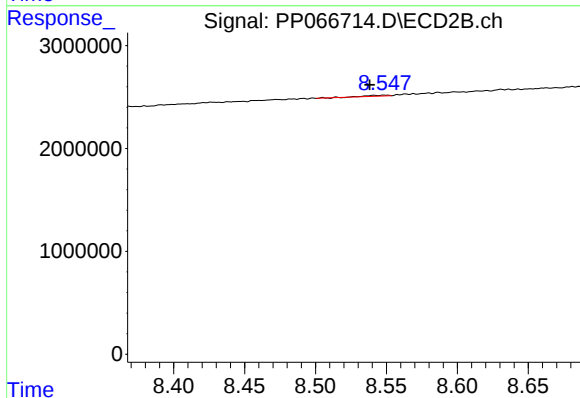


#40 AR-1262-5

R.T.: 8.549 min
Delta R.T.: 0.011 min
Response: 98306
Conc: 3.10 ng/ml

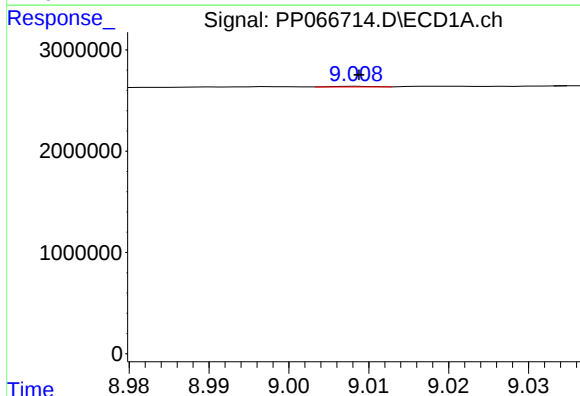


#41 AR-1268-1

R.T.: 9.009 min
Delta R.T.: 0.000 min
Response: 19950
Conc: 0.16 ng/ml

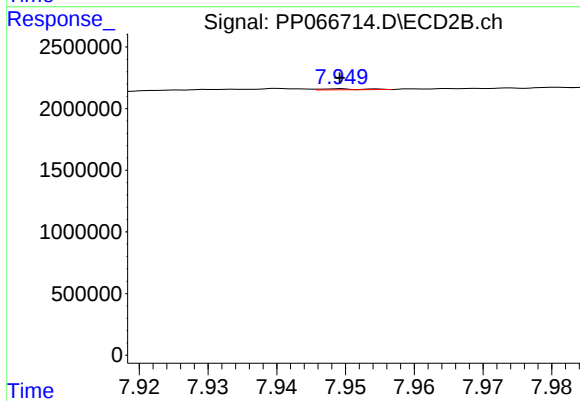

#41 AR-1268-1


R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 34200
Conc: 0.27 ng/ml

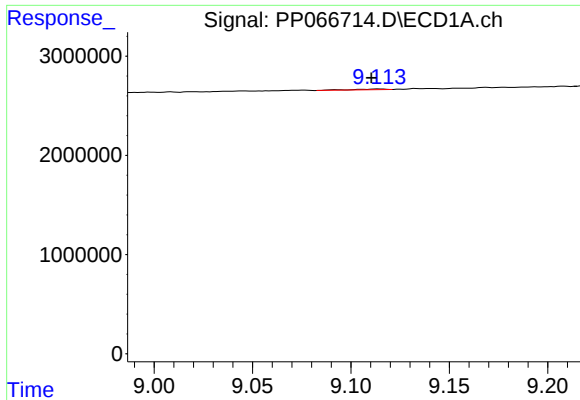

#42 AR-1268-2


R.T.: 9.114 min
Delta R.T.: 0.004 min
Response: 92683
Conc: 0.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

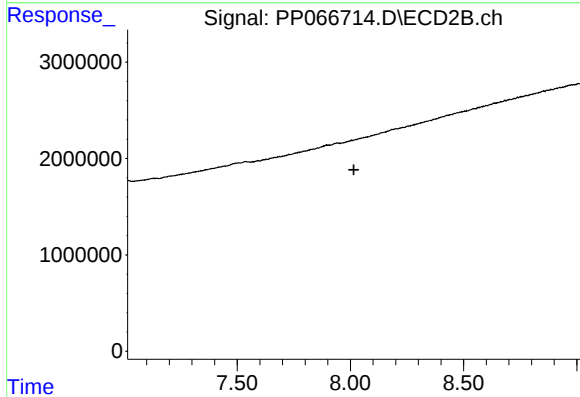


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.015 min
Response: 0
Conc: N.D.

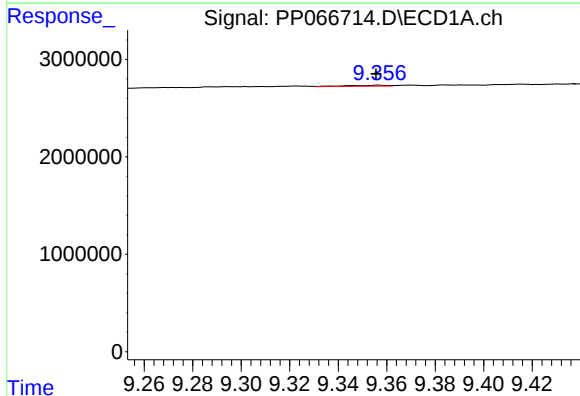


#43 AR-1268-3

R.T.: 9.357 min
Delta R.T.: 0.001 min
Response: 114636
Conc: 1.16 ng/ml

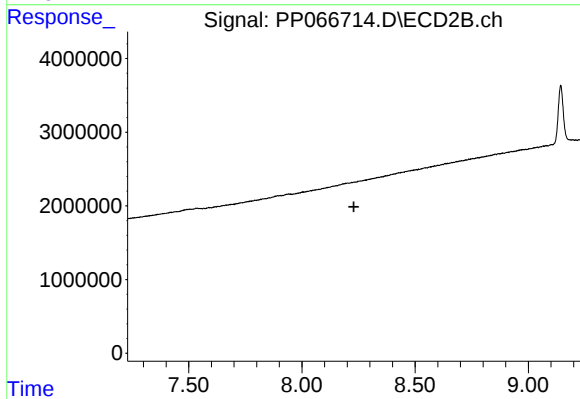

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.230 min
Response: 0
Conc: N.D.

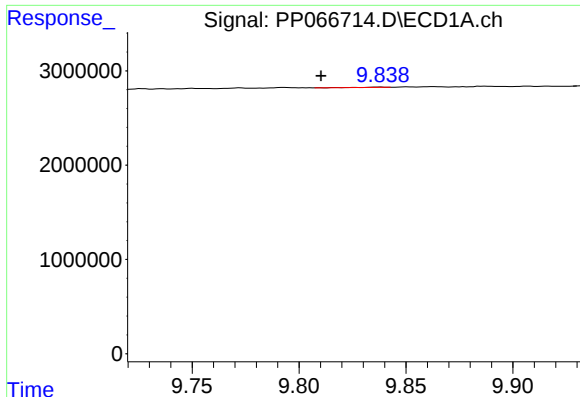

#44 AR-1268-4


R.T.: 9.838 min
Delta R.T.: 0.028 min
Response: 25106
Conc: 0.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

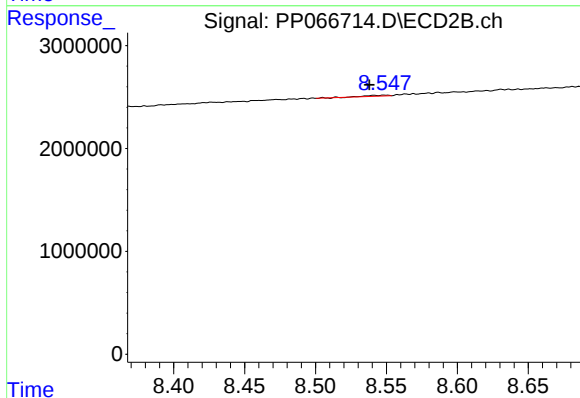


#44 AR-1268-4

R.T.: 8.549 min
Delta R.T.: 0.011 min
Response: 98306
Conc: 2.91 ng/ml

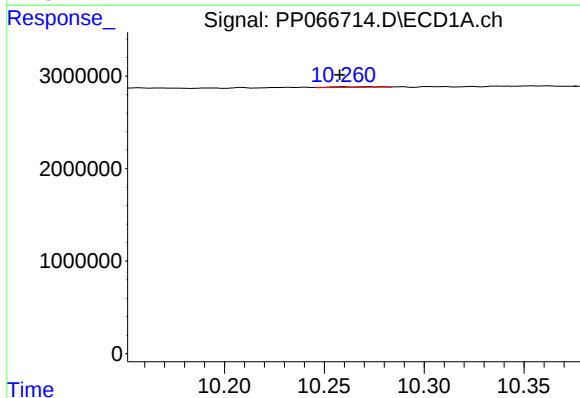

#45 AR-1268-5

R.T.: 10.273 min
Delta R.T.: 0.015 min
Response: 94231
Conc: 0.33 ng/ml

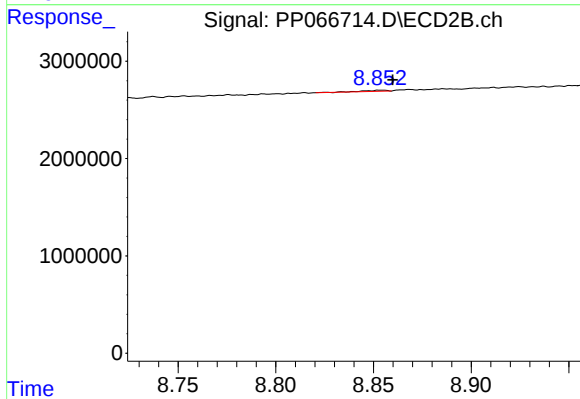

#45 AR-1268-5

R.T.: 8.854 min
Delta R.T.: -0.006 min
Response: 87222
Conc: 0.30 ng/ml