

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
 Data File : PP066712.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2024 01:24
 Operator : YP\AJ
 Sample : P3390-07
 Misc : AR1232 LOD 25 PPB
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 05:54:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 21 05:19:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.702	3.979	24593429	20429368	16.608	15.625
2) SA Decachlor...	10.621	9.144	14238685	12640764	16.225	15.174
Target Compounds						
11) L3 AR-1232-1	5.074	4.361	700937	596863	22.040	19.477
12) L3 AR-1232-2	5.607	5.106	370946	602705	21.416	22.337
13) L3 AR-1232-3	5.896	5.287	694011	232329	22.990	17.324
14) L3 AR-1232-4	6.062	5.371	309938	287750	21.044	22.385
15) L3 AR-1232-5	6.148	5.552	332445	325846	28.006	23.529



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
Data File : PP066712.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2024 01:24
Operator : YP\AJ
Sample : P3390-07
Misc : AR1232 LOD 25 PPB
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 05:54:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 21 05:19:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

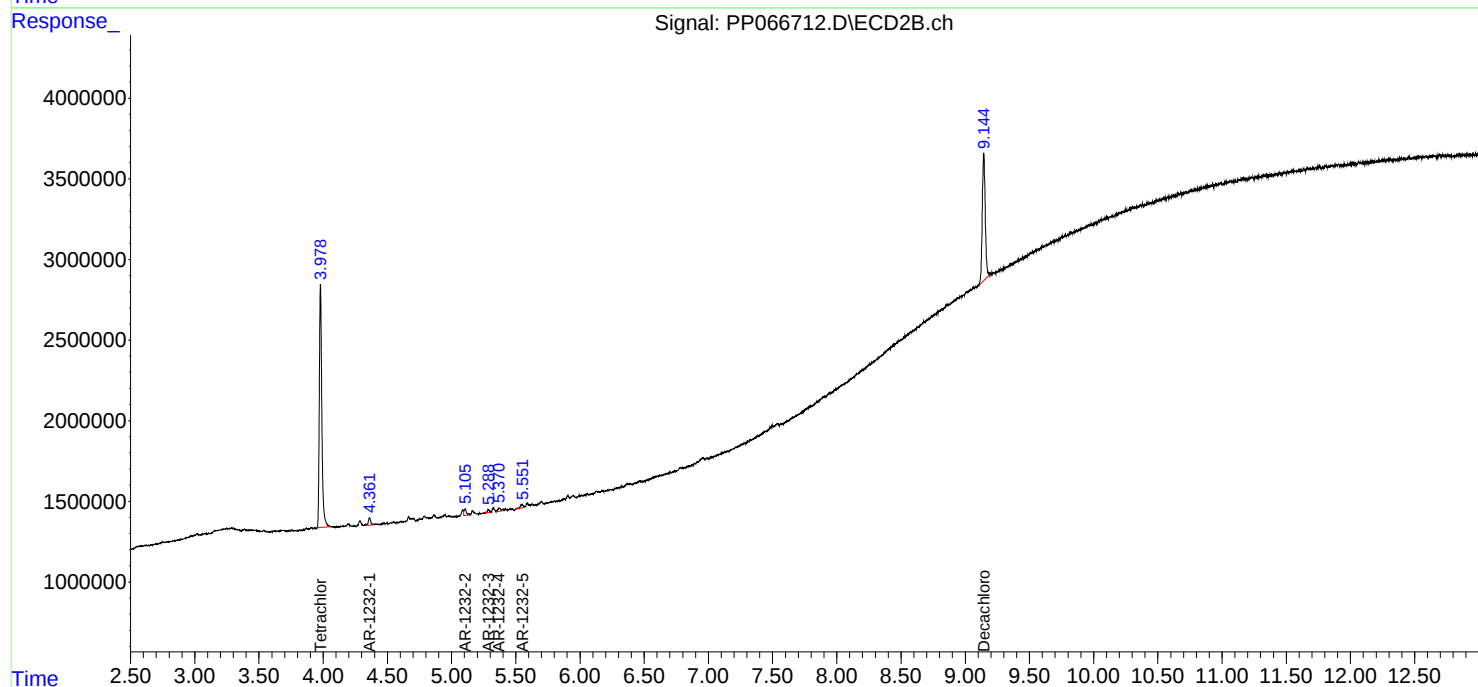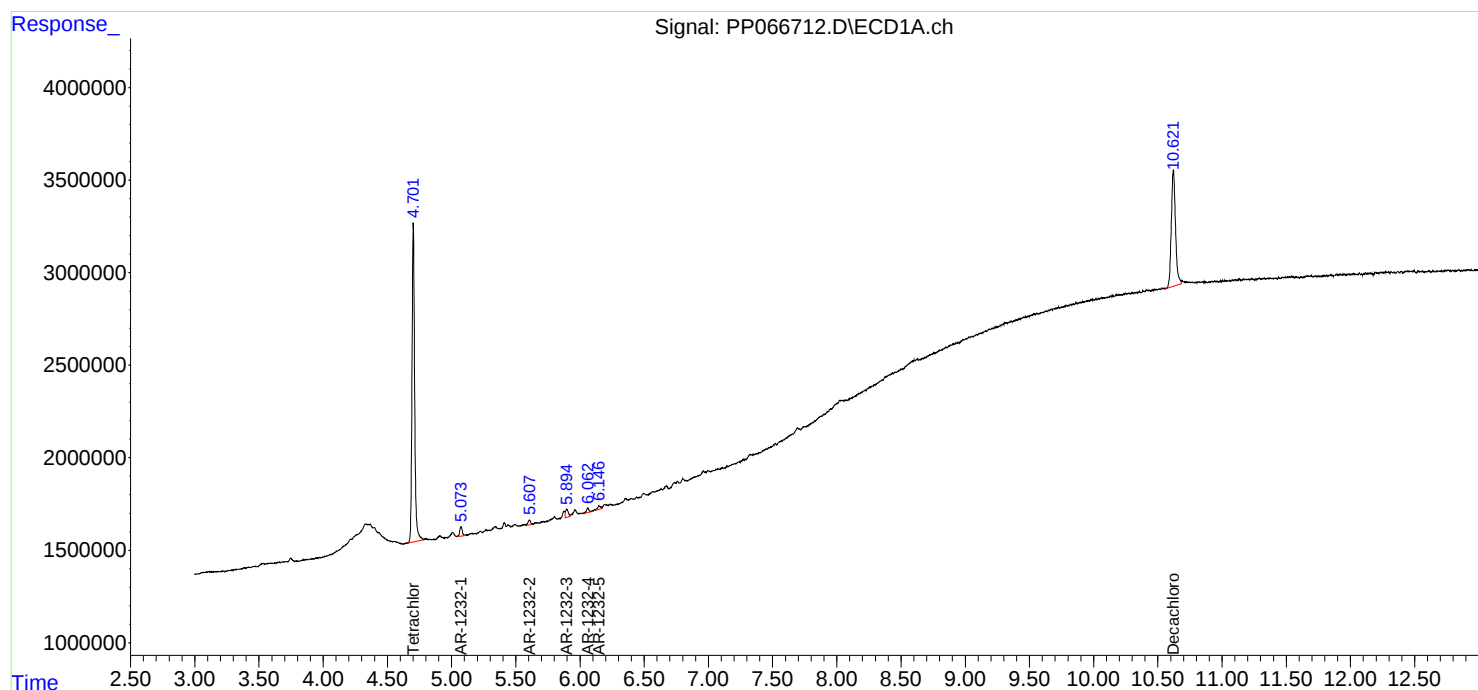


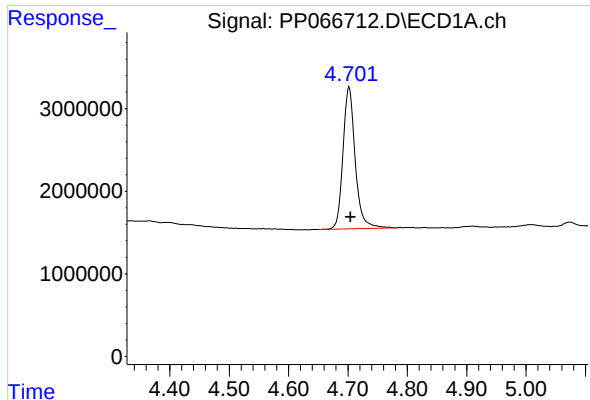

#1 Tetrachloro-m-xylene


R.T.: 4.702 min
Delta R.T.: -0.003 min
Response: 24593429
Conc: 16.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

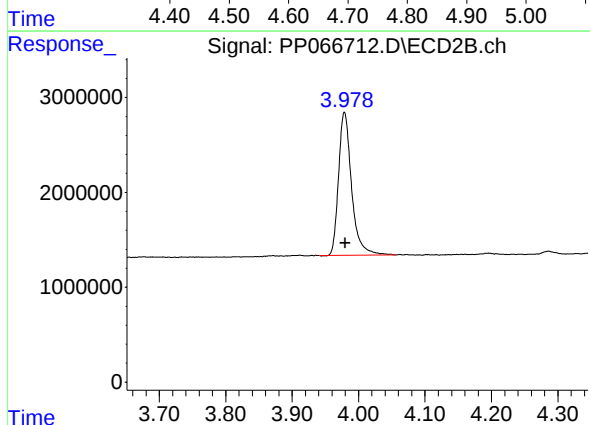


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.001 min
Response: 20429368
Conc: 15.62 ng/ml

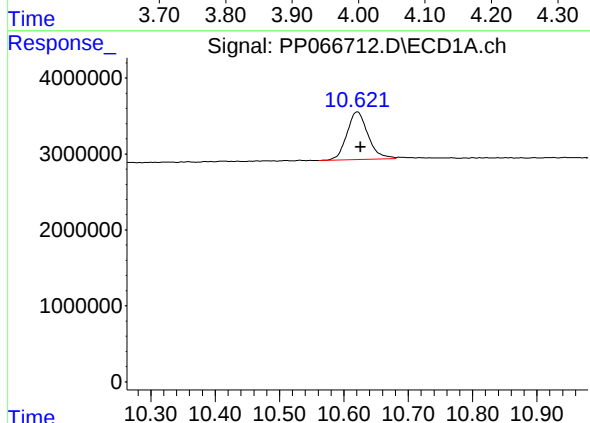


#2 Decachlorobiphenyl

R.T.: 10.621 min
Delta R.T.: -0.005 min
Response: 14238685
Conc: 16.23 ng/ml

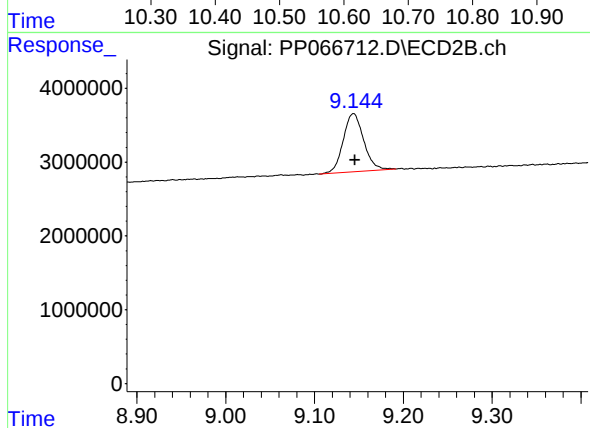

#2 Decachlorobiphenyl


R.T.: 9.144 min
Delta R.T.: -0.002 min
Response: 12640764
Conc: 15.17 ng/ml

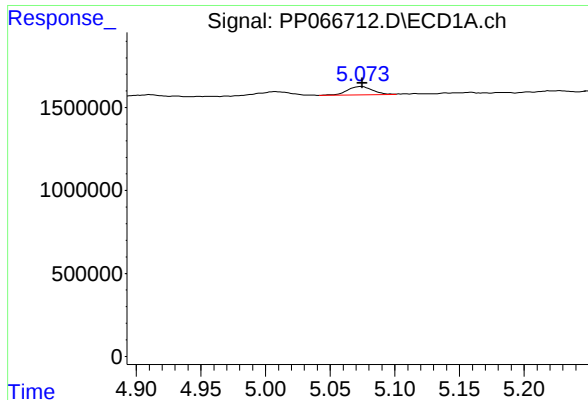

#11 AR-1232-1


R.T.: 5.074 min
Delta R.T.: 0.000 min
Response: 700937
Conc: 22.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

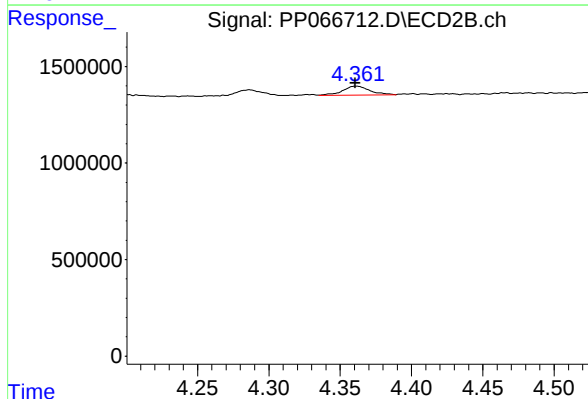


#11 AR-1232-1

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 596863
Conc: 19.48 ng/ml

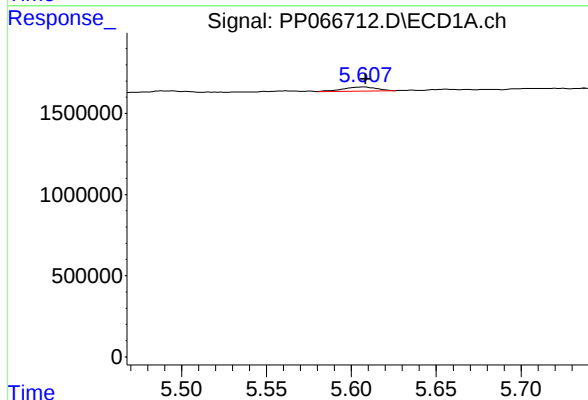


#12 AR-1232-2

R.T.: 5.607 min
Delta R.T.: -0.001 min
Response: 370946
Conc: 21.42 ng/ml

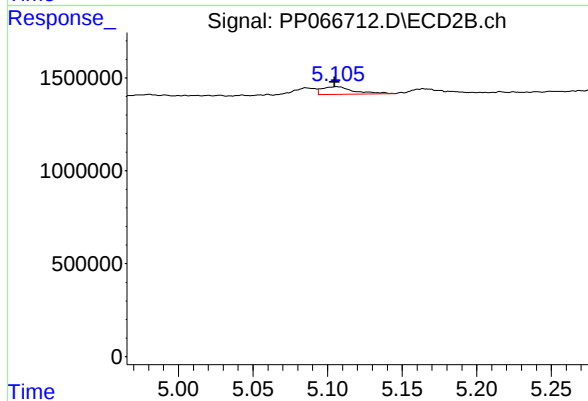

#12 AR-1232-2


R.T.: 5.106 min
Delta R.T.: 0.001 min
Response: 602705
Conc: 22.34 ng/ml

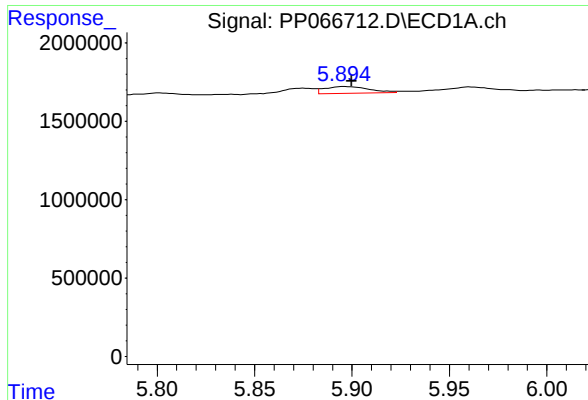

#13 AR-1232-3


R.T.: 5.896 min
Delta R.T.: -0.004 min
Response: 694011
Conc: 22.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

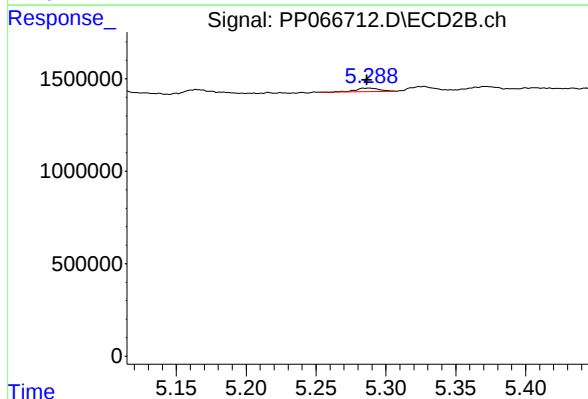


#13 AR-1232-3

R.T.: 5.287 min
Delta R.T.: 0.001 min
Response: 232329
Conc: 17.32 ng/ml

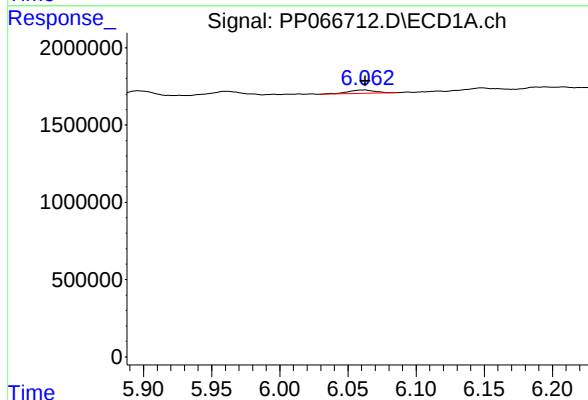


#14 AR-1232-4

R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 309938
Conc: 21.04 ng/ml

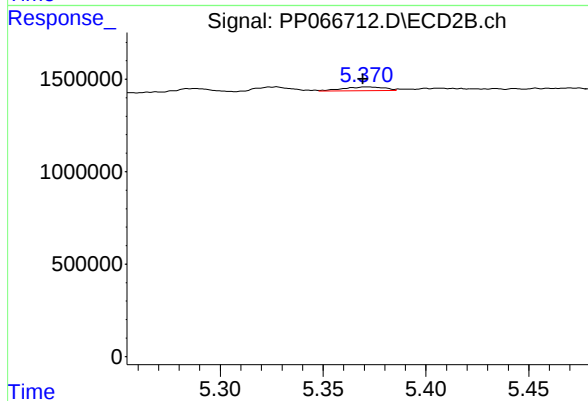

#14 AR-1232-4


R.T.: 5.371 min
Delta R.T.: 0.002 min
Response: 287750
Conc: 22.39 ng/ml

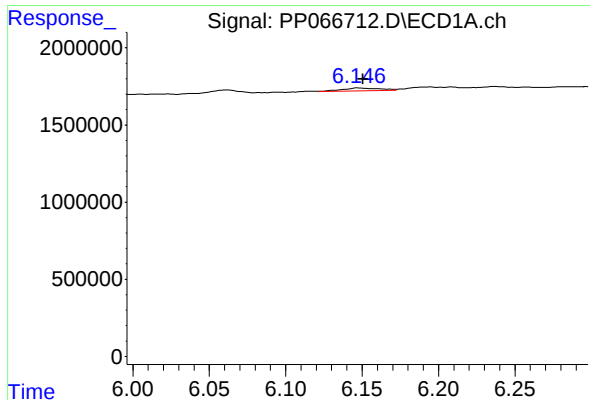

#15 AR-1232-5

R.T.: 6.148 min
Delta R.T.: -0.003 min
Response: 332445
Conc: 28.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

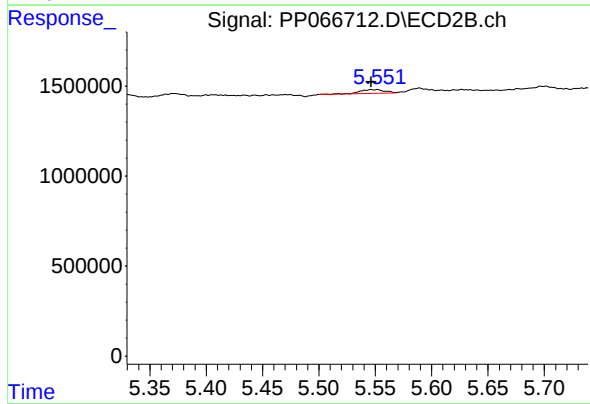

#15 AR-1232-5

R.T.: 5.552 min
Delta R.T.: 0.005 min
Response: 325846
Conc: 23.53 ng/ml