

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
 Data File : PP066731.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2024 06:42
 Operator : YP\AJ
 Sample : P3390-07
 Misc : AR1221 LOD 40 PPB
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 08:35:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 21 05:19:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.701	3.978	23455626	18356766	15.840	14.039
2) SA Decachlor...	10.621	9.143	13959167	11531212	15.907	13.842
Target Compounds						
8) L2 AR-1221-1	4.911	4.195	638064	398941	37.704	26.296 #
9) L2 AR-1221-2	5.005	4.285	641535	549076	51.736	46.783
10) L2 AR-1221-3	5.074	4.361	1329156	1019356	35.025	27.971



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
Data File : PP066731.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2024 06:42
Operator : YP\AJ
Sample : P3390-07
Misc : AR1221 LOD 40 PPB
ALS Vial : 63 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 08:35:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 21 05:19:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

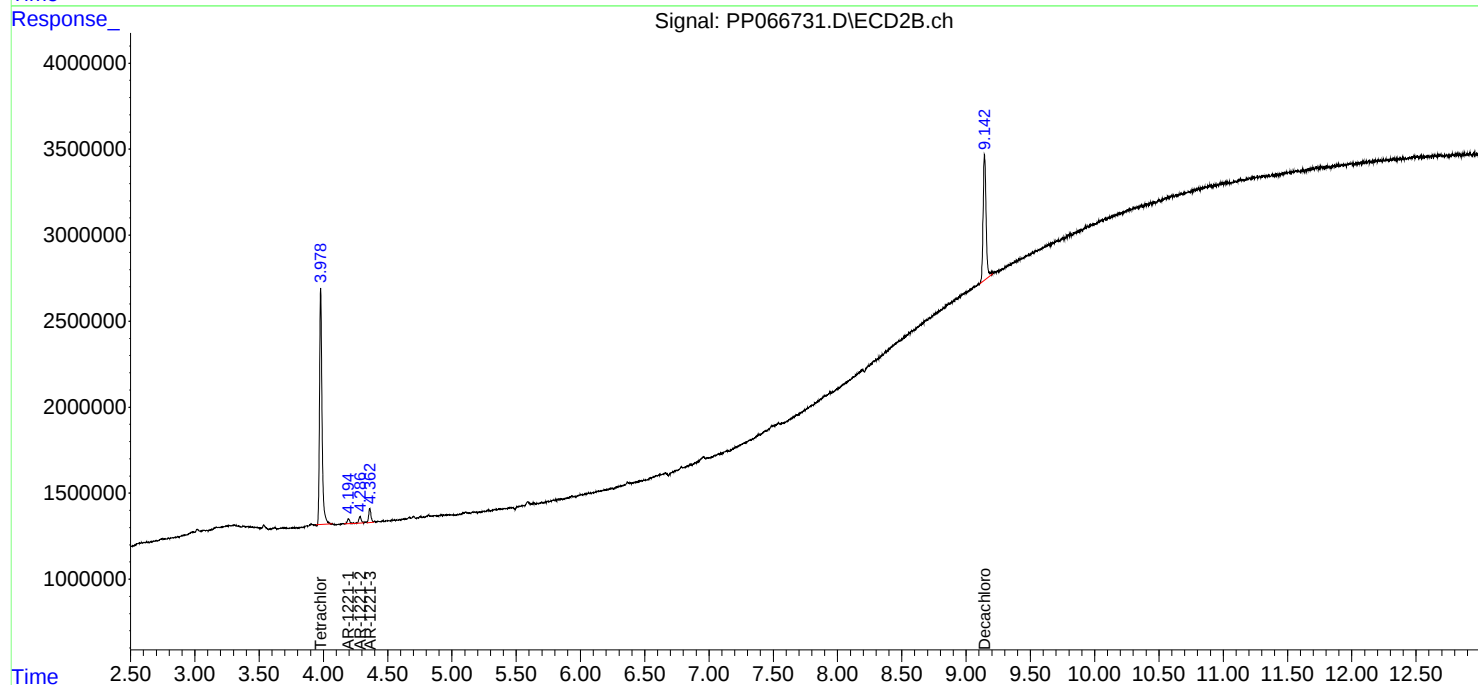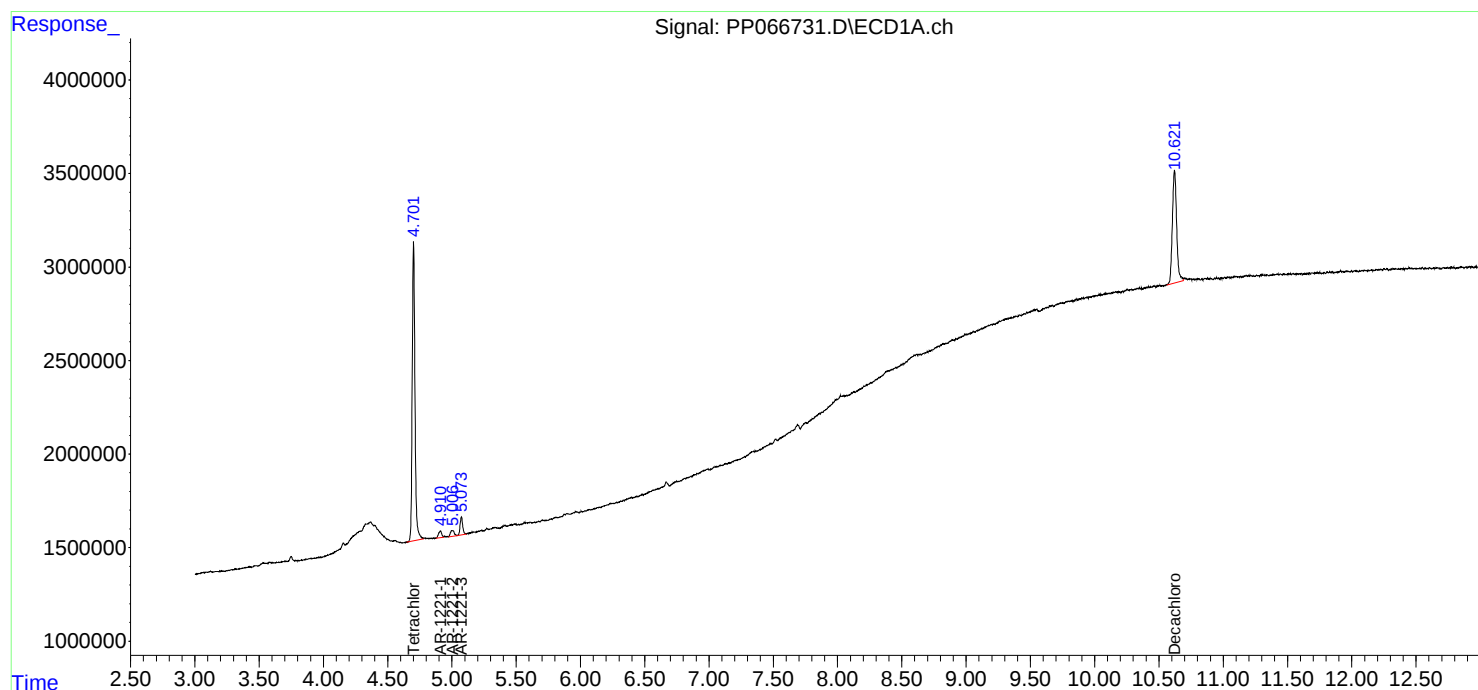


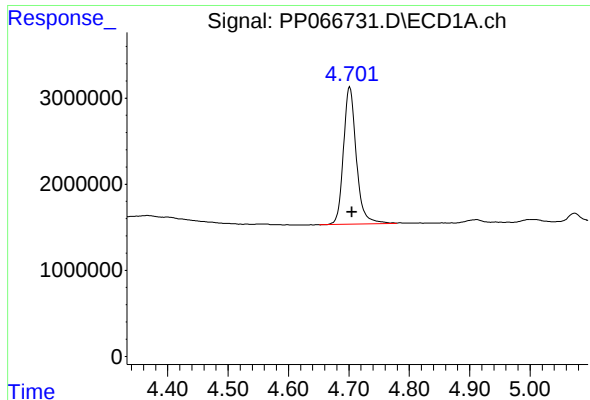

#1 Tetrachloro-m-xylene


R.T.: 4.701 min
Delta R.T.: -0.004 min
Response: 23455626
Conc: 15.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

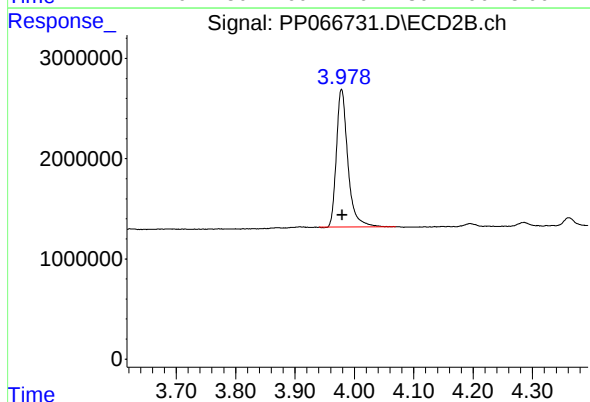


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.002 min
Response: 18356766
Conc: 14.04 ng/ml

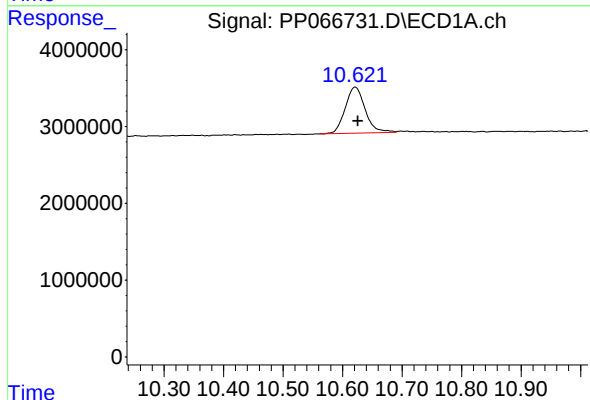


#2 Decachlorobiphenyl

R.T.: 10.621 min
Delta R.T.: -0.005 min
Response: 13959167
Conc: 15.91 ng/ml

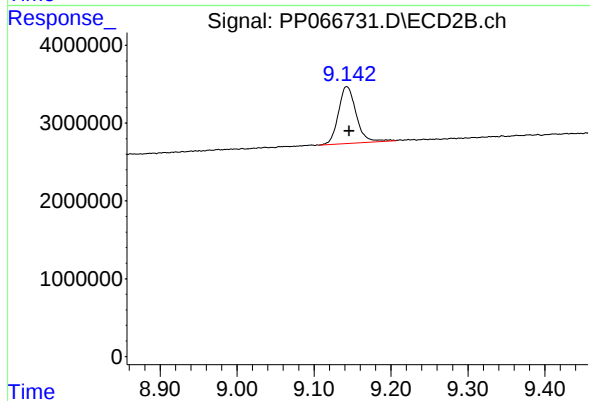

#2 Decachlorobiphenyl


R.T.: 9.143 min
Delta R.T.: -0.003 min
Response: 11531212
Conc: 13.84 ng/ml

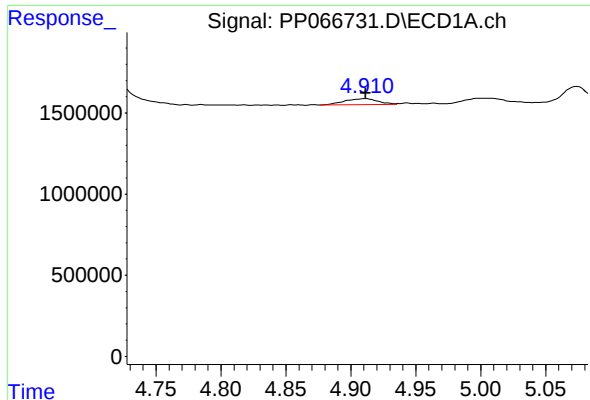

#8 AR-1221-1


R.T.: 4.911 min
Delta R.T.: 0.000 min
Response: 638064
Conc: 37.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

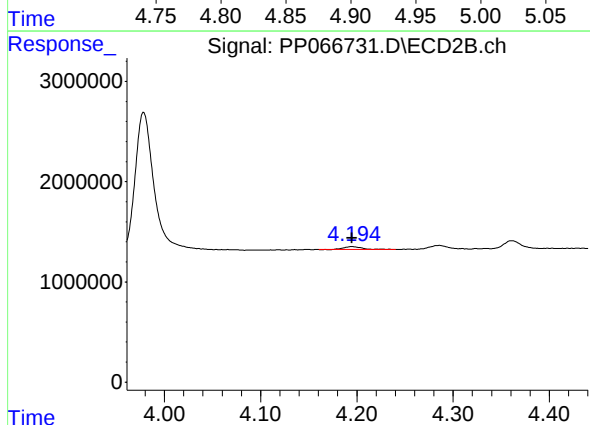


#8 AR-1221-1

R.T.: 4.195 min
Delta R.T.: 0.000 min
Response: 398941
Conc: 26.30 ng/ml

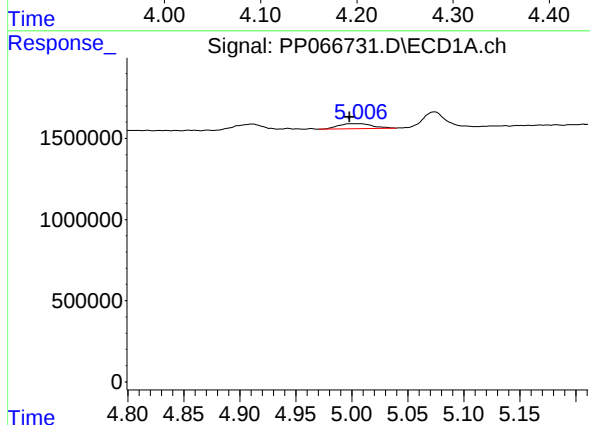


#9 AR-1221-2

R.T.: 5.005 min
Delta R.T.: 0.007 min
Response: 641535
Conc: 51.74 ng/ml

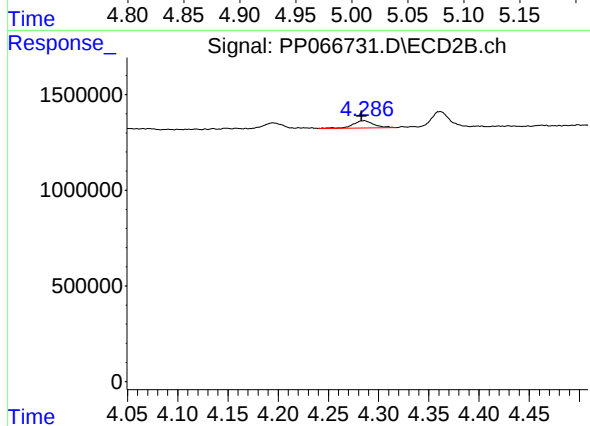

#9 AR-1221-2


R.T.: 4.285 min
Delta R.T.: 0.002 min
Response: 549076
Conc: 46.78 ng/ml

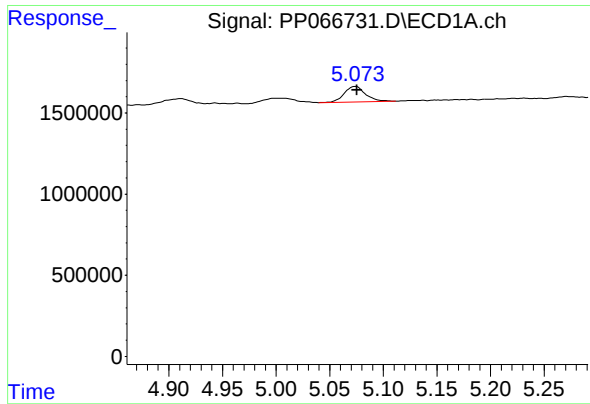

#10 AR-1221-3

R.T.: 5.074 min
Delta R.T.: -0.001 min
Response: 1329156
Conc: 35.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

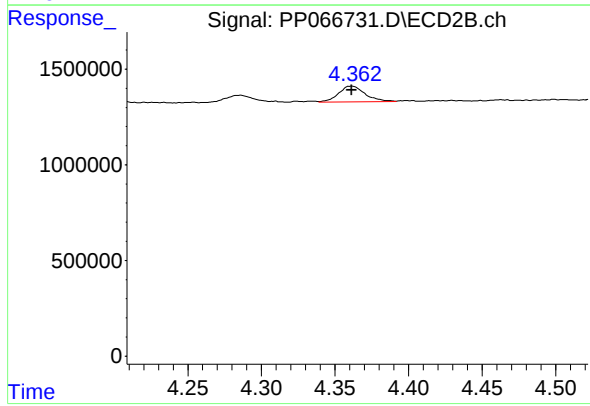

#10 AR-1221-3

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 1019356
Conc: 27.97 ng/ml