

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
 Data File : PP066734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2024 07:33
 Operator : YP\AJ
 Sample : P3390-07
 Misc : AR1248 LOD 40 PPB
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 08:36:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 21 05:19:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.702	3.979	22545952	17867846	15.226	13.666
2) SA Decachlor...	10.619	9.143	13405097	10786532	15.276	12.948
Target Compounds						
21) L5 AR-1248-1	5.876	5.086	890449	762380	34.840	31.488
22) L5 AR-1248-2	6.148	5.326	1414291	1108893	35.198	30.703
23) L5 AR-1248-3	6.355	5.370	1506196	1135488	34.544	30.414
24) L5 AR-1248-4	6.759	5.547	1485740	1255090	33.632	28.445
25) L5 AR-1248-5	6.799	5.947	1556828	1101900	33.960	29.170



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082024\
Data File : PP066734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2024 07:33
Operator : YP\AJ
Sample : P3390-07
Misc : AR1248 LOD 40 PPB
ALS Vial : 66 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 08:36:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 21 05:19:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

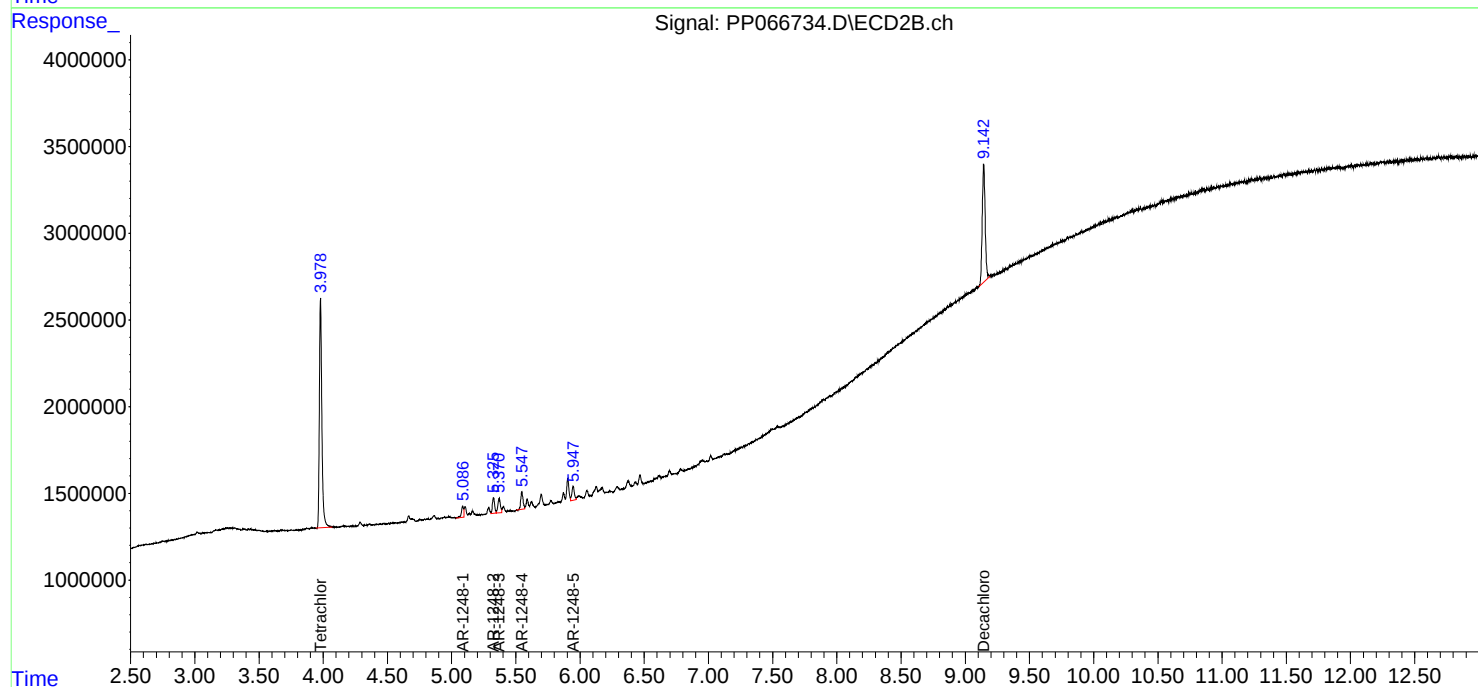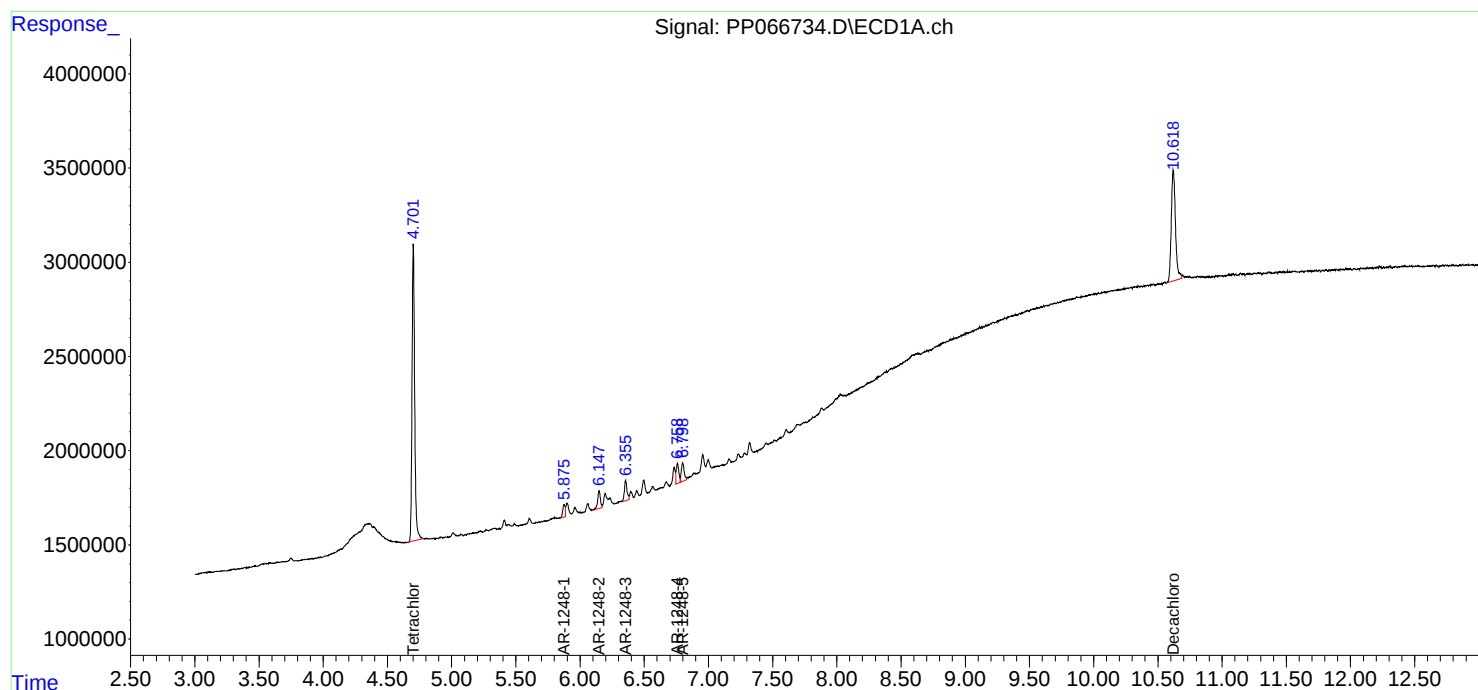


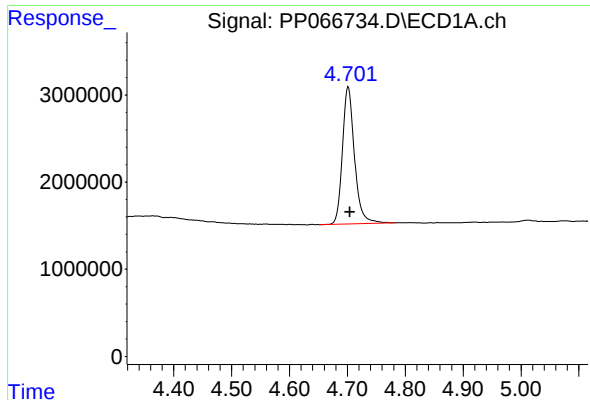

#1 Tetrachloro-m-xylene


R.T.: 4.702 min
Delta R.T.: -0.003 min
Response: 22545952
Conc: 15.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

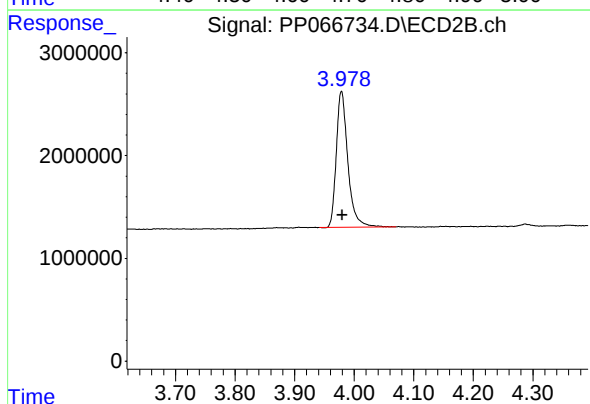


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.001 min
Response: 17867846
Conc: 13.67 ng/ml

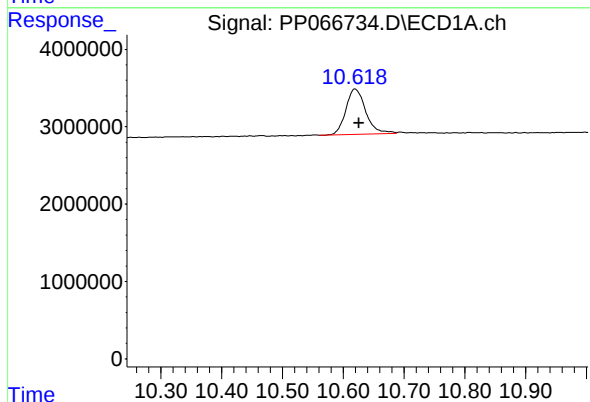


#2 Decachlorobiphenyl

R.T.: 10.619 min
Delta R.T.: -0.007 min
Response: 13405097
Conc: 15.28 ng/ml

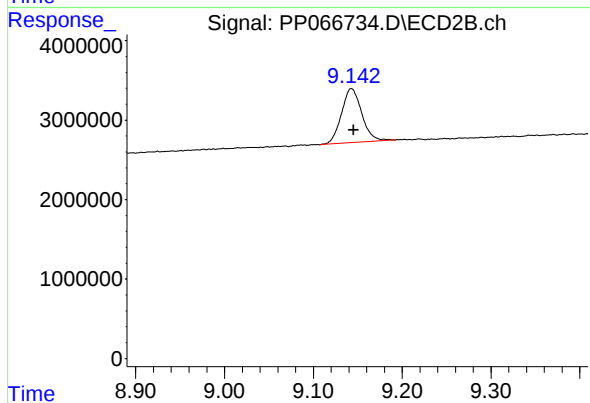

#2 Decachlorobiphenyl


R.T.: 9.143 min
Delta R.T.: -0.003 min
Response: 10786532
Conc: 12.95 ng/ml

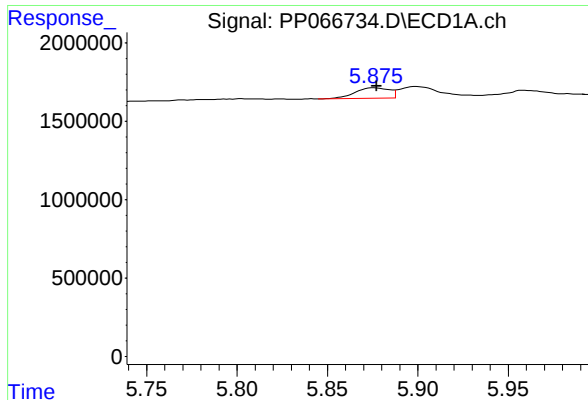

#21 AR-1248-1


R.T.: 5.876 min
Delta R.T.: -0.002 min
Response: 890449
Conc: 34.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

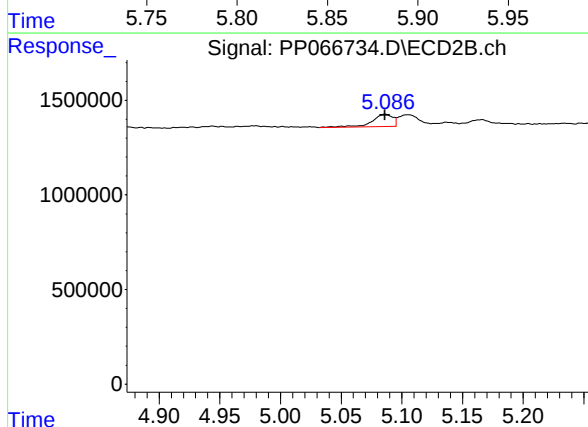


#21 AR-1248-1

R.T.: 5.086 min
Delta R.T.: 0.000 min
Response: 762380
Conc: 31.49 ng/ml

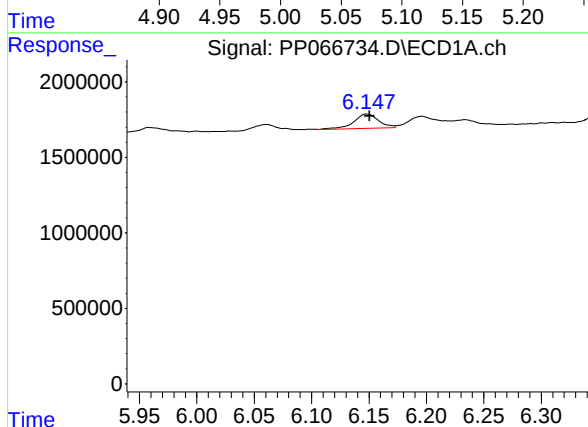


#22 AR-1248-2

R.T.: 6.148 min
Delta R.T.: -0.002 min
Response: 1414291
Conc: 35.20 ng/ml

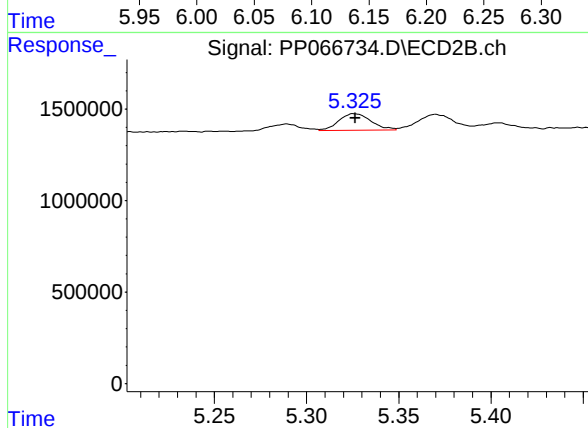

#22 AR-1248-2


R.T.: 5.326 min
Delta R.T.: 0.000 min
Response: 1108893
Conc: 30.70 ng/ml

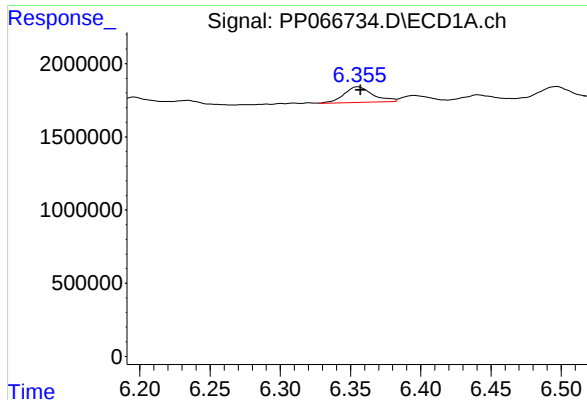

#23 AR-1248-3


R.T.: 6.355 min
Delta R.T.: -0.002 min
Response: 1506196
Conc: 34.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

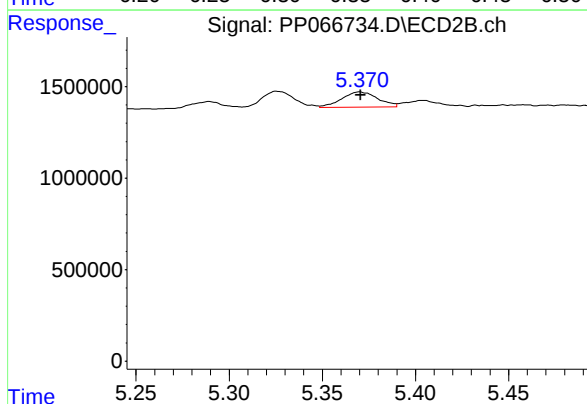


#23 AR-1248-3

R.T.: 5.370 min
Delta R.T.: 0.000 min
Response: 1135488
Conc: 30.41 ng/ml

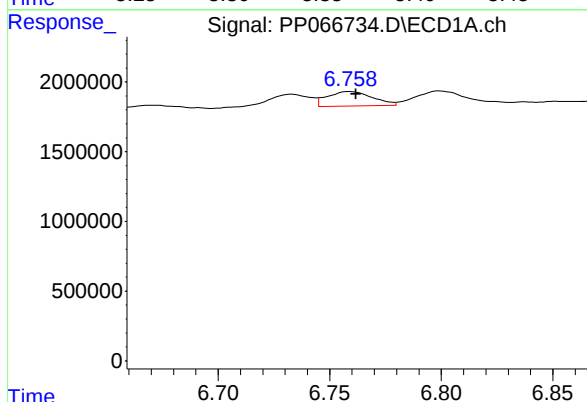


#24 AR-1248-4

R.T.: 6.759 min
Delta R.T.: -0.003 min
Response: 1485740
Conc: 33.63 ng/ml

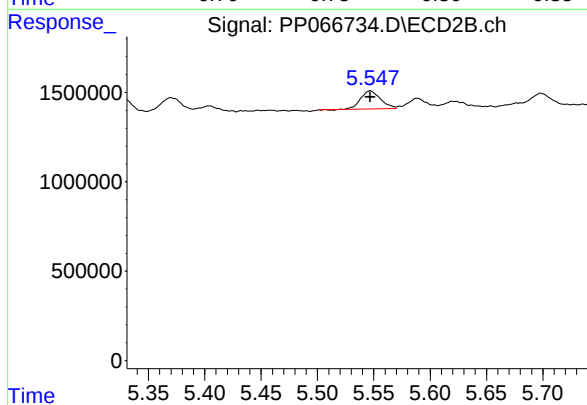

#24 AR-1248-4


R.T.: 5.547 min
Delta R.T.: 0.000 min
Response: 1255090
Conc: 28.45 ng/ml

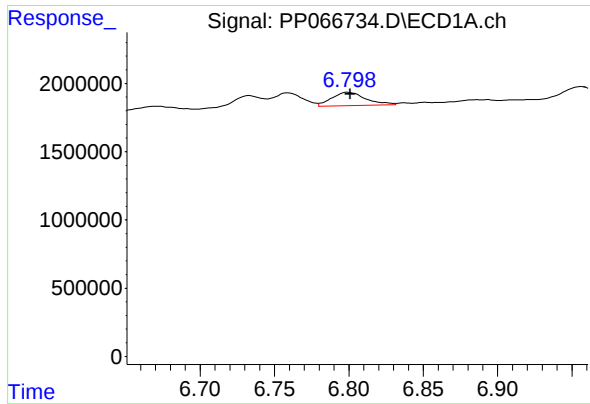

#25 AR-1248-5

R.T.: 6.799 min
Delta R.T.: -0.002 min
Response: 1556828
Conc: 33.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

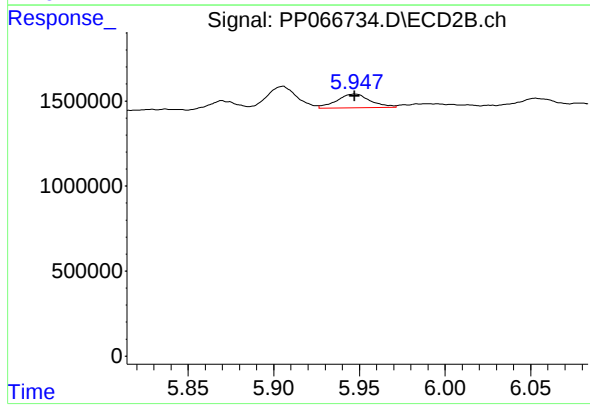

#25 AR-1248-5

R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 1101900
Conc: 29.17 ng/ml