

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082124\
 Data File : PP066767.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2024 17:19
 Operator : YP\AJ
 Sample : P3674-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB08724RB02

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/22/2024
 Supervised By :Ankita Jodhani 08/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 04:20:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 21 05:19:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.704	3.983	29010883	20943657	19.592m	16.018
2) SA Decachlor...	10.626	9.148	58245468	18438787	66.373	22.134m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082124\
Data File : PP066767.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2024 17:19
Operator : YP\AJ
Sample : P3674-02
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PCB08724RB02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/22/2024
Supervised By :Ankita Jodhani 08/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 04:20:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082024.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 21 05:19:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

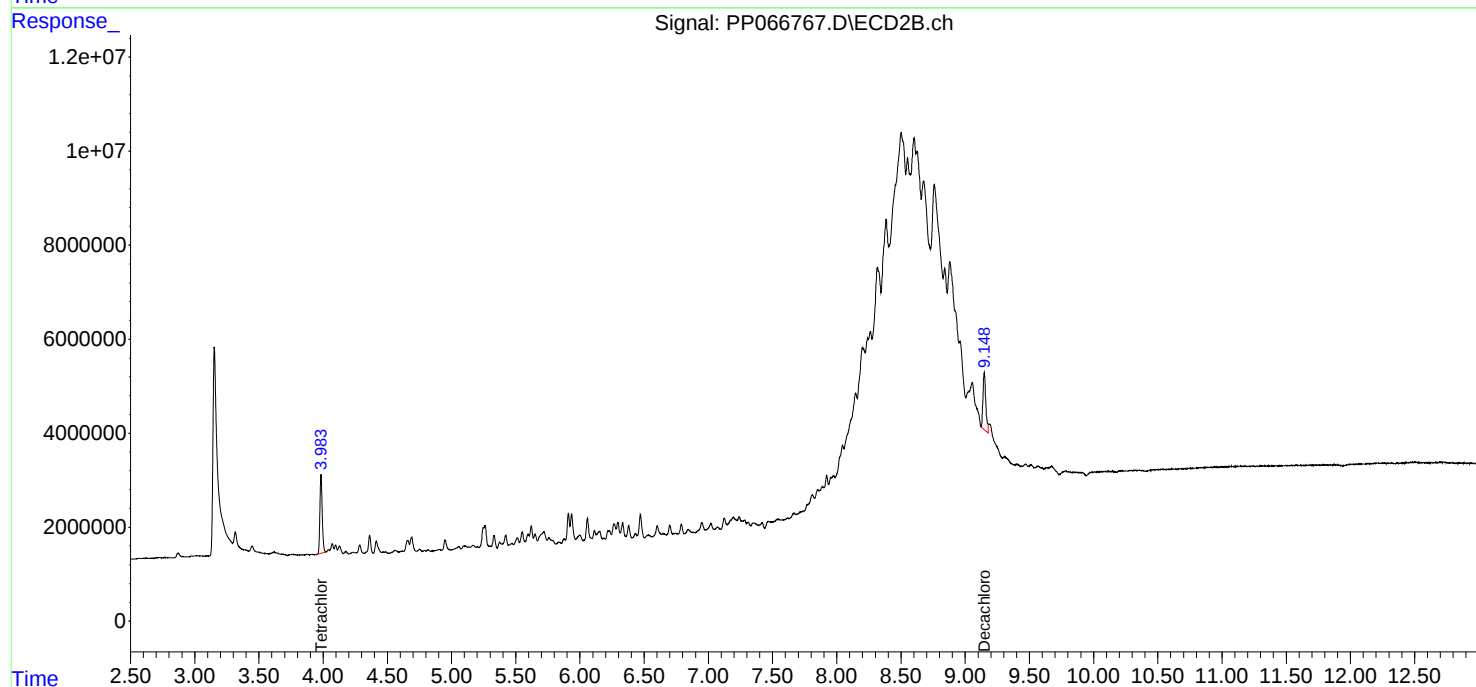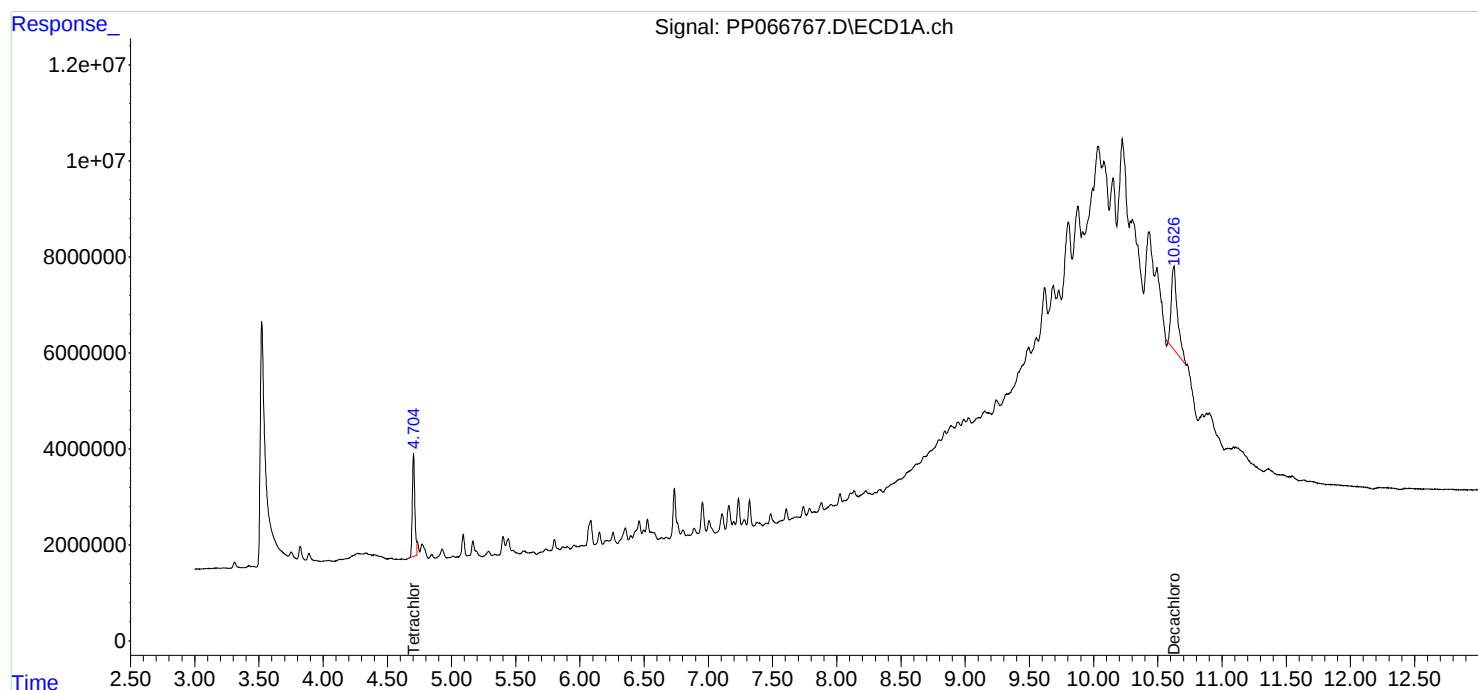

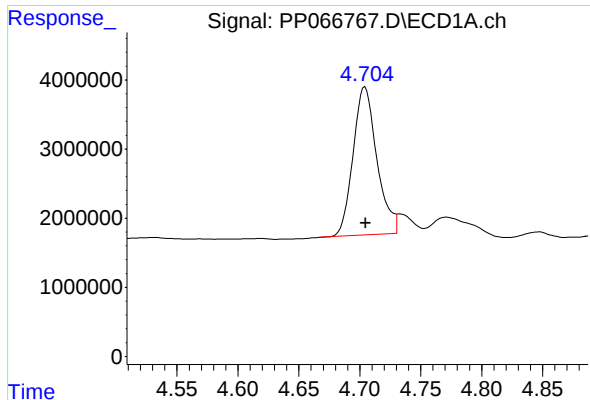


#1 Tetrachloro-m-xylene

R.T.: 4.704 min
Delta R.T.: -0.001 min
Response: 29010883
Conc: 19.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB08724RB02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/22/2024
Supervised By :Ankita Jodhani 08/22/2024

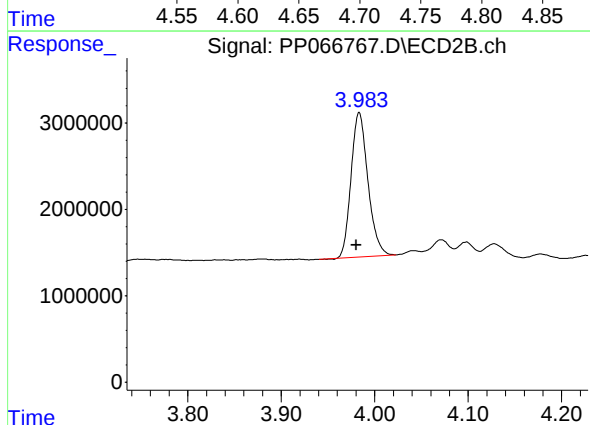


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.003 min
Response: 20943657
Conc: 16.02 ng/ml

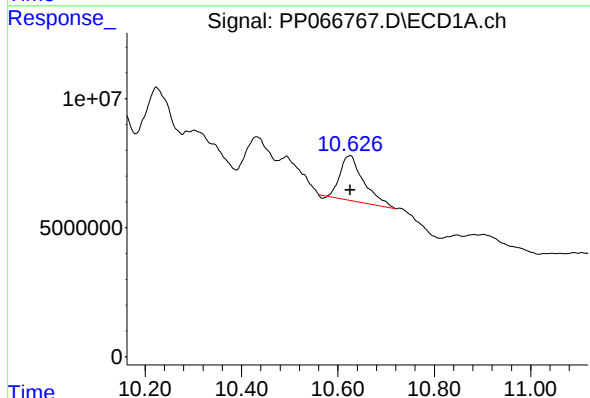

#2 Decachlorobiphenyl

R.T.: 10.626 min
Delta R.T.: 0.000 min
Response: 58245468
Conc: 66.37 ng/ml

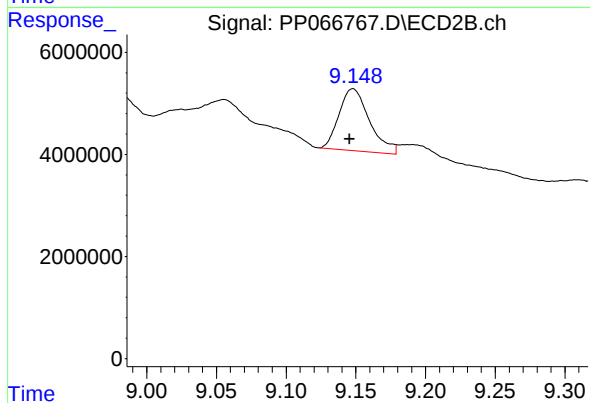

#2 Decachlorobiphenyl

R.T.: 9.148 min
Delta R.T.: 0.002 min
Response: 18438787
Conc: 22.13 ng/ml m