

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082125\
 Data File : PP074554.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2025 18:38
 Operator : YP\AJ
 Sample : Q2923-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 K262-DUP3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/22/2025
 Supervised By :mohammad ahmed 08/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 00:25:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.658	3.800	24308305	82780387	19.865	17.120
2) SA Decachlor...	10.456	8.819	52136713	158.7E6	52.796m	21.164m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082125\
Data File : PP074554.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2025 18:38
Operator : YP\AJ
Sample : Q2923-11
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
K262-DUP3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/22/2025
Supervised By :mohammad ahmed 08/25/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 00:25:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

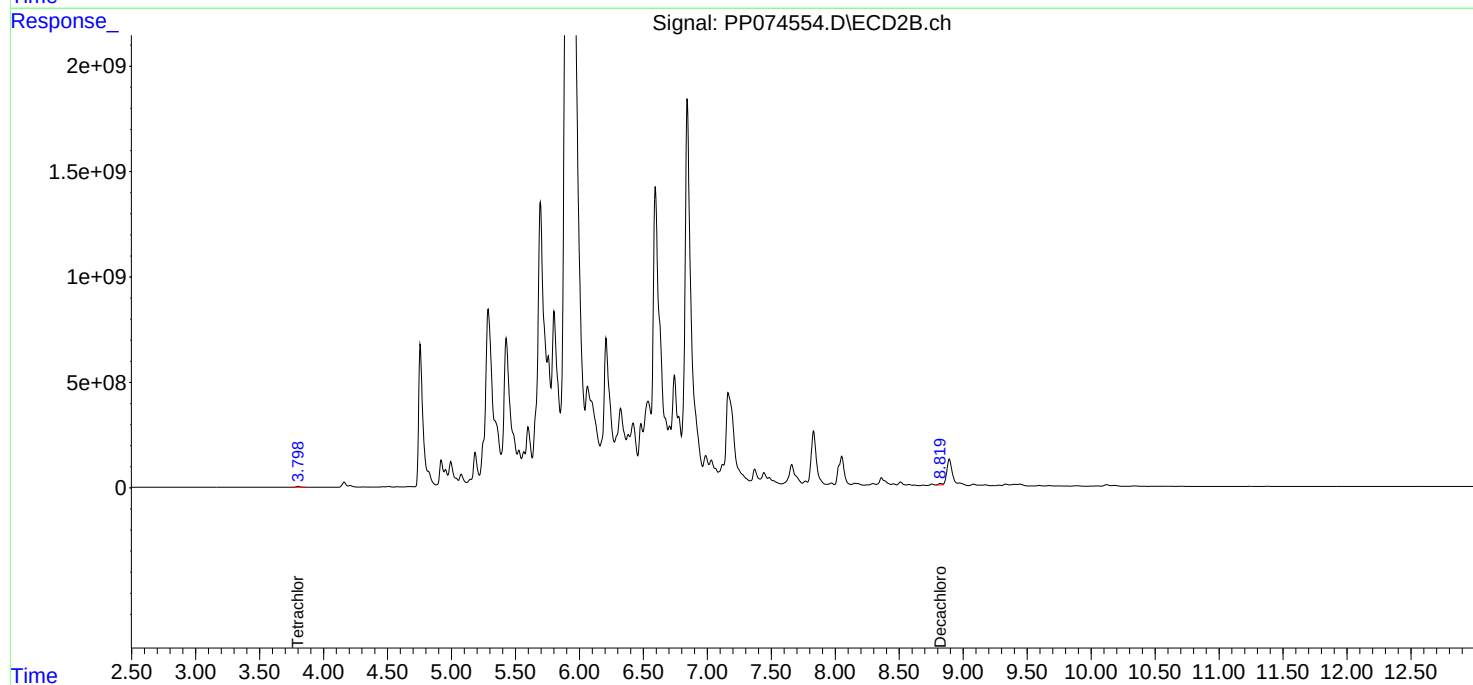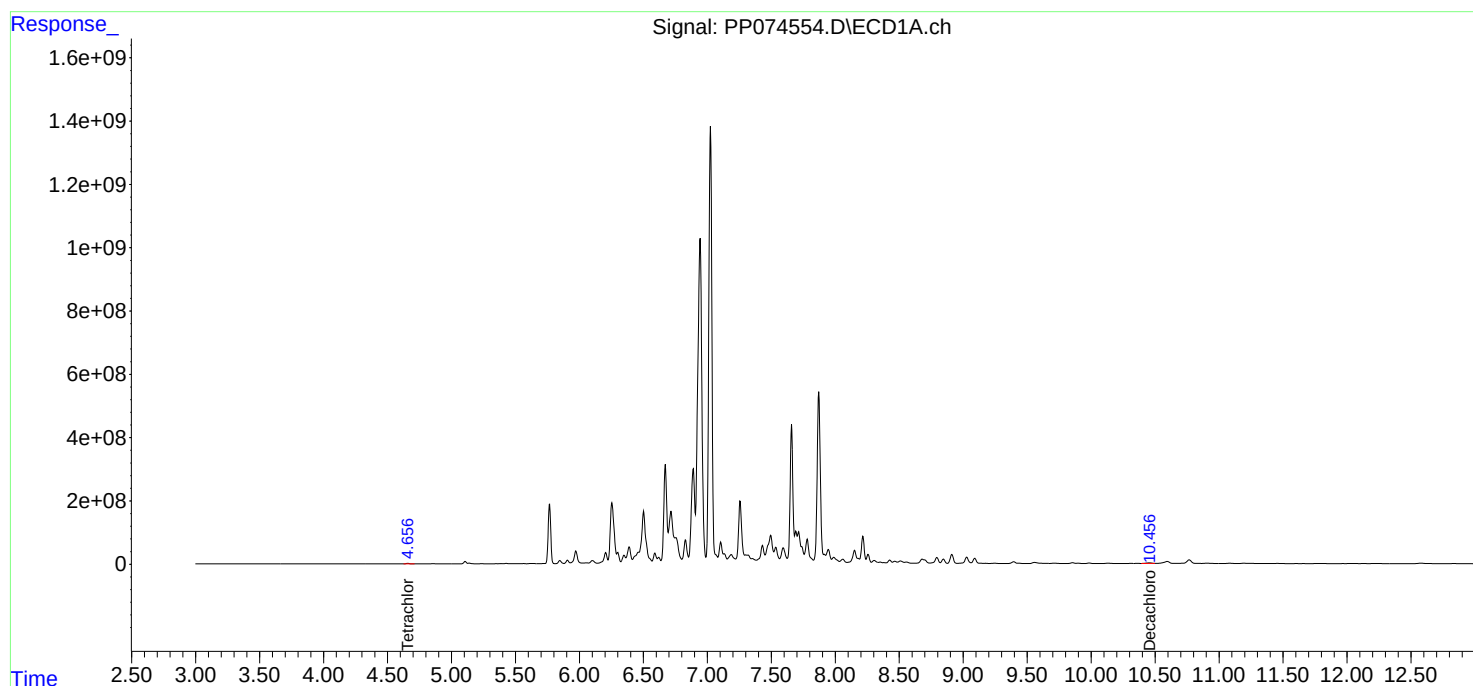

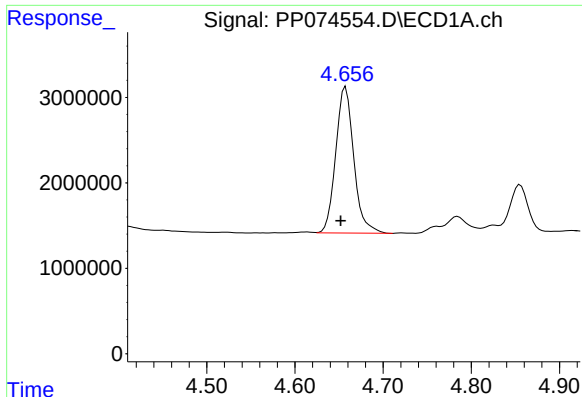


#1 Tetrachloro-m-xylene

R.T.: 4.658 min
Delta R.T.: 0.006 min
Response: 24308305
Conc: 19.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
K262-DUP3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/22/2025
Supervised By :mohammad ahmed 08/25/2025

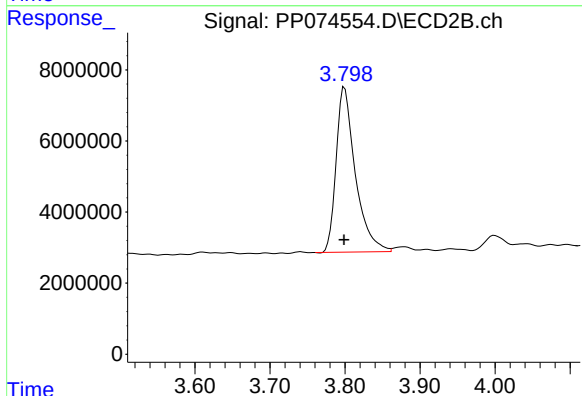


#1 Tetrachloro-m-xylene

R.T.: 3.800 min
Delta R.T.: 0.000 min
Response: 82780387
Conc: 17.12 ng/ml

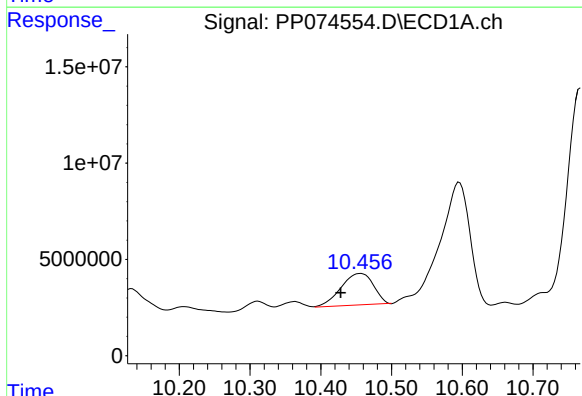

#2 Decachlorobiphenyl

R.T.: 10.456 min
Delta R.T.: 0.027 min
Response: 52136713
Conc: 52.80 ng/ml m

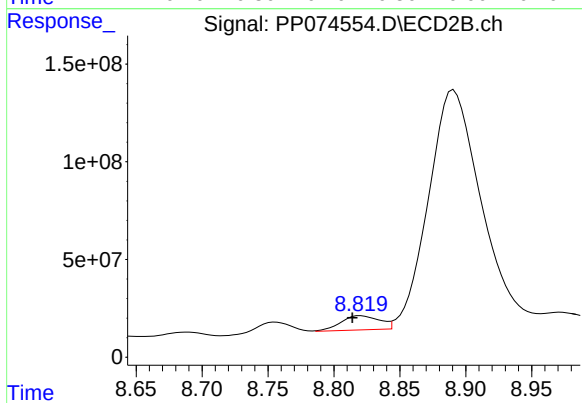

#2 Decachlorobiphenyl

R.T.: 8.819 min
Delta R.T.: 0.005 min
Response: 158715927
Conc: 21.16 ng/ml m