

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082225\
 Data File : PP074603.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2025 22:39
 Operator : YP\AJ
 Sample : Q2919-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 OK-02-08202025

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/25/2025
 Supervised By :mohammad ahmed 08/27/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 05:37:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.658	3.802	25318869	103.5E6	20.691m	21.414
2) SA Decachlor...	10.436	8.815	19595270	102.2E6	19.843	13.623 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082225\
Data File : PP074603.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2025 22:39
Operator : YP\AJ
Sample : Q2919-01
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
OK-02-08202025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/25/2025
Supervised By :mohammad ahmed 08/27/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 05:37:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

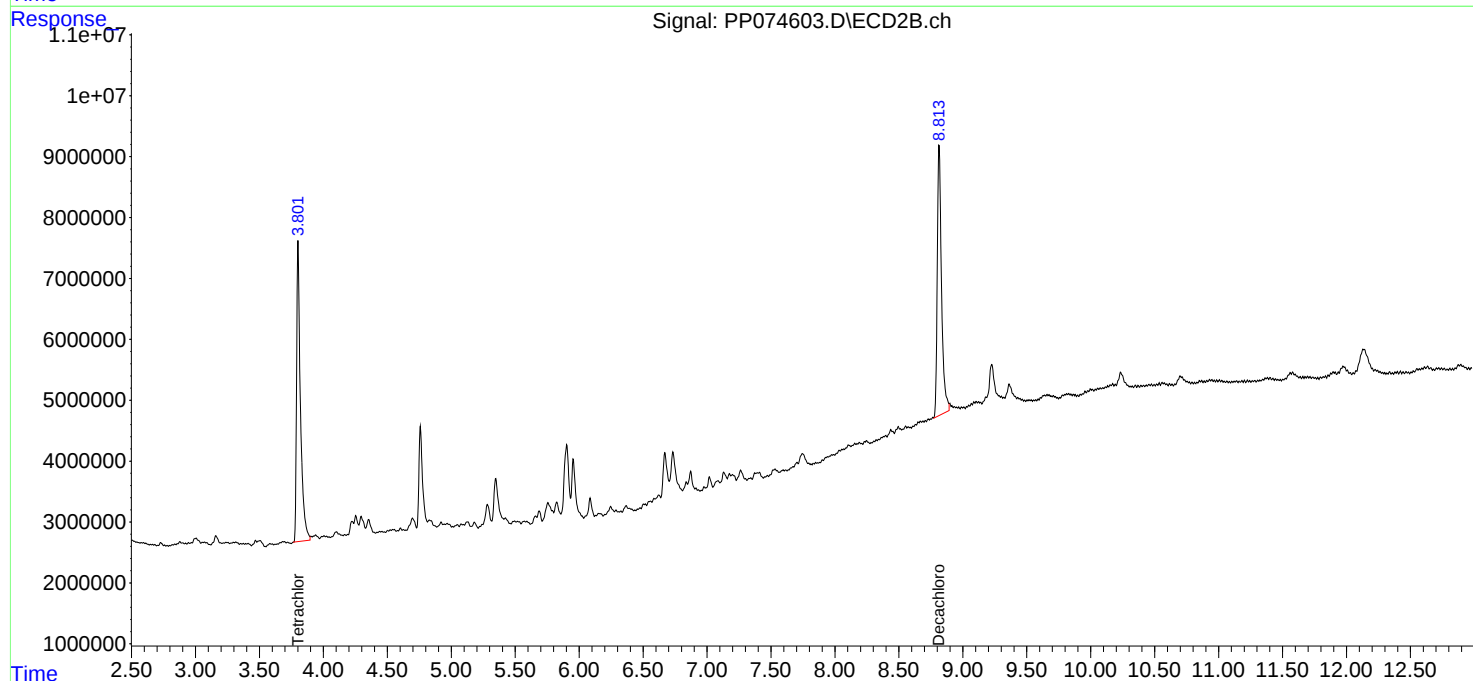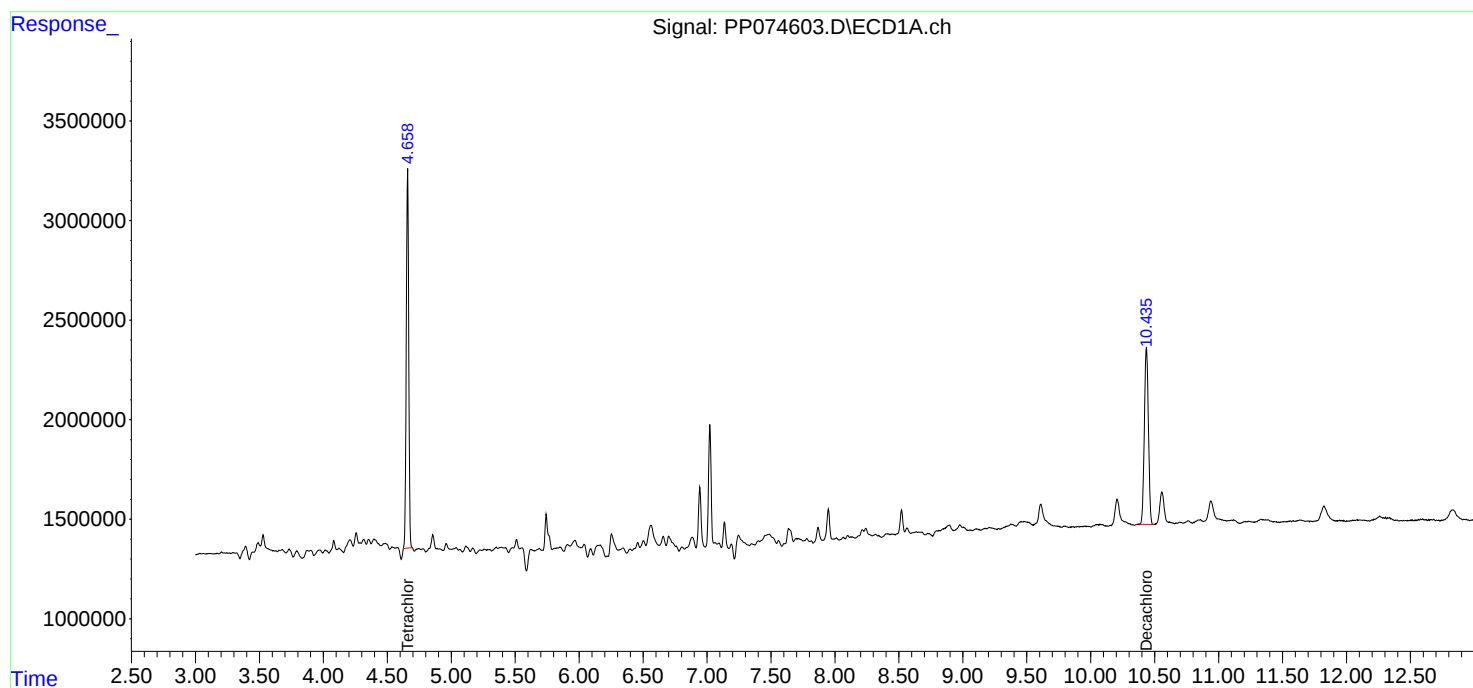

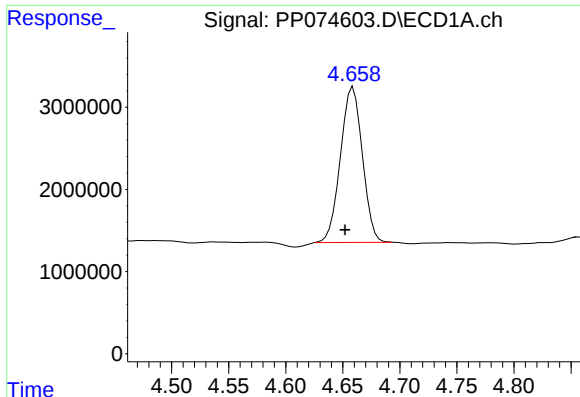


#1 Tetrachloro-m-xylene

R.T.: 4.658 min
Delta R.T.: 0.006 min
Response: 25318869
Conc: 20.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
OK-02-08202025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/25/2025
Supervised By :mohammad ahmed 08/27/2025

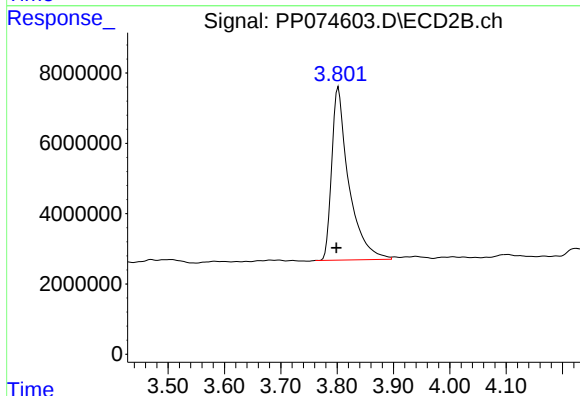


#1 Tetrachloro-m-xylene

R.T.: 3.802 min
Delta R.T.: 0.004 min
Response: 103545277
Conc: 21.41 ng/ml

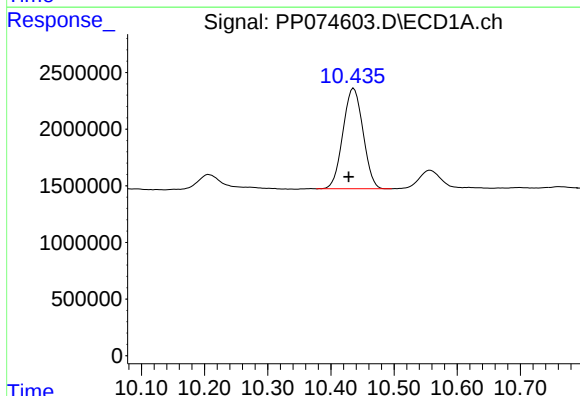

#2 Decachlorobiphenyl

R.T.: 10.436 min
Delta R.T.: 0.008 min
Response: 19595270
Conc: 19.84 ng/ml

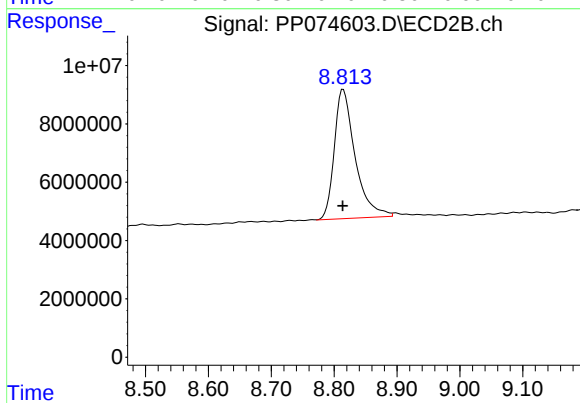

#2 Decachlorobiphenyl

R.T.: 8.815 min
Delta R.T.: 0.000 min
Response: 102158765
Conc: 13.62 ng/ml