

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD P\Data\PP082318\
Data File : PP027172.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Aug 2018 10:18
Operator : EI\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 12:10:48 2018
Quant Method : Z:\bestpcbsrv\HPCHEM1\ECD_P\methods\PP073018.M
Quant Title : 8080.M
QLast Update : Tue Jul 31 01:31:14 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.096	0.000	111.0E6	0	464.809	N.D. #
Target Compounds							
15) T	Picloram	17.603	0.000	11874718	0	2.875	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD P\Data\PP082318\
Data File : PP027172.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Aug 2018 10:18
Operator : EI\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 12:10:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP073018.M
Quant Title : 8080.M
QLast Update : Tue Jul 31 01:31:14 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

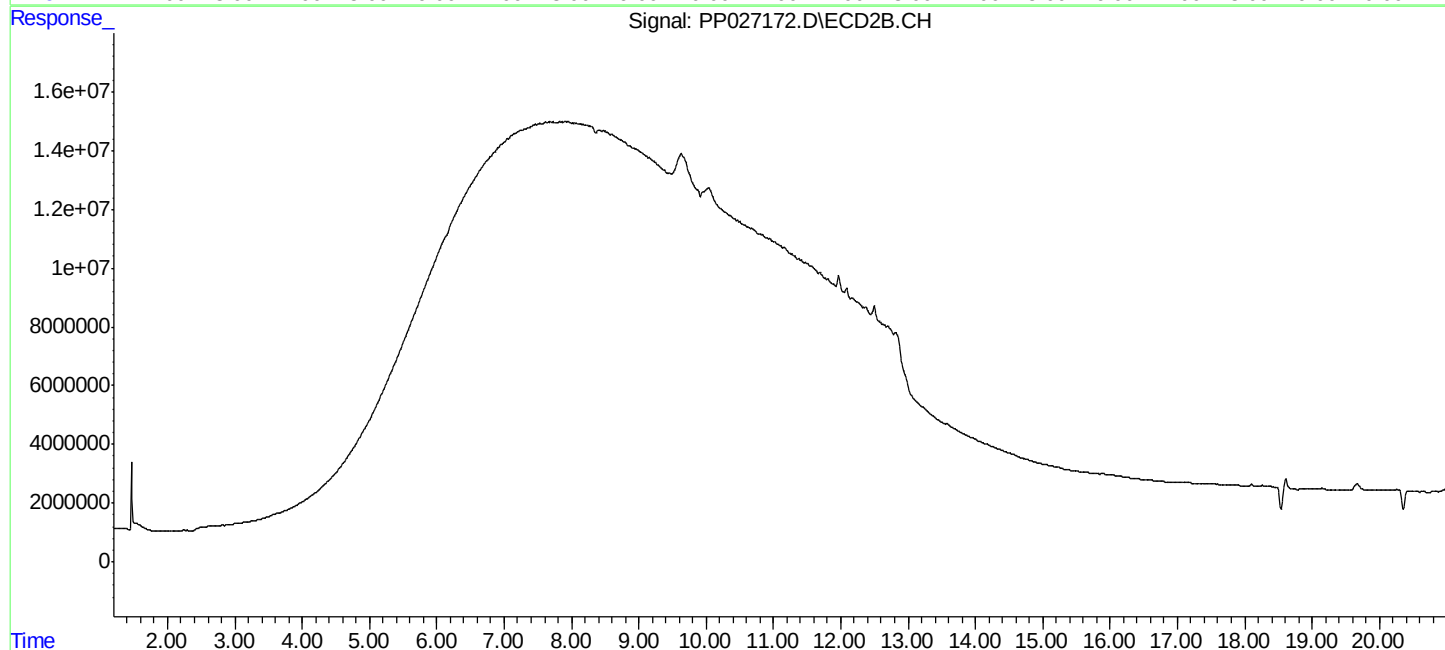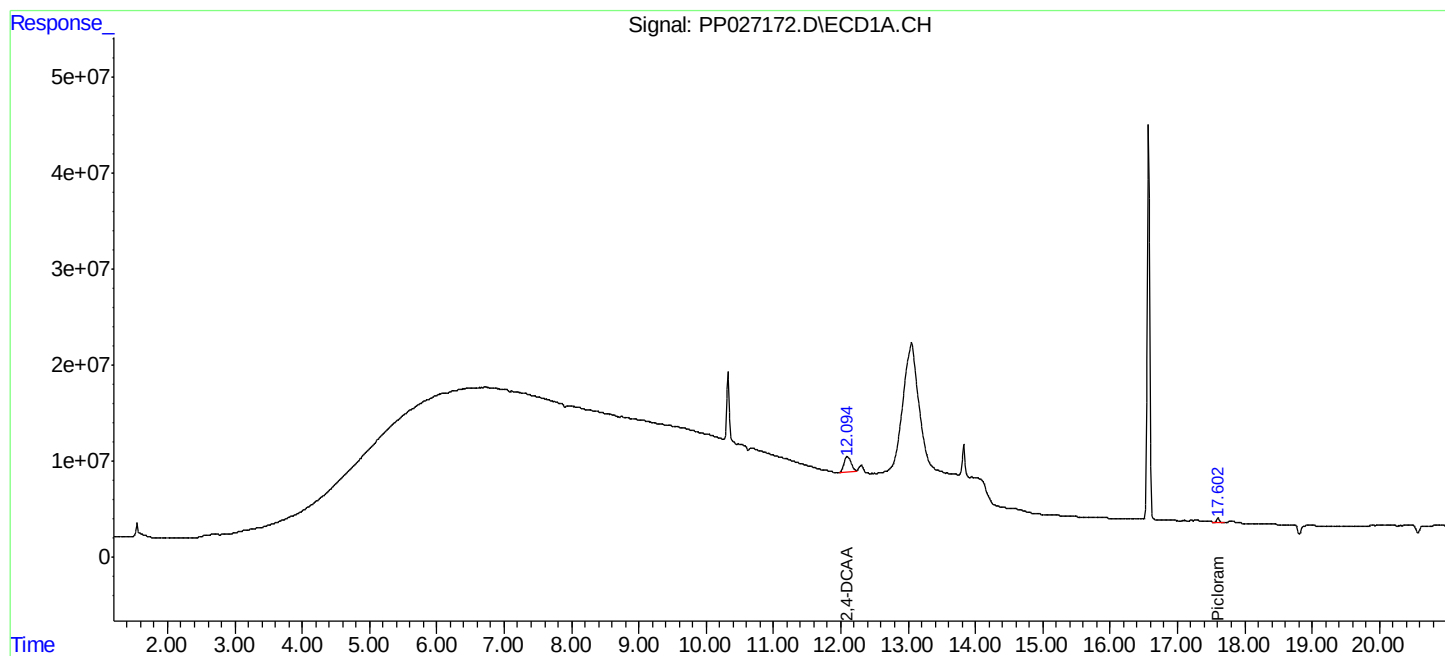


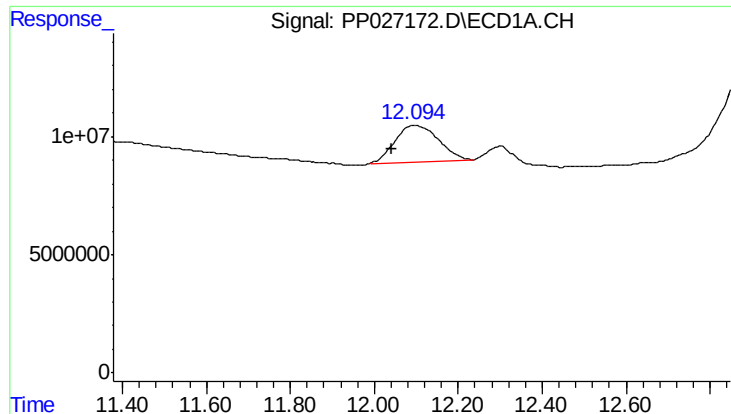

#4 2,4-DCAA


R.T.: 12.096 min
Delta R.T.: 0.053 min
Response: 111006916
Conc: 464.81 ng/ml

Instrument :
ECD_P
ClientSampleId :

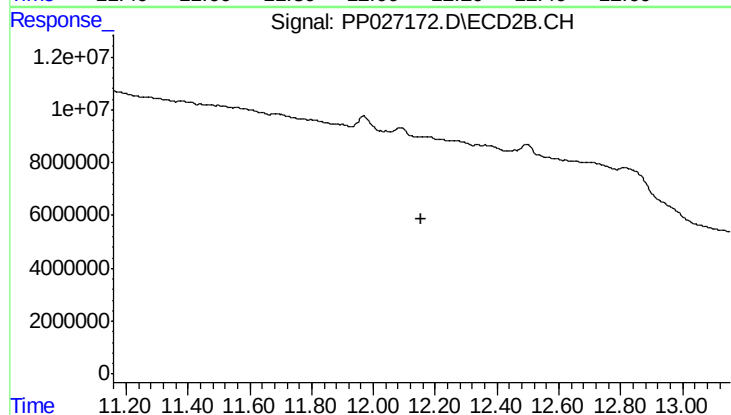


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 12.156 min
Response: 0
Conc: N.D.

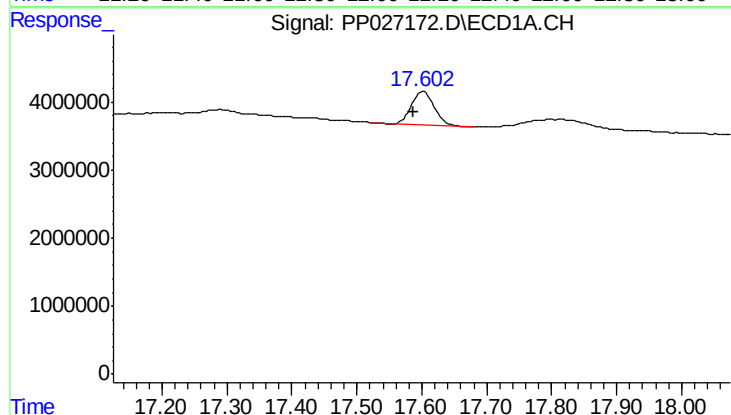

#15 Picloram

R.T.: 17.603 min
Delta R.T.: 0.016 min
Response: 11874718
Conc: 2.88 ng/ml

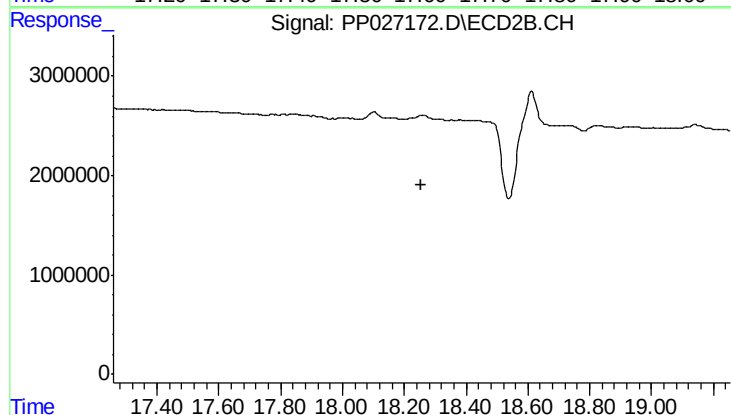

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 18.255 min
Response: 0
Conc: N.D.