

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082321\
 Data File : PP038786.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Aug 2021 16:45
 Operator : AJ\MA
 Sample : M3463-43
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 2021-08-17-FD-05

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 05:46:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 18 04:51:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.883	3.868	714397	456423	17.702	19.046
2) SA Decachlor...	10.870	9.128	324599	316022	13.193	12.975
Target Compounds						
8) L2 AR-1221-1	5.134	0.000	30184	0	64.543	N.D. #
30) L6 AR-1254-5	8.444	0.000	13479	0	10.898	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082321\
Data File : PP038786.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Aug 2021 16:45
Operator : AJ\MA
Sample : M3463-43
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
2021-08-17-FD-05

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 05:46:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 18 04:51:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

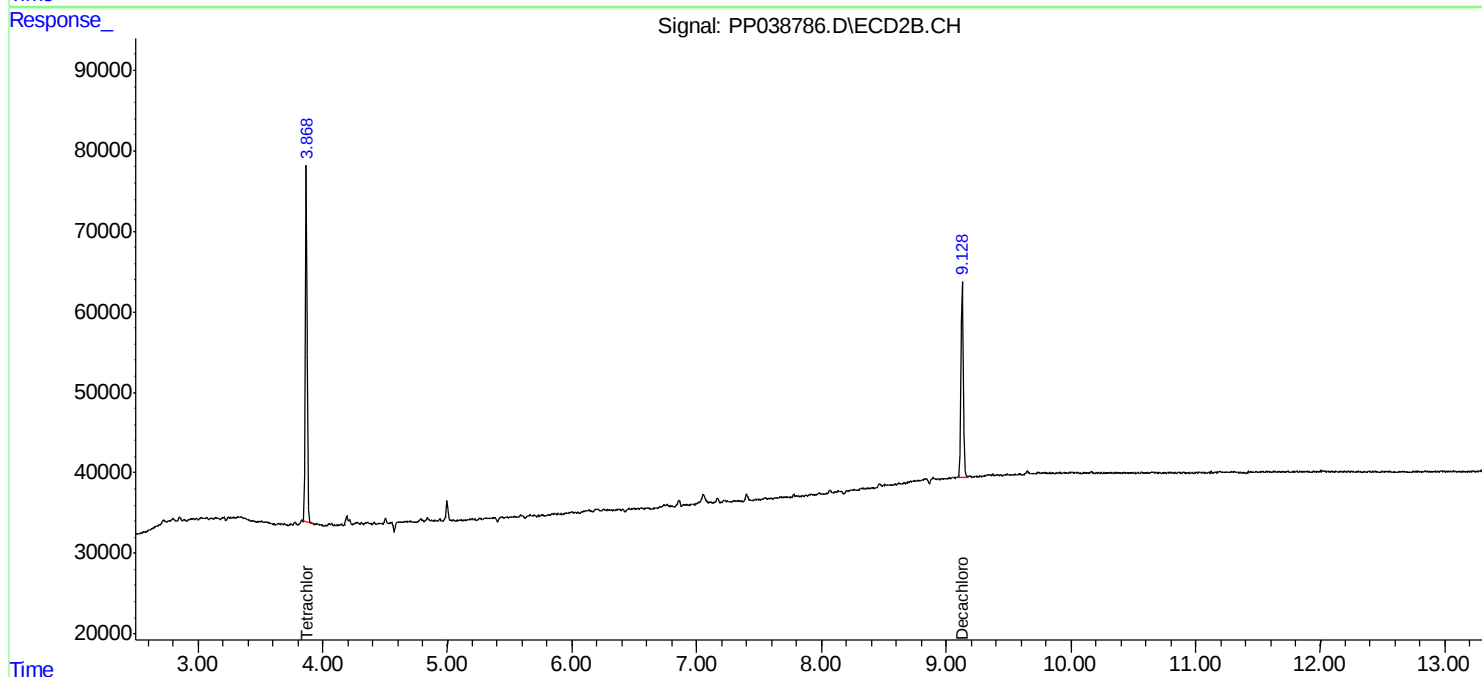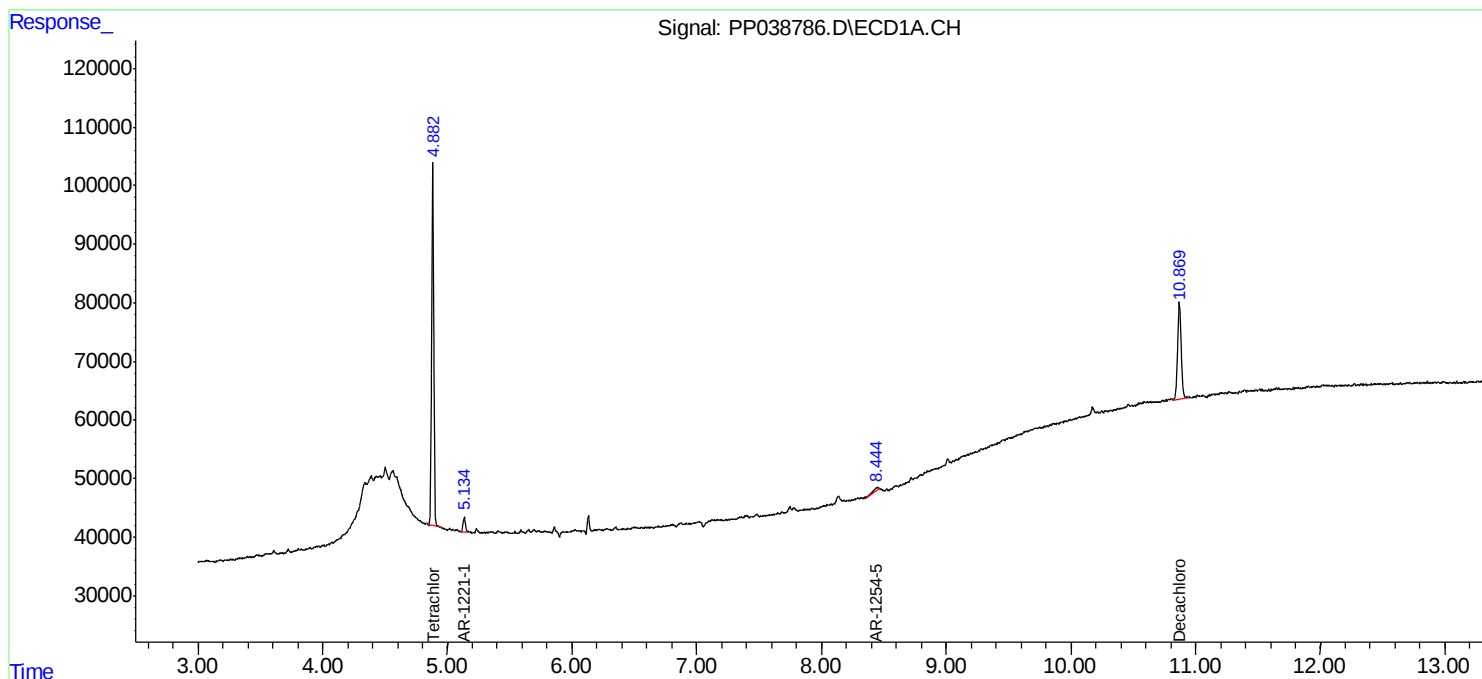


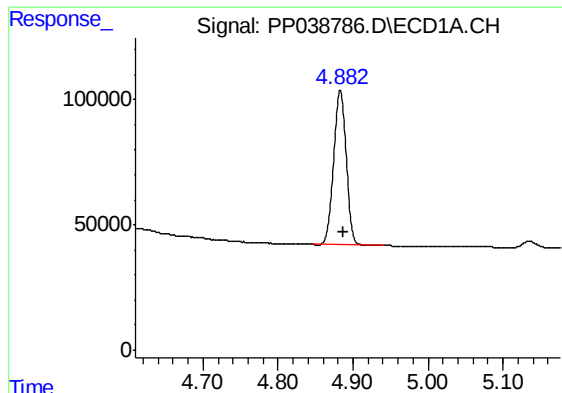

#1 Tetrachloro-m-xylene


R.T.: 4.883 min
Delta R.T.: -0.005 min
Response: 714397
Conc: 17.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
2021-08-17-FD-05

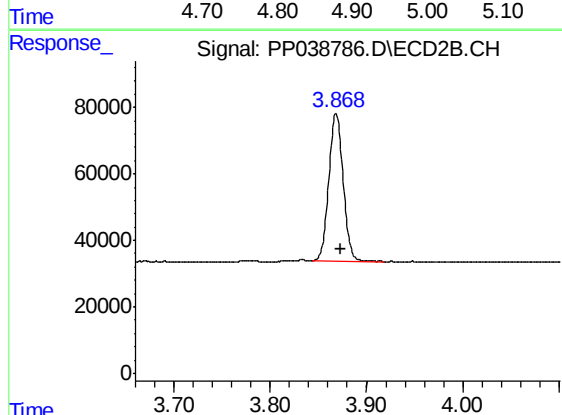


#1 Tetrachloro-m-xylene

R.T.: 3.868 min
Delta R.T.: -0.006 min
Response: 456423
Conc: 19.05 ng/ml

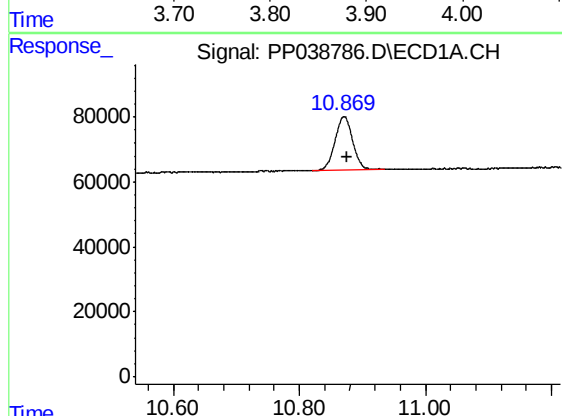


#2 Decachlorobiphenyl

R.T.: 10.870 min
Delta R.T.: -0.007 min
Response: 324599
Conc: 13.19 ng/ml

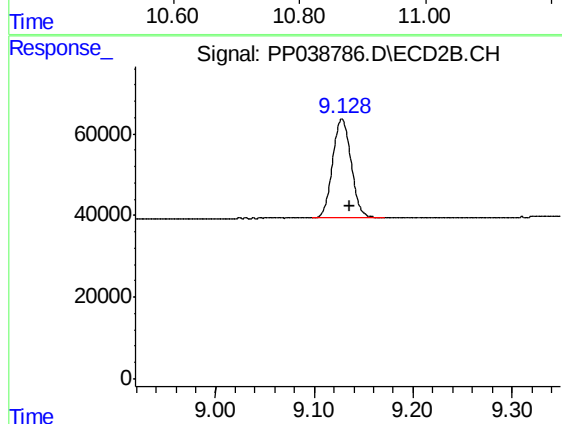

#2 Decachlorobiphenyl


R.T.: 9.128 min
Delta R.T.: -0.008 min
Response: 316022
Conc: 12.98 ng/ml

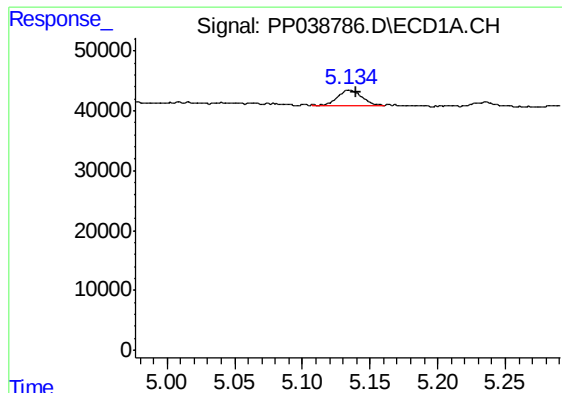

#8 AR-1221-1


R.T.: 5.134 min
Delta R.T.: -0.006 min
Response: 30184
Conc: 64.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
2021-08-17-FD-05

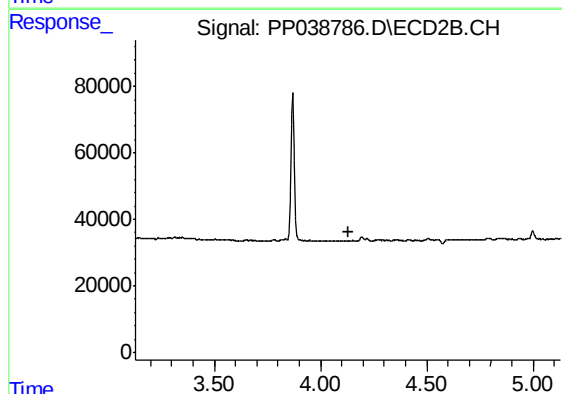


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.129 min
Response: 0
Conc: N.D.

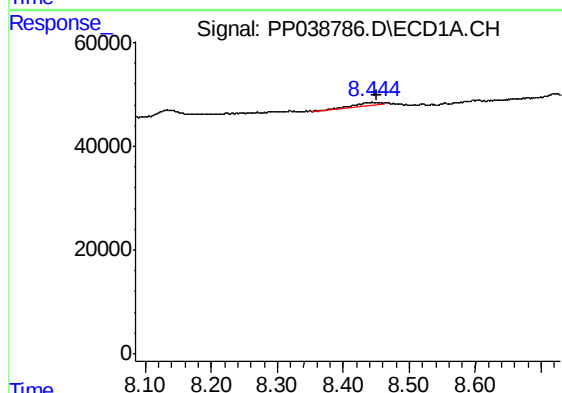

#30 AR-1254-5

R.T.: 8.444 min
Delta R.T.: -0.006 min
Response: 13479
Conc: 10.90 ng/ml

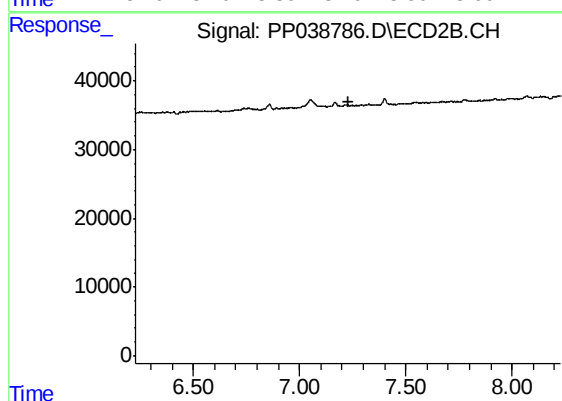

#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.228 min
Response: 0
Conc: N.D.