

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082321\
 Data File : PP038787.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Aug 2021 17:02
 Operator : AJ\MA
 Sample : M3489-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 1-BMENT-F

Manual Integrations
 APPROVED

mohammad
 8/24/2021 10:28:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 05:47:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 18 04:51:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.883	3.868	711672	437081	17.634	18.239m
2) SA Decachlor...	10.874	9.127	733460	677140	29.811	27.802m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082321\
Data File : PP038787.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Aug 2021 17:02
Operator : AJ\MA
Sample : M3489-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
1-BMENT-F


Manual Integrations
APPROVED

mohammad
8/24/2021 10:28:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 05:47:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 18 04:51:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

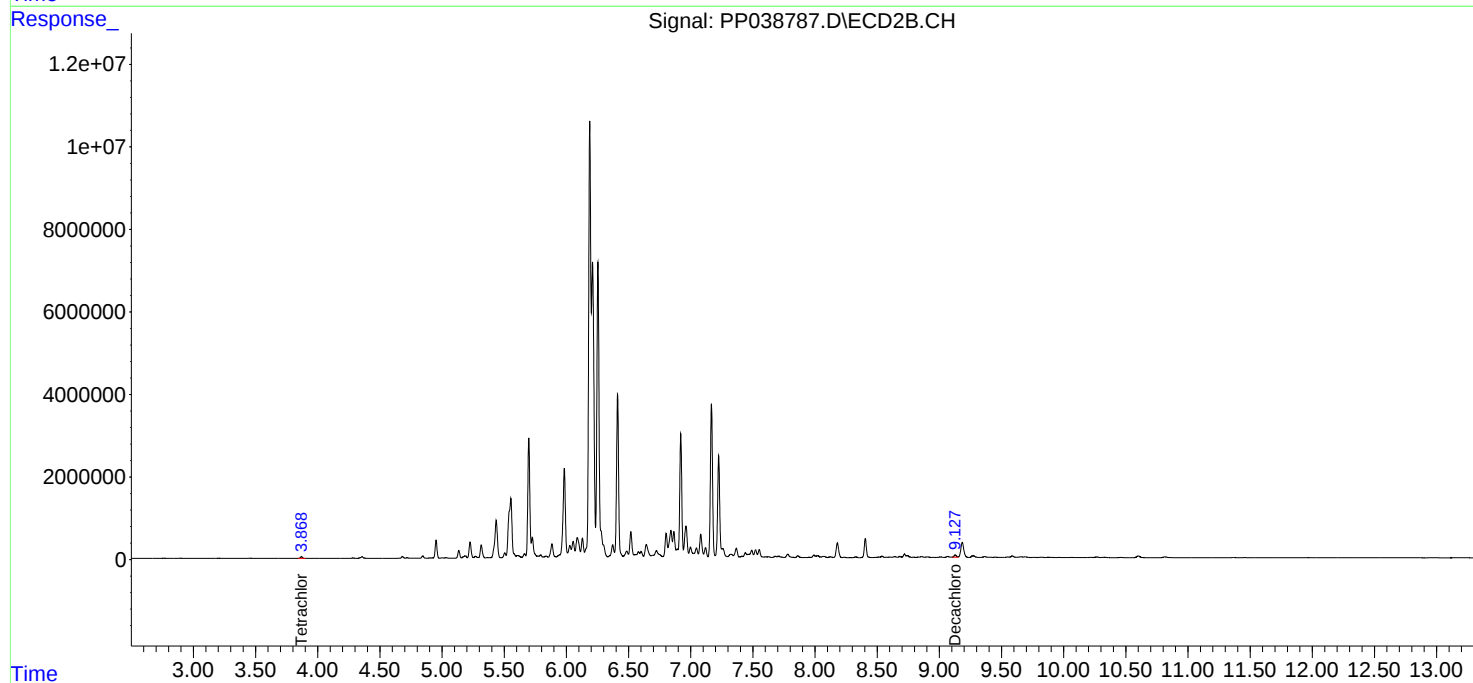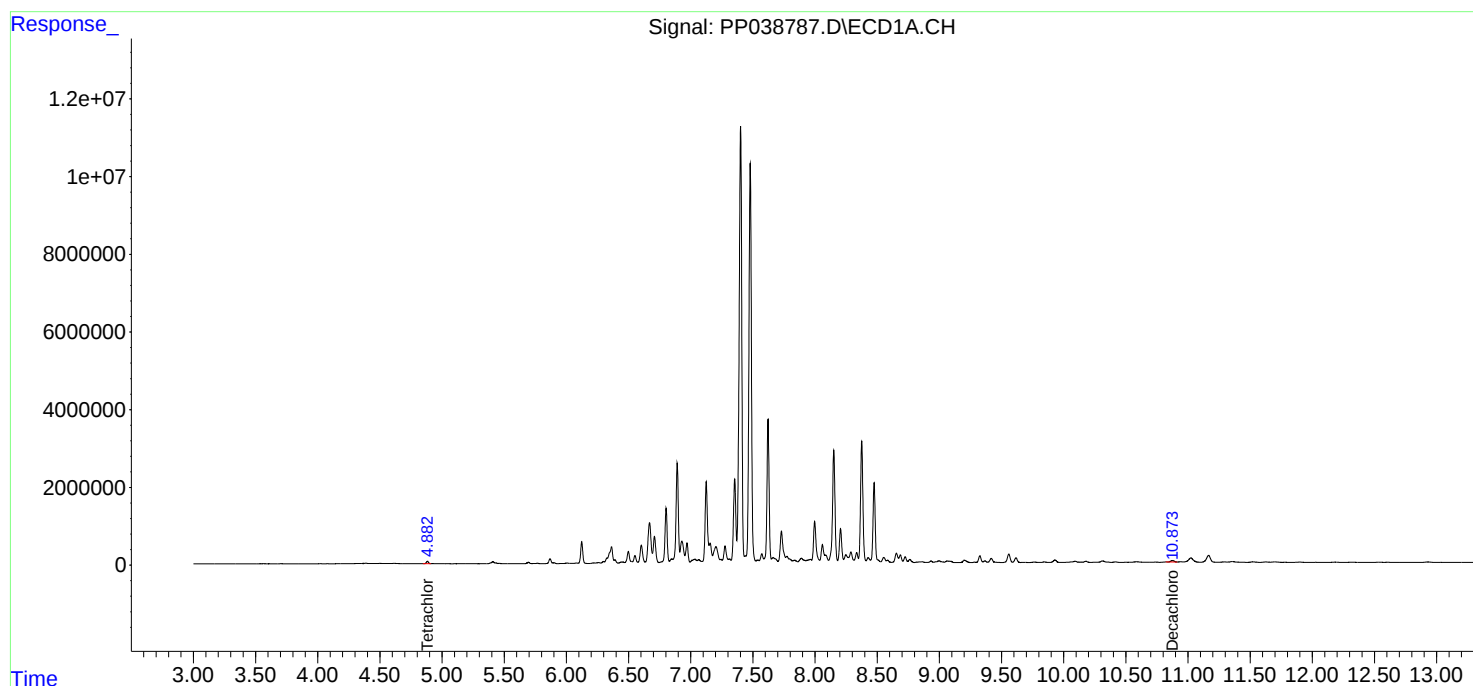

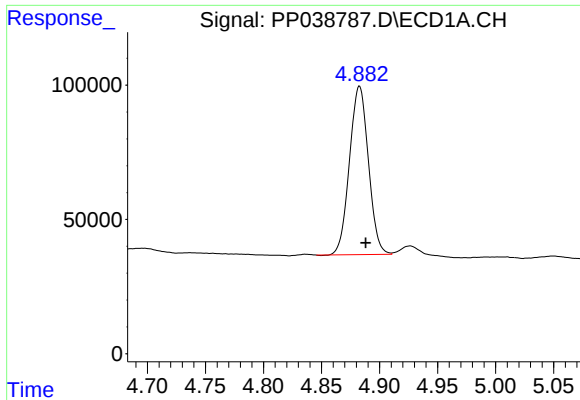


#1 Tetrachloro-m-xylene

R.T.: 4.883 min
Delta R.T.: -0.005 min
Response: 711672
Conc: 17.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
1-BMENT-F


Manual Integrations
APPROVED

mohammad
8/24/2021 10:28:52 AM

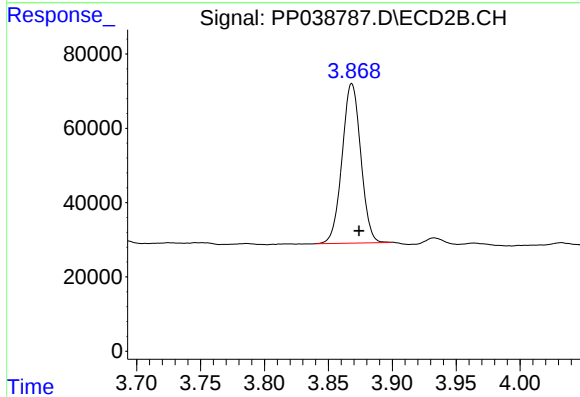


#1 Tetrachloro-m-xylene

R.T.: 3.868 min
Delta R.T.: -0.006 min
Response: 437081
Conc: 18.24 ng/ml m

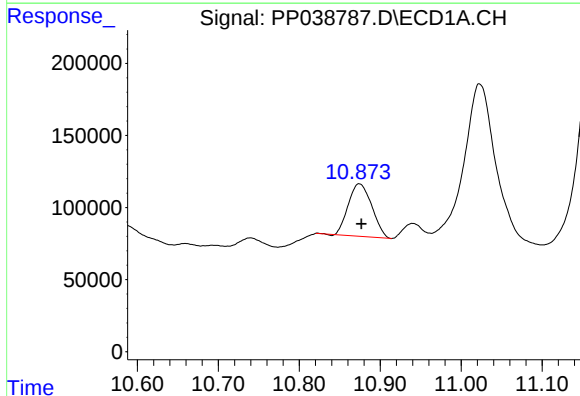

#2 Decachlorobiphenyl

R.T.: 10.874 min
Delta R.T.: -0.003 min
Response: 733460
Conc: 29.81 ng/ml

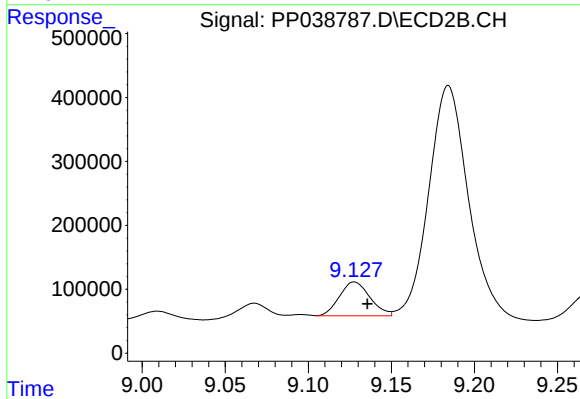

#2 Decachlorobiphenyl

R.T.: 9.127 min
Delta R.T.: -0.008 min
Response: 677140
Conc: 27.80 ng/ml m