

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082321\
 Data File : PP038813.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Aug 2021 00:56
 Operator : AJ\MA
 Sample : M3434-37RE
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SWCS-15-0510RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 07:46:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 18 04:51:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.881	3.867	453832	279262	11.245	11.653
2)	SA Decachlor...	10.865	9.125	141583	137077	5.755	5.628

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082321\
Data File : PP038813.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Aug 2021 00:56
Operator : AJ\MA
Sample : M3434-37RE
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SWCS-15-0510RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 07:46:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 18 04:51:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

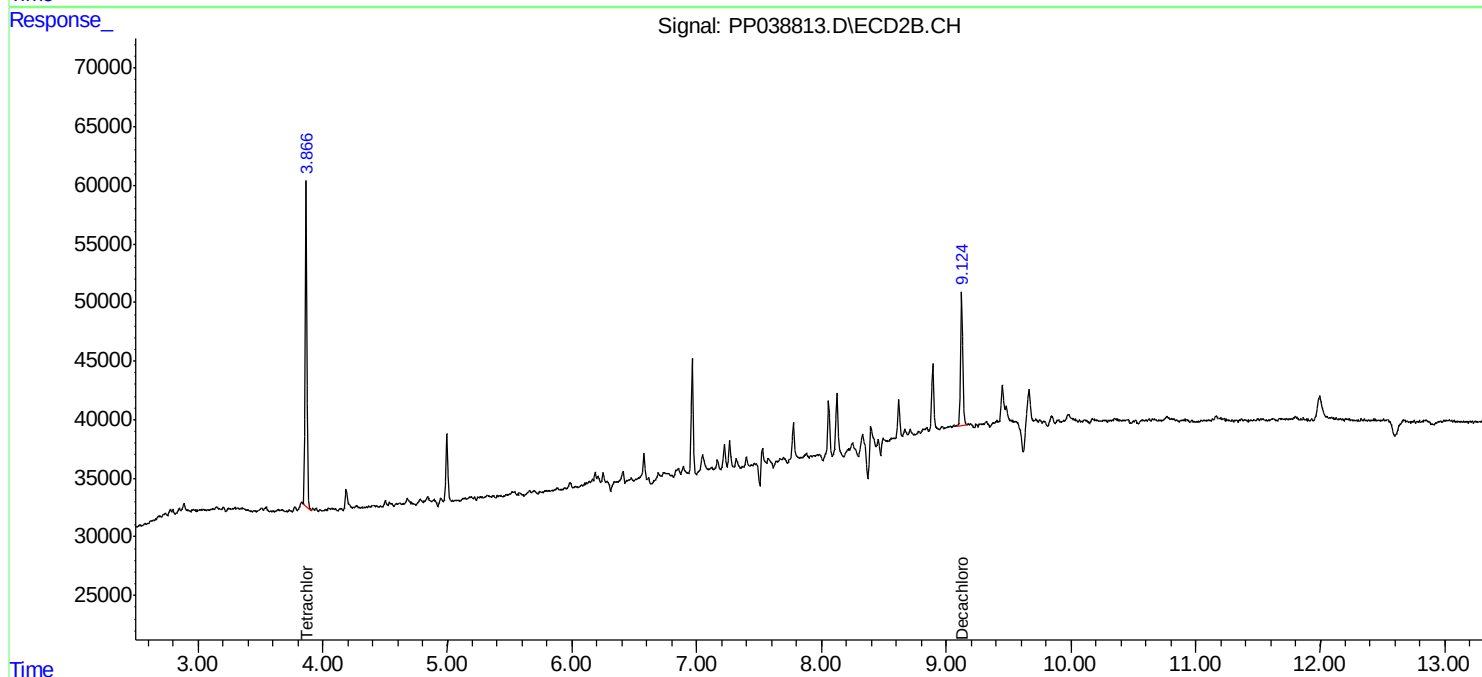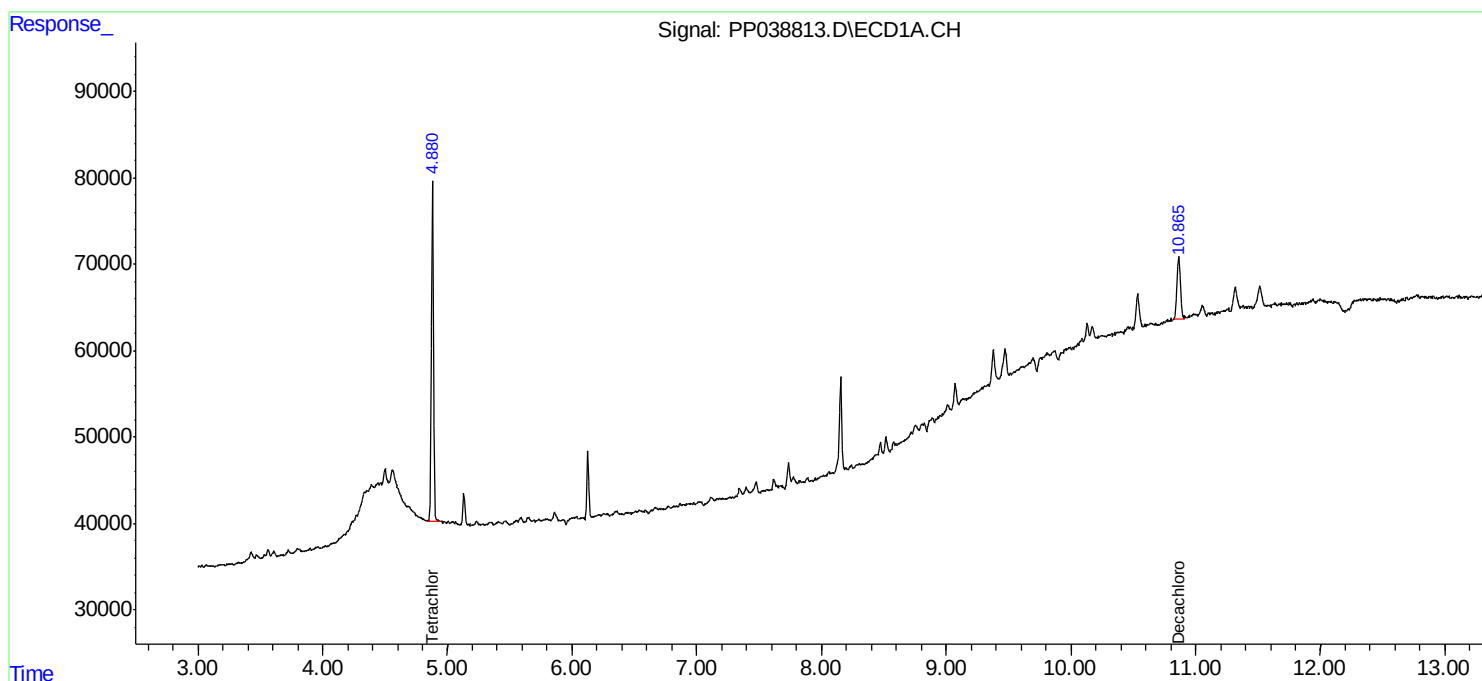


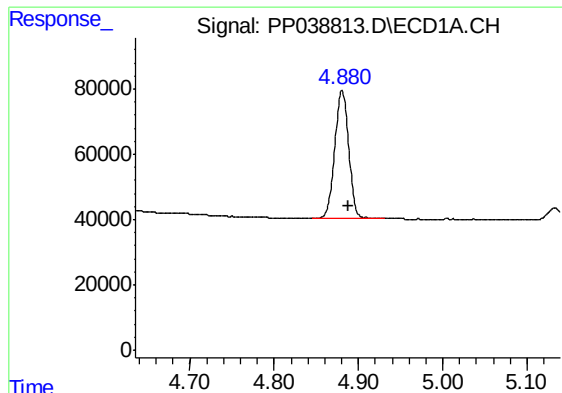

#1 Tetrachloro-m-xylene


R.T.: 4.881 min
Delta R.T.: -0.007 min
Response: 453832
Conc: 11.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
SWCS-15-0510RE

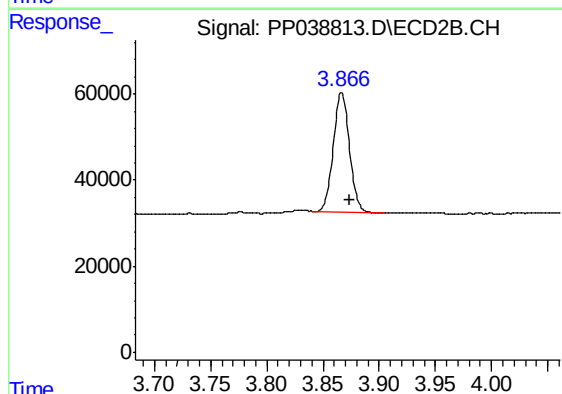


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: -0.007 min
Response: 279262
Conc: 11.65 ng/ml

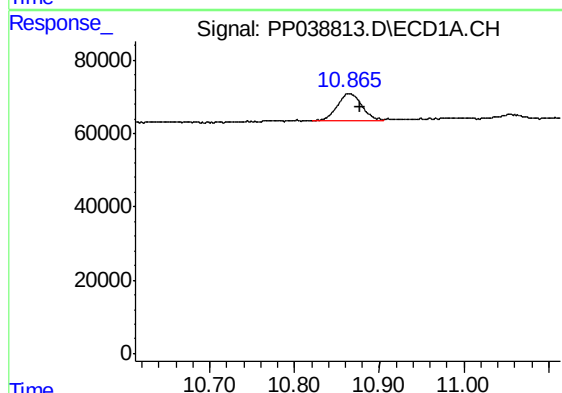

#2 Decachlorobiphenyl

R.T.: 10.865 min
Delta R.T.: -0.012 min
Response: 141583
Conc: 5.75 ng/ml

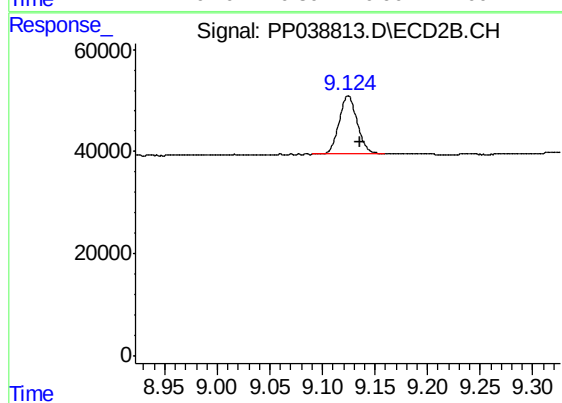

#2 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: -0.011 min
Response: 137077
Conc: 5.63 ng/ml