

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD P\Data\PP082418\
 Data File : PP027193.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Aug 2018 10:47
 Operator : EI\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 14:36:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP073018.M
 Quant Title : 8080.M
 QLast Update : Tue Jul 31 01:31:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

5) T	DICAMBA	0.000	12.502	0	21533521	N.D.	13.232	#
15) T	Picloram	17.608	0.000	13598332	0	3.293	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD P\Data\PP082418\
Data File : PP027193.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Aug 2018 10:47
Operator : EI\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 14:36:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP073018.M
Quant Title : 8080.M
QLast Update : Tue Jul 31 01:31:14 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

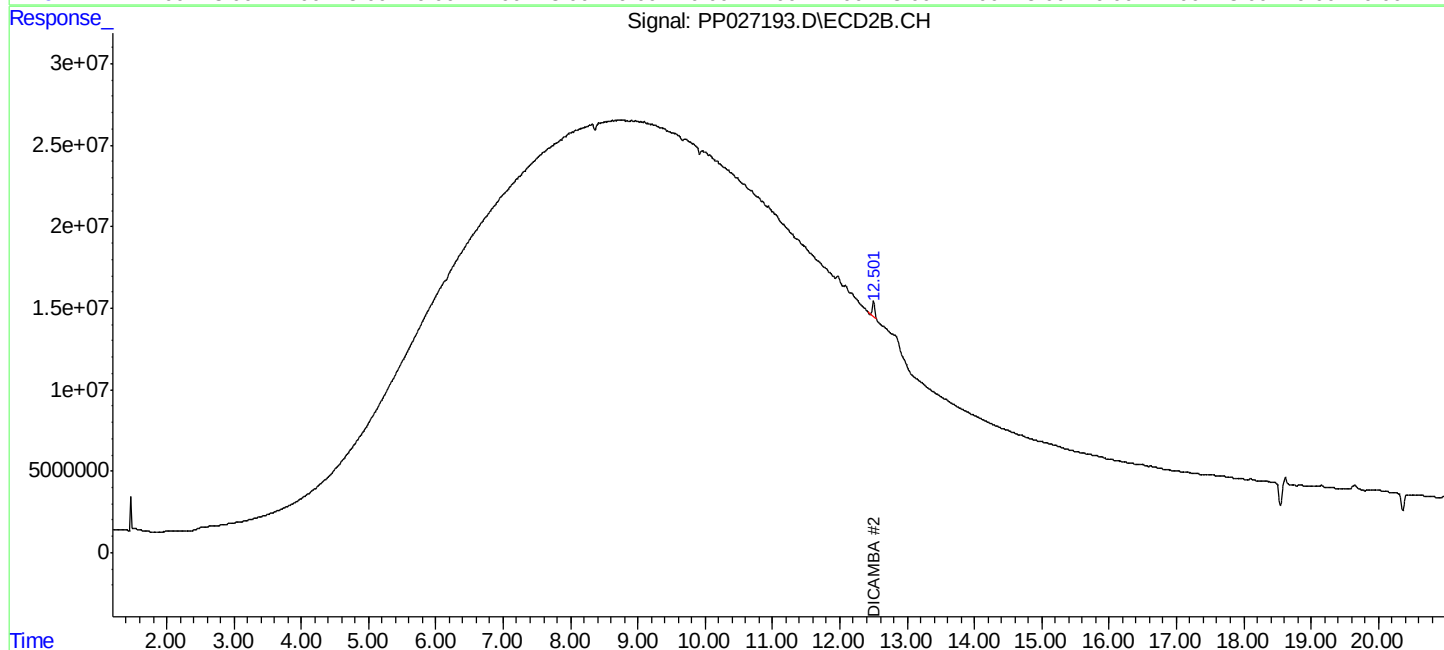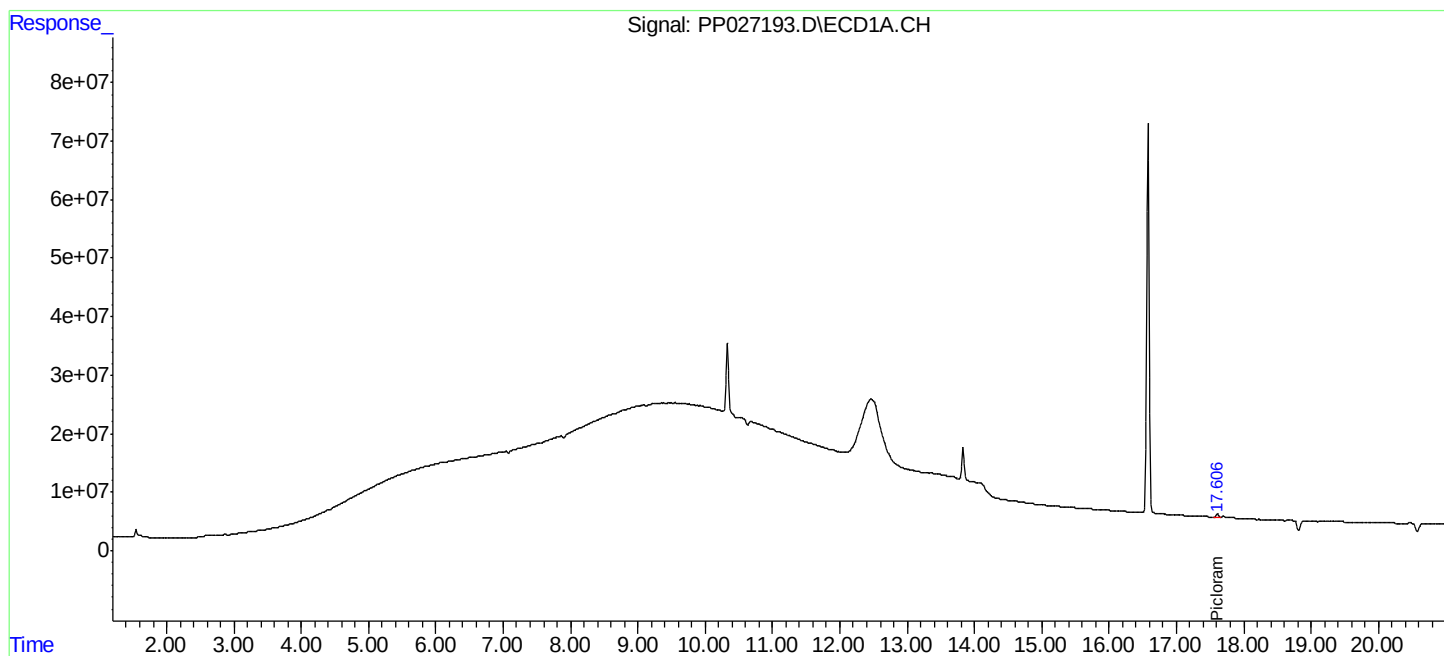


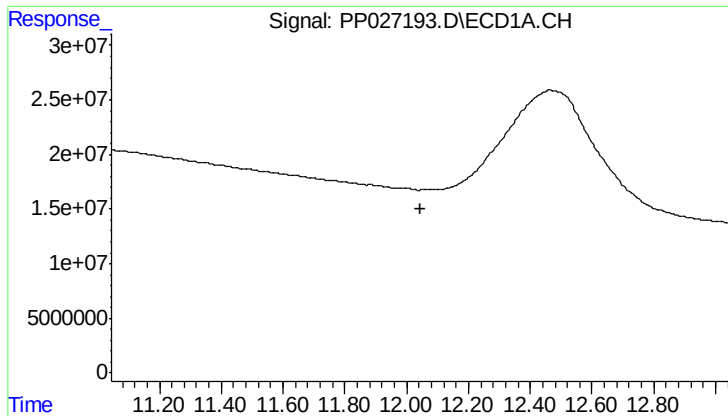

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 12.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

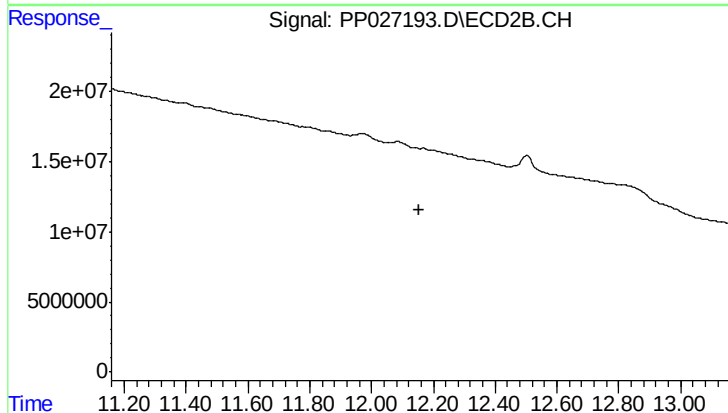


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 12.156 min
Response: 0
Conc: N.D.

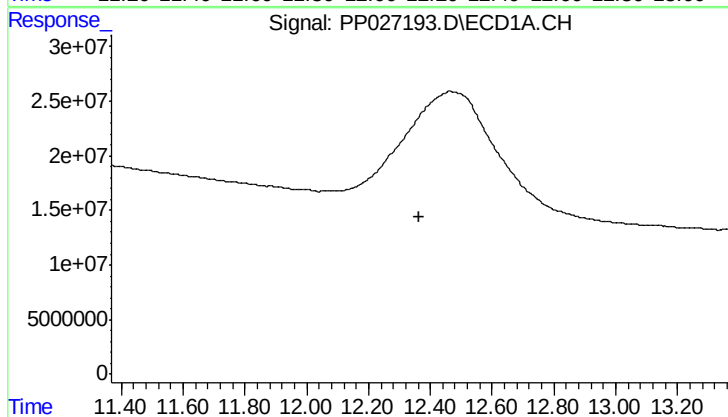


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 12.365 min
Response: 0
Conc: N.D.

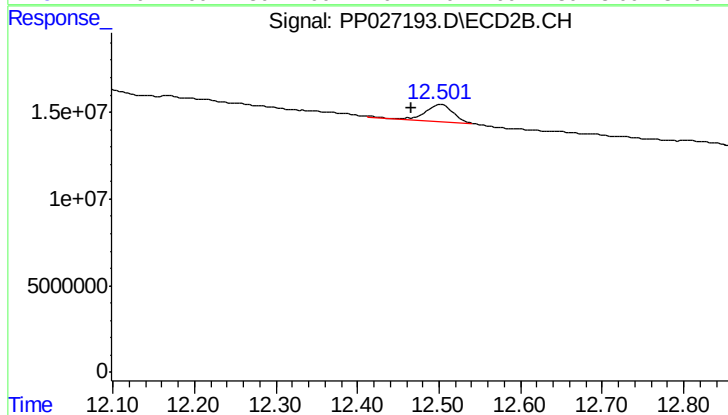

#5 DICAMBA


R.T.: 12.502 min
Delta R.T.: 0.035 min
Response: 21533521
Conc: 13.23 ng/ml

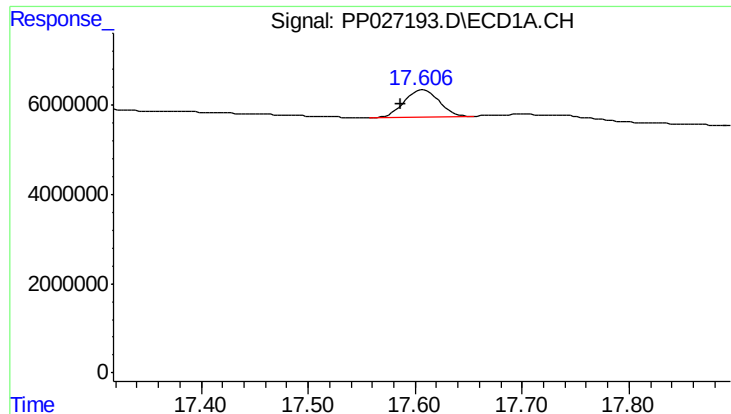

#15 Picloram

R.T.: 17.608 min
Delta R.T.: 0.020 min
Response: 13598332
Conc: 3.29 ng/ml

Instrument :
ECD_P
ClientSampleId :

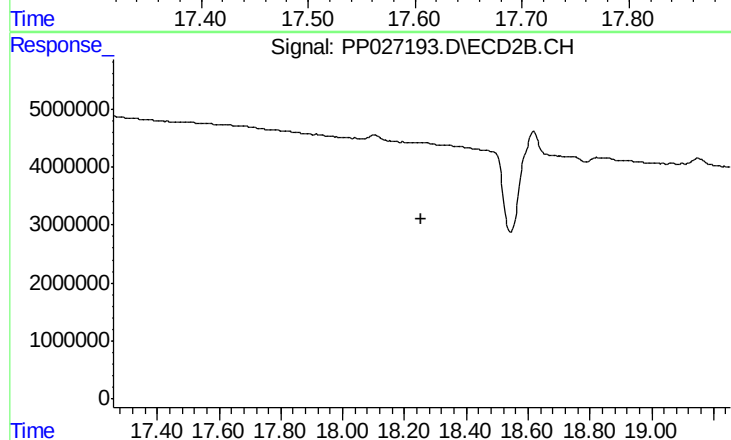

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 18.255 min
Response: 0
Conc: N.D.