

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082421\
 Data File : PP038878.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Aug 2021 1:47
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 09:52:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 18 04:51:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.880	3.866	793108	502393	19.652	20.964
2)	SA Decachlor...	10.861	9.121	540812	534954	21.981	21.964
Target Compounds							
7)	L1 AR-1016-5	0.000	5.636f	0	4744	N.D.	7.152 #
9)	L2 AR-1221-2	5.232	0.000	10170	0	28.708	N.D. #
24)	L5 AR-1248-4	7.149	0.000	960	0	0.777	N.D. #
26)	L6 AR-1254-1	7.116	0.000	23879	0	20.927	N.D. #
28)	L6 AR-1254-3	7.741f	0.000	10045	0	5.596	N.D. #
32)	L7 AR-1260-2	8.132f	0.000	5127	0	3.495	N.D. #
33)	L7 AR-1260-3	0.000	7.050	0	16796	N.D.	11.679 #
34)	L7 AR-1260-4	8.760	0.000	983	0	0.864	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082421\
Data File : PP038878.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Aug 2021 1:47
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 09:52:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 18 04:51:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

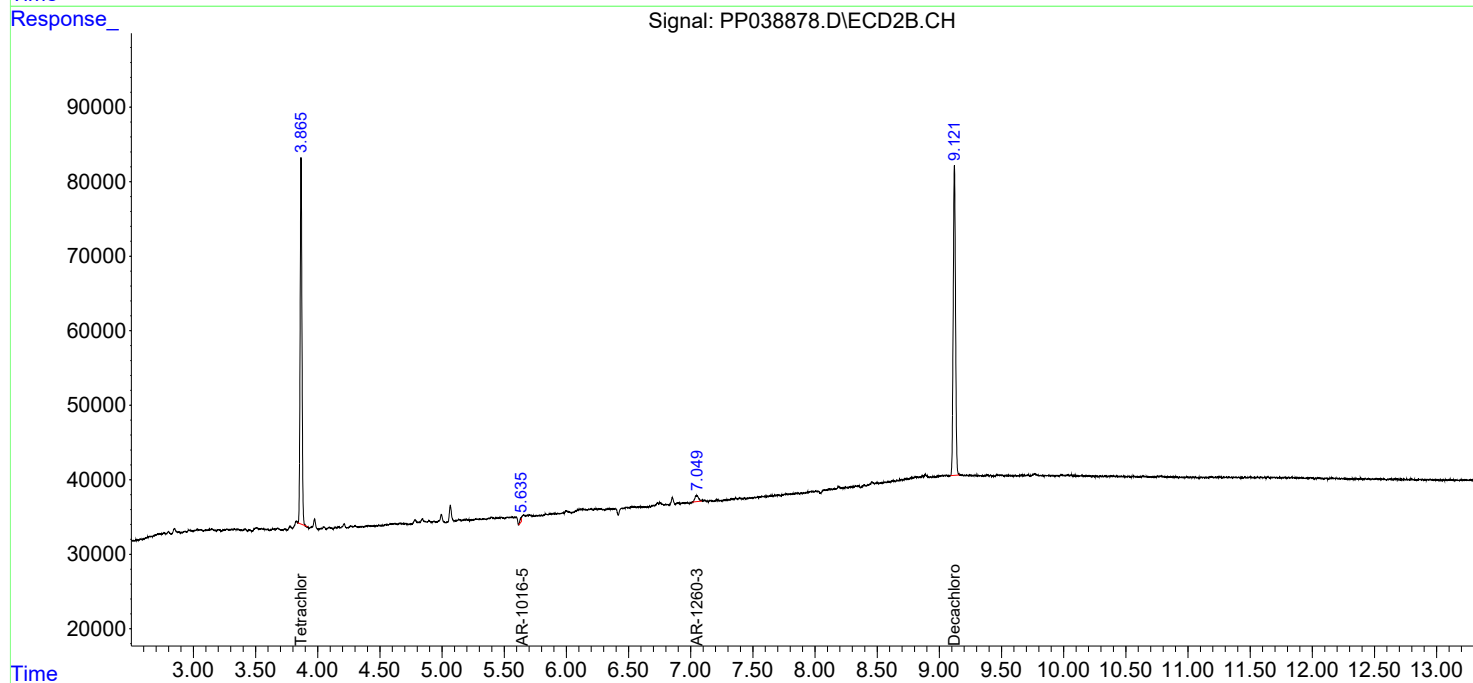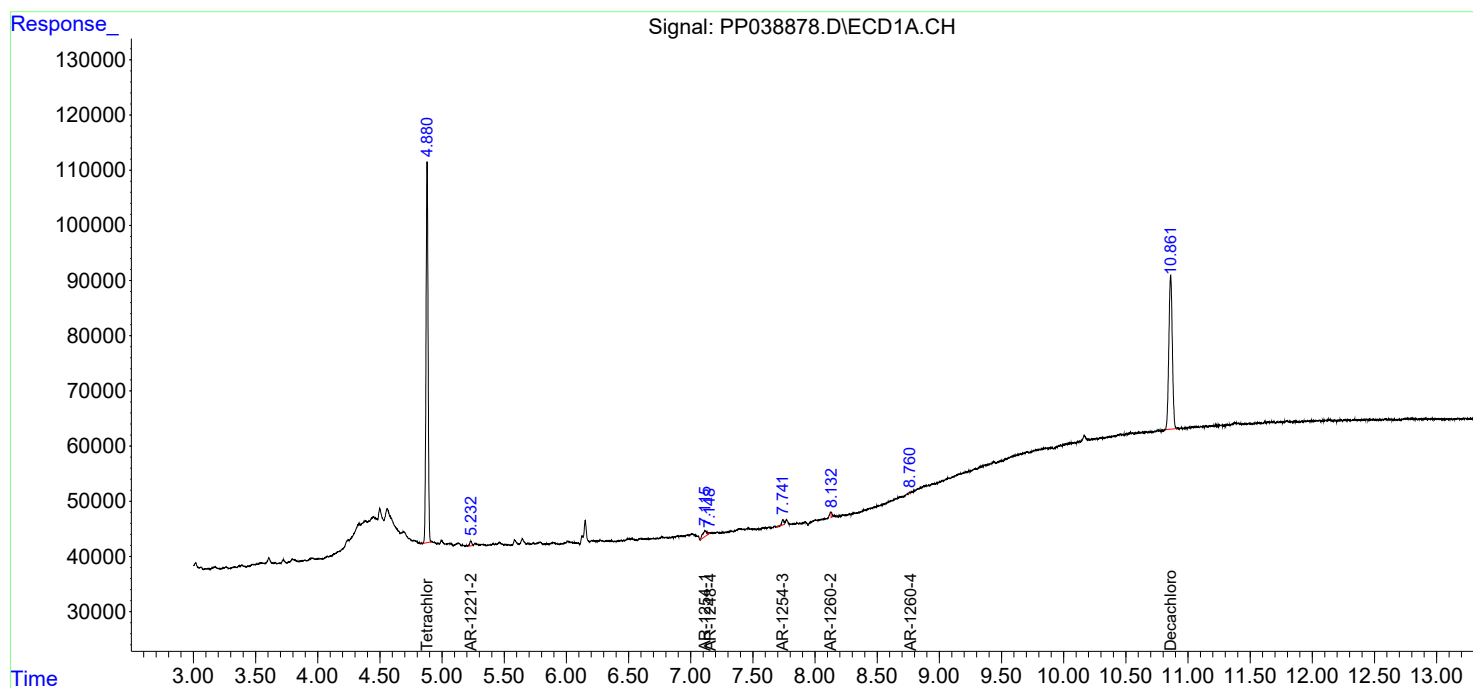


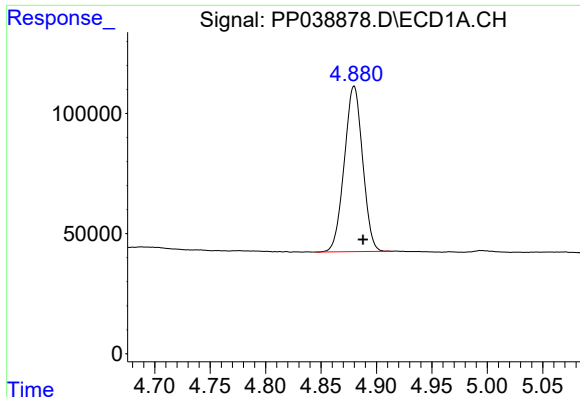

#1 Tetrachloro-m-xylene


R.T.: 4.880 min
Delta R.T.: -0.008 min
Response: 793108
Conc: 19.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

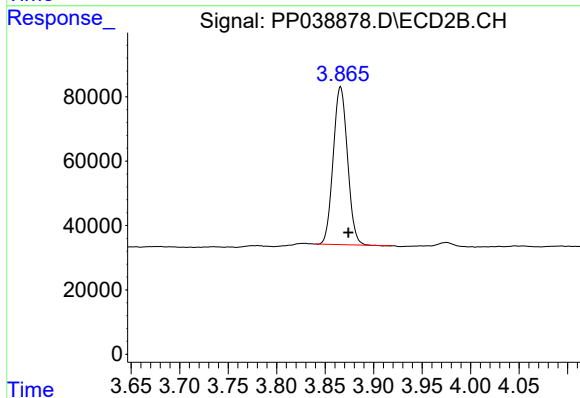


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: -0.008 min
Response: 502393
Conc: 20.96 ng/ml

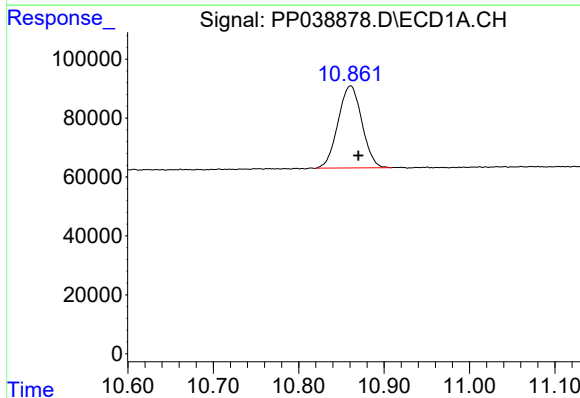


#2 Decachlorobiphenyl

R.T.: 10.861 min
Delta R.T.: -0.009 min
Response: 540812
Conc: 21.98 ng/ml

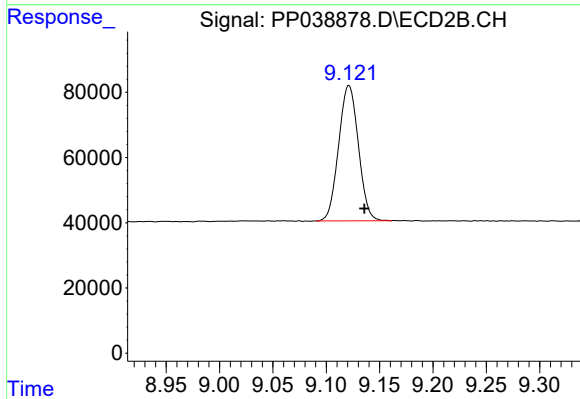

#2 Decachlorobiphenyl


R.T.: 9.121 min
Delta R.T.: -0.014 min
Response: 534954
Conc: 21.96 ng/ml

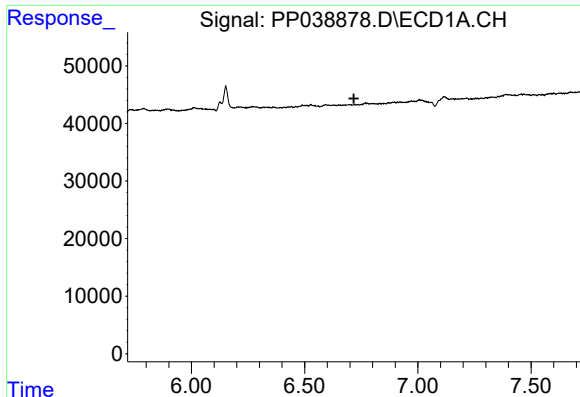

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.717 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

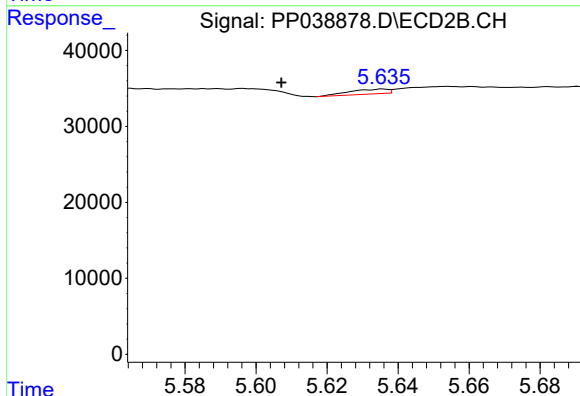


#7 AR-1016-5

R.T.: 5.636 min
Delta R.T.: 0.029 min
Response: 4744
Conc: 7.15 ng/ml

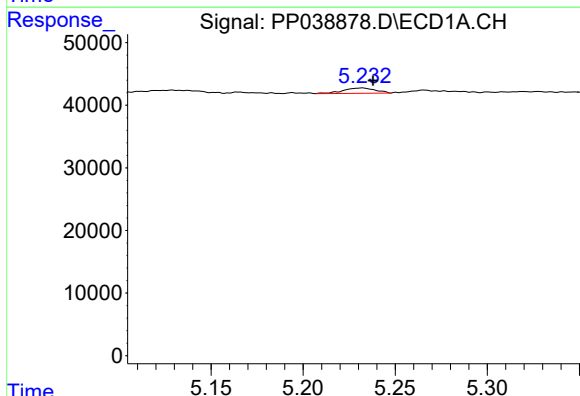


#9 AR-1221-2

R.T.: 5.232 min
Delta R.T.: -0.006 min
Response: 10170
Conc: 28.71 ng/ml

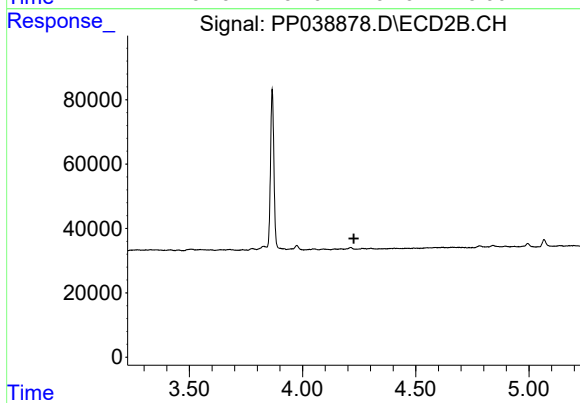

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.227 min
Response: 0
Conc: N.D.

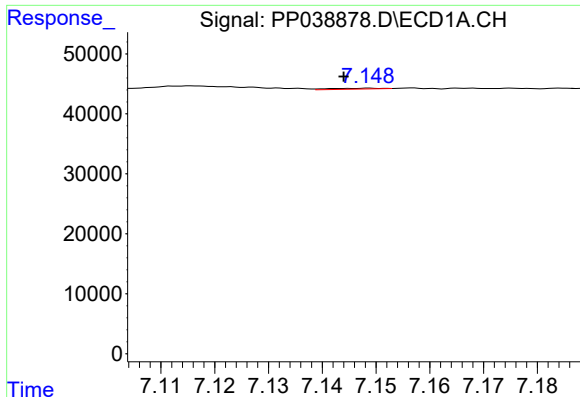

#24 AR-1248-4


R.T.: 7.149 min
Delta R.T.: 0.005 min
Response: 960
Conc: 0.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

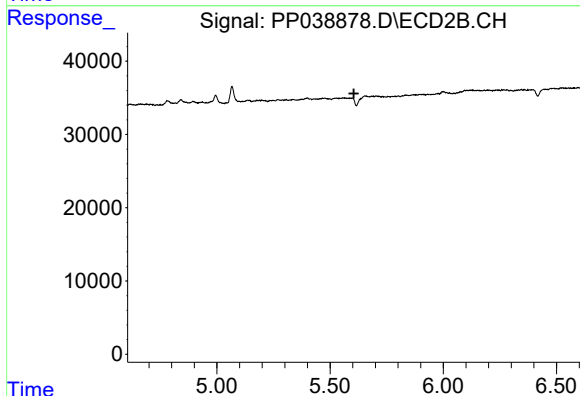


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.605 min
Response: 0
Conc: N.D.

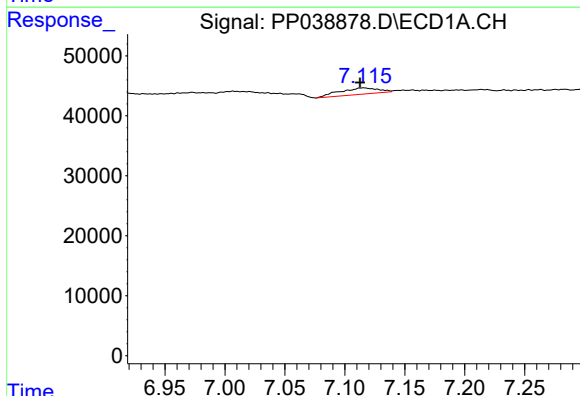


#26 AR-1254-1

R.T.: 7.116 min
Delta R.T.: 0.003 min
Response: 23879
Conc: 20.93 ng/ml

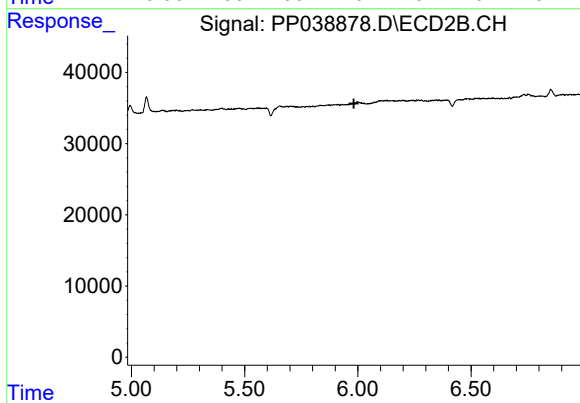

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

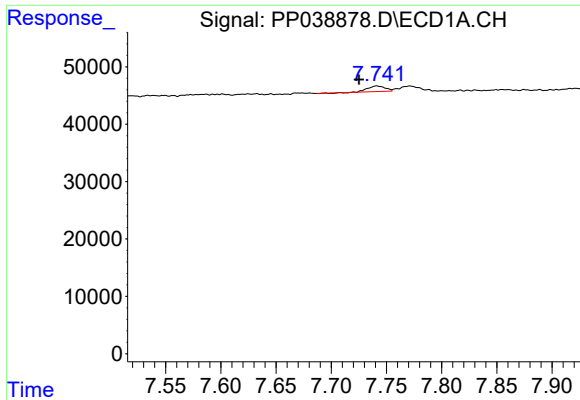

#28 AR-1254-3


R.T.: 7.741 min
Delta R.T.: 0.016 min
Response: 10045
Conc: 5.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

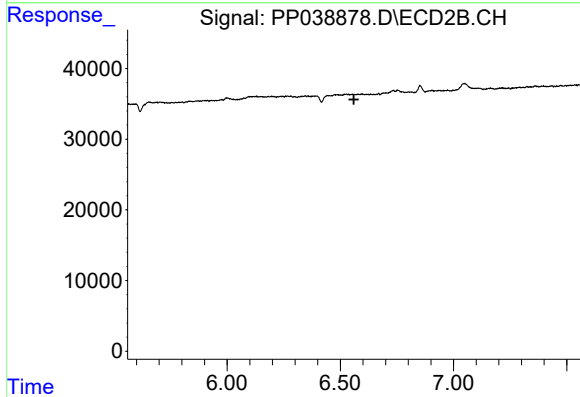


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.560 min
Response: 0
Conc: N.D.

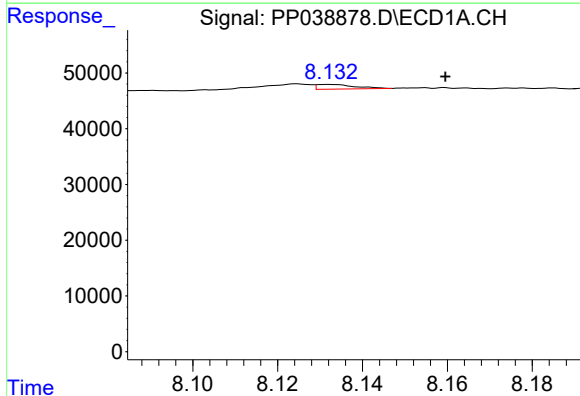


#32 AR-1260-2

R.T.: 8.132 min
Delta R.T.: -0.027 min
Response: 5127
Conc: 3.49 ng/ml

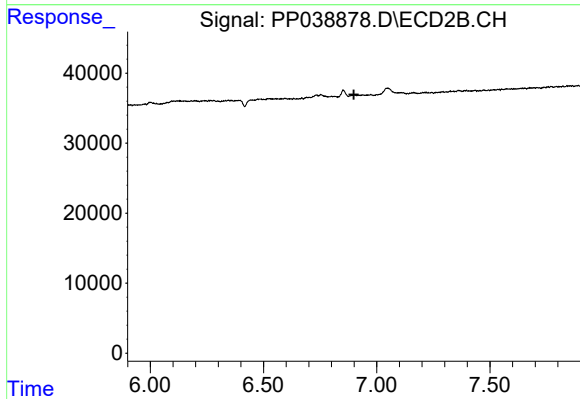

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.899 min
Response: 0
Conc: N.D.

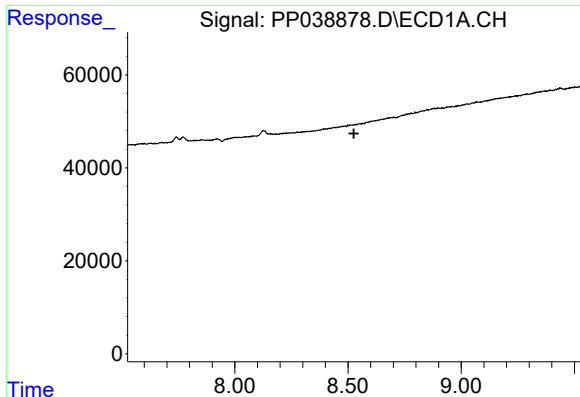

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

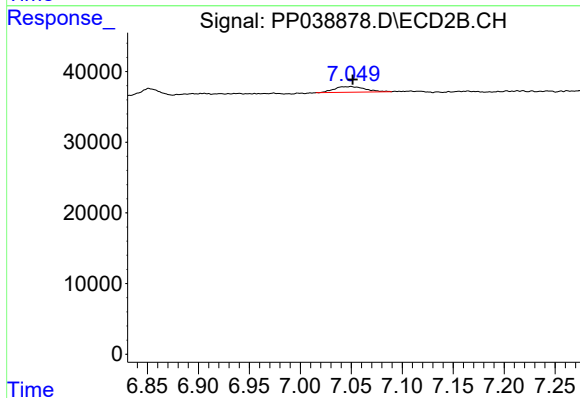


#33 AR-1260-3

R.T.: 7.050 min
Delta R.T.: -0.001 min
Response: 16796
Conc: 11.68 ng/ml

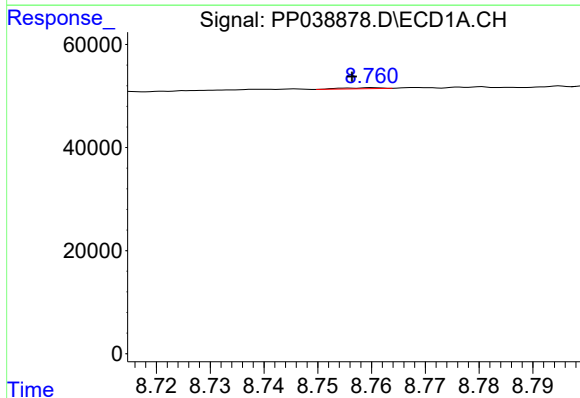

#34 AR-1260-4

R.T.: 8.760 min
Delta R.T.: 0.004 min
Response: 983
Conc: 0.86 ng/ml

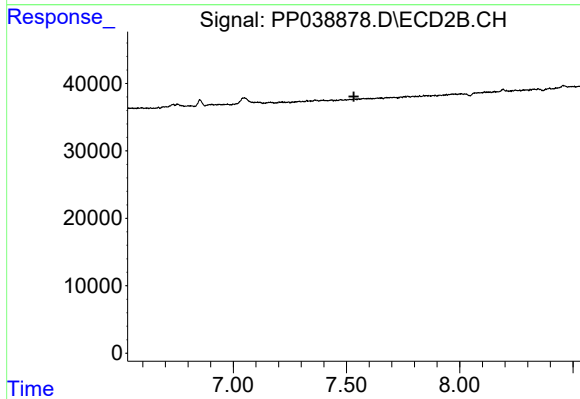

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.533 min
Response: 0
Conc: N.D.