

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082421\
 Data File : PP038884.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Aug 2021 3:28
 Operator : AJ\MA
 Sample : M3508-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BUILDING-5-6-7-GREY-DOOR-CAU

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 09:55:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 18 04:51:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.880	3.866	782117	512054	19.380	21.368
2)	SA Decachlor...	10.861	9.122	462517	425414	18.799	17.467
Target Compounds							
3)	L1 AR-1016-1	6.224f	0.000	5490	0	4.231	N.D. #
4)	L1 AR-1016-2	6.224	0.000	5490	0	2.971	N.D. #
5)	L1 AR-1016-3	6.289	0.000	1610	0	1.409	N.D. #
6)	L1 AR-1016-4	0.000	5.387	0	6845	N.D.	13.072 #
7)	L1 AR-1016-5	6.714	5.588f	9576	31271	11.296	47.148 #
8)	L2 AR-1221-1	5.131	0.000	48985	0	104.745	N.D. #
9)	L2 AR-1221-2	5.230	0.000	8416	0	23.757	N.D. #
10)	L2 AR-1221-3	5.331	0.000	10812	0	10.152	N.D. #
11)	L3 AR-1232-1	5.331	0.000	10812	0	10.932	N.D. #
12)	L3 AR-1232-2	5.904	0.000	2920	0	6.272	N.D. #
13)	L3 AR-1232-3	6.224	0.000	5490	0	6.431	N.D. #
14)	L3 AR-1232-4	0.000	5.414	0	14214	N.D.	57.451 #
15)	L3 AR-1232-5	6.514	5.588f	32283	31271	120.139	115.661
16)	L4 AR-1242-1	6.224f	0.000	5490	0	5.512	N.D. #
17)	L4 AR-1242-2	6.224	0.000	5490	0	3.821	N.D. #
18)	L4 AR-1242-3	6.289	0.000	1610	0	1.798	N.D. #
19)	L4 AR-1242-4	0.000	5.414	0	14214	N.D.	29.737 #
20)	L4 AR-1242-5	7.163f	5.994	80462	29408	112.540	47.505 #
21)	L5 AR-1248-1	6.224f	0.000	5490	0	6.890	N.D. #
22)	L5 AR-1248-2	6.514f	5.387	32283	6845	32.927	9.210 #
23)	L5 AR-1248-3	6.714	5.414	9576	14214	8.296	18.719 #
24)	L5 AR-1248-4	7.129f	5.588f	75870	31271	61.440	33.808 #
25)	L5 AR-1248-5	7.163f	6.013	80462	10893	65.808	12.064 #
26)	L6 AR-1254-1	7.129f	5.994	75870	29408	66.493	22.392 #
27)	L6 AR-1254-2	7.357	6.143	47446	63513	27.475	55.335 #
28)	L6 AR-1254-3	7.737	6.567	35956	116520	20.030	62.620 #
29)	L6 AR-1254-4	7.993f	6.795	6790	71010	5.262	60.764 #
30)	L6 AR-1254-5	8.466f	7.215	65908	37789	53.289	23.380 #
31)	L7 AR-1260-1	7.905	6.682f	53297	72370	44.533	61.845 #
32)	L7 AR-1260-2	8.178f	6.870f	396282	89821	270.096	63.100 #
33)	L7 AR-1260-3	8.504f	7.047	129338	21080	134.798	14.657 #
34)	L7 AR-1260-4	8.743	7.531	443814	283606	390.290	252.530 #
35)	L7 AR-1260-5	9.076	7.793	18258	102445	8.136	37.821 #
36)	L8 AR-1262-1	8.504f	7.215	129338	37789	87.006	41.808 #
37)	L8 AR-1262-2	9.076	7.793	18258	102445	6.858	33.158 #
38)	L8 AR-1262-3	9.387	8.075	558897	82019	469.076	65.281 #
39)	L8 AR-1262-4	9.487	8.138	432240	168525	536.518	71.307 #
40)	L8 AR-1262-5	10.158f	0.000	103233	0	96.849	N.D. #
41)	L9 AR-1268-1	9.387	8.075	558897	82019	174.242	22.461 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082421\
 Data File : PP038884.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Aug 2021 3:28
 Operator : AJ\MA
 Sample : M3508-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1


Instrument :
 ECD_P
 ClientSampleId :
 BUILDING-5-6-7-GREY-DOOR-CAU

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 09:55:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 18 04:51:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	9.487	8.138	432240	168525	140.298	48.851 #
43) L9	AR-1268-3	0.000	8.336	0	27212	N.D.	9.347 #
44) L9	AR-1268-4	10.158f	0.000	103233	0	84.738	N.D. #
45) L9	AR-1268-5	0.000	8.886	0	24525	N.D.	2.524 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

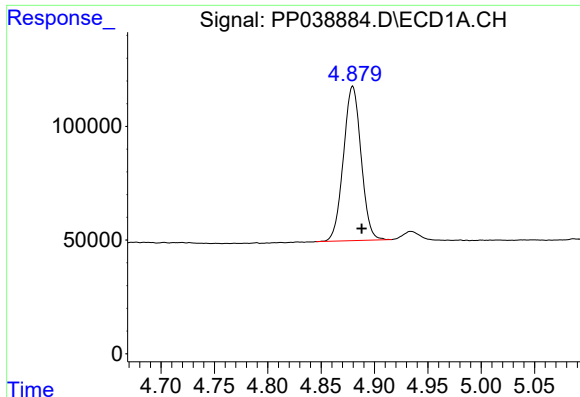

#1 Tetrachloro-m-xylene


R.T.: 4.880 min
Delta R.T.: -0.008 min
Response: 782117
Conc: 19.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

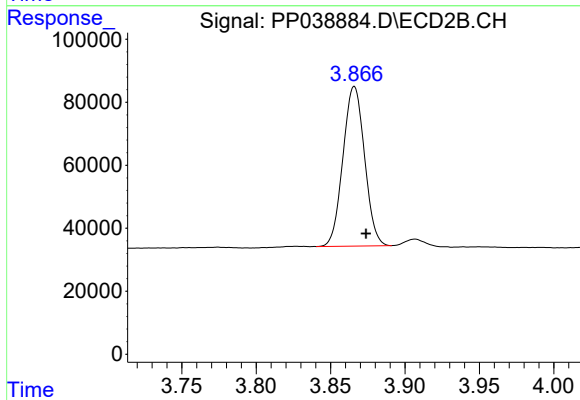


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: -0.008 min
Response: 512054
Conc: 21.37 ng/ml

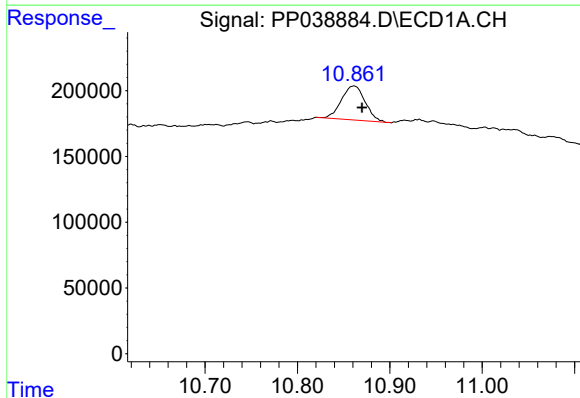


#2 Decachlorobiphenyl

R.T.: 10.861 min
Delta R.T.: -0.009 min
Response: 462517
Conc: 18.80 ng/ml

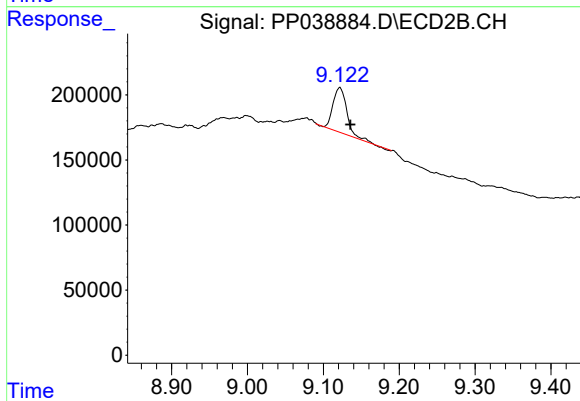

#2 Decachlorobiphenyl


R.T.: 9.122 min
Delta R.T.: -0.014 min
Response: 425414
Conc: 17.47 ng/ml

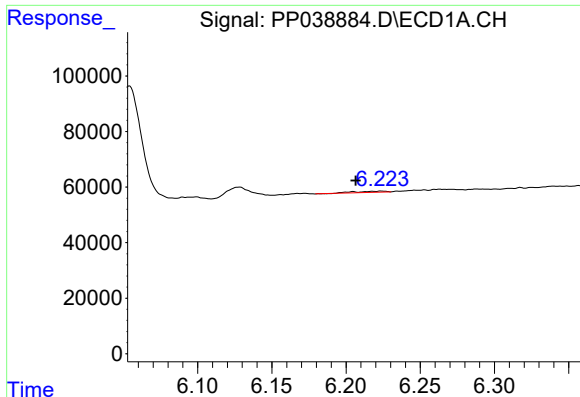

#3 AR-1016-1


R.T.: 6.224 min
Delta R.T.: 0.018 min
Response: 5490
Conc: 4.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

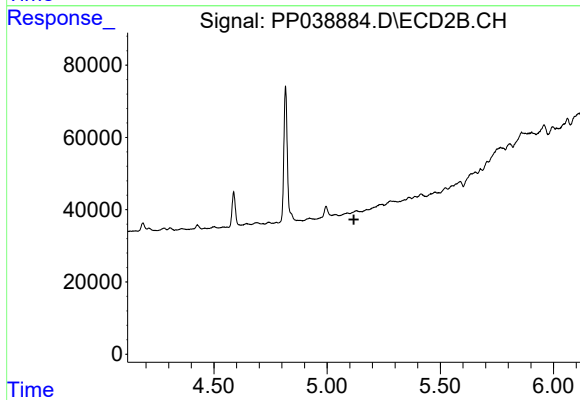


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 5.118 min
Response: 0
Conc: N.D.

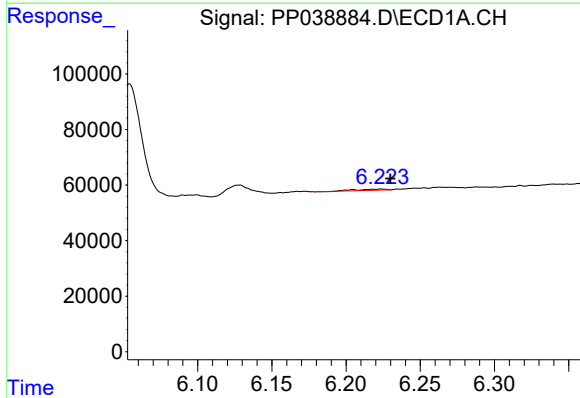


#4 AR-1016-2

R.T.: 6.224 min
Delta R.T.: -0.006 min
Response: 5490
Conc: 2.97 ng/ml

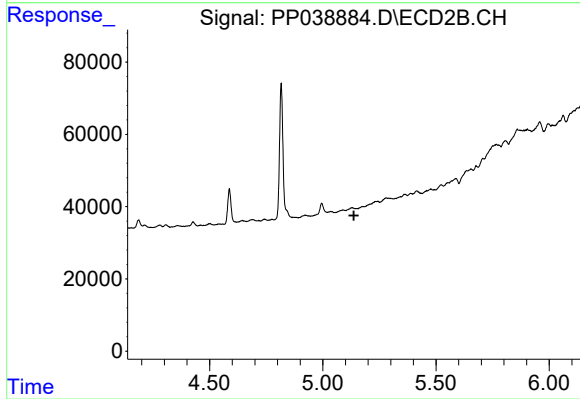

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 5.138 min
Response: 0
Conc: N.D.

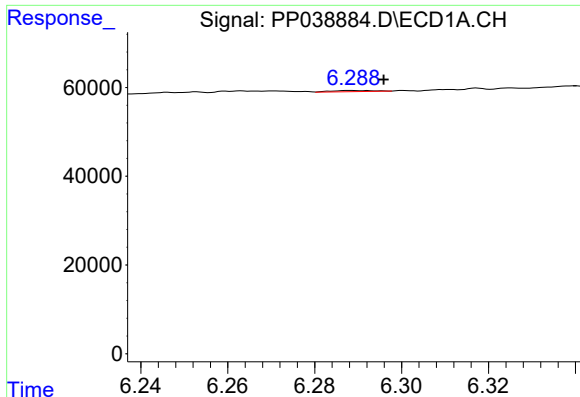

#5 AR-1016-3


R.T.: 6.289 min
Delta R.T.: -0.007 min
Response: 1610
Conc: 1.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

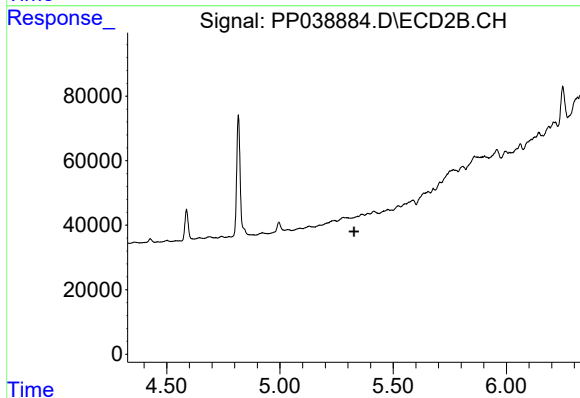


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 5.327 min
Response: 0
Conc: N.D.

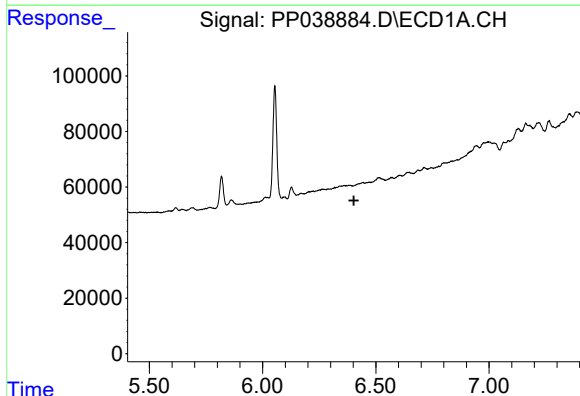


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 6.403 min
Response: 0
Conc: N.D.

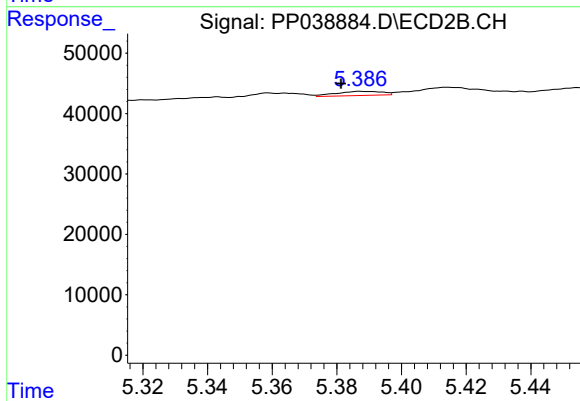

#6 AR-1016-4


R.T.: 5.387 min
Delta R.T.: 0.006 min
Response: 6845
Conc: 13.07 ng/ml

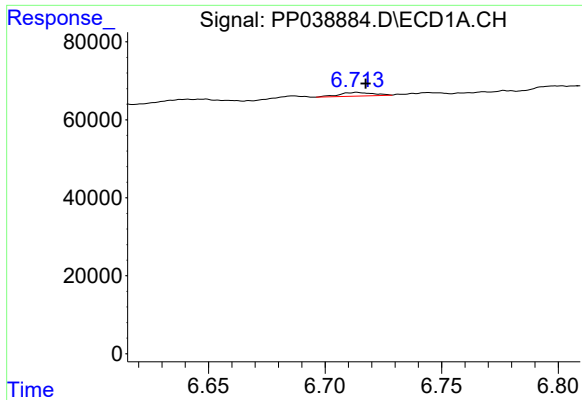

#7 AR-1016-5


R.T.: 6.714 min
Delta R.T.: -0.004 min
Response: 9576
Conc: 11.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

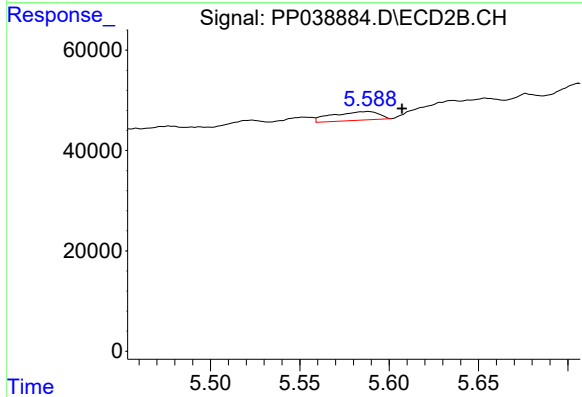


#7 AR-1016-5

R.T.: 5.588 min
Delta R.T.: -0.019 min
Response: 31271
Conc: 47.15 ng/ml

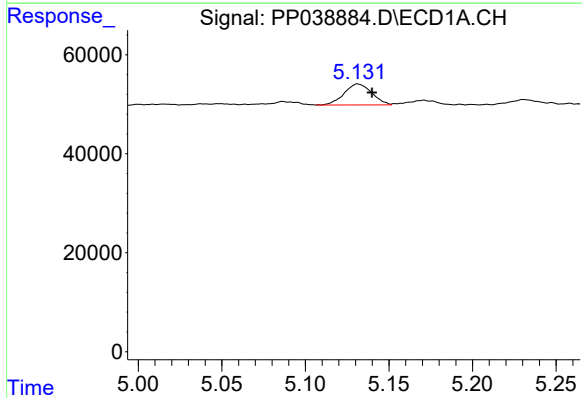


#8 AR-1221-1

R.T.: 5.131 min
Delta R.T.: -0.008 min
Response: 48985
Conc: 104.75 ng/ml

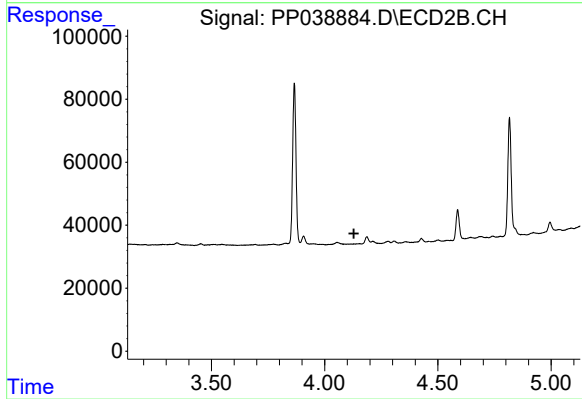

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.129 min
Response: 0
Conc: N.D.

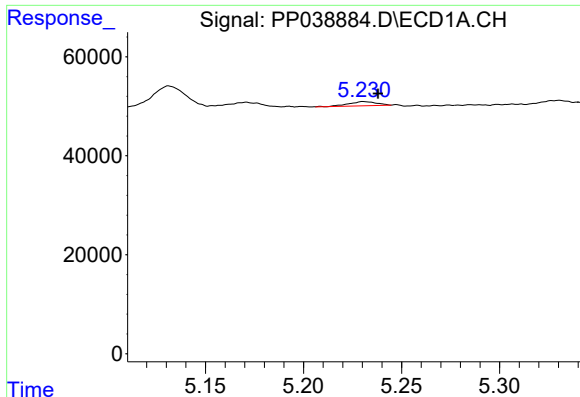

#9 AR-1221-2


R.T.: 5.230 min
Delta R.T.: -0.008 min
Response: 8416
Conc: 23.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

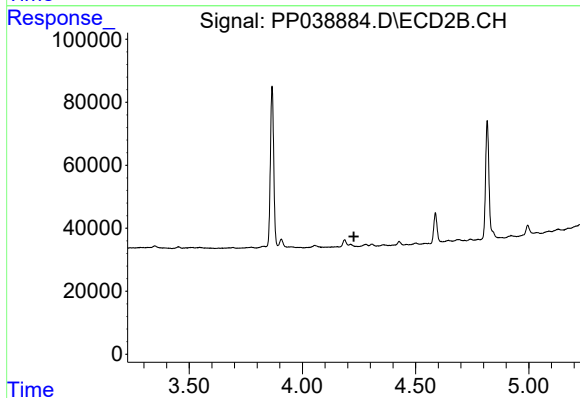


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.227 min
Response: 0
Conc: N.D.

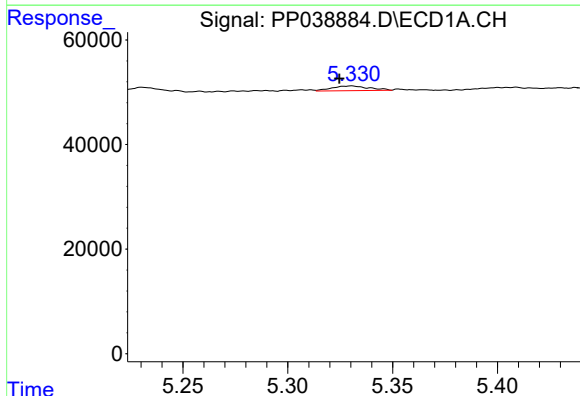


#10 AR-1221-3

R.T.: 5.331 min
Delta R.T.: 0.006 min
Response: 10812
Conc: 10.15 ng/ml

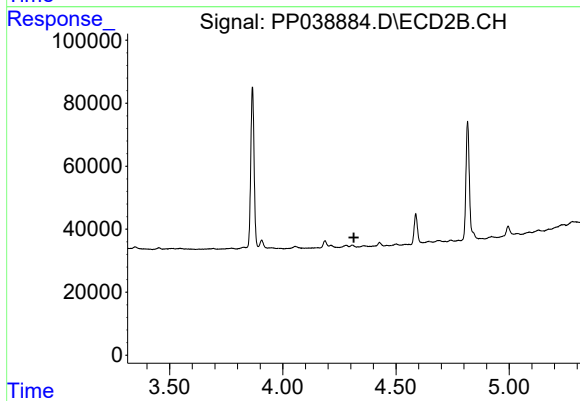

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.314 min
Response: 0
Conc: N.D.

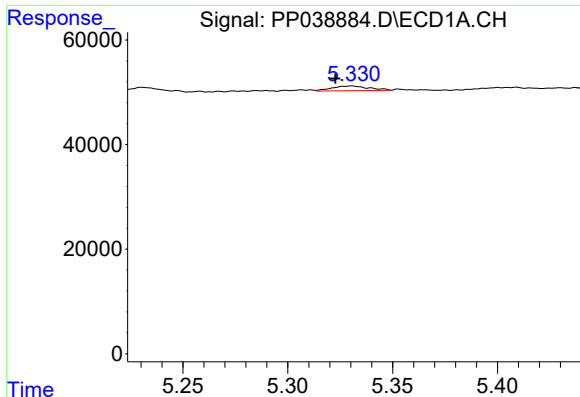

#11 AR-1232-1


R.T.: 5.331 min
Delta R.T.: 0.008 min
Response: 10812
Conc: 10.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

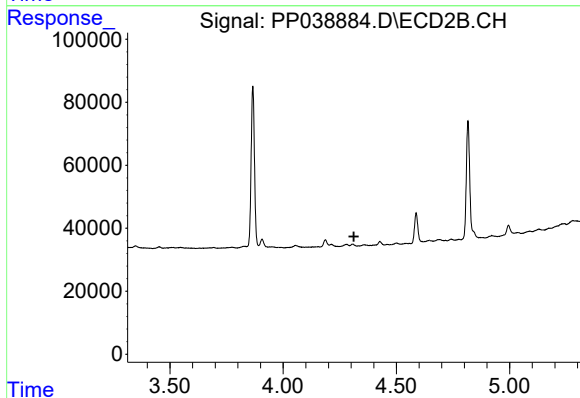


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.312 min
Response: 0
Conc: N.D.

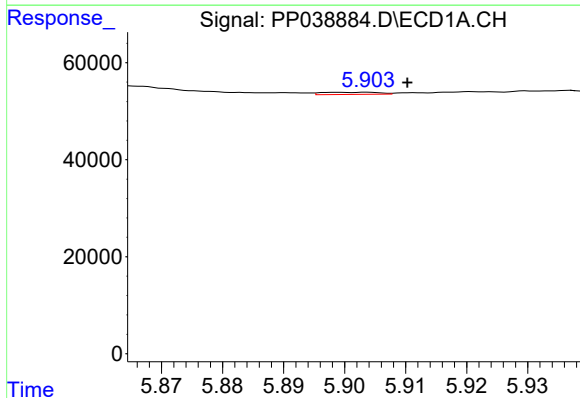


#12 AR-1232-2

R.T.: 5.904 min
Delta R.T.: -0.006 min
Response: 2920
Conc: 6.27 ng/ml

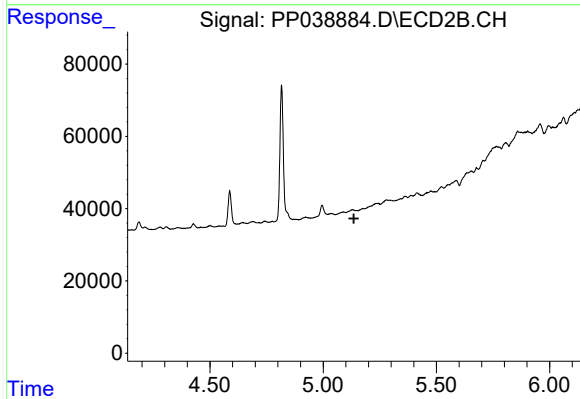

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 5.136 min
Response: 0
Conc: N.D.

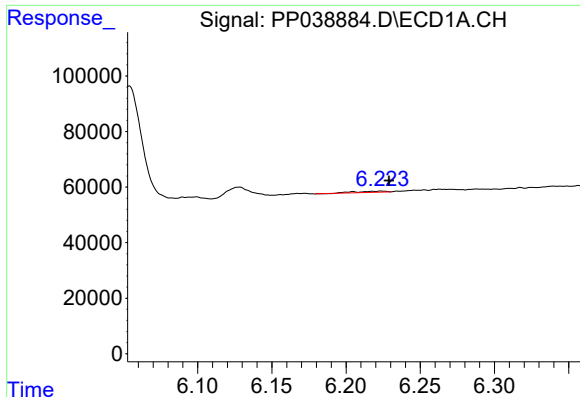

#13 AR-1232-3


R.T.: 6.224 min
Delta R.T.: -0.005 min
Response: 5490
Conc: 6.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

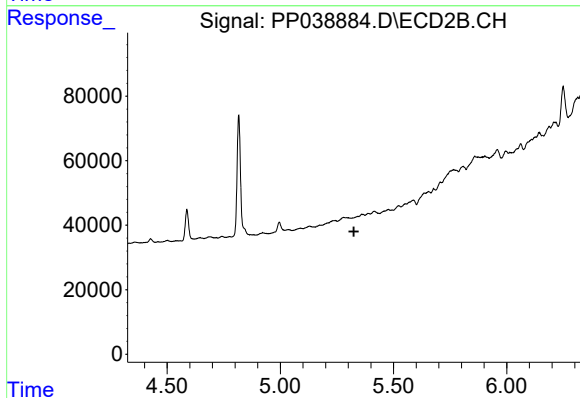


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 5.325 min
Response: 0
Conc: N.D.

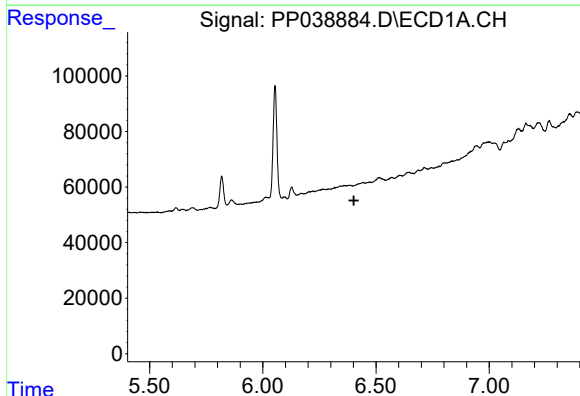


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

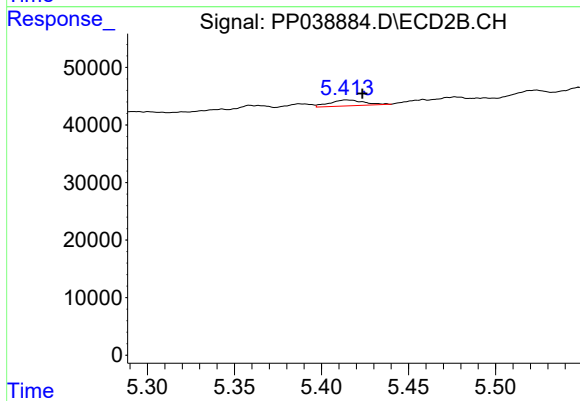

#14 AR-1232-4


R.T.: 5.414 min
Delta R.T.: -0.009 min
Response: 14214
Conc: 57.45 ng/ml

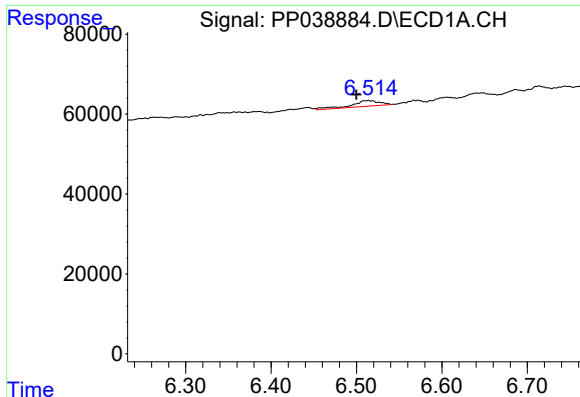

#15 AR-1232-5


R.T.: 6.514 min
Delta R.T.: 0.014 min
Response: 32283
Conc: 120.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

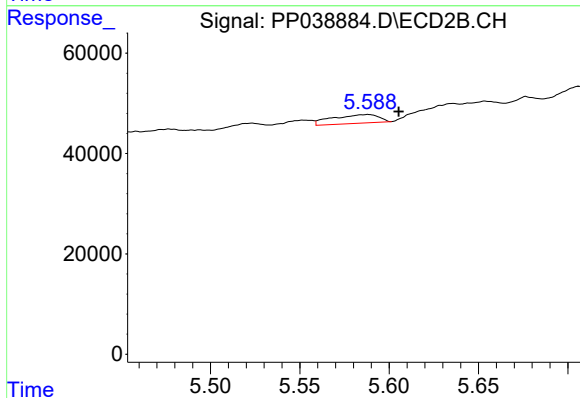


#15 AR-1232-5

R.T.: 5.588 min
Delta R.T.: -0.017 min
Response: 31271
Conc: 115.66 ng/ml

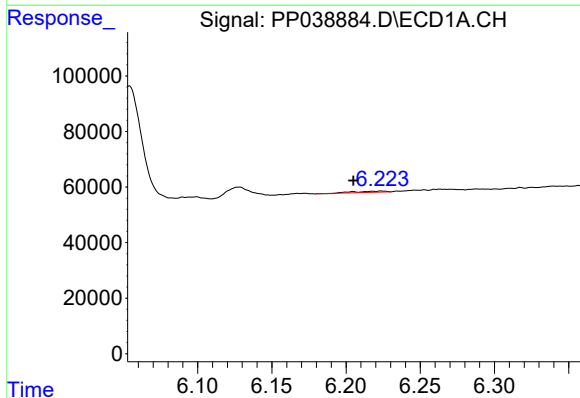


#16 AR-1242-1

R.T.: 6.224 min
Delta R.T.: 0.019 min
Response: 5490
Conc: 5.51 ng/ml

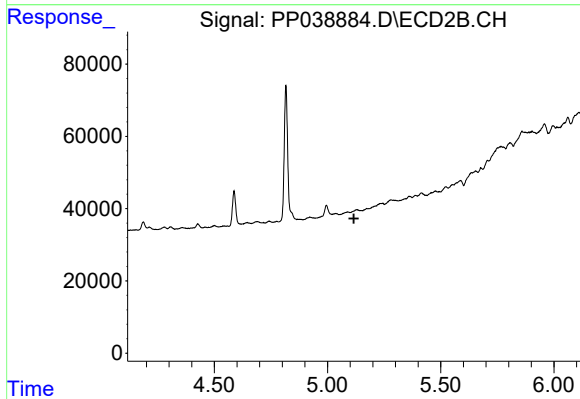

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 5.116 min
Response: 0
Conc: N.D.

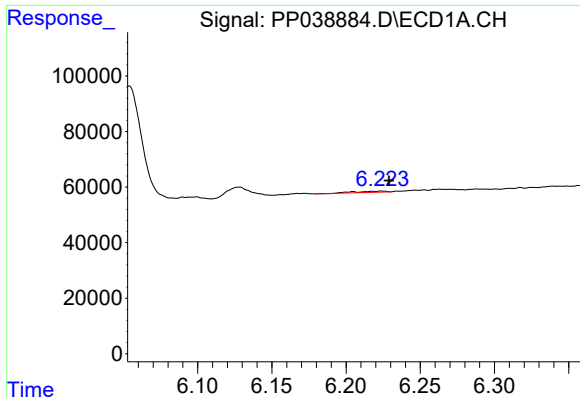

#17 AR-1242-2


R.T.: 6.224 min
Delta R.T.: -0.005 min
Response: 5490
Conc: 3.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

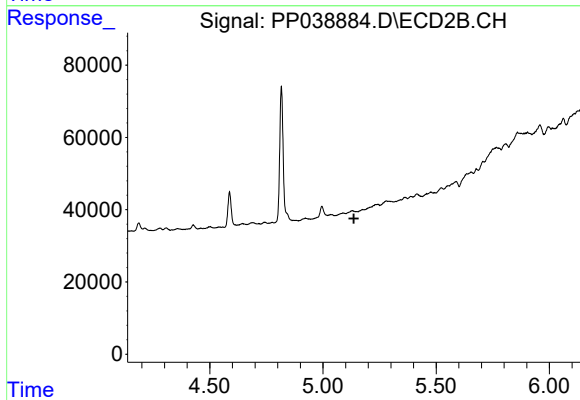


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 5.136 min
Response: 0
Conc: N.D.

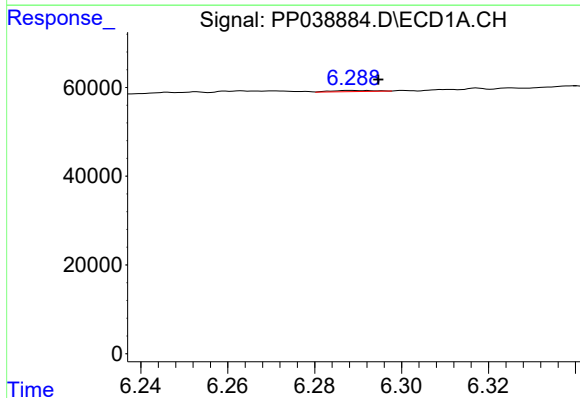


#18 AR-1242-3

R.T.: 6.289 min
Delta R.T.: -0.006 min
Response: 1610
Conc: 1.80 ng/ml

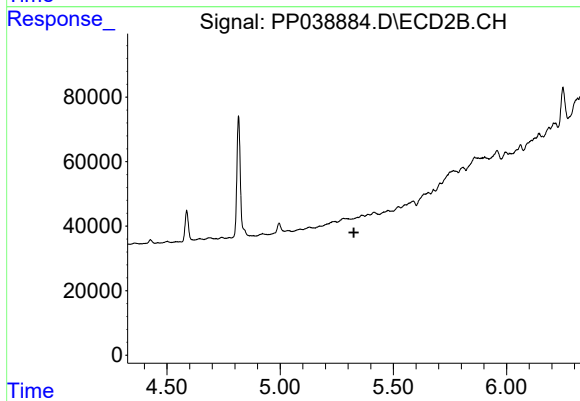

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 5.326 min
Response: 0
Conc: N.D.

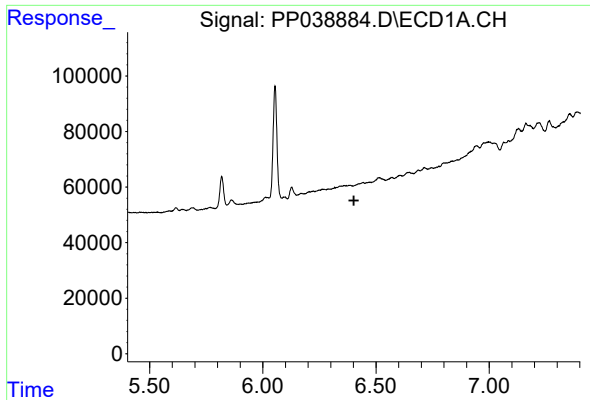

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 6.403 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

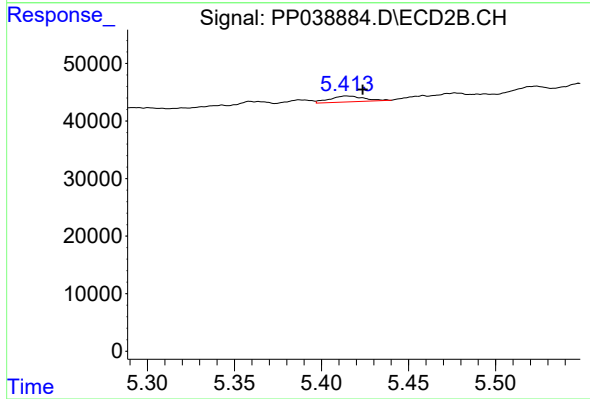


#19 AR-1242-4

R.T.: 5.414 min
Delta R.T.: -0.010 min
Response: 14214
Conc: 29.74 ng/ml

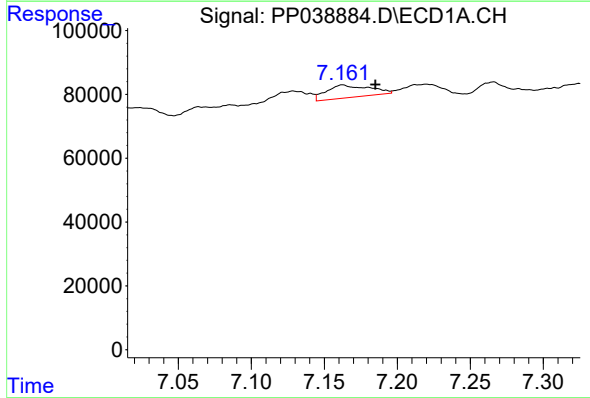


#20 AR-1242-5

R.T.: 7.163 min
Delta R.T.: -0.023 min
Response: 80462
Conc: 112.54 ng/ml

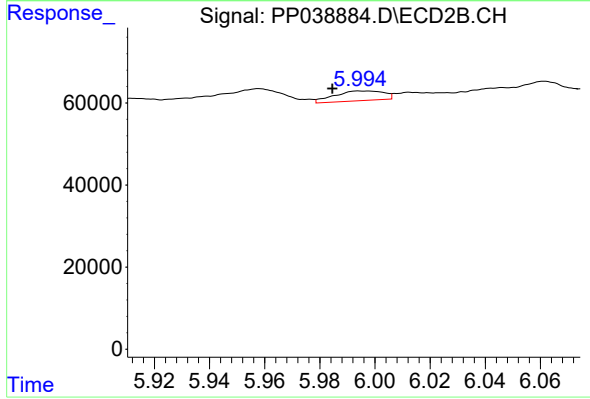

#20 AR-1242-5


R.T.: 5.994 min
Delta R.T.: 0.010 min
Response: 29408
Conc: 47.50 ng/ml

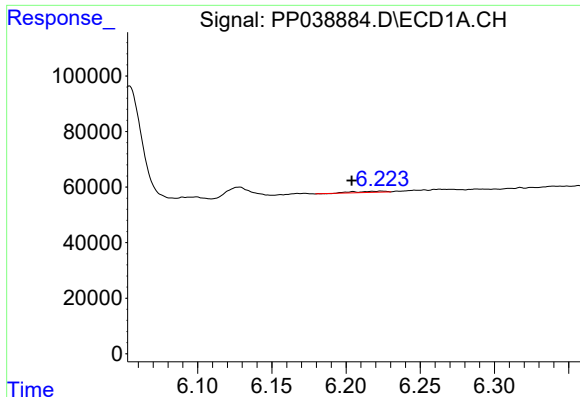

#21 AR-1248-1


R.T.: 6.224 min
Delta R.T.: 0.020 min
Response: 5490
Conc: 6.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

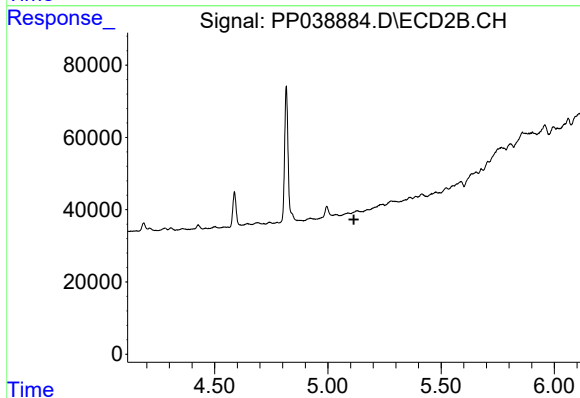


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

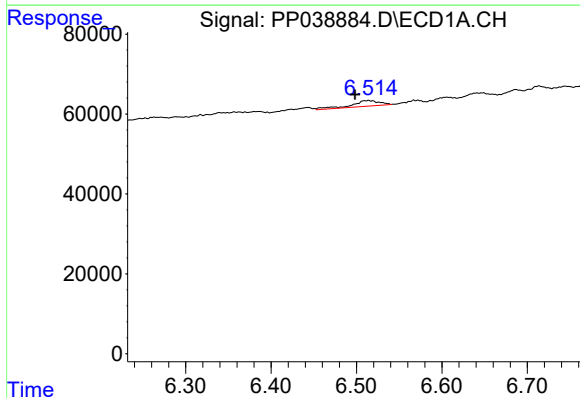


#22 AR-1248-2

R.T.: 6.514 min
Delta R.T.: 0.016 min
Response: 32283
Conc: 32.93 ng/ml

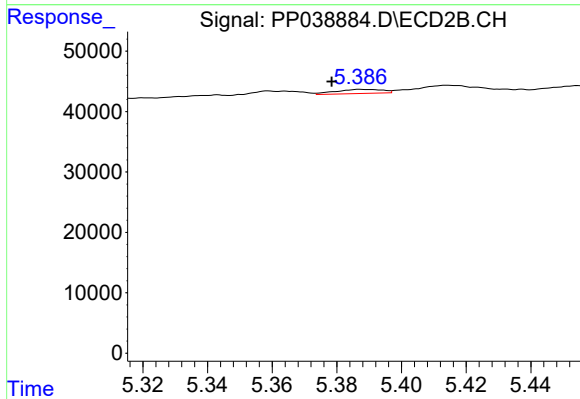

#22 AR-1248-2


R.T.: 5.387 min
Delta R.T.: 0.009 min
Response: 6845
Conc: 9.21 ng/ml

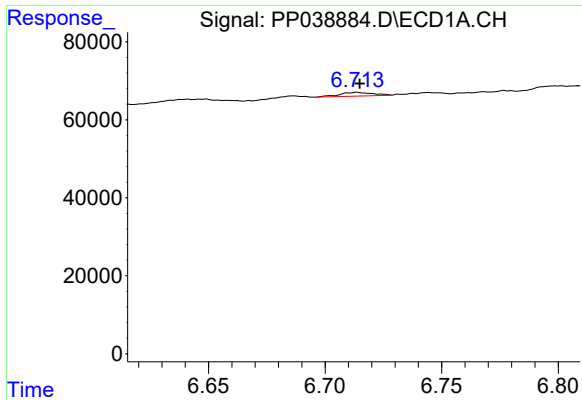

#23 AR-1248-3


R.T.: 6.714 min
Delta R.T.: -0.001 min
Response: 9576
Conc: 8.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

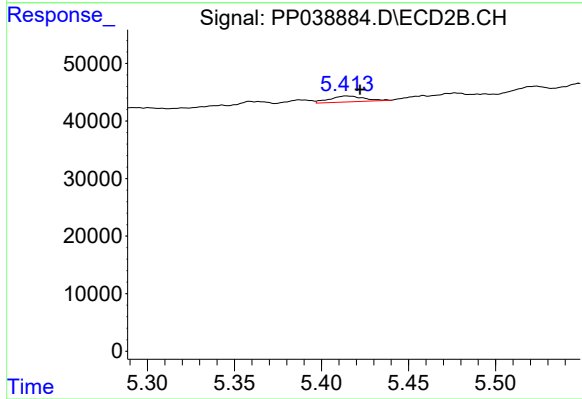


#23 AR-1248-3

R.T.: 5.414 min
Delta R.T.: -0.008 min
Response: 14214
Conc: 18.72 ng/ml

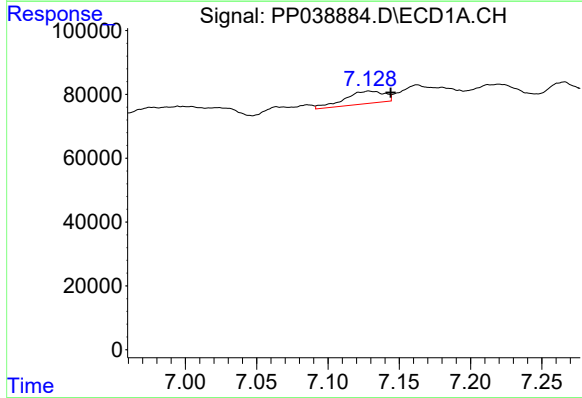


#24 AR-1248-4

R.T.: 7.129 min
Delta R.T.: -0.015 min
Response: 75870
Conc: 61.44 ng/ml

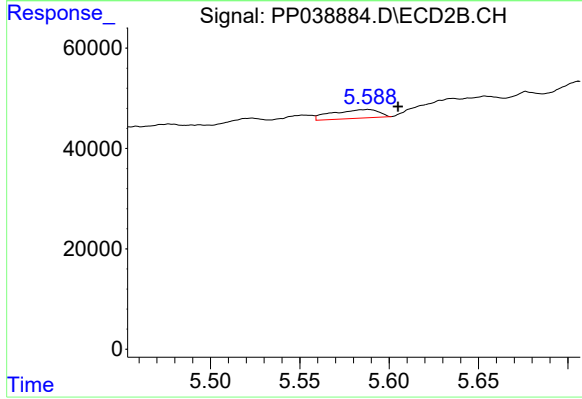

#24 AR-1248-4


R.T.: 5.588 min
Delta R.T.: -0.017 min
Response: 31271
Conc: 33.81 ng/ml

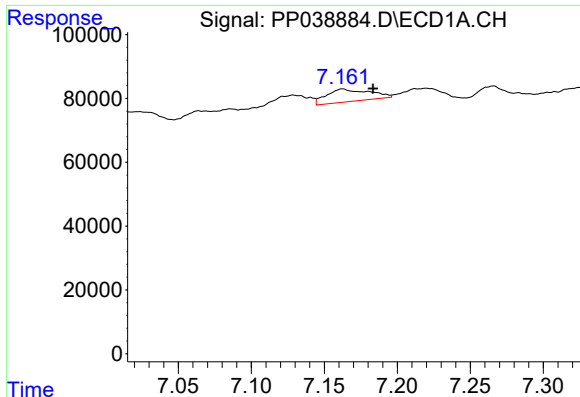

#25 AR-1248-5


R.T.: 7.163 min
Delta R.T.: -0.021 min
Response: 80462
Conc: 65.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

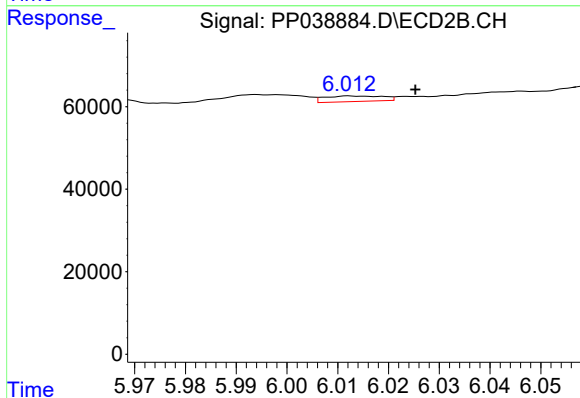


#25 AR-1248-5

R.T.: 6.013 min
Delta R.T.: -0.012 min
Response: 10893
Conc: 12.06 ng/ml

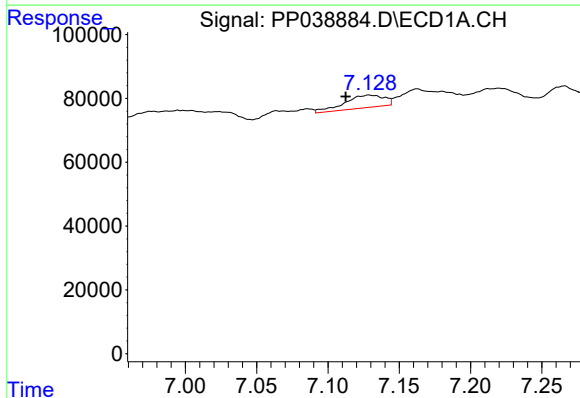


#26 AR-1254-1

R.T.: 7.129 min
Delta R.T.: 0.016 min
Response: 75870
Conc: 66.49 ng/ml

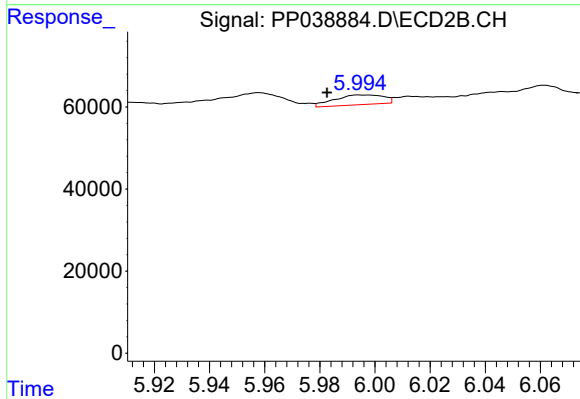

#26 AR-1254-1


R.T.: 5.994 min
Delta R.T.: 0.011 min
Response: 29408
Conc: 22.39 ng/ml

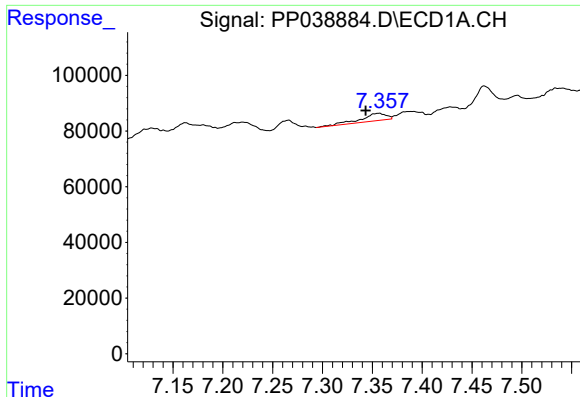

#27 AR-1254-2


R.T.: 7.357 min
Delta R.T.: 0.013 min
Response: 47446
Conc: 27.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

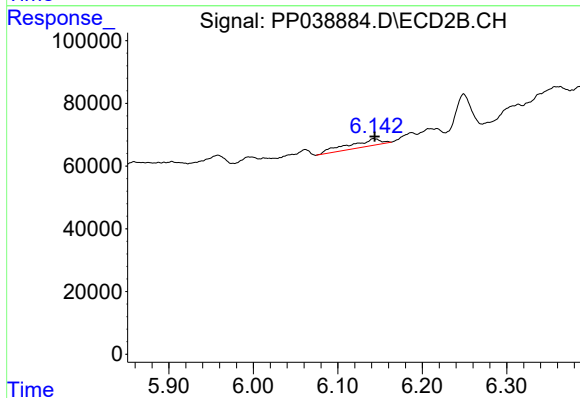


#27 AR-1254-2

R.T.: 6.143 min
Delta R.T.: -0.001 min
Response: 63513
Conc: 55.34 ng/ml

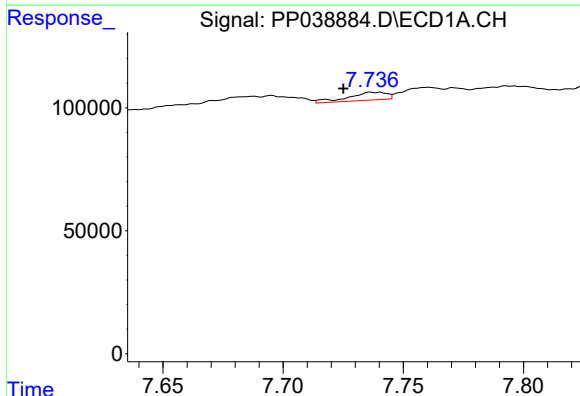


#28 AR-1254-3

R.T.: 7.737 min
Delta R.T.: 0.012 min
Response: 35956
Conc: 20.03 ng/ml

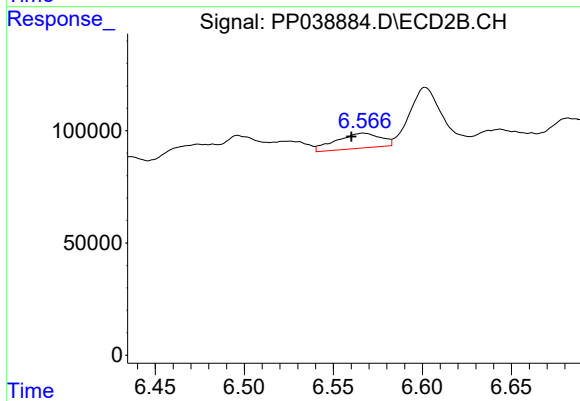

#28 AR-1254-3


R.T.: 6.567 min
Delta R.T.: 0.007 min
Response: 116520
Conc: 62.62 ng/ml

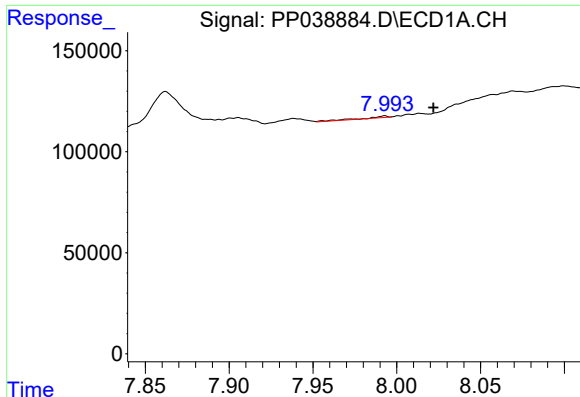

#29 AR-1254-4


R.T.: 7.993 min
Delta R.T.: -0.029 min
Response: 6790
Conc: 5.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

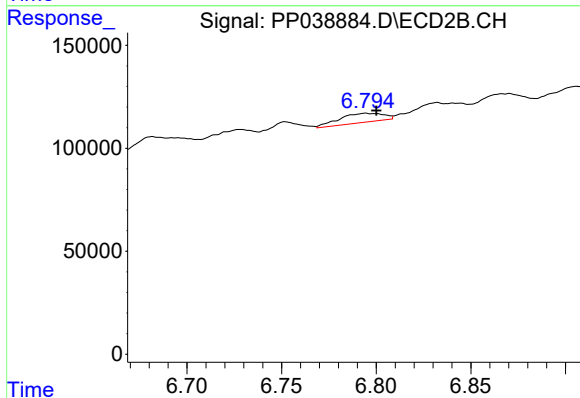


#29 AR-1254-4

R.T.: 6.795 min
Delta R.T.: -0.006 min
Response: 71010
Conc: 60.76 ng/ml

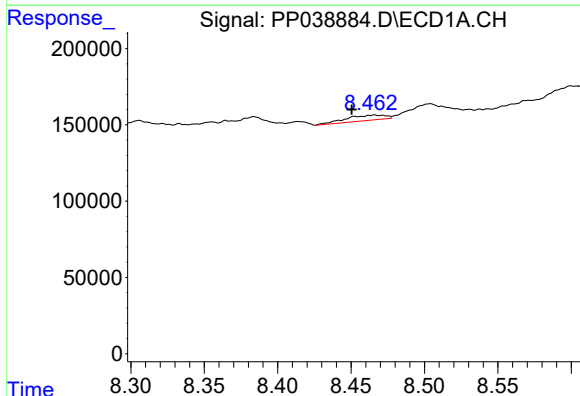


#30 AR-1254-5

R.T.: 8.466 min
Delta R.T.: 0.015 min
Response: 65908
Conc: 53.29 ng/ml

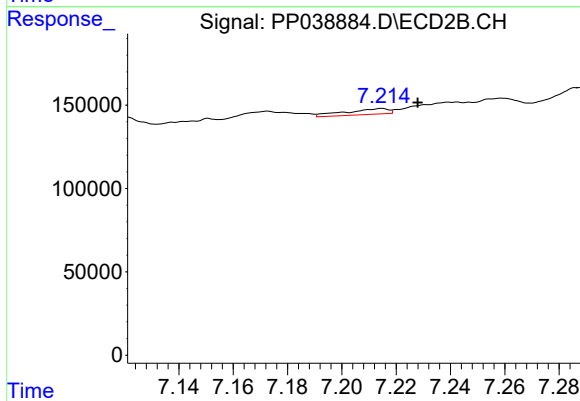

#30 AR-1254-5


R.T.: 7.215 min
Delta R.T.: -0.013 min
Response: 37789
Conc: 23.38 ng/ml

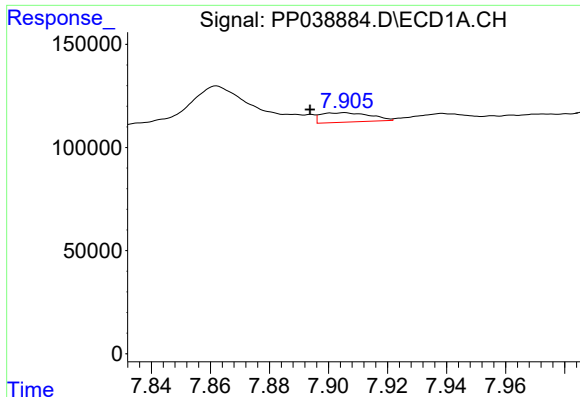

#31 AR-1260-1


R.T.: 7.905 min
Delta R.T.: 0.012 min
Response: 53297
Conc: 44.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

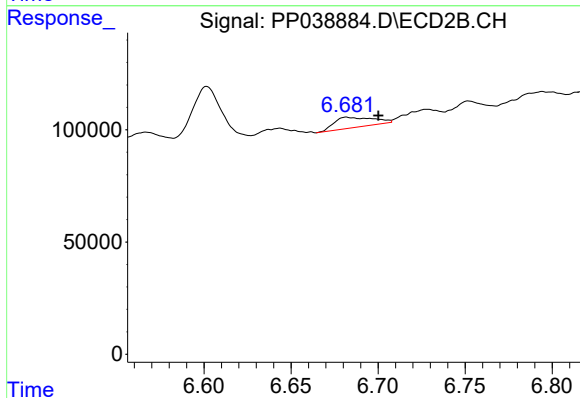


#31 AR-1260-1

R.T.: 6.682 min
Delta R.T.: -0.018 min
Response: 72370
Conc: 61.84 ng/ml

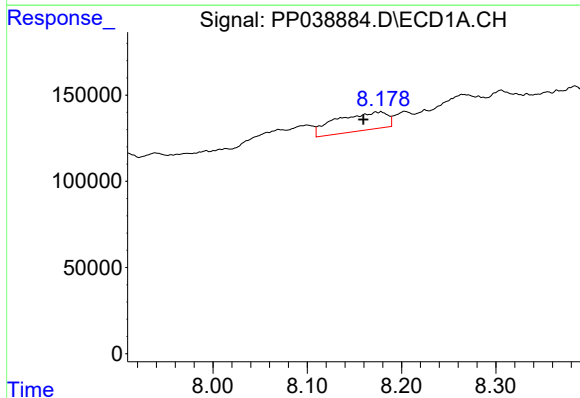


#32 AR-1260-2

R.T.: 8.178 min
Delta R.T.: 0.019 min
Response: 396282
Conc: 270.10 ng/ml

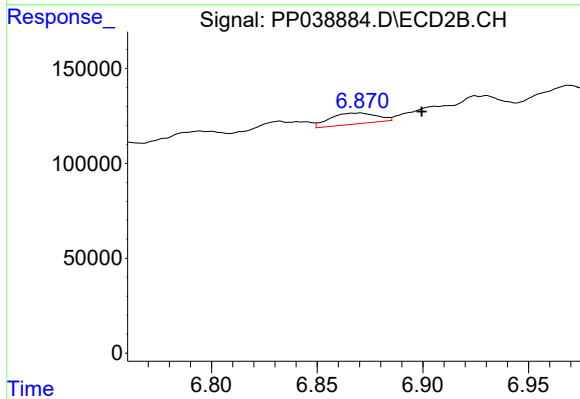

#32 AR-1260-2


R.T.: 6.870 min
Delta R.T.: -0.030 min
Response: 89821
Conc: 63.10 ng/ml

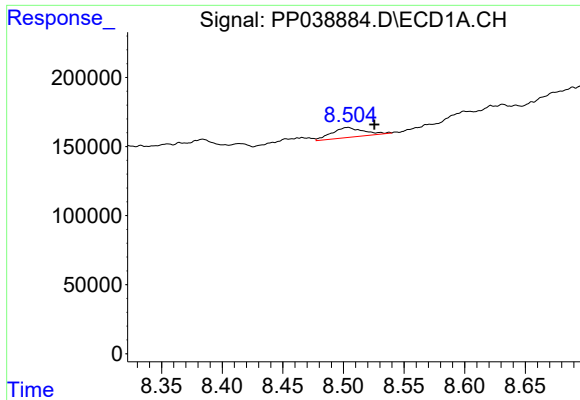

#33 AR-1260-3


R.T.: 8.504 min
Delta R.T.: -0.022 min
Response: 129338
Conc: 134.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

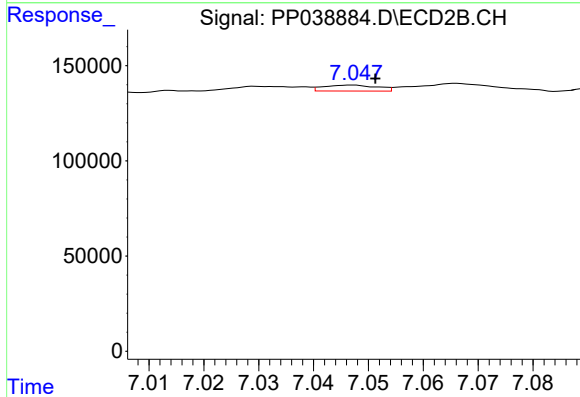


#33 AR-1260-3

R.T.: 7.047 min
Delta R.T.: -0.004 min
Response: 21080
Conc: 14.66 ng/ml

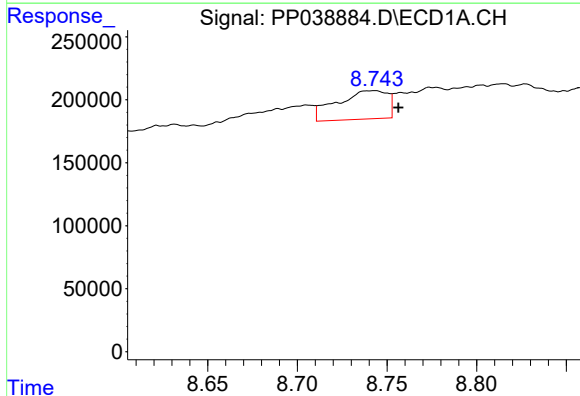


#34 AR-1260-4

R.T.: 8.743 min
Delta R.T.: -0.013 min
Response: 443814
Conc: 390.29 ng/ml

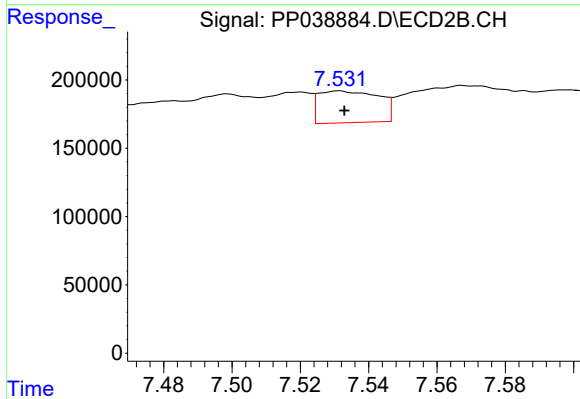

#34 AR-1260-4


R.T.: 7.531 min
Delta R.T.: -0.002 min
Response: 283606
Conc: 252.53 ng/ml

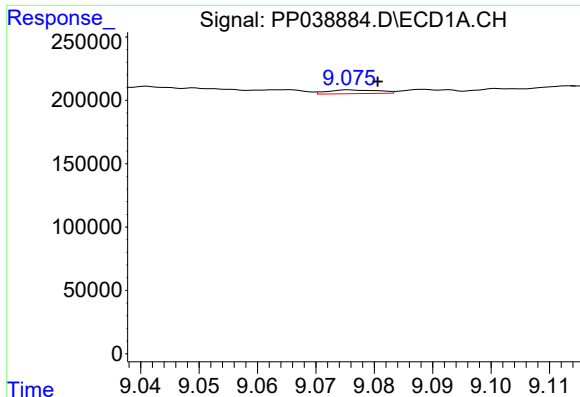

#35 AR-1260-5


R.T.: 9.076 min
Delta R.T.: -0.004 min
Response: 18258
Conc: 8.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

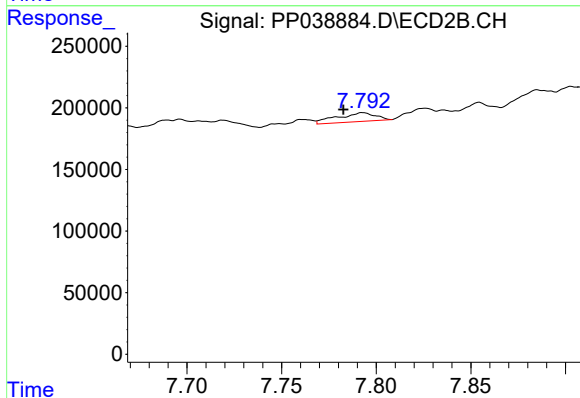


#35 AR-1260-5

R.T.: 7.793 min
Delta R.T.: 0.010 min
Response: 102445
Conc: 37.82 ng/ml

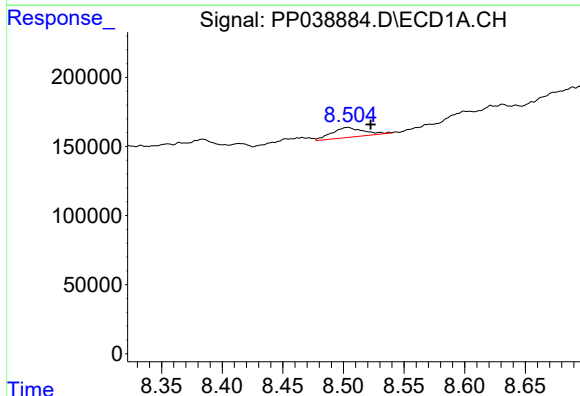


#36 AR-1262-1

R.T.: 8.504 min
Delta R.T.: -0.019 min
Response: 129338
Conc: 87.01 ng/ml

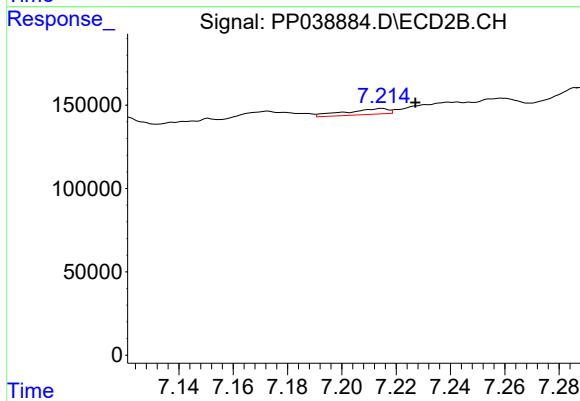

#36 AR-1262-1


R.T.: 7.215 min
Delta R.T.: -0.012 min
Response: 37789
Conc: 41.81 ng/ml

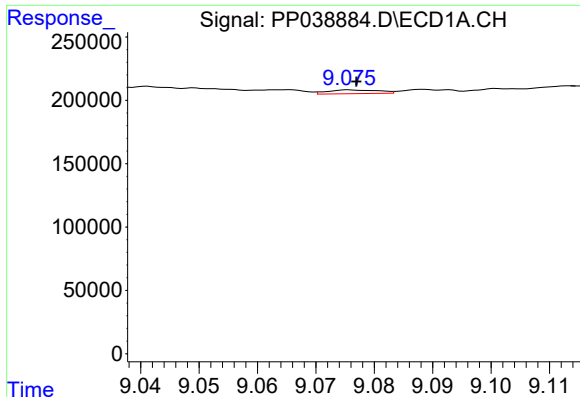

#37 AR-1262-2


R.T.: 9.076 min
Delta R.T.: 0.000 min
Response: 18258
Conc: 6.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

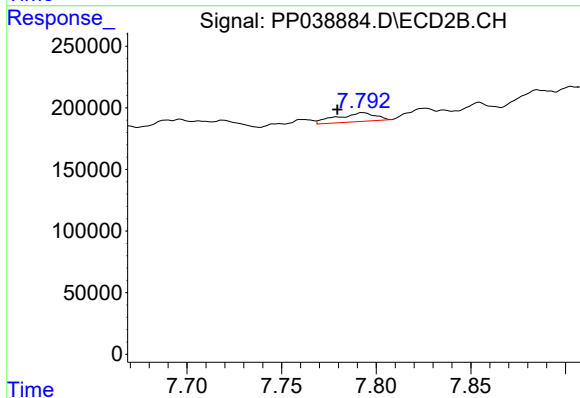


#37 AR-1262-2

R.T.: 7.793 min
Delta R.T.: 0.014 min
Response: 102445
Conc: 33.16 ng/ml

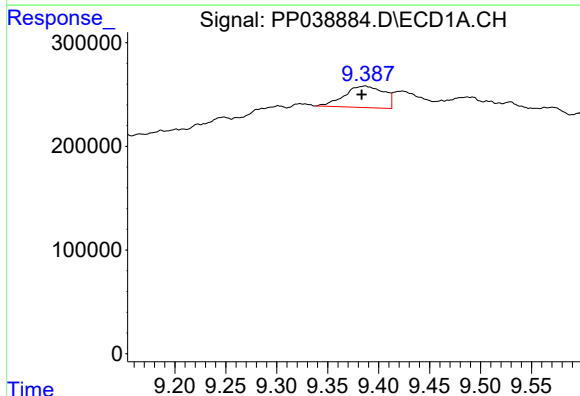


#38 AR-1262-3

R.T.: 9.387 min
Delta R.T.: 0.003 min
Response: 558897
Conc: 469.08 ng/ml

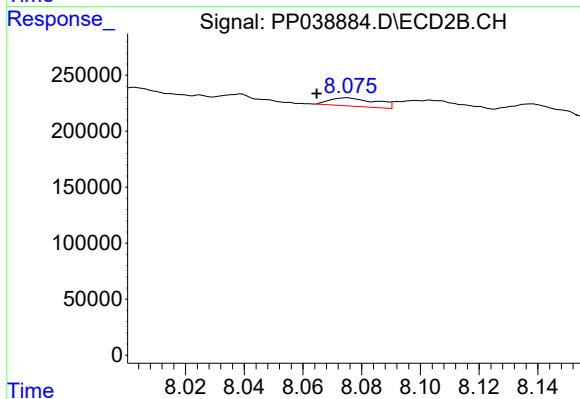

#38 AR-1262-3


R.T.: 8.075 min
Delta R.T.: 0.010 min
Response: 82019
Conc: 65.28 ng/ml

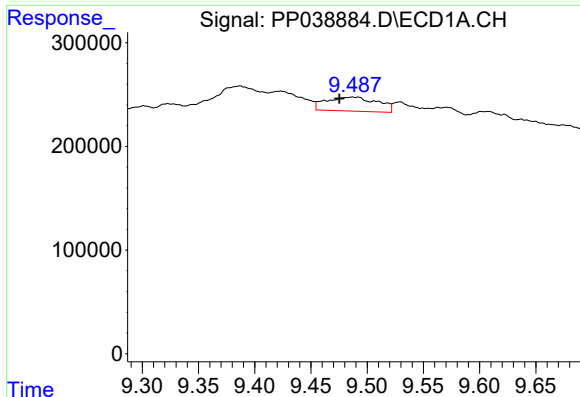

#39 AR-1262-4


R.T.: 9.487 min
Delta R.T.: 0.012 min
Response: 432240
Conc: 536.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

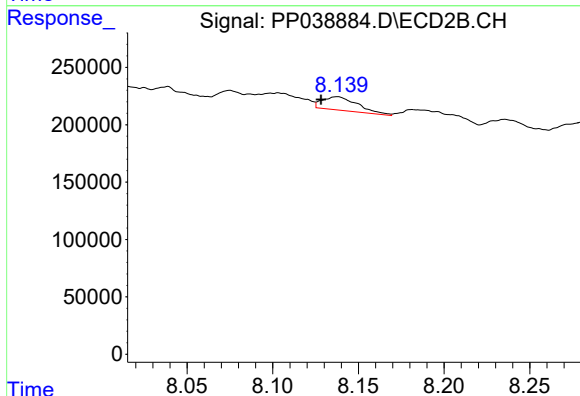


#39 AR-1262-4

R.T.: 8.138 min
Delta R.T.: 0.009 min
Response: 168525
Conc: 71.31 ng/ml

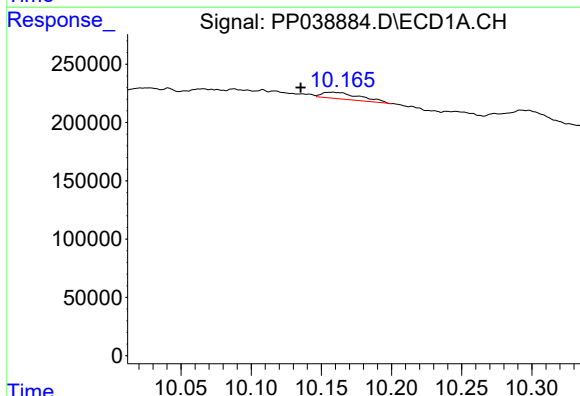


#40 AR-1262-5

R.T.: 10.158 min
Delta R.T.: 0.023 min
Response: 103233
Conc: 96.85 ng/ml

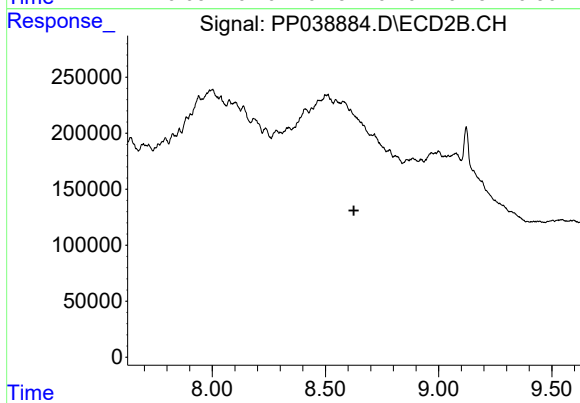

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 8.626 min
Response: 0
Conc: N.D.

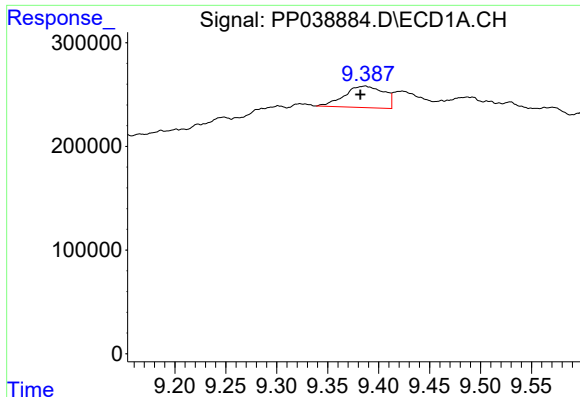

#41 AR-1268-1


R.T.: 9.387 min
Delta R.T.: 0.005 min
Response: 558897
Conc: 174.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

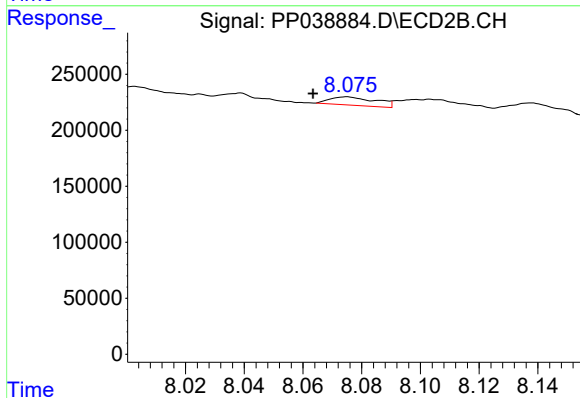


#41 AR-1268-1

R.T.: 8.075 min
Delta R.T.: 0.011 min
Response: 82019
Conc: 22.46 ng/ml

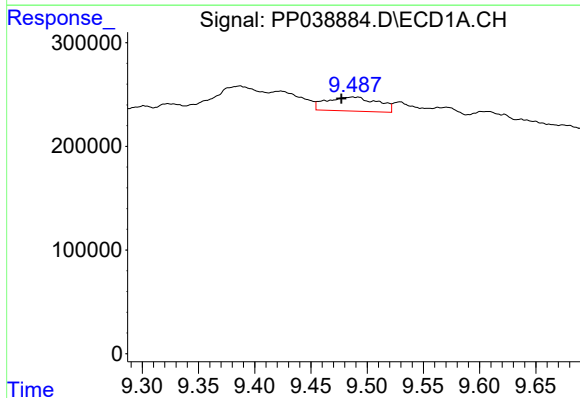


#42 AR-1268-2

R.T.: 9.487 min
Delta R.T.: 0.010 min
Response: 432240
Conc: 140.30 ng/ml

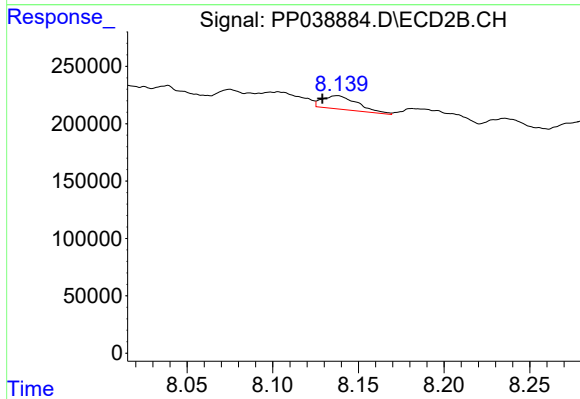

#42 AR-1268-2


R.T.: 8.138 min
Delta R.T.: 0.009 min
Response: 168525
Conc: 48.85 ng/ml

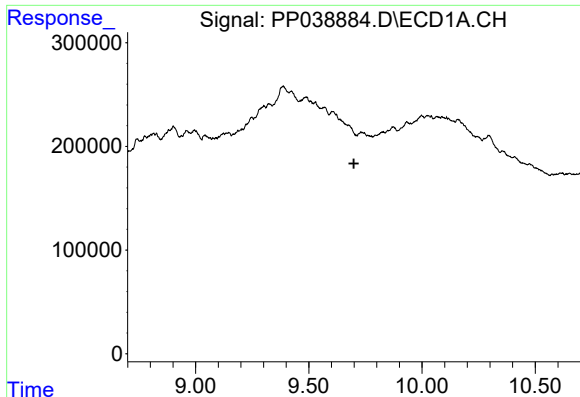

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.699 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

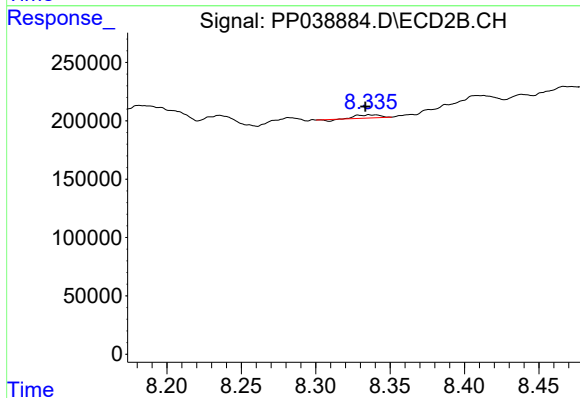


#43 AR-1268-3

R.T.: 8.336 min
Delta R.T.: 0.003 min
Response: 27212
Conc: 9.35 ng/ml

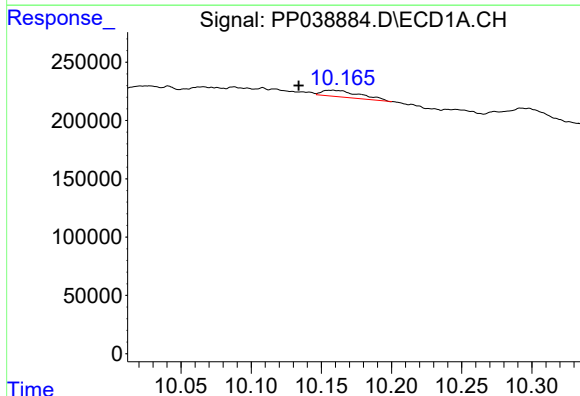


#44 AR-1268-4

R.T.: 10.158 min
Delta R.T.: 0.024 min
Response: 103233
Conc: 84.74 ng/ml

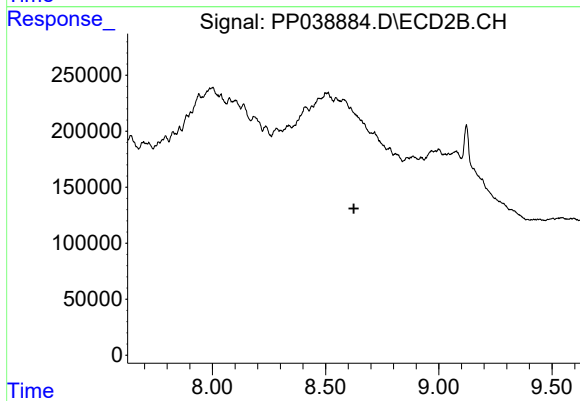

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 8.625 min
Response: 0
Conc: N.D.

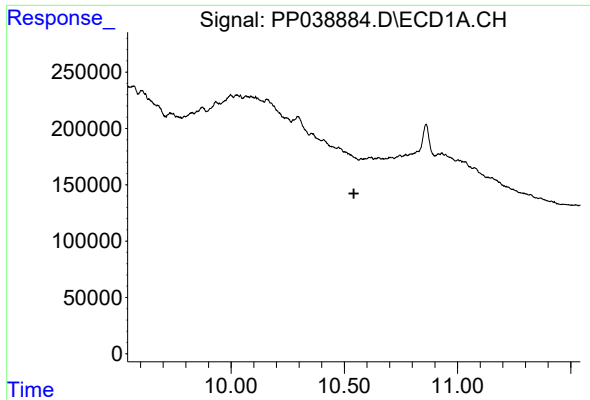

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

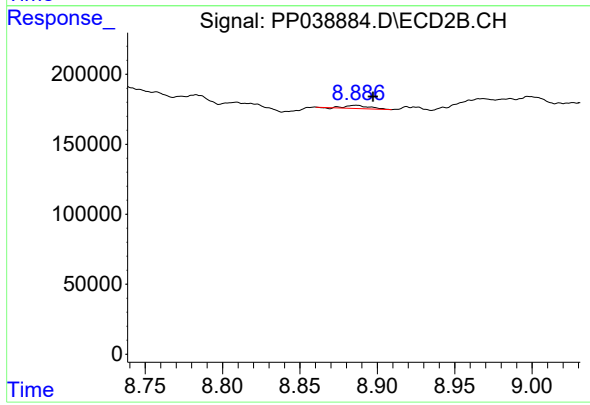

#45 AR-1268-5

R.T.: 8.886 min
Delta R.T.: -0.011 min
Response: 24525
Conc: 2.52 ng/ml