

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082421\
 Data File : PP038884.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Aug 2021 3:28
 Operator : AJ\MA
 Sample : M3508-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BUILDING-5-6-7-GREY-DOOR-CAU

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 09:55:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 18 04:51:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.880	3.866	782117	512054	19.380	21.368
2) SA Decachlor...	10.861	9.122	462517	425414	18.799	17.467

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082421\
Data File : PP038884.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Aug 2021 3:28
Operator : AJ\MA
Sample : M3508-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 09:55:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 18 04:51:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

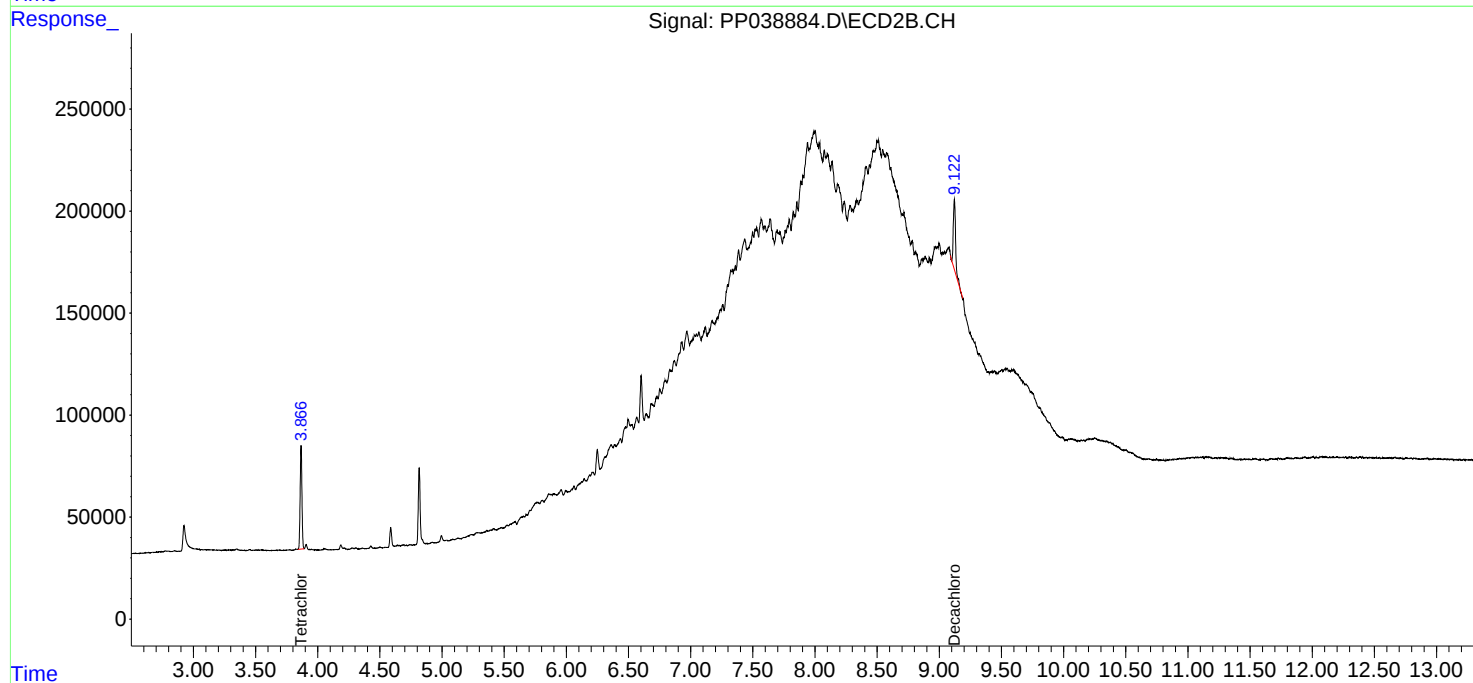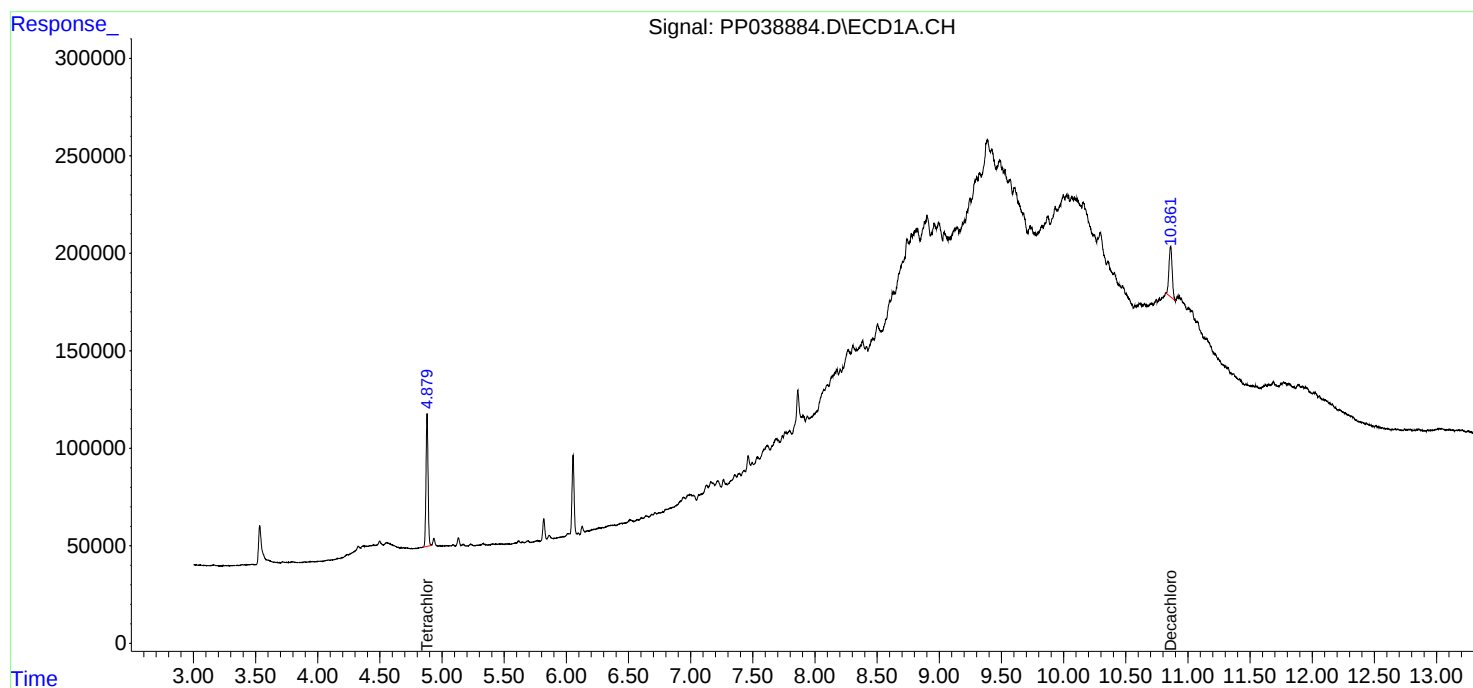


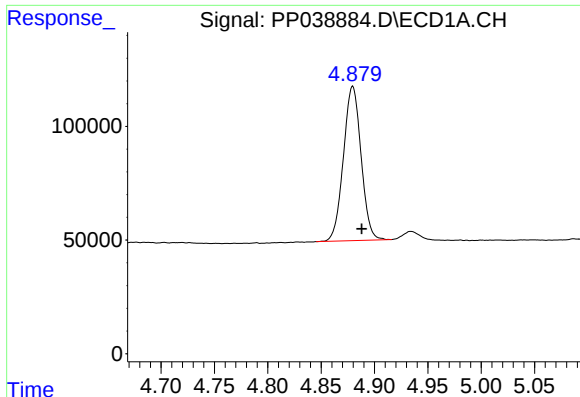

#1 Tetrachloro-m-xylene


R.T.: 4.880 min
Delta R.T.: -0.008 min
Response: 782117
Conc: 19.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUILDING-5-6-7-GREY-DOOR-CAU

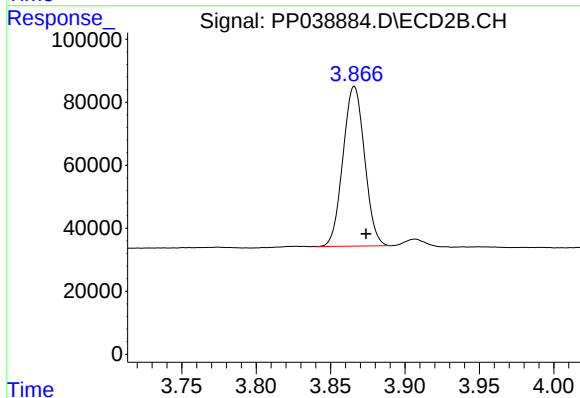


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: -0.008 min
Response: 512054
Conc: 21.37 ng/ml

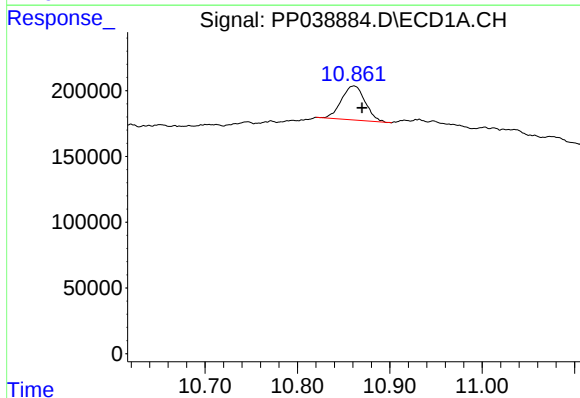

#2 Decachlorobiphenyl

R.T.: 10.861 min
Delta R.T.: -0.009 min
Response: 462517
Conc: 18.80 ng/ml

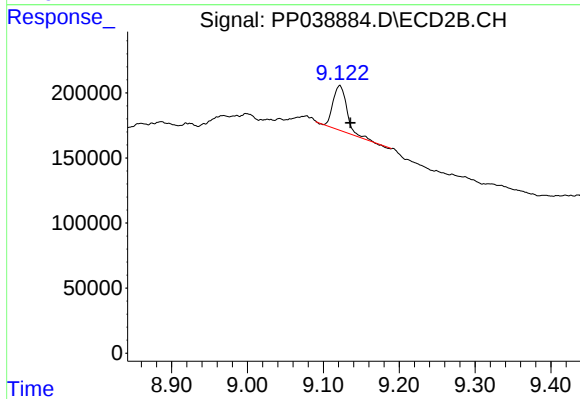

#2 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: -0.014 min
Response: 425414
Conc: 17.47 ng/ml