

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082423\
 Data File : PP059514.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2023 16:01
 Operator : YP\AJ
 Sample : 04147-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-05(46-47)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/25/2023
 Supervised By :mohammad ahmed 08/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 01:27:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 24 01:16:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.432	3.641	19991870	33643794	16.914m	17.414
2) SA Decachlor...	10.216	8.668	12954067	21089167	16.567	15.280

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082423\
Data File : PP059514.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2023 16:01
Operator : YP\AJ
Sample : 04147-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-05(46-47)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/25/2023
Supervised By :mohammad ahmed 08/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 01:27:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082323.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 24 01:16:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

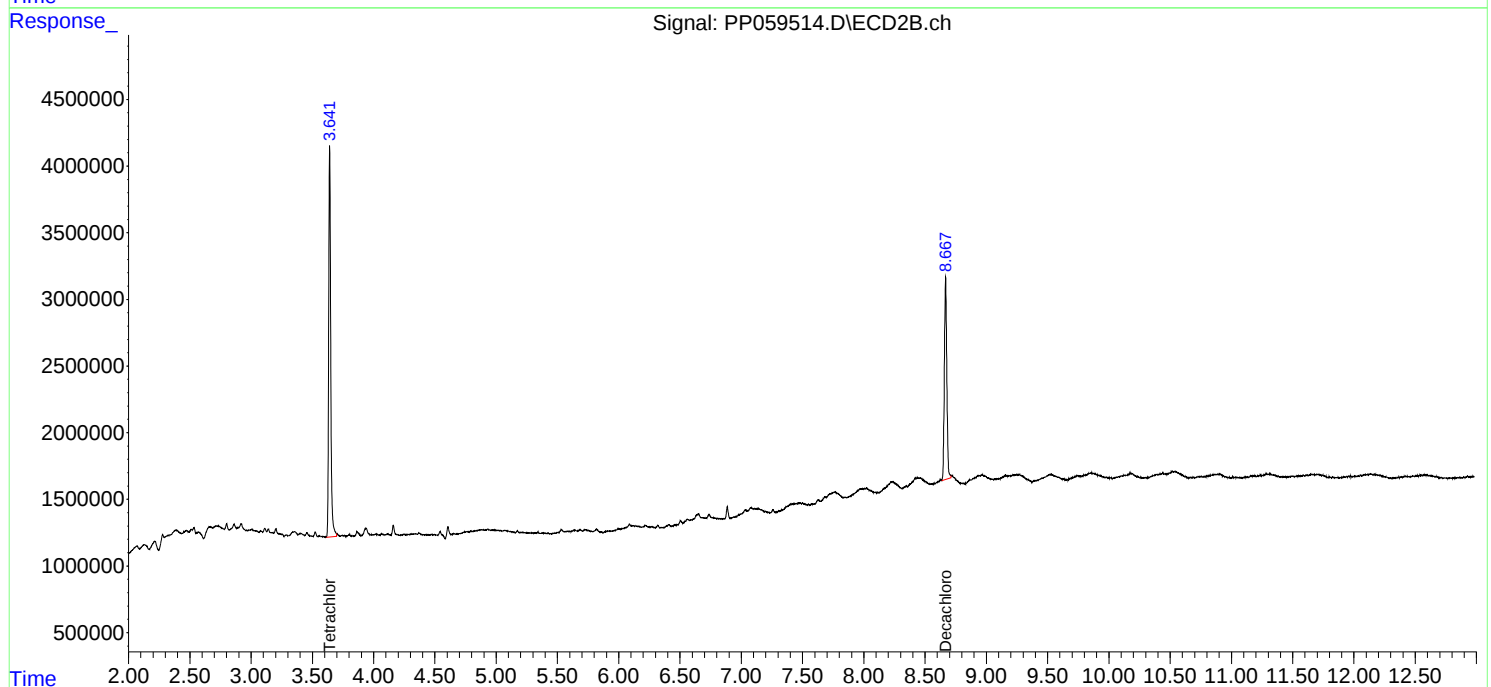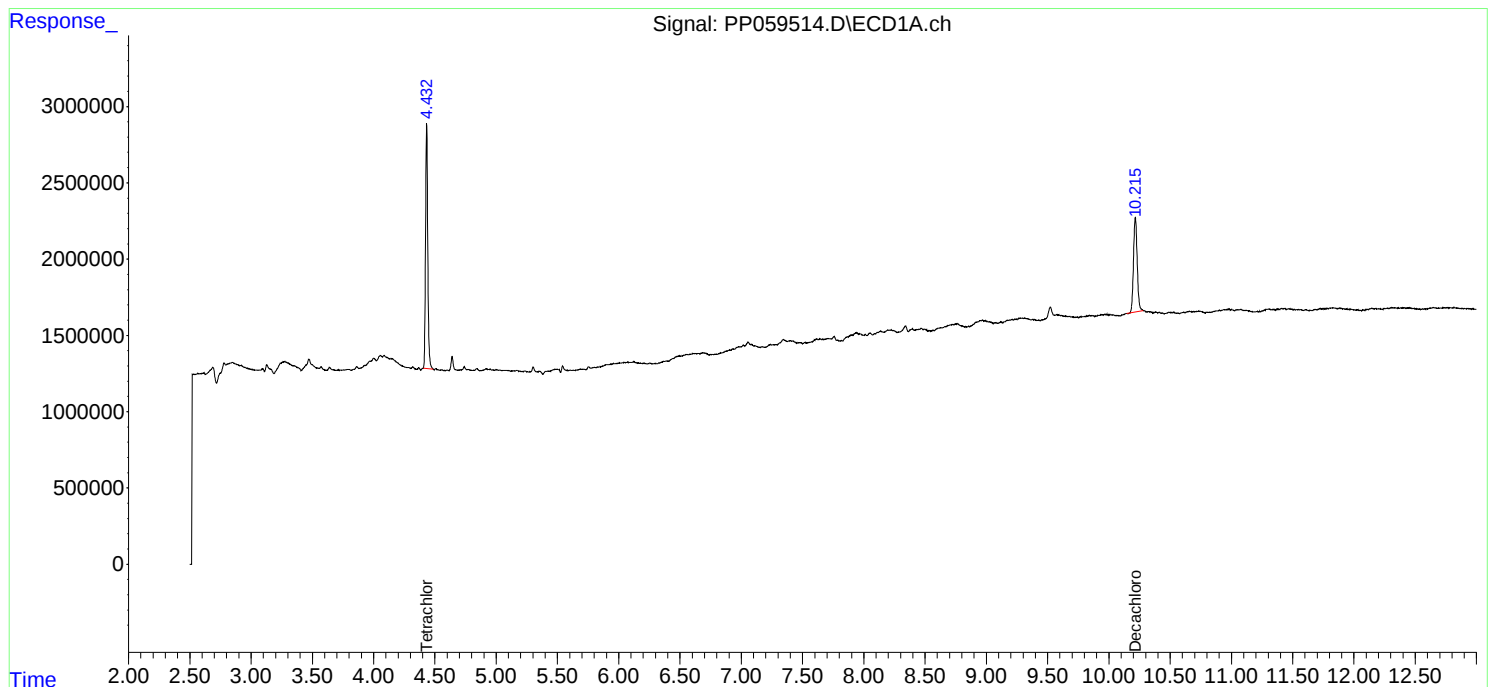

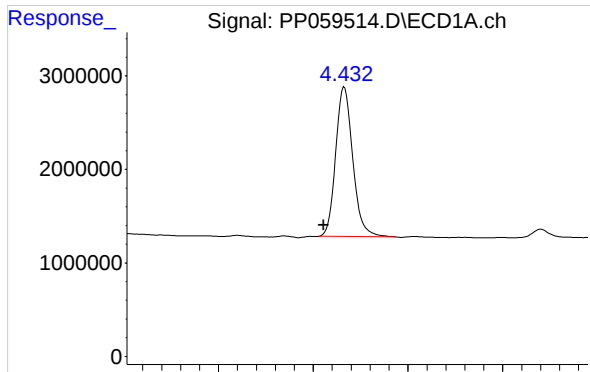

#1 Tetrachloro-m-xylene

R.T.: 4.432 min
Delta R.T.: 0.021 min
Response: 19991870
Conc: 16.91 ng/ml

Instrument :


ECD_P

ClientSampleId :

SB-05(46-47)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/25/2023
Supervised By :mohammad ahmed 08/25/2023

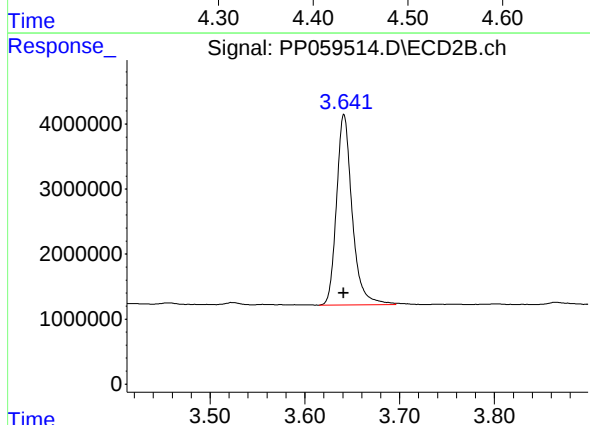


#1 Tetrachloro-m-xylene

R.T.: 3.641 min
Delta R.T.: 0.000 min
Response: 33643794
Conc: 17.41 ng/ml

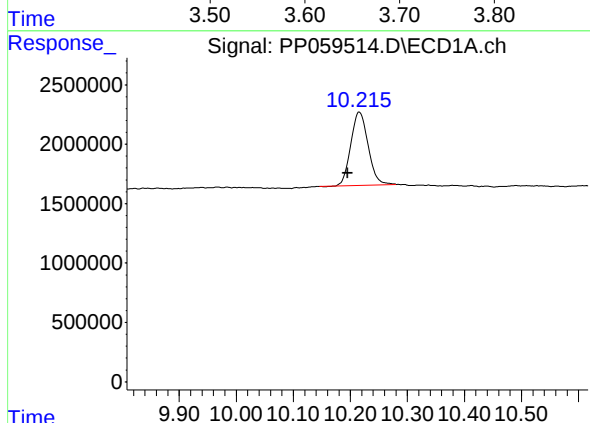

#2 Decachlorobiphenyl

R.T.: 10.216 min
Delta R.T.: 0.021 min
Response: 12954067
Conc: 16.57 ng/ml

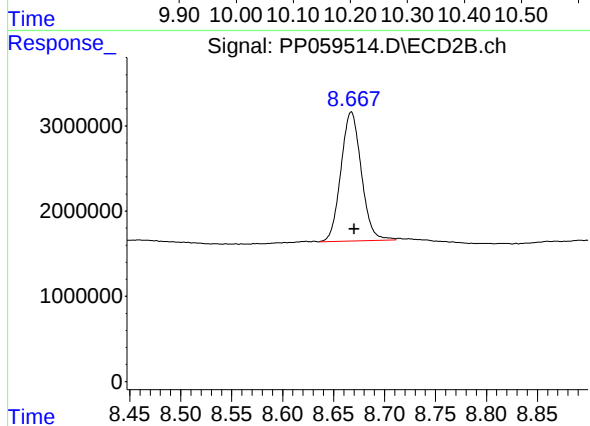

#2 Decachlorobiphenyl

R.T.: 8.668 min
Delta R.T.: -0.003 min
Response: 21089167
Conc: 15.28 ng/ml