

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082423\
 Data File : PP059528.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Aug 2023 00:23
 Operator : YP\AJ
 Sample : 04147-04
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-04(21.5-23)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/25/2023
 Supervised By :mohammad ahmed 08/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 01:31:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 24 01:16:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.411	3.641	13697983	21069135	11.589m	10.906m
2) SA Decachlor...	10.194	8.665	12408351	16293519	15.869	11.805 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082423\
Data File : PP059528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Aug 2023 00:23
Operator : YP\AJ
Sample : 04147-04
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-04(21.5-23)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/25/2023
Supervised By :mohammad ahmed 08/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 01:31:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082323.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 24 01:16:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

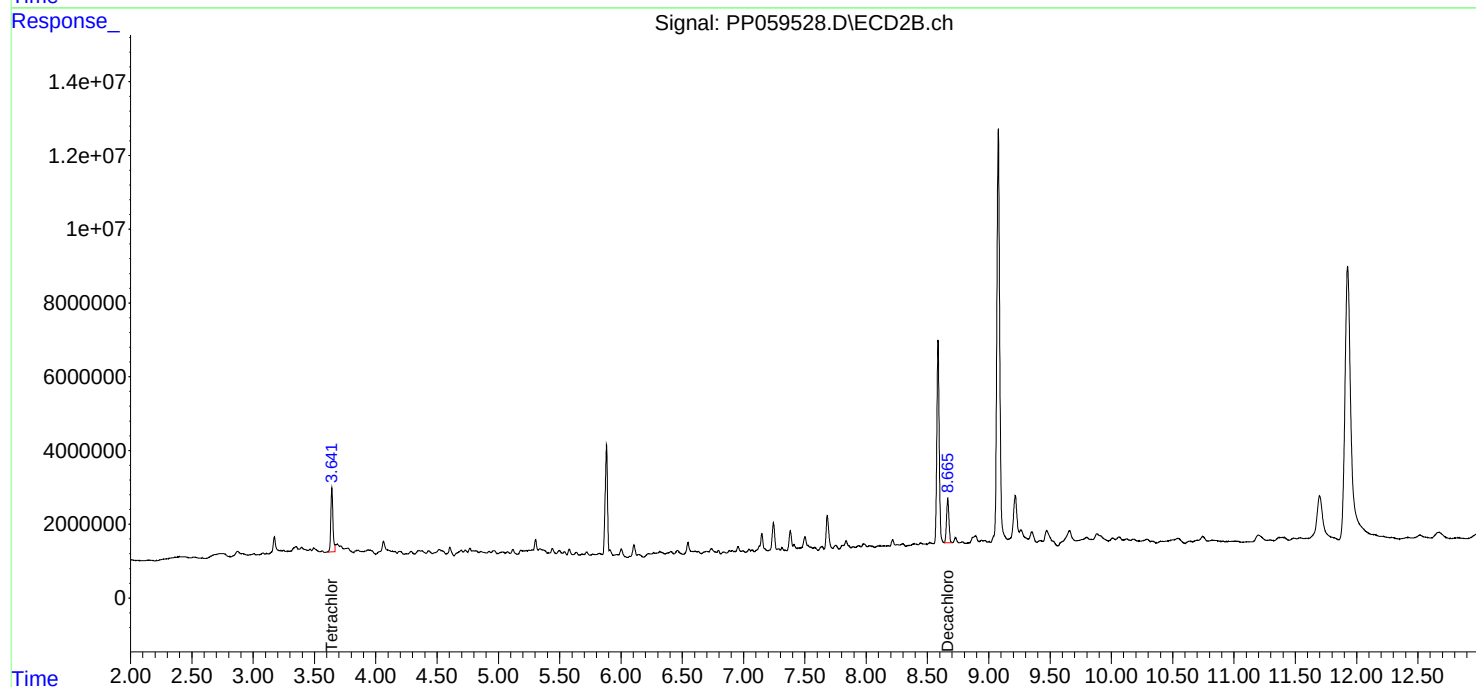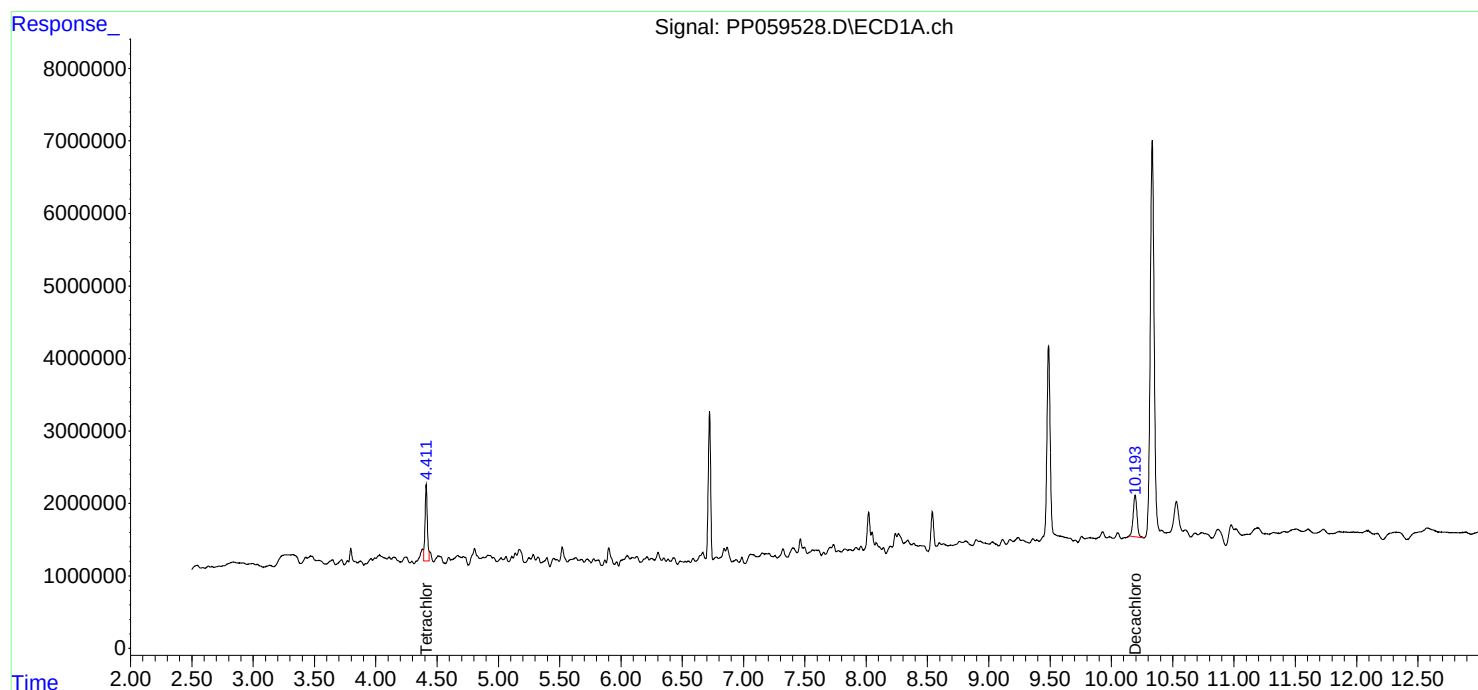

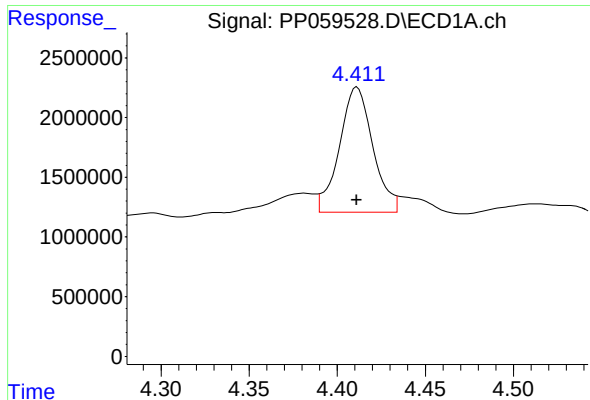


#1 Tetrachloro-m-xylene

R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 13697983
Conc: 11.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-04(21.5-23)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/25/2023
Supervised By :mohammad ahmed 08/25/2023

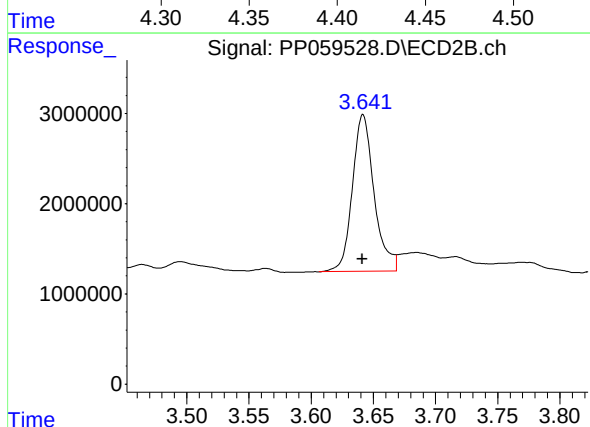


#1 Tetrachloro-m-xylene

R.T.: 3.641 min
Delta R.T.: 0.000 min
Response: 21069135
Conc: 10.91 ng/ml

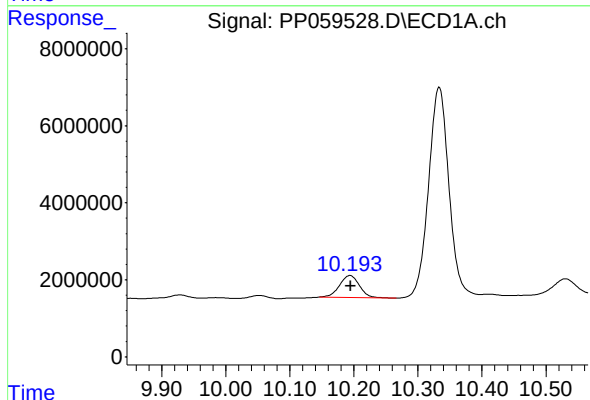

#2 Decachlorobiphenyl

R.T.: 10.194 min
Delta R.T.: -0.001 min
Response: 12408351
Conc: 15.87 ng/ml

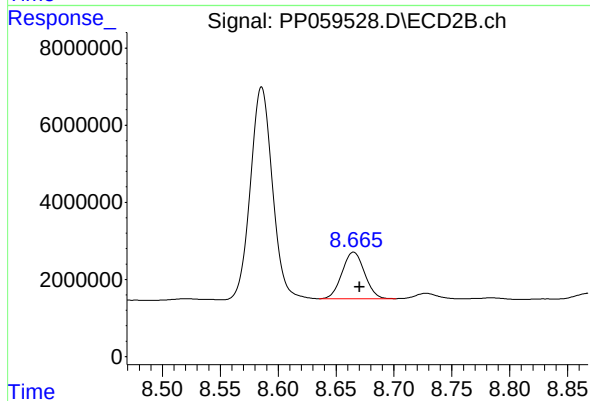

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: -0.005 min
Response: 16293519
Conc: 11.81 ng/ml