

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082621\
 Data File : PP038955.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Aug 2021 15:31
 Operator : AJ\MA
 Sample : M3542-01 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JEB882V-END-1-1

Manual Integrations
 APPROVED

mohammad
 8/27/2021 5:00:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 02:11:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 26 09:31:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.875	3.861	55704	33985	1.459	1.410m
2) SA Decachlor...	10.856	9.118	44407	41069	1.844	1.816

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082621\
Data File : PP038955.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Aug 2021 15:31
Operator : AJ\MA
Sample : M3542-01 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
JEB882V-END-1-1


Manual Integrations
APPROVED

mohammad
8/27/2021 5:00:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 02:11:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 26 09:31:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

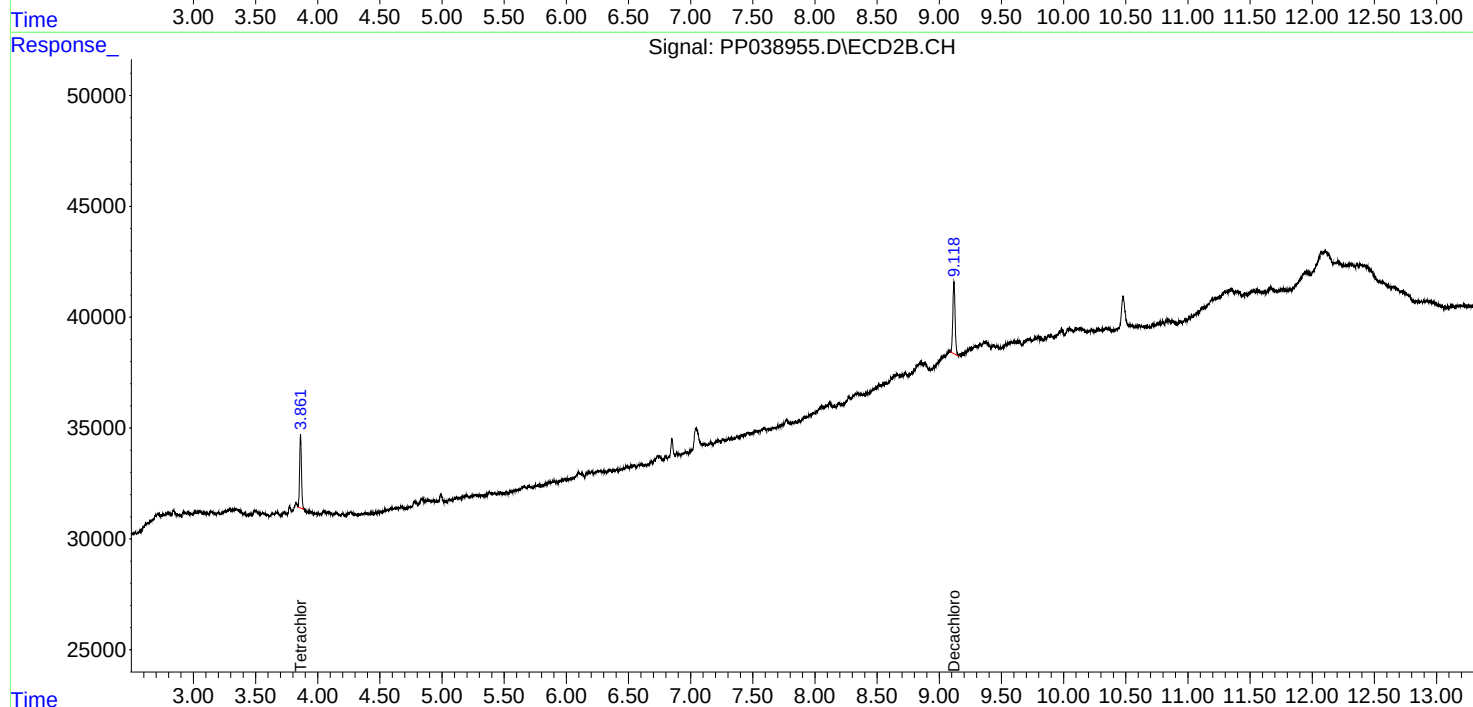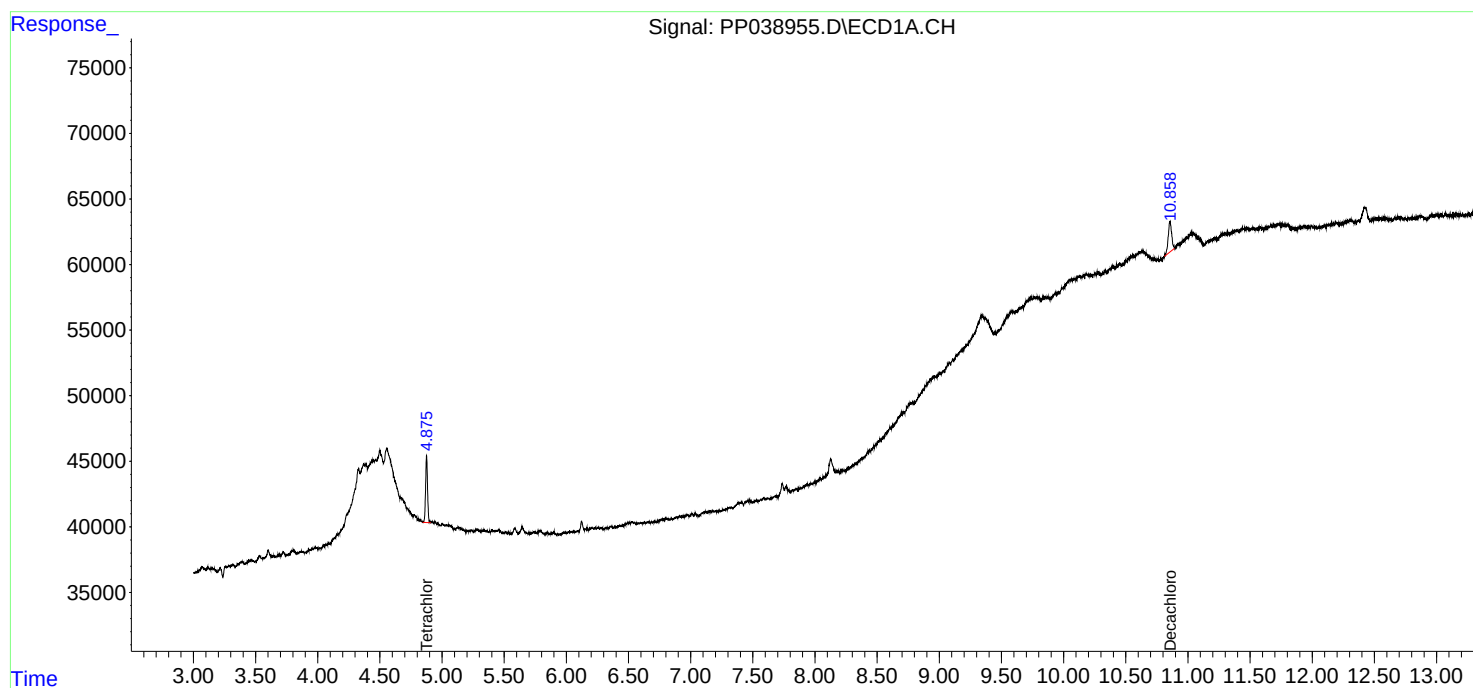

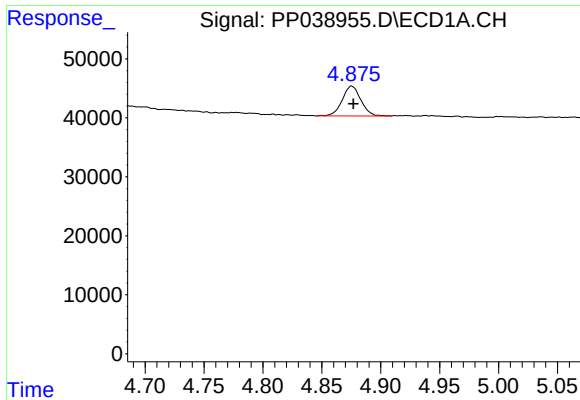


#1 Tetrachloro-m-xylene

R.T.: 4.875 min
Delta R.T.: -0.002 min
Response: 55704
Conc: 1.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
JEB882V-END-1-1


Manual Integrations
APPROVED

mohammad
8/27/2021 5:00:35 PM

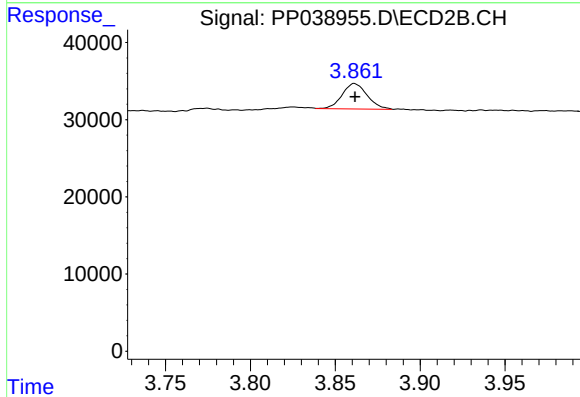


#1 Tetrachloro-m-xylene

R.T.: 3.861 min
Delta R.T.: 0.000 min
Response: 33985
Conc: 1.41 ng/ml m

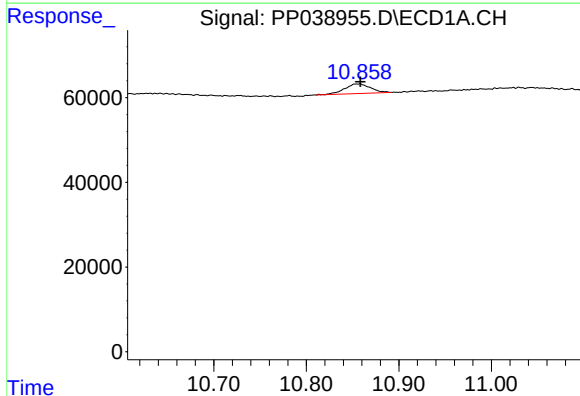

#2 Decachlorobiphenyl

R.T.: 10.856 min
Delta R.T.: -0.003 min
Response: 44407
Conc: 1.84 ng/ml

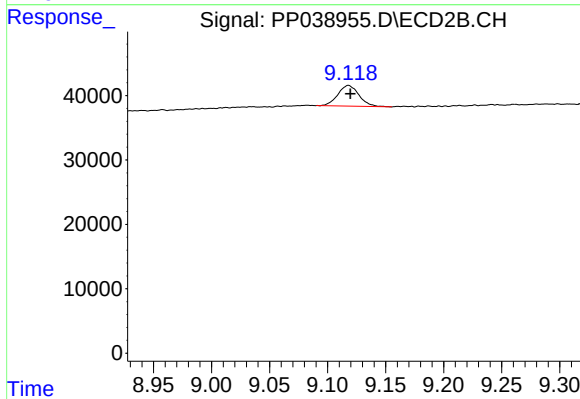

#2 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: -0.002 min
Response: 41069
Conc: 1.82 ng/ml