

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082721\
 Data File : PP038997.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Aug 2021 15:24
 Operator : AJ\MA
 Sample : M3558-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TPR-14-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 04:08:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 26 09:31:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.876	3.862	742382	492151	19.449	20.422
2)	SA Decachlor...	10.855	9.117	365598	374137	15.184	16.546
Target Compounds							
8)	L2 AR-1221-1	5.130	0.000	26424	0	58.665	N.D. #
9)	L2 AR-1221-2	5.225	0.000	11230	0	33.712	N.D. #
27)	L6 AR-1254-2	7.328	0.000	30216	0	19.958	N.D. #
28)	L6 AR-1254-3	7.711	0.000	143494	0	93.136	N.D. #
30)	L6 AR-1254-5	8.424f	0.000	18892	0	16.734	N.D. #
31)	L7 AR-1260-1	7.886	0.000	85062	0	89.239	N.D. #
33)	L7 AR-1260-3	0.000	7.045	0	18436	N.D.	13.341 #
34)	L7 AR-1260-4	8.750	0.000	3573	0	3.530	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082721\
Data File : PP038997.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Aug 2021 15:24
Operator : AJ\MA
Sample : M3558-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TPR-14-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 04:08:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 26 09:31:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

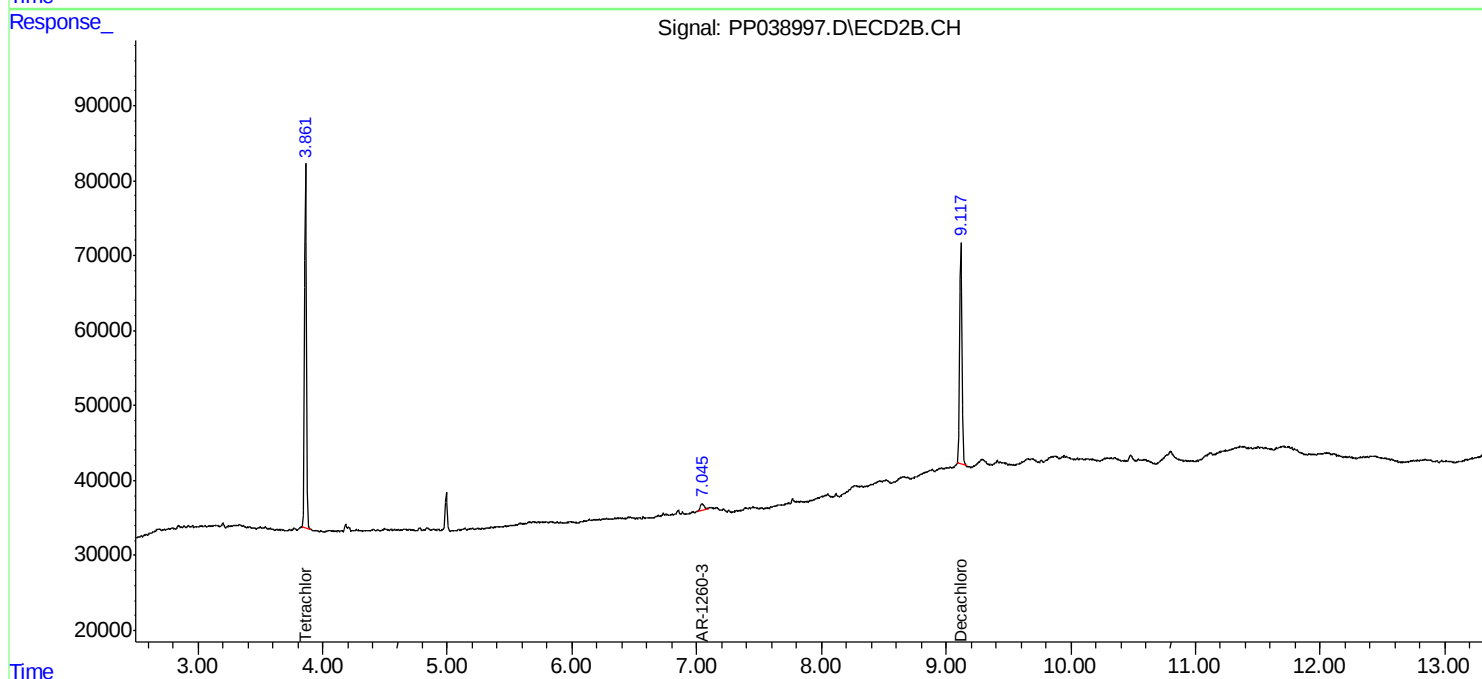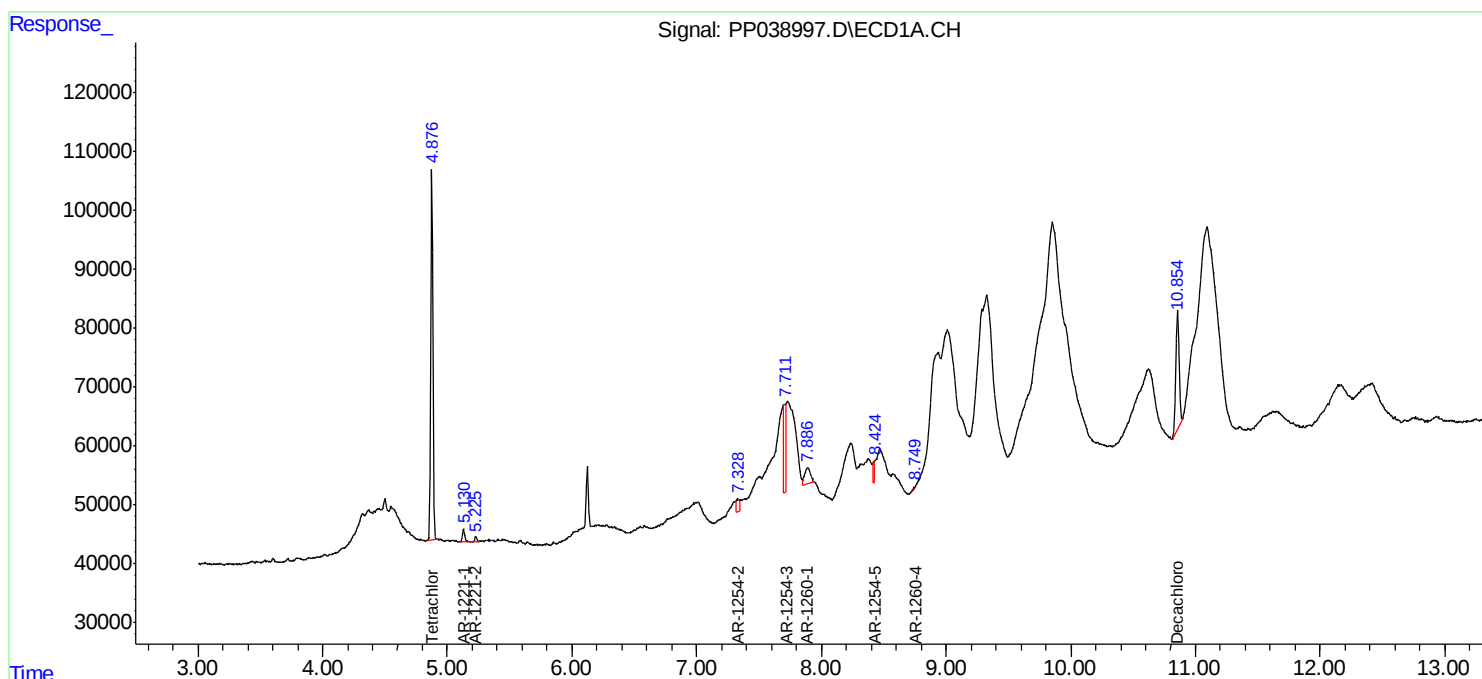


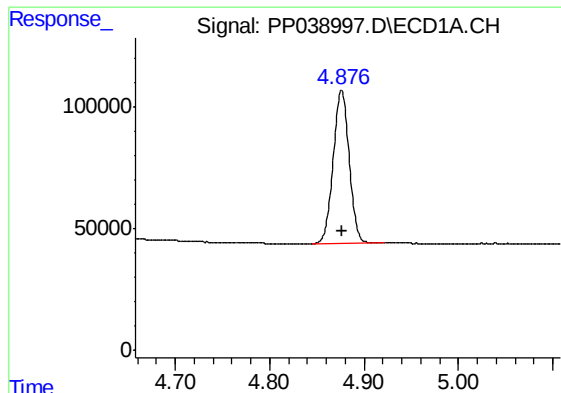

#1 Tetrachloro-m-xylene


R.T.: 4.876 min
Delta R.T.: 0.000 min
Response: 742382
Conc: 19.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
TPR-14-COMP

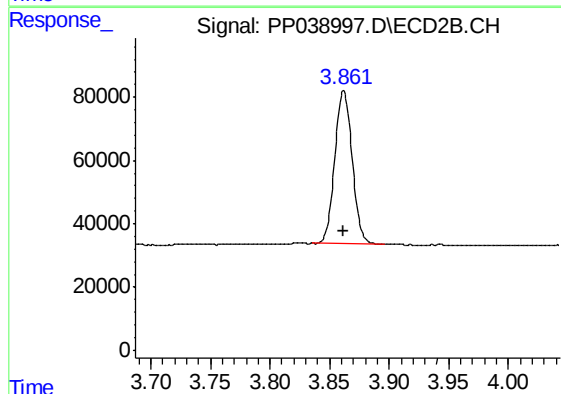


#1 Tetrachloro-m-xylene

R.T.: 3.862 min
Delta R.T.: 0.000 min
Response: 492151
Conc: 20.42 ng/ml

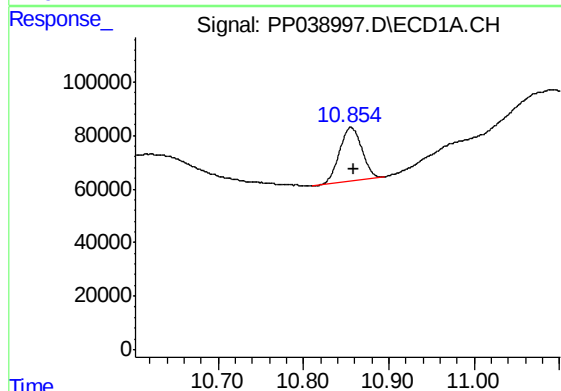


#2 Decachlorobiphenyl

R.T.: 10.855 min
Delta R.T.: -0.003 min
Response: 365598
Conc: 15.18 ng/ml

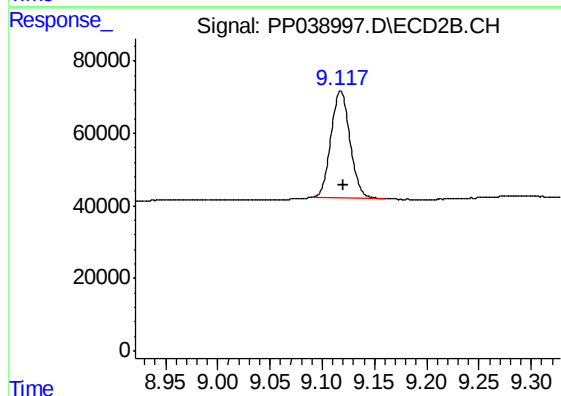

#2 Decachlorobiphenyl


R.T.: 9.117 min
Delta R.T.: -0.002 min
Response: 374137
Conc: 16.55 ng/ml

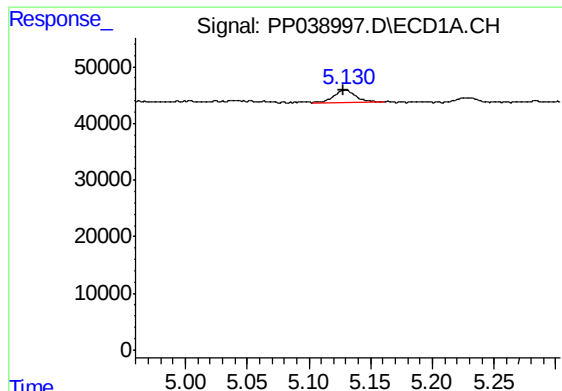

#8 AR-1221-1


R.T.: 5.130 min
Delta R.T.: 0.002 min
Response: 26424
Conc: 58.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
TPR-14-COMP

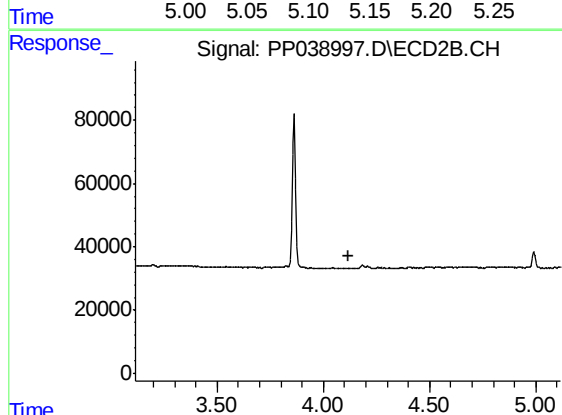


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.116 min
Response: 0
Conc: N.D.

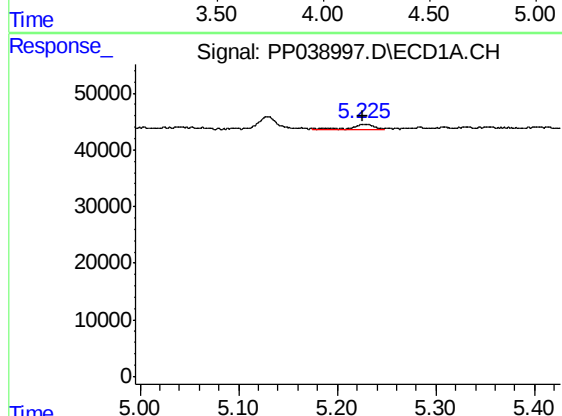


#9 AR-1221-2

R.T.: 5.225 min
Delta R.T.: 0.000 min
Response: 11230
Conc: 33.71 ng/ml

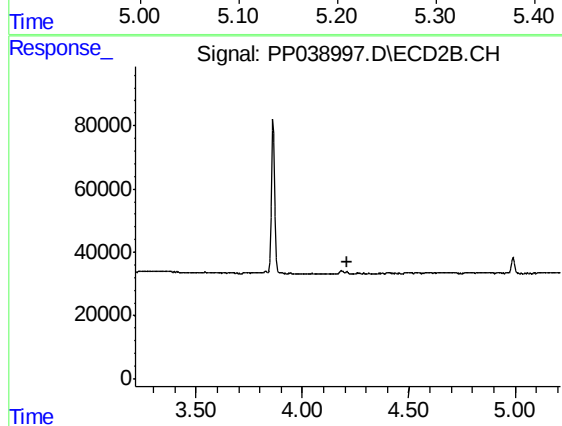

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.214 min
Response: 0
Conc: N.D.

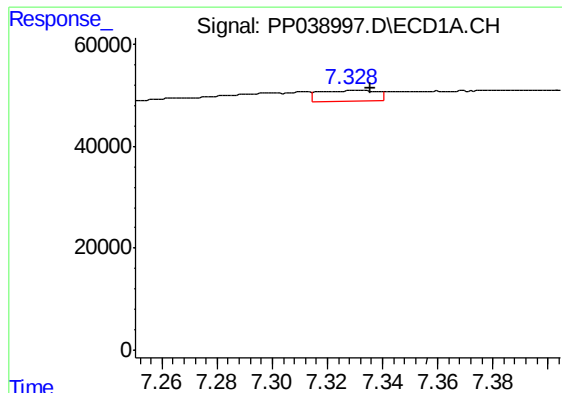

#27 AR-1254-2


R.T.: 7.328 min
Delta R.T.: -0.007 min
Response: 30216
Conc: 19.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
TPR-14-COMP

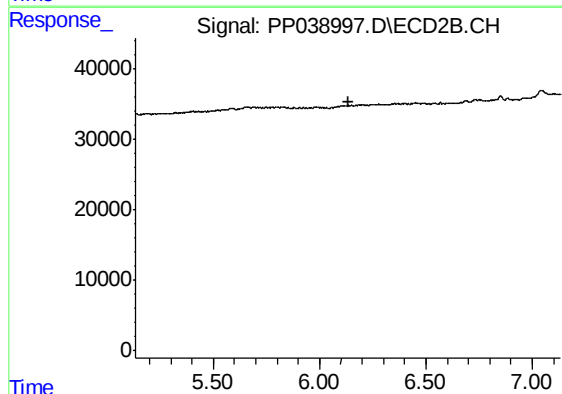


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.134 min
Response: 0
Conc: N.D.

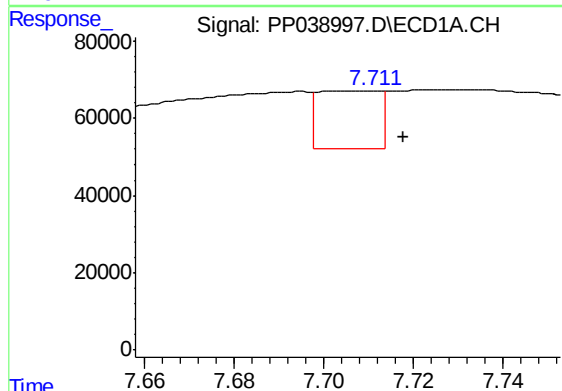


#28 AR-1254-3

R.T.: 7.711 min
Delta R.T.: -0.007 min
Response: 143494
Conc: 93.14 ng/ml

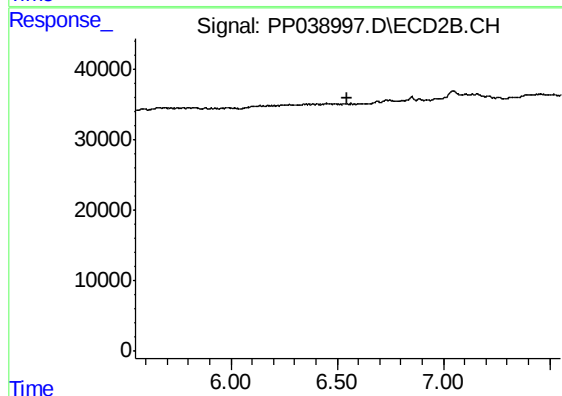

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.551 min
Response: 0
Conc: N.D.

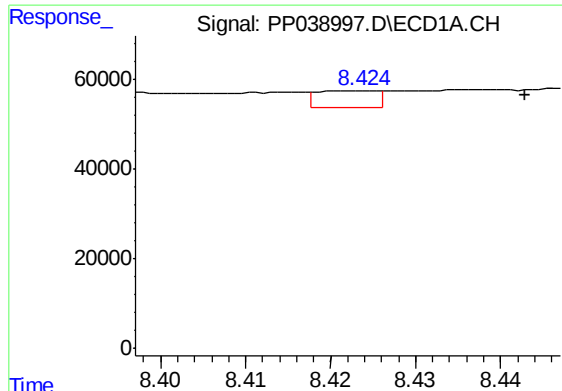

#30 AR-1254-5


R.T.: 8.424 min
Delta R.T.: -0.019 min
Response: 18892
Conc: 16.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
TPR-14-COMP

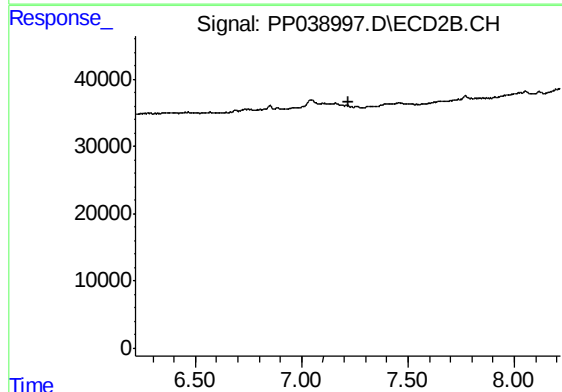


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.218 min
Response: 0
Conc: N.D.

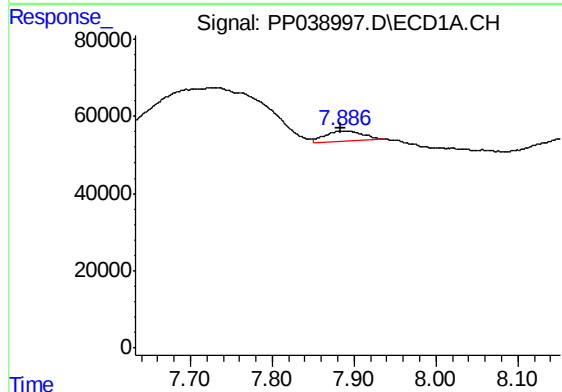


#31 AR-1260-1

R.T.: 7.886 min
Delta R.T.: 0.003 min
Response: 85062
Conc: 89.24 ng/ml

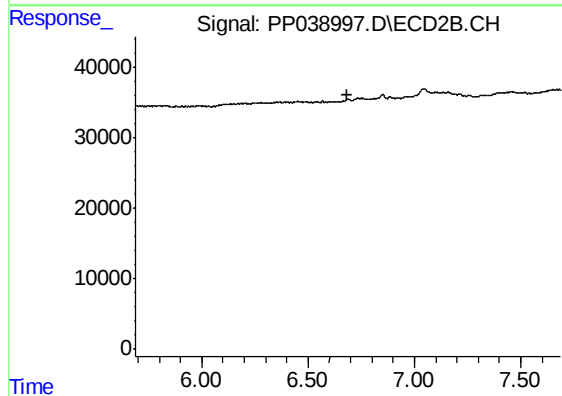

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.687 min
Response: 0
Conc: N.D.

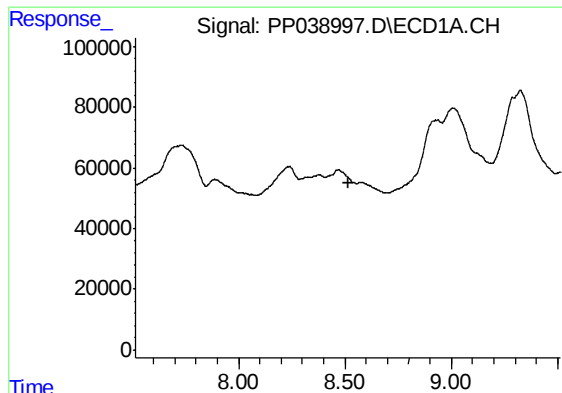

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 8.514 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TPR-14-COMP

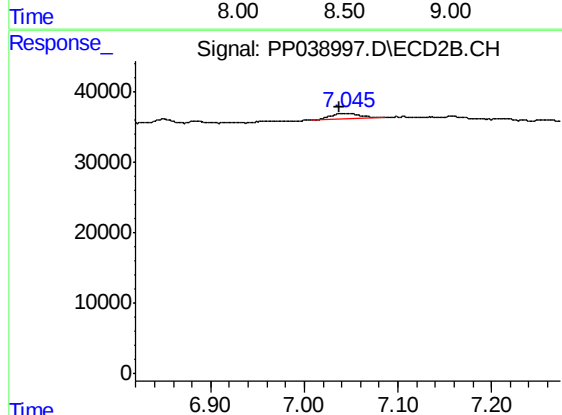


#33 AR-1260-3

R.T.: 7.045 min
Delta R.T.: 0.007 min
Response: 18436
Conc: 13.34 ng/ml

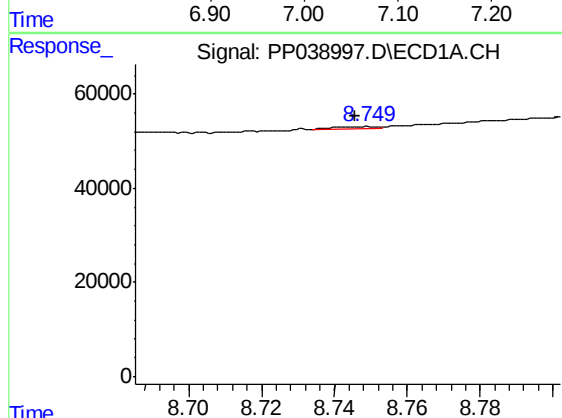

#34 AR-1260-4

R.T.: 8.750 min
Delta R.T.: 0.004 min
Response: 3573
Conc: 3.53 ng/ml

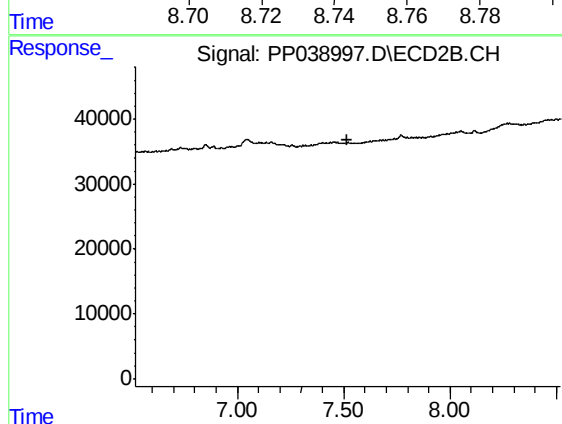

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.520 min
Response: 0
Conc: N.D.