

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082721\
 Data File : PP039007.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Aug 2021 18:31
 Operator : AJ\MA
 Sample : M3551-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 250EM-139-0204

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 04:14:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 26 09:31:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.875	3.861	861758	549737	22.576	22.811
2)	SA Decachlor...	10.852	9.116	497037	454271	20.644	20.090
Target Compounds							
8)	L2 AR-1221-1	5.128	0.000	27360	0	60.744	N.D. #
9)	L2 AR-1221-2	5.226	0.000	11004	0	33.032	N.D. #
30)	L6 AR-1254-5	8.450	0.000	1655	0	1.466	N.D. #
32)	L7 AR-1260-2	8.123f	0.000	1630	0	1.354	N.D. #
33)	L7 AR-1260-3	8.524	7.043	4484	16471	5.086	11.919 #
36)	L8 AR-1262-1	8.524	0.000	4484	0	3.358	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082721\
Data File : PP039007.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Aug 2021 18:31
Operator : AJ\MA
Sample : M3551-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
250EM-139-0204

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 04:14:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 26 09:31:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

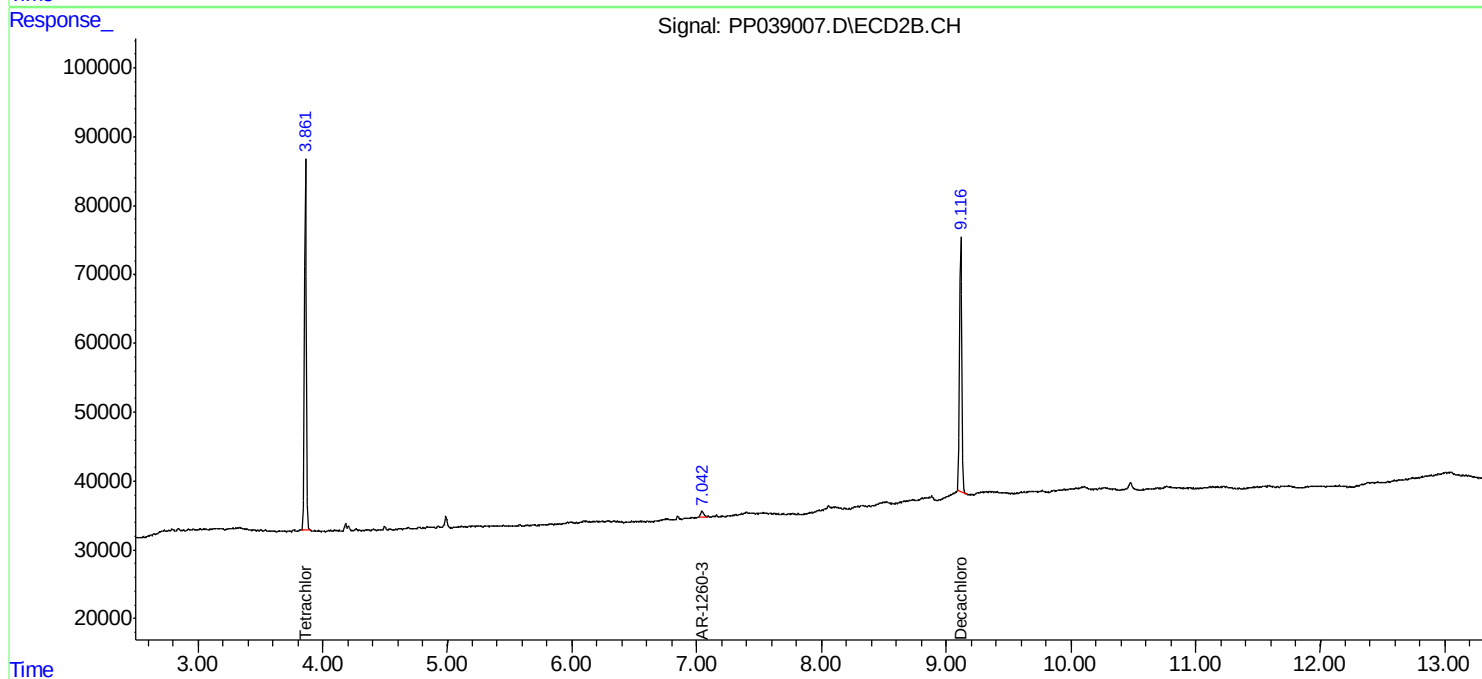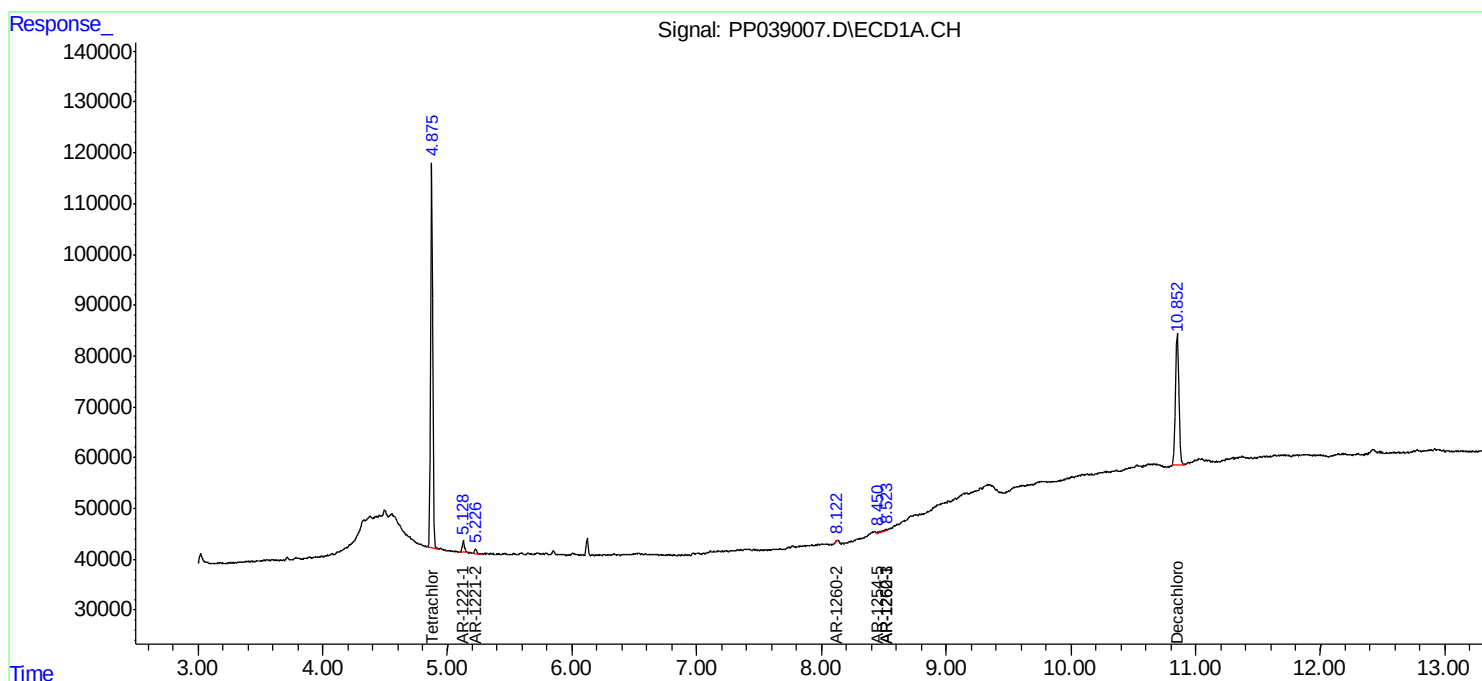


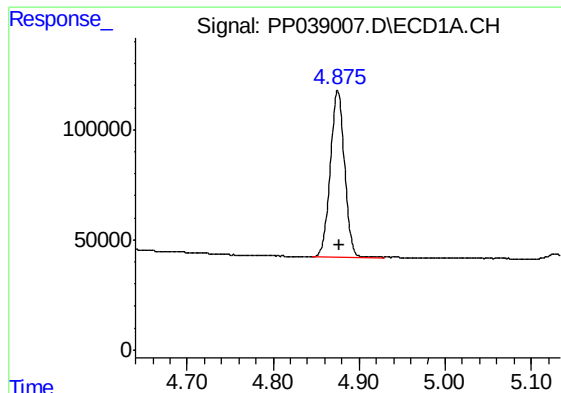

#1 Tetrachloro-m-xylene


R.T.: 4.875 min
Delta R.T.: -0.002 min
Response: 861758
Conc: 22.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
250EM-139-0204

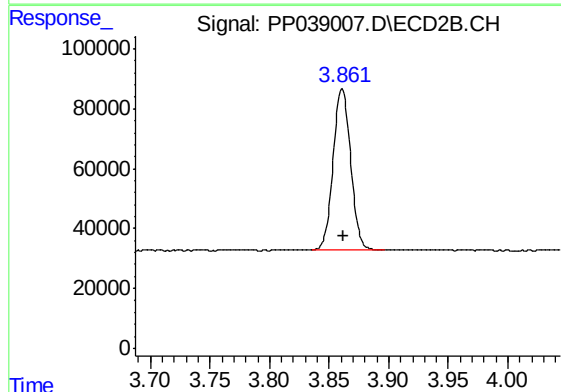


#1 Tetrachloro-m-xylene

R.T.: 3.861 min
Delta R.T.: 0.000 min
Response: 549737
Conc: 22.81 ng/ml

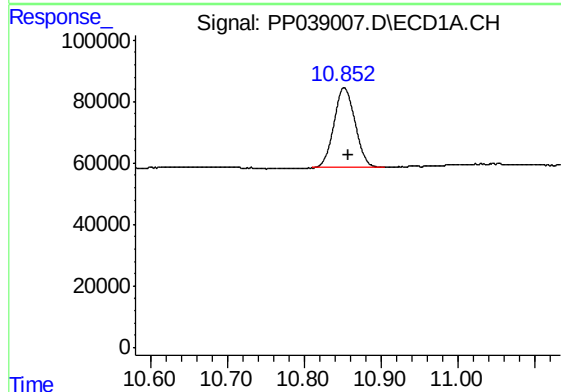


#2 Decachlorobiphenyl

R.T.: 10.852 min
Delta R.T.: -0.007 min
Response: 497037
Conc: 20.64 ng/ml

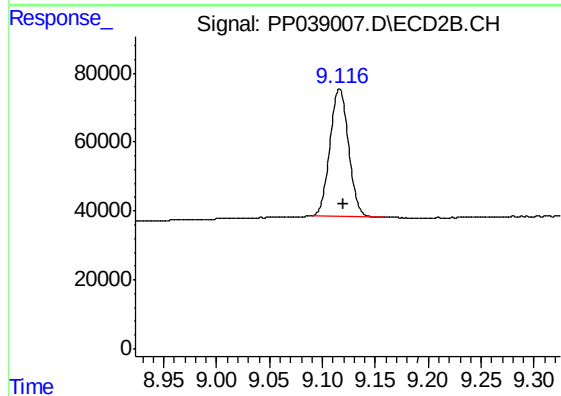

#2 Decachlorobiphenyl


R.T.: 9.116 min
Delta R.T.: -0.004 min
Response: 454271
Conc: 20.09 ng/ml

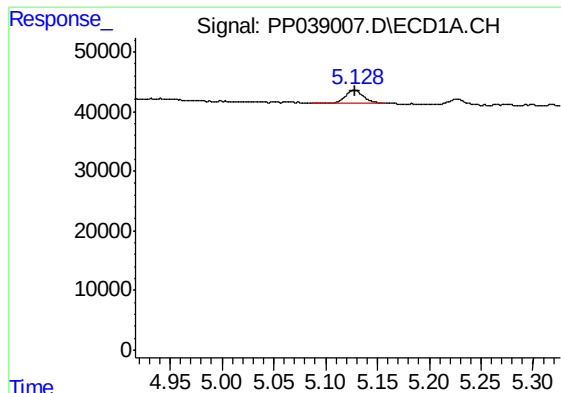

#8 AR-1221-1


R.T.: 5.128 min
Delta R.T.: 0.000 min
Response: 27360
Conc: 60.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
250EM-139-0204

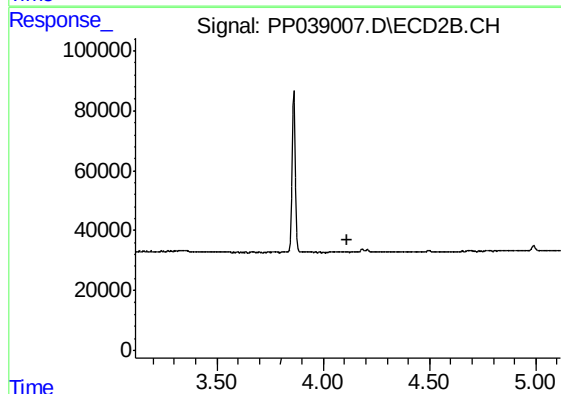


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.116 min
Response: 0
Conc: N.D.

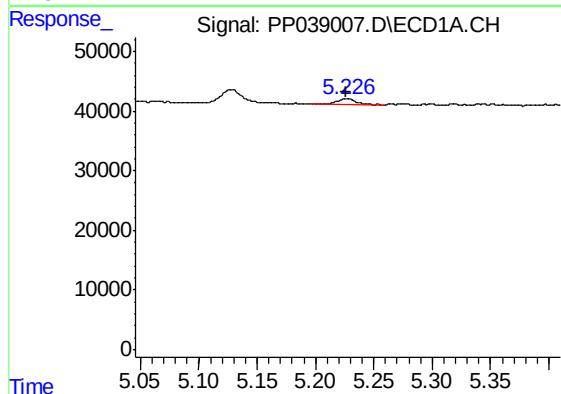


#9 AR-1221-2

R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 11004
Conc: 33.03 ng/ml

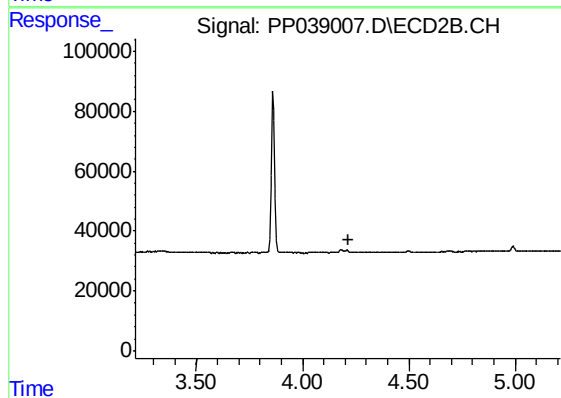

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.214 min
Response: 0
Conc: N.D.

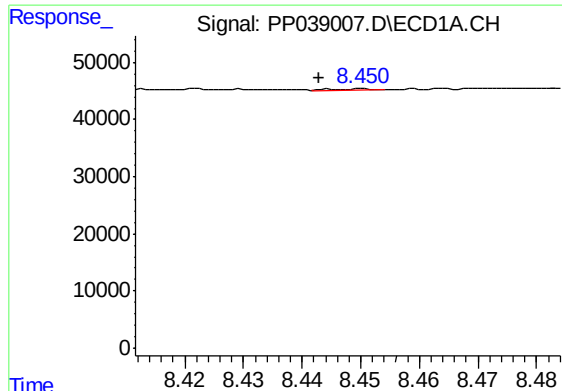

#30 AR-1254-5


R.T.: 8.450 min
Delta R.T.: 0.007 min
Response: 1655
Conc: 1.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
250EM-139-0204

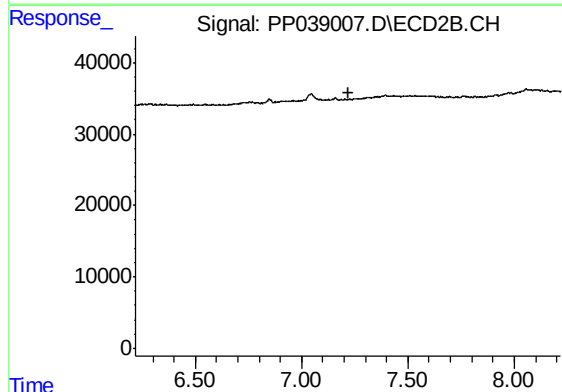


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.218 min
Response: 0
Conc: N.D.

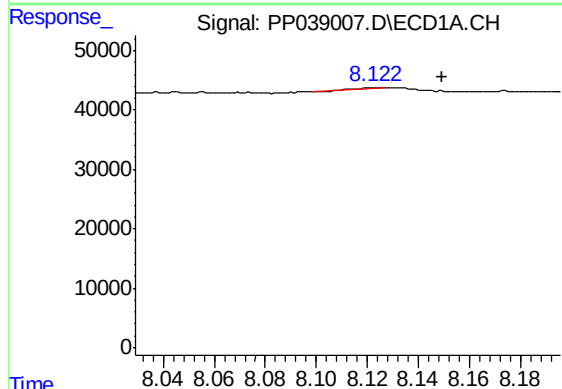


#32 AR-1260-2

R.T.: 8.123 min
Delta R.T.: -0.026 min
Response: 1630
Conc: 1.35 ng/ml

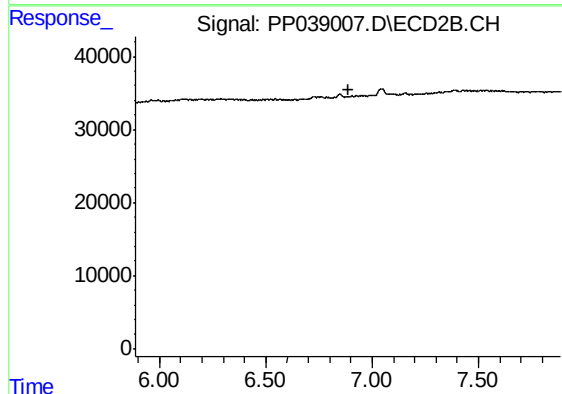

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.886 min
Response: 0
Conc: N.D.

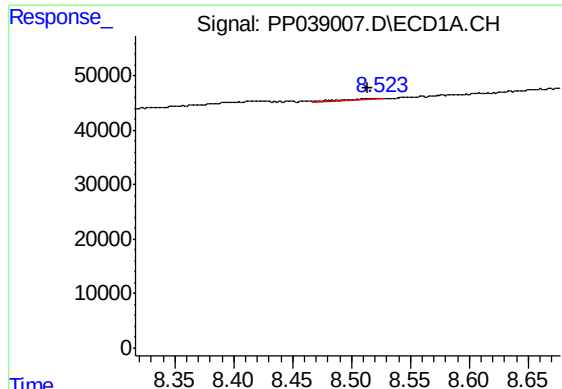

#33 AR-1260-3


R.T.: 8.524 min
Delta R.T.: 0.010 min
Response: 4484
Conc: 5.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
250EM-139-0204

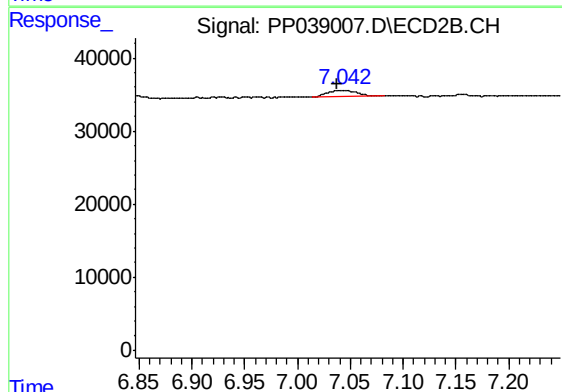


#33 AR-1260-3

R.T.: 7.043 min
Delta R.T.: 0.005 min
Response: 16471
Conc: 11.92 ng/ml

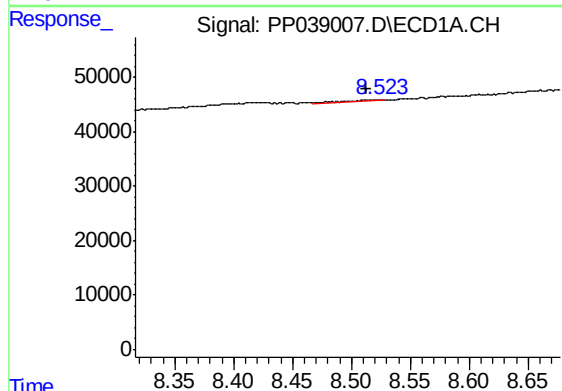

#36 AR-1262-1

R.T.: 8.524 min
Delta R.T.: 0.011 min
Response: 4484
Conc: 3.36 ng/ml

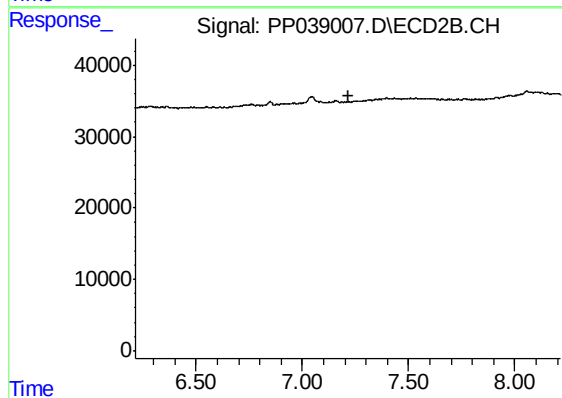

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.215 min
Response: 0
Conc: N.D.