

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
 Data File : PP066946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2024 13:44
 Operator : YP\AJ
 Sample : P3390-09
 Misc : AR1660 MDL 25 PPB
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 04:34:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 09:05:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.625	3.914	23683472	19709699	14.071	13.750
2)	SA Decachlor...	10.489	9.054	10275848	9063428	12.255	12.101
Target Compounds							
3)	L1 AR-1016-1	5.799	5.022	889790	790695	18.806	18.113
4)	L1 AR-1016-2	5.822	5.042	1461743	1079052	19.756	16.769
5)	L1 AR-1016-3	5.885	5.223	952400	712612	20.299	20.752
6)	L1 AR-1016-4	5.985	5.263	622785	608884	17.225	20.102
7)	L1 AR-1016-5	6.278	5.482	633572	632408	18.495	17.518
9)	L2 AR-1221-2	4.933	4.222	435337	356378	32.337	30.458
10)	L2 AR-1221-3	4.998	4.297	555206	546291	13.738	14.348
11)	L3 AR-1232-1	4.998	4.297	555206	546291	16.654	17.357
12)	L3 AR-1232-2	5.531	5.042	805776	1079052	45.644	36.592
13)	L3 AR-1232-3	5.822	5.223	1461743	712612	46.815	50.176
14)	L3 AR-1232-4	5.985	5.306	622785	698125	40.705	49.667
15)	L3 AR-1232-5	6.071	5.482	727401	632408	57.809	44.460
16)	L4 AR-1242-1	5.799	5.022	889790	790695	25.868	25.453
17)	L4 AR-1242-2	5.822	5.042	1461743	1079052	27.519	24.176
18)	L4 AR-1242-3	5.885	5.223	952400	712612	27.773	29.541
19)	L4 AR-1242-4	5.985	5.306	622785	698125	24.000	26.088
20)	L4 AR-1242-5	6.720	5.839	192437	618484	8.282	22.160 #
21)	L5 AR-1248-1	5.799	5.022	889790	790695	36.859	35.926
22)	L5 AR-1248-2	6.071	5.263	727401	608884	18.677	17.331
23)	L5 AR-1248-3	6.278	5.306	633572	698125	15.554	19.186
24)	L5 AR-1248-4	6.688	5.482	273987	632408	7.072	15.563 #
25)	L5 AR-1248-5	6.720	5.867	192437	282453	4.887	8.842 #
26)	L6 AR-1254-1	6.656	5.839	939952	618484	18.890	10.422 #
27)	L6 AR-1254-2	6.871	5.986	686592	443411	9.720	8.462
28)	L6 AR-1254-3	7.242	6.411	453627	1297836	6.658	17.012 #
29)	L6 AR-1254-4	7.529	6.628	148854	247210	3.555	6.544 #
30)	L6 AR-1254-5	7.943	7.048	2451220	1539608	46.649	24.463 #
31)	L7 AR-1260-1	7.404	6.528	1276088	1465659	21.084	23.136
32)	L7 AR-1260-2	7.660	6.716	1301108	1425938	20.240	21.089
33)	L7 AR-1260-3	8.020	6.875	1162817	1585656	26.049	23.807
34)	L7 AR-1260-4	8.254	7.351	1188641	1091101	23.724	24.895
35)	L7 AR-1260-5	8.584	7.590	1631850	1675040	19.526	18.781
36)	L8 AR-1262-1	8.254	7.086	1188641	1078224	18.176	14.924
37)	L8 AR-1262-2	8.584	7.351	1631850	1091101	15.776	17.732
38)	L8 AR-1262-3	8.922	7.874	1150808	1088161	16.114	25.869 #
39)	L8 AR-1262-4	9.012	7.941	639400	1194093	10.830	15.394 #
40)	L8 AR-1262-5	9.700	8.459	459356	182484	16.696	6.910 #
41)	L9 AR-1268-1	8.922	7.874	1150808	1088161	8.806	8.700
42)	L9 AR-1268-2	9.012	7.941	639400	1194093	5.464	10.684 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
Data File : PP066946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2024 13:44
Operator : YP\AJ
Sample : P3390-09
Misc : AR1660 MDL 25 PPB
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 04:34:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 09:05:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43)	L9 AR-1268-3	9.250	8.156	133651	187566	1.284	1.835 #
44)	L9 AR-1268-4	9.700	8.459	459356	182484	15.346	6.428 #
45)	L9 AR-1268-5	10.122	8.768	98360	143680	0.351	0.586 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
Data File : PP066946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2024 13:44
Operator : YP\AJ
Sample : P3390-09
Misc : AR1660 MDL 25 PPB
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 04:34:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 09:05:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

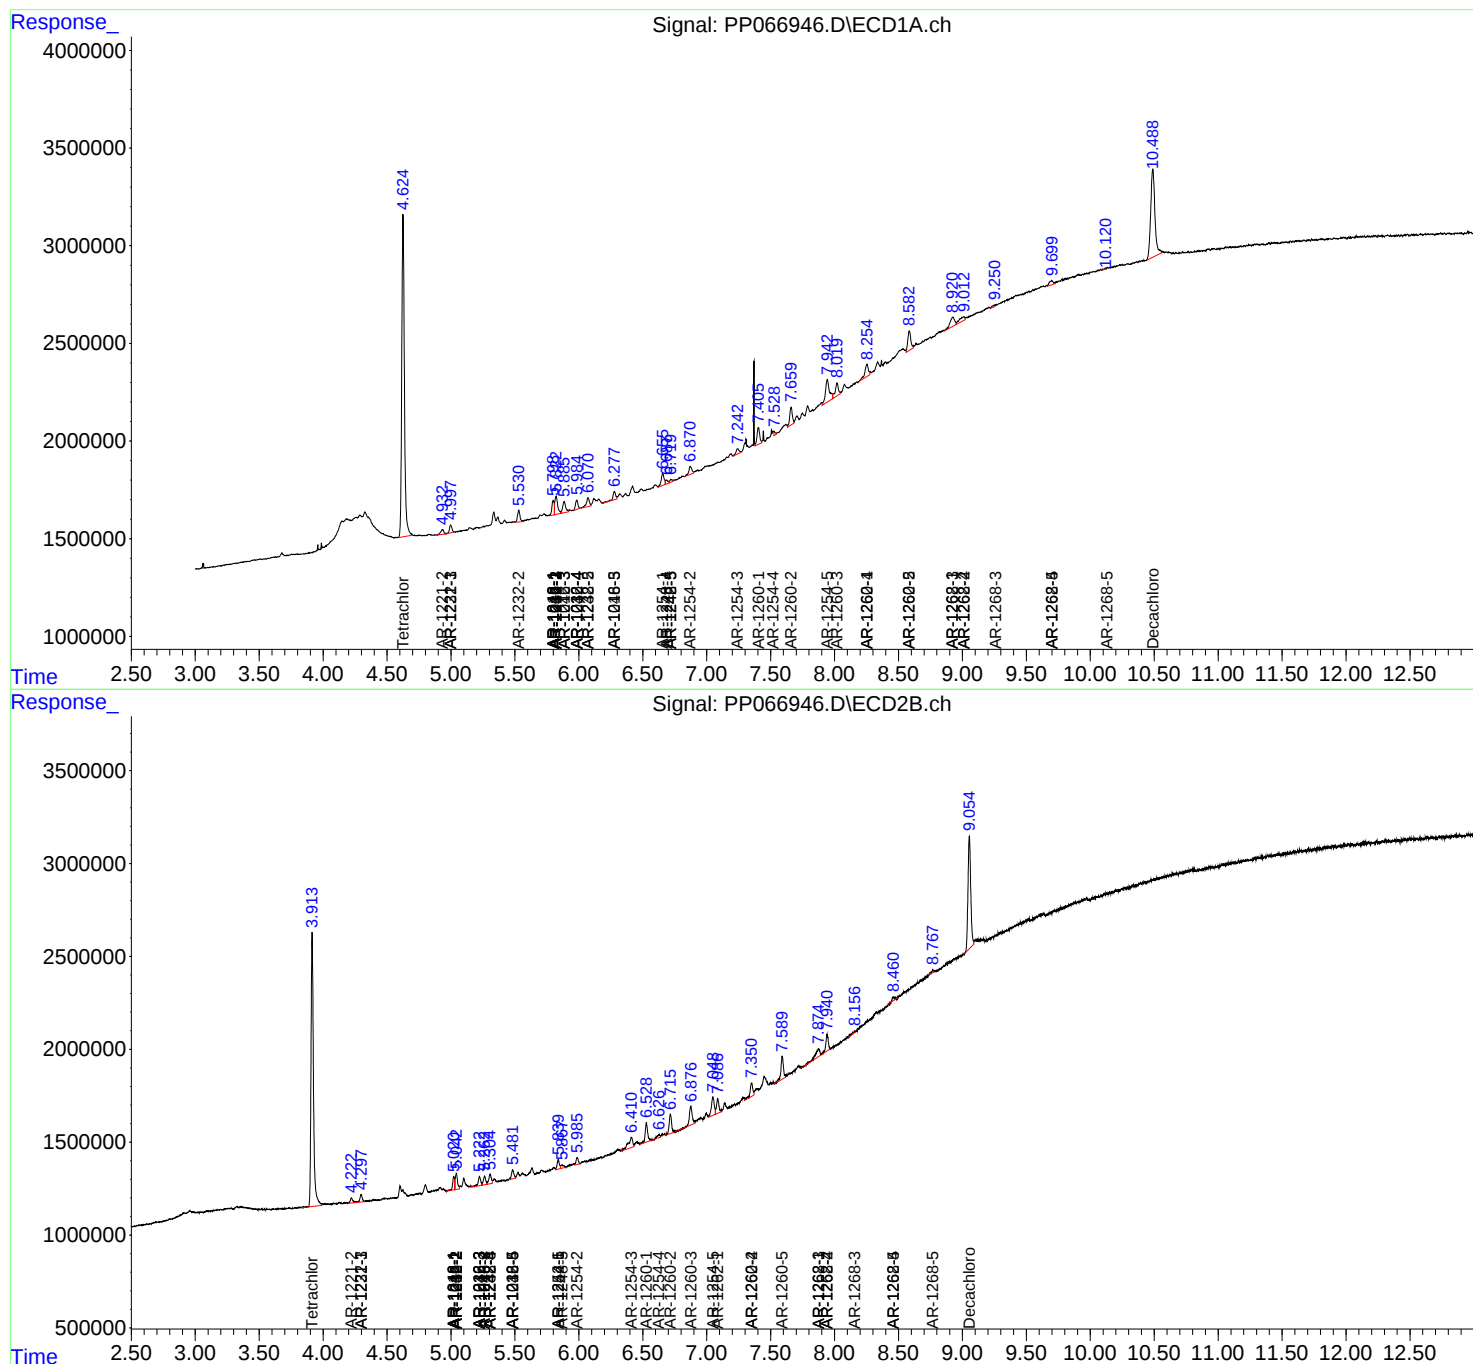


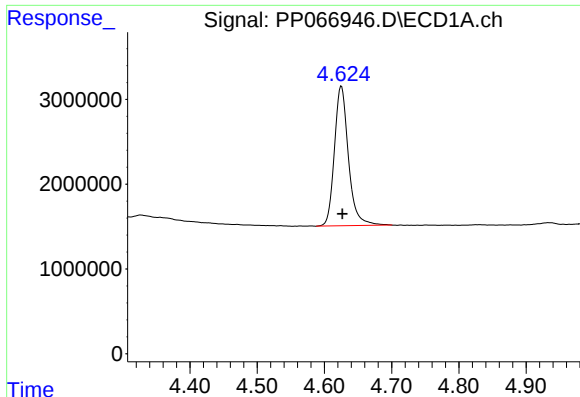

#1 Tetrachloro-m-xylene


R.T.: 4.625 min
Delta R.T.: -0.002 min
Response: 23683472
Conc: 14.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

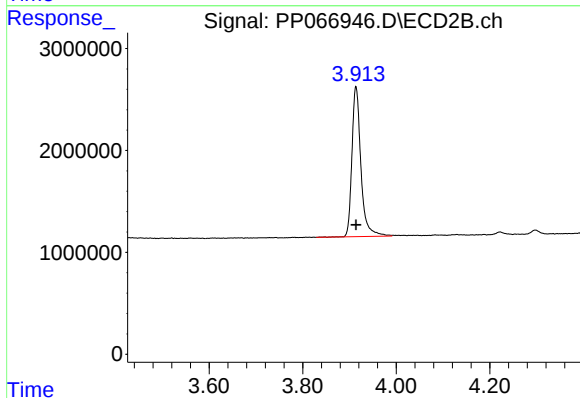


#1 Tetrachloro-m-xylene

R.T.: 3.914 min
Delta R.T.: 0.000 min
Response: 19709699
Conc: 13.75 ng/ml

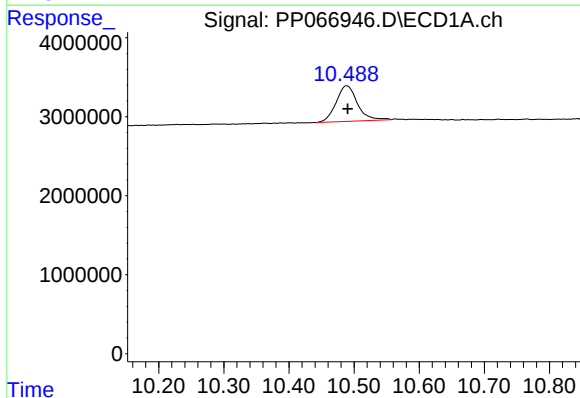


#2 Decachlorobiphenyl

R.T.: 10.489 min
Delta R.T.: -0.001 min
Response: 10275848
Conc: 12.25 ng/ml

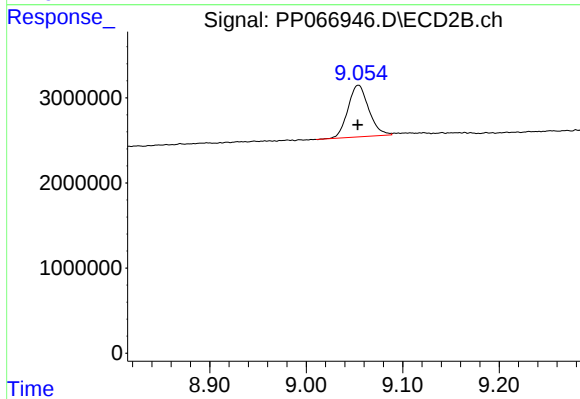

#2 Decachlorobiphenyl


R.T.: 9.054 min
Delta R.T.: 0.000 min
Response: 9063428
Conc: 12.10 ng/ml

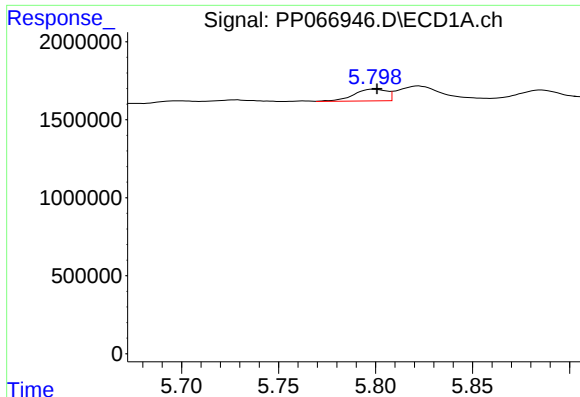

#3 AR-1016-1


R.T.: 5.799 min
Delta R.T.: -0.002 min
Response: 889790
Conc: 18.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

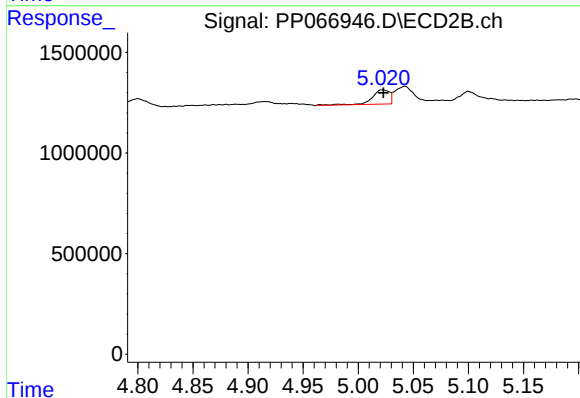


#3 AR-1016-1

R.T.: 5.022 min
Delta R.T.: 0.000 min
Response: 790695
Conc: 18.11 ng/ml

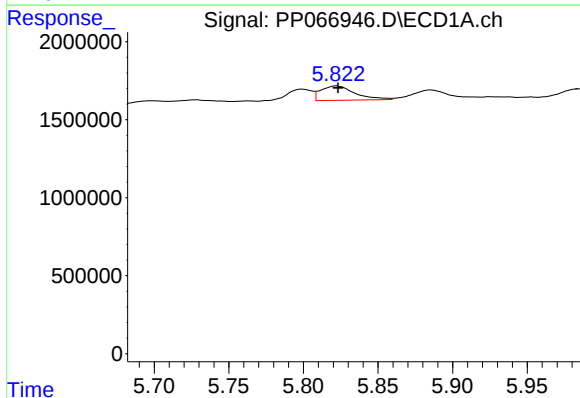


#4 AR-1016-2

R.T.: 5.822 min
Delta R.T.: -0.001 min
Response: 1461743
Conc: 19.76 ng/ml

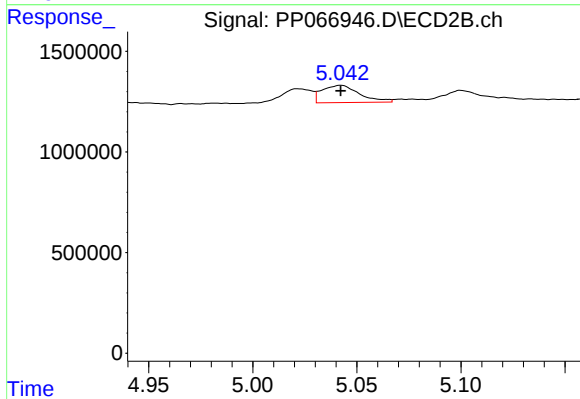

#4 AR-1016-2


R.T.: 5.042 min
Delta R.T.: 0.000 min
Response: 1079052
Conc: 16.77 ng/ml

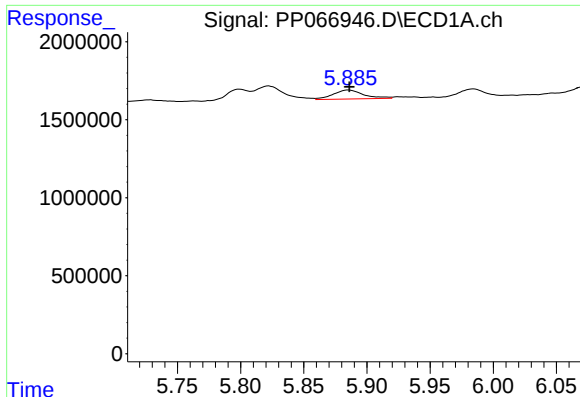

#5 AR-1016-3


R.T.: 5.885 min
Delta R.T.: 0.000 min
Response: 952400
Conc: 20.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

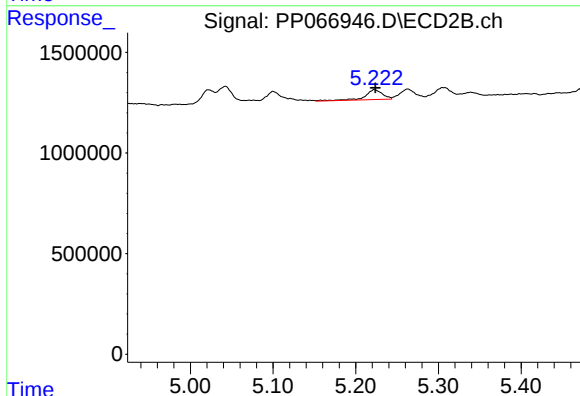


#5 AR-1016-3

R.T.: 5.223 min
Delta R.T.: -0.001 min
Response: 712612
Conc: 20.75 ng/ml

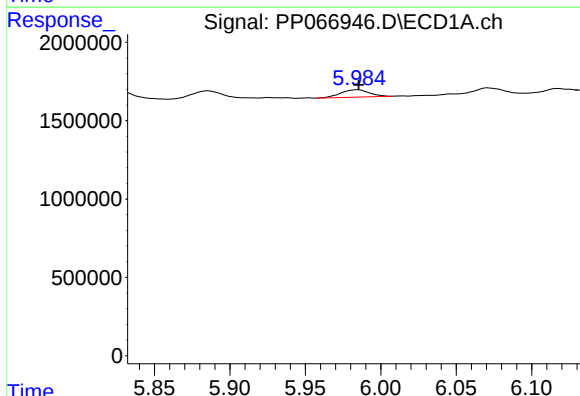


#6 AR-1016-4

R.T.: 5.985 min
Delta R.T.: 0.000 min
Response: 622785
Conc: 17.23 ng/ml

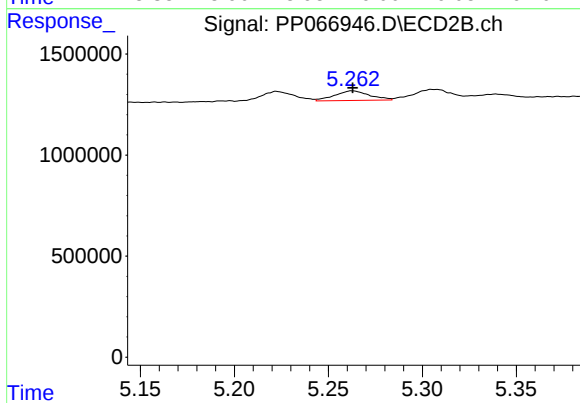

#6 AR-1016-4


R.T.: 5.263 min
Delta R.T.: 0.000 min
Response: 608884
Conc: 20.10 ng/ml

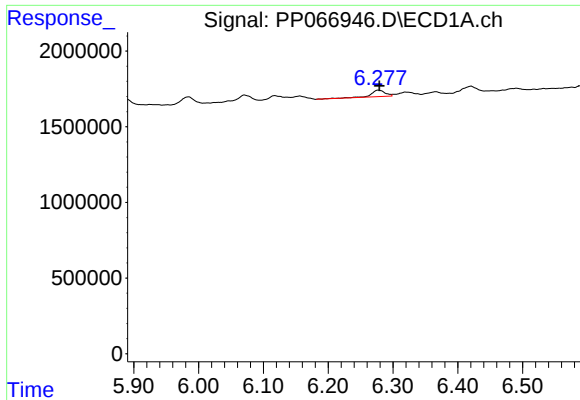

#7 AR-1016-5


R.T.: 6.278 min
Delta R.T.: -0.002 min
Response: 633572
Conc: 18.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

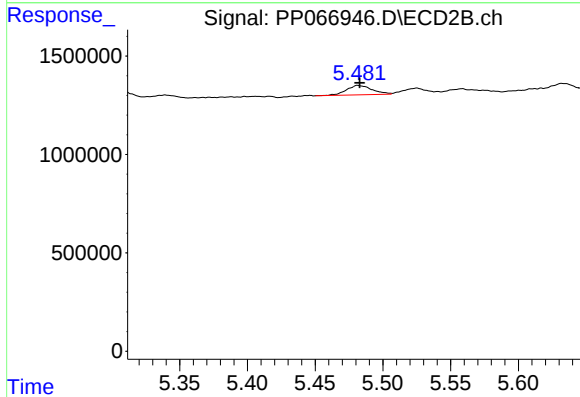


#7 AR-1016-5

R.T.: 5.482 min
Delta R.T.: -0.001 min
Response: 632408
Conc: 17.52 ng/ml

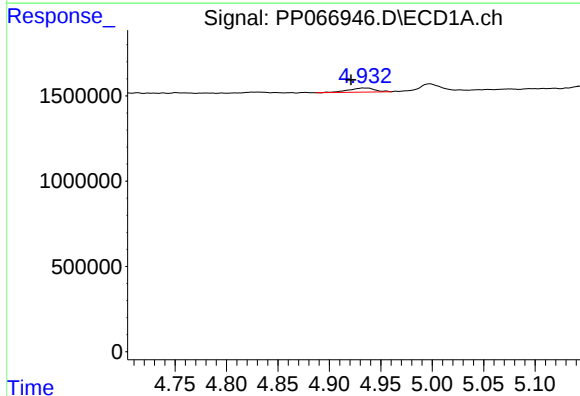


#9 AR-1221-2

R.T.: 4.933 min
Delta R.T.: 0.012 min
Response: 435337
Conc: 32.34 ng/ml

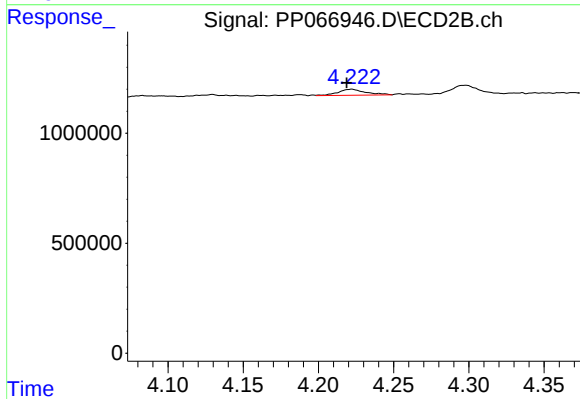

#9 AR-1221-2


R.T.: 4.222 min
Delta R.T.: 0.003 min
Response: 356378
Conc: 30.46 ng/ml

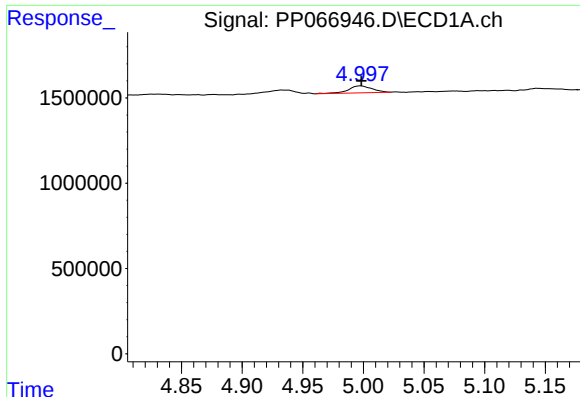

#10 AR-1221-3


R.T.: 4.998 min
Delta R.T.: 0.000 min
Response: 555206
Conc: 13.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

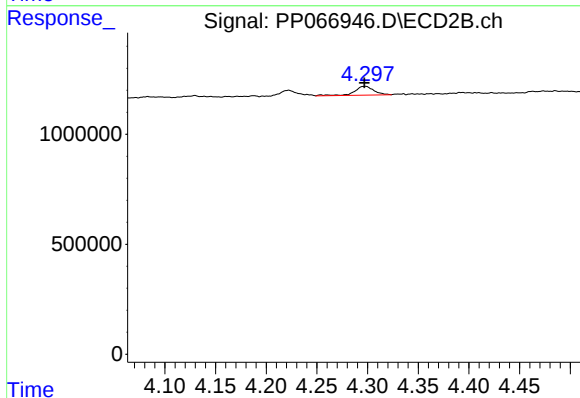


#10 AR-1221-3

R.T.: 4.297 min
Delta R.T.: 0.000 min
Response: 546291
Conc: 14.35 ng/ml

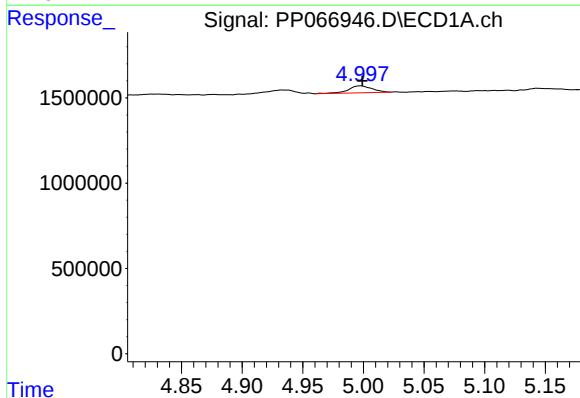


#11 AR-1232-1

R.T.: 4.998 min
Delta R.T.: -0.002 min
Response: 555206
Conc: 16.65 ng/ml

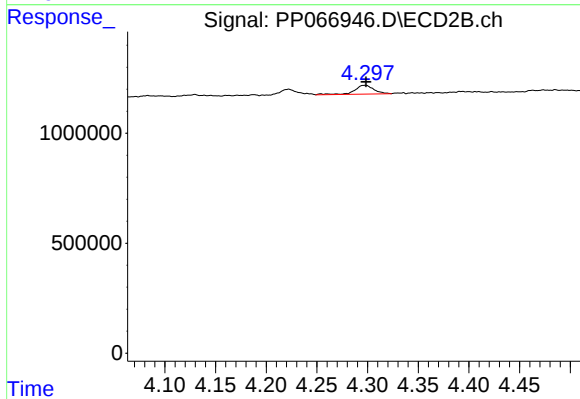

#11 AR-1232-1


R.T.: 4.297 min
Delta R.T.: -0.001 min
Response: 546291
Conc: 17.36 ng/ml

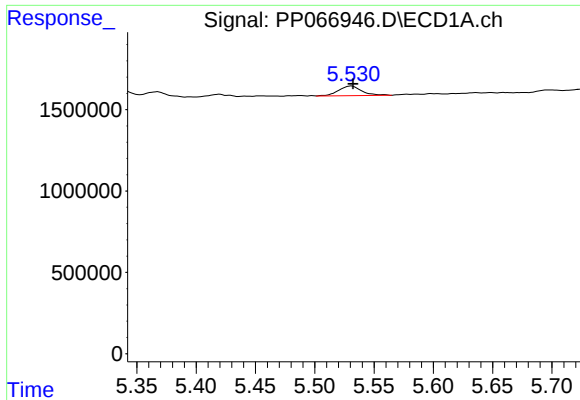

#12 AR-1232-2


R.T.: 5.531 min
Delta R.T.: -0.001 min
Response: 805776
Conc: 45.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

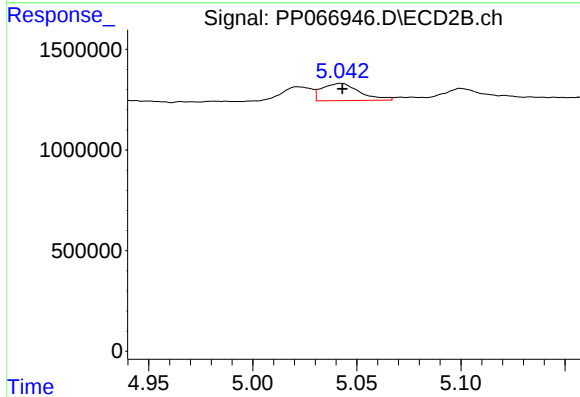


#12 AR-1232-2

R.T.: 5.042 min
Delta R.T.: 0.000 min
Response: 1079052
Conc: 36.59 ng/ml

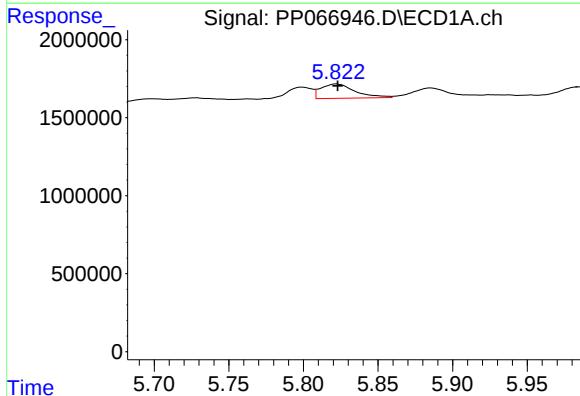


#13 AR-1232-3

R.T.: 5.822 min
Delta R.T.: 0.000 min
Response: 1461743
Conc: 46.81 ng/ml

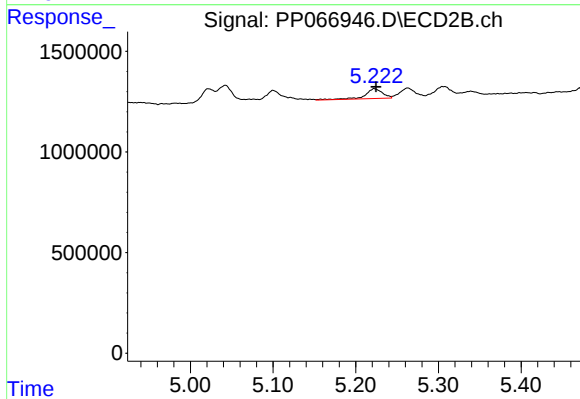

#13 AR-1232-3


R.T.: 5.223 min
Delta R.T.: -0.002 min
Response: 712612
Conc: 50.18 ng/ml

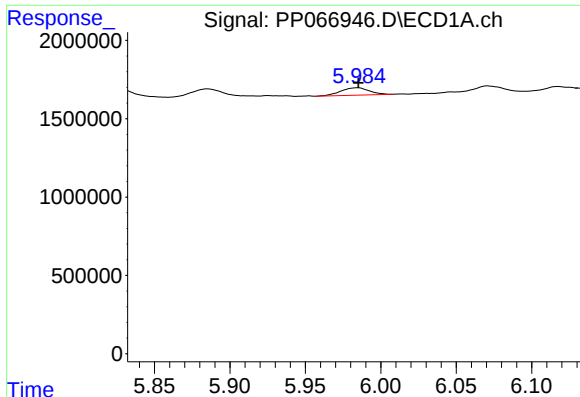

#14 AR-1232-4


R.T.: 5.985 min
Delta R.T.: 0.000 min
Response: 622785
Conc: 40.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

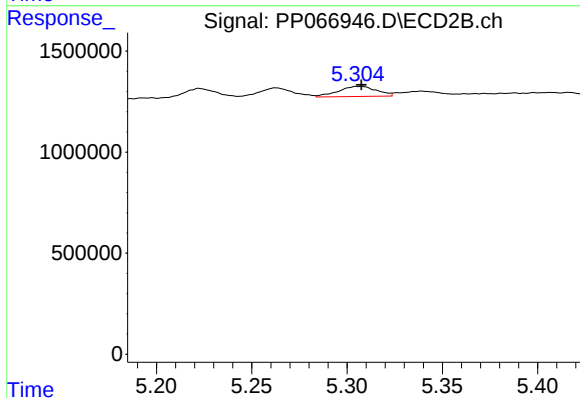


#14 AR-1232-4

R.T.: 5.306 min
Delta R.T.: -0.001 min
Response: 698125
Conc: 49.67 ng/ml

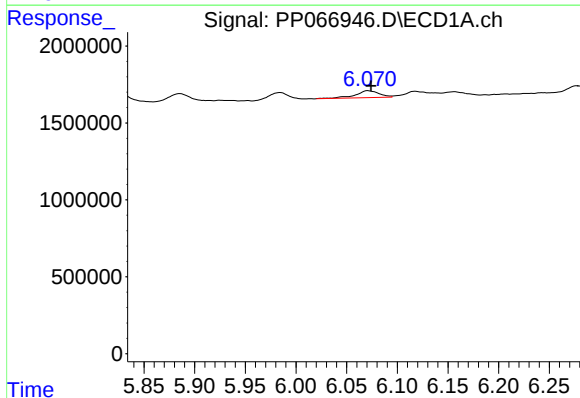


#15 AR-1232-5

R.T.: 6.071 min
Delta R.T.: -0.003 min
Response: 727401
Conc: 57.81 ng/ml

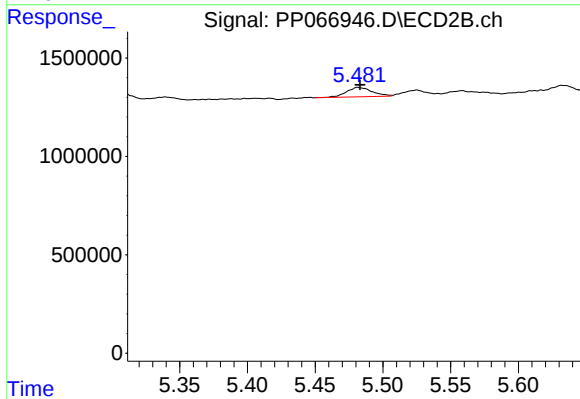

#15 AR-1232-5


R.T.: 5.482 min
Delta R.T.: -0.001 min
Response: 632408
Conc: 44.46 ng/ml

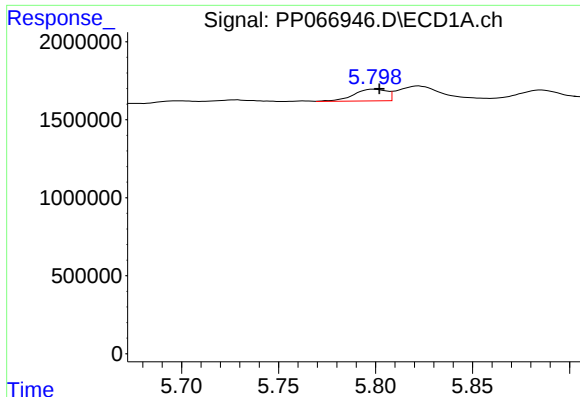

#16 AR-1242-1


R.T.: 5.799 min
Delta R.T.: -0.003 min
Response: 889790
Conc: 25.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

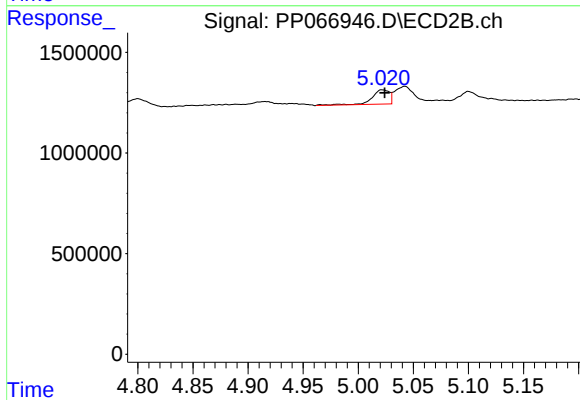


#16 AR-1242-1

R.T.: 5.022 min
Delta R.T.: -0.002 min
Response: 790695
Conc: 25.45 ng/ml

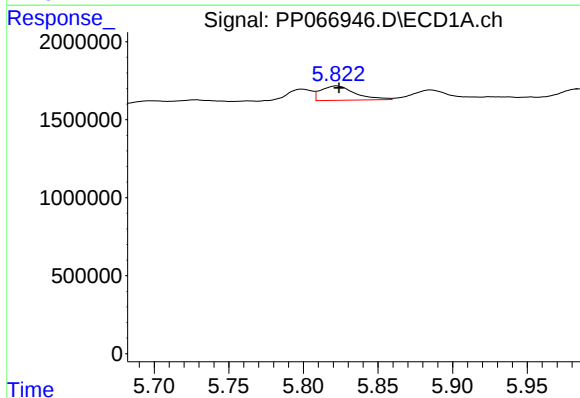


#17 AR-1242-2

R.T.: 5.822 min
Delta R.T.: -0.002 min
Response: 1461743
Conc: 27.52 ng/ml

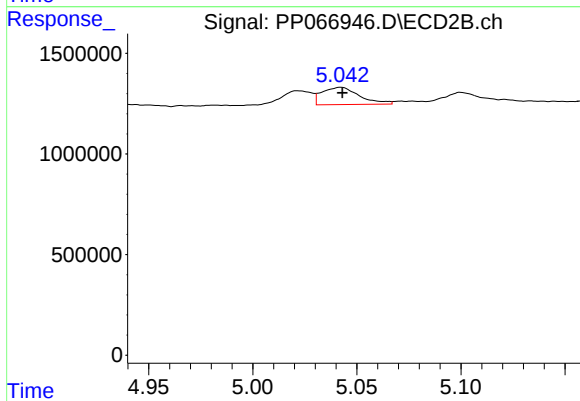

#17 AR-1242-2


R.T.: 5.042 min
Delta R.T.: 0.000 min
Response: 1079052
Conc: 24.18 ng/ml

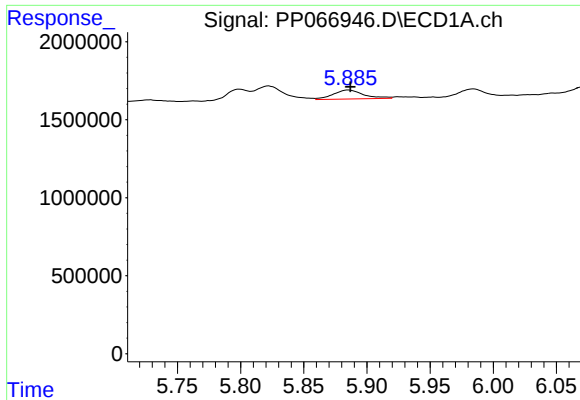

#18 AR-1242-3


R.T.: 5.885 min
Delta R.T.: -0.001 min
Response: 952400
Conc: 27.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

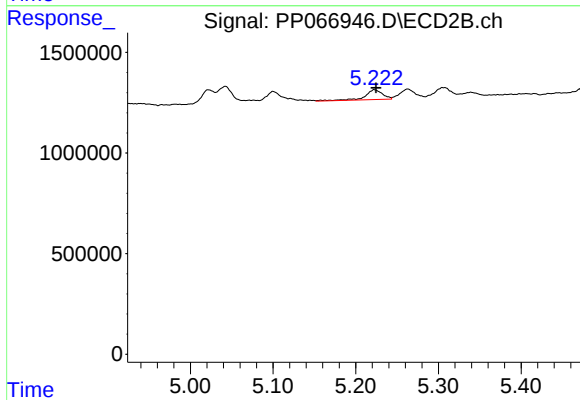


#18 AR-1242-3

R.T.: 5.223 min
Delta R.T.: -0.002 min
Response: 712612
Conc: 29.54 ng/ml

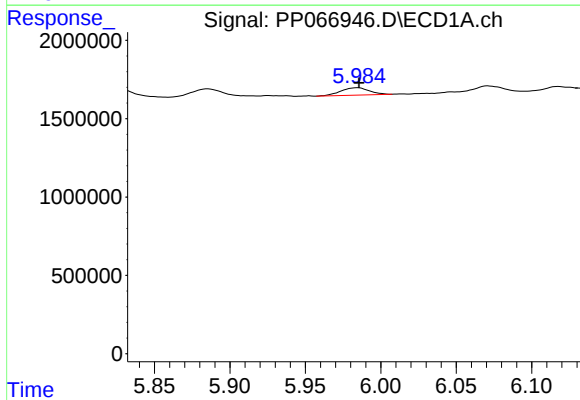


#19 AR-1242-4

R.T.: 5.985 min
Delta R.T.: 0.000 min
Response: 622785
Conc: 24.00 ng/ml

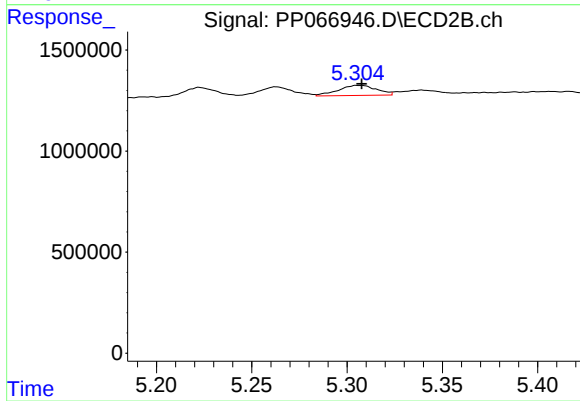

#19 AR-1242-4


R.T.: 5.306 min
Delta R.T.: -0.001 min
Response: 698125
Conc: 26.09 ng/ml

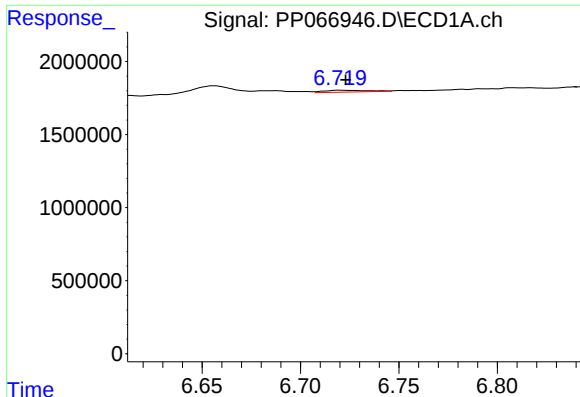

#20 AR-1242-5


R.T.: 6.720 min
Delta R.T.: -0.003 min
Response: 192437
Conc: 8.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

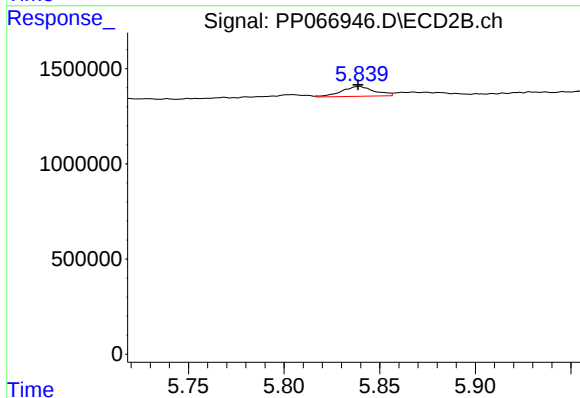


#20 AR-1242-5

R.T.: 5.839 min
Delta R.T.: 0.000 min
Response: 618484
Conc: 22.16 ng/ml

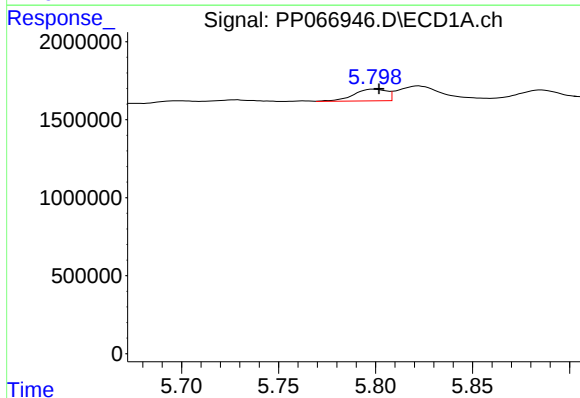


#21 AR-1248-1

R.T.: 5.799 min
Delta R.T.: -0.003 min
Response: 889790
Conc: 36.86 ng/ml

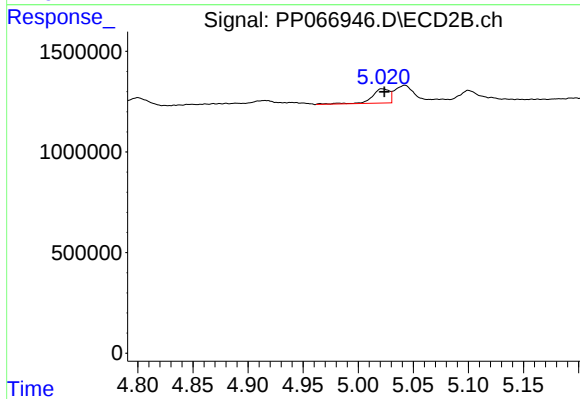

#21 AR-1248-1


R.T.: 5.022 min
Delta R.T.: -0.002 min
Response: 790695
Conc: 35.93 ng/ml

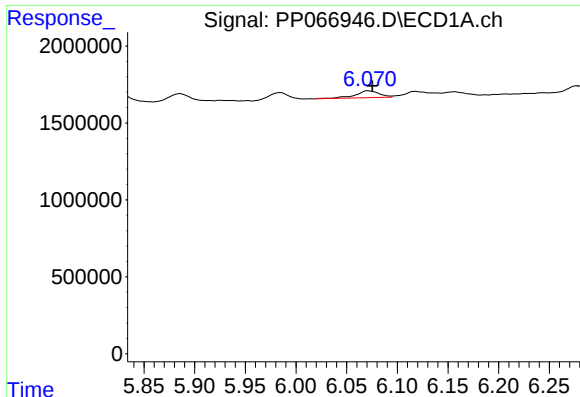

#22 AR-1248-2


R.T.: 6.071 min
Delta R.T.: -0.004 min
Response: 727401
Conc: 18.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

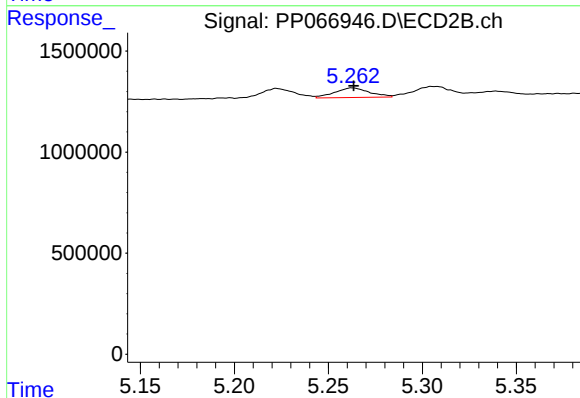


#22 AR-1248-2

R.T.: 5.263 min
Delta R.T.: 0.000 min
Response: 608884
Conc: 17.33 ng/ml

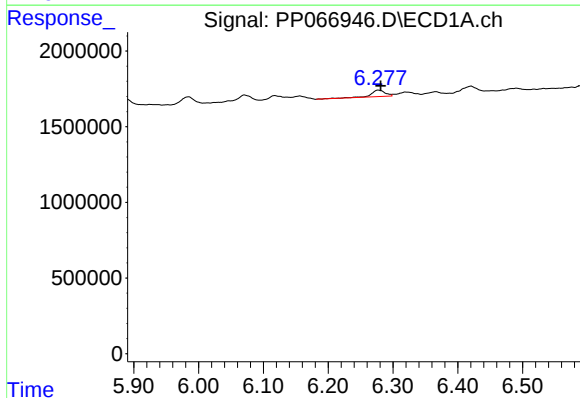


#23 AR-1248-3

R.T.: 6.278 min
Delta R.T.: -0.003 min
Response: 633572
Conc: 15.55 ng/ml

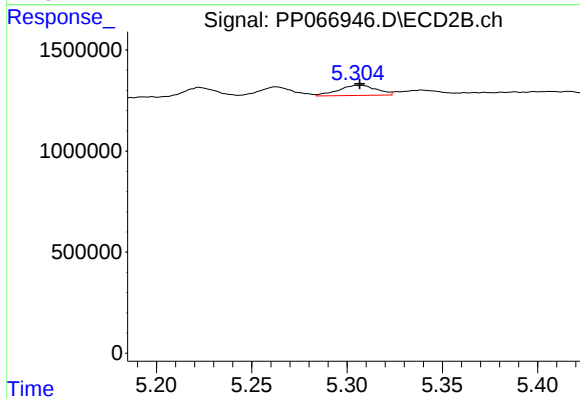

#23 AR-1248-3


R.T.: 5.306 min
Delta R.T.: 0.000 min
Response: 698125
Conc: 19.19 ng/ml

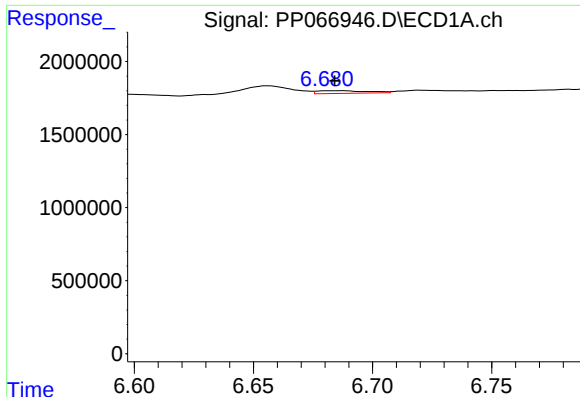

#24 AR-1248-4


R.T.: 6.688 min
Delta R.T.: 0.004 min
Response: 273987
Conc: 7.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

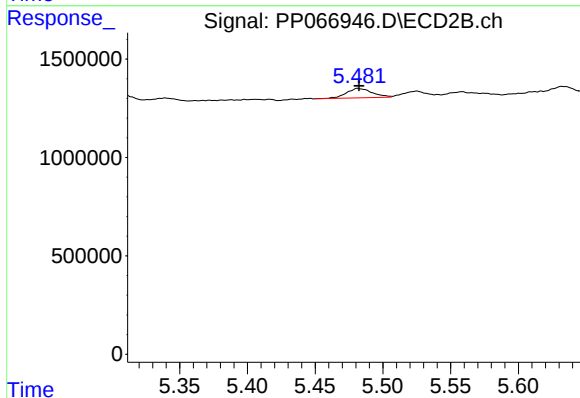


#24 AR-1248-4

R.T.: 5.482 min
Delta R.T.: 0.000 min
Response: 632408
Conc: 15.56 ng/ml

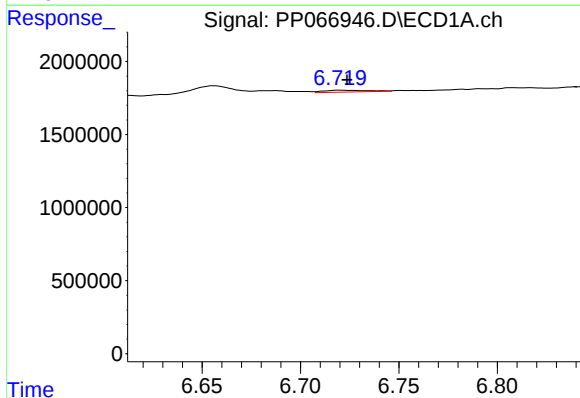


#25 AR-1248-5

R.T.: 6.720 min
Delta R.T.: -0.004 min
Response: 192437
Conc: 4.89 ng/ml

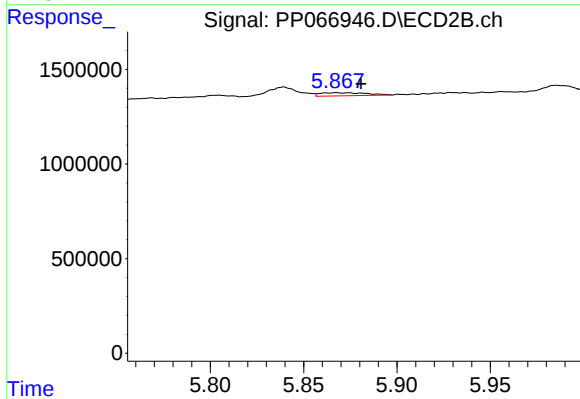

#25 AR-1248-5


R.T.: 5.867 min
Delta R.T.: -0.013 min
Response: 282453
Conc: 8.84 ng/ml

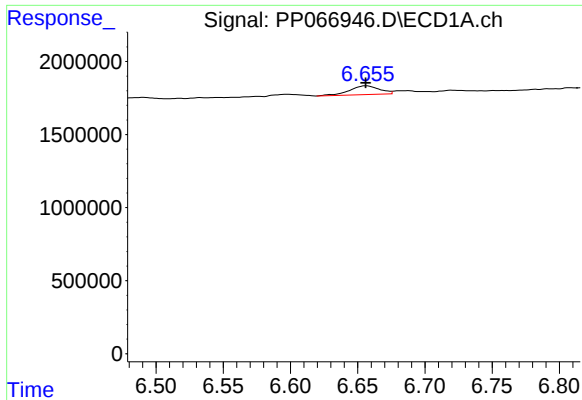

#26 AR-1254-1


R.T.: 6.656 min
Delta R.T.: 0.000 min
Response: 939952
Conc: 18.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

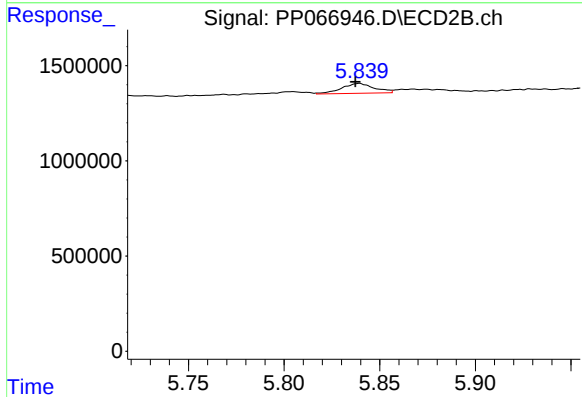


#26 AR-1254-1

R.T.: 5.839 min
Delta R.T.: 0.002 min
Response: 618484
Conc: 10.42 ng/ml

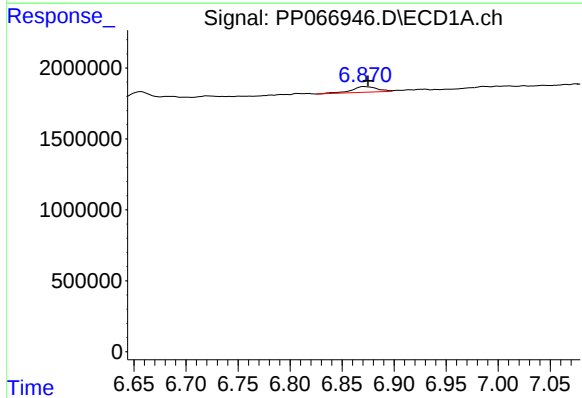


#27 AR-1254-2

R.T.: 6.871 min
Delta R.T.: -0.004 min
Response: 686592
Conc: 9.72 ng/ml

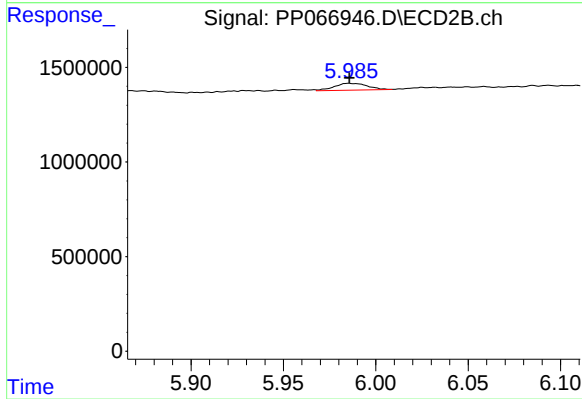

#27 AR-1254-2


R.T.: 5.986 min
Delta R.T.: 0.000 min
Response: 443411
Conc: 8.46 ng/ml

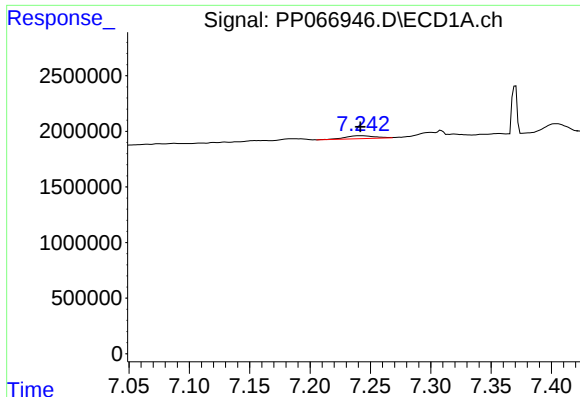

#28 AR-1254-3


R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 453627
Conc: 6.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

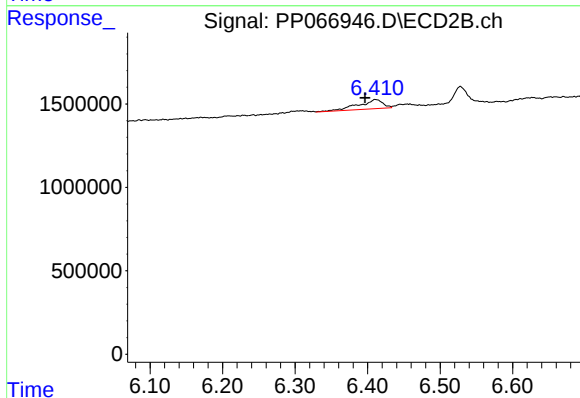


#28 AR-1254-3

R.T.: 6.411 min
Delta R.T.: 0.014 min
Response: 1297836
Conc: 17.01 ng/ml

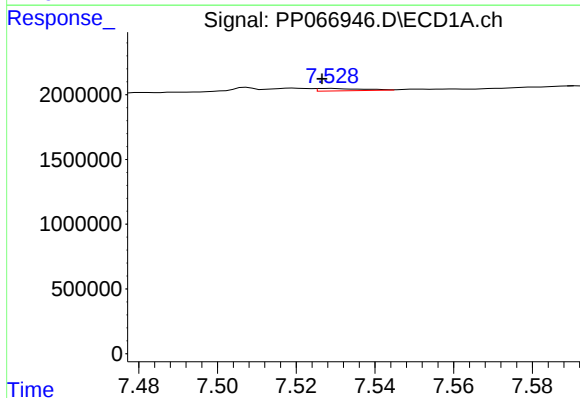


#29 AR-1254-4

R.T.: 7.529 min
Delta R.T.: 0.002 min
Response: 148854
Conc: 3.55 ng/ml

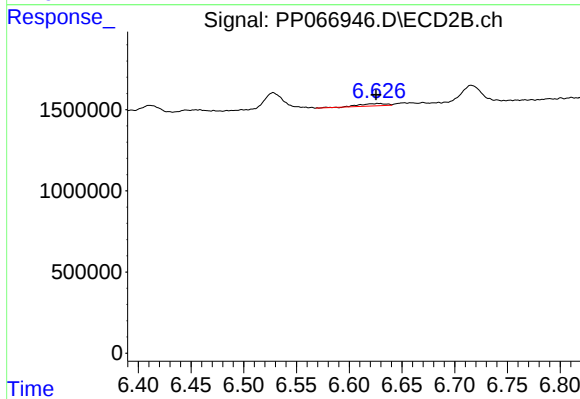

#29 AR-1254-4


R.T.: 6.628 min
Delta R.T.: 0.002 min
Response: 247210
Conc: 6.54 ng/ml

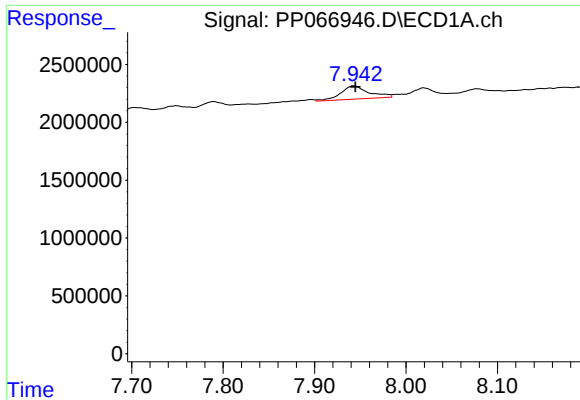

#30 AR-1254-5


R.T.: 7.943 min
Delta R.T.: -0.002 min
Response: 2451220
Conc: 46.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

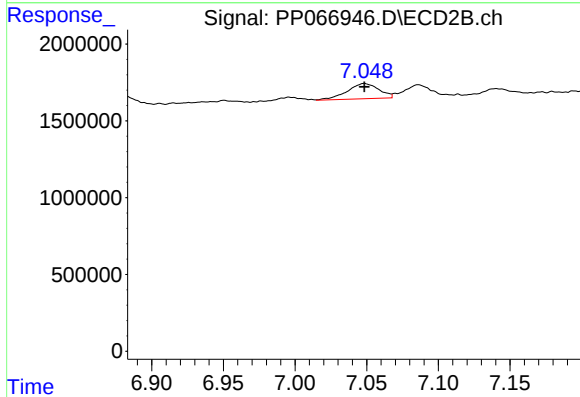


#30 AR-1254-5

R.T.: 7.048 min
Delta R.T.: 0.000 min
Response: 1539608
Conc: 24.46 ng/ml

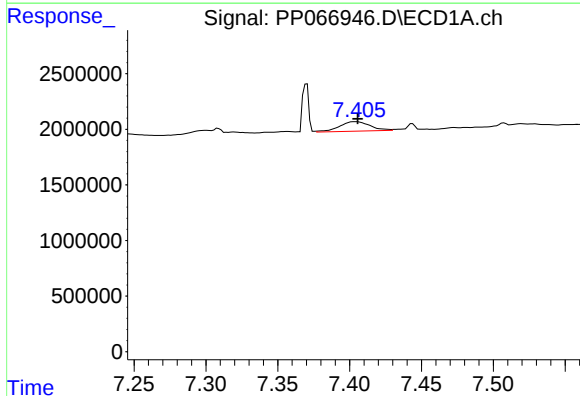


#31 AR-1260-1

R.T.: 7.404 min
Delta R.T.: -0.001 min
Response: 1276088
Conc: 21.08 ng/ml

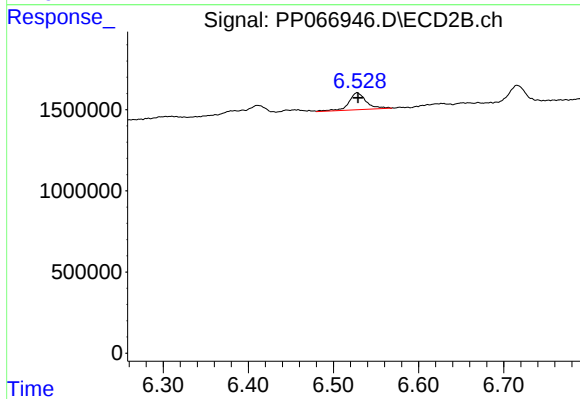

#31 AR-1260-1


R.T.: 6.528 min
Delta R.T.: -0.001 min
Response: 1465659
Conc: 23.14 ng/ml

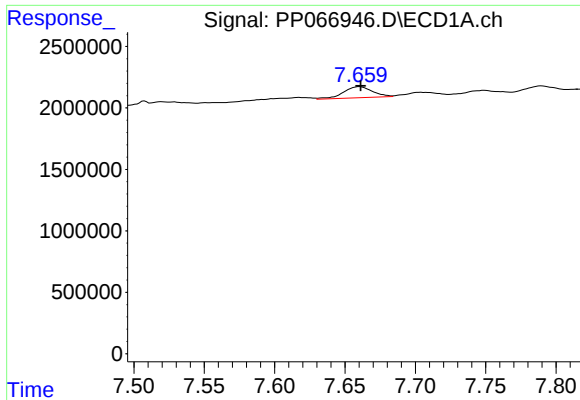

#32 AR-1260-2


R.T.: 7.660 min
Delta R.T.: 0.000 min
Response: 1301108
Conc: 20.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

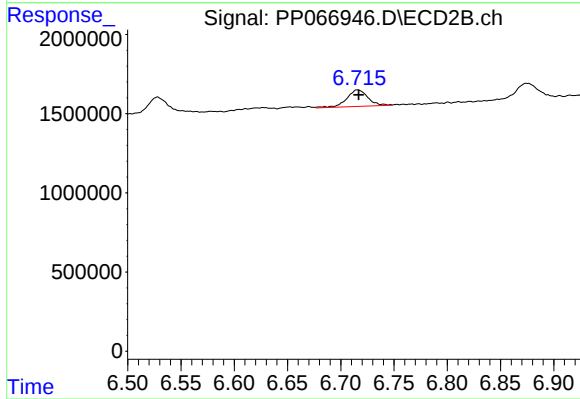


#32 AR-1260-2

R.T.: 6.716 min
Delta R.T.: -0.001 min
Response: 1425938
Conc: 21.09 ng/ml

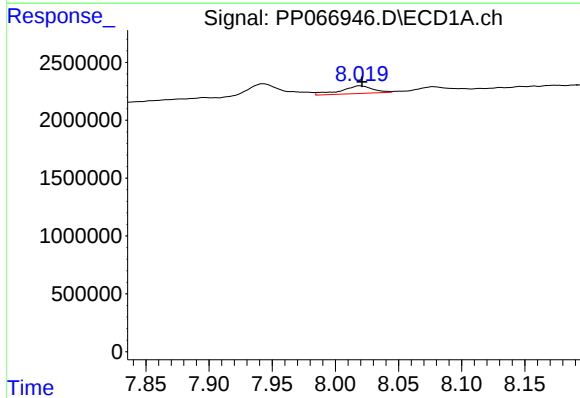


#33 AR-1260-3

R.T.: 8.020 min
Delta R.T.: -0.002 min
Response: 1162817
Conc: 26.05 ng/ml

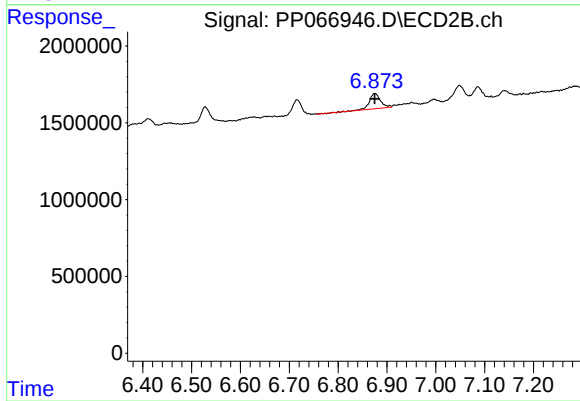

#33 AR-1260-3


R.T.: 6.875 min
Delta R.T.: 0.000 min
Response: 1585656
Conc: 23.81 ng/ml

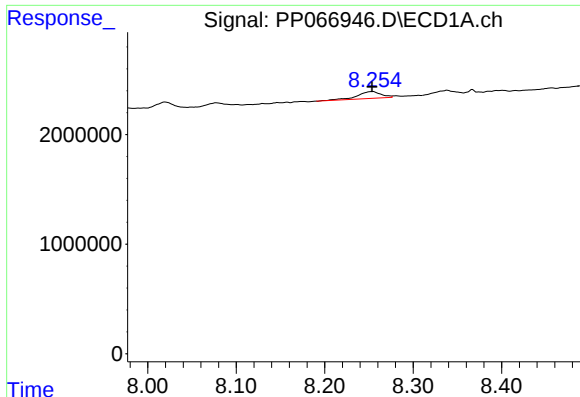

#34 AR-1260-4


R.T.: 8.254 min
Delta R.T.: 0.000 min
Response: 1188641
Conc: 23.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

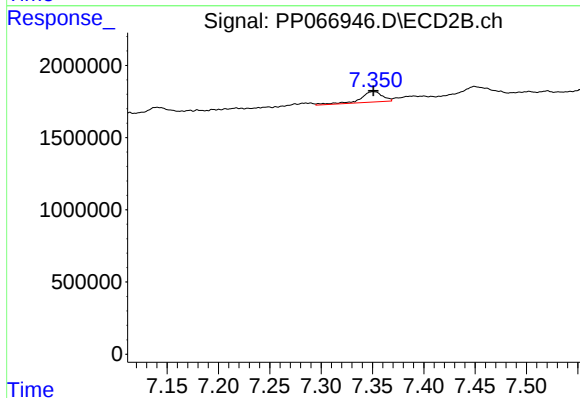


#34 AR-1260-4

R.T.: 7.351 min
Delta R.T.: 0.000 min
Response: 1091101
Conc: 24.90 ng/ml

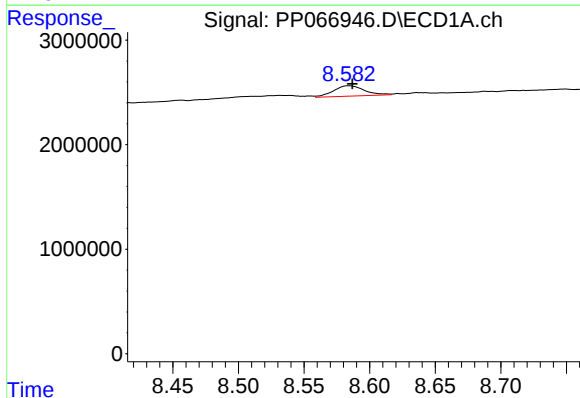


#35 AR-1260-5

R.T.: 8.584 min
Delta R.T.: -0.003 min
Response: 1631850
Conc: 19.53 ng/ml

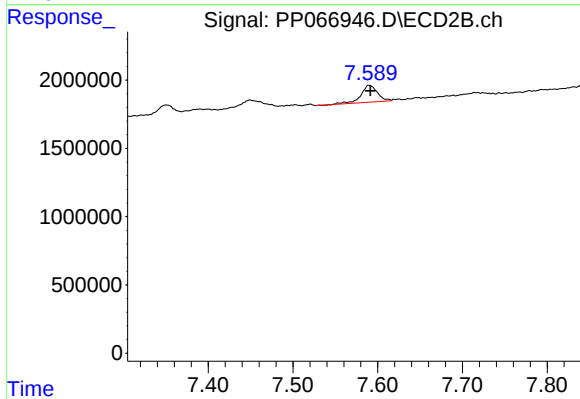

#35 AR-1260-5


R.T.: 7.590 min
Delta R.T.: -0.001 min
Response: 1675040
Conc: 18.78 ng/ml

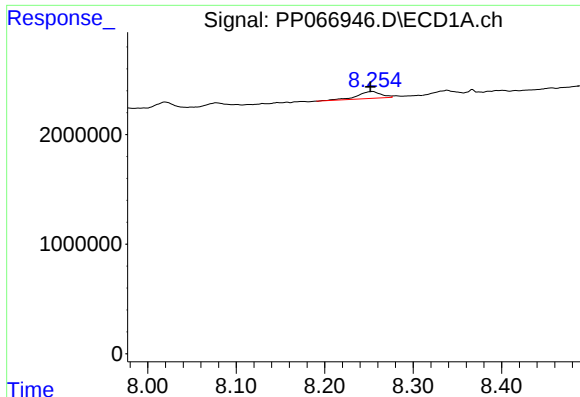

#36 AR-1262-1


R.T.: 8.254 min
Delta R.T.: 0.003 min
Response: 1188641
Conc: 18.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

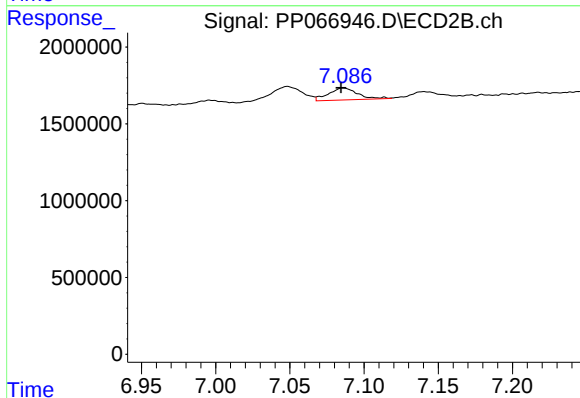


#36 AR-1262-1

R.T.: 7.086 min
Delta R.T.: 0.002 min
Response: 1078224
Conc: 14.92 ng/ml

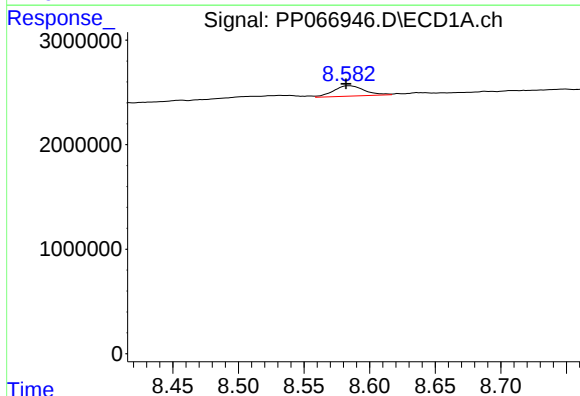


#37 AR-1262-2

R.T.: 8.584 min
Delta R.T.: 0.002 min
Response: 1631850
Conc: 15.78 ng/ml

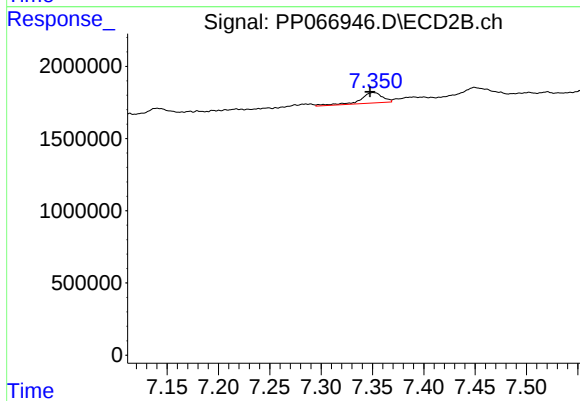

#37 AR-1262-2


R.T.: 7.351 min
Delta R.T.: 0.003 min
Response: 1091101
Conc: 17.73 ng/ml

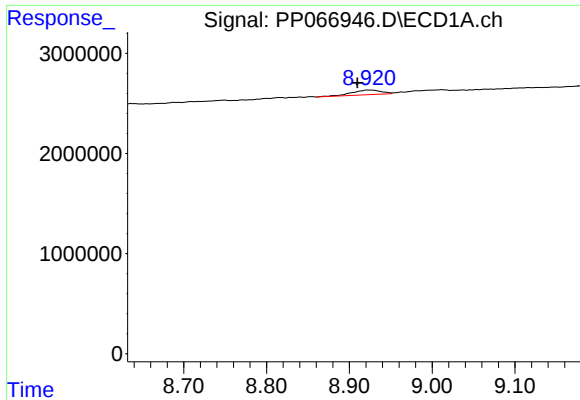

#38 AR-1262-3


R.T.: 8.922 min
Delta R.T.: 0.012 min
Response: 1150808
Conc: 16.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

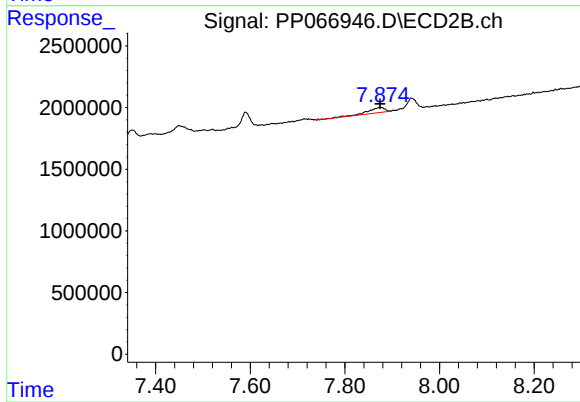


#38 AR-1262-3

R.T.: 7.874 min
Delta R.T.: 0.000 min
Response: 1088161
Conc: 25.87 ng/ml

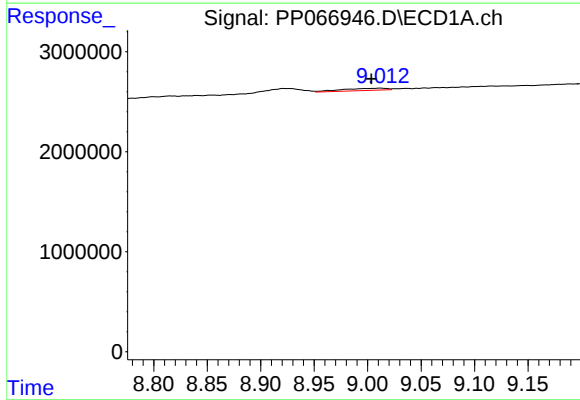


#39 AR-1262-4

R.T.: 9.012 min
Delta R.T.: 0.009 min
Response: 639400
Conc: 10.83 ng/ml

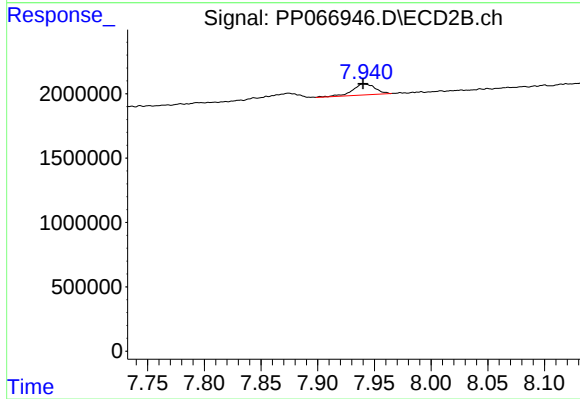

#39 AR-1262-4


R.T.: 7.941 min
Delta R.T.: 0.000 min
Response: 1194093
Conc: 15.39 ng/ml

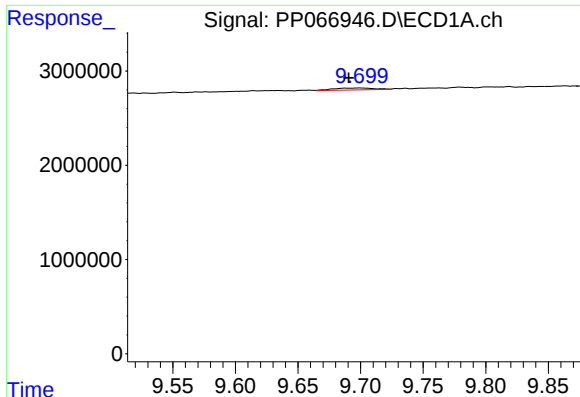

#40 AR-1262-5


R.T.: 9.700 min
Delta R.T.: 0.009 min
Response: 459356
Conc: 16.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

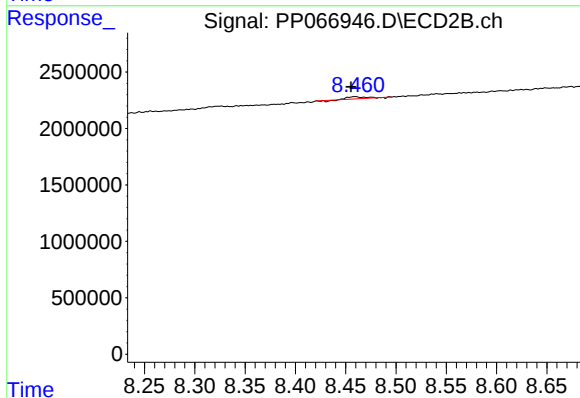


#40 AR-1262-5

R.T.: 8.459 min
Delta R.T.: 0.004 min
Response: 182484
Conc: 6.91 ng/ml

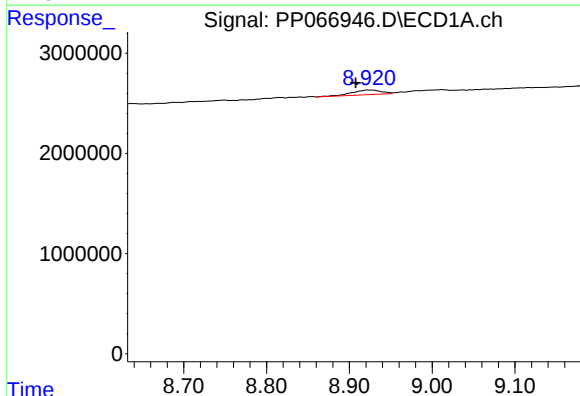


#41 AR-1268-1

R.T.: 8.922 min
Delta R.T.: 0.014 min
Response: 1150808
Conc: 8.81 ng/ml

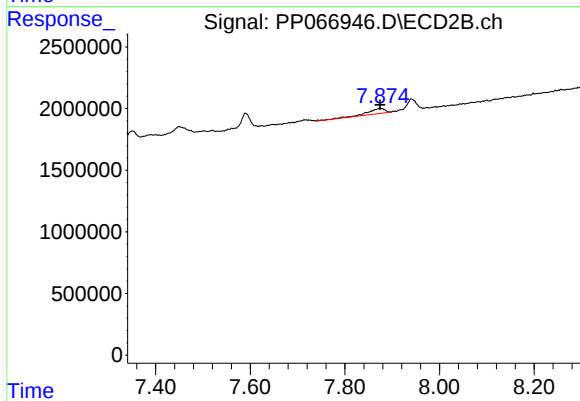

#41 AR-1268-1


R.T.: 7.874 min
Delta R.T.: 0.000 min
Response: 1088161
Conc: 8.70 ng/ml

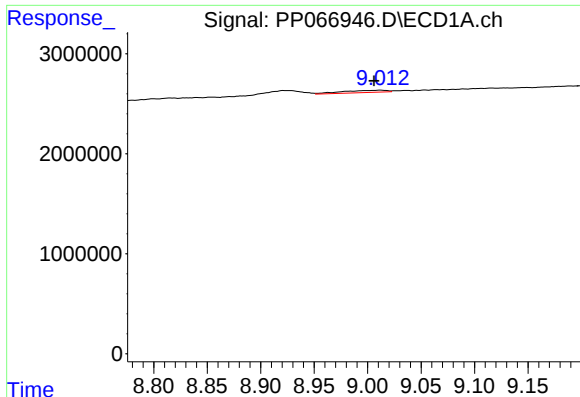

#42 AR-1268-2


R.T.: 9.012 min
Delta R.T.: 0.006 min
Response: 639400
Conc: 5.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

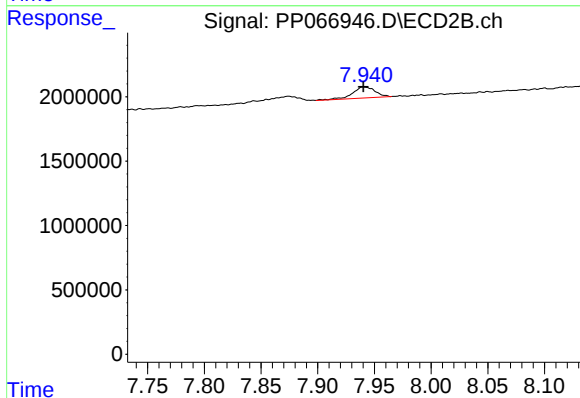


#42 AR-1268-2

R.T.: 7.941 min
Delta R.T.: 0.000 min
Response: 1194093
Conc: 10.68 ng/ml

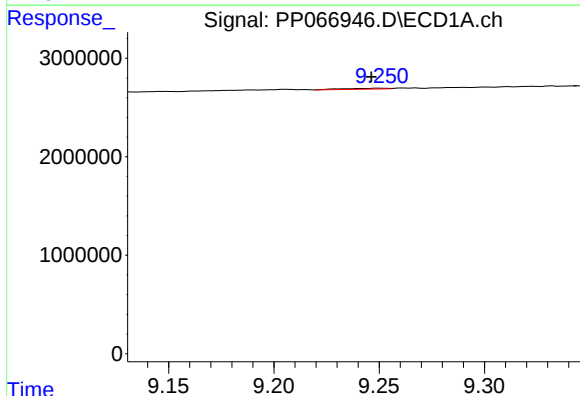


#43 AR-1268-3

R.T.: 9.250 min
Delta R.T.: 0.004 min
Response: 133651
Conc: 1.28 ng/ml

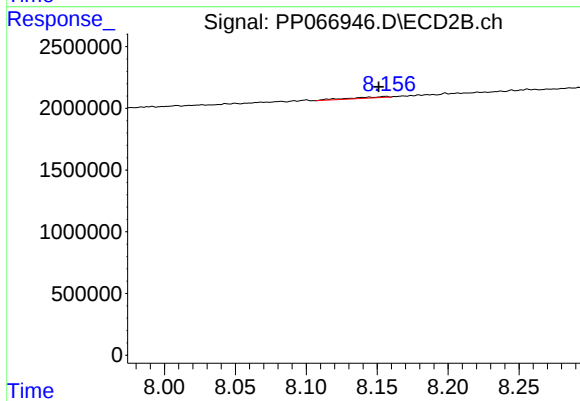

#43 AR-1268-3


R.T.: 8.156 min
Delta R.T.: 0.005 min
Response: 187566
Conc: 1.83 ng/ml

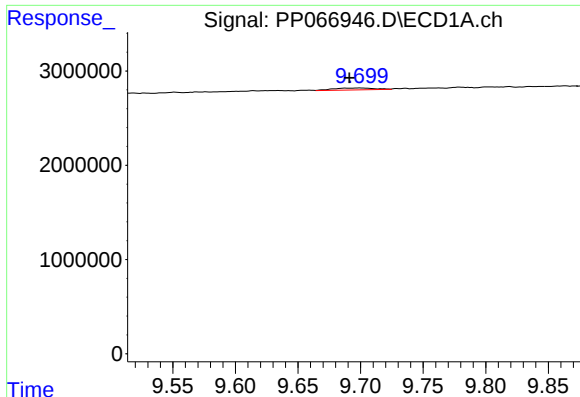

#44 AR-1268-4


R.T.: 9.700 min
Delta R.T.: 0.009 min
Response: 459356
Conc: 15.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

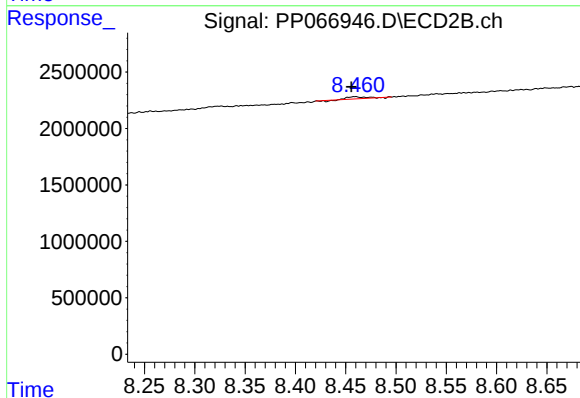


#44 AR-1268-4

R.T.: 8.459 min
Delta R.T.: 0.004 min
Response: 182484
Conc: 6.43 ng/ml

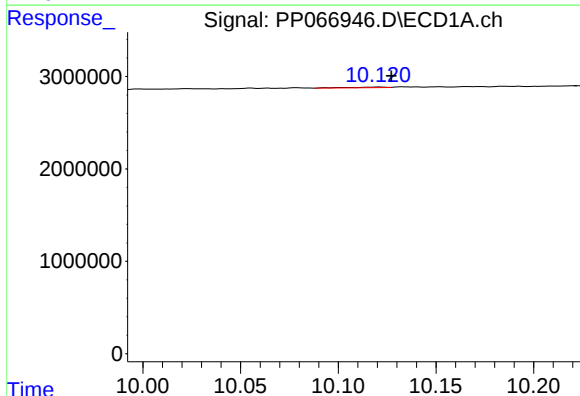

#45 AR-1268-5

R.T.: 10.122 min
Delta R.T.: -0.006 min
Response: 98360
Conc: 0.35 ng/ml

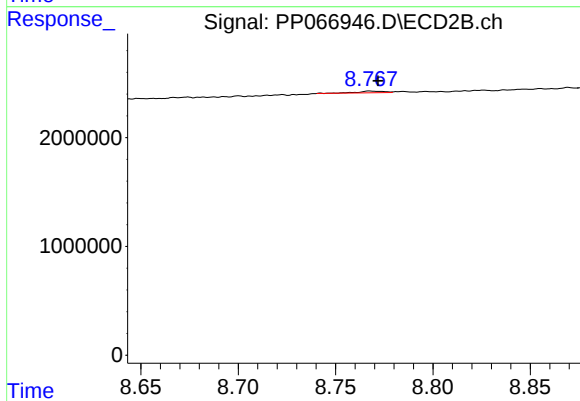

#45 AR-1268-5

R.T.: 8.768 min
Delta R.T.: -0.004 min
Response: 143680
Conc: 0.59 ng/ml