

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
 Data File : PP066947.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2024 14:00
 Operator : YP\AJ
 Sample : P3390-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 04:35:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 09:05:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.626	3.915	28515975	23123298	16.942	16.132
2)	SA Decachlor...	10.489	9.054	12311115	11576878	14.682	15.457
Target Compounds							
3)	L1 AR-1016-1	5.827	5.024	225280	152083	4.761	3.484 #
4)	L1 AR-1016-2	5.827	5.046	225280	121964	3.045	1.895 #
5)	L1 AR-1016-3	5.884	5.227	69319	329697	1.477	9.601 #
6)	L1 AR-1016-4	5.987	5.269	55329	210544	1.530	6.951 #
7)	L1 AR-1016-5	6.240f	5.445f	89851	98861	2.623	2.739
8)	L2 AR-1221-1	4.836	4.133	382815	305887	21.103	19.669
9)	L2 AR-1221-2	4.932	4.224	672298	584658	49.939	49.968
10)	L2 AR-1221-3	4.998	4.298	997489	894900	24.681	23.504
11)	L3 AR-1232-1	4.998	4.298	997489	894900	29.921	28.434
12)	L3 AR-1232-2	5.528	5.046	53044	121964	3.005	4.136 #
13)	L3 AR-1232-3	5.827	5.227	225280	329697	7.215	23.215 #
14)	L3 AR-1232-4	5.987	5.269f	55329	210544	3.616	14.979 #
15)	L3 AR-1232-5	6.080	5.445f	124229	98861	9.873	6.950 #
16)	L4 AR-1242-1	5.827	5.024	225280	152083	6.549	4.896 #
17)	L4 AR-1242-2	5.827	5.046	225280	121964	4.241	2.733 #
18)	L4 AR-1242-3	5.884	5.227	69319	329697	2.021	13.667 #
19)	L4 AR-1242-4	5.987	5.269f	55329	210544	2.132	7.868 #
20)	L4 AR-1242-5	6.735	5.827	94331	255156	4.060	9.142 #
21)	L5 AR-1248-1	5.827	5.024	225280	152083	9.332	6.910 #
22)	L5 AR-1248-2	6.080	5.269	124229	210544	3.190	5.993 #
23)	L5 AR-1248-3	6.240f	5.269f	89851	210544	2.206	5.786 #
24)	L5 AR-1248-4	6.694	5.445f	120181	98861	3.102	2.433
25)	L5 AR-1248-5	6.735	5.867	94331	373472	2.396	11.691 #
26)	L6 AR-1254-1	6.657	5.827	331027	255156	6.653	4.300 #
27)	L6 AR-1254-2	6.933f	6.039f	535242	395945	7.577	7.556
28)	L6 AR-1254-3	7.246	0.000	438982	0	6.443	N.D. #
29)	L6 AR-1254-4	7.522	6.629	384712	314034	9.188	8.313
30)	L6 AR-1254-5	7.947	7.049	1200438	696040	22.846	11.059 #
31)	L7 AR-1260-1	7.405	6.553	168992	1173759	2.792	18.529 #
32)	L7 AR-1260-2	7.660	6.713	237415	308444	3.693	4.562
33)	L7 AR-1260-3	8.020	6.885	41662	457436	0.933	6.868 #
34)	L7 AR-1260-4	8.250	7.395f	185571	648924	3.704	14.806 #
35)	L7 AR-1260-5	8.604	0.000	261414	0	3.128	N.D. #
36)	L8 AR-1262-1	8.250	7.049f	185571	696040	2.838	9.634 #
37)	L8 AR-1262-2	8.604	7.395f	261414	648924	2.527	10.546 #
38)	L8 AR-1262-3	8.919	7.866	129787	825264	1.817	19.619 #
39)	L8 AR-1262-4	9.017	0.000	50402	0	0.854	N.D. #
40)	L8 AR-1262-5	9.696	0.000	35063	0	1.274	N.D. #
41)	L9 AR-1268-1	8.919	7.866	129787	825264	0.993	6.598 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
Data File : PP066947.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2024 14:00
Operator : YP\AJ
Sample : P3390-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 04:35:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 09:05:47 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm


	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	
42)	L9 AR-1268-2	9.017	0.000	50402	0	0.431	N.D.	#
43)	L9 AR-1268-3	9.249	0.000	161710	0	1.554	N.D.	#
44)	L9 AR-1268-4	9.696	0.000	35063	0	1.171	N.D.	#
45)	L9 AR-1268-5	10.176f	0.000	38624	0	0.138	N.D.	#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-OT3-2024

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

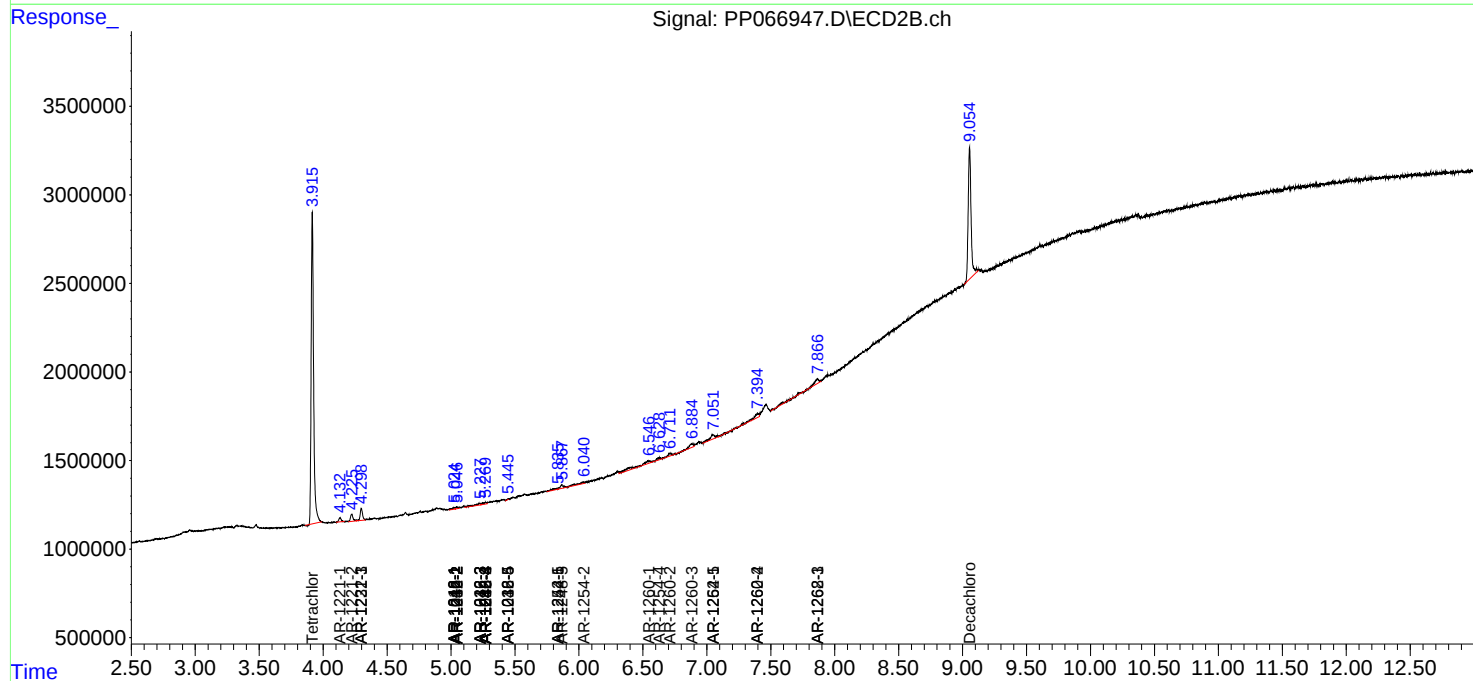


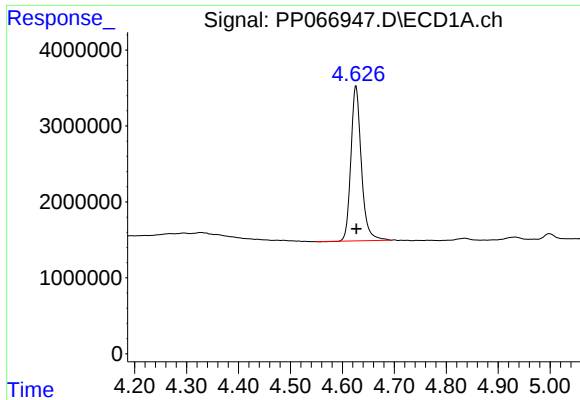

#1 Tetrachloro-m-xylene


R.T.: 4.626 min
Delta R.T.: 0.000 min
Response: 28515975
Conc: 16.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

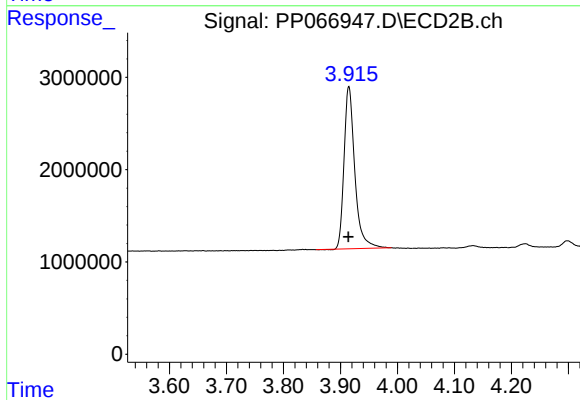


#1 Tetrachloro-m-xylene

R.T.: 3.915 min
Delta R.T.: 0.001 min
Response: 23123298
Conc: 16.13 ng/ml

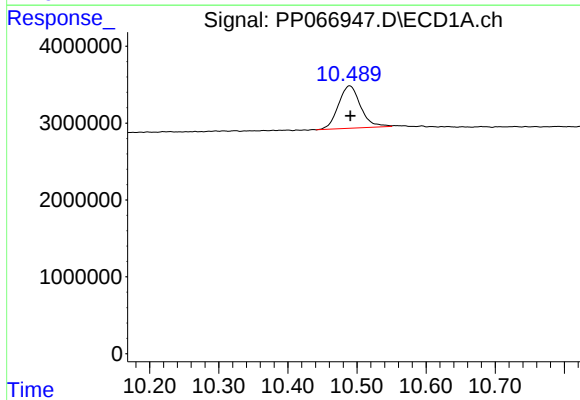


#2 Decachlorobiphenyl

R.T.: 10.489 min
Delta R.T.: 0.000 min
Response: 12311115
Conc: 14.68 ng/ml

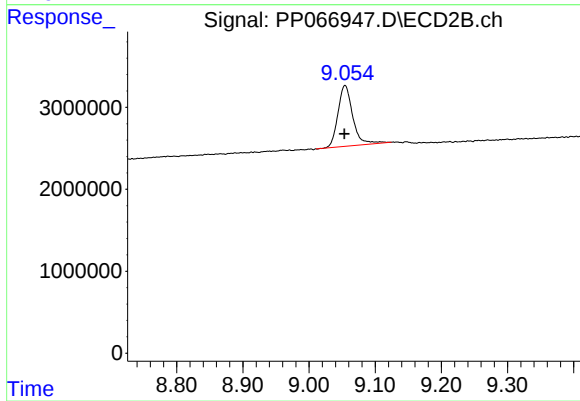

#2 Decachlorobiphenyl


R.T.: 9.054 min
Delta R.T.: 0.000 min
Response: 11576878
Conc: 15.46 ng/ml

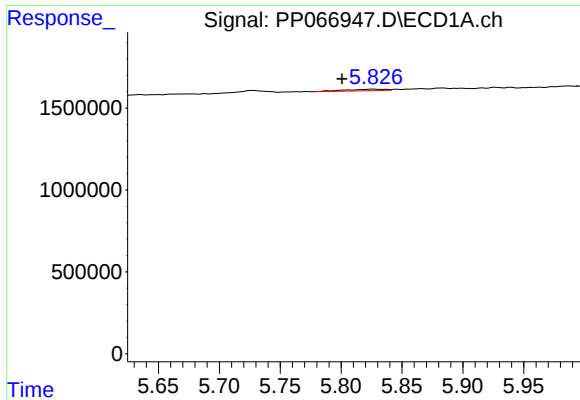

#3 AR-1016-1


R.T.: 5.827 min
Delta R.T.: 0.026 min
Response: 225280
Conc: 4.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

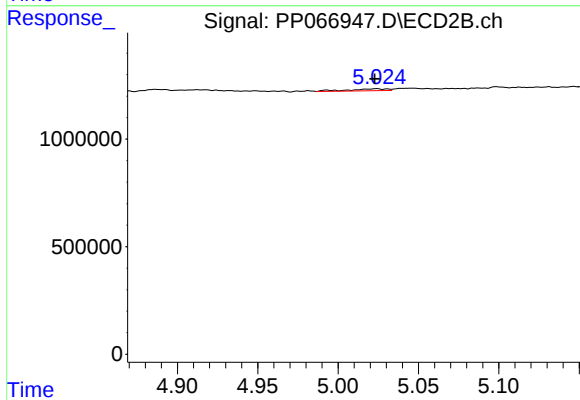


#3 AR-1016-1

R.T.: 5.024 min
Delta R.T.: 0.001 min
Response: 152083
Conc: 3.48 ng/ml

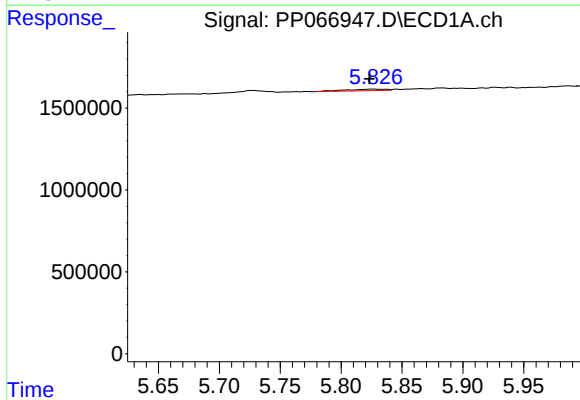


#4 AR-1016-2

R.T.: 5.827 min
Delta R.T.: 0.004 min
Response: 225280
Conc: 3.04 ng/ml

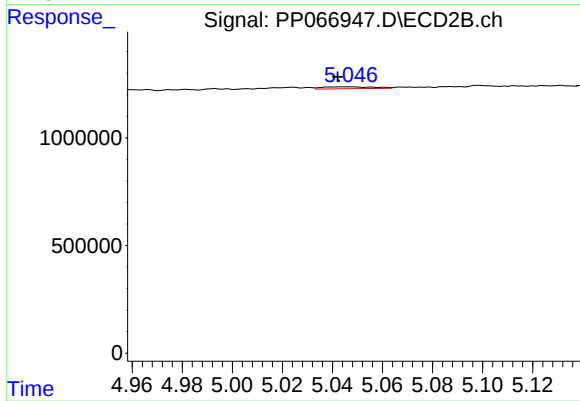

#4 AR-1016-2


R.T.: 5.046 min
Delta R.T.: 0.004 min
Response: 121964
Conc: 1.90 ng/ml

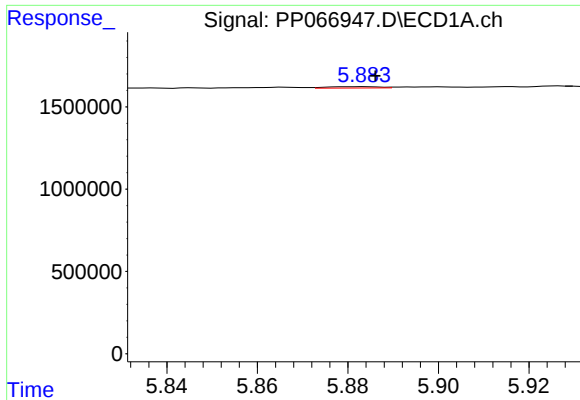

#5 AR-1016-3


R.T.: 5.884 min
Delta R.T.: -0.002 min
Response: 69319
Conc: 1.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

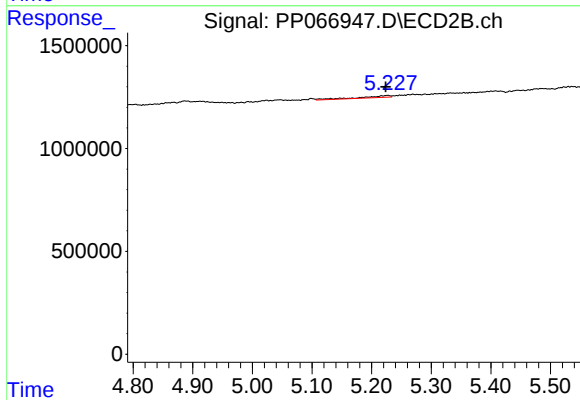


#5 AR-1016-3

R.T.: 5.227 min
Delta R.T.: 0.003 min
Response: 329697
Conc: 9.60 ng/ml

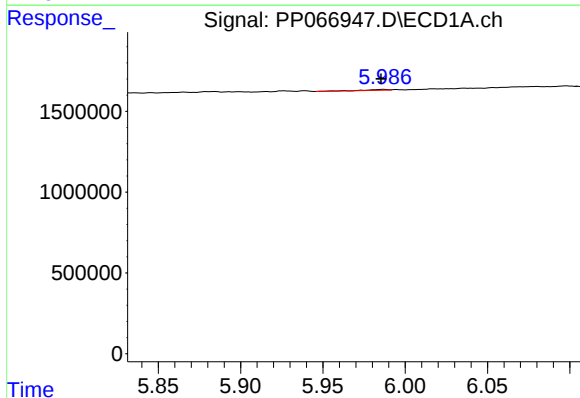


#6 AR-1016-4

R.T.: 5.987 min
Delta R.T.: 0.001 min
Response: 55329
Conc: 1.53 ng/ml

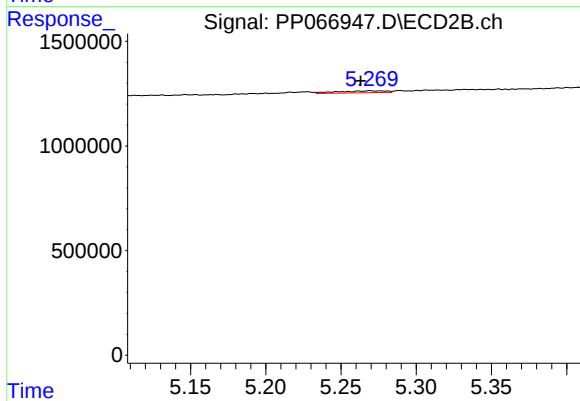

#6 AR-1016-4


R.T.: 5.269 min
Delta R.T.: 0.006 min
Response: 210544
Conc: 6.95 ng/ml

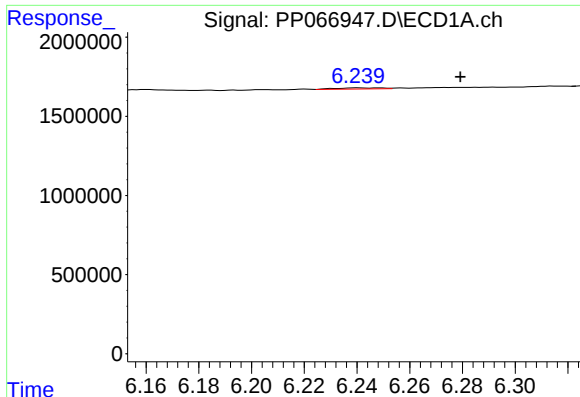

#7 AR-1016-5


R.T.: 6.240 min
Delta R.T.: -0.039 min
Response: 89851
Conc: 2.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

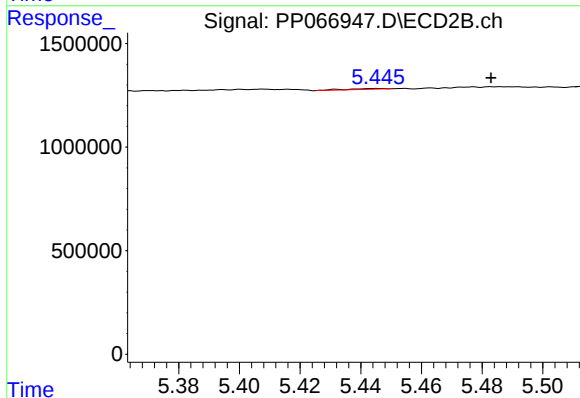


#7 AR-1016-5

R.T.: 5.445 min
Delta R.T.: -0.038 min
Response: 98861
Conc: 2.74 ng/ml

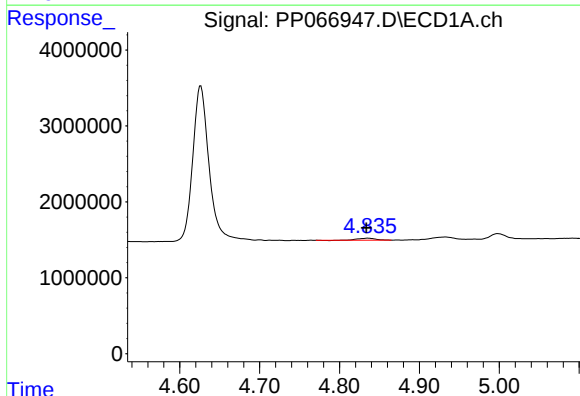


#8 AR-1221-1

R.T.: 4.836 min
Delta R.T.: 0.002 min
Response: 382815
Conc: 21.10 ng/ml

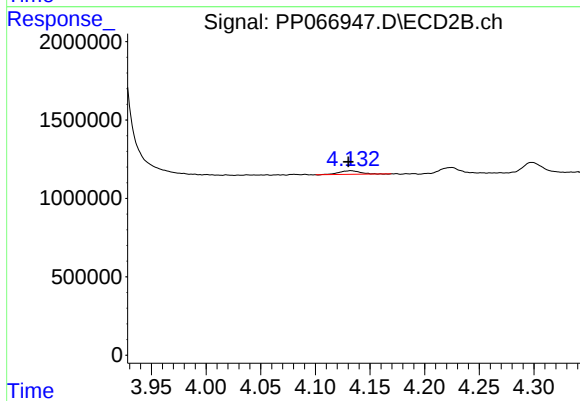

#8 AR-1221-1


R.T.: 4.133 min
Delta R.T.: 0.002 min
Response: 305887
Conc: 19.67 ng/ml

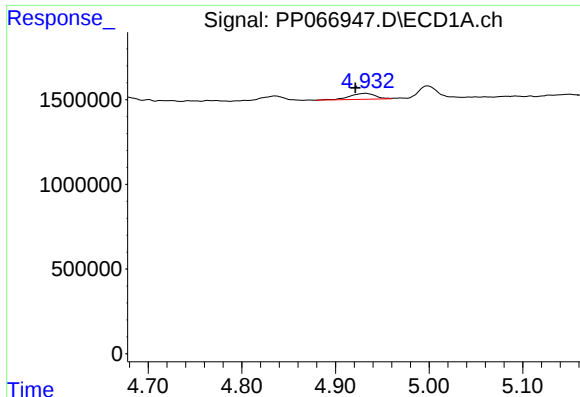

#9 AR-1221-2


R.T.: 4.932 min
Delta R.T.: 0.011 min
Response: 672298
Conc: 49.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

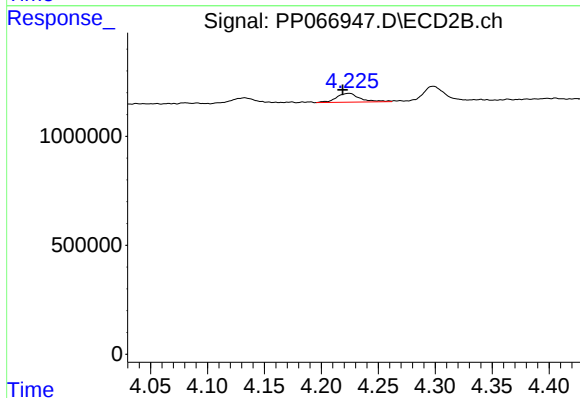


#9 AR-1221-2

R.T.: 4.224 min
Delta R.T.: 0.005 min
Response: 584658
Conc: 49.97 ng/ml

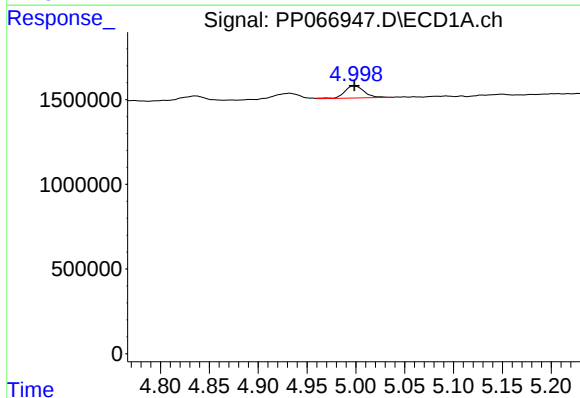


#10 AR-1221-3

R.T.: 4.998 min
Delta R.T.: 0.000 min
Response: 997489
Conc: 24.68 ng/ml

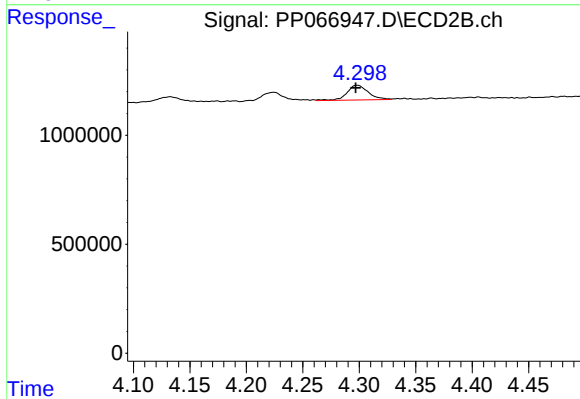

#10 AR-1221-3


R.T.: 4.298 min
Delta R.T.: 0.001 min
Response: 894900
Conc: 23.50 ng/ml

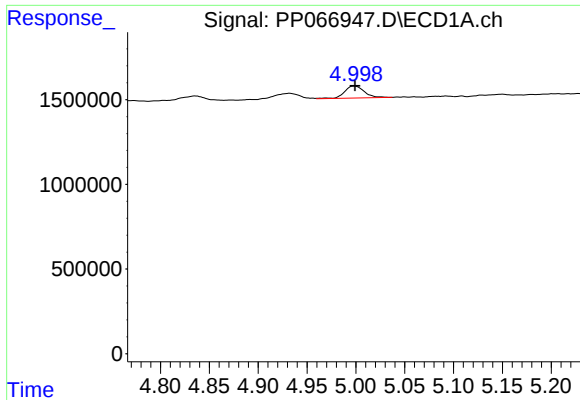

#11 AR-1232-1


R.T.: 4.998 min
Delta R.T.: 0.000 min
Response: 997489
Conc: 29.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

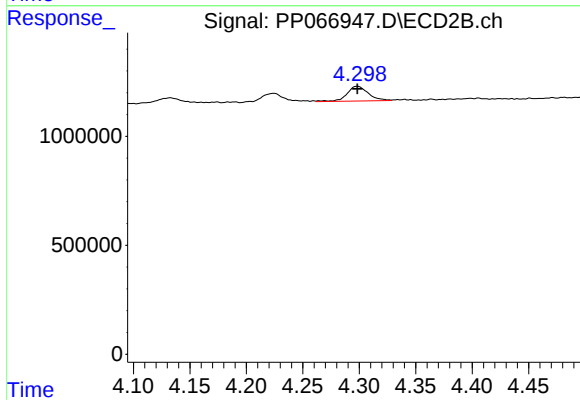


#11 AR-1232-1

R.T.: 4.298 min
Delta R.T.: 0.000 min
Response: 894900
Conc: 28.43 ng/ml

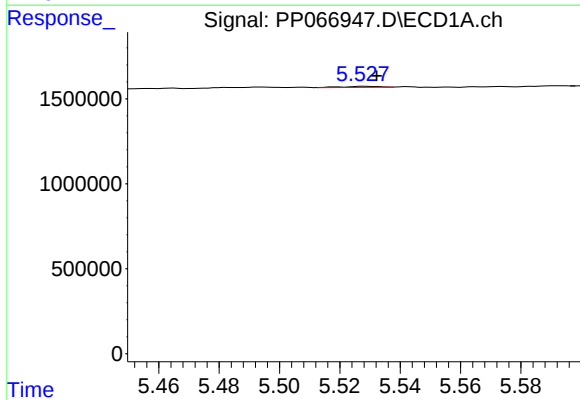


#12 AR-1232-2

R.T.: 5.528 min
Delta R.T.: -0.004 min
Response: 53044
Conc: 3.00 ng/ml

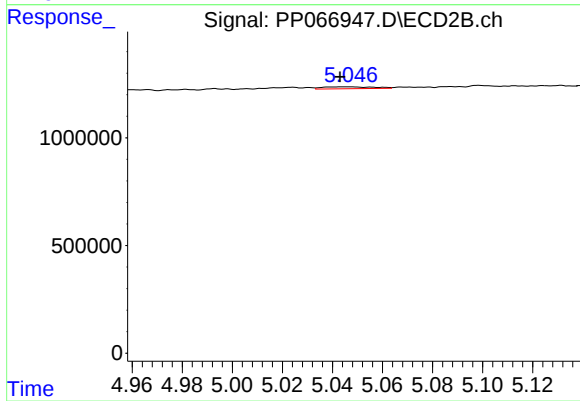

#12 AR-1232-2


R.T.: 5.046 min
Delta R.T.: 0.003 min
Response: 121964
Conc: 4.14 ng/ml

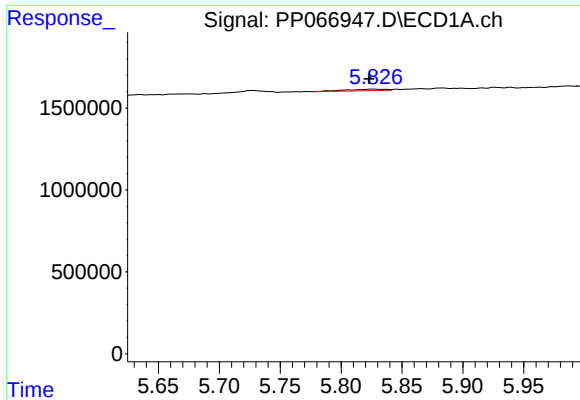

#13 AR-1232-3


R.T.: 5.827 min
Delta R.T.: 0.004 min
Response: 225280
Conc: 7.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

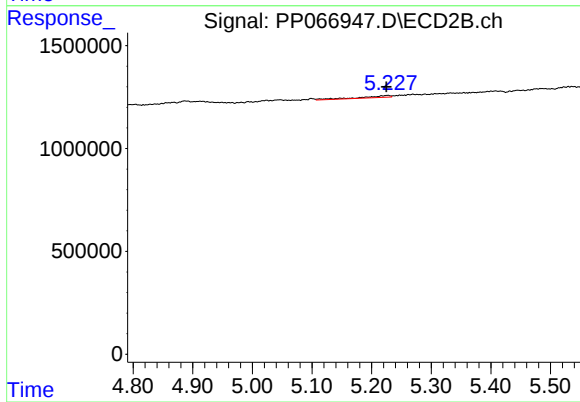


#13 AR-1232-3

R.T.: 5.227 min
Delta R.T.: 0.002 min
Response: 329697
Conc: 23.21 ng/ml

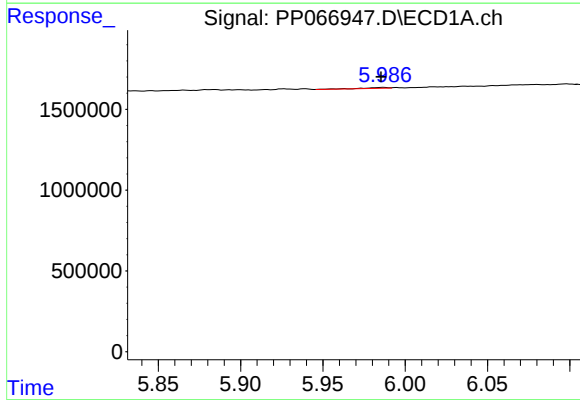


#14 AR-1232-4

R.T.: 5.987 min
Delta R.T.: 0.002 min
Response: 55329
Conc: 3.62 ng/ml

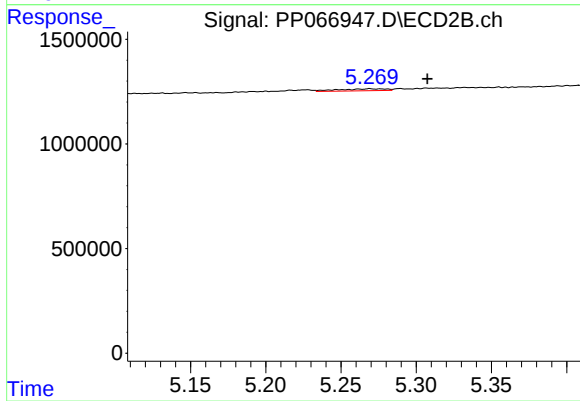

#14 AR-1232-4


R.T.: 5.269 min
Delta R.T.: -0.038 min
Response: 210544
Conc: 14.98 ng/ml

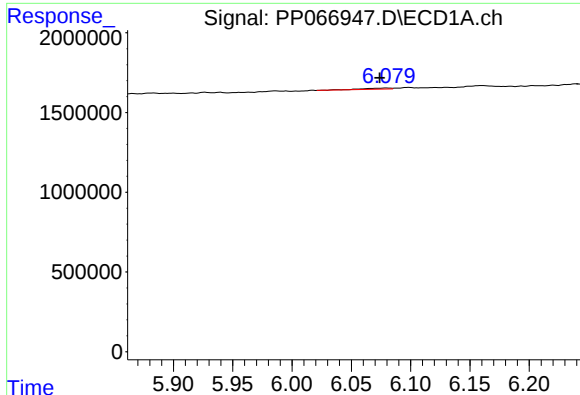

#15 AR-1232-5


R.T.: 6.080 min
Delta R.T.: 0.006 min
Response: 124229
Conc: 9.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

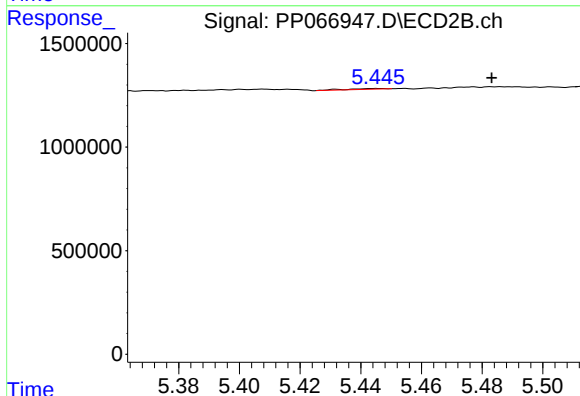


#15 AR-1232-5

R.T.: 5.445 min
Delta R.T.: -0.038 min
Response: 98861
Conc: 6.95 ng/ml

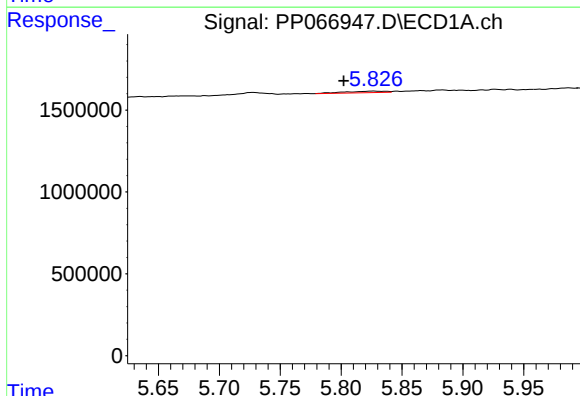


#16 AR-1242-1

R.T.: 5.827 min
Delta R.T.: 0.025 min
Response: 225280
Conc: 6.55 ng/ml

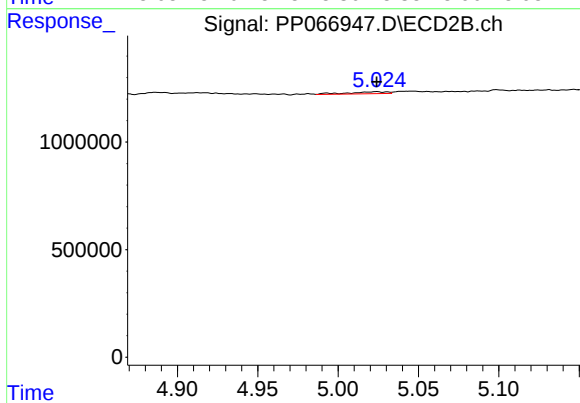

#16 AR-1242-1


R.T.: 5.024 min
Delta R.T.: 0.000 min
Response: 152083
Conc: 4.90 ng/ml

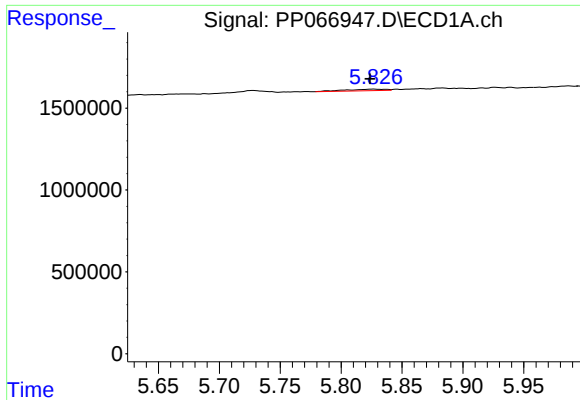

#17 AR-1242-2


R.T.: 5.827 min
Delta R.T.: 0.003 min
Response: 225280
Conc: 4.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

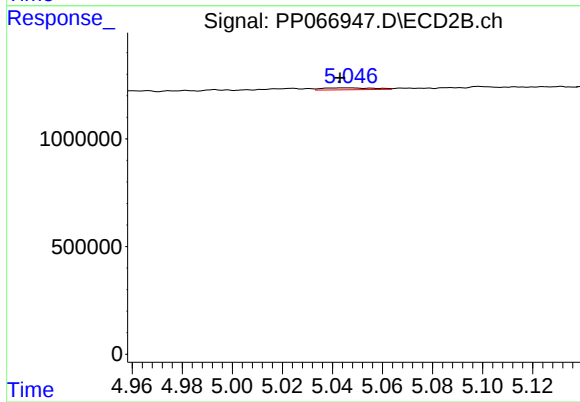


#17 AR-1242-2

R.T.: 5.046 min
Delta R.T.: 0.003 min
Response: 121964
Conc: 2.73 ng/ml

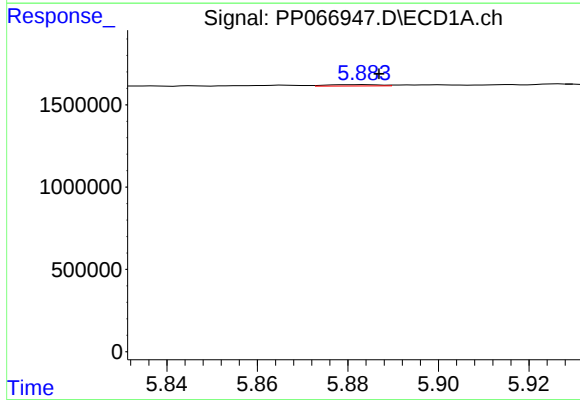


#18 AR-1242-3

R.T.: 5.884 min
Delta R.T.: -0.003 min
Response: 69319
Conc: 2.02 ng/ml

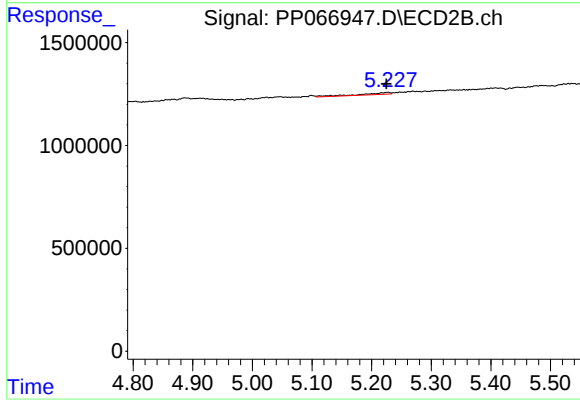

#18 AR-1242-3


R.T.: 5.227 min
Delta R.T.: 0.002 min
Response: 329697
Conc: 13.67 ng/ml

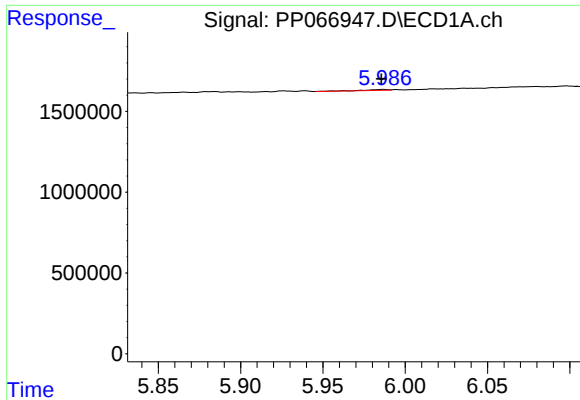

#19 AR-1242-4


R.T.: 5.987 min
Delta R.T.: 0.001 min
Response: 55329
Conc: 2.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

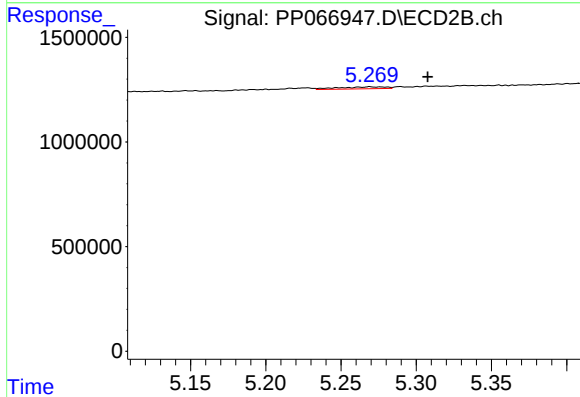


#19 AR-1242-4

R.T.: 5.269 min
Delta R.T.: -0.038 min
Response: 210544
Conc: 7.87 ng/ml

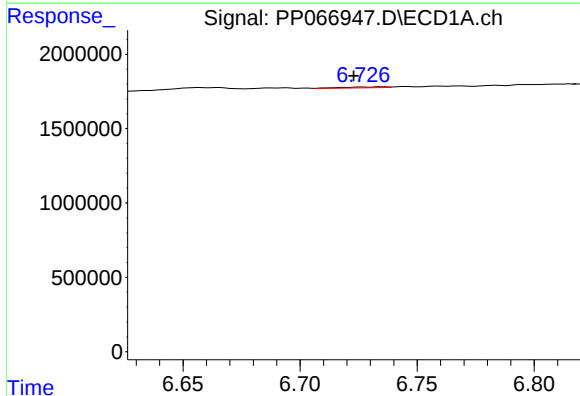


#20 AR-1242-5

R.T.: 6.735 min
Delta R.T.: 0.012 min
Response: 94331
Conc: 4.06 ng/ml

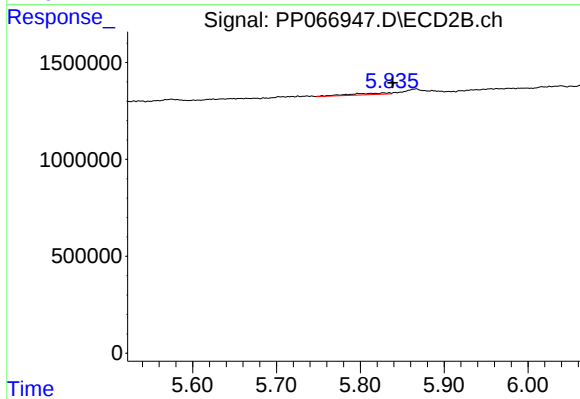

#20 AR-1242-5


R.T.: 5.827 min
Delta R.T.: -0.011 min
Response: 255156
Conc: 9.14 ng/ml

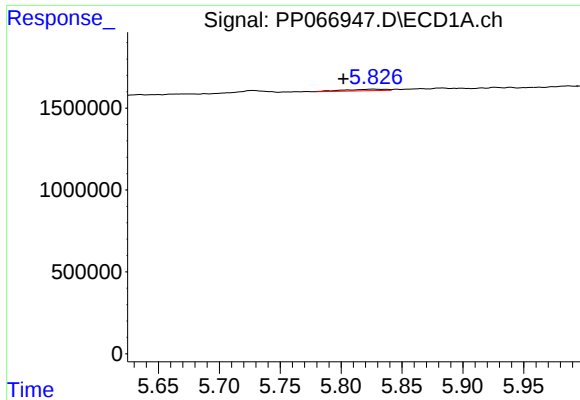

#21 AR-1248-1


R.T.: 5.827 min
Delta R.T.: 0.025 min
Response: 225280
Conc: 9.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

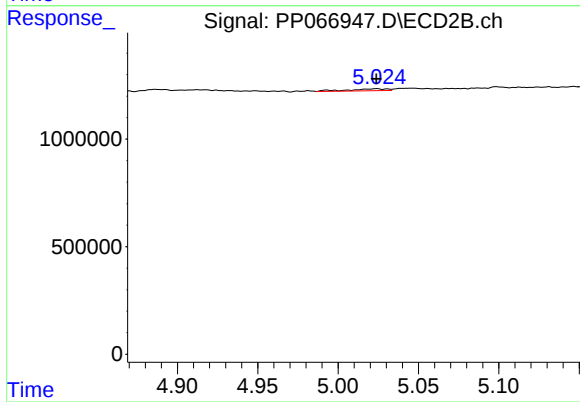


#21 AR-1248-1

R.T.: 5.024 min
Delta R.T.: 0.000 min
Response: 152083
Conc: 6.91 ng/ml

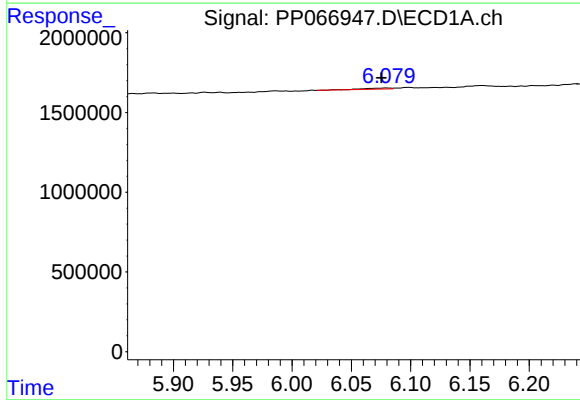


#22 AR-1248-2

R.T.: 6.080 min
Delta R.T.: 0.004 min
Response: 124229
Conc: 3.19 ng/ml

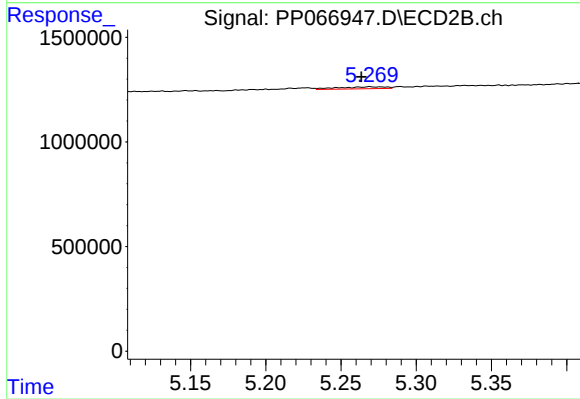

#22 AR-1248-2


R.T.: 5.269 min
Delta R.T.: 0.006 min
Response: 210544
Conc: 5.99 ng/ml

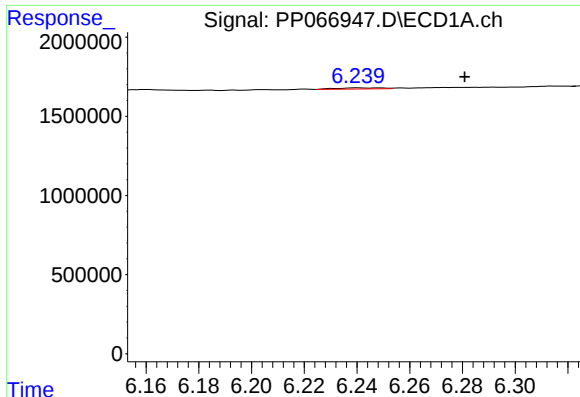

#23 AR-1248-3


R.T.: 6.240 min
Delta R.T.: -0.041 min
Response: 89851
Conc: 2.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

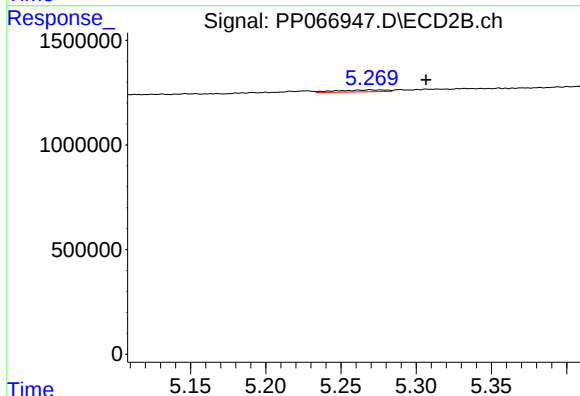


#23 AR-1248-3

R.T.: 5.269 min
Delta R.T.: -0.038 min
Response: 210544
Conc: 5.79 ng/ml

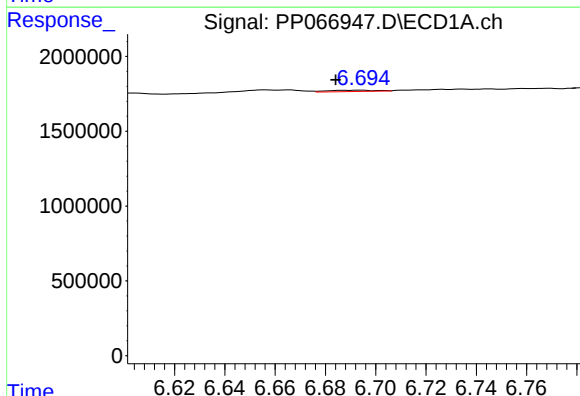


#24 AR-1248-4

R.T.: 6.694 min
Delta R.T.: 0.010 min
Response: 120181
Conc: 3.10 ng/ml

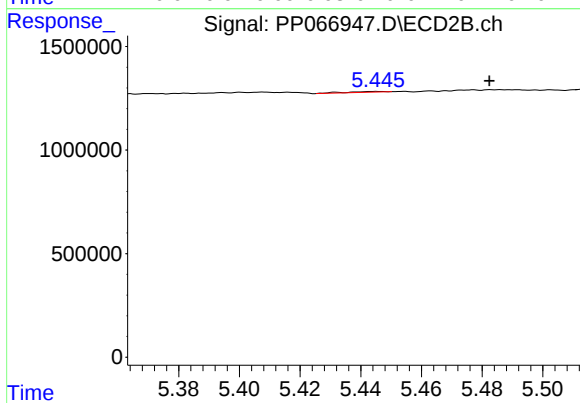

#24 AR-1248-4


R.T.: 5.445 min
Delta R.T.: -0.037 min
Response: 98861
Conc: 2.43 ng/ml

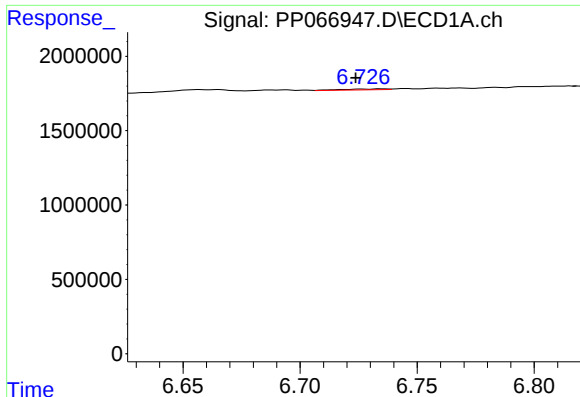

#25 AR-1248-5


R.T.: 6.735 min
Delta R.T.: 0.011 min
Response: 94331
Conc: 2.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

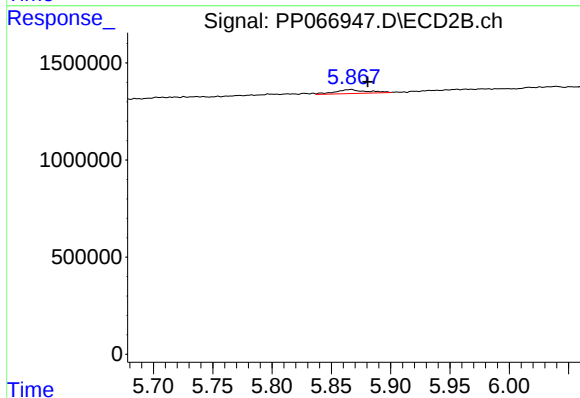


#25 AR-1248-5

R.T.: 5.867 min
Delta R.T.: -0.014 min
Response: 373472
Conc: 11.69 ng/ml

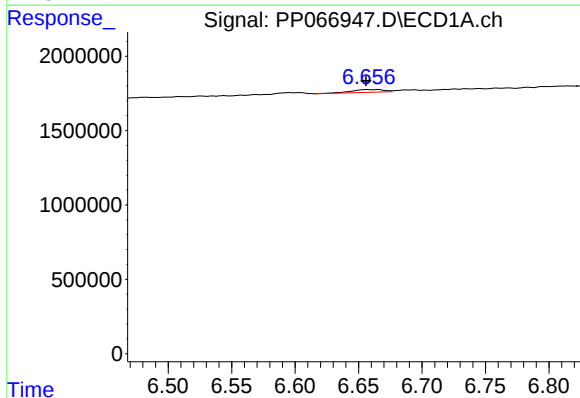


#26 AR-1254-1

R.T.: 6.657 min
Delta R.T.: 0.000 min
Response: 331027
Conc: 6.65 ng/ml

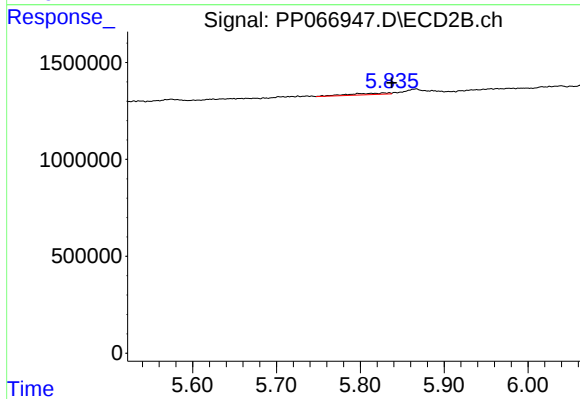

#26 AR-1254-1


R.T.: 5.827 min
Delta R.T.: -0.010 min
Response: 255156
Conc: 4.30 ng/ml

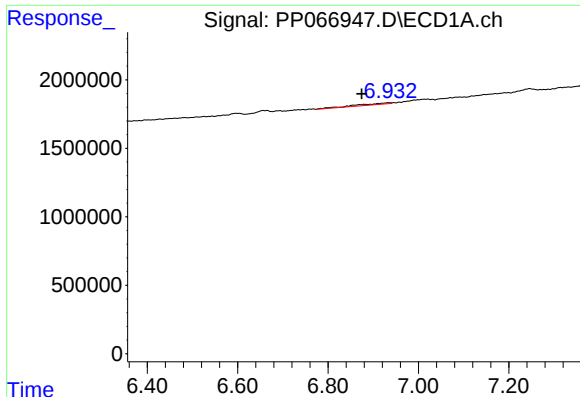

#27 AR-1254-2


R.T.: 6.933 min
Delta R.T.: 0.058 min
Response: 535242
Conc: 7.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

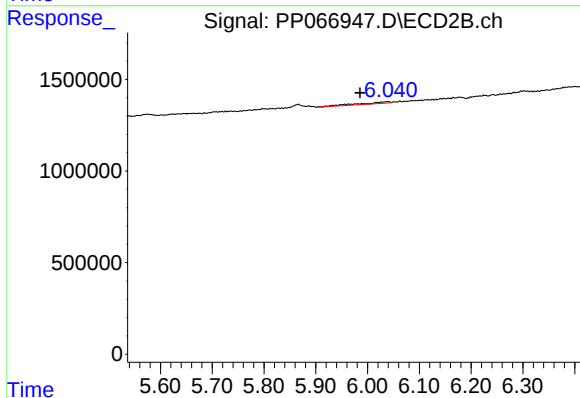


#27 AR-1254-2

R.T.: 6.039 min
Delta R.T.: 0.054 min
Response: 395945
Conc: 7.56 ng/ml

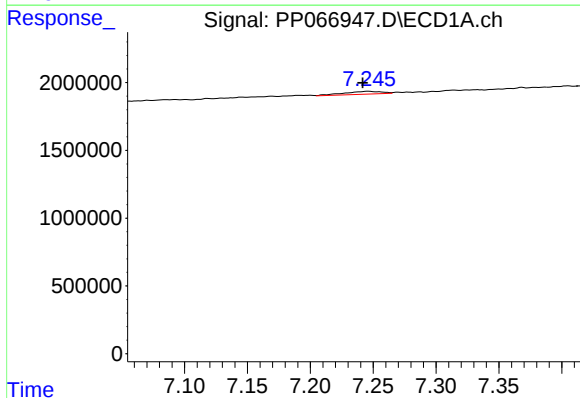


#28 AR-1254-3

R.T.: 7.246 min
Delta R.T.: 0.005 min
Response: 438982
Conc: 6.44 ng/ml

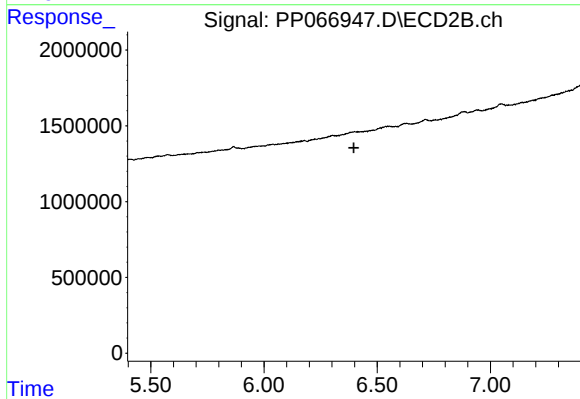

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.397 min
Response: 0
Conc: N.D.

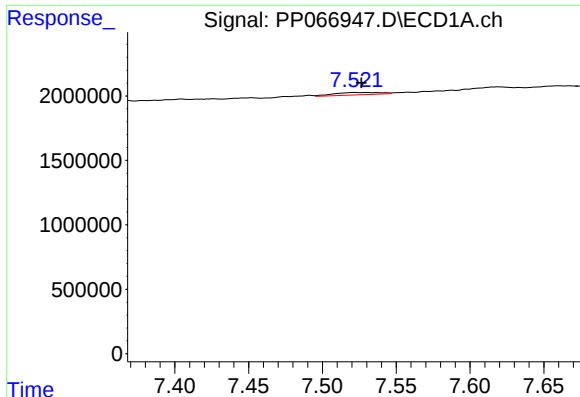

#29 AR-1254-4


R.T.: 7.522 min
Delta R.T.: -0.004 min
Response: 384712
Conc: 9.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

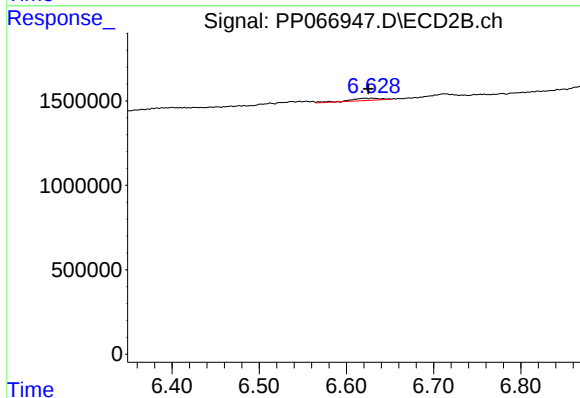


#29 AR-1254-4

R.T.: 6.629 min
Delta R.T.: 0.004 min
Response: 314034
Conc: 8.31 ng/ml

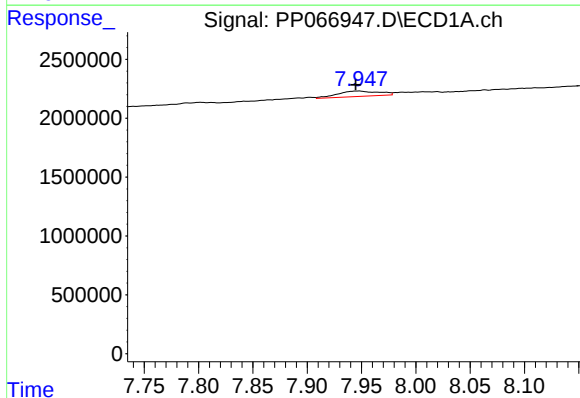


#30 AR-1254-5

R.T.: 7.947 min
Delta R.T.: 0.002 min
Response: 1200438
Conc: 22.85 ng/ml

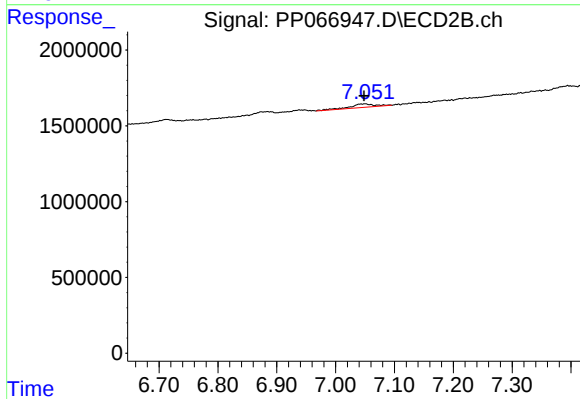

#30 AR-1254-5


R.T.: 7.049 min
Delta R.T.: 0.000 min
Response: 696040
Conc: 11.06 ng/ml

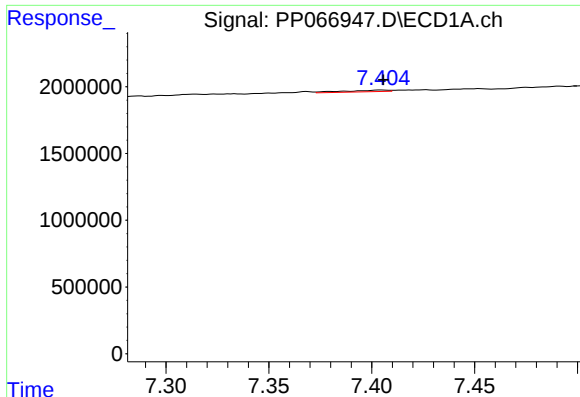

#31 AR-1260-1


R.T.: 7.405 min
Delta R.T.: 0.000 min
Response: 168992
Conc: 2.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

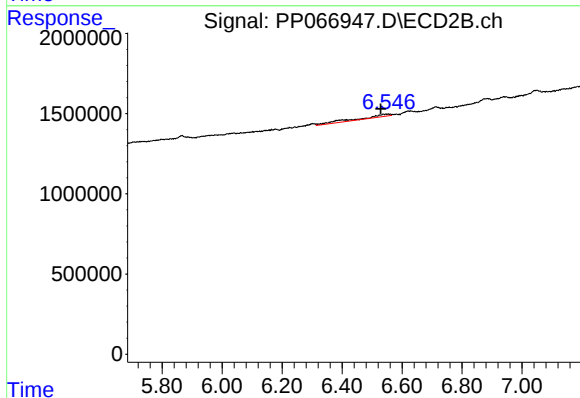


#31 AR-1260-1

R.T.: 6.553 min
Delta R.T.: 0.024 min
Response: 1173759
Conc: 18.53 ng/ml

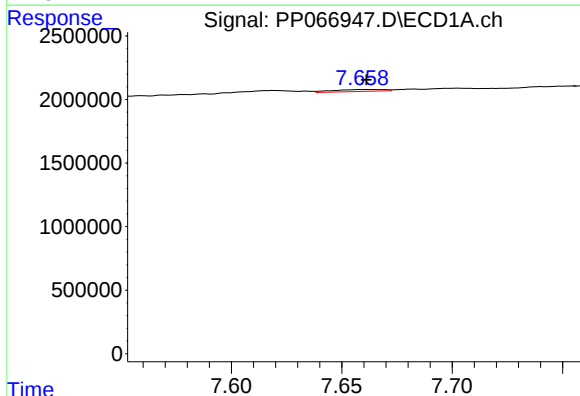


#32 AR-1260-2

R.T.: 7.660 min
Delta R.T.: -0.001 min
Response: 237415
Conc: 3.69 ng/ml

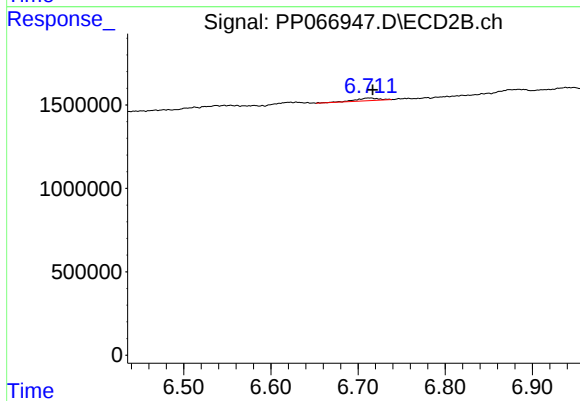

#32 AR-1260-2


R.T.: 6.713 min
Delta R.T.: -0.004 min
Response: 308444
Conc: 4.56 ng/ml

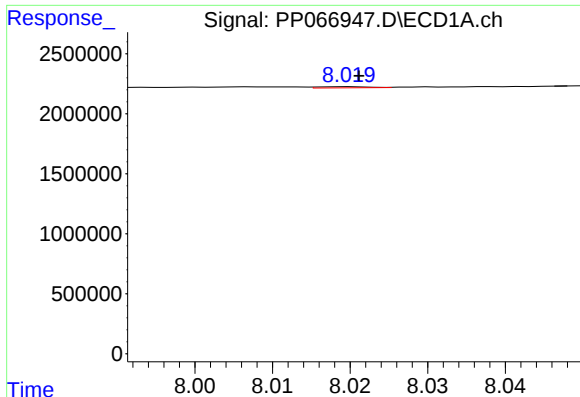

#33 AR-1260-3


R.T.: 8.020 min
Delta R.T.: -0.001 min
Response: 41662
Conc: 0.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

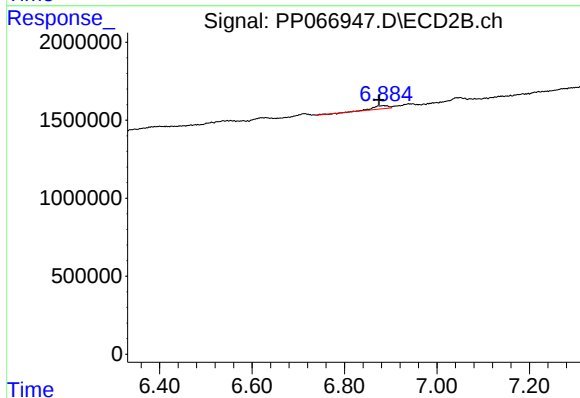


#33 AR-1260-3

R.T.: 6.885 min
Delta R.T.: 0.010 min
Response: 457436
Conc: 6.87 ng/ml

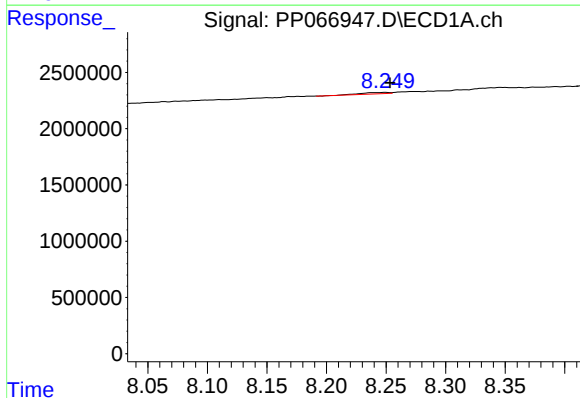


#34 AR-1260-4

R.T.: 8.250 min
Delta R.T.: -0.004 min
Response: 185571
Conc: 3.70 ng/ml

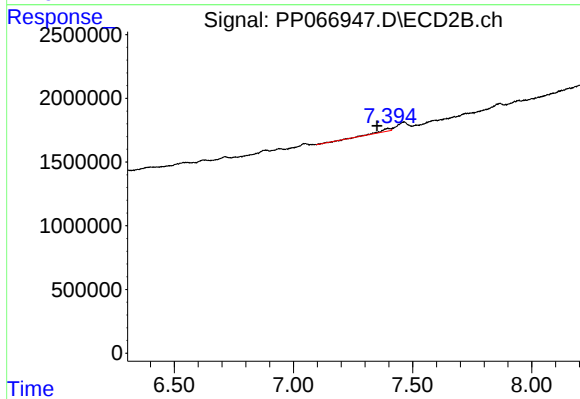

#34 AR-1260-4


R.T.: 7.395 min
Delta R.T.: 0.044 min
Response: 648924
Conc: 14.81 ng/ml

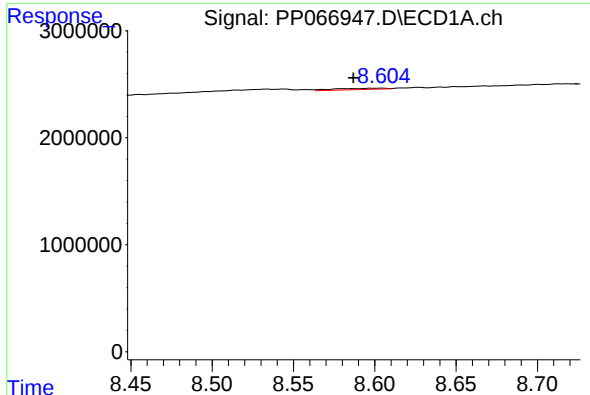

#35 AR-1260-5


R.T.: 8.604 min
Delta R.T.: 0.017 min
Response: 261414
Conc: 3.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

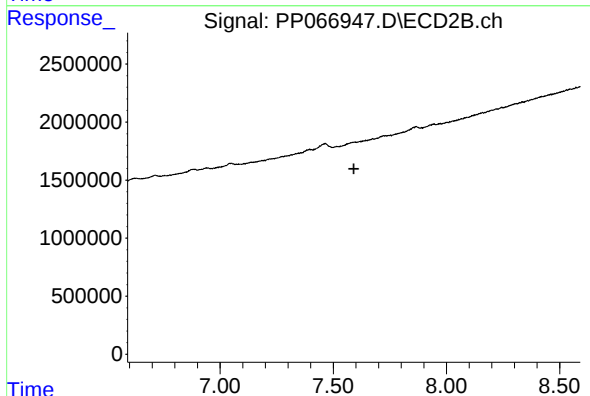


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.591 min
Response: 0
Conc: N.D.

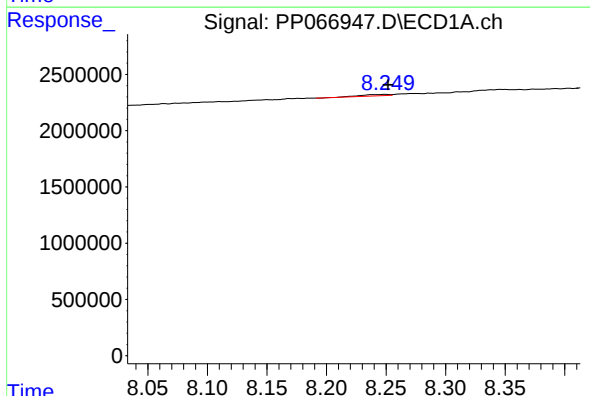


#36 AR-1262-1

R.T.: 8.250 min
Delta R.T.: -0.002 min
Response: 185571
Conc: 2.84 ng/ml

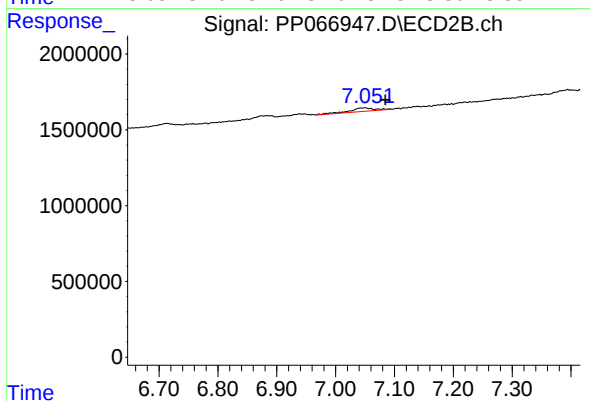

#36 AR-1262-1


R.T.: 7.049 min
Delta R.T.: -0.035 min
Response: 696040
Conc: 9.63 ng/ml

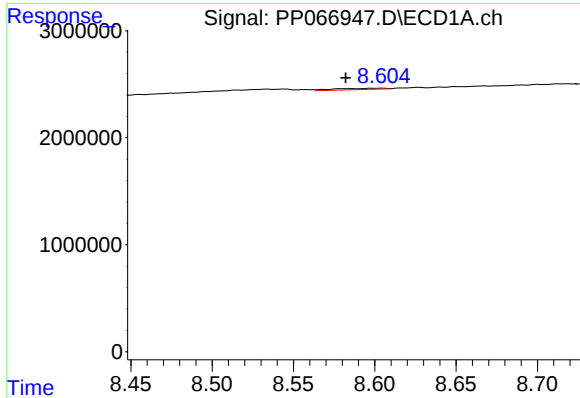

#37 AR-1262-2


R.T.: 8.604 min
Delta R.T.: 0.022 min
Response: 261414
Conc: 2.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

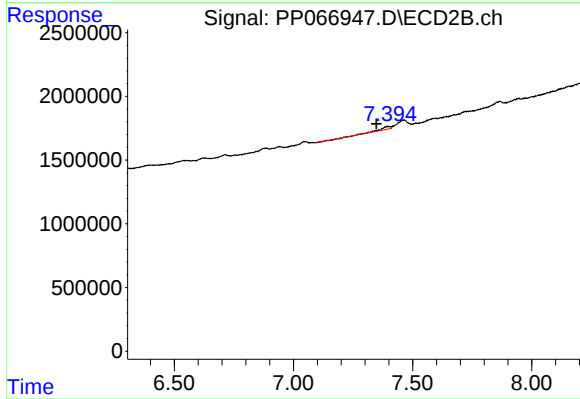


#37 AR-1262-2

R.T.: 7.395 min
Delta R.T.: 0.048 min
Response: 648924
Conc: 10.55 ng/ml

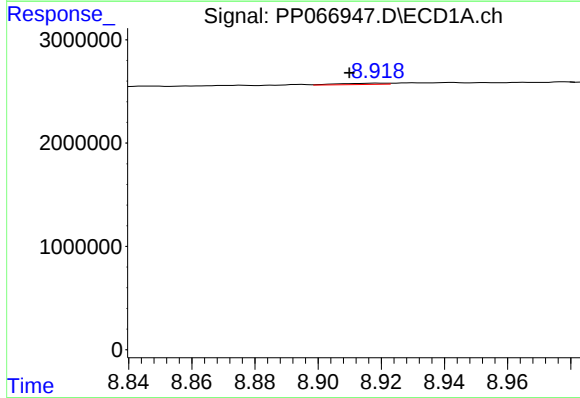


#38 AR-1262-3

R.T.: 8.919 min
Delta R.T.: 0.009 min
Response: 129787
Conc: 1.82 ng/ml

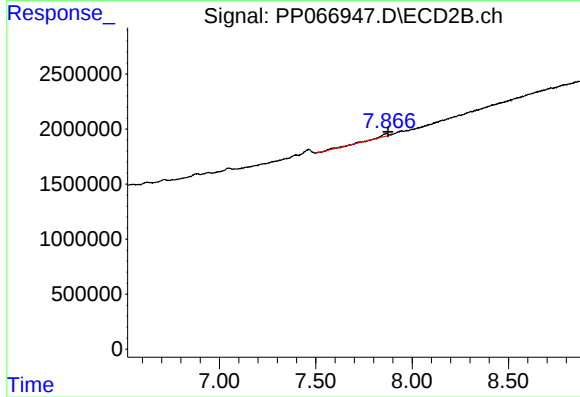

#38 AR-1262-3


R.T.: 7.866 min
Delta R.T.: -0.008 min
Response: 825264
Conc: 19.62 ng/ml

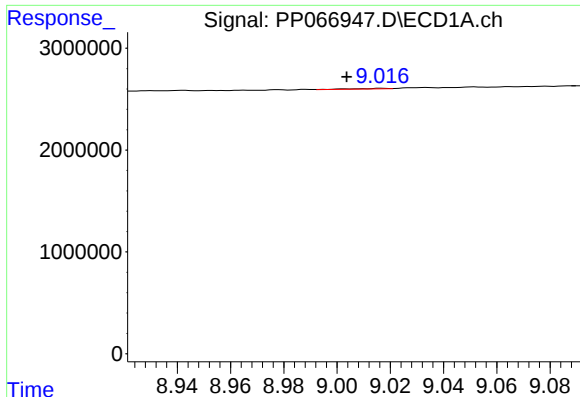

#39 AR-1262-4


R.T.: 9.017 min
Delta R.T.: 0.013 min
Response: 50402
Conc: 0.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

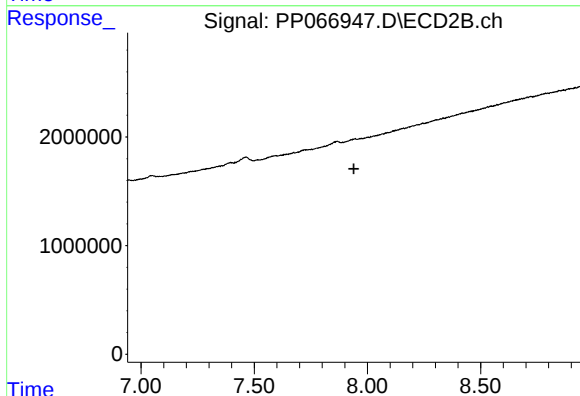


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.940 min
Response: 0
Conc: N.D.

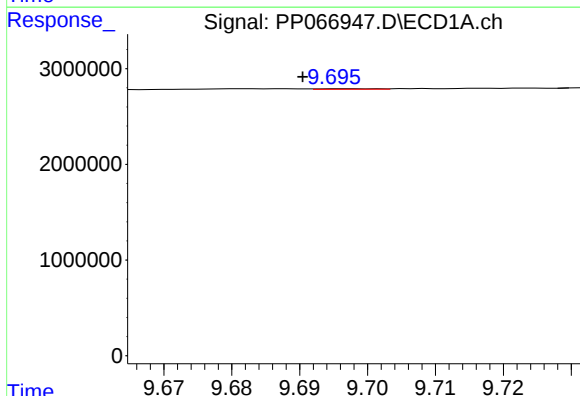


#40 AR-1262-5

R.T.: 9.696 min
Delta R.T.: 0.006 min
Response: 35063
Conc: 1.27 ng/ml

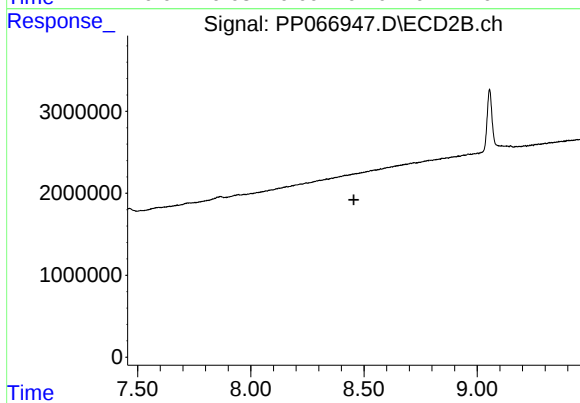

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.455 min
Response: 0
Conc: N.D.

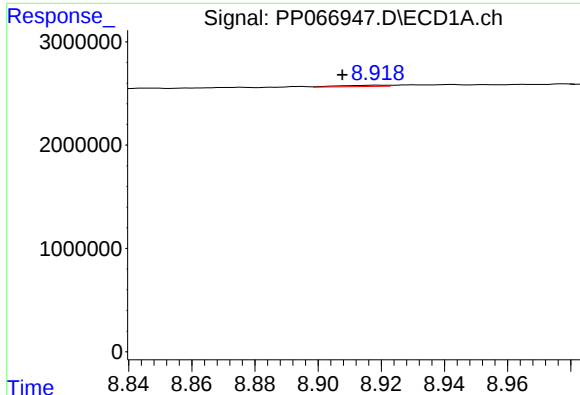

#41 AR-1268-1


R.T.: 8.919 min
Delta R.T.: 0.012 min
Response: 129787
Conc: 0.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

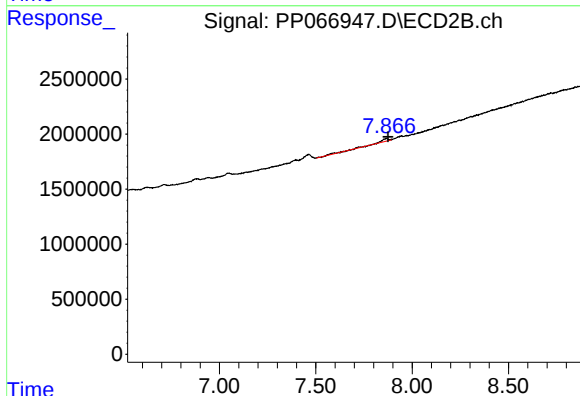


#41 AR-1268-1

R.T.: 7.866 min
Delta R.T.: -0.008 min
Response: 825264
Conc: 6.60 ng/ml

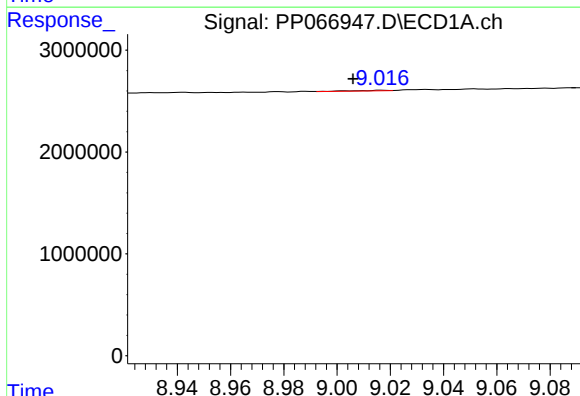


#42 AR-1268-2

R.T.: 9.017 min
Delta R.T.: 0.011 min
Response: 50402
Conc: 0.43 ng/ml

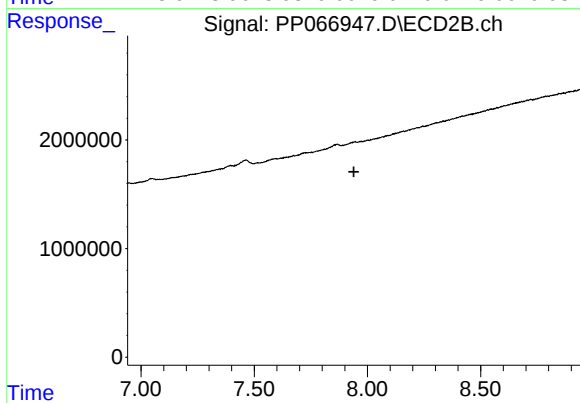

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 7.940 min
Response: 0
Conc: N.D.

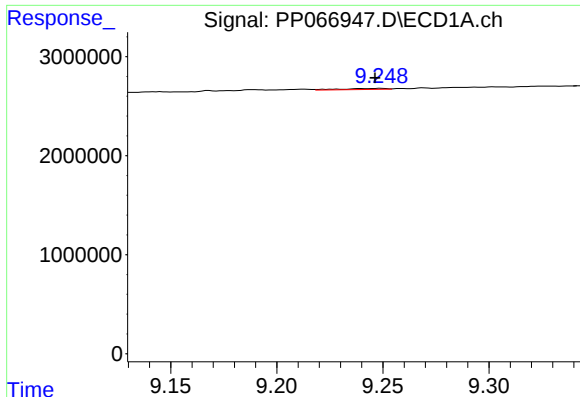

#43 AR-1268-3


R.T.: 9.249 min
Delta R.T.: 0.002 min
Response: 161710
Conc: 1.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

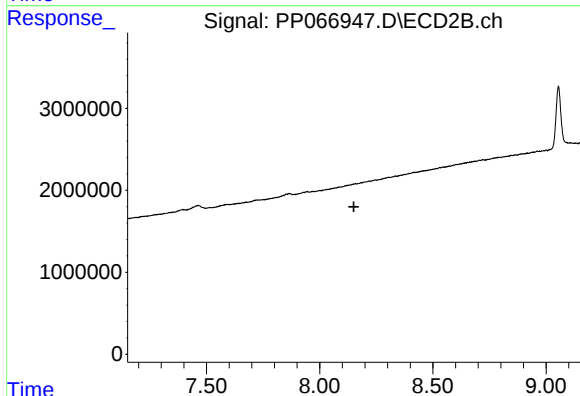


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

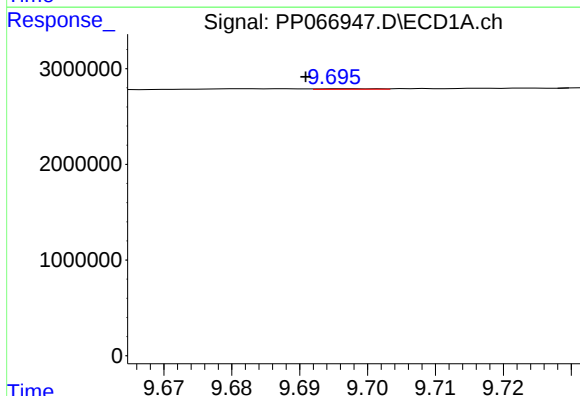


#44 AR-1268-4

R.T.: 9.696 min
Delta R.T.: 0.006 min
Response: 35063
Conc: 1.17 ng/ml

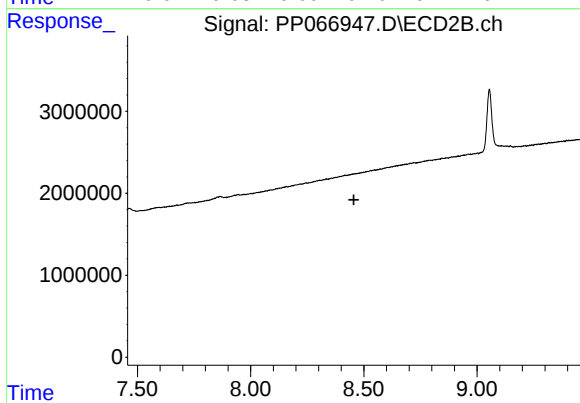

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.456 min
Response: 0
Conc: N.D.

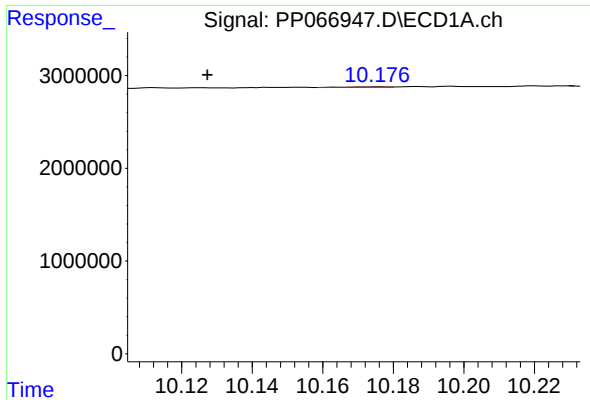

#45 AR-1268-5

R.T.: 10.176 min
Delta R.T.: 0.049 min
Response: 38624
Conc: 0.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

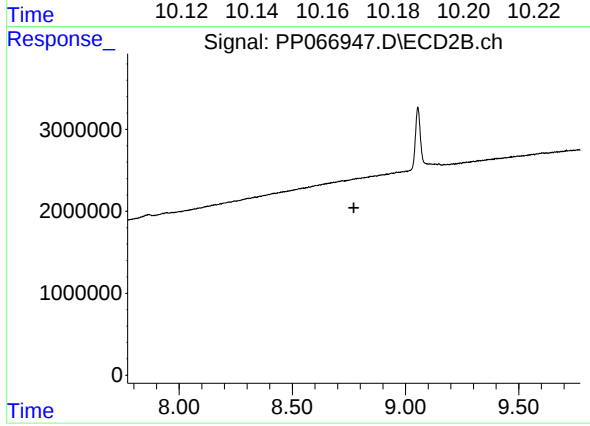

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.772 min
Response: 0
Conc: N.D.