

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
 Data File : PP066948.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2024 14:17
 Operator : YP\AJ
 Sample : P3390-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 04:36:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 09:05:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.626	3.913	26088112	21580939	15.499	15.056
2)	SA Decachlor...	10.489	9.054	11487298	10323779	13.699	13.784
Target Compounds							
3)	L1 AR-1016-1	5.799	5.022	430462	364979	9.098	8.361
4)	L1 AR-1016-2	5.823	5.042	662462	528919	8.953	8.219
5)	L1 AR-1016-3	5.886	5.223	466817	287739	9.950	8.379
6)	L1 AR-1016-4	5.985	5.261	274393	261845	7.589	8.645
7)	L1 AR-1016-5	6.280	5.482	303710	277317	8.866	7.682
8)	L2 AR-1221-1	4.829	4.130	245074	156906	13.510	10.089 #
9)	L2 AR-1221-2	4.932	4.222	526771	451713	39.129	38.606
10)	L2 AR-1221-3	4.998	4.297	707246	688090	17.500	18.072
11)	L3 AR-1232-1	4.998	4.297	707246	688090	21.215	21.863
12)	L3 AR-1232-2	5.533	5.042	403647	528919	22.865	17.936
13)	L3 AR-1232-3	5.823	5.223	662462	287739	21.216	20.260
14)	L3 AR-1232-4	5.985	5.309	274393	282153	17.934	20.074
15)	L3 AR-1232-5	6.073	5.482	407031	277317	32.348	19.496 #
16)	L4 AR-1242-1	5.799	5.022	430462	364979	12.514	11.749
17)	L4 AR-1242-2	5.823	5.042	662462	528919	12.472	11.850
18)	L4 AR-1242-3	5.886	5.223	466817	287739	13.613	11.928
19)	L4 AR-1242-4	5.985	5.309	274393	282153	10.574	10.544
20)	L4 AR-1242-5	6.722	5.839	368998	316086	15.881	11.325 #
21)	L5 AR-1248-1	5.799	5.022	430462	364979	17.832	16.583
22)	L5 AR-1248-2	6.073	5.261	407031	261845	10.451	7.453 #
23)	L5 AR-1248-3	6.280	5.309	303710	282153	7.456	7.754
24)	L5 AR-1248-4	6.684	5.482	275288	277317	7.105	6.824
25)	L5 AR-1248-5	6.722	5.877	368998	377615	9.371	11.820 #
26)	L6 AR-1254-1	6.658	5.839	500113	316086	10.051	5.326 #
27)	L6 AR-1254-2	6.882	5.987	488089	208165	6.910	3.973 #
28)	L6 AR-1254-3	7.240	6.398	418578	552787	6.143	7.246
29)	L6 AR-1254-4	7.523	6.625	483230	380521	11.540	10.073
30)	L6 AR-1254-5	7.949	7.049	1395913	654769	26.566	10.404 #
31)	L7 AR-1260-1	7.410	6.537	260220	465530	4.300	7.349 #
32)	L7 AR-1260-2	7.662	6.712	312834	419868	4.867	6.210 #
33)	L7 AR-1260-3	8.026	6.885	38739	659892	0.868	9.908 #
34)	L7 AR-1260-4	8.262	7.353	343825	296799	6.862	6.772
35)	L7 AR-1260-5	8.587	7.586	197274	495630	2.361	5.557 #
36)	L8 AR-1262-1	8.262	7.085	343825	24005	5.258	0.332 #
37)	L8 AR-1262-2	8.587	7.353	197274	296799	1.907	4.823 #
38)	L8 AR-1262-3	8.901	7.868	175826	1411606	2.462	33.558 #
39)	L8 AR-1262-4	8.981	7.944	72045	821287	1.220	10.588 #
40)	L8 AR-1262-5	9.687	0.000	73262	0	2.663	N.D. #
41)	L9 AR-1268-1	8.901	7.868	175826	1411606	1.345	11.286 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
Data File : PP066948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2024 14:17
Operator : YP\AJ
Sample : P3390-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 15 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 04:36:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 09:05:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.981	7.944	72045	821287	0.616	7.348 #
43) L9	AR-1268-3	9.253	8.175	56894	441892	0.547	4.323 #
44) L9	AR-1268-4	9.687	0.000	73262	0	2.448	N.D. #
45) L9	AR-1268-5	0.000	8.793	0	53924	N.D.	0.220 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

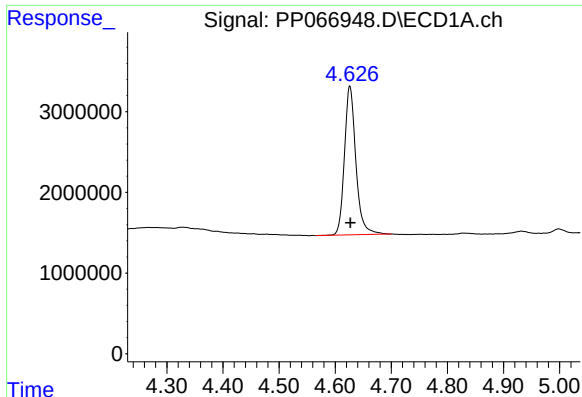

#1 Tetrachloro-m-xylene


R.T.: 4.626 min
Delta R.T.: 0.000 min
Response: 26088112
Conc: 15.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

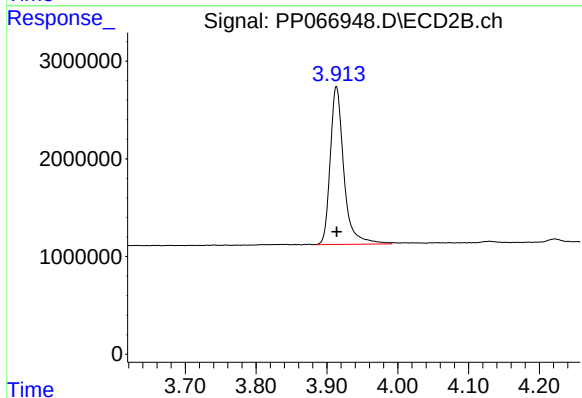


#1 Tetrachloro-m-xylene

R.T.: 3.913 min
Delta R.T.: 0.000 min
Response: 21580939
Conc: 15.06 ng/ml

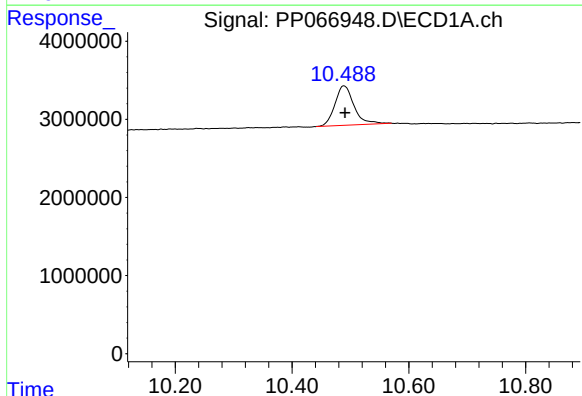


#2 Decachlorobiphenyl

R.T.: 10.489 min
Delta R.T.: -0.001 min
Response: 11487298
Conc: 13.70 ng/ml

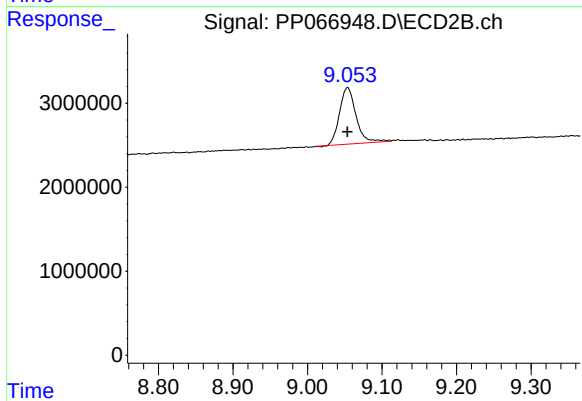

#2 Decachlorobiphenyl


R.T.: 9.054 min
Delta R.T.: 0.000 min
Response: 10323779
Conc: 13.78 ng/ml

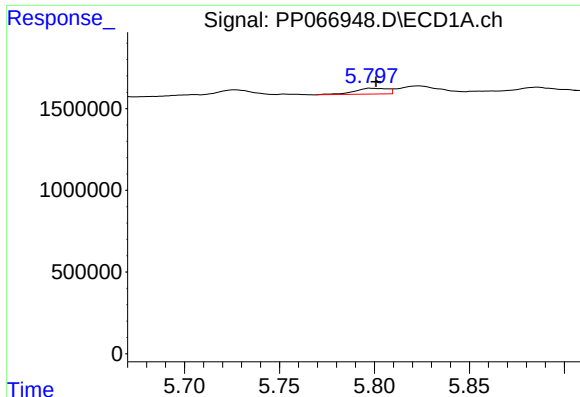

#3 AR-1016-1


R.T.: 5.799 min
Delta R.T.: -0.002 min
Response: 430462
Conc: 9.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

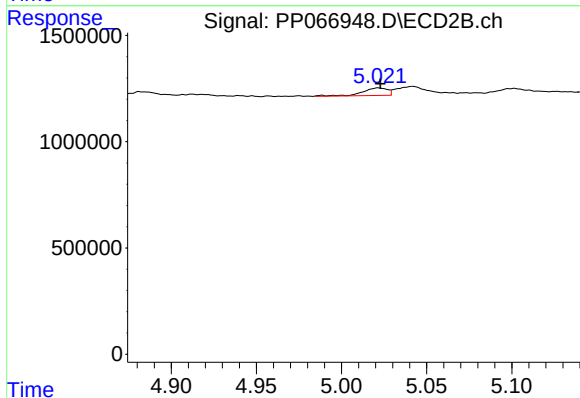


#3 AR-1016-1

R.T.: 5.022 min
Delta R.T.: -0.001 min
Response: 364979
Conc: 8.36 ng/ml

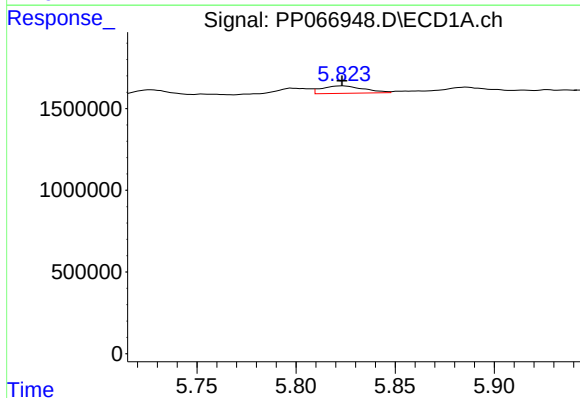


#4 AR-1016-2

R.T.: 5.823 min
Delta R.T.: 0.000 min
Response: 662462
Conc: 8.95 ng/ml

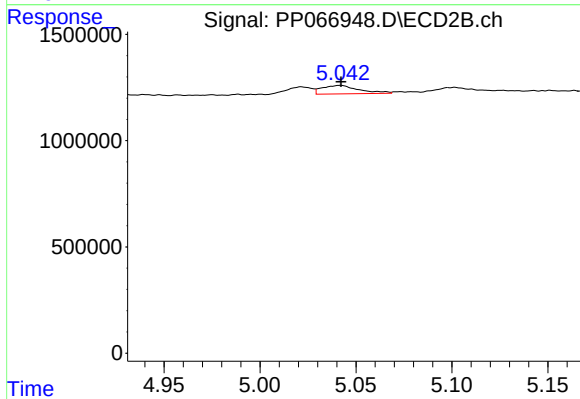

#4 AR-1016-2


R.T.: 5.042 min
Delta R.T.: 0.000 min
Response: 528919
Conc: 8.22 ng/ml

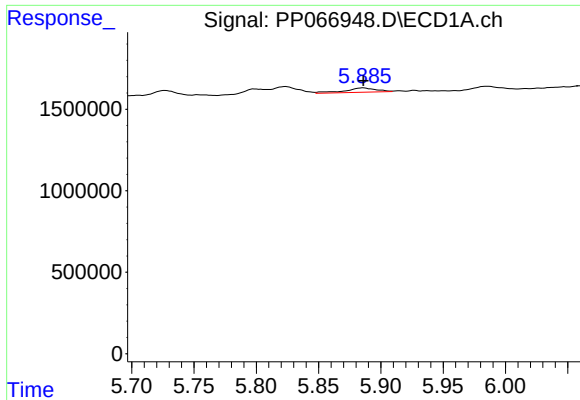

#5 AR-1016-3


R.T.: 5.886 min
Delta R.T.: 0.000 min
Response: 466817
Conc: 9.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

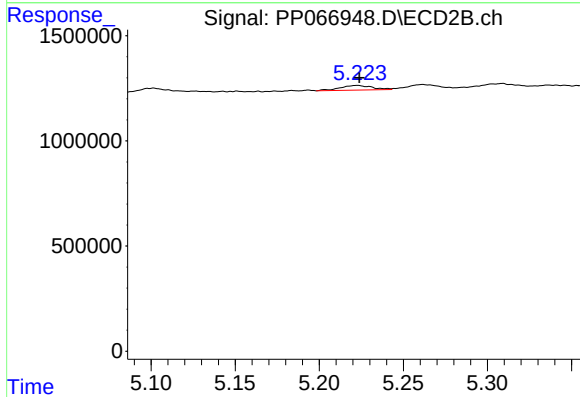


#5 AR-1016-3

R.T.: 5.223 min
Delta R.T.: -0.001 min
Response: 287739
Conc: 8.38 ng/ml

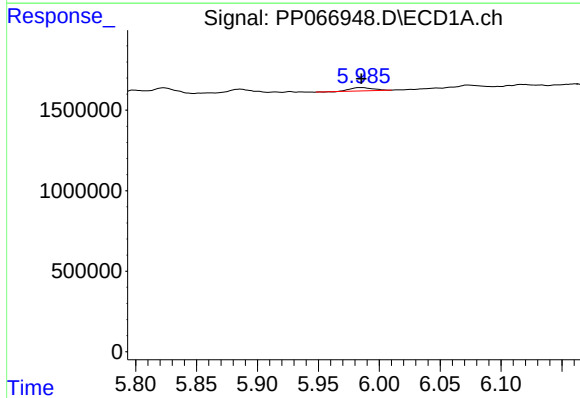


#6 AR-1016-4

R.T.: 5.985 min
Delta R.T.: 0.000 min
Response: 274393
Conc: 7.59 ng/ml

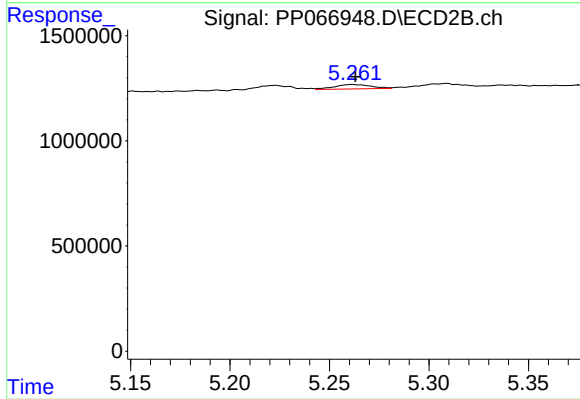

#6 AR-1016-4


R.T.: 5.261 min
Delta R.T.: -0.002 min
Response: 261845
Conc: 8.64 ng/ml

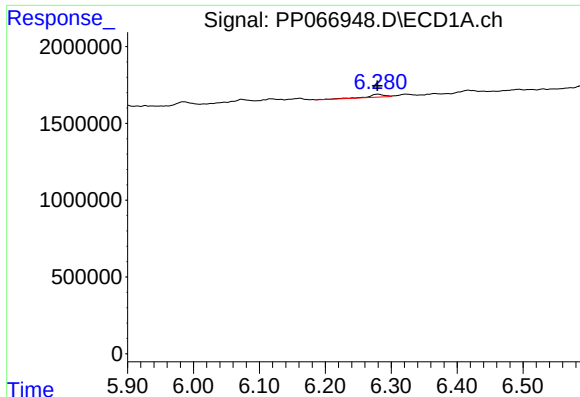

#7 AR-1016-5


R.T.: 6.280 min
Delta R.T.: 0.000 min
Response: 303710
Conc: 8.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

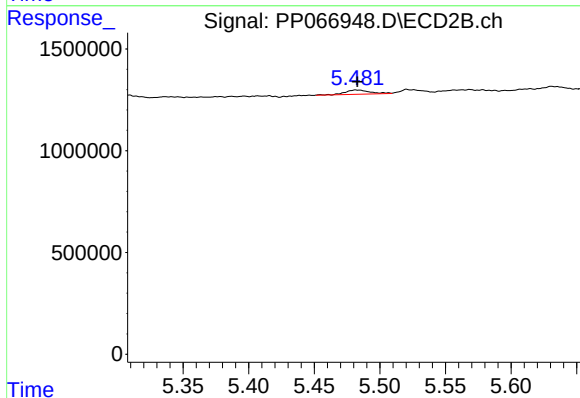


#7 AR-1016-5

R.T.: 5.482 min
Delta R.T.: 0.000 min
Response: 277317
Conc: 7.68 ng/ml

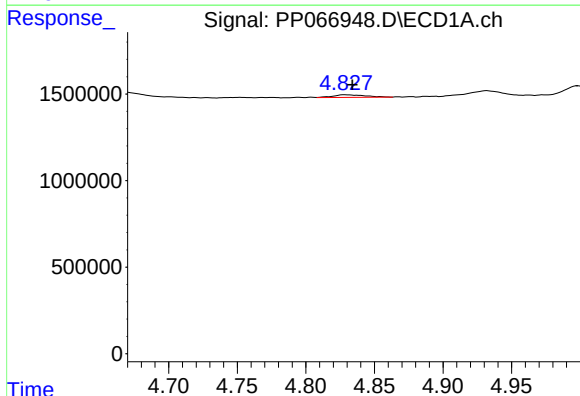


#8 AR-1221-1

R.T.: 4.829 min
Delta R.T.: -0.005 min
Response: 245074
Conc: 13.51 ng/ml

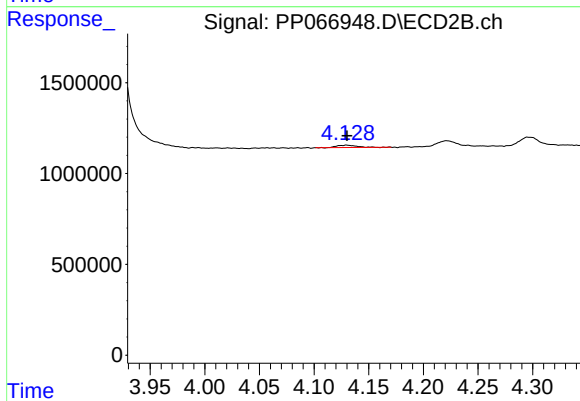

#8 AR-1221-1


R.T.: 4.130 min
Delta R.T.: 0.000 min
Response: 156906
Conc: 10.09 ng/ml

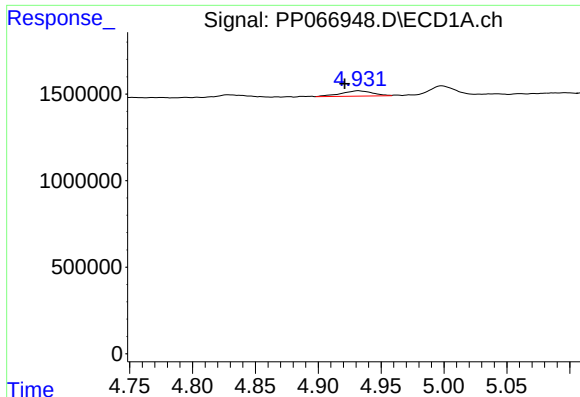

#9 AR-1221-2


R.T.: 4.932 min
Delta R.T.: 0.011 min
Response: 526771
Conc: 39.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

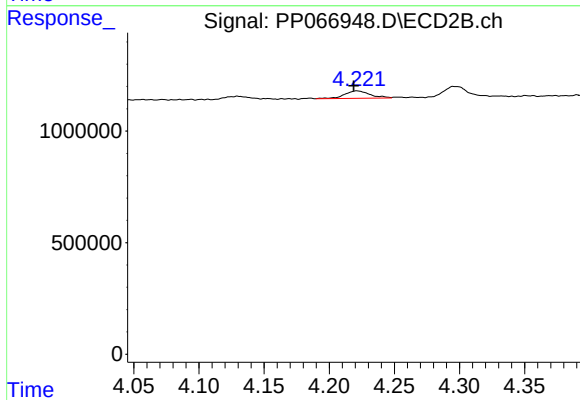


#9 AR-1221-2

R.T.: 4.222 min
Delta R.T.: 0.003 min
Response: 451713
Conc: 38.61 ng/ml

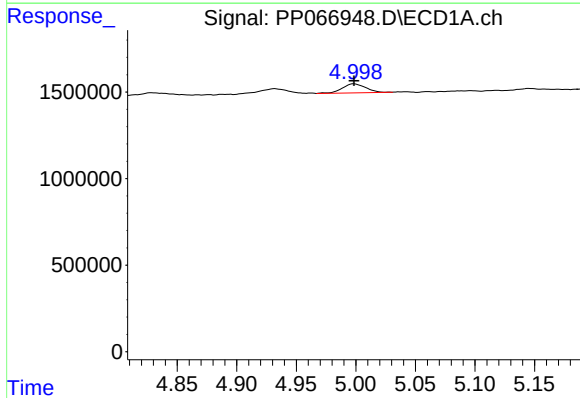


#10 AR-1221-3

R.T.: 4.998 min
Delta R.T.: 0.000 min
Response: 707246
Conc: 17.50 ng/ml

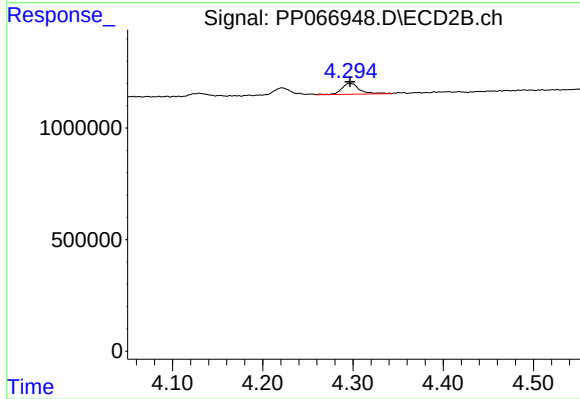

#10 AR-1221-3


R.T.: 4.297 min
Delta R.T.: 0.000 min
Response: 688090
Conc: 18.07 ng/ml

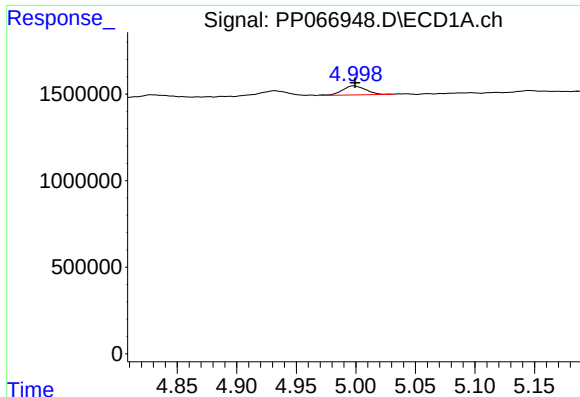

#11 AR-1232-1


R.T.: 4.998 min
Delta R.T.: 0.000 min
Response: 707246
Conc: 21.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

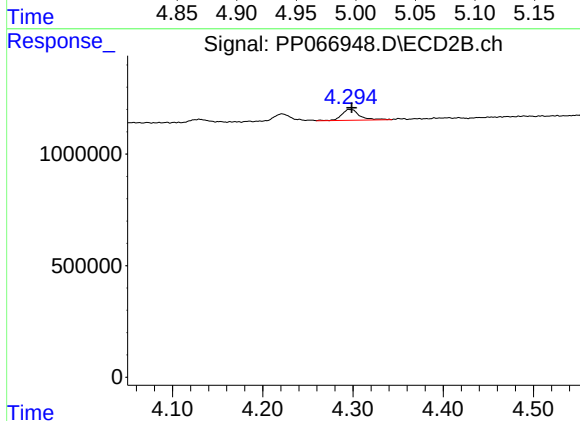


#11 AR-1232-1

R.T.: 4.297 min
Delta R.T.: -0.002 min
Response: 688090
Conc: 21.86 ng/ml

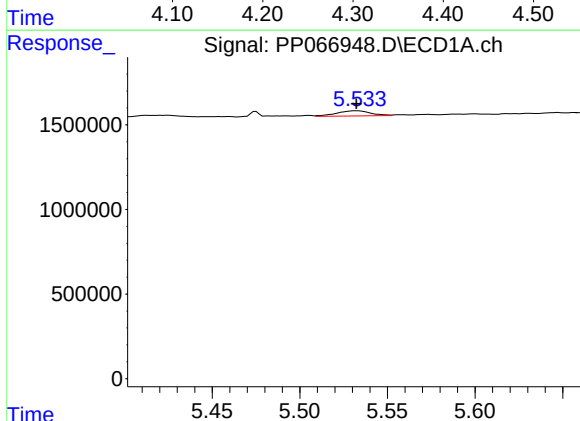


#12 AR-1232-2

R.T.: 5.533 min
Delta R.T.: 0.000 min
Response: 403647
Conc: 22.87 ng/ml

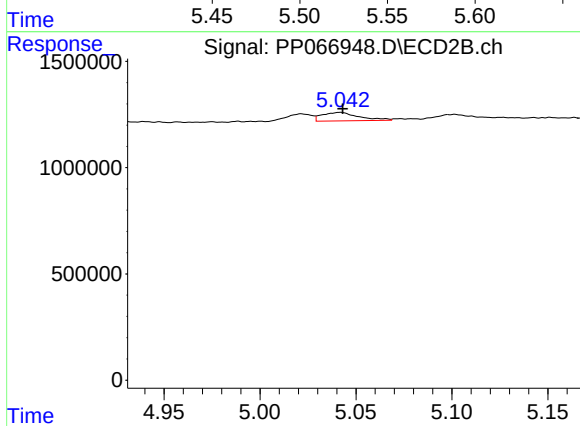

#12 AR-1232-2


R.T.: 5.042 min
Delta R.T.: -0.001 min
Response: 528919
Conc: 17.94 ng/ml

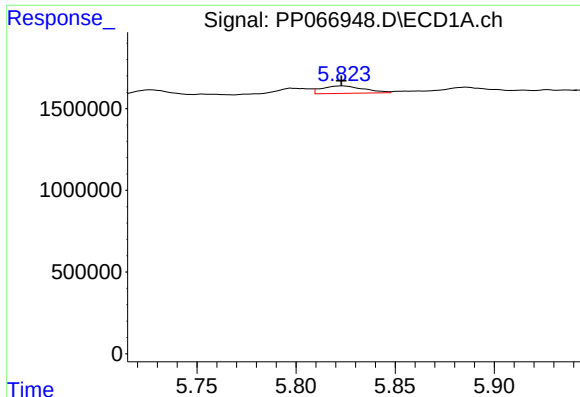

#13 AR-1232-3


R.T.: 5.823 min
Delta R.T.: 0.000 min
Response: 662462
Conc: 21.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

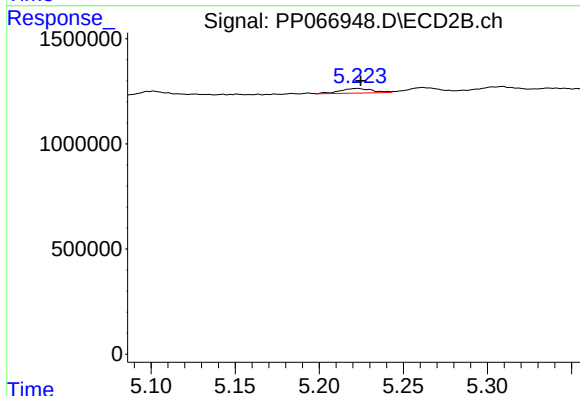


#13 AR-1232-3

R.T.: 5.223 min
Delta R.T.: -0.002 min
Response: 287739
Conc: 20.26 ng/ml

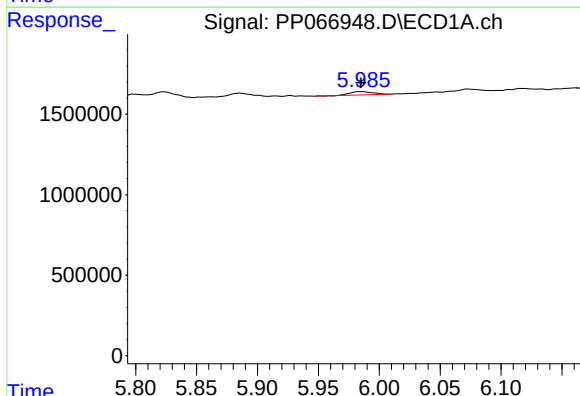


#14 AR-1232-4

R.T.: 5.985 min
Delta R.T.: 0.000 min
Response: 274393
Conc: 17.93 ng/ml

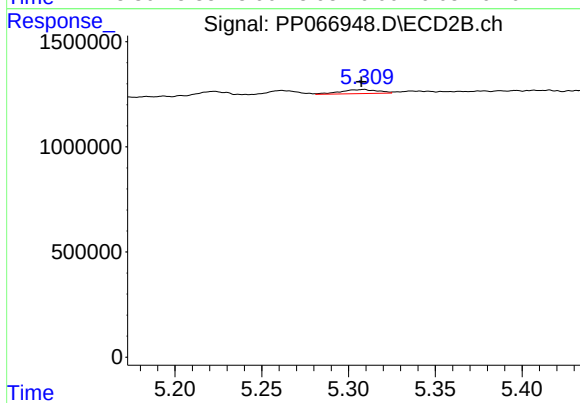

#14 AR-1232-4


R.T.: 5.309 min
Delta R.T.: 0.001 min
Response: 282153
Conc: 20.07 ng/ml

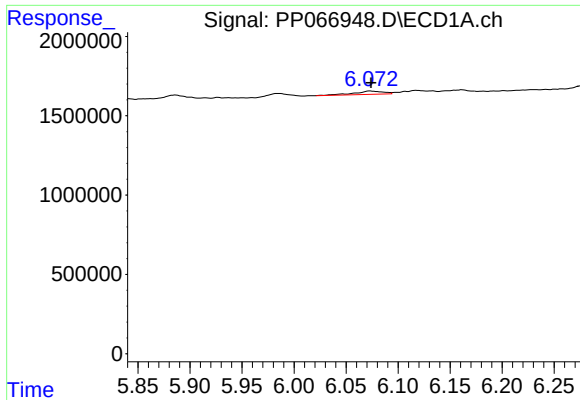

#15 AR-1232-5


R.T.: 6.073 min
Delta R.T.: -0.001 min
Response: 407031
Conc: 32.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

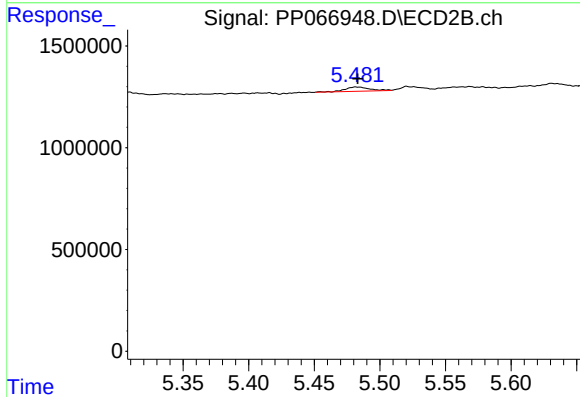


#15 AR-1232-5

R.T.: 5.482 min
Delta R.T.: -0.001 min
Response: 277317
Conc: 19.50 ng/ml

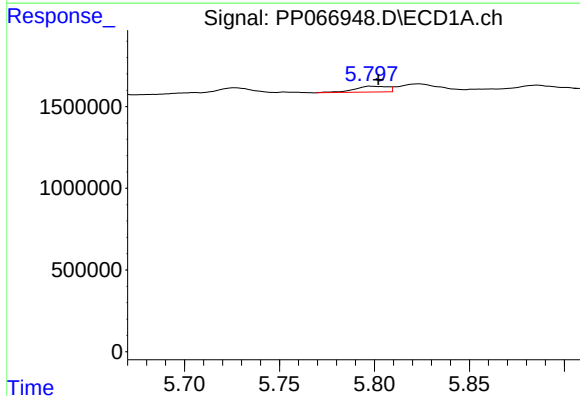


#16 AR-1242-1

R.T.: 5.799 min
Delta R.T.: -0.003 min
Response: 430462
Conc: 12.51 ng/ml

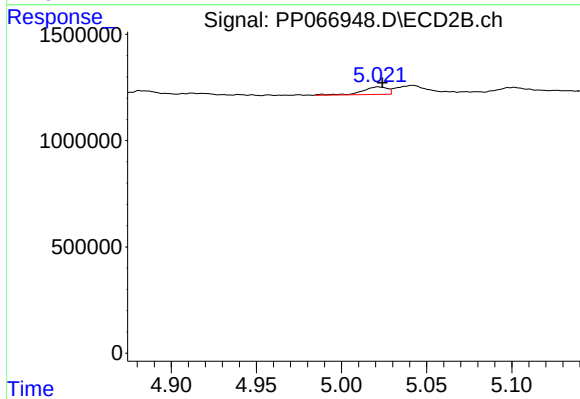

#16 AR-1242-1


R.T.: 5.022 min
Delta R.T.: -0.002 min
Response: 364979
Conc: 11.75 ng/ml

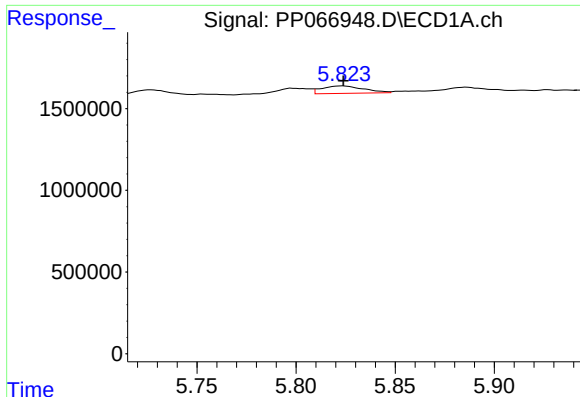

#17 AR-1242-2


R.T.: 5.823 min
Delta R.T.: 0.000 min
Response: 662462
Conc: 12.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

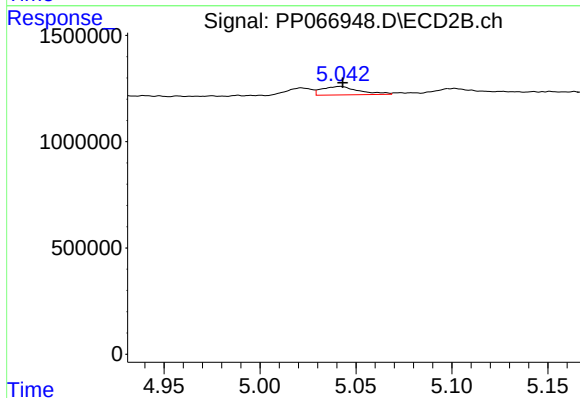


#17 AR-1242-2

R.T.: 5.042 min
Delta R.T.: -0.001 min
Response: 528919
Conc: 11.85 ng/ml

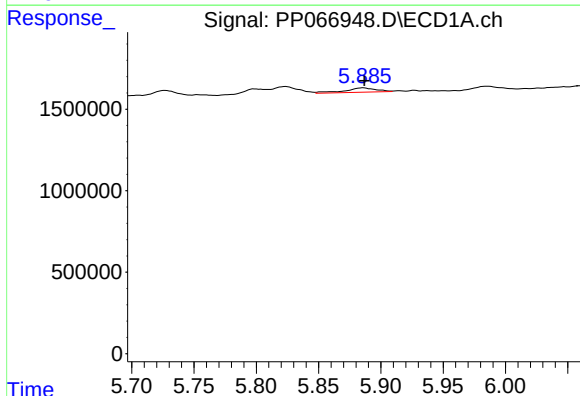


#18 AR-1242-3

R.T.: 5.886 min
Delta R.T.: 0.000 min
Response: 466817
Conc: 13.61 ng/ml

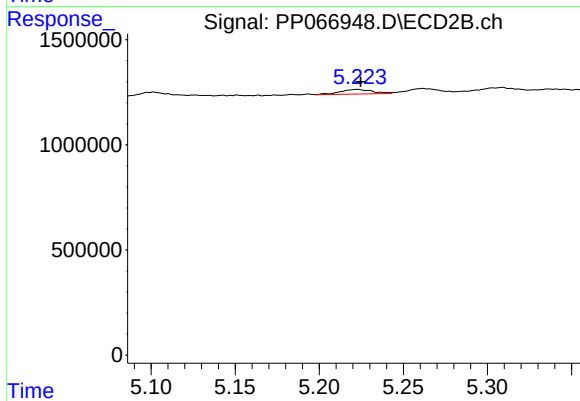

#18 AR-1242-3


R.T.: 5.223 min
Delta R.T.: -0.002 min
Response: 287739
Conc: 11.93 ng/ml

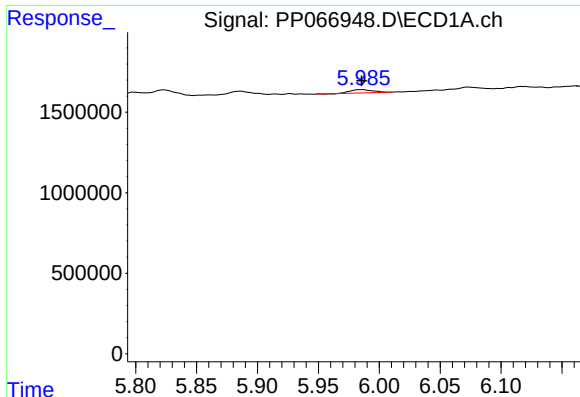

#19 AR-1242-4


R.T.: 5.985 min
Delta R.T.: 0.000 min
Response: 274393
Conc: 10.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

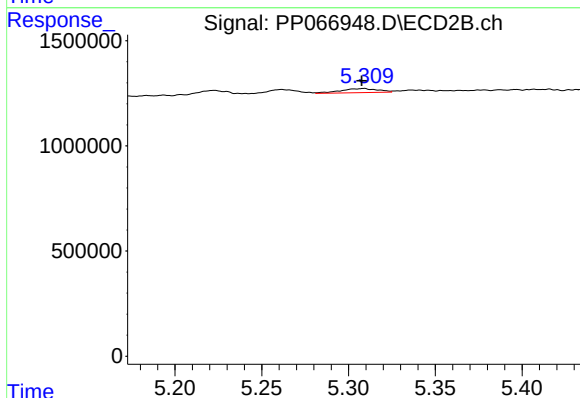


#19 AR-1242-4

R.T.: 5.309 min
Delta R.T.: 0.000 min
Response: 282153
Conc: 10.54 ng/ml

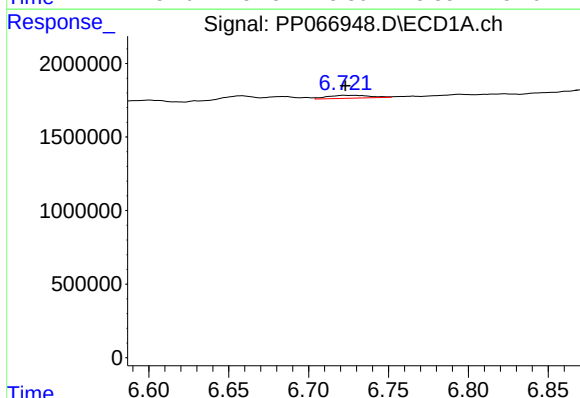


#20 AR-1242-5

R.T.: 6.722 min
Delta R.T.: 0.000 min
Response: 368998
Conc: 15.88 ng/ml

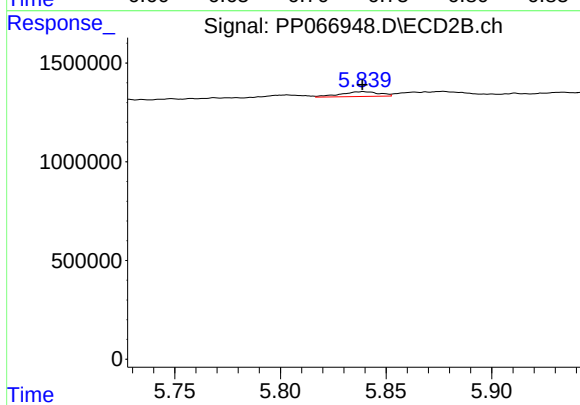

#20 AR-1242-5


R.T.: 5.839 min
Delta R.T.: 0.000 min
Response: 316086
Conc: 11.33 ng/ml

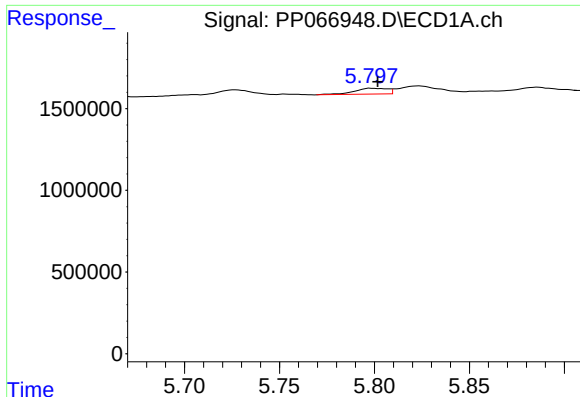

#21 AR-1248-1


R.T.: 5.799 min
Delta R.T.: -0.003 min
Response: 430462
Conc: 17.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

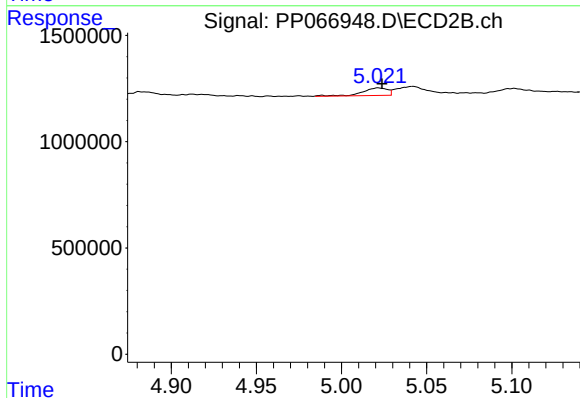


#21 AR-1248-1

R.T.: 5.022 min
Delta R.T.: -0.002 min
Response: 364979
Conc: 16.58 ng/ml

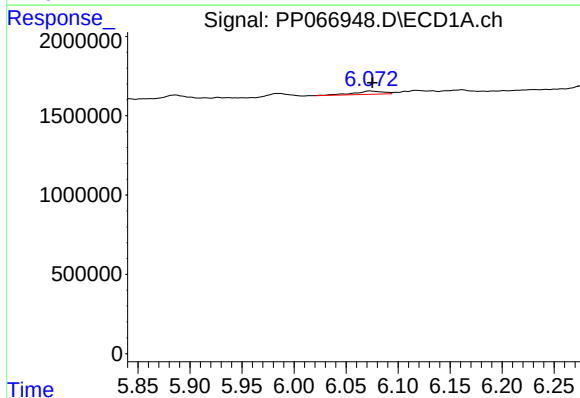


#22 AR-1248-2

R.T.: 6.073 min
Delta R.T.: -0.002 min
Response: 407031
Conc: 10.45 ng/ml

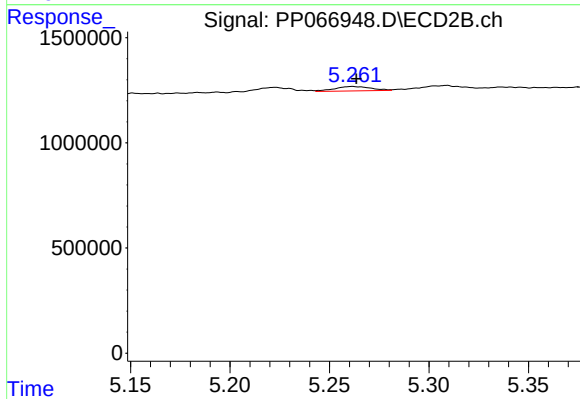

#22 AR-1248-2


R.T.: 5.261 min
Delta R.T.: -0.002 min
Response: 261845
Conc: 7.45 ng/ml

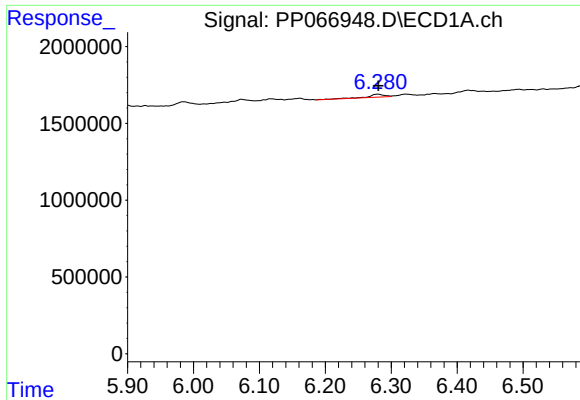

#23 AR-1248-3


R.T.: 6.280 min
Delta R.T.: -0.001 min
Response: 303710
Conc: 7.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

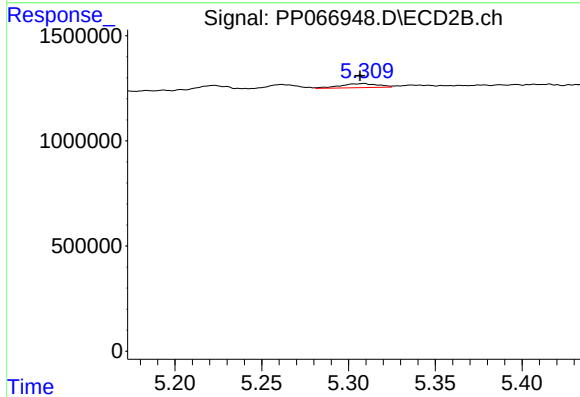


#23 AR-1248-3

R.T.: 5.309 min
Delta R.T.: 0.002 min
Response: 282153
Conc: 7.75 ng/ml

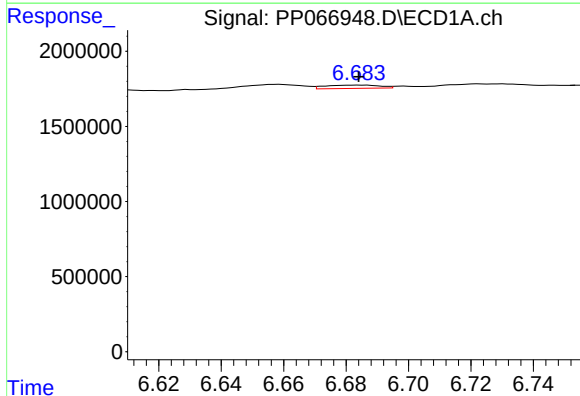


#24 AR-1248-4

R.T.: 6.684 min
Delta R.T.: 0.000 min
Response: 275288
Conc: 7.11 ng/ml

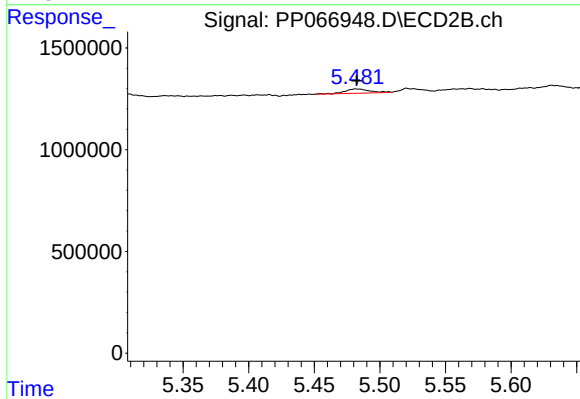

#24 AR-1248-4


R.T.: 5.482 min
Delta R.T.: 0.000 min
Response: 277317
Conc: 6.82 ng/ml

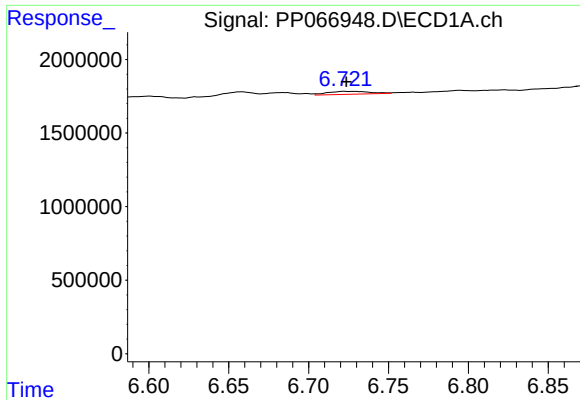

#25 AR-1248-5


R.T.: 6.722 min
Delta R.T.: -0.001 min
Response: 368998
Conc: 9.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

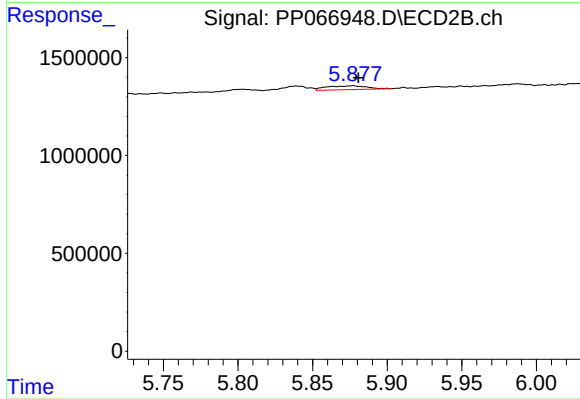


#25 AR-1248-5

R.T.: 5.877 min
Delta R.T.: -0.004 min
Response: 377615
Conc: 11.82 ng/ml

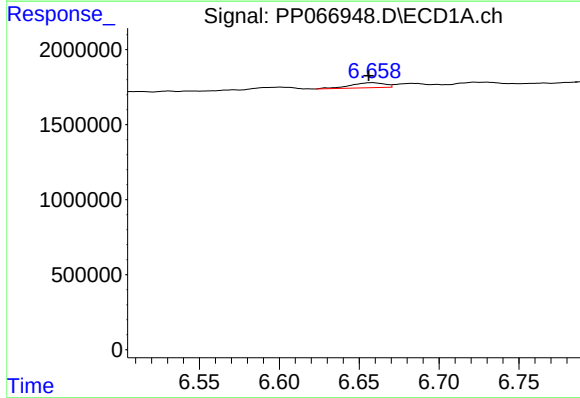


#26 AR-1254-1

R.T.: 6.658 min
Delta R.T.: 0.002 min
Response: 500113
Conc: 10.05 ng/ml

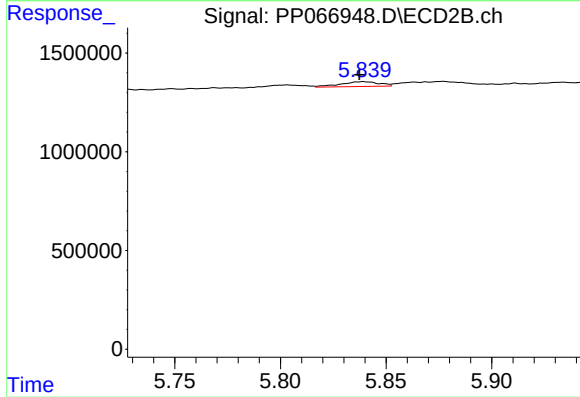

#26 AR-1254-1


R.T.: 5.839 min
Delta R.T.: 0.002 min
Response: 316086
Conc: 5.33 ng/ml

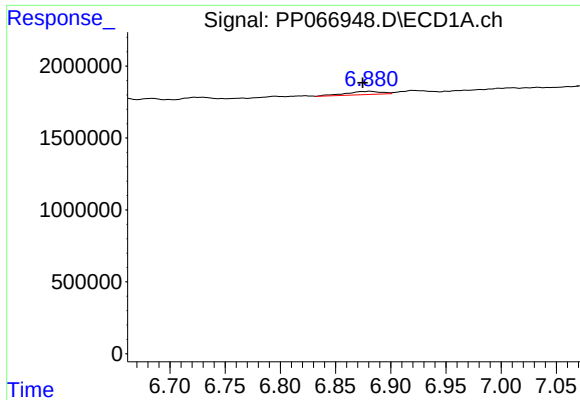

#27 AR-1254-2


R.T.: 6.882 min
Delta R.T.: 0.007 min
Response: 488089
Conc: 6.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

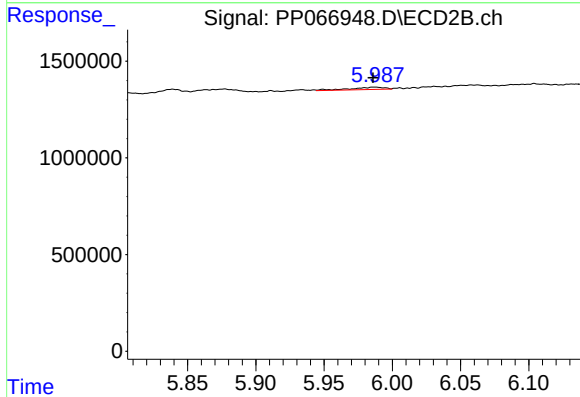


#27 AR-1254-2

R.T.: 5.987 min
Delta R.T.: 0.001 min
Response: 208165
Conc: 3.97 ng/ml

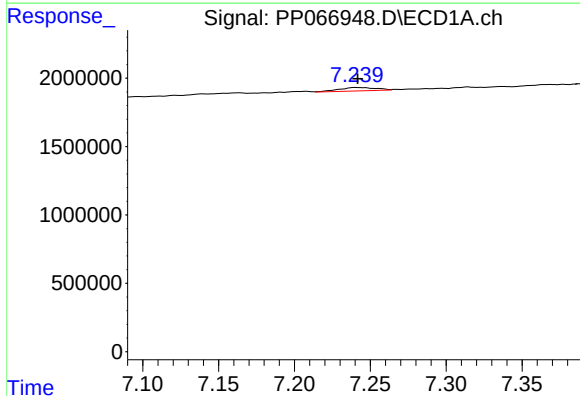


#28 AR-1254-3

R.T.: 7.240 min
Delta R.T.: -0.002 min
Response: 418578
Conc: 6.14 ng/ml

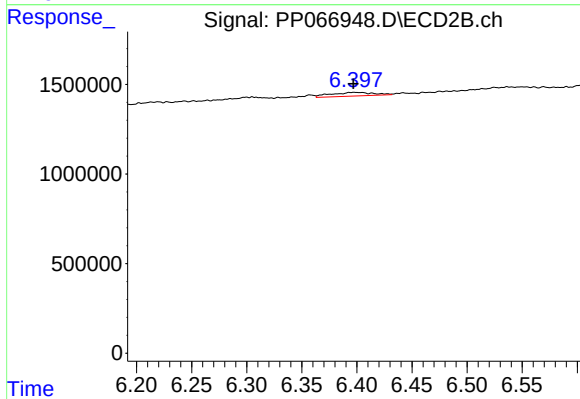

#28 AR-1254-3


R.T.: 6.398 min
Delta R.T.: 0.001 min
Response: 552787
Conc: 7.25 ng/ml

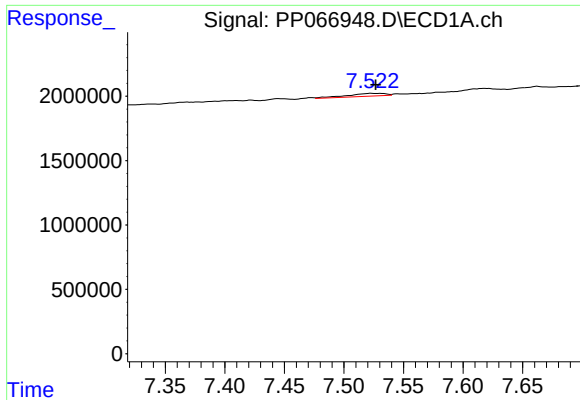

#29 AR-1254-4


R.T.: 7.523 min
Delta R.T.: -0.004 min
Response: 483230
Conc: 11.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

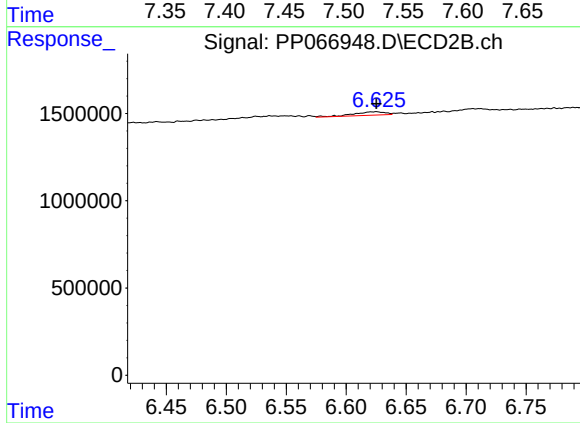


#29 AR-1254-4

R.T.: 6.625 min
Delta R.T.: 0.000 min
Response: 380521
Conc: 10.07 ng/ml

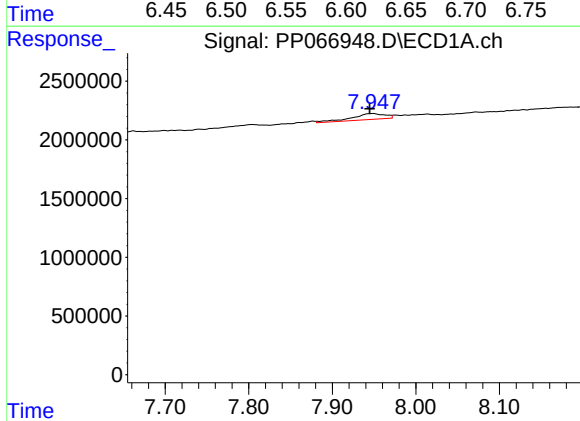


#30 AR-1254-5

R.T.: 7.949 min
Delta R.T.: 0.004 min
Response: 1395913
Conc: 26.57 ng/ml

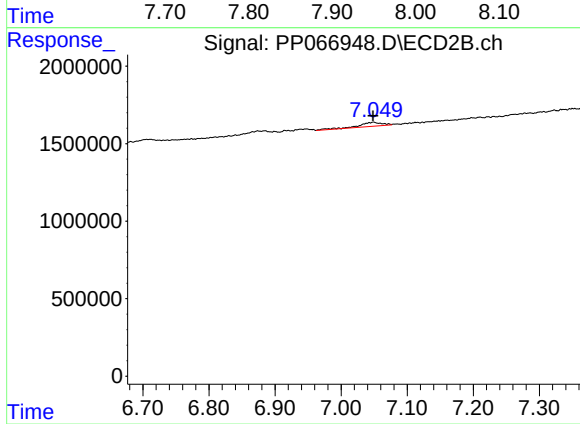

#30 AR-1254-5


R.T.: 7.049 min
Delta R.T.: 0.000 min
Response: 654769
Conc: 10.40 ng/ml

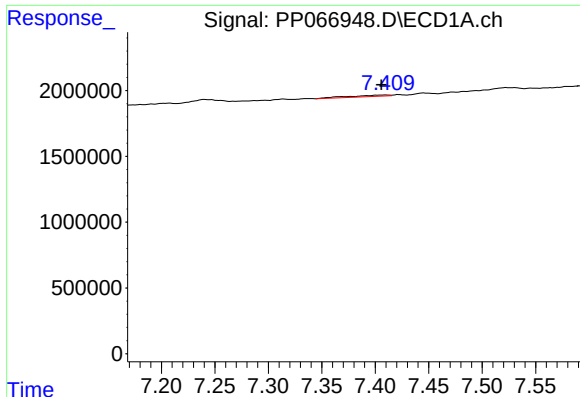

#31 AR-1260-1


R.T.: 7.410 min
Delta R.T.: 0.005 min
Response: 260220
Conc: 4.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

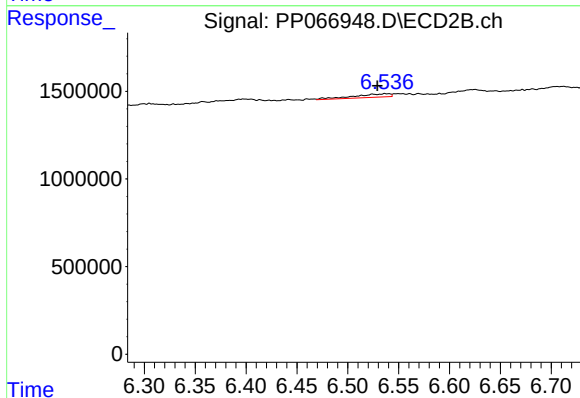


#31 AR-1260-1

R.T.: 6.537 min
Delta R.T.: 0.008 min
Response: 465530
Conc: 7.35 ng/ml

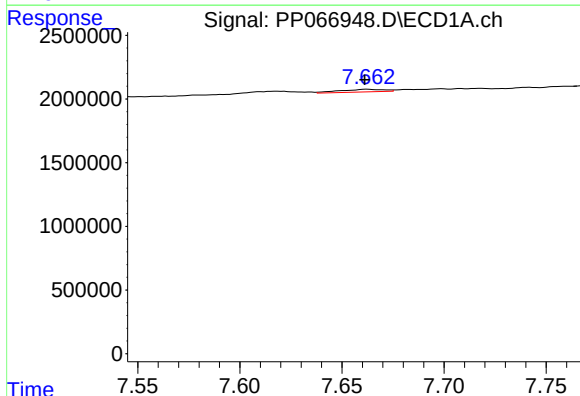


#32 AR-1260-2

R.T.: 7.662 min
Delta R.T.: 0.001 min
Response: 312834
Conc: 4.87 ng/ml

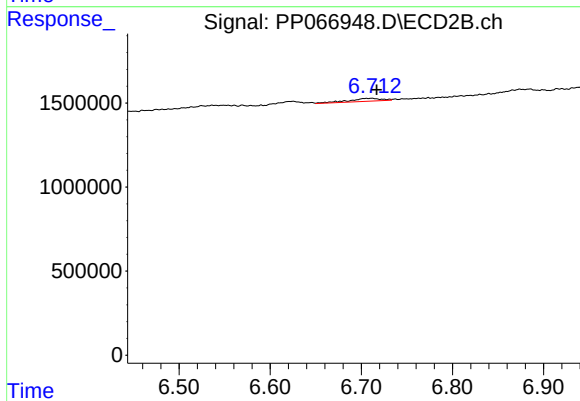

#32 AR-1260-2


R.T.: 6.712 min
Delta R.T.: -0.005 min
Response: 419868
Conc: 6.21 ng/ml

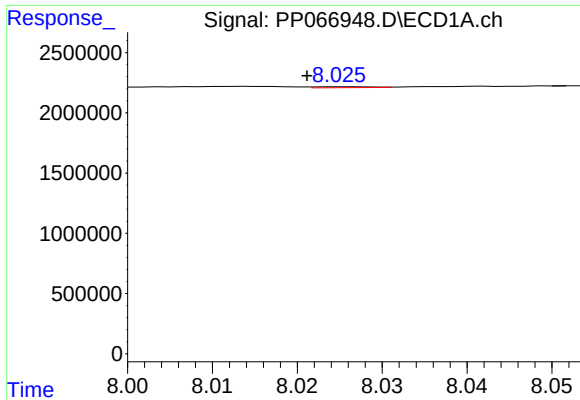

#33 AR-1260-3


R.T.: 8.026 min
Delta R.T.: 0.004 min
Response: 38739
Conc: 0.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

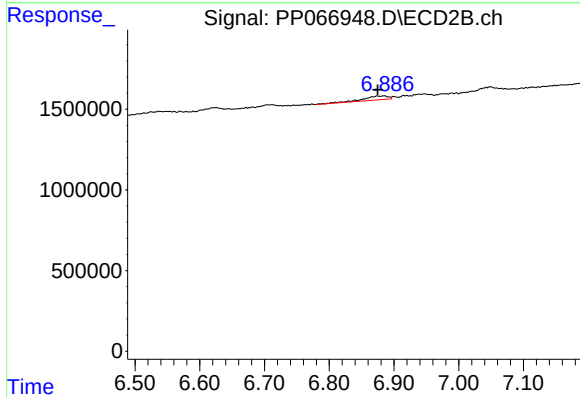


#33 AR-1260-3

R.T.: 6.885 min
Delta R.T.: 0.010 min
Response: 659892
Conc: 9.91 ng/ml

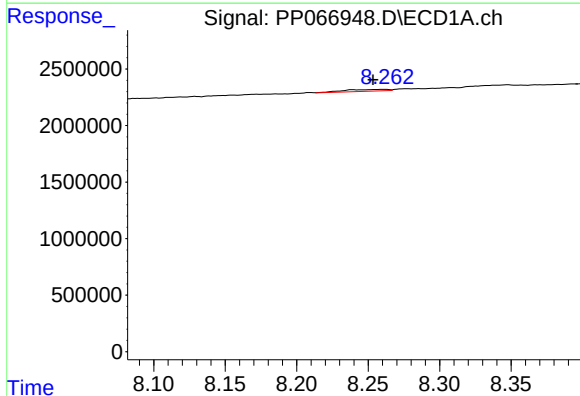


#34 AR-1260-4

R.T.: 8.262 min
Delta R.T.: 0.008 min
Response: 343825
Conc: 6.86 ng/ml

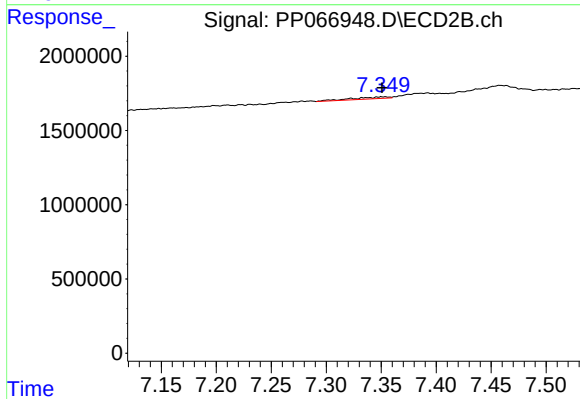

#34 AR-1260-4


R.T.: 7.353 min
Delta R.T.: 0.002 min
Response: 296799
Conc: 6.77 ng/ml

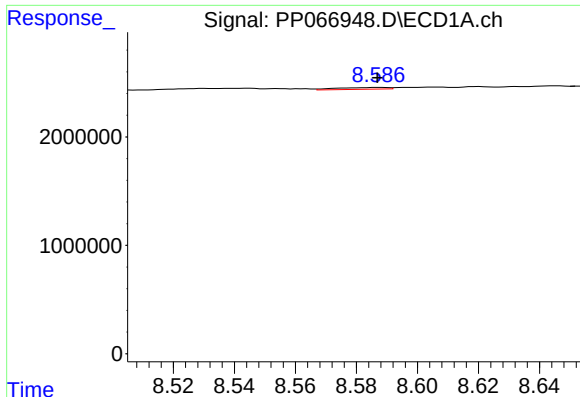

#35 AR-1260-5


R.T.: 8.587 min
Delta R.T.: 0.000 min
Response: 197274
Conc: 2.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

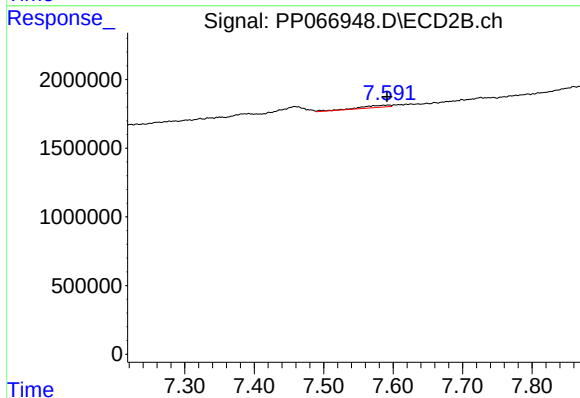


#35 AR-1260-5

R.T.: 7.586 min
Delta R.T.: -0.005 min
Response: 495630
Conc: 5.56 ng/ml

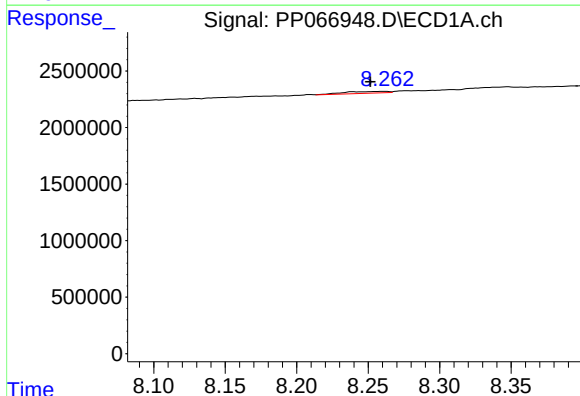


#36 AR-1262-1

R.T.: 8.262 min
Delta R.T.: 0.010 min
Response: 343825
Conc: 5.26 ng/ml

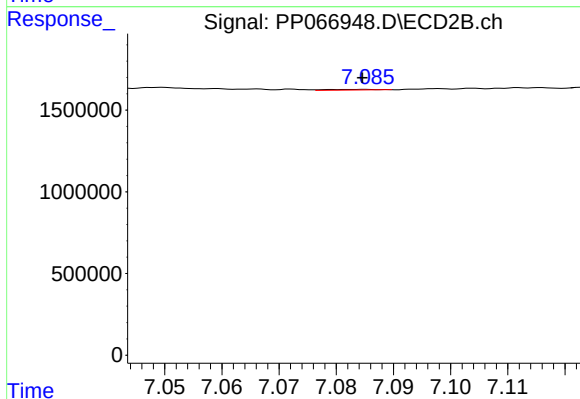

#36 AR-1262-1


R.T.: 7.085 min
Delta R.T.: 0.000 min
Response: 24005
Conc: 0.33 ng/ml

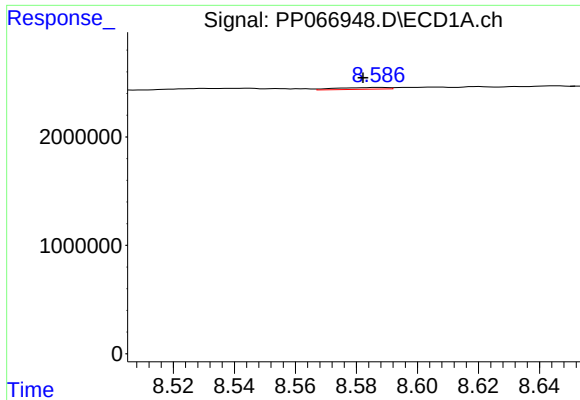

#37 AR-1262-2


R.T.: 8.587 min
Delta R.T.: 0.005 min
Response: 197274
Conc: 1.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

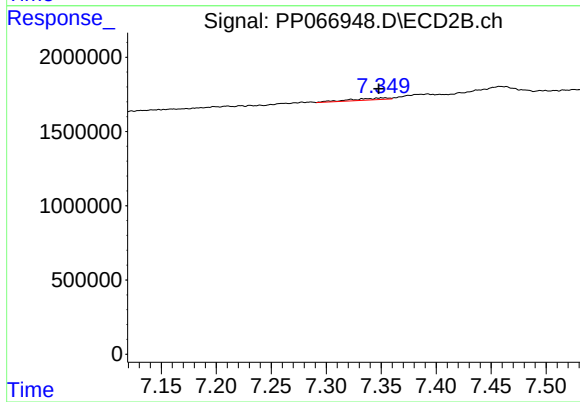


#37 AR-1262-2

R.T.: 7.353 min
Delta R.T.: 0.005 min
Response: 296799
Conc: 4.82 ng/ml

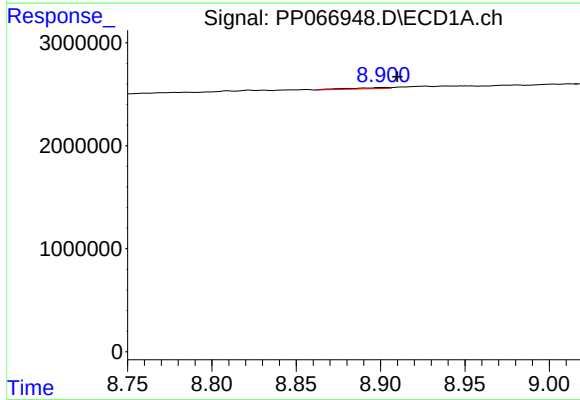


#38 AR-1262-3

R.T.: 8.901 min
Delta R.T.: -0.008 min
Response: 175826
Conc: 2.46 ng/ml

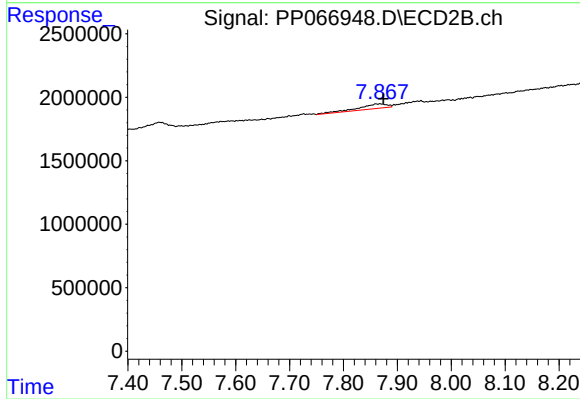

#38 AR-1262-3


R.T.: 7.868 min
Delta R.T.: -0.007 min
Response: 1411606
Conc: 33.56 ng/ml

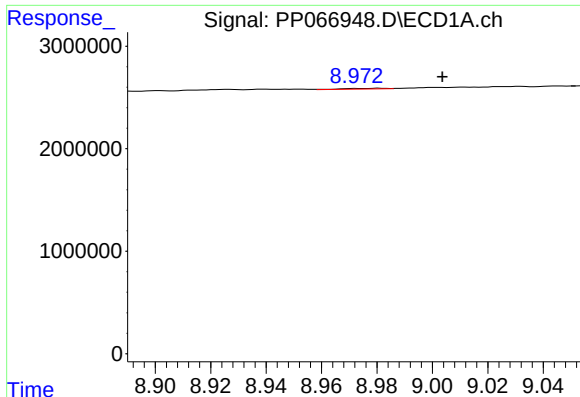

#39 AR-1262-4


R.T.: 8.981 min
Delta R.T.: -0.023 min
Response: 72045
Conc: 1.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

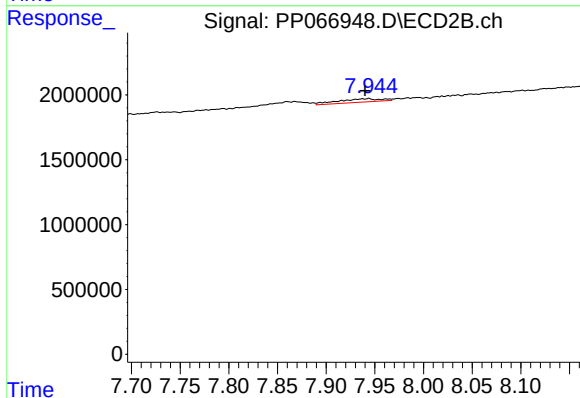


#39 AR-1262-4

R.T.: 7.944 min
Delta R.T.: 0.004 min
Response: 821287
Conc: 10.59 ng/ml

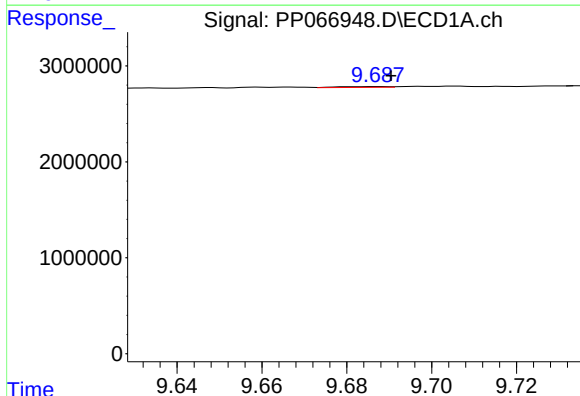


#40 AR-1262-5

R.T.: 9.687 min
Delta R.T.: -0.003 min
Response: 73262
Conc: 2.66 ng/ml

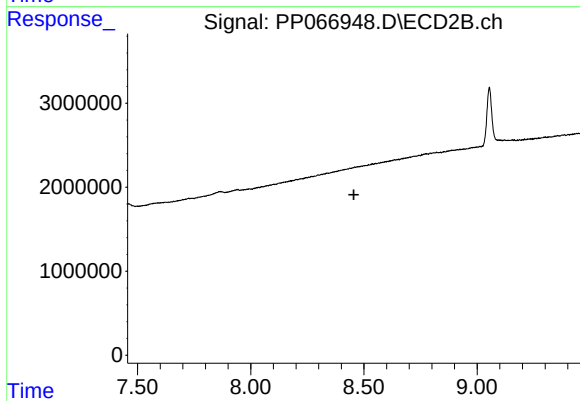

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.455 min
Response: 0
Conc: N.D.

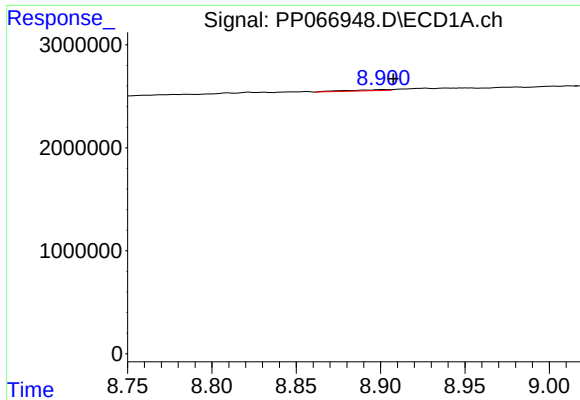

#41 AR-1268-1


R.T.: 8.901 min
Delta R.T.: -0.006 min
Response: 175826
Conc: 1.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

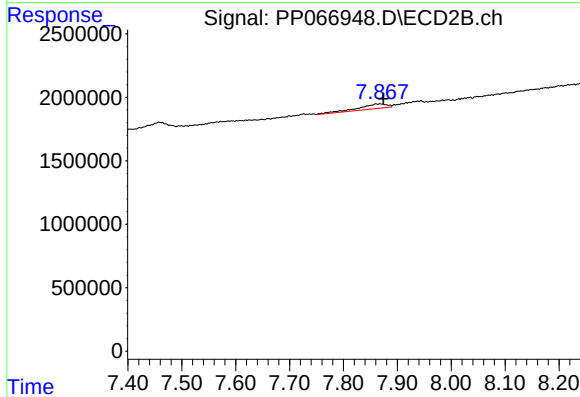


#41 AR-1268-1

R.T.: 7.868 min
Delta R.T.: -0.006 min
Response: 1411606
Conc: 11.29 ng/ml

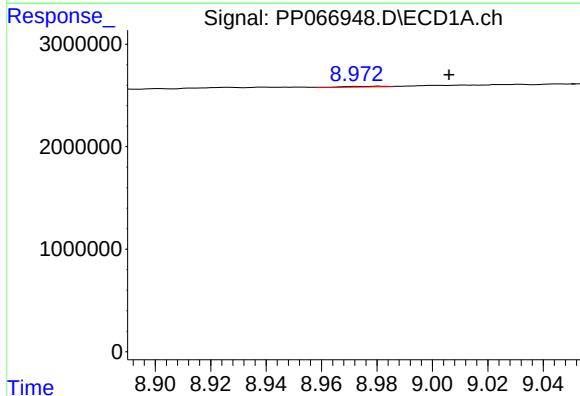


#42 AR-1268-2

R.T.: 8.981 min
Delta R.T.: -0.025 min
Response: 72045
Conc: 0.62 ng/ml

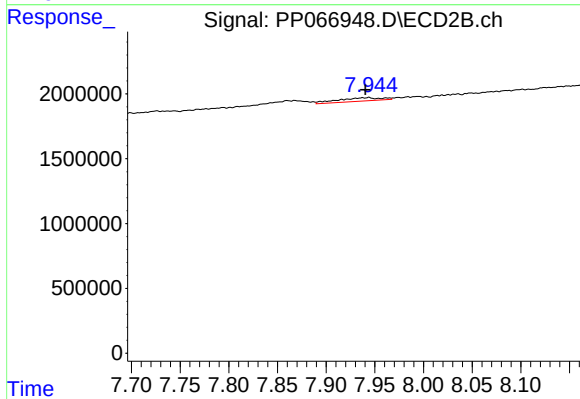

#42 AR-1268-2


R.T.: 7.944 min
Delta R.T.: 0.004 min
Response: 821287
Conc: 7.35 ng/ml

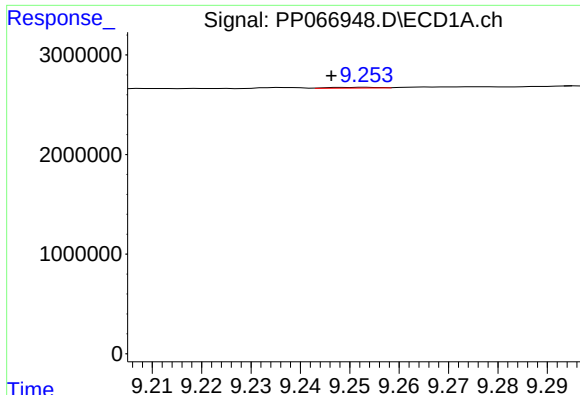

#43 AR-1268-3


R.T.: 9.253 min
Delta R.T.: 0.007 min
Response: 56894
Conc: 0.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

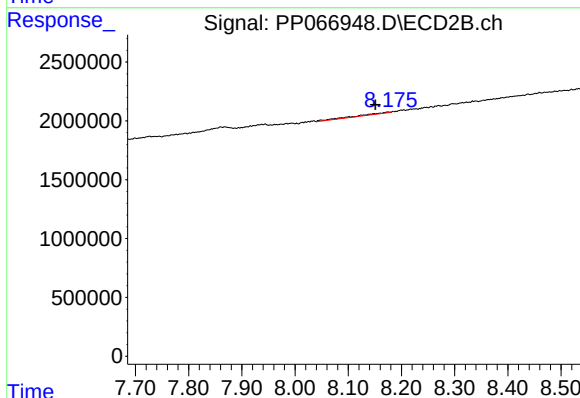


#43 AR-1268-3

R.T.: 8.175 min
Delta R.T.: 0.024 min
Response: 441892
Conc: 4.32 ng/ml

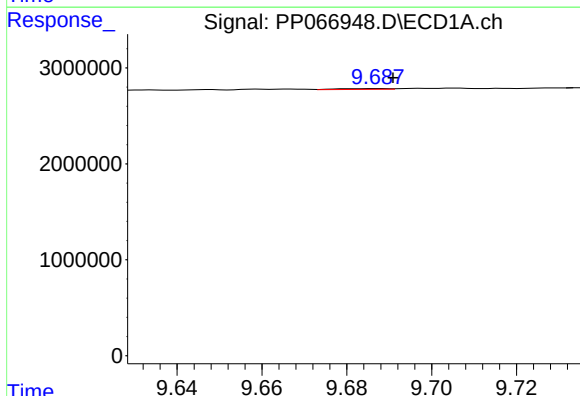


#44 AR-1268-4

R.T.: 9.687 min
Delta R.T.: -0.004 min
Response: 73262
Conc: 2.45 ng/ml

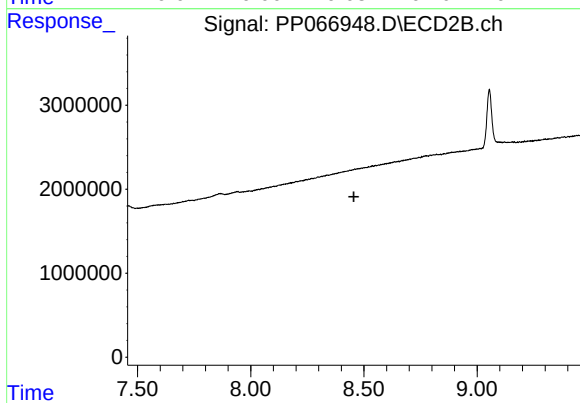

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.456 min
Response: 0
Conc: N.D.

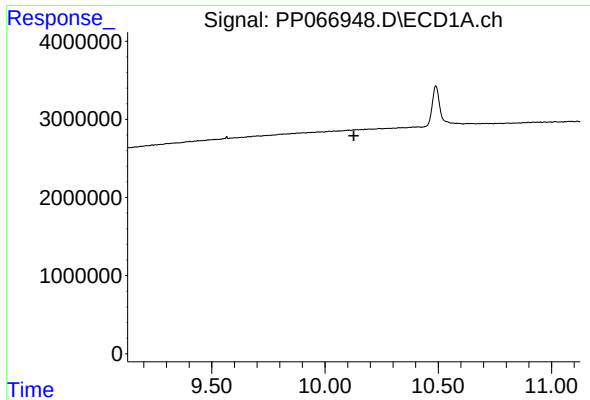

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.127 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

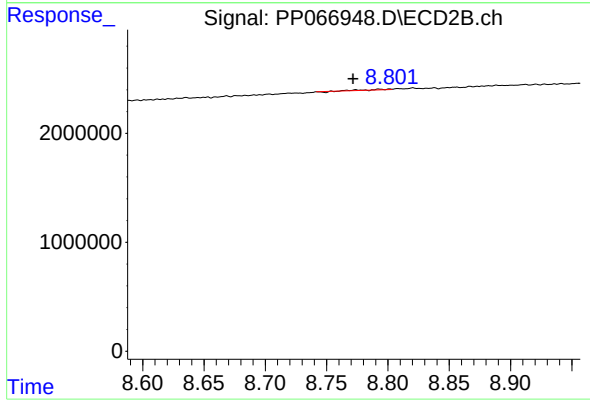

#45 AR-1268-5

R.T.: 8.793 min
Delta R.T.: 0.021 min
Response: 53924
Conc: 0.22 ng/ml