

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
 Data File : PP066949.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2024 14:33
 Operator : YP\AJ
 Sample : P3390-09
 Misc : AR1242 MDL 25 PPB
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 04:36:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 09:05:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.627	3.914	30957553	25018544	18.392	17.454
2)	SA Decachlor...	10.488	9.052	12763054	11725042	15.221	15.655
Target Compounds							
3)	L1 AR-1016-1	5.802	5.022	856922	808192	18.111	18.514
4)	L1 AR-1016-2	5.824	5.042	1445496	1162995	19.537	18.073
5)	L1 AR-1016-3	5.885	5.223	965924	678755	20.588	19.766
6)	L1 AR-1016-4	5.986	5.264	556995	583979	15.405	19.279 #
7)	L1 AR-1016-5	6.278	5.482	646087	584853	18.860	16.201
8)	L2 AR-1221-1	4.902f	0.000	141762	0	7.815	N.D. #
9)	L2 AR-1221-2	4.936	4.222	513631	465505	38.153	39.785
10)	L2 AR-1221-3	4.998	4.296	587957	593794	14.548	15.595
11)	L3 AR-1232-1	4.998	4.296	587957	593794	17.636	18.867
12)	L3 AR-1232-2	5.532	5.042	844797	1162995	47.855	39.439
13)	L3 AR-1232-3	5.824	5.223	1445496	678755	46.294	47.792
14)	L3 AR-1232-4	5.986	5.306	556995	723429	36.405	51.468 #
15)	L3 AR-1232-5	6.072	5.482	648730	584853	51.557	41.117
16)	L4 AR-1242-1	5.802	5.022	856922	808192	24.912	26.016
17)	L4 AR-1242-2	5.824	5.042	1445496	1162995	27.213	26.057
18)	L4 AR-1242-3	5.885	5.223	965924	678755	28.167	28.137
19)	L4 AR-1242-4	5.986	5.306	556995	723429	21.465	27.034 #
20)	L4 AR-1242-5	6.722	5.837	599486	682153	25.800	24.441
21)	L5 AR-1248-1	5.802	5.022	856922	808192	35.498	36.721
22)	L5 AR-1248-2	6.072	5.264	648730	583979	16.657	16.622
23)	L5 AR-1248-3	6.278	5.306	646087	723429	15.862	19.881 #
24)	L5 AR-1248-4	6.681	5.482	563237	584853	14.537	14.393
25)	L5 AR-1248-5	6.722	5.880	599486	640105	15.224	20.037 #
26)	L6 AR-1254-1	6.657	5.837	741905	682153	14.910	11.495
27)	L6 AR-1254-2	6.880	5.987	710237	180745	10.055	3.449 #
28)	L6 AR-1254-3	7.246	6.396	617775	836373	9.067	10.963
29)	L6 AR-1254-4	7.524	6.626	428873	599623	10.242	15.874 #
30)	L6 AR-1254-5	7.945	7.049	1680944	577164	31.990	9.170 #
31)	L7 AR-1260-1	7.402	6.541	160885	745695	2.658	11.771 #
32)	L7 AR-1260-2	7.661	6.710	272408	397084	4.238	5.873 #
33)	L7 AR-1260-3	8.018	6.881	105413	666559	2.361	10.008 #
34)	L7 AR-1260-4	8.238	7.392f	147991	1102482	2.954	25.155 #
35)	L7 AR-1260-5	8.583	7.592	274807	325646	3.288	3.651
36)	L8 AR-1262-1	8.238	7.049f	147991	577164	2.263	7.989 #
37)	L8 AR-1262-2	8.583	7.392f	274807	1102482	2.657	17.917 #
38)	L8 AR-1262-3	8.924	7.865	197110	728318	2.760	17.314 #
39)	L8 AR-1262-4	9.019	7.940	314103	538014	5.320	6.936 #
40)	L8 AR-1262-5	9.688	8.451	58676	37540	2.133	1.422 #
41)	L9 AR-1268-1	8.924	7.865	197110	728318	1.508	5.823 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
Data File : PP066949.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2024 14:33
Operator : YP\AJ
Sample : P3390-09
Misc : AR1242 MDL 25 PPB
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 04:36:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 09:05:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	9.019	7.940	314103	538014	2.684	4.814 #
43) L9	AR-1268-3	9.233	8.165	45997	162246	0.442	1.587 #
44) L9	AR-1268-4	9.688	8.451	58676	37540	1.960	1.322 #
45) L9	AR-1268-5	10.142	0.000	57200	0	0.204	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
Data File : PP066949.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2024 14:33
Operator : YP\AJ
Sample : P3390-09
Misc : AR1242 MDL 25 PPB
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 04:36:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 09:05:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

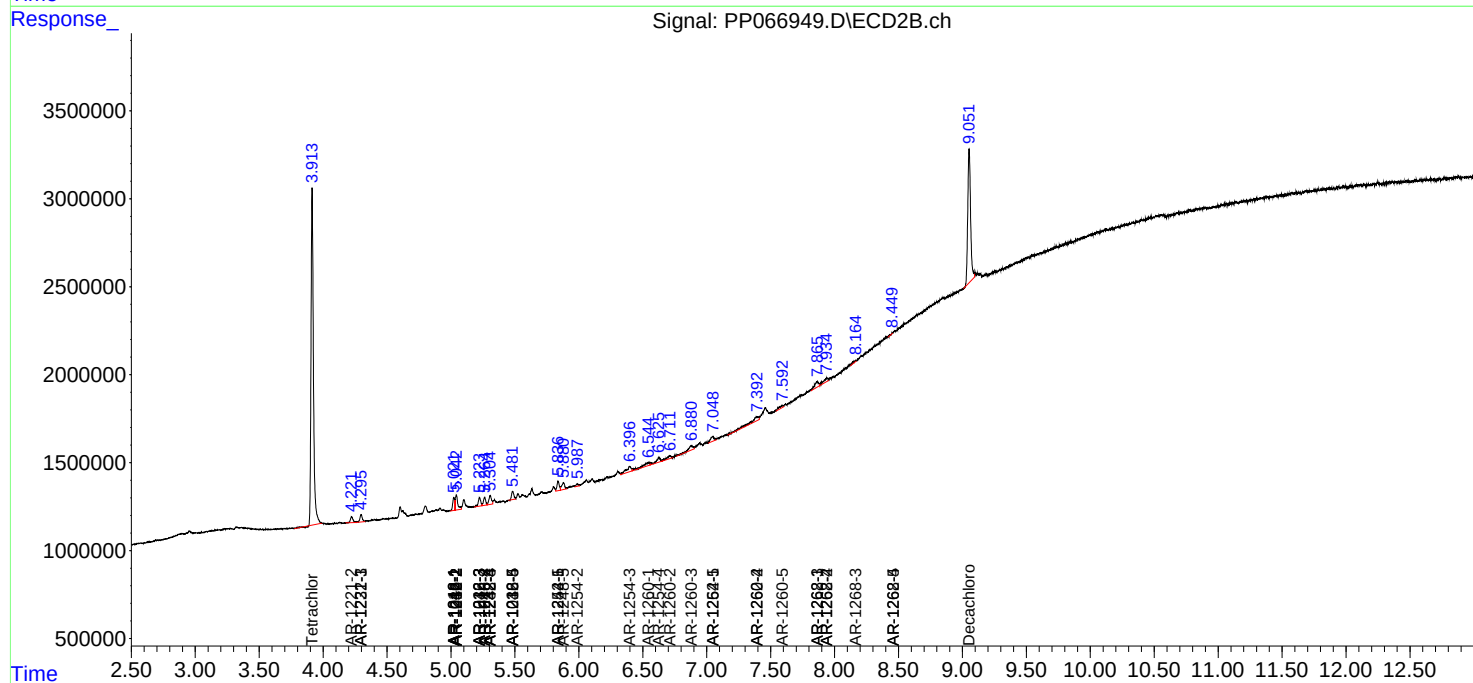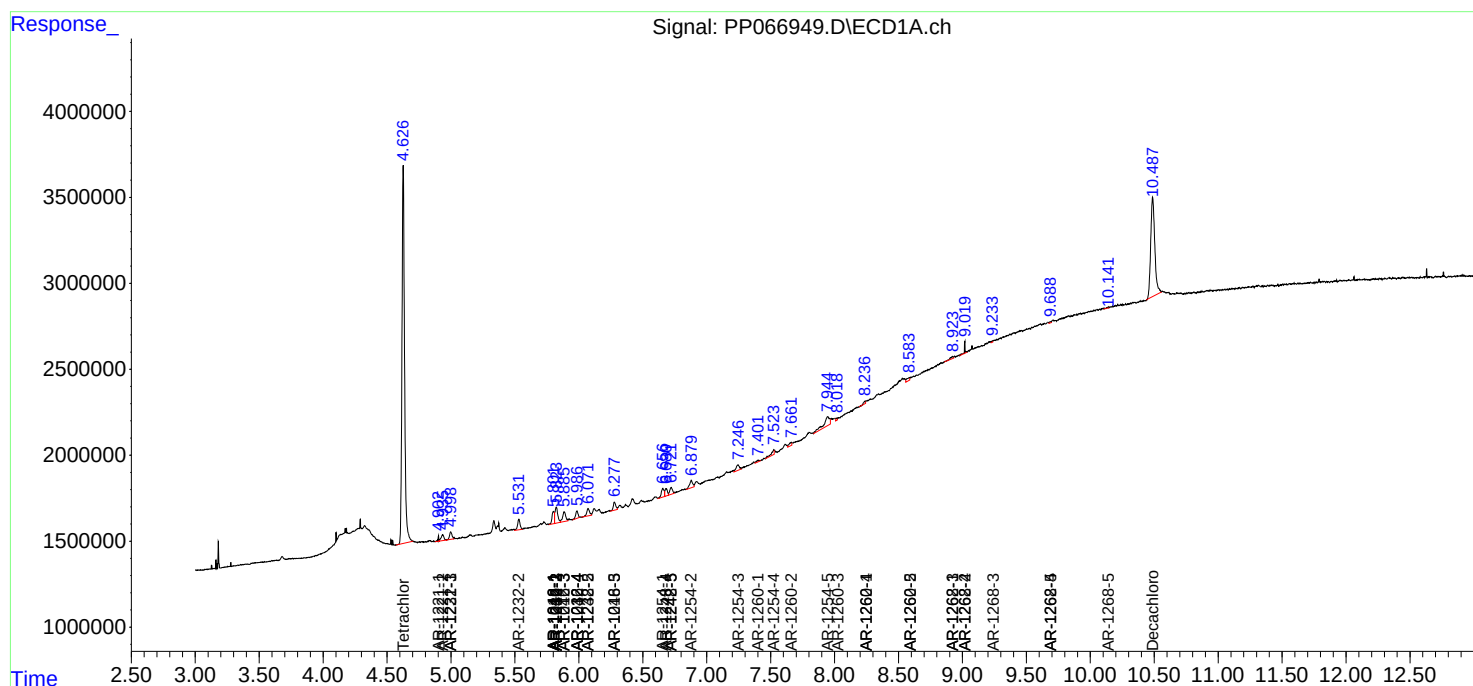


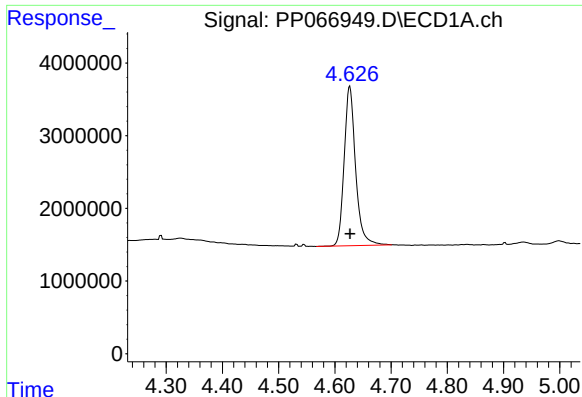

#1 Tetrachloro-m-xylene


R.T.: 4.627 min
Delta R.T.: 0.000 min
Response: 30957553
Conc: 18.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

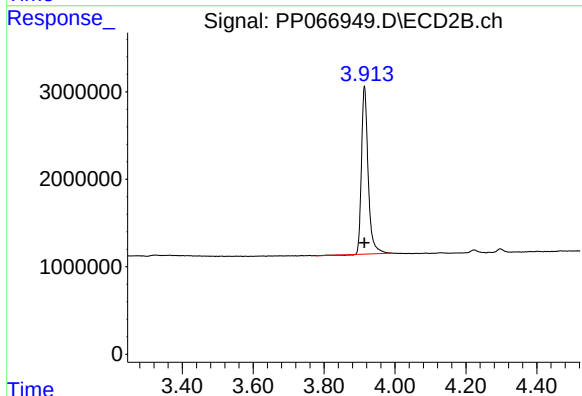


#1 Tetrachloro-m-xylene

R.T.: 3.914 min
Delta R.T.: 0.000 min
Response: 25018544
Conc: 17.45 ng/ml

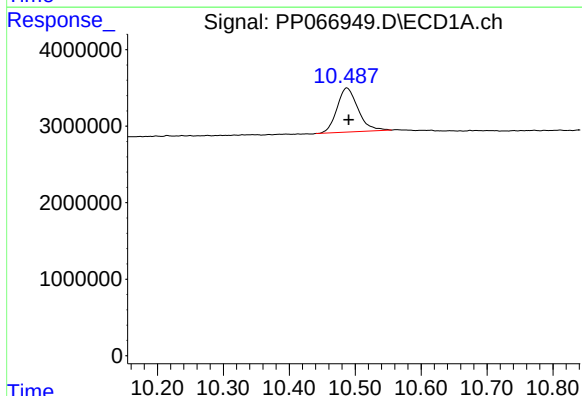


#2 Decachlorobiphenyl

R.T.: 10.488 min
Delta R.T.: -0.003 min
Response: 12763054
Conc: 15.22 ng/ml

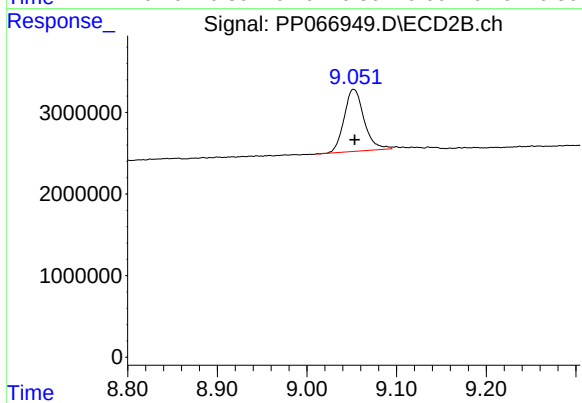

#2 Decachlorobiphenyl


R.T.: 9.052 min
Delta R.T.: -0.001 min
Response: 11725042
Conc: 15.65 ng/ml

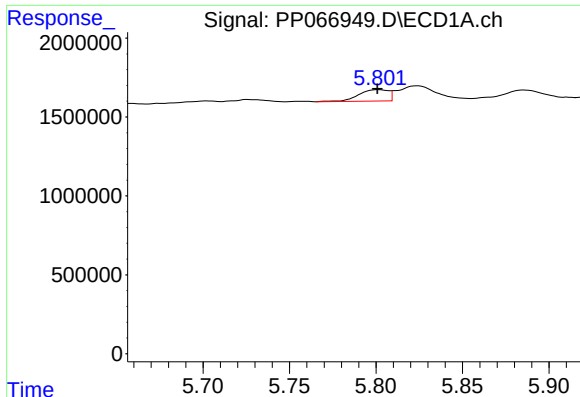

#3 AR-1016-1


R.T.: 5.802 min
Delta R.T.: 0.000 min
Response: 856922
Conc: 18.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

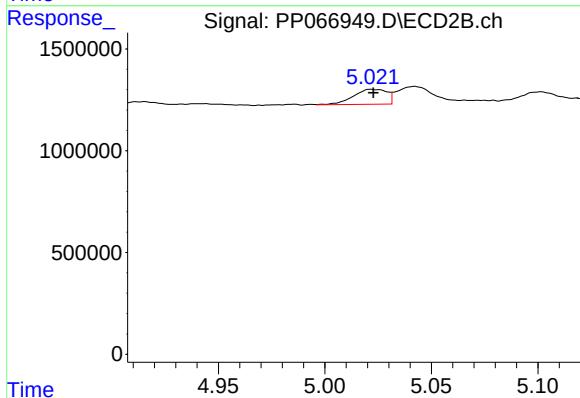


#3 AR-1016-1

R.T.: 5.022 min
Delta R.T.: 0.000 min
Response: 808192
Conc: 18.51 ng/ml

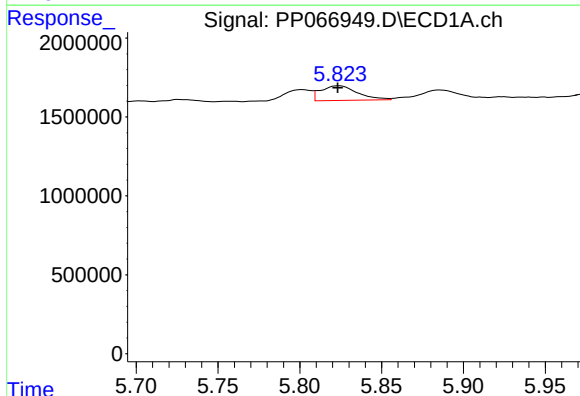


#4 AR-1016-2

R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 1445496
Conc: 19.54 ng/ml

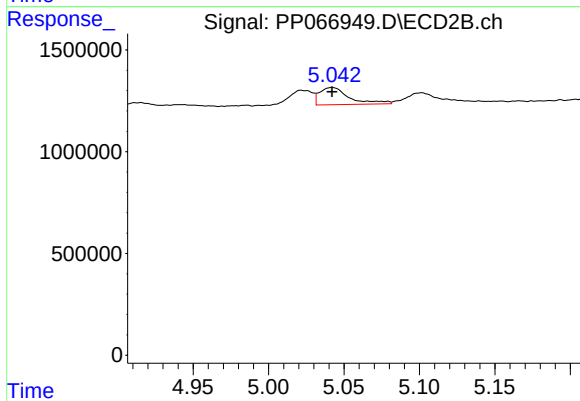

#4 AR-1016-2


R.T.: 5.042 min
Delta R.T.: 0.000 min
Response: 1162995
Conc: 18.07 ng/ml

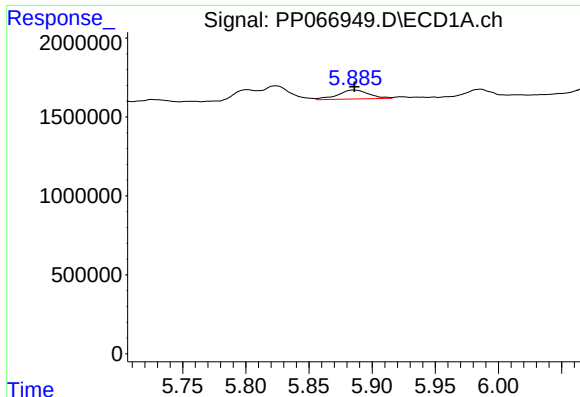

#5 AR-1016-3


R.T.: 5.885 min
Delta R.T.: 0.000 min
Response: 965924
Conc: 20.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

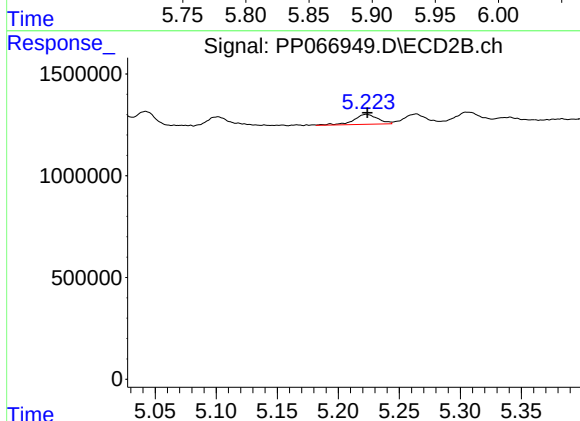


#5 AR-1016-3

R.T.: 5.223 min
Delta R.T.: 0.000 min
Response: 678755
Conc: 19.77 ng/ml

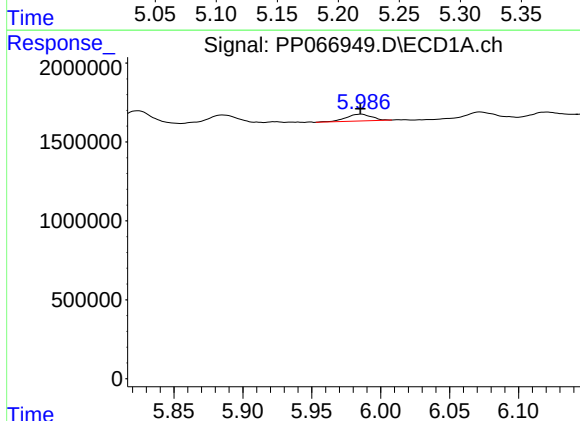


#6 AR-1016-4

R.T.: 5.986 min
Delta R.T.: 0.000 min
Response: 556995
Conc: 15.41 ng/ml

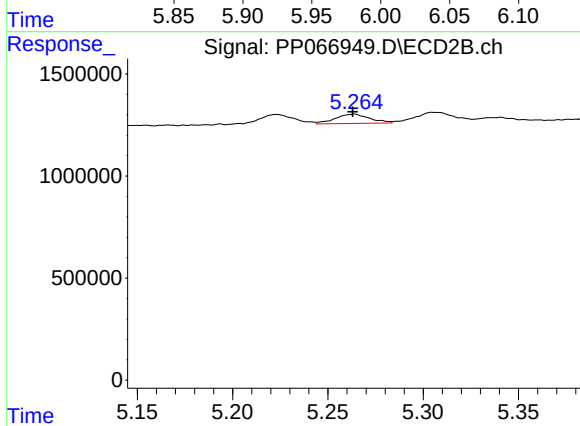

#6 AR-1016-4


R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 583979
Conc: 19.28 ng/ml

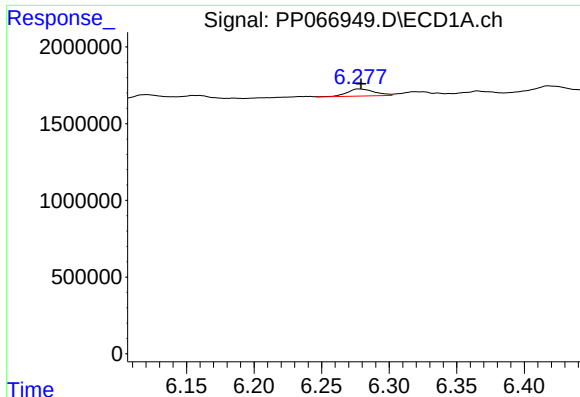

#7 AR-1016-5


R.T.: 6.278 min
Delta R.T.: -0.001 min
Response: 646087
Conc: 18.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

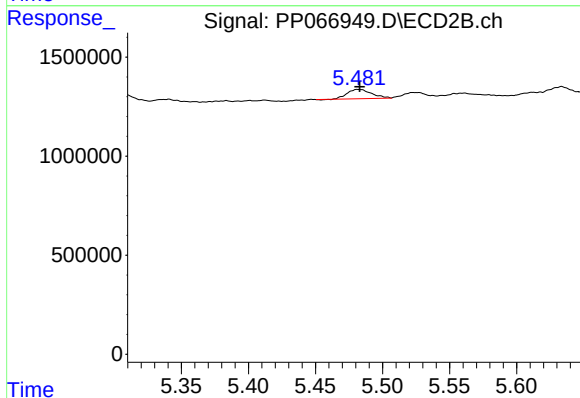


#7 AR-1016-5

R.T.: 5.482 min
Delta R.T.: 0.000 min
Response: 584853
Conc: 16.20 ng/ml

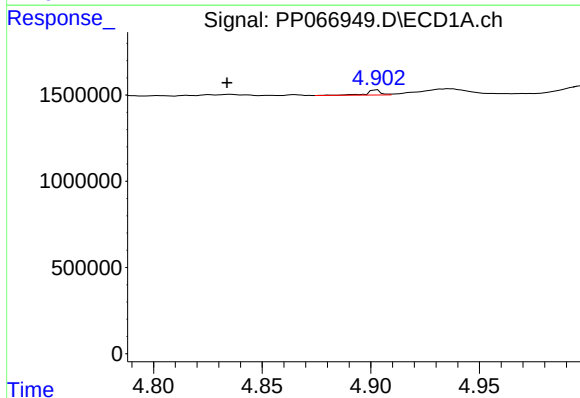


#8 AR-1221-1

R.T.: 4.902 min
Delta R.T.: 0.069 min
Response: 141762
Conc: 7.81 ng/ml

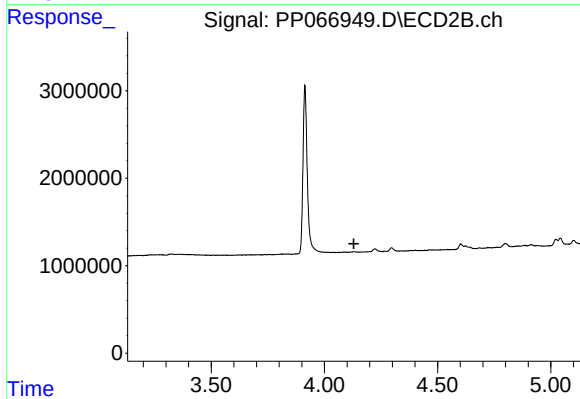

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 4.130 min
Response: 0
Conc: N.D.

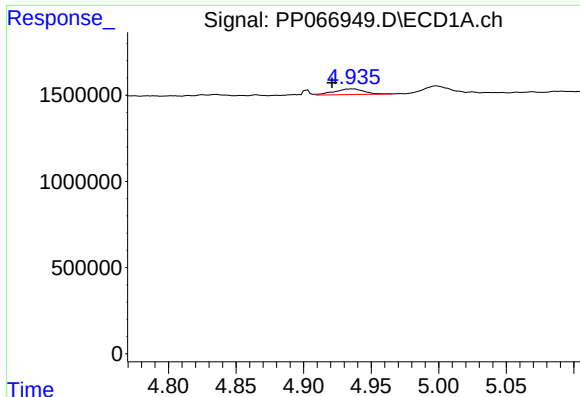

#9 AR-1221-2


R.T.: 4.936 min
Delta R.T.: 0.015 min
Response: 513631
Conc: 38.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

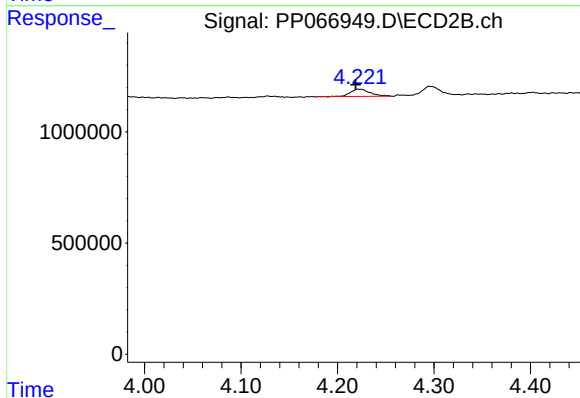


#9 AR-1221-2

R.T.: 4.222 min
Delta R.T.: 0.003 min
Response: 465505
Conc: 39.78 ng/ml

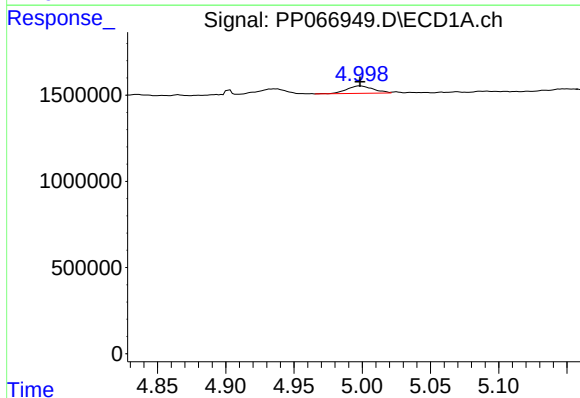


#10 AR-1221-3

R.T.: 4.998 min
Delta R.T.: 0.000 min
Response: 587957
Conc: 14.55 ng/ml

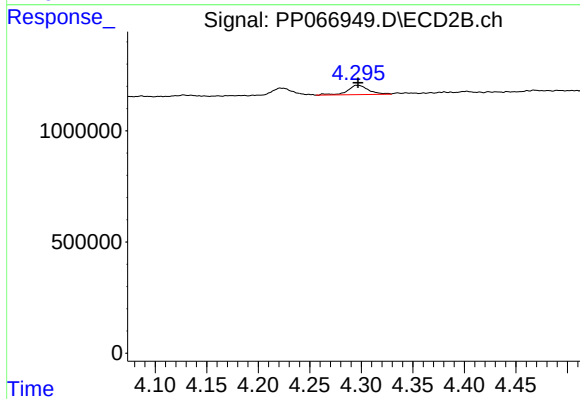

#10 AR-1221-3


R.T.: 4.296 min
Delta R.T.: 0.000 min
Response: 593794
Conc: 15.60 ng/ml

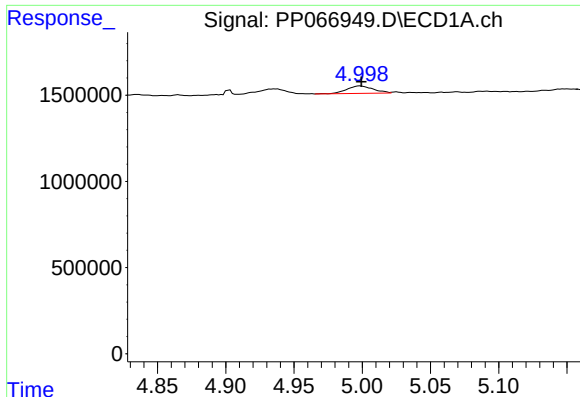

#11 AR-1232-1


R.T.: 4.998 min
Delta R.T.: 0.000 min
Response: 587957
Conc: 17.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

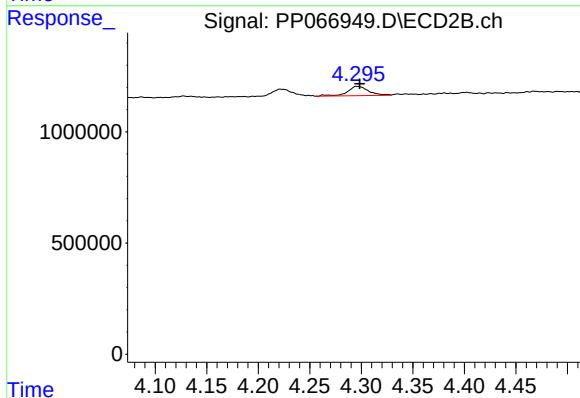


#11 AR-1232-1

R.T.: 4.296 min
Delta R.T.: -0.002 min
Response: 593794
Conc: 18.87 ng/ml

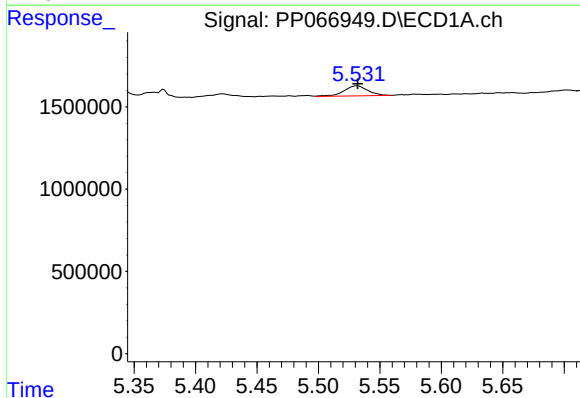


#12 AR-1232-2

R.T.: 5.532 min
Delta R.T.: 0.000 min
Response: 844797
Conc: 47.85 ng/ml

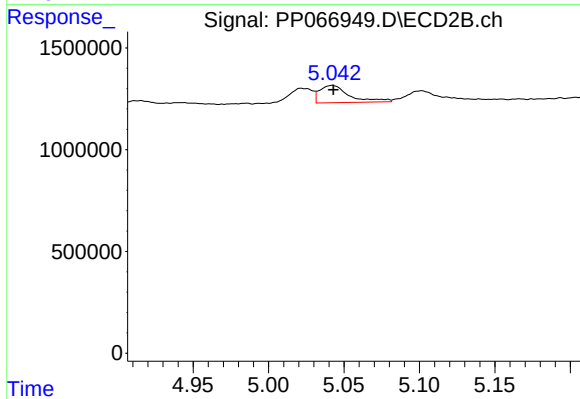

#12 AR-1232-2


R.T.: 5.042 min
Delta R.T.: 0.000 min
Response: 1162995
Conc: 39.44 ng/ml

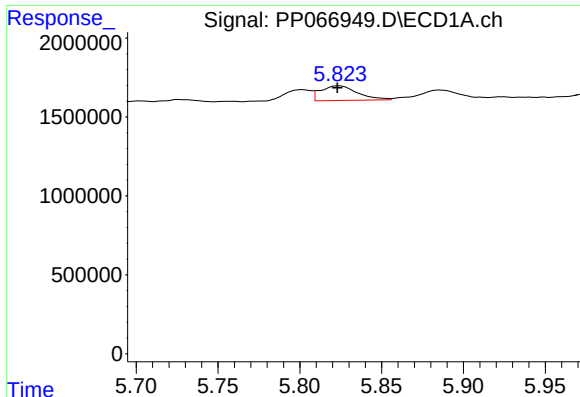

#13 AR-1232-3


R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 1445496
Conc: 46.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

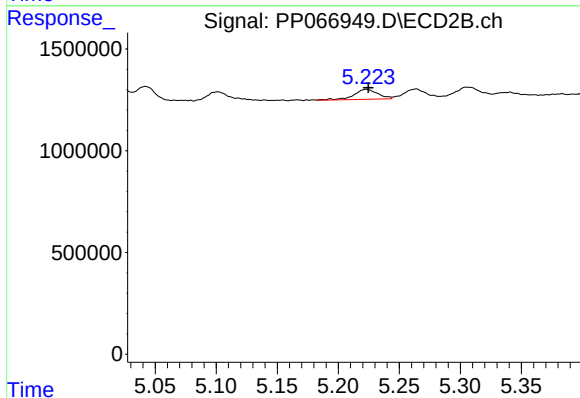


#13 AR-1232-3

R.T.: 5.223 min
Delta R.T.: -0.001 min
Response: 678755
Conc: 47.79 ng/ml

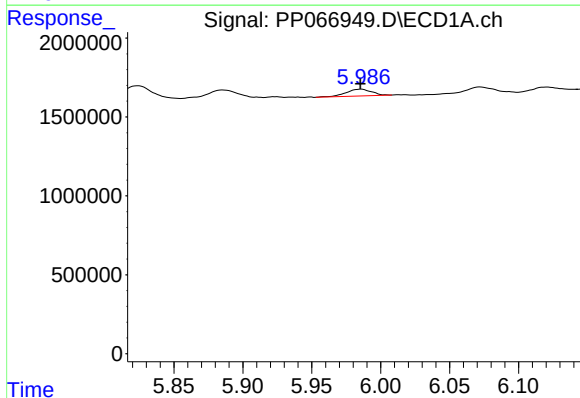


#14 AR-1232-4

R.T.: 5.986 min
Delta R.T.: 0.000 min
Response: 556995
Conc: 36.40 ng/ml

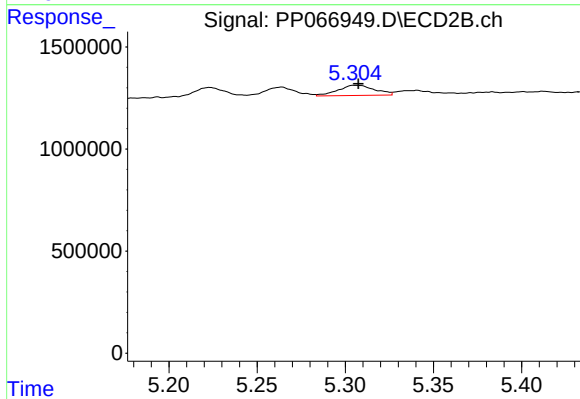

#14 AR-1232-4


R.T.: 5.306 min
Delta R.T.: -0.002 min
Response: 723429
Conc: 51.47 ng/ml

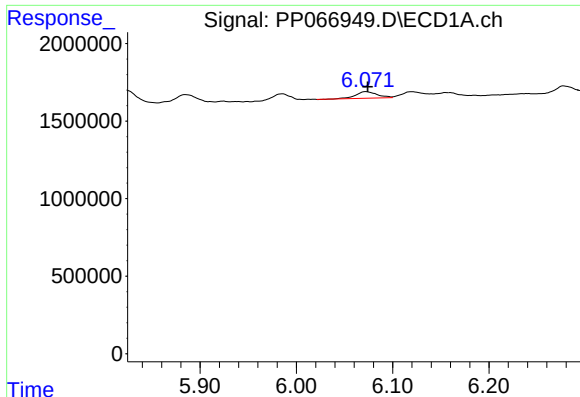

#15 AR-1232-5


R.T.: 6.072 min
Delta R.T.: -0.002 min
Response: 648730
Conc: 51.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

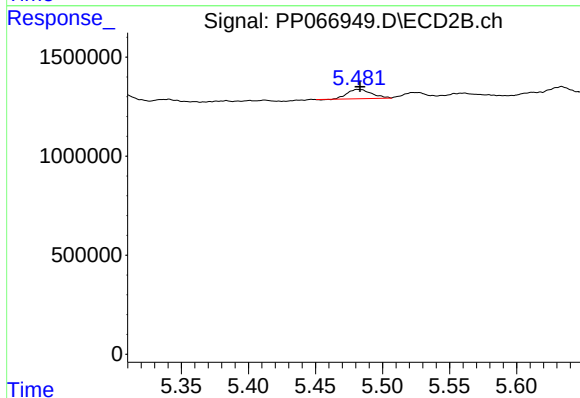


#15 AR-1232-5

R.T.: 5.482 min
Delta R.T.: 0.000 min
Response: 584853
Conc: 41.12 ng/ml

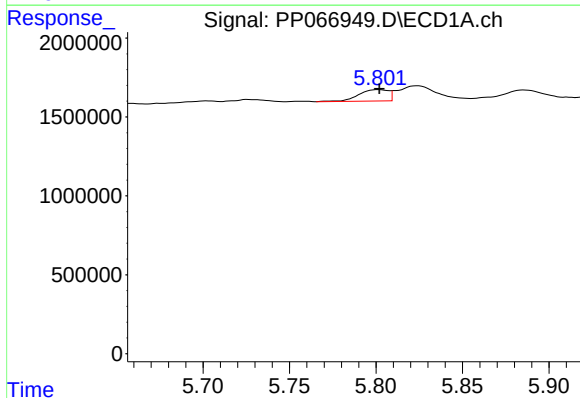


#16 AR-1242-1

R.T.: 5.802 min
Delta R.T.: 0.000 min
Response: 856922
Conc: 24.91 ng/ml

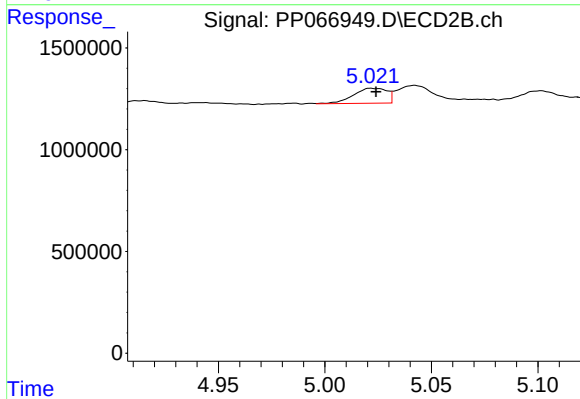

#16 AR-1242-1


R.T.: 5.022 min
Delta R.T.: -0.002 min
Response: 808192
Conc: 26.02 ng/ml

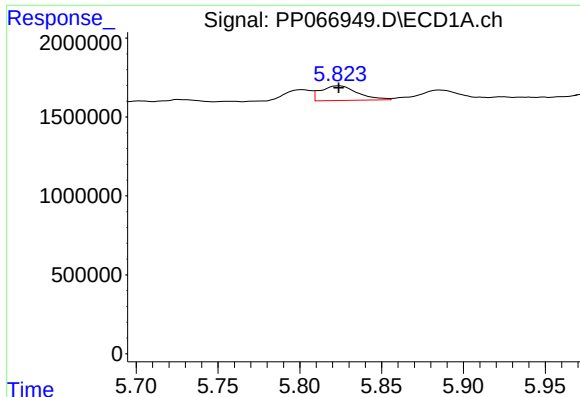

#17 AR-1242-2


R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 1445496
Conc: 27.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

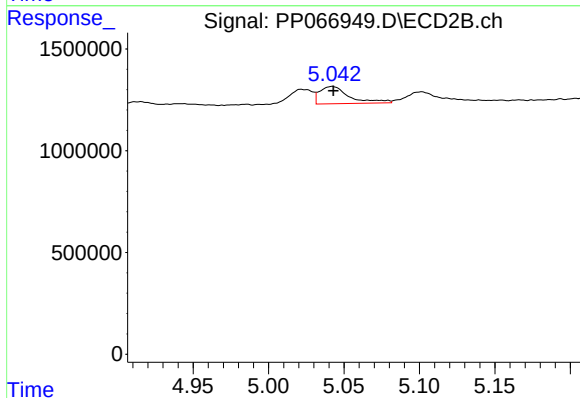


#17 AR-1242-2

R.T.: 5.042 min
Delta R.T.: 0.000 min
Response: 1162995
Conc: 26.06 ng/ml

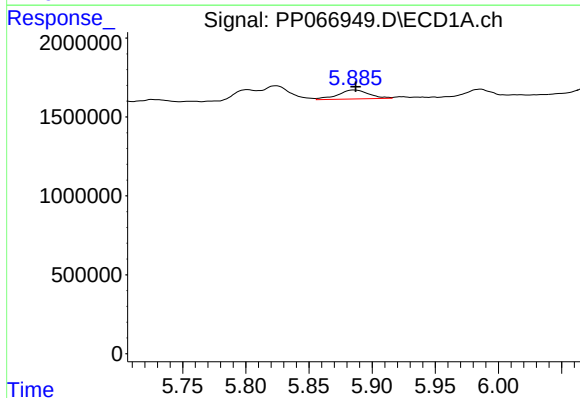


#18 AR-1242-3

R.T.: 5.885 min
Delta R.T.: -0.002 min
Response: 965924
Conc: 28.17 ng/ml

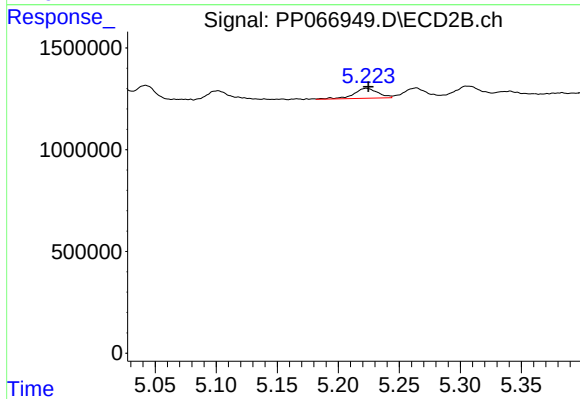

#18 AR-1242-3


R.T.: 5.223 min
Delta R.T.: -0.001 min
Response: 678755
Conc: 28.14 ng/ml

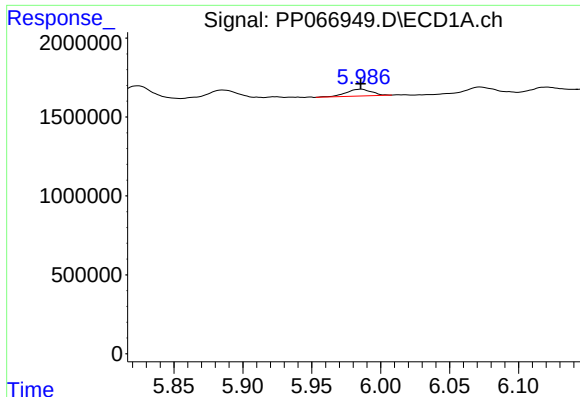

#19 AR-1242-4


R.T.: 5.986 min
Delta R.T.: 0.000 min
Response: 556995
Conc: 21.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

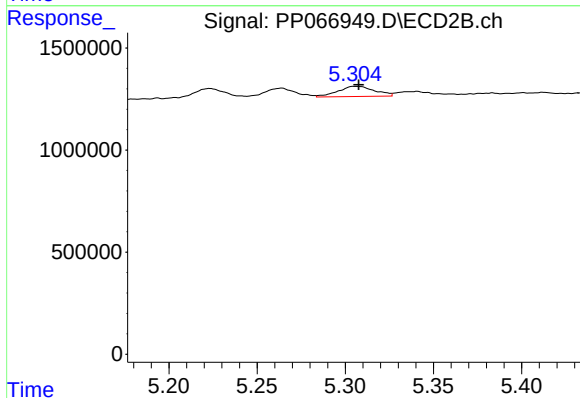


#19 AR-1242-4

R.T.: 5.306 min
Delta R.T.: -0.002 min
Response: 723429
Conc: 27.03 ng/ml

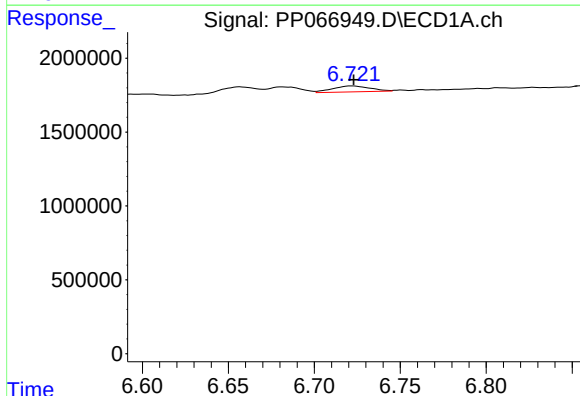


#20 AR-1242-5

R.T.: 6.722 min
Delta R.T.: 0.000 min
Response: 599486
Conc: 25.80 ng/ml

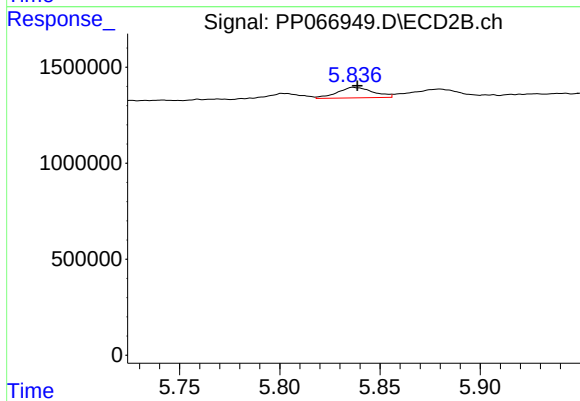

#20 AR-1242-5


R.T.: 5.837 min
Delta R.T.: -0.002 min
Response: 682153
Conc: 24.44 ng/ml

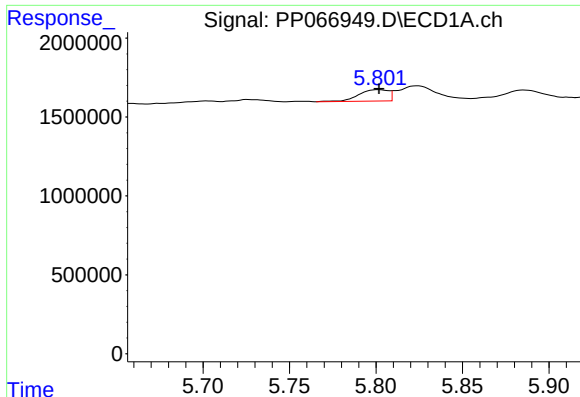

#21 AR-1248-1


R.T.: 5.802 min
Delta R.T.: 0.000 min
Response: 856922
Conc: 35.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

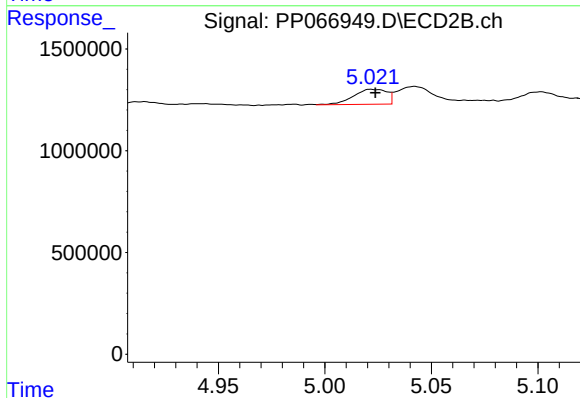


#21 AR-1248-1

R.T.: 5.022 min
Delta R.T.: -0.002 min
Response: 808192
Conc: 36.72 ng/ml

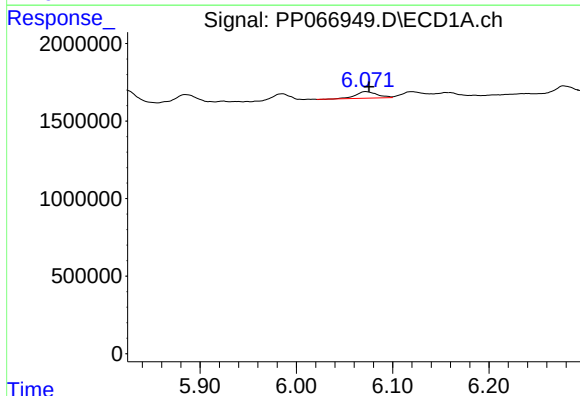


#22 AR-1248-2

R.T.: 6.072 min
Delta R.T.: -0.003 min
Response: 648730
Conc: 16.66 ng/ml

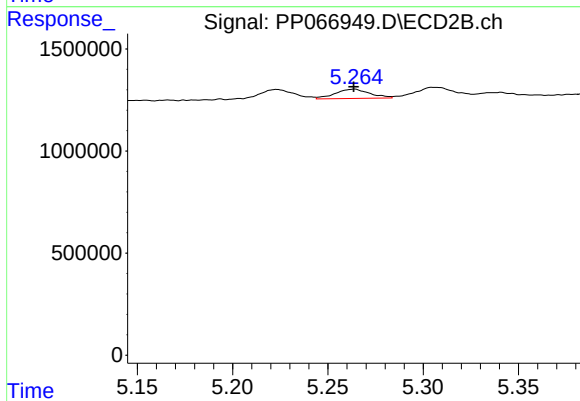

#22 AR-1248-2


R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 583979
Conc: 16.62 ng/ml

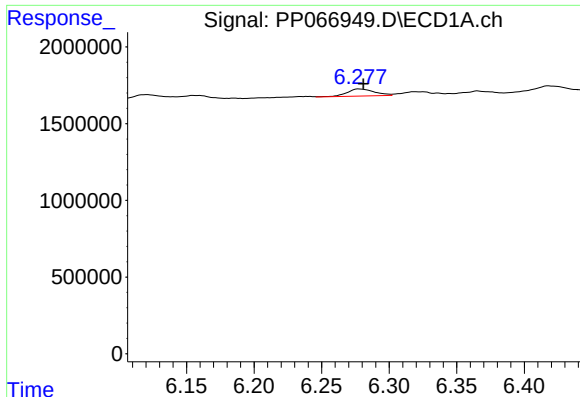

#23 AR-1248-3


R.T.: 6.278 min
Delta R.T.: -0.003 min
Response: 646087
Conc: 15.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

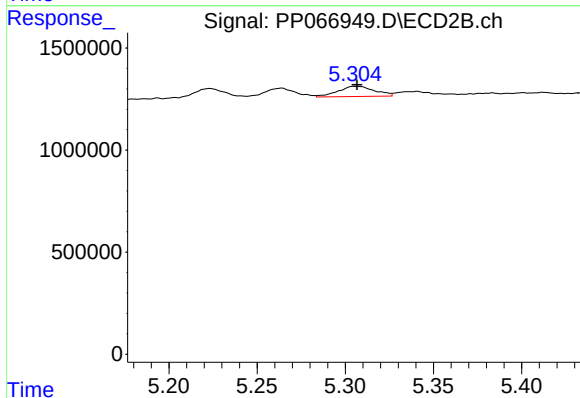


#23 AR-1248-3

R.T.: 5.306 min
Delta R.T.: 0.000 min
Response: 723429
Conc: 19.88 ng/ml

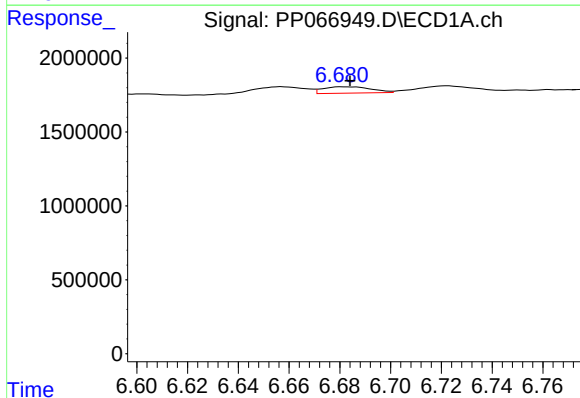


#24 AR-1248-4

R.T.: 6.681 min
Delta R.T.: -0.003 min
Response: 563237
Conc: 14.54 ng/ml

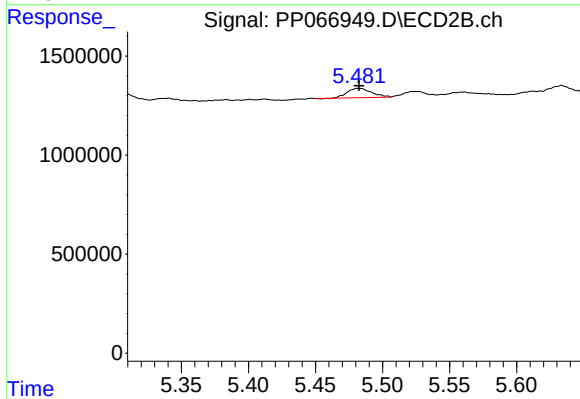

#24 AR-1248-4


R.T.: 5.482 min
Delta R.T.: 0.000 min
Response: 584853
Conc: 14.39 ng/ml

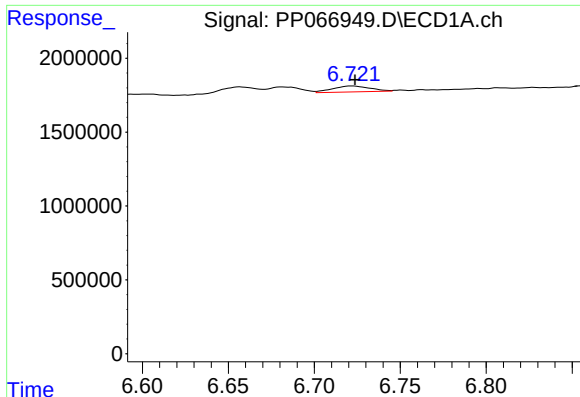

#25 AR-1248-5


R.T.: 6.722 min
Delta R.T.: -0.002 min
Response: 599486
Conc: 15.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

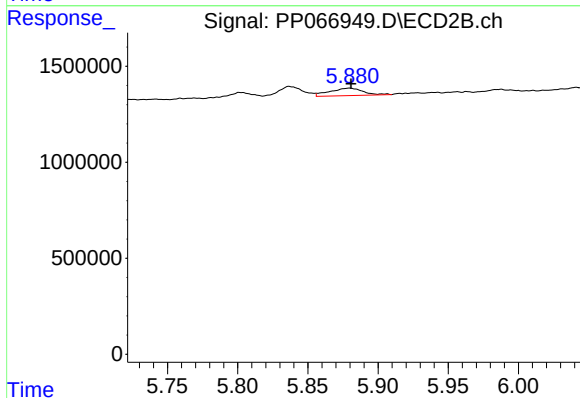


#25 AR-1248-5

R.T.: 5.880 min
Delta R.T.: 0.000 min
Response: 640105
Conc: 20.04 ng/ml

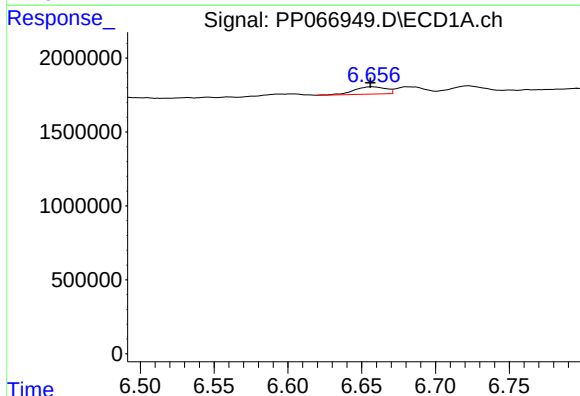


#26 AR-1254-1

R.T.: 6.657 min
Delta R.T.: 0.001 min
Response: 741905
Conc: 14.91 ng/ml

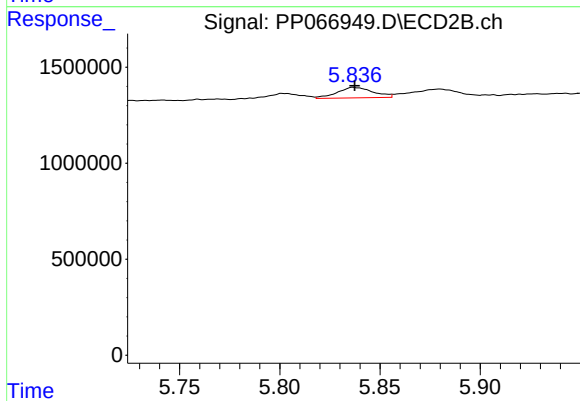

#26 AR-1254-1


R.T.: 5.837 min
Delta R.T.: 0.000 min
Response: 682153
Conc: 11.50 ng/ml

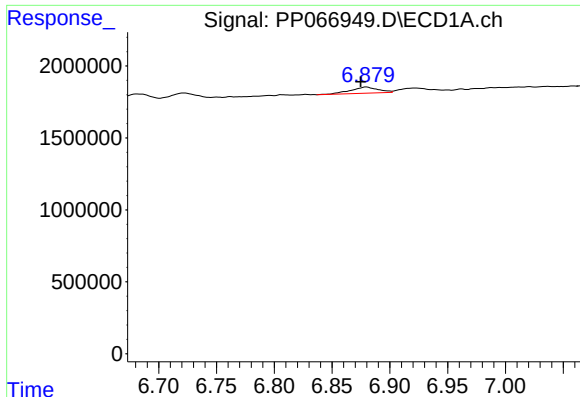

#27 AR-1254-2


R.T.: 6.880 min
Delta R.T.: 0.005 min
Response: 710237
Conc: 10.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

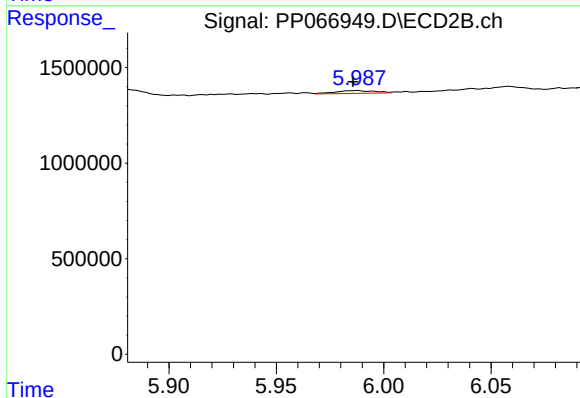


#27 AR-1254-2

R.T.: 5.987 min
Delta R.T.: 0.001 min
Response: 180745
Conc: 3.45 ng/ml

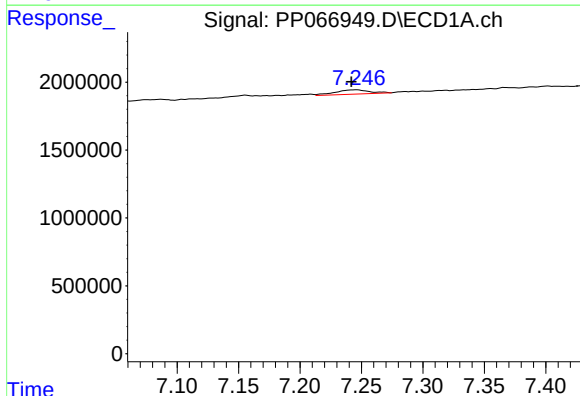


#28 AR-1254-3

R.T.: 7.246 min
Delta R.T.: 0.004 min
Response: 617775
Conc: 9.07 ng/ml

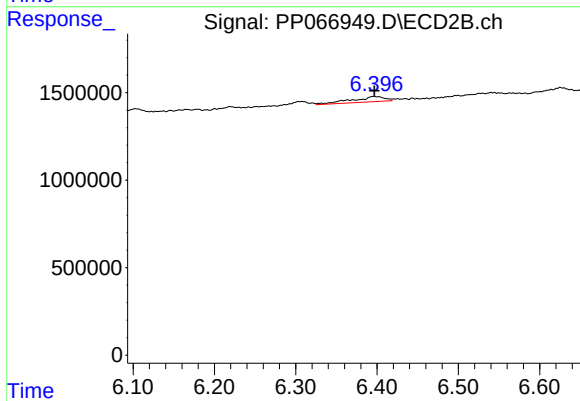

#28 AR-1254-3


R.T.: 6.396 min
Delta R.T.: 0.000 min
Response: 836373
Conc: 10.96 ng/ml

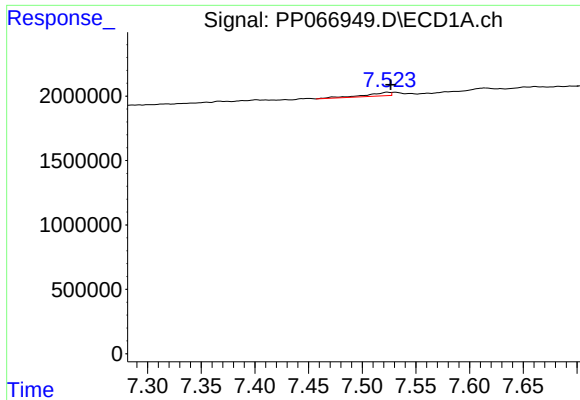

#29 AR-1254-4


R.T.: 7.524 min
Delta R.T.: -0.003 min
Response: 428873
Conc: 10.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

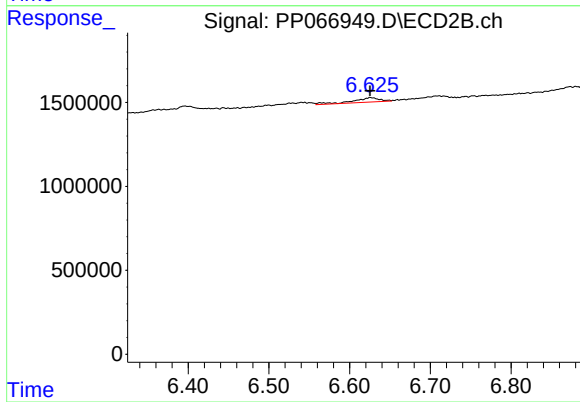


#29 AR-1254-4

R.T.: 6.626 min
Delta R.T.: 0.000 min
Response: 599623
Conc: 15.87 ng/ml

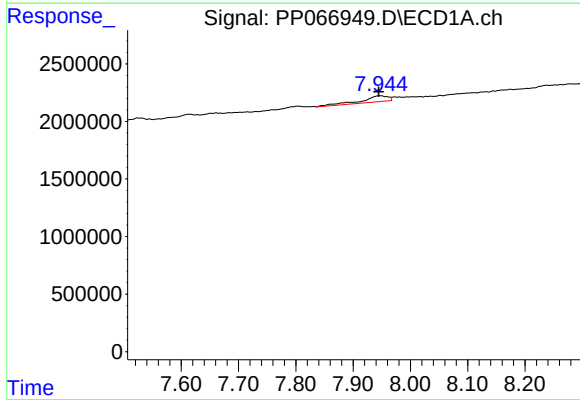


#30 AR-1254-5

R.T.: 7.945 min
Delta R.T.: 0.000 min
Response: 1680944
Conc: 31.99 ng/ml

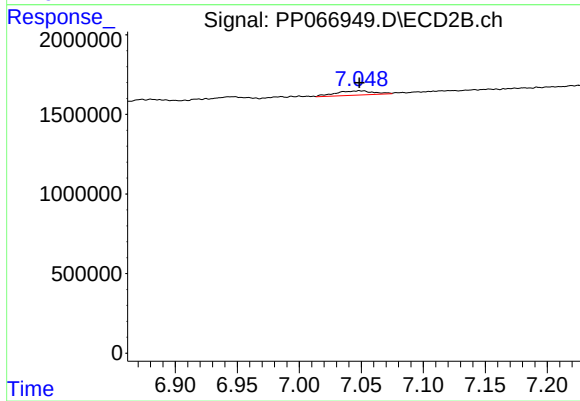

#30 AR-1254-5


R.T.: 7.049 min
Delta R.T.: 0.000 min
Response: 577164
Conc: 9.17 ng/ml

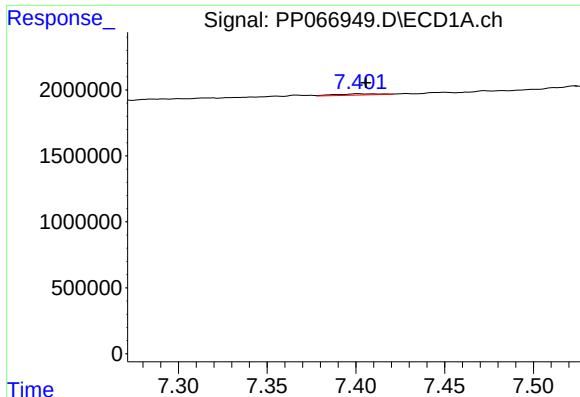

#31 AR-1260-1


R.T.: 7.402 min
Delta R.T.: -0.004 min
Response: 160885
Conc: 2.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

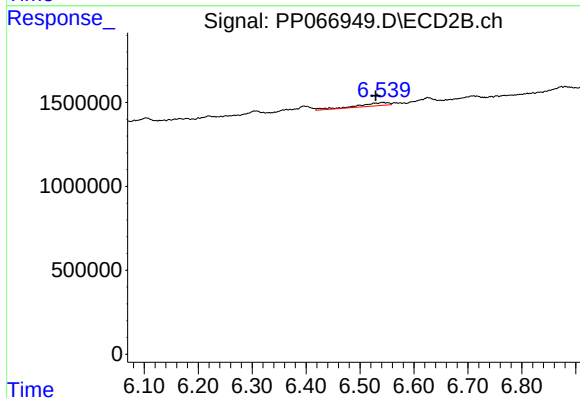


#31 AR-1260-1

R.T.: 6.541 min
Delta R.T.: 0.011 min
Response: 745695
Conc: 11.77 ng/ml

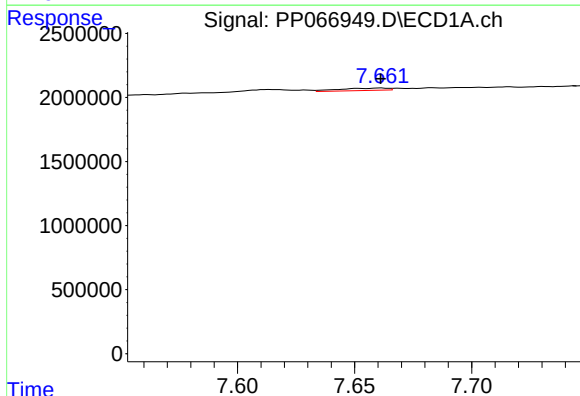


#32 AR-1260-2

R.T.: 7.661 min
Delta R.T.: 0.000 min
Response: 272408
Conc: 4.24 ng/ml

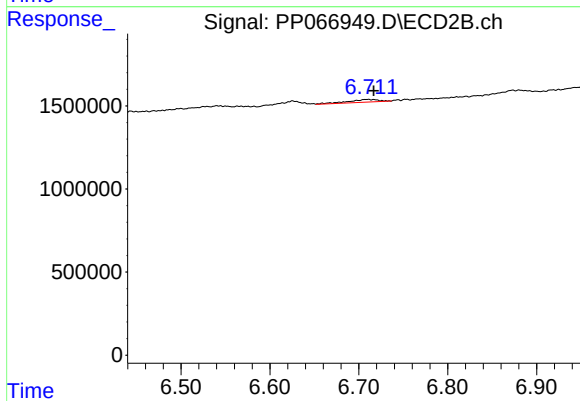

#32 AR-1260-2


R.T.: 6.710 min
Delta R.T.: -0.007 min
Response: 397084
Conc: 5.87 ng/ml

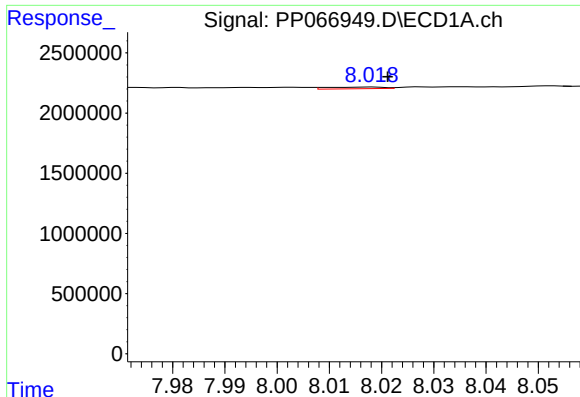

#33 AR-1260-3


R.T.: 8.018 min
Delta R.T.: -0.003 min
Response: 105413
Conc: 2.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

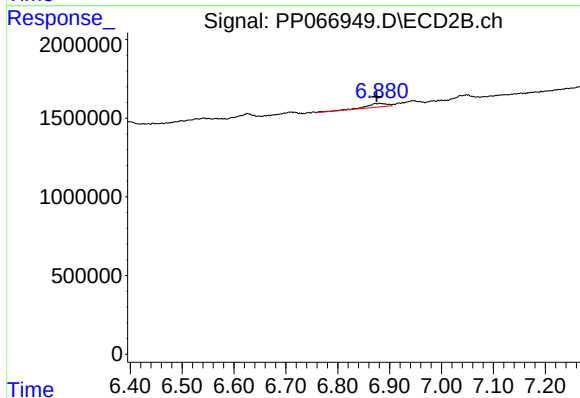


#33 AR-1260-3

R.T.: 6.881 min
Delta R.T.: 0.006 min
Response: 666559
Conc: 10.01 ng/ml

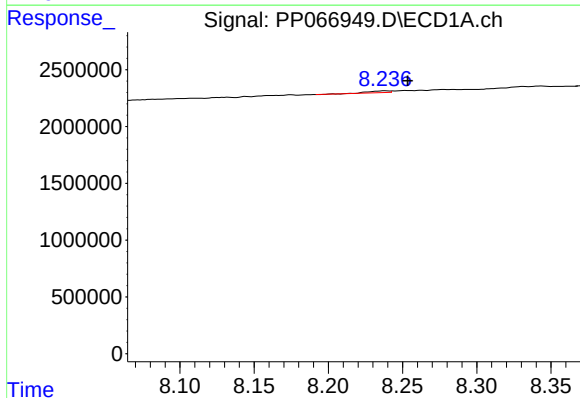


#34 AR-1260-4

R.T.: 8.238 min
Delta R.T.: -0.015 min
Response: 147991
Conc: 2.95 ng/ml

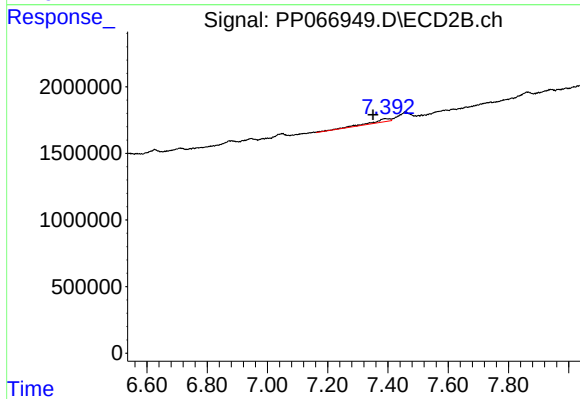

#34 AR-1260-4


R.T.: 7.392 min
Delta R.T.: 0.041 min
Response: 1102482
Conc: 25.16 ng/ml

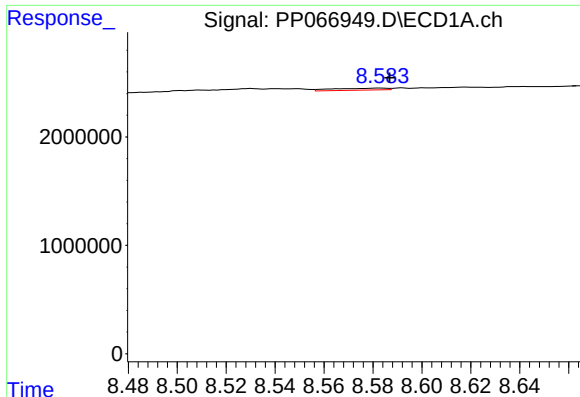

#35 AR-1260-5


R.T.: 8.583 min
Delta R.T.: -0.004 min
Response: 274807
Conc: 3.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

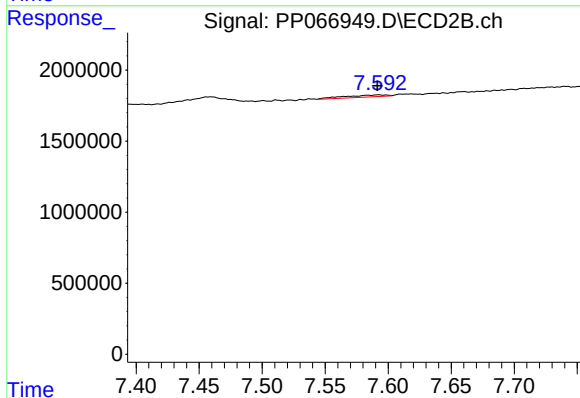


#35 AR-1260-5

R.T.: 7.592 min
Delta R.T.: 0.000 min
Response: 325646
Conc: 3.65 ng/ml

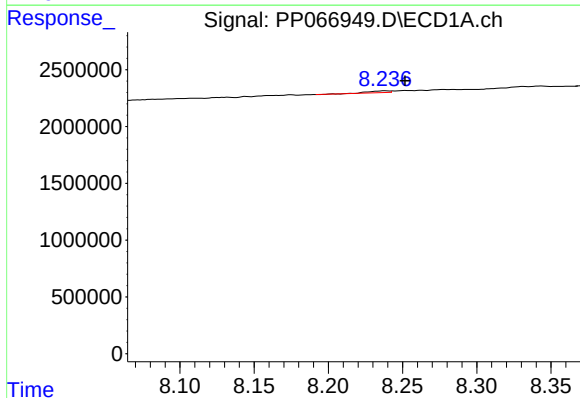


#36 AR-1262-1

R.T.: 8.238 min
Delta R.T.: -0.013 min
Response: 147991
Conc: 2.26 ng/ml

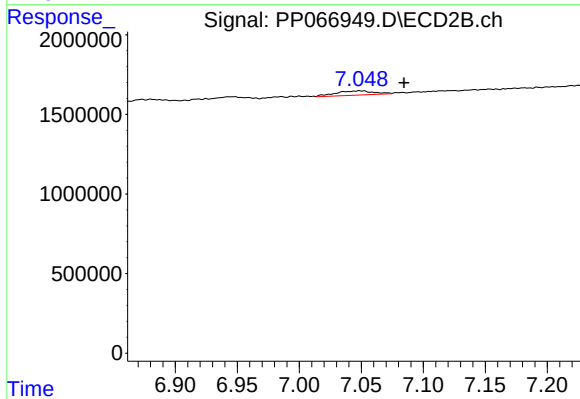

#36 AR-1262-1


R.T.: 7.049 min
Delta R.T.: -0.036 min
Response: 577164
Conc: 7.99 ng/ml

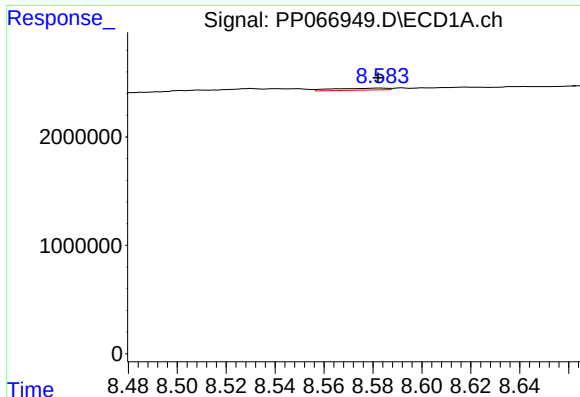

#37 AR-1262-2


R.T.: 8.583 min
Delta R.T.: 0.001 min
Response: 274807
Conc: 2.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

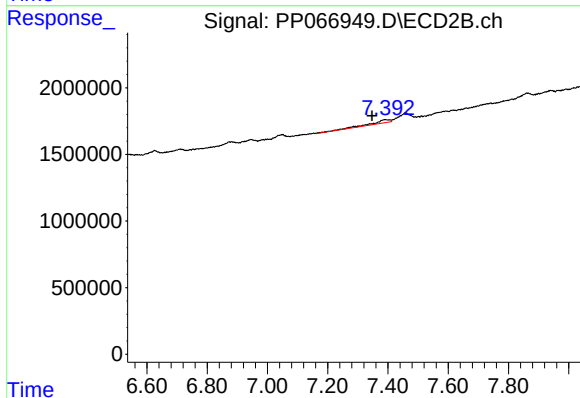


#37 AR-1262-2

R.T.: 7.392 min
Delta R.T.: 0.044 min
Response: 1102482
Conc: 17.92 ng/ml

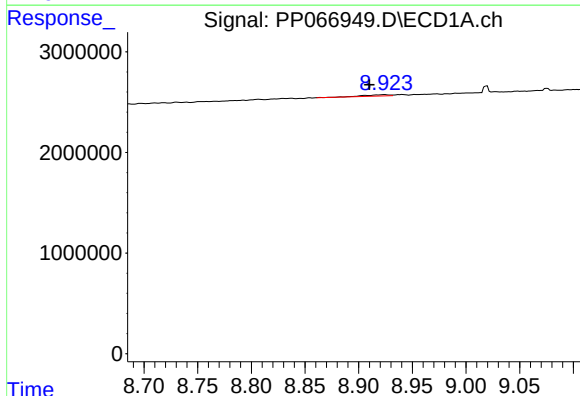


#38 AR-1262-3

R.T.: 8.924 min
Delta R.T.: 0.014 min
Response: 197110
Conc: 2.76 ng/ml

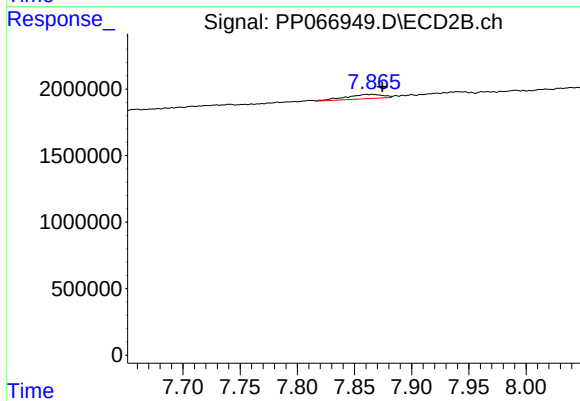

#38 AR-1262-3


R.T.: 7.865 min
Delta R.T.: -0.009 min
Response: 728318
Conc: 17.31 ng/ml

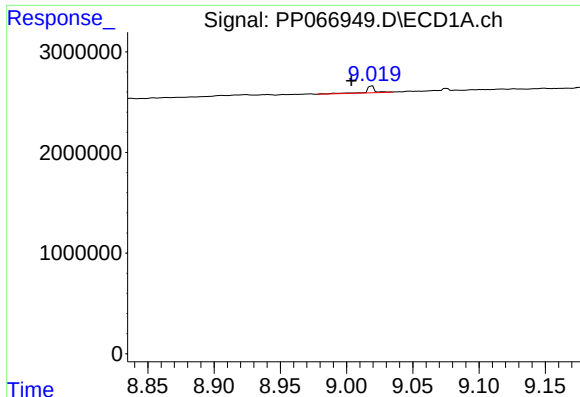

#39 AR-1262-4


R.T.: 9.019 min
Delta R.T.: 0.015 min
Response: 314103
Conc: 5.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

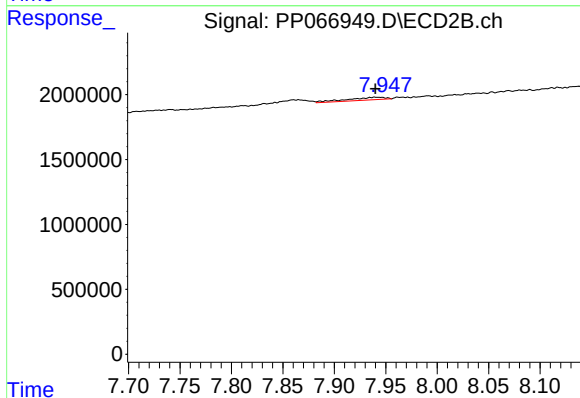


#39 AR-1262-4

R.T.: 7.940 min
Delta R.T.: 0.000 min
Response: 538014
Conc: 6.94 ng/ml

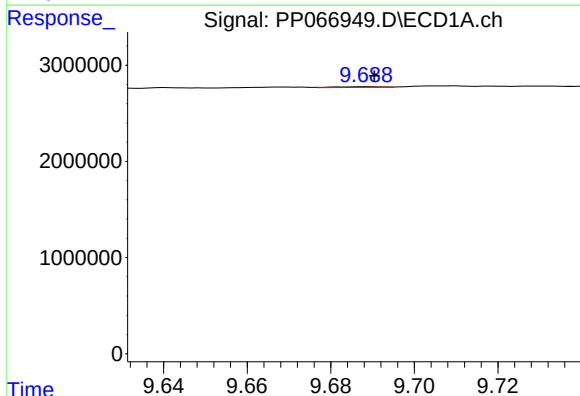


#40 AR-1262-5

R.T.: 9.688 min
Delta R.T.: -0.002 min
Response: 58676
Conc: 2.13 ng/ml

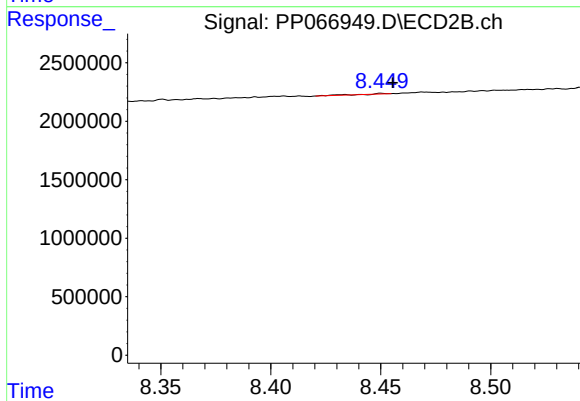

#40 AR-1262-5


R.T.: 8.451 min
Delta R.T.: -0.005 min
Response: 37540
Conc: 1.42 ng/ml

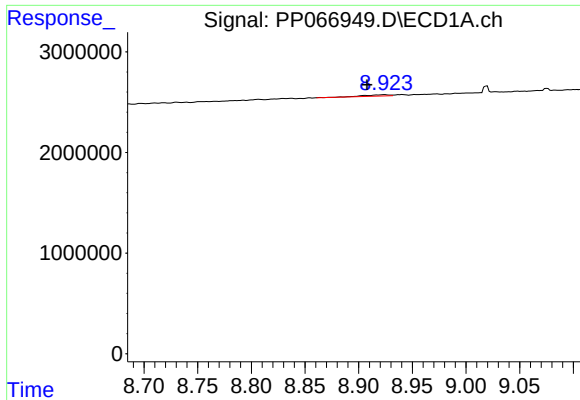

#41 AR-1268-1


R.T.: 8.924 min
Delta R.T.: 0.016 min
Response: 197110
Conc: 1.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

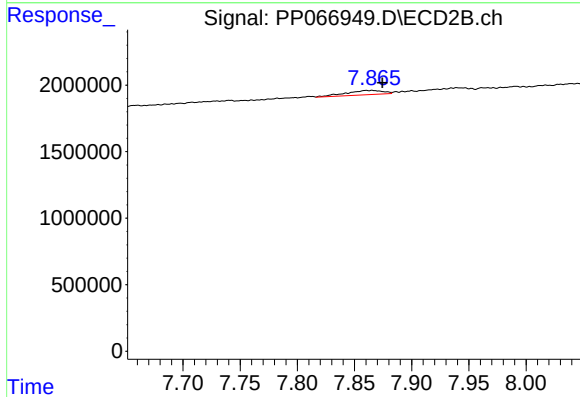


#41 AR-1268-1

R.T.: 7.865 min
Delta R.T.: -0.009 min
Response: 728318
Conc: 5.82 ng/ml

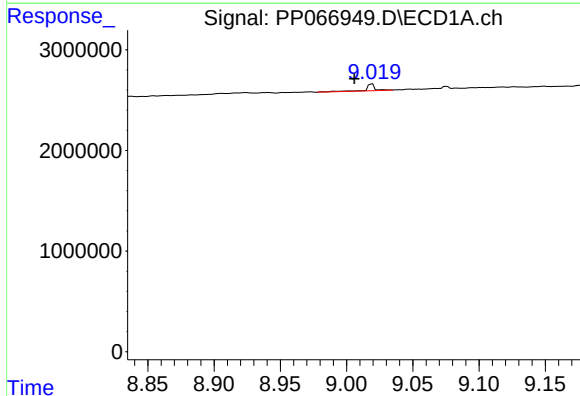


#42 AR-1268-2

R.T.: 9.019 min
Delta R.T.: 0.013 min
Response: 314103
Conc: 2.68 ng/ml

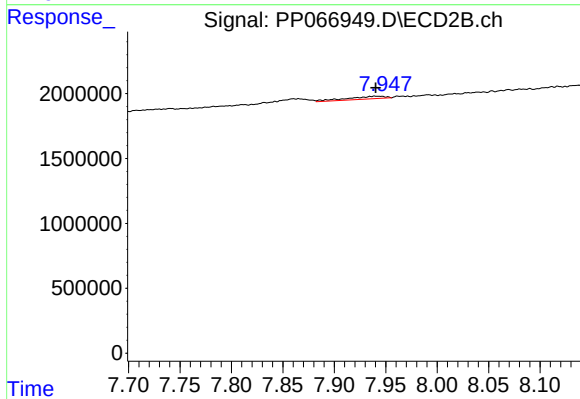

#42 AR-1268-2


R.T.: 7.940 min
Delta R.T.: 0.000 min
Response: 538014
Conc: 4.81 ng/ml

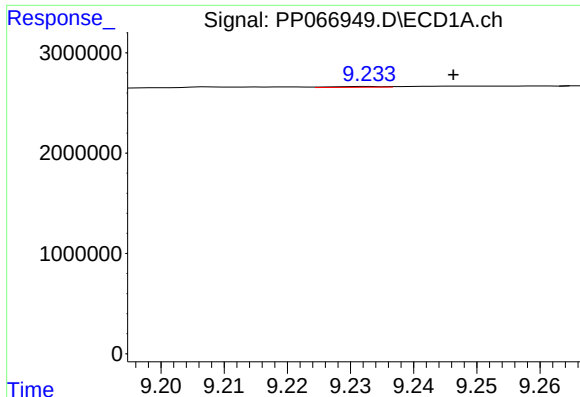

#43 AR-1268-3


R.T.: 9.233 min
Delta R.T.: -0.013 min
Response: 45997
Conc: 0.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

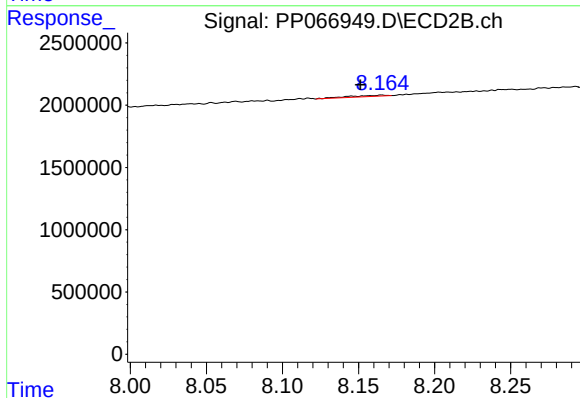


#43 AR-1268-3

R.T.: 8.165 min
Delta R.T.: 0.014 min
Response: 162246
Conc: 1.59 ng/ml

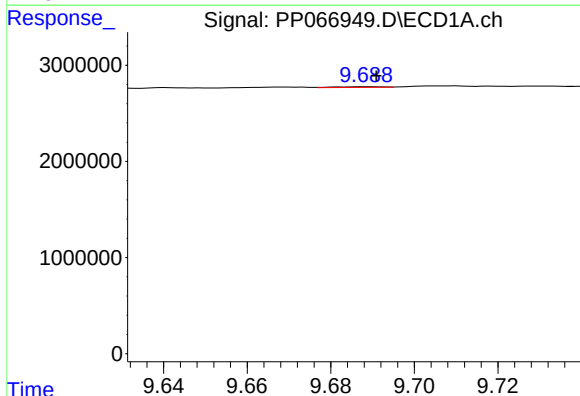


#44 AR-1268-4

R.T.: 9.688 min
Delta R.T.: -0.002 min
Response: 58676
Conc: 1.96 ng/ml

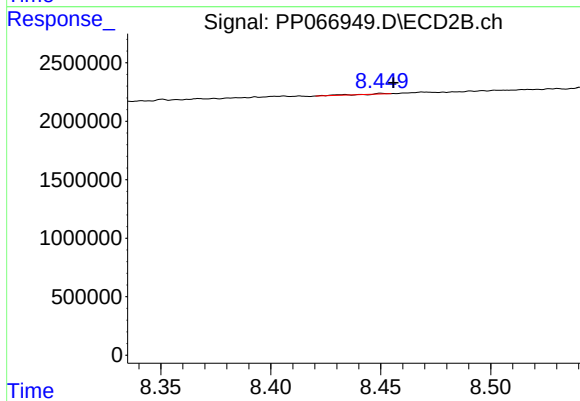

#44 AR-1268-4


R.T.: 8.451 min
Delta R.T.: -0.005 min
Response: 37540
Conc: 1.32 ng/ml

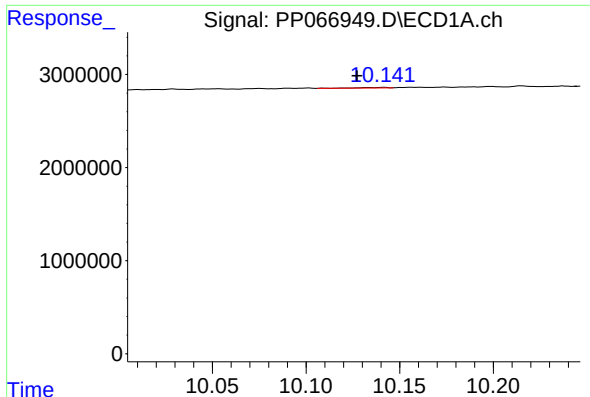

#45 AR-1268-5

R.T.: 10.142 min
Delta R.T.: 0.014 min
Response: 57200
Conc: 0.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

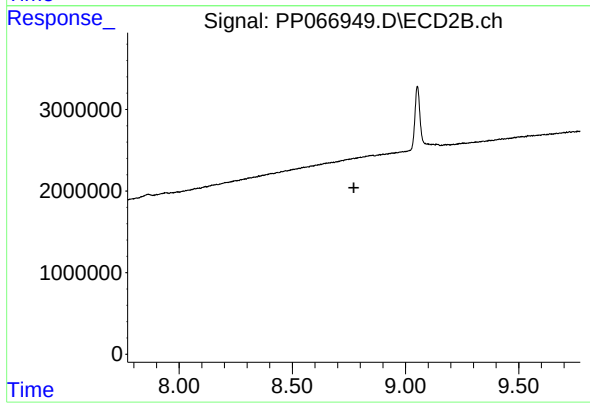

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.772 min
Response: 0
Conc: N.D.