

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
 Data File : PP066951.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2024 15:06
 Operator : YP\AJ
 Sample : P3390-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 04:38:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 09:05:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.625	3.913	33691172	27782370	20.016	19.382
2)	SA Decachlor...	10.489	9.053	14357852	13459310	17.123	17.970
Target Compounds							
3)	L1 AR-1016-1	5.774	5.071f	43423	103968	0.918	2.382 #
4)	L1 AR-1016-2	5.836	5.071	105867	103968	1.431	1.616
5)	L1 AR-1016-3	5.882	5.262f	13686	939494	0.292	27.359 #
6)	L1 AR-1016-4	0.000	5.262	0	939494	N.D.	31.016 #
7)	L1 AR-1016-5	6.279	5.481	527249	436873	15.391	12.102
9)	L2 AR-1221-2	4.934	4.223	418596	369920	31.093	31.615
10)	L2 AR-1221-3	4.934f	0.000	418596	0	10.358	N.D. #
11)	L3 AR-1232-1	4.934f	0.000	418596	0	12.556	N.D. #
12)	L3 AR-1232-2	5.534	5.071	103622	103968	5.870	3.526 #
13)	L3 AR-1232-3	5.836	5.262f	105867	939494	3.391	66.151 #
14)	L3 AR-1232-4	0.000	5.305	0	278797	N.D.	19.835 #
15)	L3 AR-1232-5	6.072	5.481	888972	436873	70.650	30.713 #
16)	L4 AR-1242-1	5.774	5.071f	43423	103968	1.262	3.347 #
17)	L4 AR-1242-2	5.836	5.071	105867	103968	1.993	2.329
18)	L4 AR-1242-3	5.882	5.262f	13686	939494	0.399	38.946 #
19)	L4 AR-1242-4	0.000	5.305	0	278797	N.D.	10.418 #
20)	L4 AR-1242-5	6.724	5.838	432313	1923640	18.605	68.922 #
21)	L5 AR-1248-1	5.774	5.071f	43423	103968	1.799	4.724 #
22)	L5 AR-1248-2	6.072	5.262	888972	939494	22.826	26.741
23)	L5 AR-1248-3	6.279	5.305	527249	278797	12.944	7.662 #
24)	L5 AR-1248-4	6.681	5.481	576812	436873	14.887	10.751 #
25)	L5 AR-1248-5	6.724	5.878	432313	147195	10.979	4.608 #
26)	L6 AR-1254-1	6.656	5.838	1812190	1923640	36.420	32.416
27)	L6 AR-1254-2	6.871	5.987	2309980	1586510	32.702	30.278
28)	L6 AR-1254-3	7.241	6.397	2163739	2577568	31.757	33.788
29)	L6 AR-1254-4	7.526	6.626	1276634	1338225	30.488	35.426
30)	L6 AR-1254-5	7.944	7.050	2662463	2042372	50.670	32.451 #
31)	L7 AR-1260-1	7.404	6.528	560478	1467208	9.261	23.161 #
32)	L7 AR-1260-2	7.660	6.716	1040212	1003998	16.182	14.849
33)	L7 AR-1260-3	8.028	6.874	67540	1321637	1.513	19.843 #
34)	L7 AR-1260-4	8.240	7.341	510962	276785	10.198	6.315 #
35)	L7 AR-1260-5	8.588	7.585	537943	477534	6.437	5.354
36)	L8 AR-1262-1	8.240	7.050	510962	2042372	7.813	28.270 #
37)	L8 AR-1262-2	8.588	7.341	537943	276785	5.201	4.498
38)	L8 AR-1262-3	8.920	7.864	402010	976746	5.629	23.220 #
39)	L8 AR-1262-4	9.029	7.944	205456	435824	3.480	5.618 #
40)	L8 AR-1262-5	9.685	0.000	174276	0	6.334	N.D. #
41)	L9 AR-1268-1	8.920	7.864	402010	976746	3.076	7.809 #
42)	L9 AR-1268-2	9.029	7.944	205456	435824	1.756	3.899 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
Data File : PP066951.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2024 15:06
Operator : YP\AJ
Sample : P3390-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 04:38:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 09:05:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43)	L9 AR-1268-3	9.235	8.159	63138	167995	0.607	1.643 #
44)	L9 AR-1268-4	9.685	0.000	174276	0	5.822	N.D. #
45)	L9 AR-1268-5	10.123	8.764	81796	41239	0.292	0.168 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
Data File : PP066951.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2024 15:06
Operator : YP\AJ
Sample : P3390-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 04:38:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 09:05:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

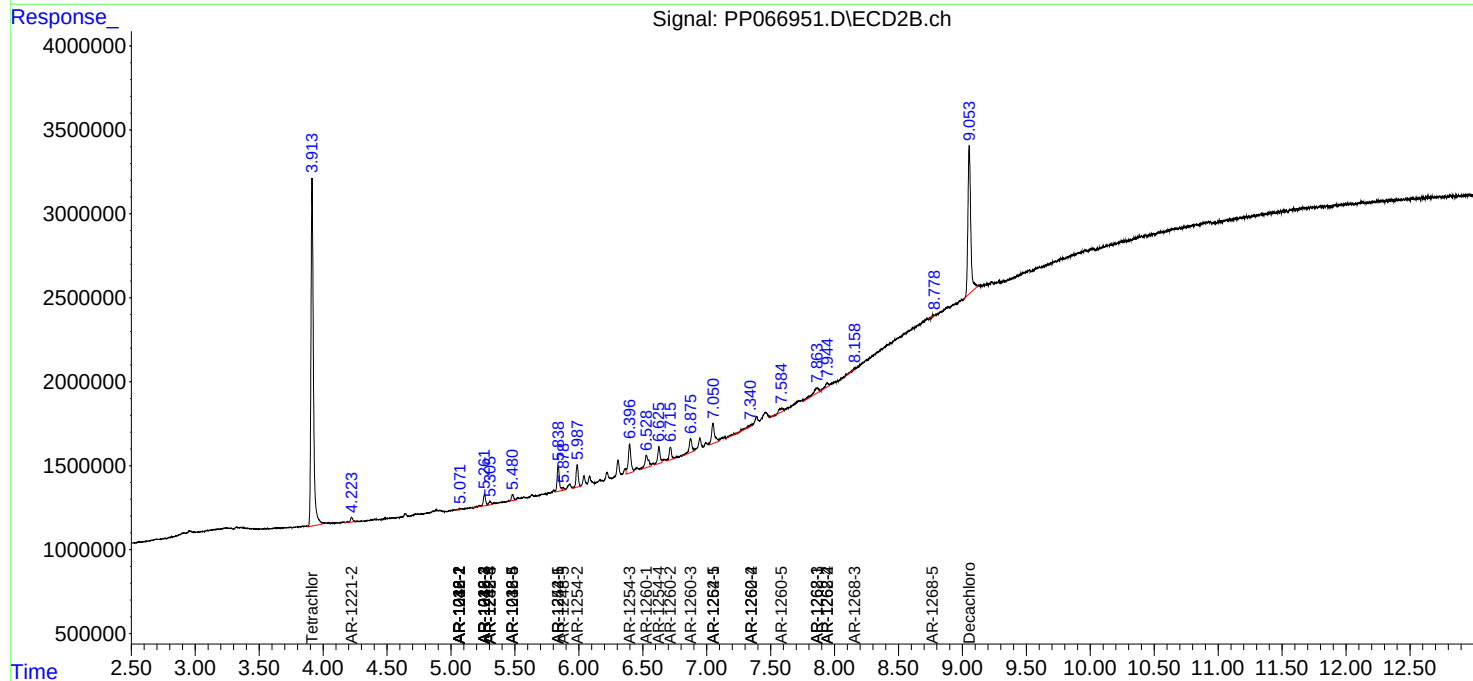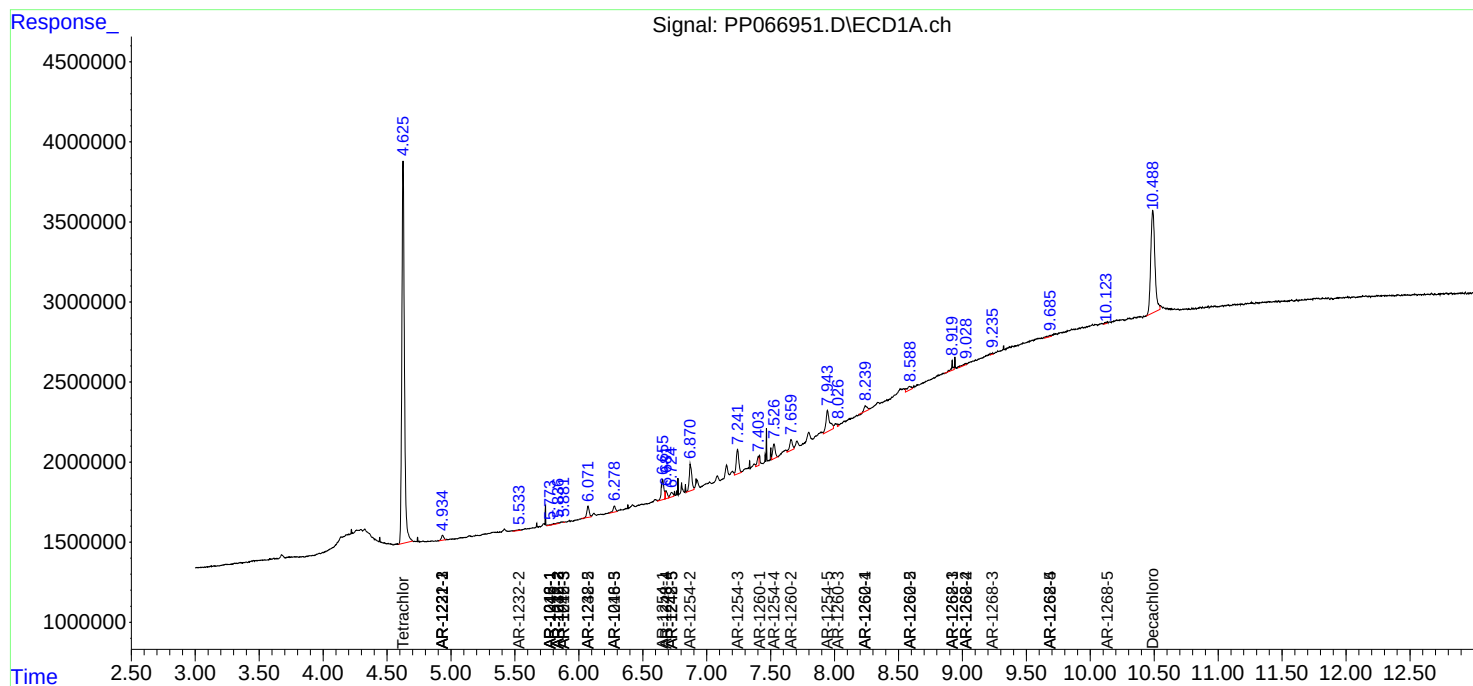


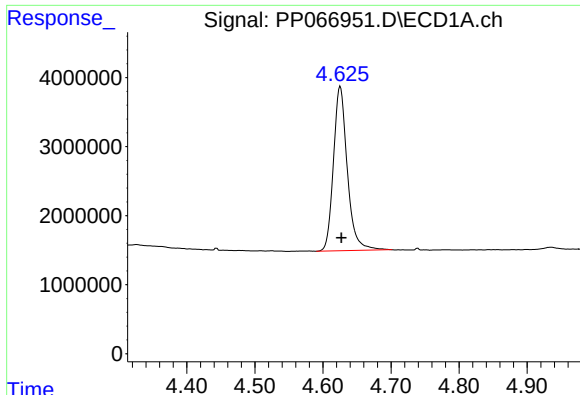

#1 Tetrachloro-m-xylene


R.T.: 4.625 min
Delta R.T.: -0.002 min
Response: 33691172
Conc: 20.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

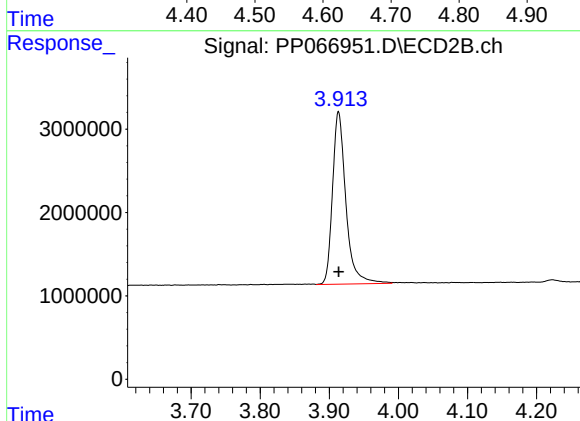


#1 Tetrachloro-m-xylene

R.T.: 3.913 min
Delta R.T.: 0.000 min
Response: 27782370
Conc: 19.38 ng/ml

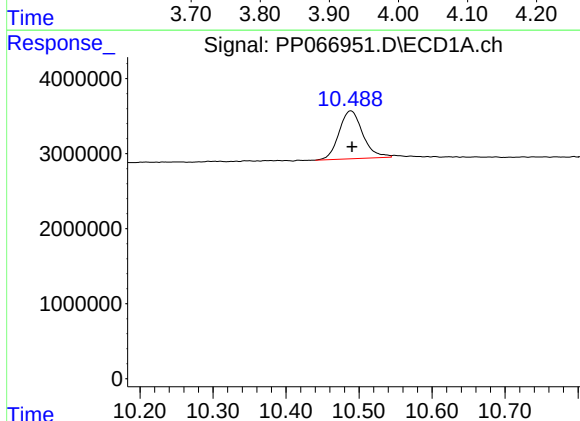


#2 Decachlorobiphenyl

R.T.: 10.489 min
Delta R.T.: -0.001 min
Response: 14357852
Conc: 17.12 ng/ml

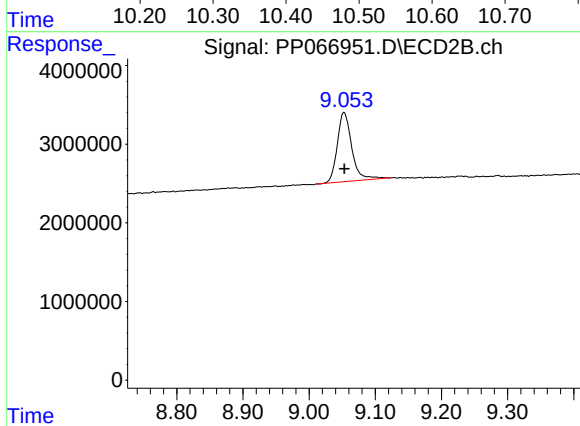

#2 Decachlorobiphenyl


R.T.: 9.053 min
Delta R.T.: 0.000 min
Response: 13459310
Conc: 17.97 ng/ml

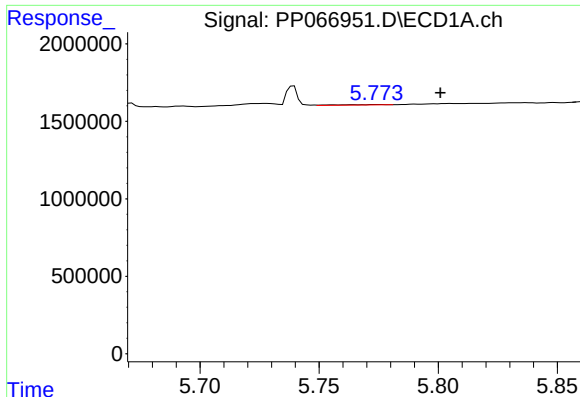

#3 AR-1016-1


R.T.: 5.774 min
Delta R.T.: -0.026 min
Response: 43423
Conc: 0.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

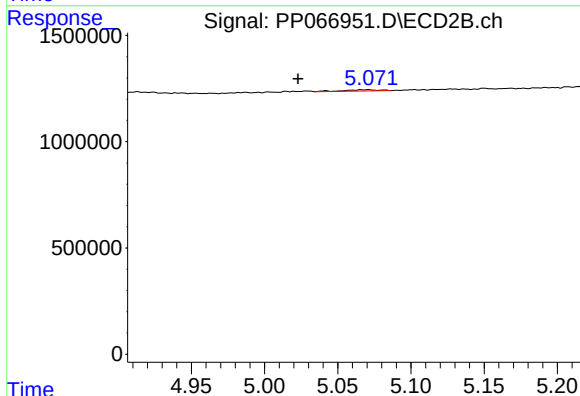


#3 AR-1016-1

R.T.: 5.071 min
Delta R.T.: 0.048 min
Response: 103968
Conc: 2.38 ng/ml

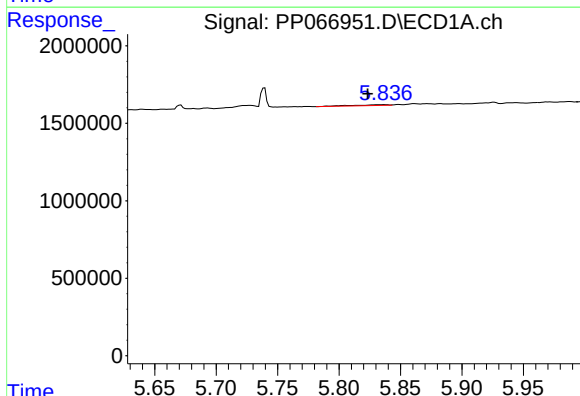


#4 AR-1016-2

R.T.: 5.836 min
Delta R.T.: 0.013 min
Response: 105867
Conc: 1.43 ng/ml

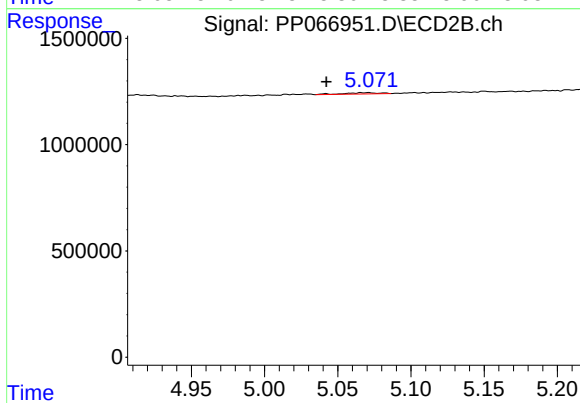

#4 AR-1016-2


R.T.: 5.071 min
Delta R.T.: 0.029 min
Response: 103968
Conc: 1.62 ng/ml

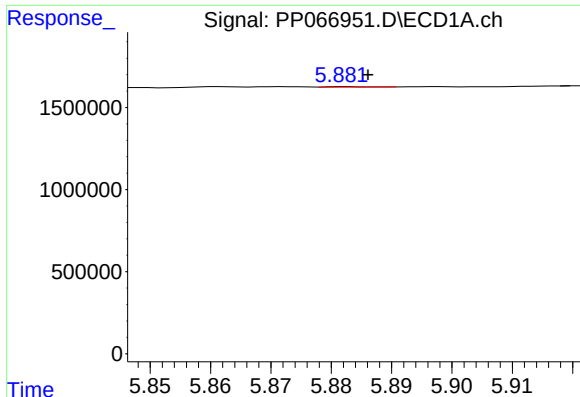

#5 AR-1016-3


R.T.: 5.882 min
Delta R.T.: -0.004 min
Response: 13686
Conc: 0.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

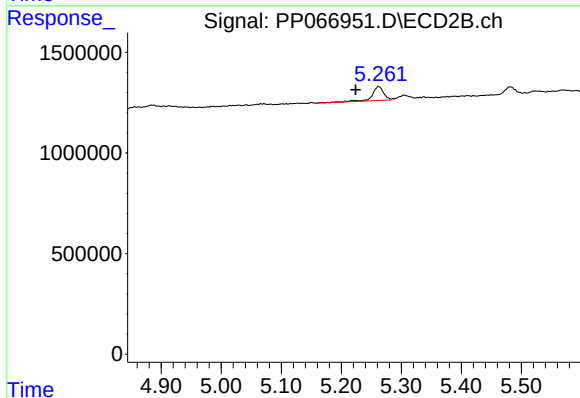


#5 AR-1016-3

R.T.: 5.262 min
Delta R.T.: 0.038 min
Response: 939494
Conc: 27.36 ng/ml

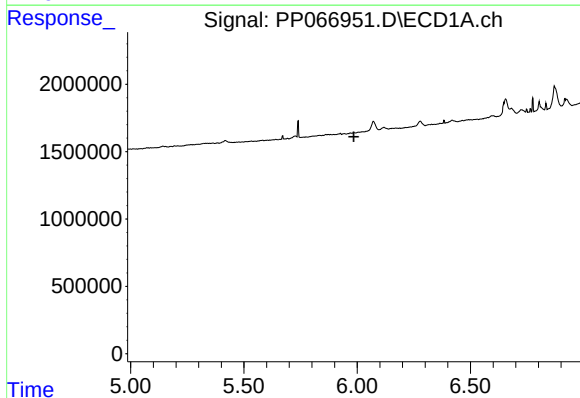


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.985 min
Response: 0
Conc: N.D.

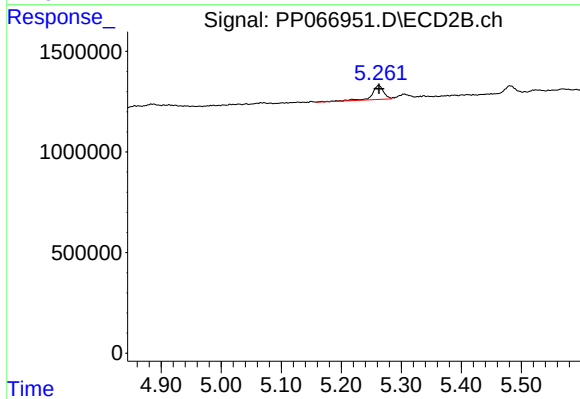

#6 AR-1016-4


R.T.: 5.262 min
Delta R.T.: 0.000 min
Response: 939494
Conc: 31.02 ng/ml

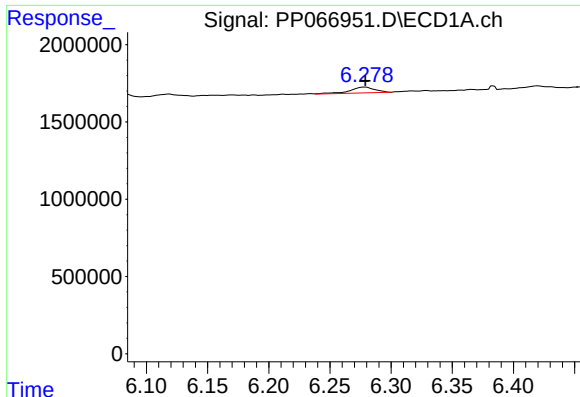

#7 AR-1016-5


R.T.: 6.279 min
Delta R.T.: 0.000 min
Response: 527249
Conc: 15.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

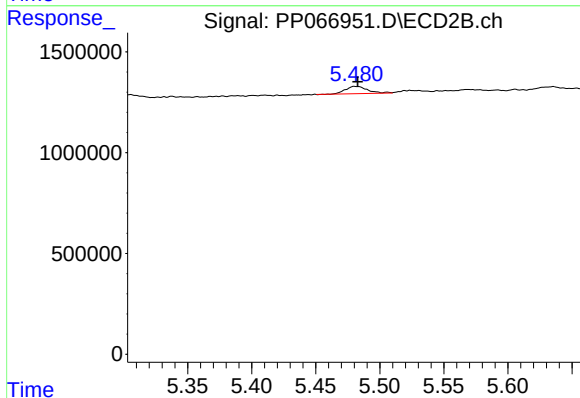


#7 AR-1016-5

R.T.: 5.481 min
Delta R.T.: -0.002 min
Response: 436873
Conc: 12.10 ng/ml

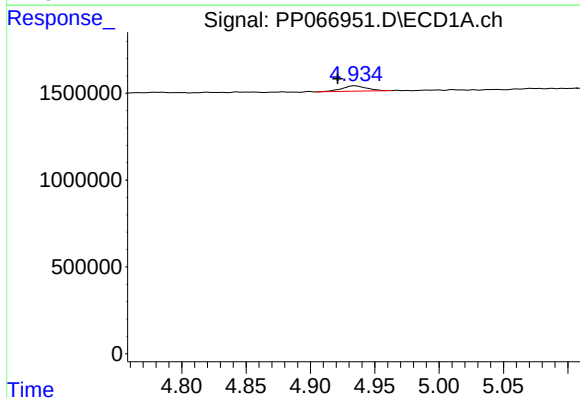


#9 AR-1221-2

R.T.: 4.934 min
Delta R.T.: 0.013 min
Response: 418596
Conc: 31.09 ng/ml

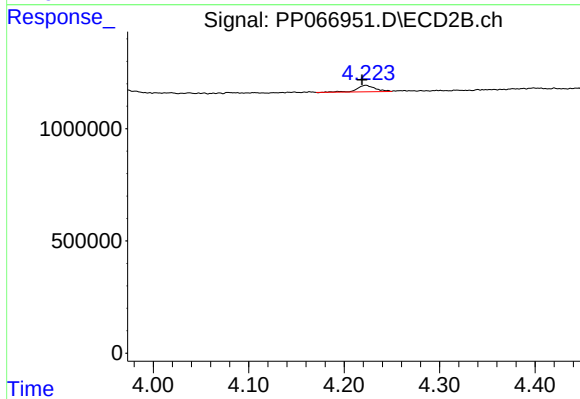

#9 AR-1221-2


R.T.: 4.223 min
Delta R.T.: 0.004 min
Response: 369920
Conc: 31.62 ng/ml

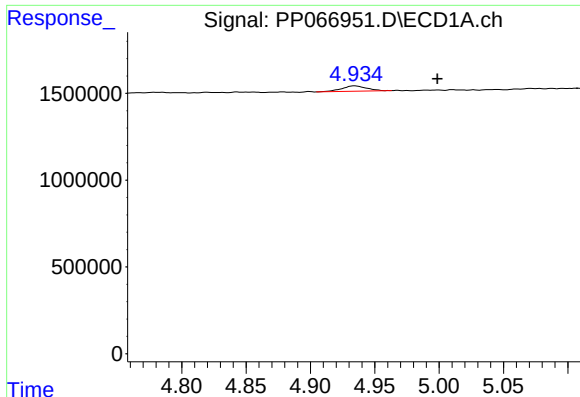

#10 AR-1221-3


R.T.: 4.934 min
Delta R.T.: -0.064 min
Response: 418596
Conc: 10.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

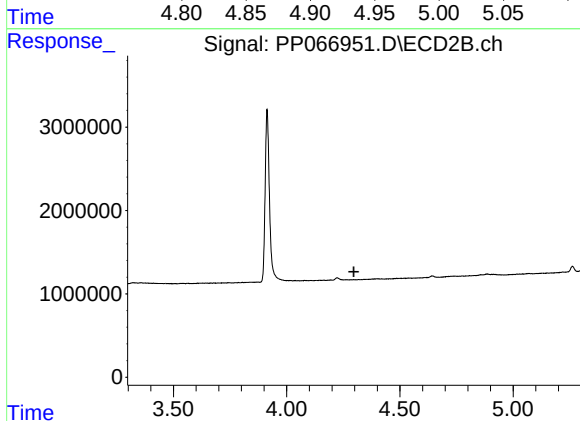


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.297 min
Response: 0
Conc: N.D.

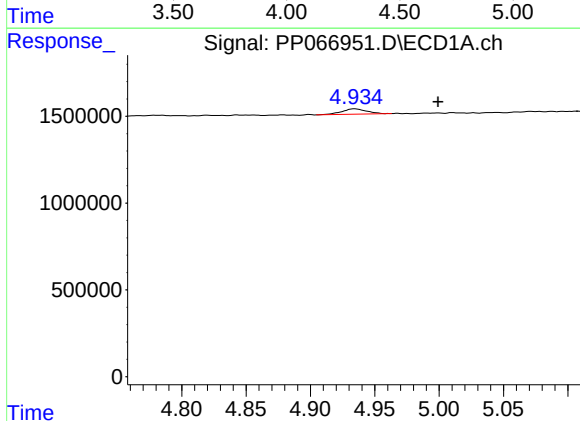


#11 AR-1232-1

R.T.: 4.934 min
Delta R.T.: -0.065 min
Response: 418596
Conc: 12.56 ng/ml

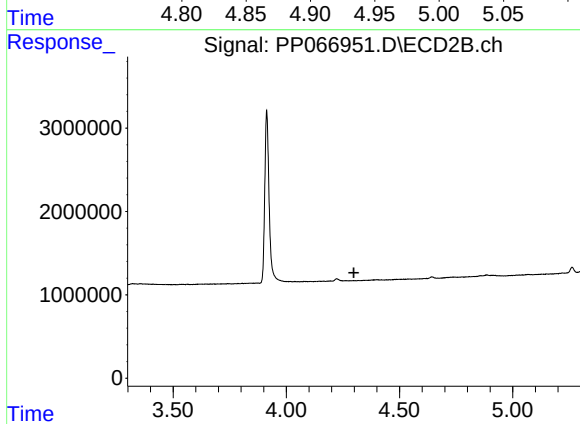

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.298 min
Response: 0
Conc: N.D.

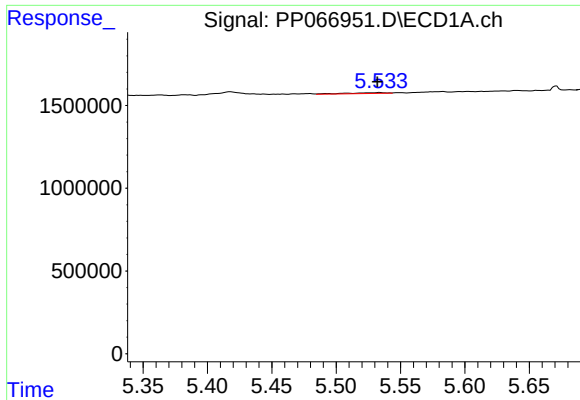

#12 AR-1232-2


R.T.: 5.534 min
Delta R.T.: 0.002 min
Response: 103622
Conc: 5.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

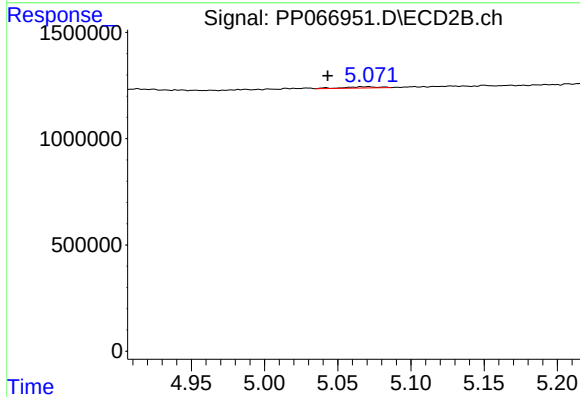


#12 AR-1232-2

R.T.: 5.071 min
Delta R.T.: 0.028 min
Response: 103968
Conc: 3.53 ng/ml

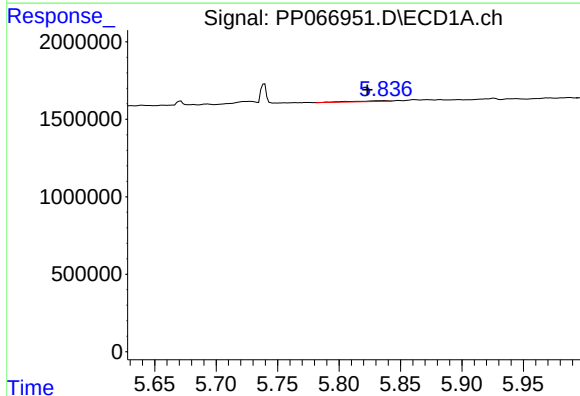


#13 AR-1232-3

R.T.: 5.836 min
Delta R.T.: 0.013 min
Response: 105867
Conc: 3.39 ng/ml

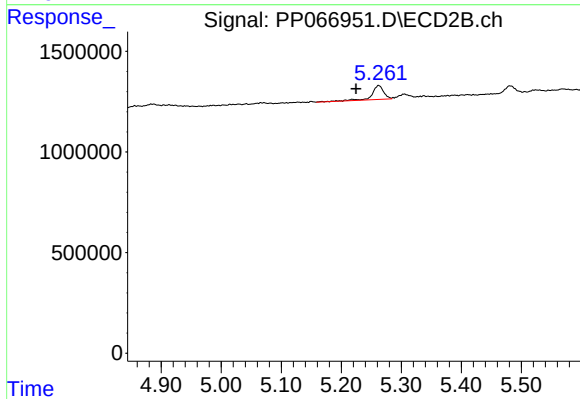

#13 AR-1232-3


R.T.: 5.262 min
Delta R.T.: 0.038 min
Response: 939494
Conc: 66.15 ng/ml

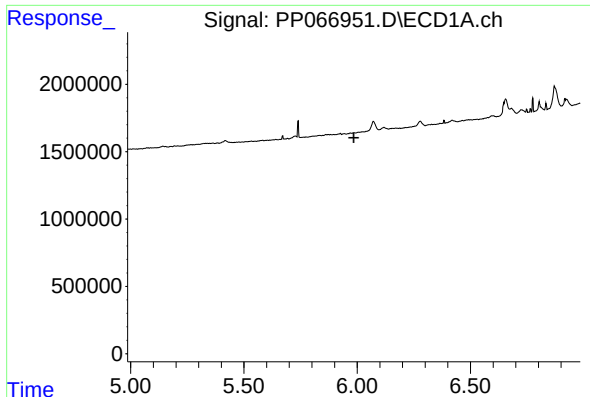

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T.: 5.985 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

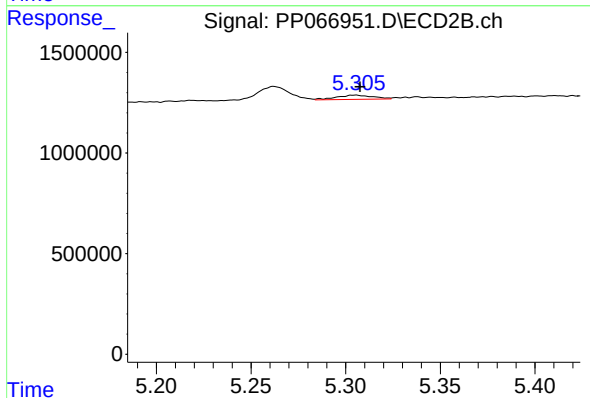


#14 AR-1232-4

R.T.: 5.305 min
Delta R.T.: -0.003 min
Response: 278797
Conc: 19.83 ng/ml

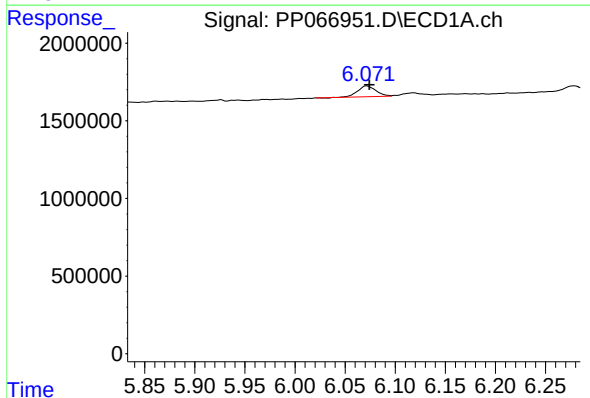


#15 AR-1232-5

R.T.: 6.072 min
Delta R.T.: -0.002 min
Response: 888972
Conc: 70.65 ng/ml

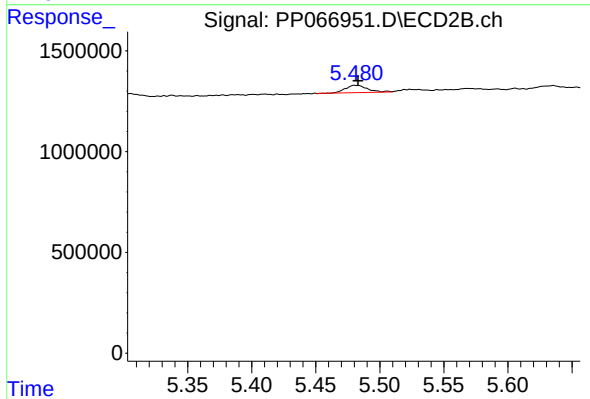

#15 AR-1232-5


R.T.: 5.481 min
Delta R.T.: -0.002 min
Response: 436873
Conc: 30.71 ng/ml

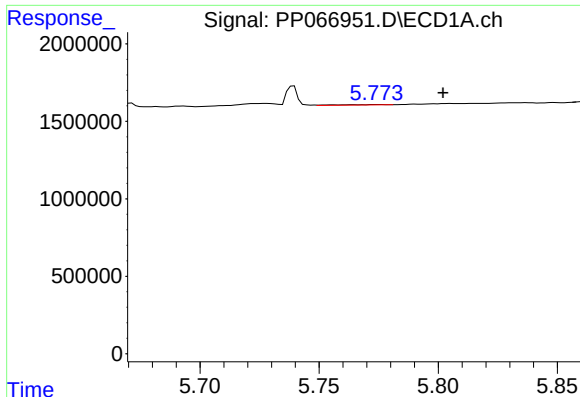

#16 AR-1242-1


R.T.: 5.774 min
Delta R.T.: -0.028 min
Response: 43423
Conc: 1.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

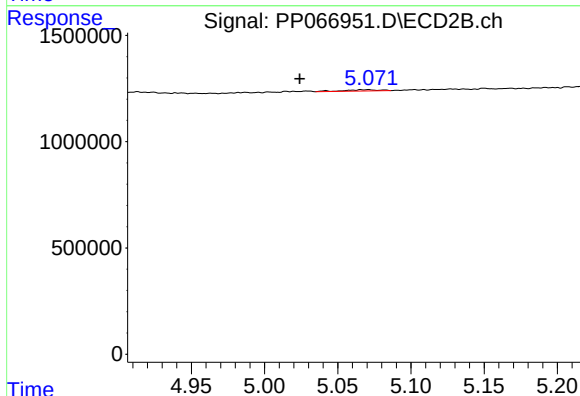


#16 AR-1242-1

R.T.: 5.071 min
Delta R.T.: 0.047 min
Response: 103968
Conc: 3.35 ng/ml

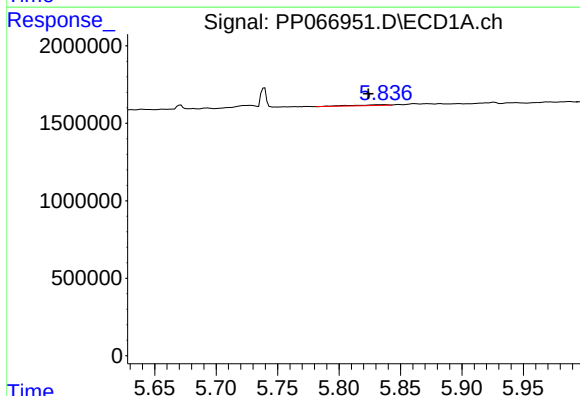


#17 AR-1242-2

R.T.: 5.836 min
Delta R.T.: 0.012 min
Response: 105867
Conc: 1.99 ng/ml

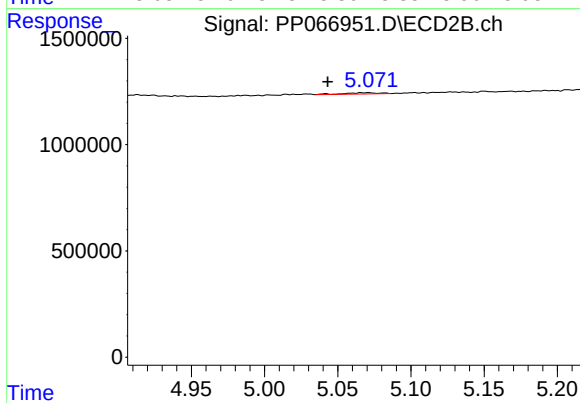

#17 AR-1242-2


R.T.: 5.071 min
Delta R.T.: 0.028 min
Response: 103968
Conc: 2.33 ng/ml

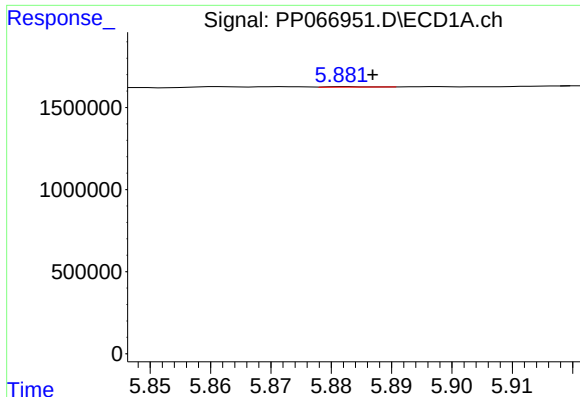

#18 AR-1242-3


R.T.: 5.882 min
Delta R.T.: -0.005 min
Response: 13686
Conc: 0.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

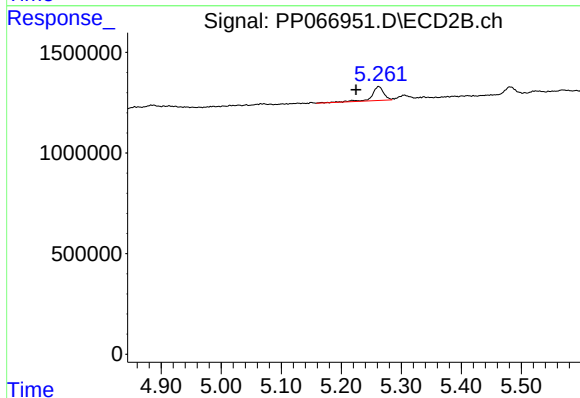


#18 AR-1242-3

R.T.: 5.262 min
Delta R.T.: 0.038 min
Response: 939494
Conc: 38.95 ng/ml

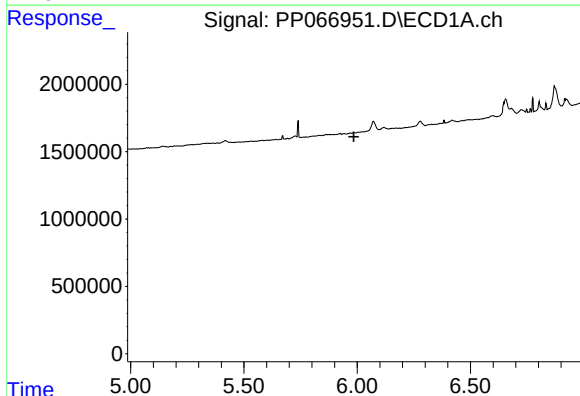


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.986 min
Response: 0
Conc: N.D.

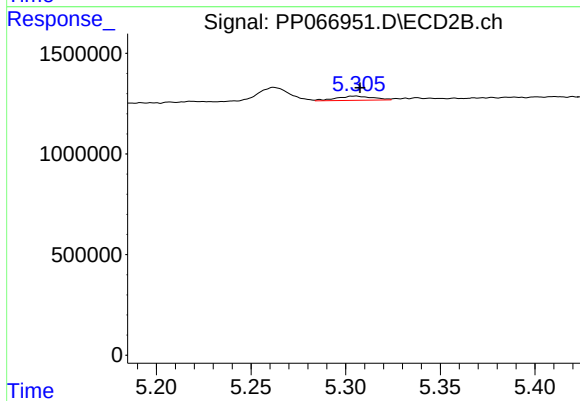

#19 AR-1242-4


R.T.: 5.305 min
Delta R.T.: -0.003 min
Response: 278797
Conc: 10.42 ng/ml

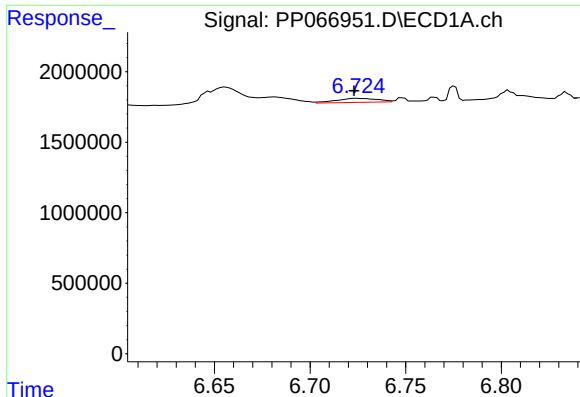

#20 AR-1242-5


R.T.: 6.724 min
Delta R.T.: 0.001 min
Response: 432313
Conc: 18.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

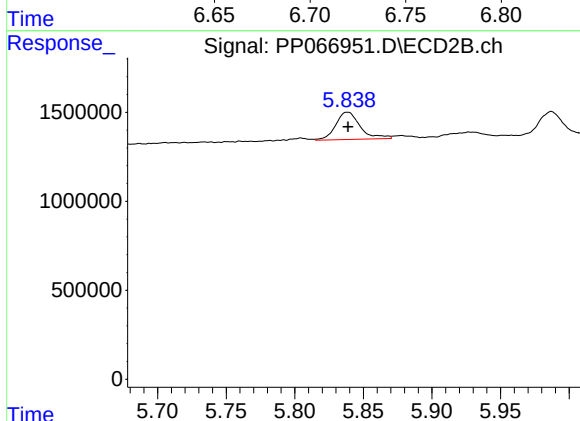


#20 AR-1242-5

R.T.: 5.838 min
Delta R.T.: 0.000 min
Response: 1923640
Conc: 68.92 ng/ml

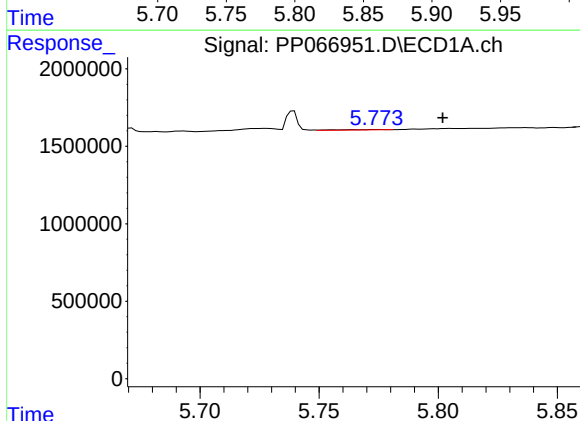


#21 AR-1248-1

R.T.: 5.774 min
Delta R.T.: -0.027 min
Response: 43423
Conc: 1.80 ng/ml

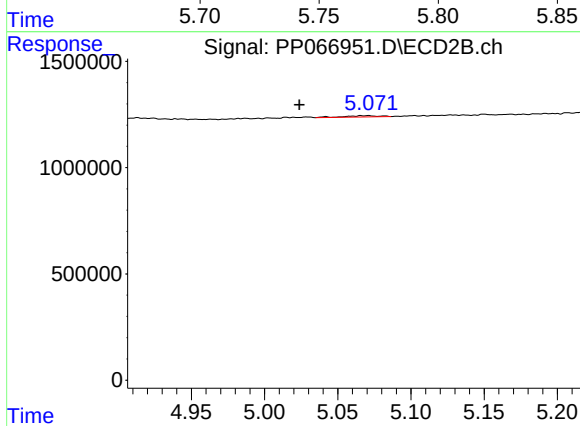

#21 AR-1248-1


R.T.: 5.071 min
Delta R.T.: 0.047 min
Response: 103968
Conc: 4.72 ng/ml

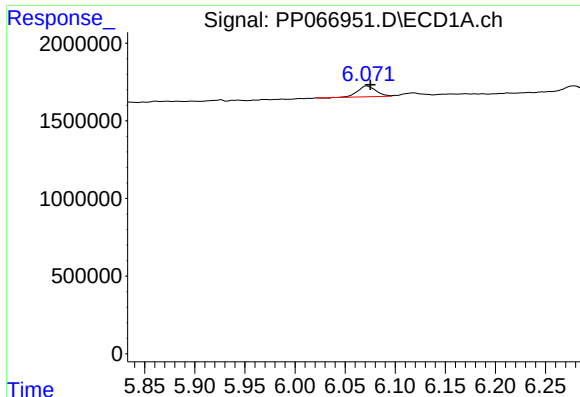

#22 AR-1248-2


R.T.: 6.072 min
Delta R.T.: -0.004 min
Response: 888972
Conc: 22.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

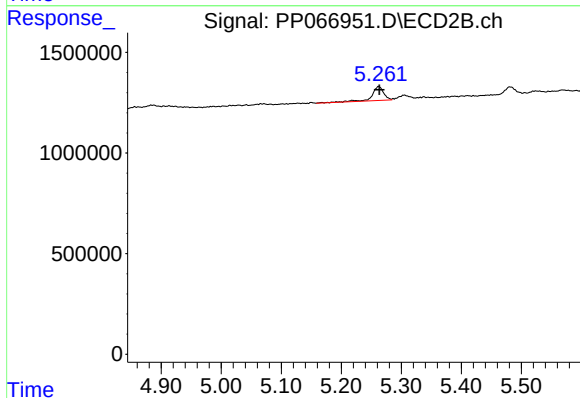


#22 AR-1248-2

R.T.: 5.262 min
Delta R.T.: -0.001 min
Response: 939494
Conc: 26.74 ng/ml

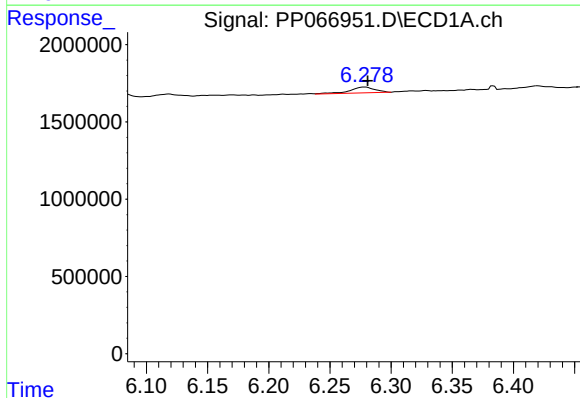


#23 AR-1248-3

R.T.: 6.279 min
Delta R.T.: -0.002 min
Response: 527249
Conc: 12.94 ng/ml

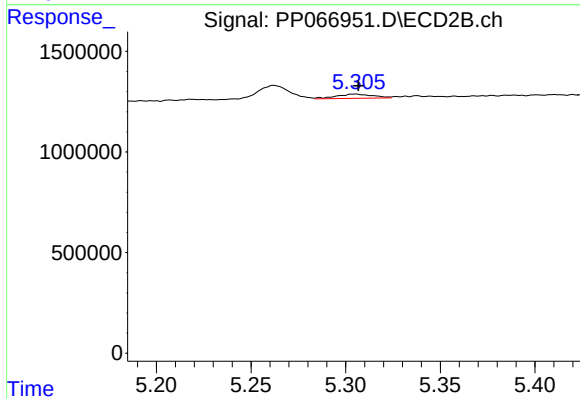

#23 AR-1248-3


R.T.: 5.305 min
Delta R.T.: -0.002 min
Response: 278797
Conc: 7.66 ng/ml

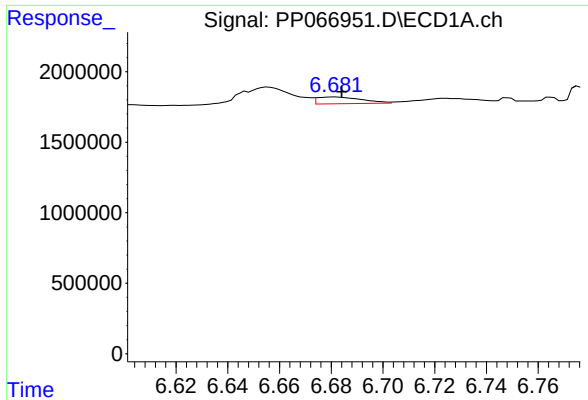

#24 AR-1248-4


R.T.: 6.681 min
Delta R.T.: -0.003 min
Response: 576812
Conc: 14.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

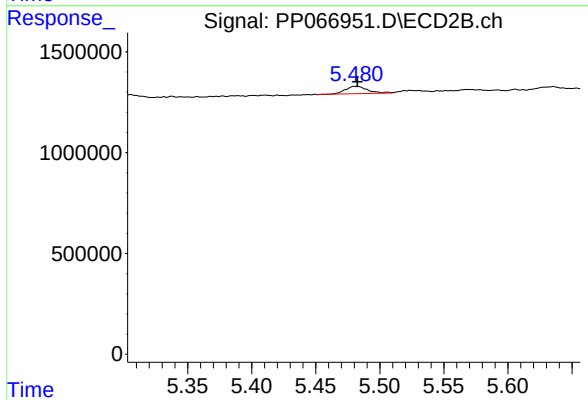


#24 AR-1248-4

R.T.: 5.481 min
Delta R.T.: -0.002 min
Response: 436873
Conc: 10.75 ng/ml

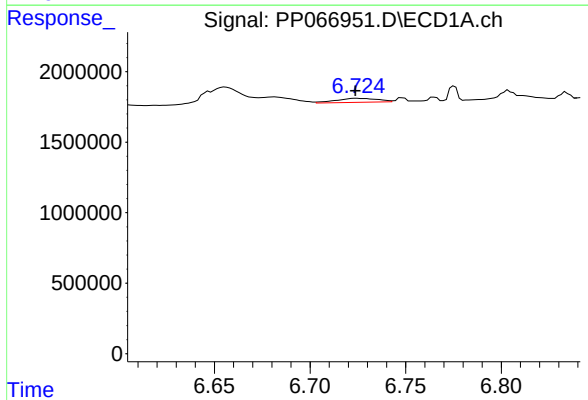


#25 AR-1248-5

R.T.: 6.724 min
Delta R.T.: 0.000 min
Response: 432313
Conc: 10.98 ng/ml

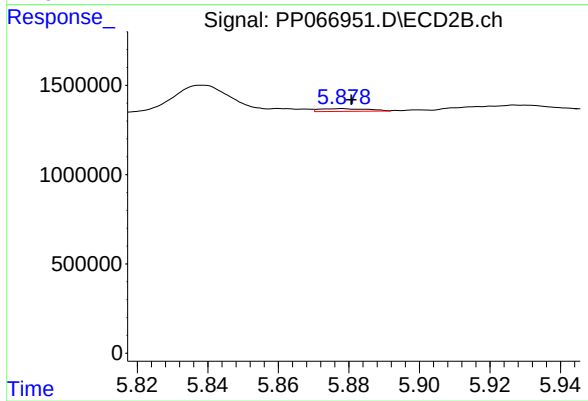

#25 AR-1248-5


R.T.: 5.878 min
Delta R.T.: -0.003 min
Response: 147195
Conc: 4.61 ng/ml

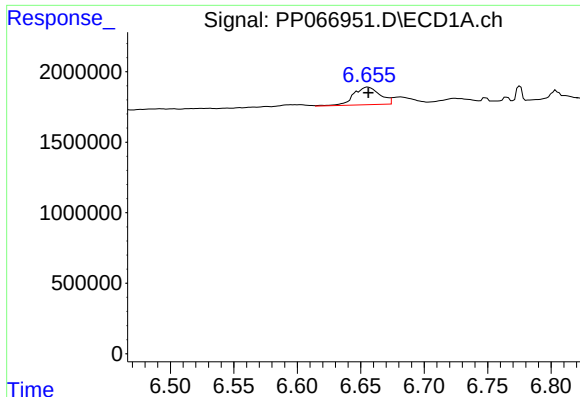

#26 AR-1254-1


R.T.: 6.656 min
Delta R.T.: 0.000 min
Response: 1812190
Conc: 36.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

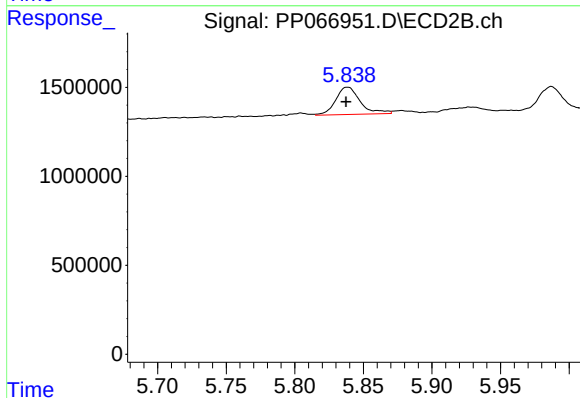


#26 AR-1254-1

R.T.: 5.838 min
Delta R.T.: 0.001 min
Response: 1923640
Conc: 32.42 ng/ml

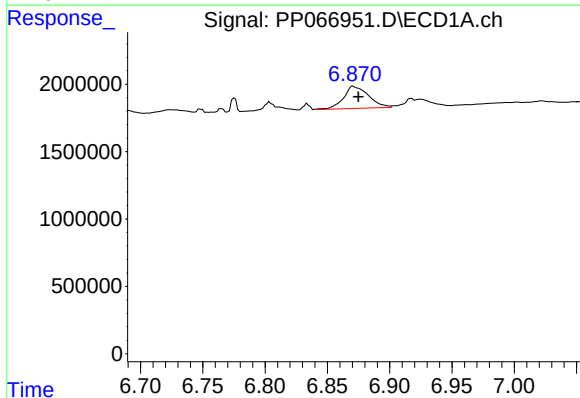


#27 AR-1254-2

R.T.: 6.871 min
Delta R.T.: -0.004 min
Response: 2309980
Conc: 32.70 ng/ml

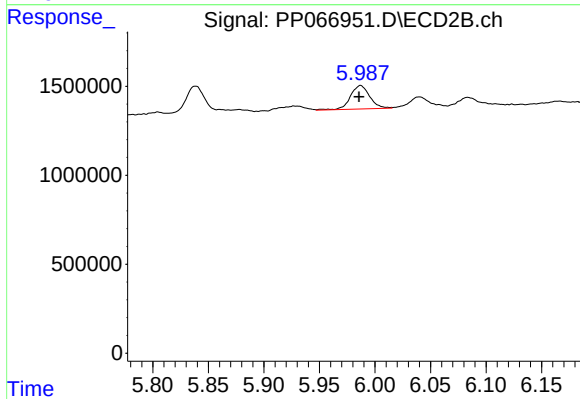

#27 AR-1254-2


R.T.: 5.987 min
Delta R.T.: 0.001 min
Response: 1586510
Conc: 30.28 ng/ml

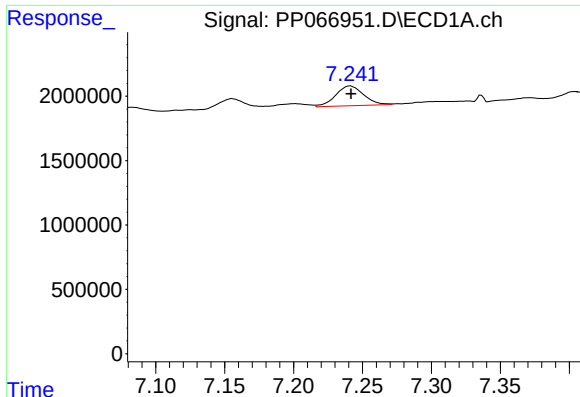

#28 AR-1254-3


R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 2163739
Conc: 31.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

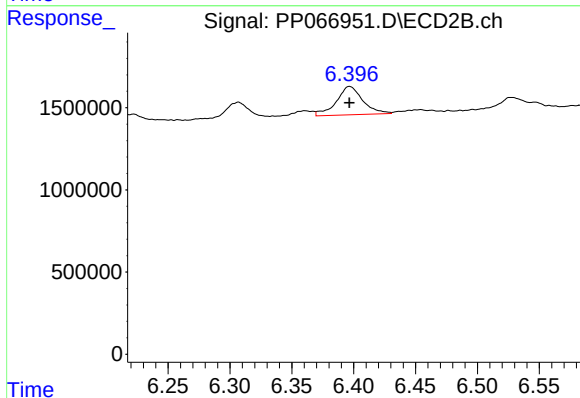


#28 AR-1254-3

R.T.: 6.397 min
Delta R.T.: 0.000 min
Response: 2577568
Conc: 33.79 ng/ml

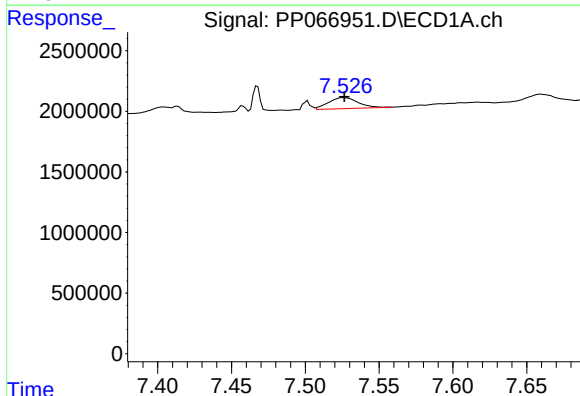


#29 AR-1254-4

R.T.: 7.526 min
Delta R.T.: 0.000 min
Response: 1276634
Conc: 30.49 ng/ml

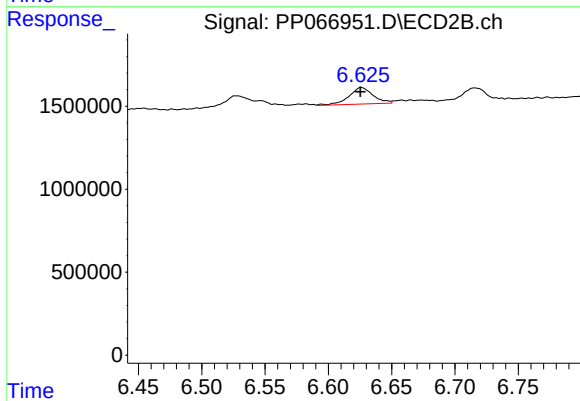

#29 AR-1254-4


R.T.: 6.626 min
Delta R.T.: 0.000 min
Response: 1338225
Conc: 35.43 ng/ml

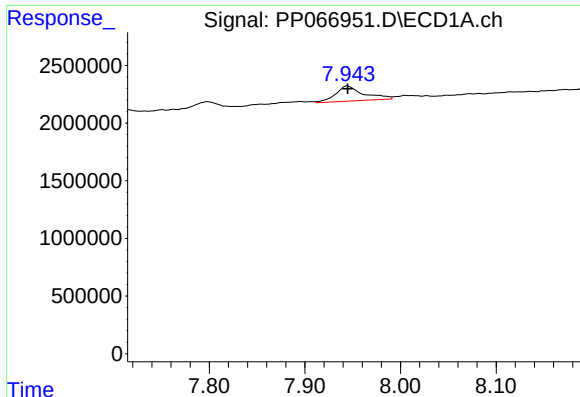

#30 AR-1254-5


R.T.: 7.944 min
Delta R.T.: 0.000 min
Response: 2662463
Conc: 50.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

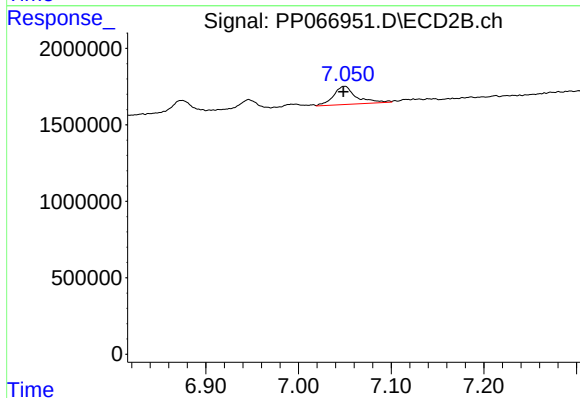


#30 AR-1254-5

R.T.: 7.050 min
Delta R.T.: 0.001 min
Response: 2042372
Conc: 32.45 ng/ml

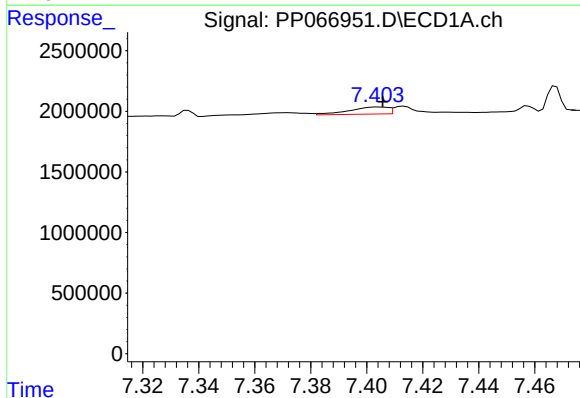


#31 AR-1260-1

R.T.: 7.404 min
Delta R.T.: -0.001 min
Response: 560478
Conc: 9.26 ng/ml

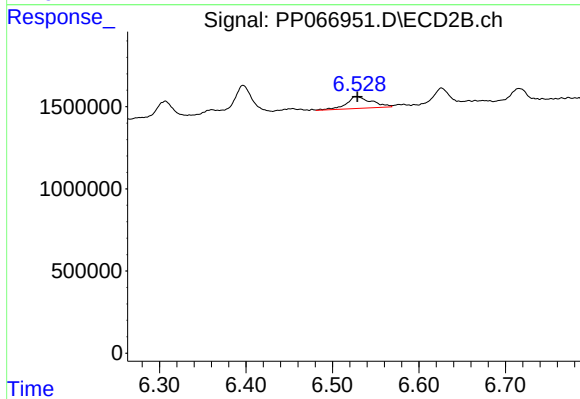

#31 AR-1260-1


R.T.: 6.528 min
Delta R.T.: -0.001 min
Response: 1467208
Conc: 23.16 ng/ml

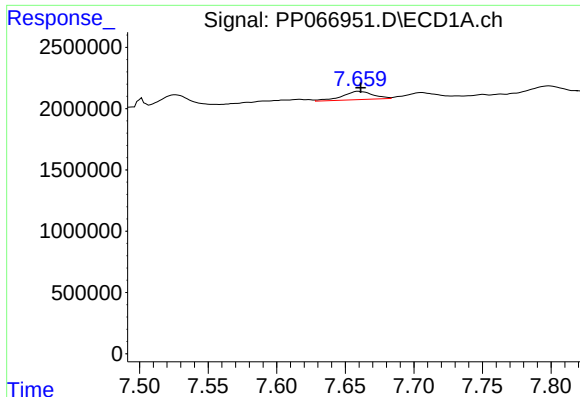

#32 AR-1260-2


R.T.: 7.660 min
Delta R.T.: -0.002 min
Response: 1040212
Conc: 16.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

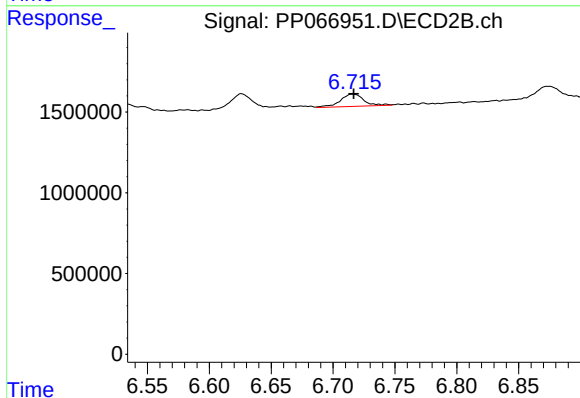


#32 AR-1260-2

R.T.: 6.716 min
Delta R.T.: -0.001 min
Response: 1003998
Conc: 14.85 ng/ml

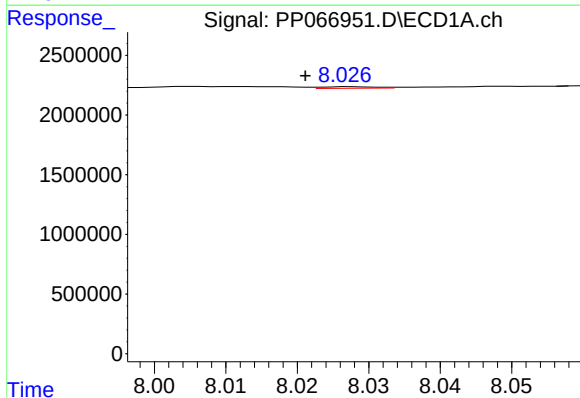


#33 AR-1260-3

R.T.: 8.028 min
Delta R.T.: 0.006 min
Response: 67540
Conc: 1.51 ng/ml

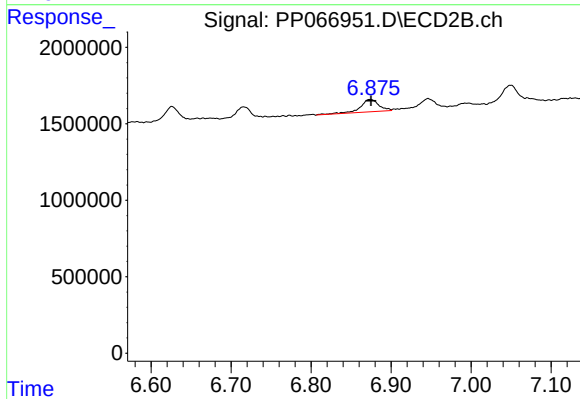

#33 AR-1260-3


R.T.: 6.874 min
Delta R.T.: 0.000 min
Response: 1321637
Conc: 19.84 ng/ml

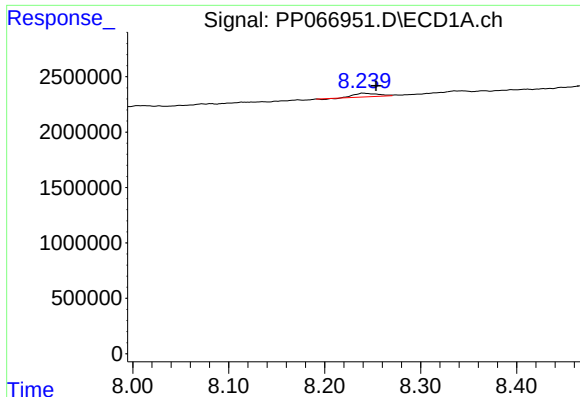

#34 AR-1260-4


R.T.: 8.240 min
Delta R.T.: -0.013 min
Response: 510962
Conc: 10.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

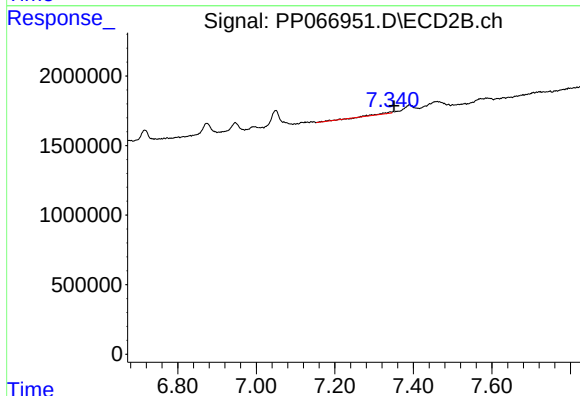


#34 AR-1260-4

R.T.: 7.341 min
Delta R.T.: -0.010 min
Response: 276785
Conc: 6.32 ng/ml

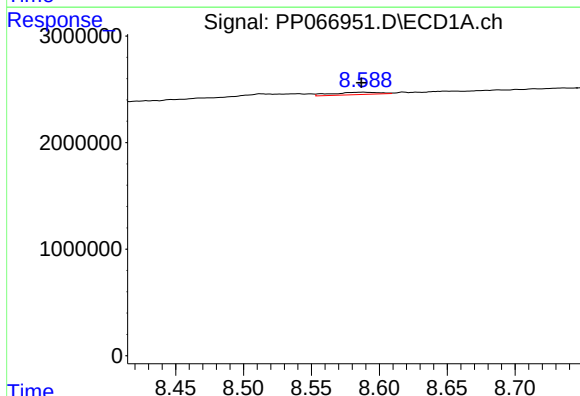


#35 AR-1260-5

R.T.: 8.588 min
Delta R.T.: 0.001 min
Response: 537943
Conc: 6.44 ng/ml

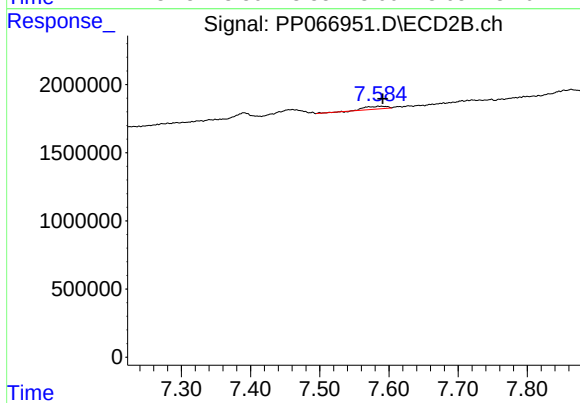

#35 AR-1260-5


R.T.: 7.585 min
Delta R.T.: -0.006 min
Response: 477534
Conc: 5.35 ng/ml

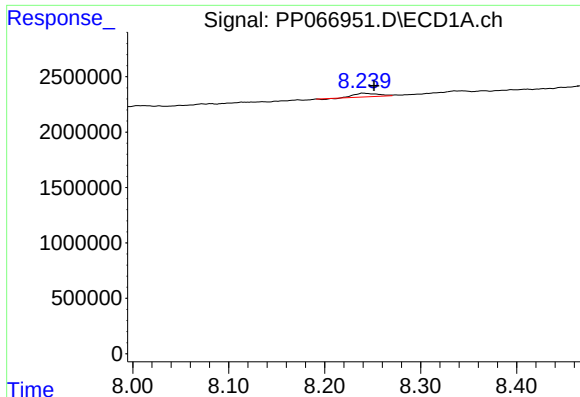

#36 AR-1262-1


R.T.: 8.240 min
Delta R.T.: -0.012 min
Response: 510962
Conc: 7.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

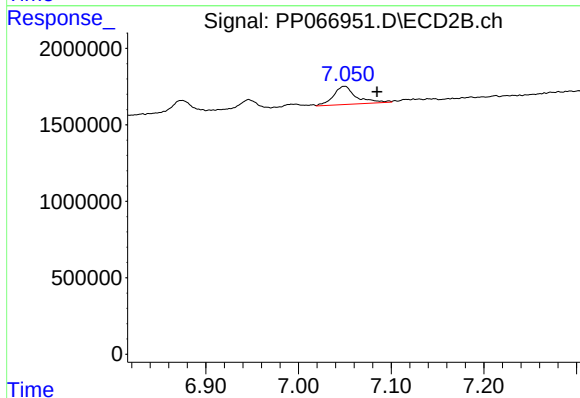


#36 AR-1262-1

R.T.: 7.050 min
Delta R.T.: -0.035 min
Response: 2042372
Conc: 28.27 ng/ml

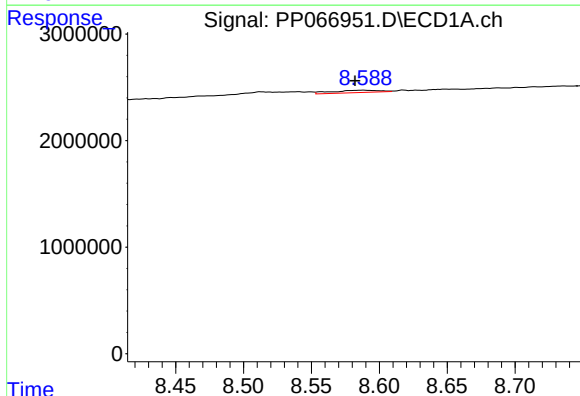


#37 AR-1262-2

R.T.: 8.588 min
Delta R.T.: 0.006 min
Response: 537943
Conc: 5.20 ng/ml

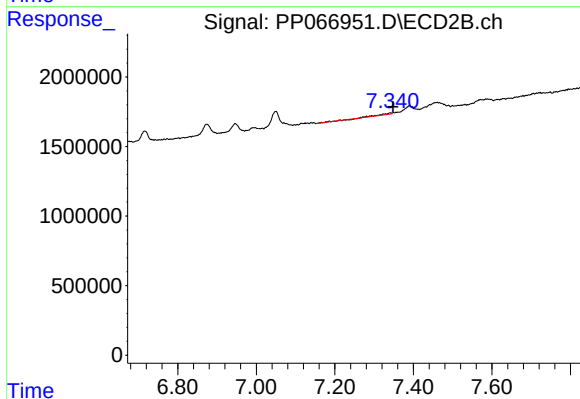

#37 AR-1262-2


R.T.: 7.341 min
Delta R.T.: -0.007 min
Response: 276785
Conc: 4.50 ng/ml

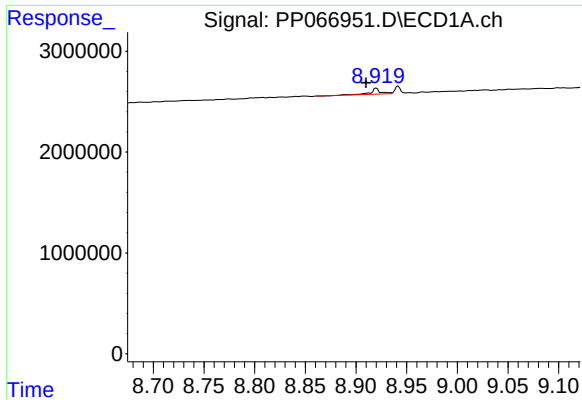

#38 AR-1262-3


R.T.: 8.920 min
Delta R.T.: 0.010 min
Response: 402010
Conc: 5.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

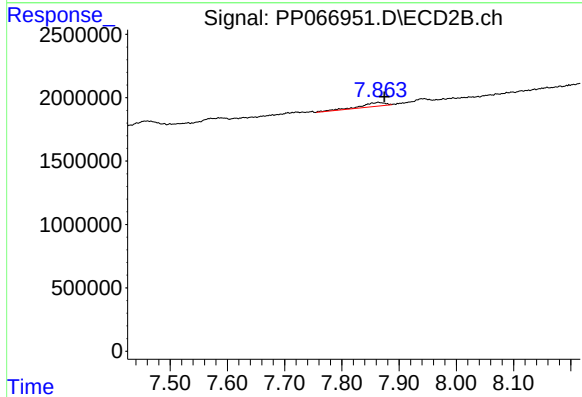


#38 AR-1262-3

R.T.: 7.864 min
Delta R.T.: -0.011 min
Response: 976746
Conc: 23.22 ng/ml

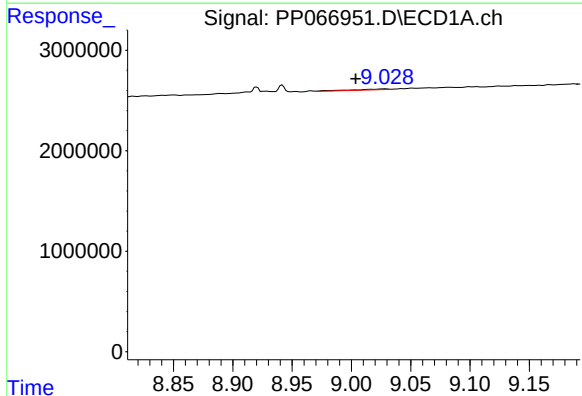


#39 AR-1262-4

R.T.: 9.029 min
Delta R.T.: 0.025 min
Response: 205456
Conc: 3.48 ng/ml

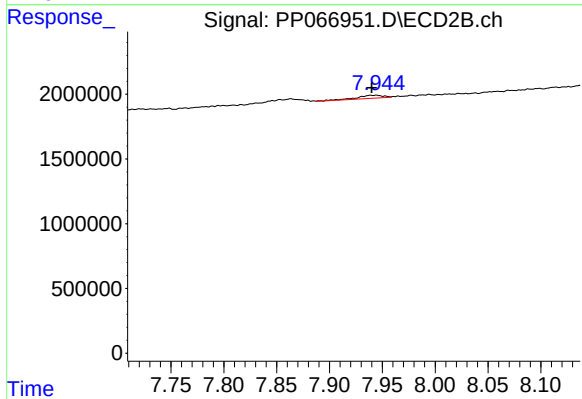

#39 AR-1262-4


R.T.: 7.944 min
Delta R.T.: 0.004 min
Response: 435824
Conc: 5.62 ng/ml

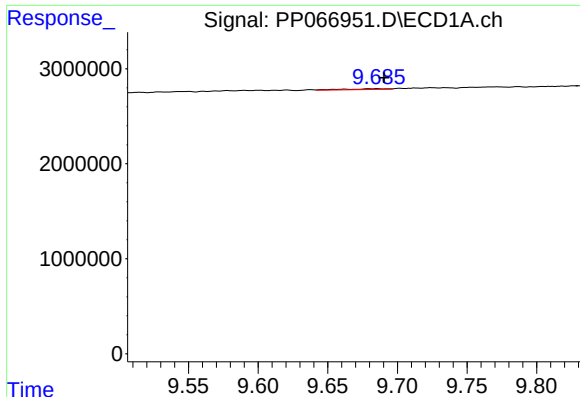

#40 AR-1262-5


R.T.: 9.685 min
Delta R.T.: -0.005 min
Response: 174276
Conc: 6.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

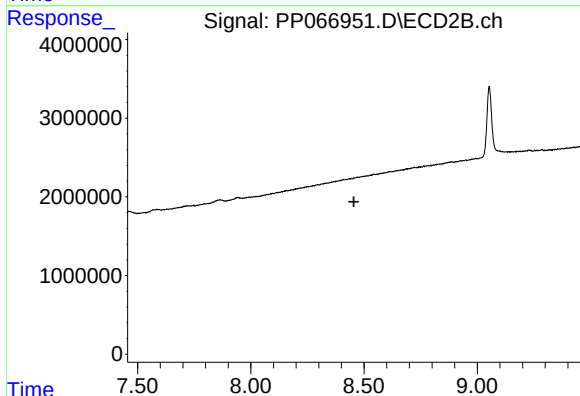


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 8.455 min
Response: 0
Conc: N.D.

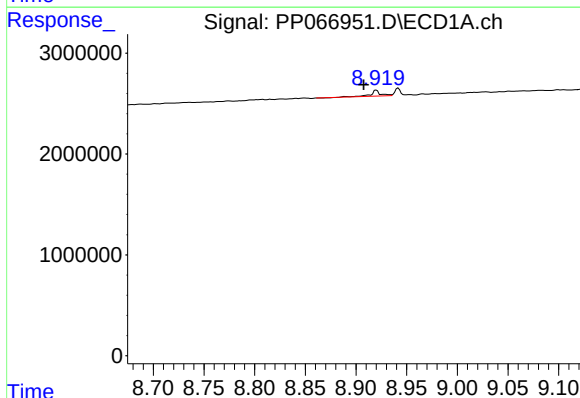


#41 AR-1268-1

R.T.: 8.920 min
Delta R.T.: 0.012 min
Response: 402010
Conc: 3.08 ng/ml

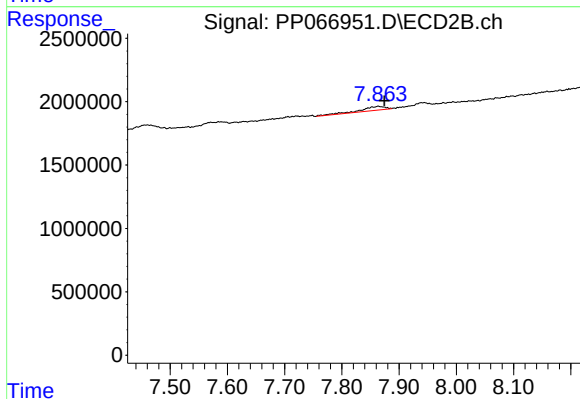

#41 AR-1268-1


R.T.: 7.864 min
Delta R.T.: -0.011 min
Response: 976746
Conc: 7.81 ng/ml

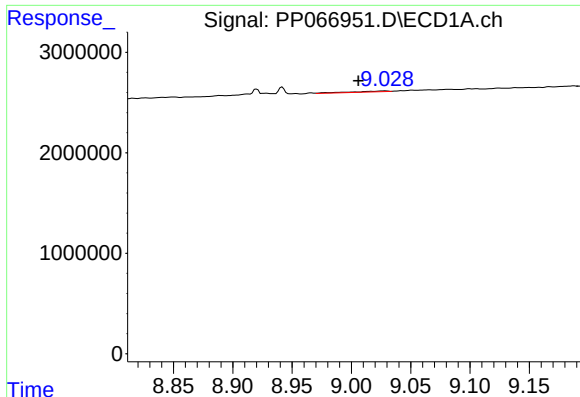

#42 AR-1268-2


R.T.: 9.029 min
Delta R.T.: 0.023 min
Response: 205456
Conc: 1.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

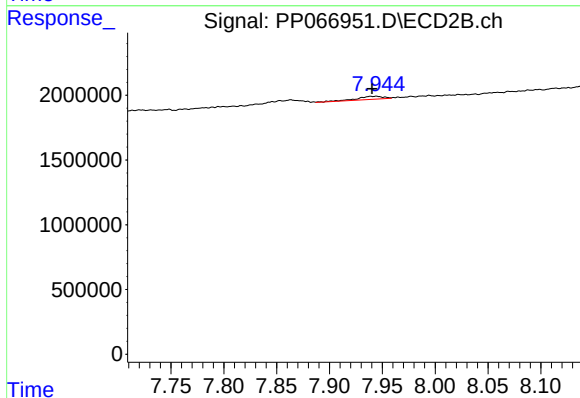


#42 AR-1268-2

R.T.: 7.944 min
Delta R.T.: 0.004 min
Response: 435824
Conc: 3.90 ng/ml

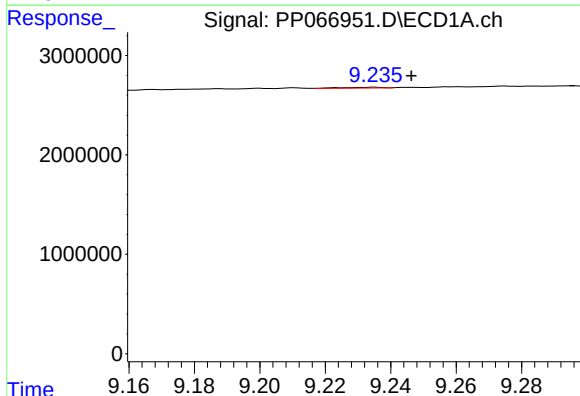


#43 AR-1268-3

R.T.: 9.235 min
Delta R.T.: -0.011 min
Response: 63138
Conc: 0.61 ng/ml

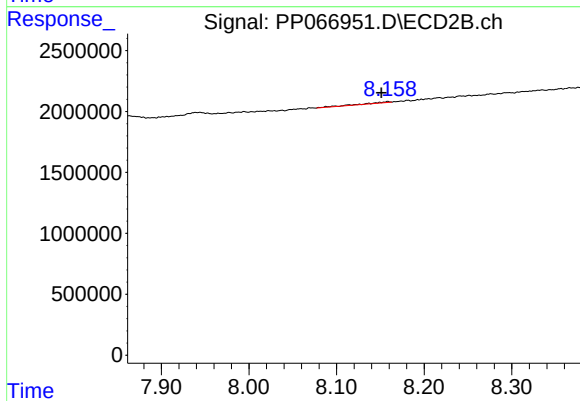

#43 AR-1268-3


R.T.: 8.159 min
Delta R.T.: 0.008 min
Response: 167995
Conc: 1.64 ng/ml

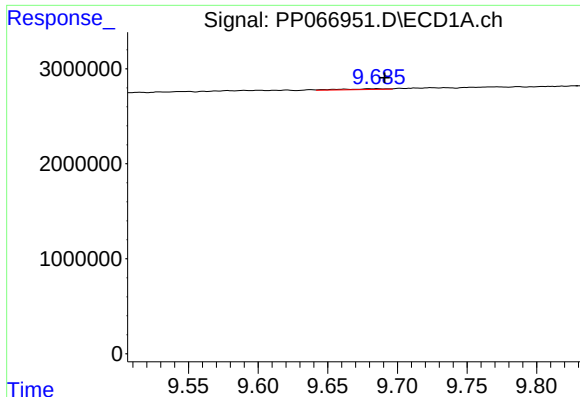

#44 AR-1268-4


R.T.: 9.685 min
Delta R.T.: -0.006 min
Response: 174276
Conc: 5.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

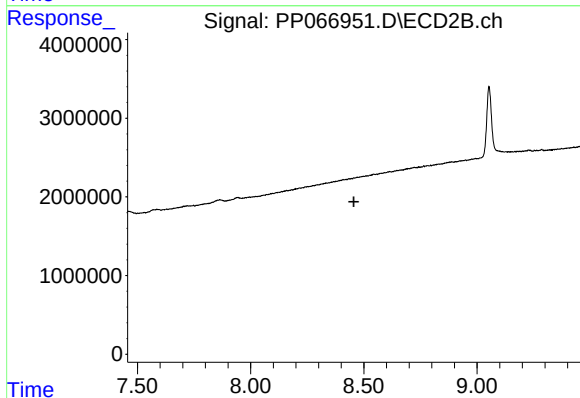


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.456 min
Response: 0
Conc: N.D.

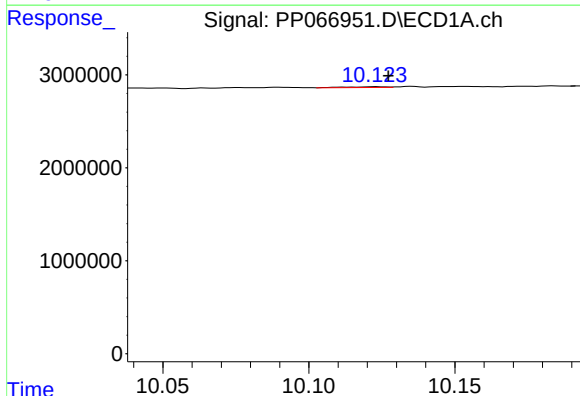

#45 AR-1268-5

R.T.: 10.123 min
Delta R.T.: -0.004 min
Response: 81796
Conc: 0.29 ng/ml

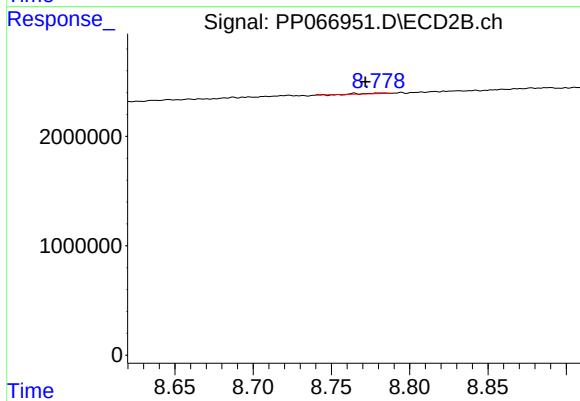

#45 AR-1268-5

R.T.: 8.764 min
Delta R.T.: -0.007 min
Response: 41239
Conc: 0.17 ng/ml