

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
 Data File : PP066953.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2024 15:39
 Operator : YP\AJ
 Sample : P3390-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 04:39:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 09:05:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.626	3.914	22780646	18646457	13.534	13.008
2)	SA Decachlor...	10.491	9.054	10518399	9512643	12.544	12.701
Target Compounds							
3)	L1 AR-1016-1	5.802	5.076f	27316	59780	0.577	1.369 #
4)	L1 AR-1016-2	5.829	5.076	44123	59780	0.596	0.929 #
5)	L1 AR-1016-3	5.879	5.238	65346	282344	1.393	8.222 #
6)	L1 AR-1016-4	5.983	5.270	21293	98125	0.589	3.239 #
7)	L1 AR-1016-5	6.280	5.531f	28254	170585	0.825	4.725 #
8)	L2 AR-1221-1	4.838	0.000	264338	0	14.572	N.D. #
9)	L2 AR-1221-2	4.936	4.222	360488	273698	26.777	23.392
10)	L2 AR-1221-3	5.000	0.000	75532	0	1.869	N.D. #
11)	L3 AR-1232-1	5.000	0.000	75532	0	2.266	N.D. #
12)	L3 AR-1232-2	5.538	5.076	92024	59780	5.213	2.027 #
13)	L3 AR-1232-3	5.829	5.238	44123	282344	1.413	19.880 #
14)	L3 AR-1232-4	5.983	5.284	21293	27702	1.392	1.971 #
15)	L3 AR-1232-5	6.089	5.531f	114587	170585	9.107	11.993 #
16)	L4 AR-1242-1	5.802	5.076f	27316	59780	0.794	1.924 #
17)	L4 AR-1242-2	5.829	5.076	44123	59780	0.831	1.339 #
18)	L4 AR-1242-3	5.879	5.238	65346	282344	1.906	11.704 #
19)	L4 AR-1242-4	5.983	5.284	21293	27702	0.821	1.035 #
20)	L4 AR-1242-5	6.715	5.814	68667	265705	2.955	9.520 #
21)	L5 AR-1248-1	5.802	5.076f	27316	59780	1.132	2.716 #
22)	L5 AR-1248-2	6.089	5.270	114587	98125	2.942	2.793
23)	L5 AR-1248-3	6.280	5.284	28254	27702	0.694	0.761
24)	L5 AR-1248-4	6.679	5.531f	73674	170585	1.902	4.198 #
25)	L5 AR-1248-5	6.715	5.868	68667	254285	1.744	7.960 #
26)	L6 AR-1254-1	6.659	5.814	286853	265705	5.765	4.477
27)	L6 AR-1254-2	6.879	5.999	204374	63798	2.893	1.218 #
28)	L6 AR-1254-3	7.245	6.396	391482	658255	5.746	8.629 #
29)	L6 AR-1254-4	7.522	6.625	149942	458967	3.581	12.150 #
30)	L6 AR-1254-5	7.944	7.045	854365	690893	16.260	10.977 #
31)	L7 AR-1260-1	7.407	6.520	91891	384281	1.518	6.066 #
32)	L7 AR-1260-2	7.658	6.711	127435	381077	1.982	5.636 #
33)	L7 AR-1260-3	8.021	6.881	569909	743939	12.767	11.170
34)	L7 AR-1260-4	8.277	7.348	824971	882052	16.466	20.126
35)	L7 AR-1260-5	8.586	7.589	194539	396341	2.328	4.444 #
36)	L8 AR-1262-1	8.277	7.087	824971	542219	12.615	7.505 #
37)	L8 AR-1262-2	8.586	7.348	194539	882052	1.881	14.334 #
38)	L8 AR-1262-3	8.912	7.877	1964351	2555964	27.505	60.763 #
39)	L8 AR-1262-4	9.011	7.943	1652861	2072124	27.996	26.713
40)	L8 AR-1262-5	9.695	8.459	778398	466162	28.292	17.652 #
41)	L9 AR-1268-1	8.912	7.877	1964351	2555964	15.032	20.435 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
 Data File : PP066953.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2024 15:39
 Operator : YP\AJ
 Sample : P3390-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 04:39:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 09:05:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	9.011	7.943	1652861	2072124	14.124	18.540 #
43) L9	AR-1268-3	9.251	8.153	1570696	1327006	15.092	12.982
44) L9	AR-1268-4	9.695	8.459	778398	466162	26.005	16.419 #
45) L9	AR-1268-5	10.132	8.775	3332639	3249813	11.898	13.251



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
Data File : PP066953.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2024 15:39
Operator : YP\AJ
Sample : P3390-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 04:39:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 09:05:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

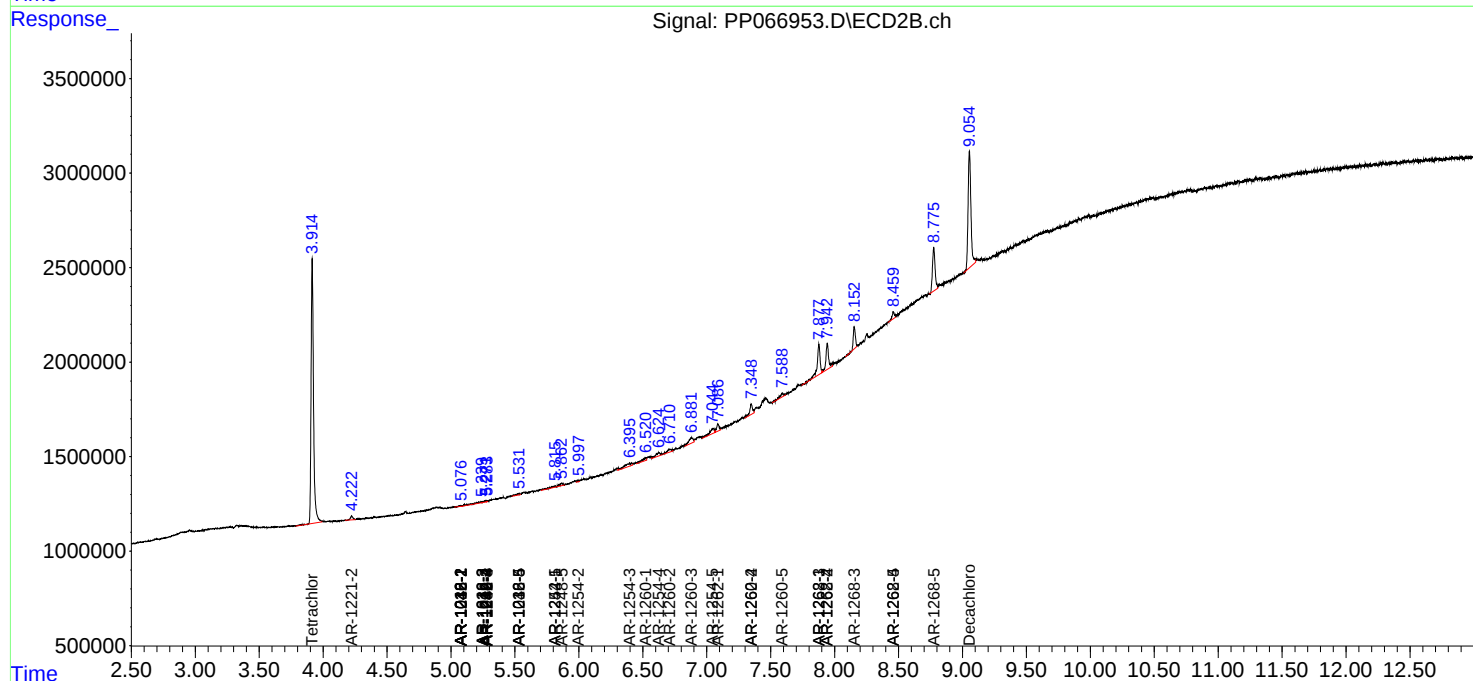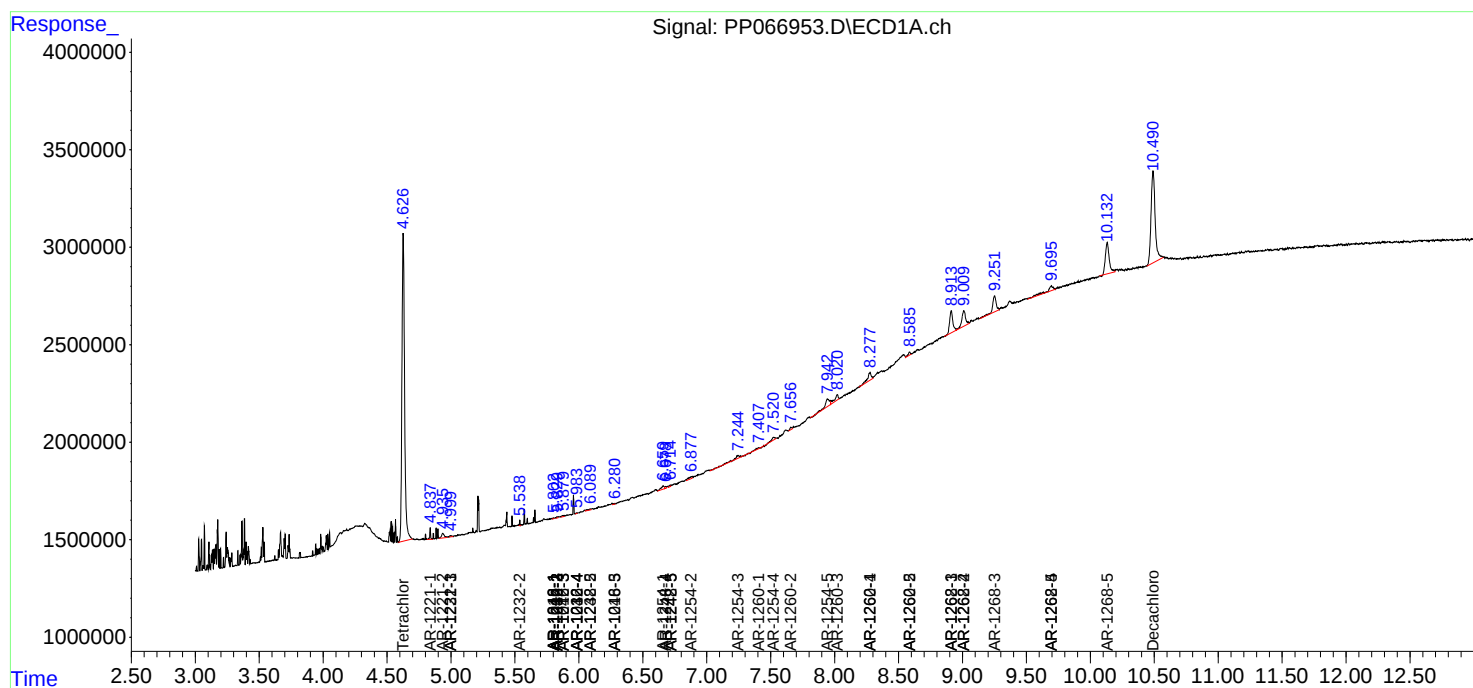


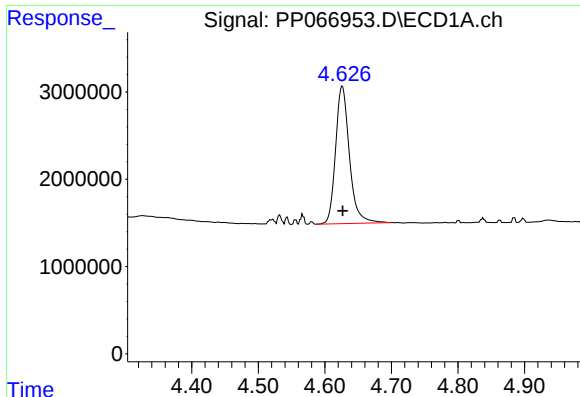

#1 Tetrachloro-m-xylene


R.T.: 4.626 min
Delta R.T.: 0.000 min
Response: 22780646
Conc: 13.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

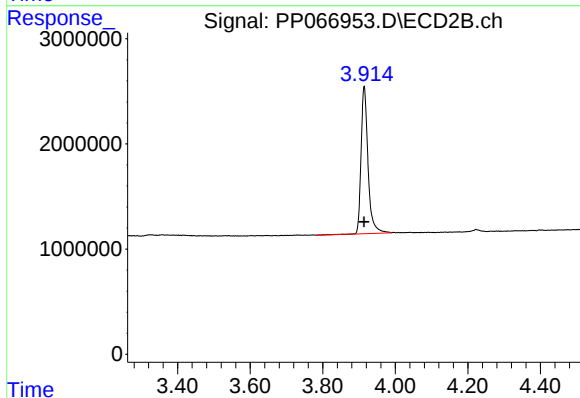


#1 Tetrachloro-m-xylene

R.T.: 3.914 min
Delta R.T.: 0.000 min
Response: 18646457
Conc: 13.01 ng/ml

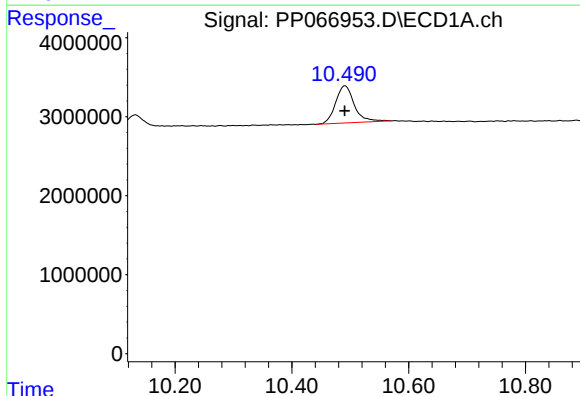


#2 Decachlorobiphenyl

R.T.: 10.491 min
Delta R.T.: 0.000 min
Response: 10518399
Conc: 12.54 ng/ml

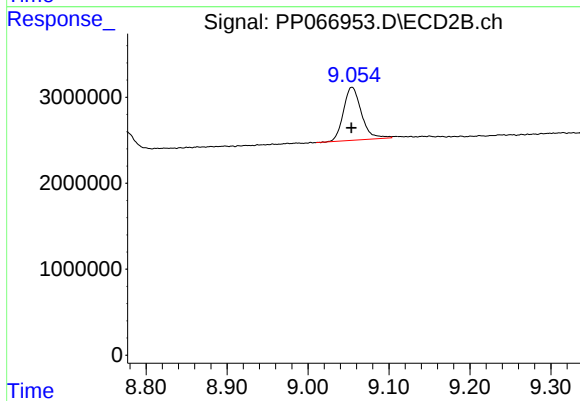

#2 Decachlorobiphenyl


R.T.: 9.054 min
Delta R.T.: 0.000 min
Response: 9512643
Conc: 12.70 ng/ml

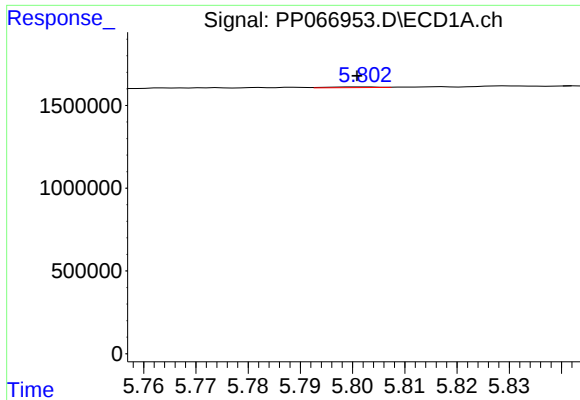

#3 AR-1016-1


R.T.: 5.802 min
Delta R.T.: 0.001 min
Response: 27316
Conc: 0.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

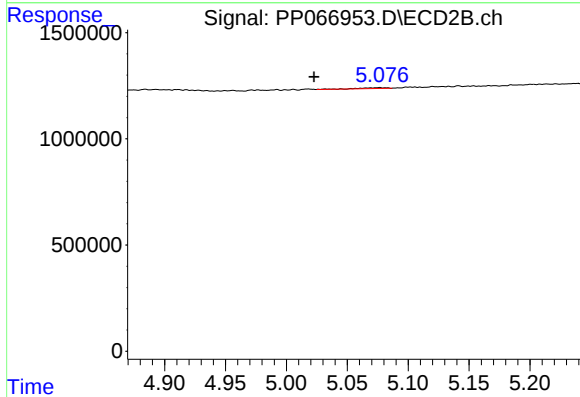


#3 AR-1016-1

R.T.: 5.076 min
Delta R.T.: 0.054 min
Response: 59780
Conc: 1.37 ng/ml

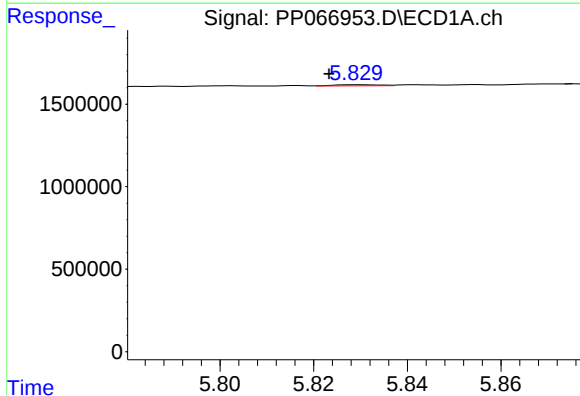


#4 AR-1016-2

R.T.: 5.829 min
Delta R.T.: 0.006 min
Response: 44123
Conc: 0.60 ng/ml

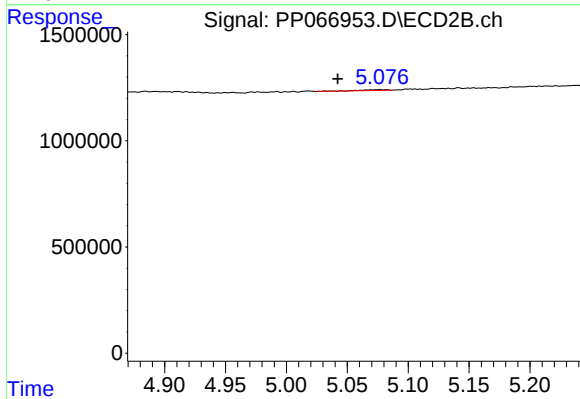

#4 AR-1016-2


R.T.: 5.076 min
Delta R.T.: 0.034 min
Response: 59780
Conc: 0.93 ng/ml

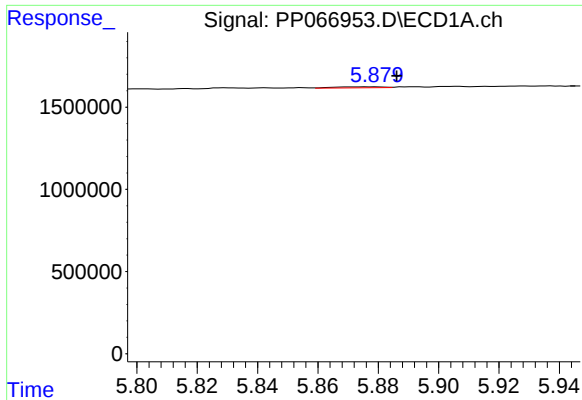

#5 AR-1016-3


R.T.: 5.879 min
Delta R.T.: -0.007 min
Response: 65346
Conc: 1.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

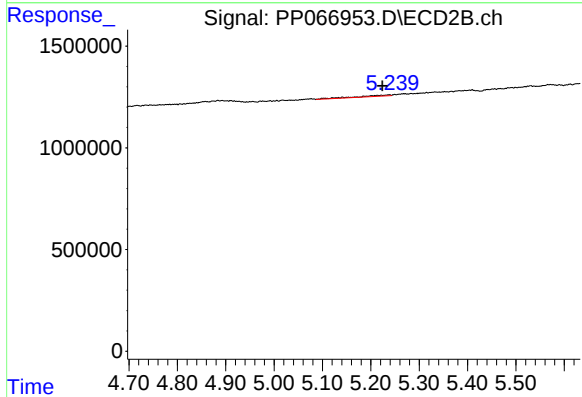


#5 AR-1016-3

R.T.: 5.238 min
Delta R.T.: 0.014 min
Response: 282344
Conc: 8.22 ng/ml

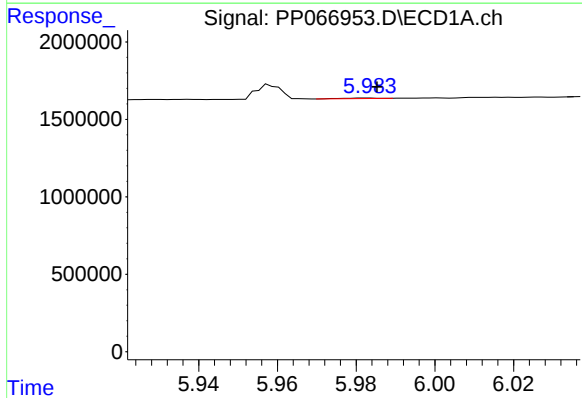


#6 AR-1016-4

R.T.: 5.983 min
Delta R.T.: -0.003 min
Response: 21293
Conc: 0.59 ng/ml

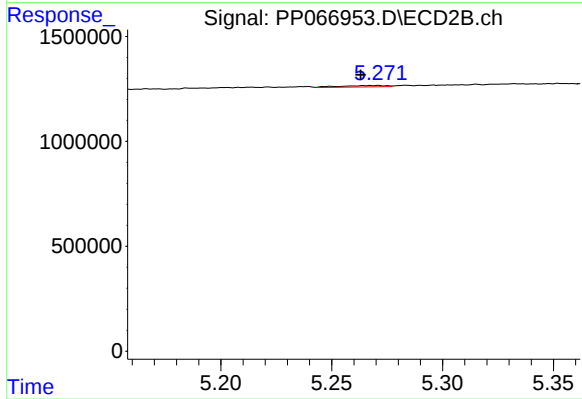

#6 AR-1016-4


R.T.: 5.270 min
Delta R.T.: 0.007 min
Response: 98125
Conc: 3.24 ng/ml

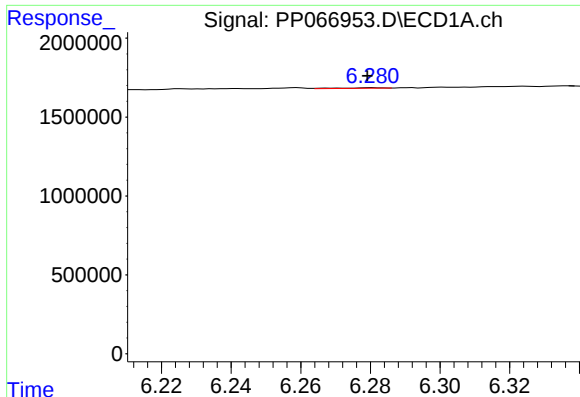

#7 AR-1016-5


R.T.: 6.280 min
Delta R.T.: 0.001 min
Response: 28254
Conc: 0.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

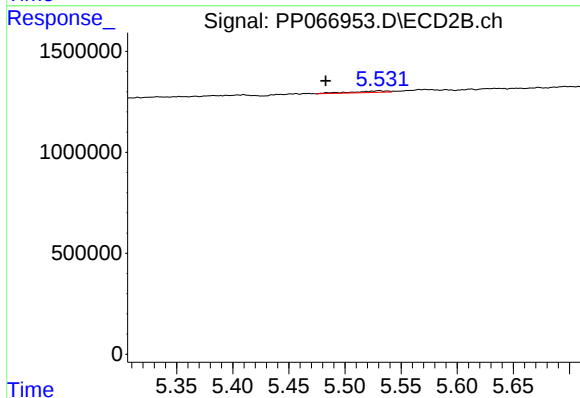


#7 AR-1016-5

R.T.: 5.531 min
Delta R.T.: 0.048 min
Response: 170585
Conc: 4.73 ng/ml

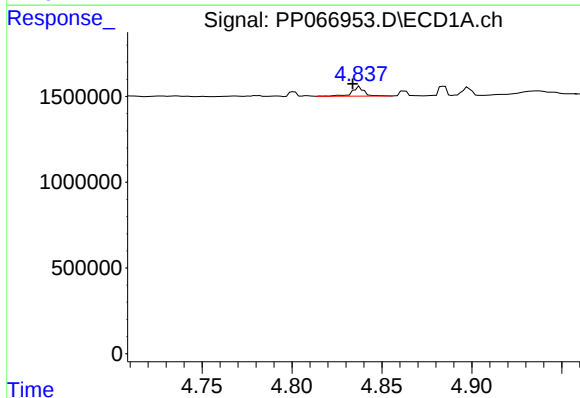


#8 AR-1221-1

R.T.: 4.838 min
Delta R.T.: 0.004 min
Response: 264338
Conc: 14.57 ng/ml

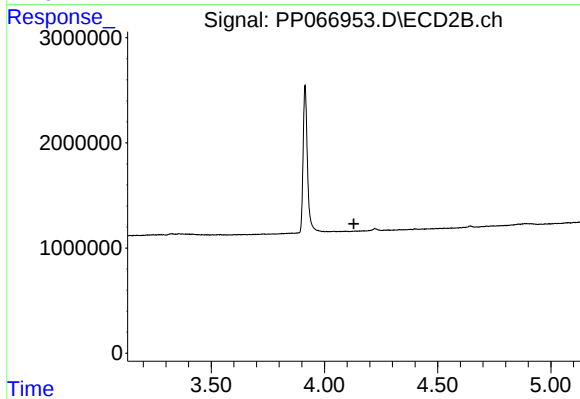

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 4.130 min
Response: 0
Conc: N.D.

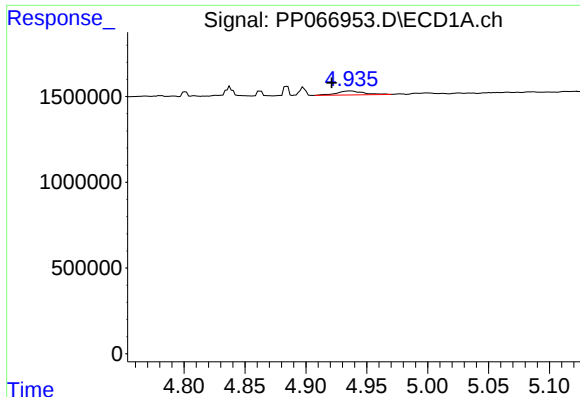

#9 AR-1221-2


R.T.: 4.936 min
Delta R.T.: 0.015 min
Response: 360488
Conc: 26.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

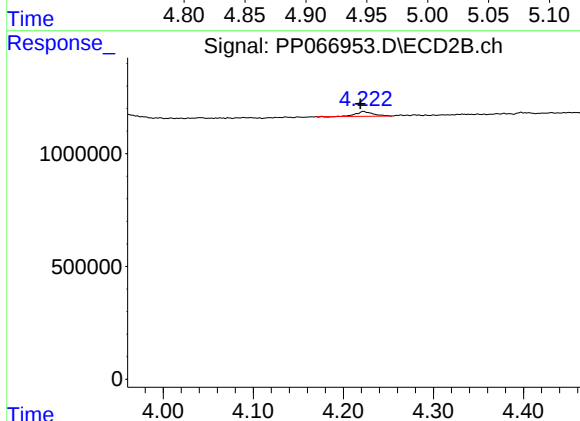


#9 AR-1221-2

R.T.: 4.222 min
Delta R.T.: 0.003 min
Response: 273698
Conc: 23.39 ng/ml

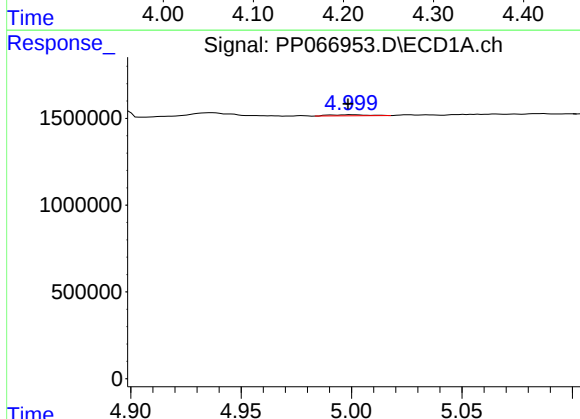


#10 AR-1221-3

R.T.: 5.000 min
Delta R.T.: 0.001 min
Response: 75532
Conc: 1.87 ng/ml

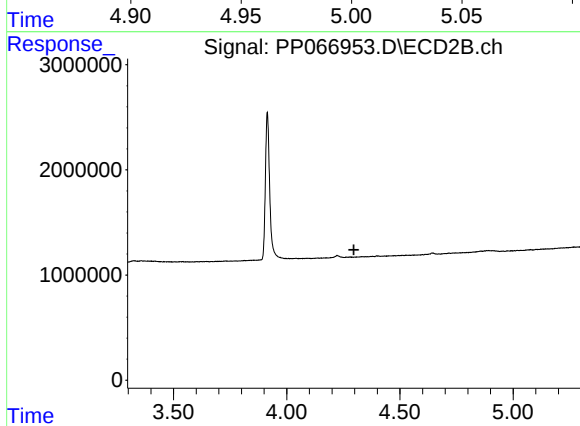

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.297 min
Response: 0
Conc: N.D.

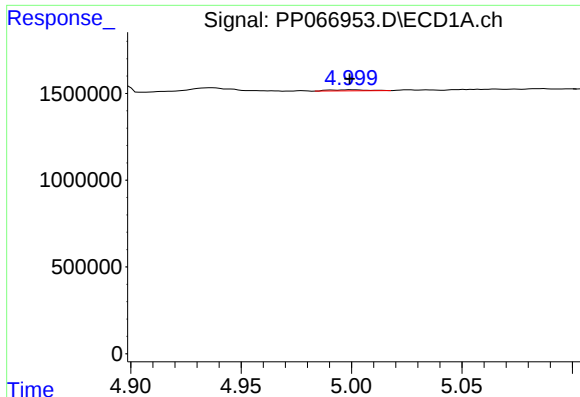

#11 AR-1232-1


R.T.: 5.000 min
Delta R.T.: 0.000 min
Response: 75532
Conc: 2.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

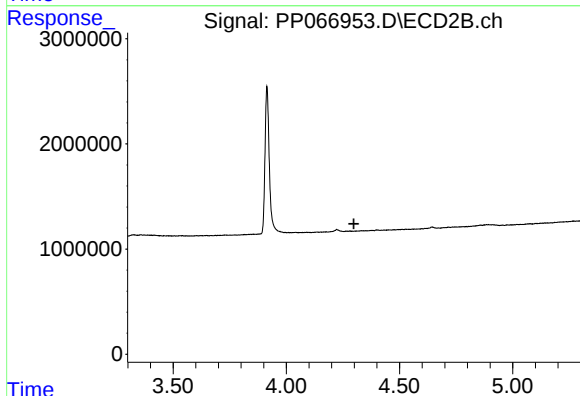


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.298 min
Response: 0
Conc: N.D.

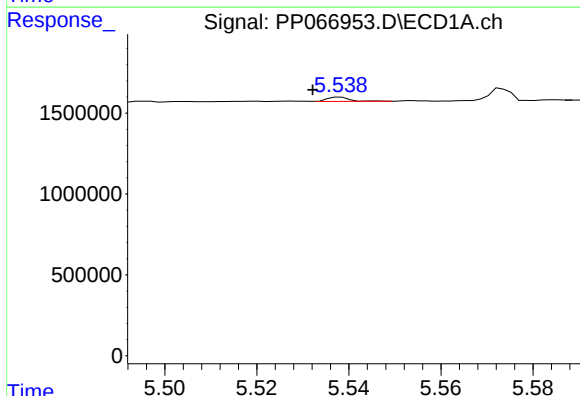


#12 AR-1232-2

R.T.: 5.538 min
Delta R.T.: 0.006 min
Response: 92024
Conc: 5.21 ng/ml

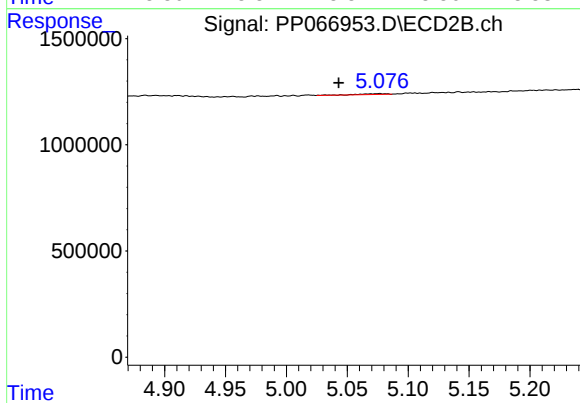

#12 AR-1232-2


R.T.: 5.076 min
Delta R.T.: 0.033 min
Response: 59780
Conc: 2.03 ng/ml

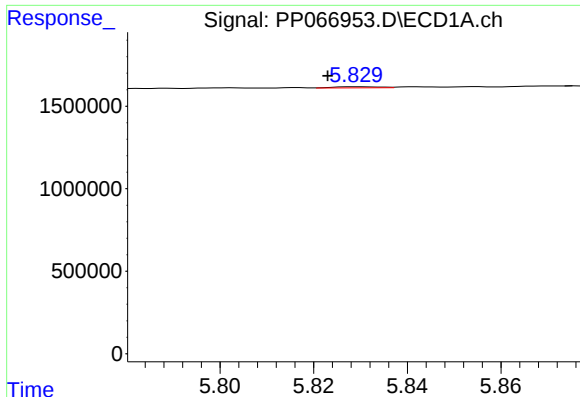

#13 AR-1232-3


R.T.: 5.829 min
Delta R.T.: 0.006 min
Response: 44123
Conc: 1.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

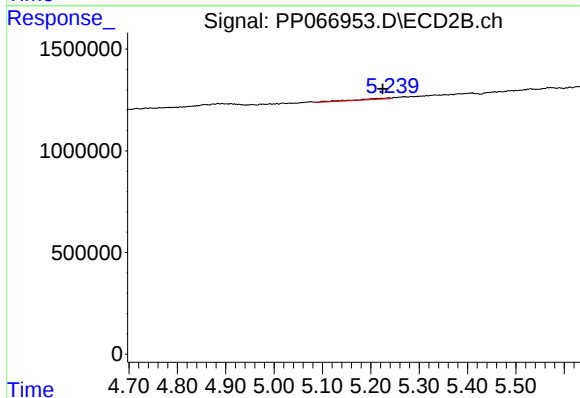


#13 AR-1232-3

R.T.: 5.238 min
Delta R.T.: 0.014 min
Response: 282344
Conc: 19.88 ng/ml

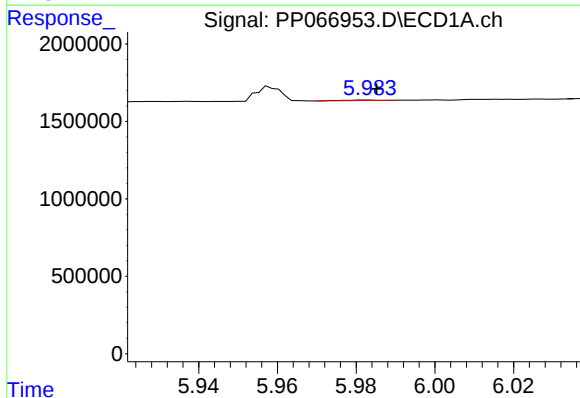


#14 AR-1232-4

R.T.: 5.983 min
Delta R.T.: -0.002 min
Response: 21293
Conc: 1.39 ng/ml

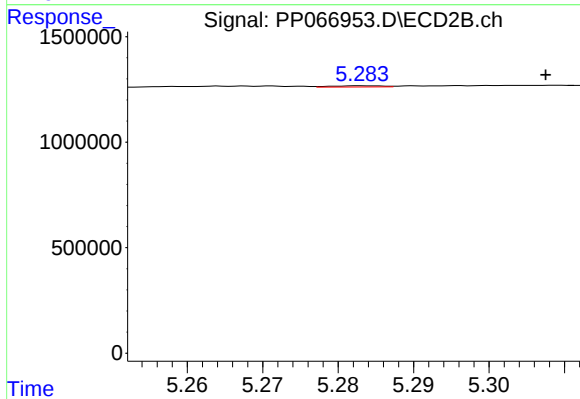

#14 AR-1232-4


R.T.: 5.284 min
Delta R.T.: -0.024 min
Response: 27702
Conc: 1.97 ng/ml

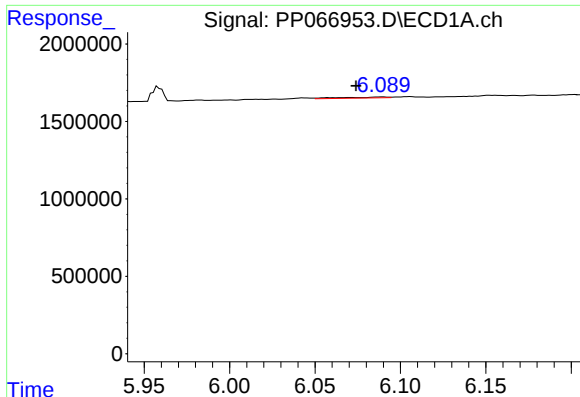

#15 AR-1232-5


R.T.: 6.089 min
Delta R.T.: 0.015 min
Response: 114587
Conc: 9.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

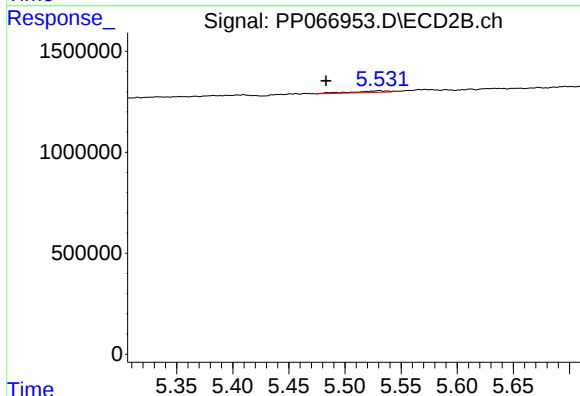


#15 AR-1232-5

R.T.: 5.531 min
Delta R.T.: 0.047 min
Response: 170585
Conc: 11.99 ng/ml

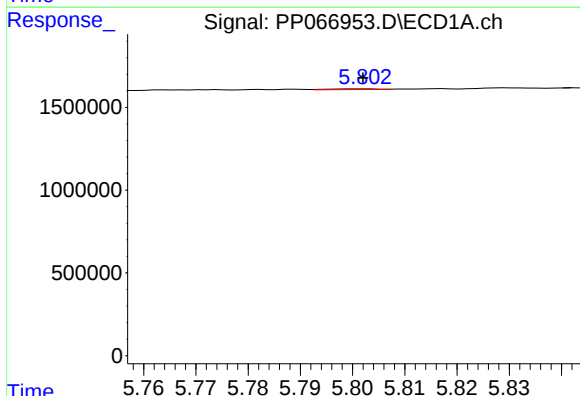


#16 AR-1242-1

R.T.: 5.802 min
Delta R.T.: 0.000 min
Response: 27316
Conc: 0.79 ng/ml

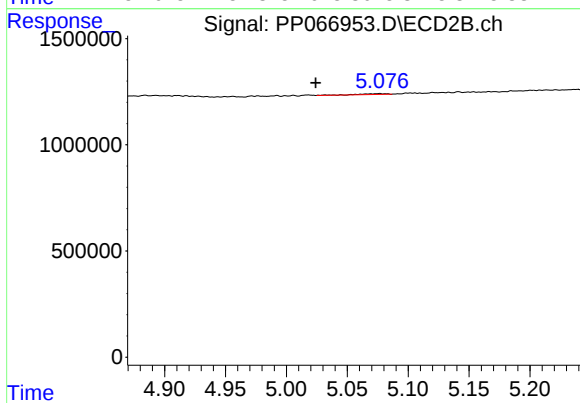

#16 AR-1242-1


R.T.: 5.076 min
Delta R.T.: 0.052 min
Response: 59780
Conc: 1.92 ng/ml

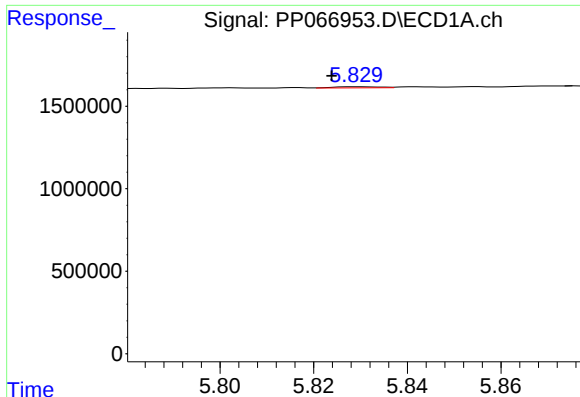

#17 AR-1242-2


R.T.: 5.829 min
Delta R.T.: 0.005 min
Response: 44123
Conc: 0.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

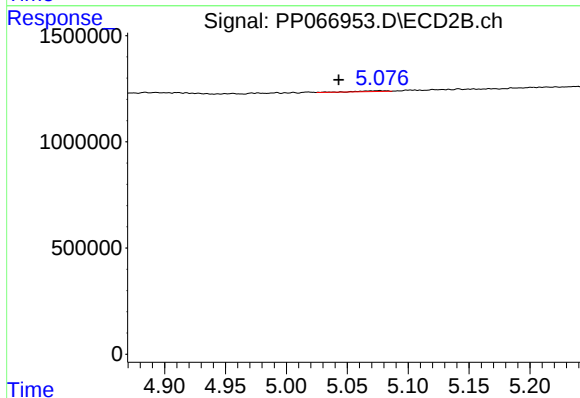


#17 AR-1242-2

R.T.: 5.076 min
Delta R.T.: 0.033 min
Response: 59780
Conc: 1.34 ng/ml

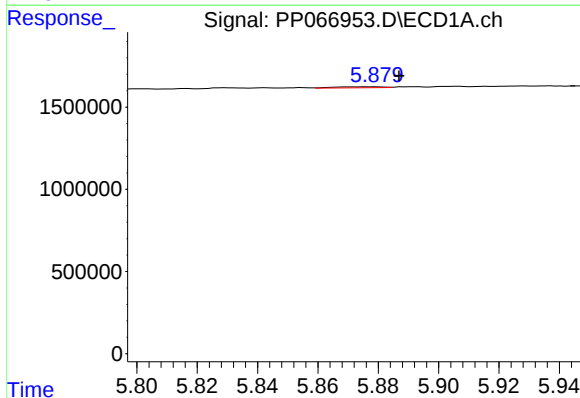


#18 AR-1242-3

R.T.: 5.879 min
Delta R.T.: -0.008 min
Response: 65346
Conc: 1.91 ng/ml

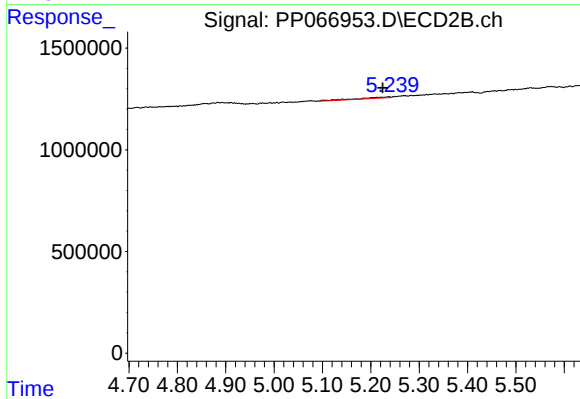

#18 AR-1242-3


R.T.: 5.238 min
Delta R.T.: 0.013 min
Response: 282344
Conc: 11.70 ng/ml

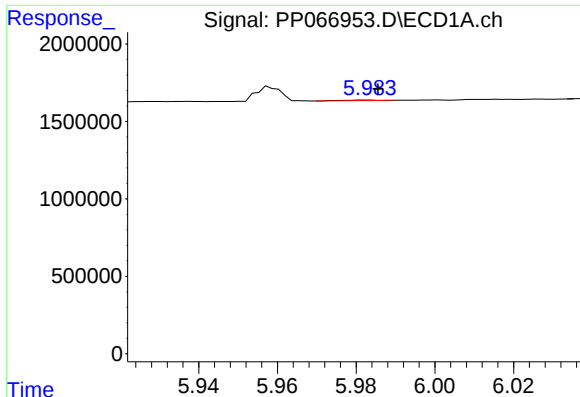

#19 AR-1242-4


R.T.: 5.983 min
Delta R.T.: -0.003 min
Response: 21293
Conc: 0.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

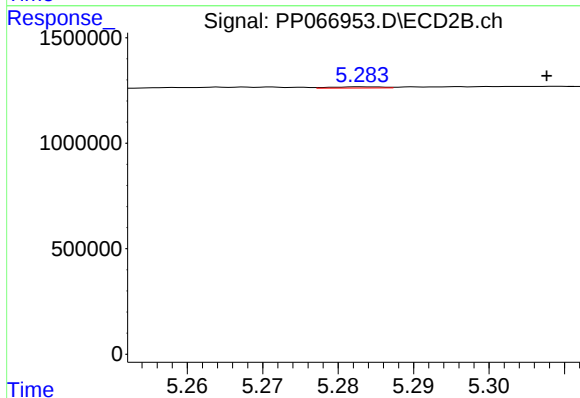


#19 AR-1242-4

R.T.: 5.284 min
Delta R.T.: -0.024 min
Response: 27702
Conc: 1.04 ng/ml

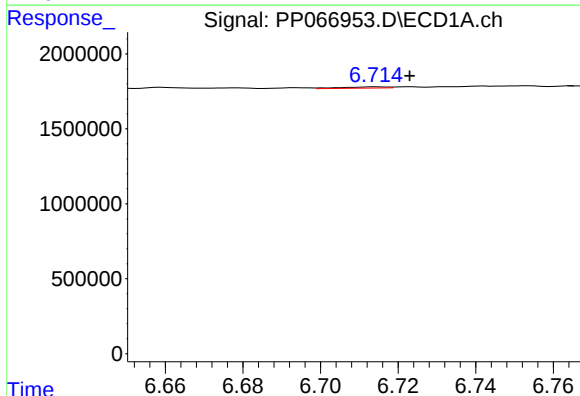


#20 AR-1242-5

R.T.: 6.715 min
Delta R.T.: -0.008 min
Response: 68667
Conc: 2.96 ng/ml

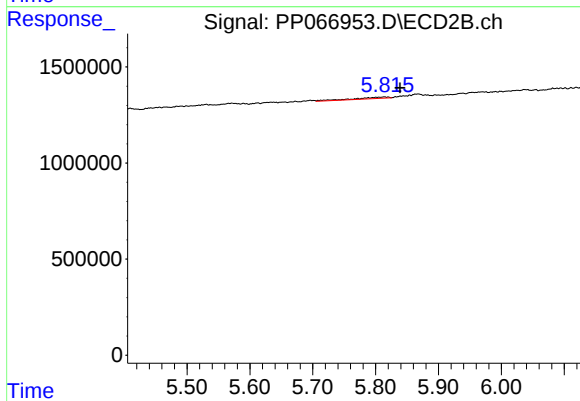

#20 AR-1242-5


R.T.: 5.814 min
Delta R.T.: -0.025 min
Response: 265705
Conc: 9.52 ng/ml

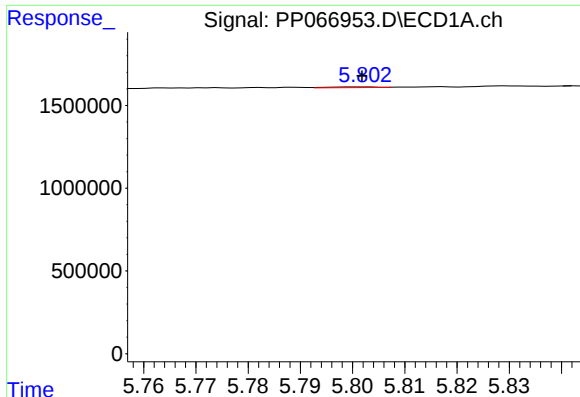

#21 AR-1248-1


R.T.: 5.802 min
Delta R.T.: 0.000 min
Response: 27316
Conc: 1.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

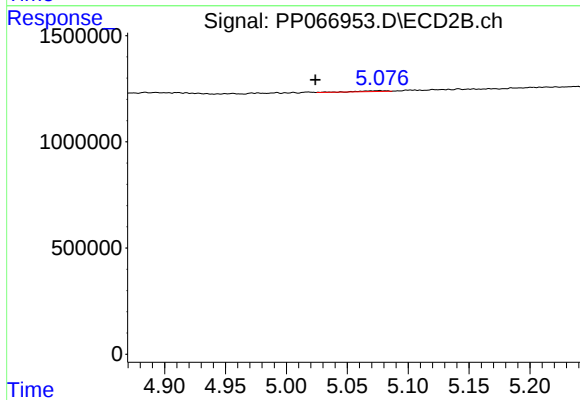


#21 AR-1248-1

R.T.: 5.076 min
Delta R.T.: 0.053 min
Response: 59780
Conc: 2.72 ng/ml

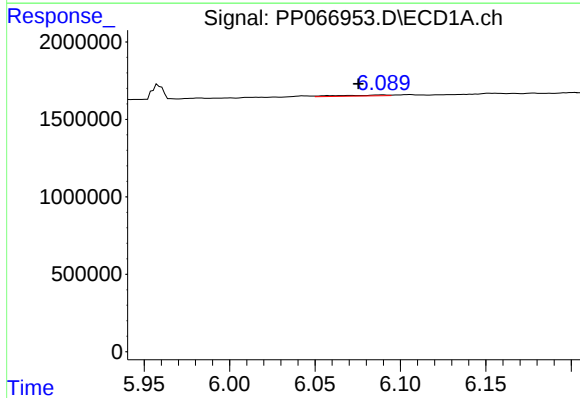


#22 AR-1248-2

R.T.: 6.089 min
Delta R.T.: 0.014 min
Response: 114587
Conc: 2.94 ng/ml

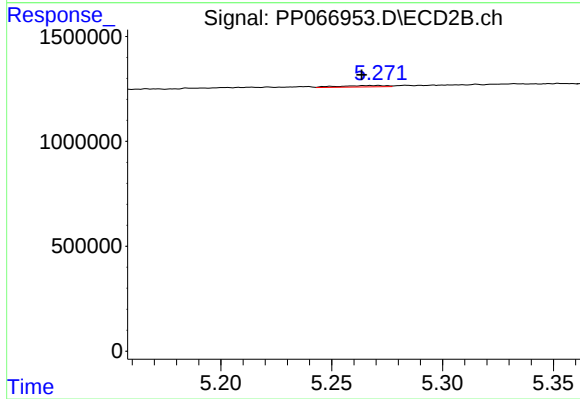

#22 AR-1248-2


R.T.: 5.270 min
Delta R.T.: 0.007 min
Response: 98125
Conc: 2.79 ng/ml

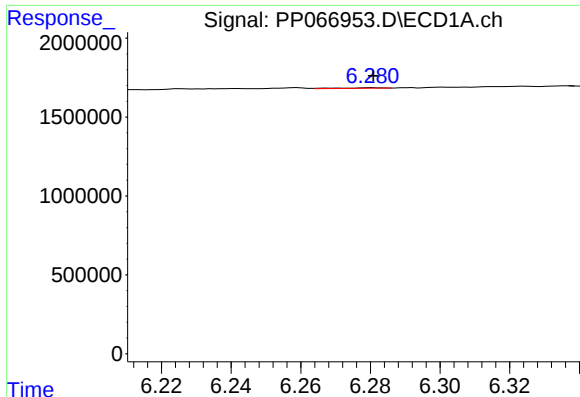

#23 AR-1248-3


R.T.: 6.280 min
Delta R.T.: 0.000 min
Response: 28254
Conc: 0.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

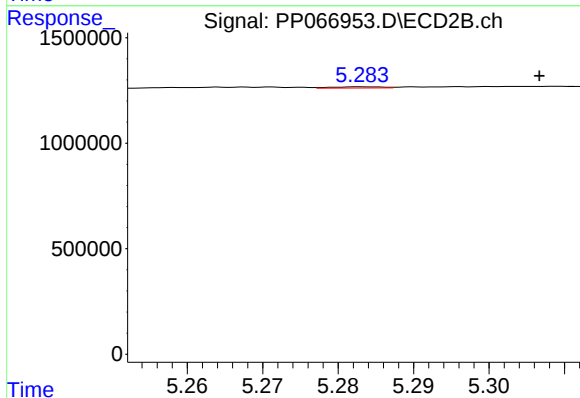


#23 AR-1248-3

R.T.: 5.284 min
Delta R.T.: -0.023 min
Response: 27702
Conc: 0.76 ng/ml

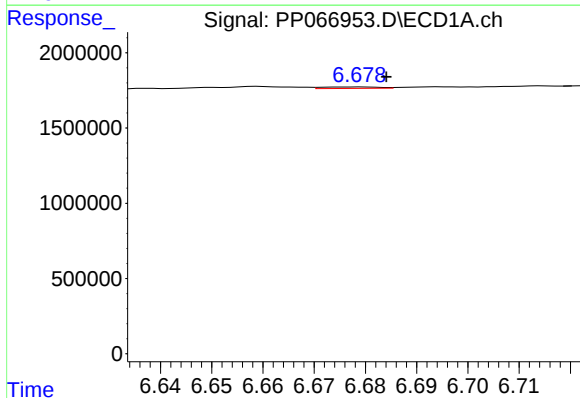


#24 AR-1248-4

R.T.: 6.679 min
Delta R.T.: -0.005 min
Response: 73674
Conc: 1.90 ng/ml

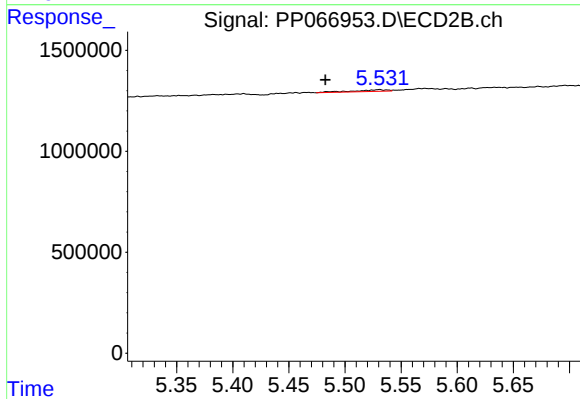

#24 AR-1248-4


R.T.: 5.531 min
Delta R.T.: 0.048 min
Response: 170585
Conc: 4.20 ng/ml

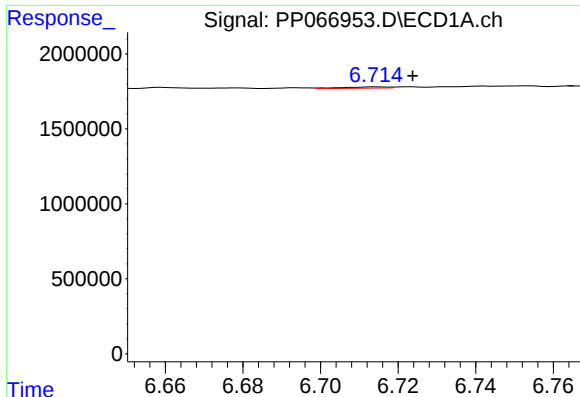

#25 AR-1248-5


R.T.: 6.715 min
Delta R.T.: -0.009 min
Response: 68667
Conc: 1.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

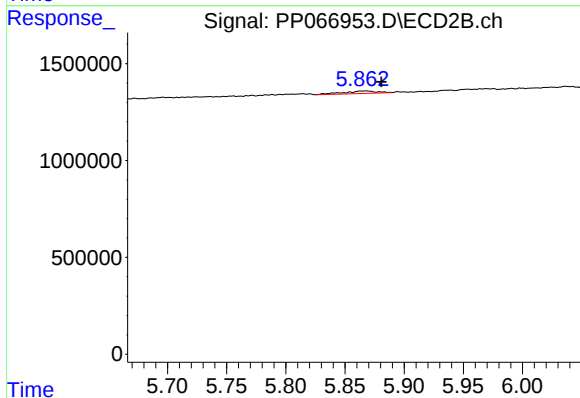


#25 AR-1248-5

R.T.: 5.868 min
Delta R.T.: -0.013 min
Response: 254285
Conc: 7.96 ng/ml

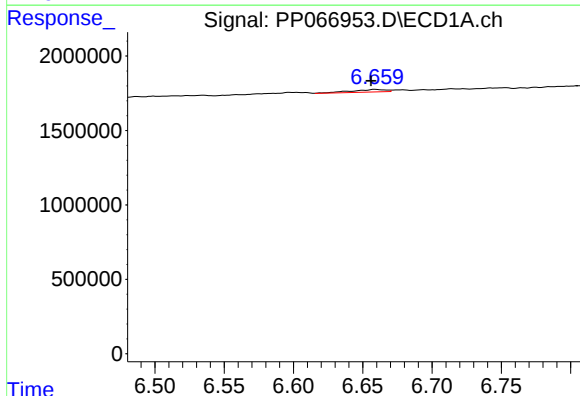


#26 AR-1254-1

R.T.: 6.659 min
Delta R.T.: 0.003 min
Response: 286853
Conc: 5.76 ng/ml

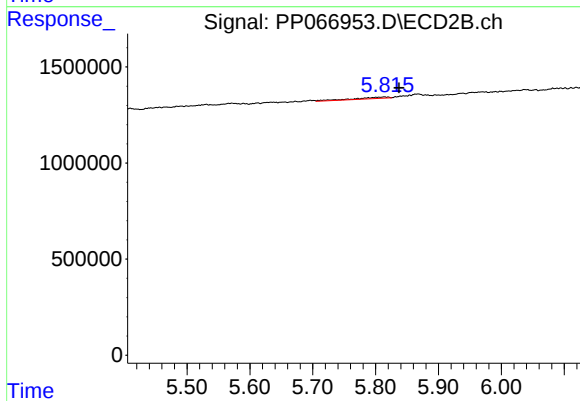

#26 AR-1254-1


R.T.: 5.814 min
Delta R.T.: -0.023 min
Response: 265705
Conc: 4.48 ng/ml

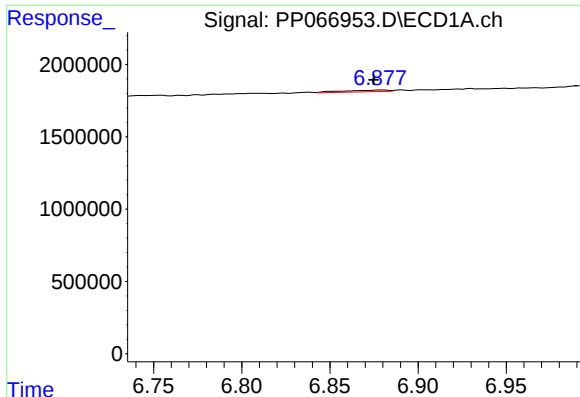

#27 AR-1254-2


R.T.: 6.879 min
Delta R.T.: 0.004 min
Response: 204374
Conc: 2.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

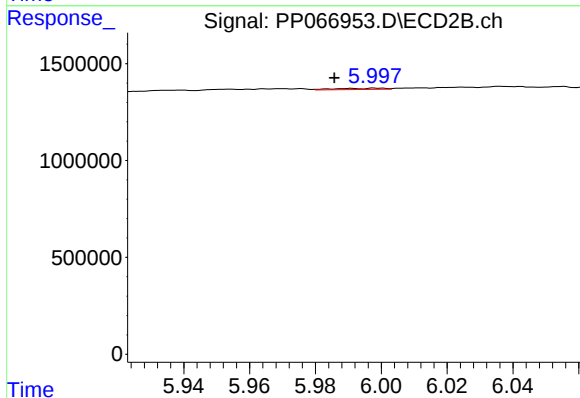


#27 AR-1254-2

R.T.: 5.999 min
Delta R.T.: 0.013 min
Response: 63798
Conc: 1.22 ng/ml

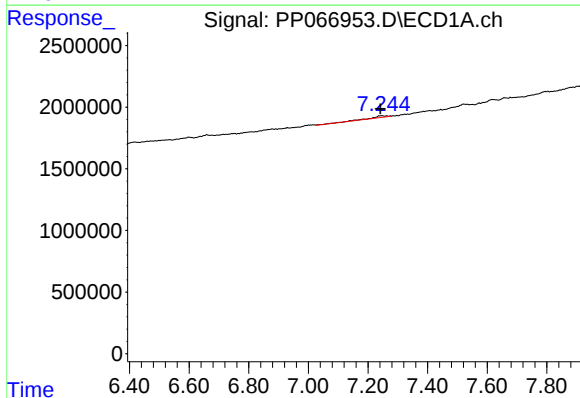


#28 AR-1254-3

R.T.: 7.245 min
Delta R.T.: 0.004 min
Response: 391482
Conc: 5.75 ng/ml

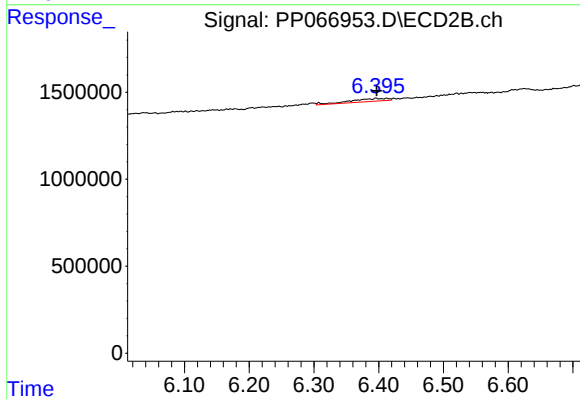

#28 AR-1254-3


R.T.: 6.396 min
Delta R.T.: 0.000 min
Response: 658255
Conc: 8.63 ng/ml

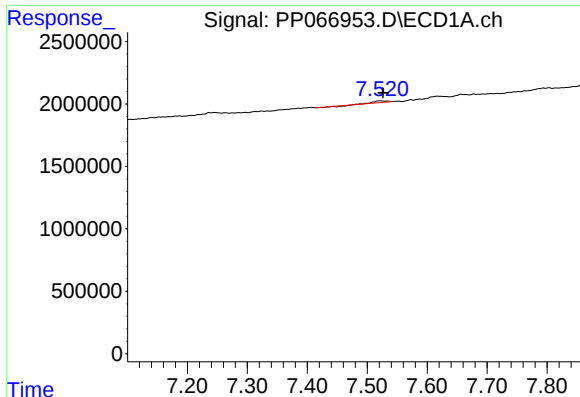

#29 AR-1254-4


R.T.: 7.522 min
Delta R.T.: -0.005 min
Response: 149942
Conc: 3.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

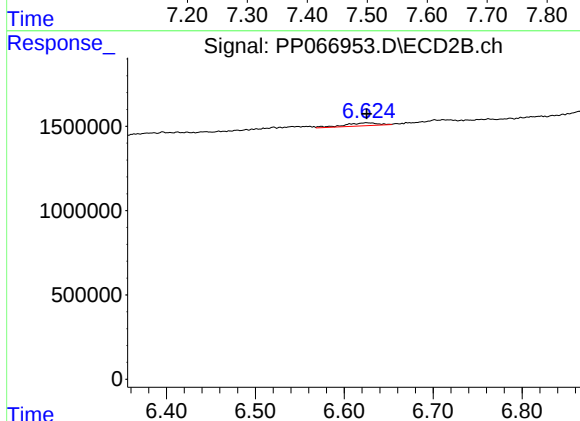


#29 AR-1254-4

R.T.: 6.625 min
Delta R.T.: 0.000 min
Response: 458967
Conc: 12.15 ng/ml

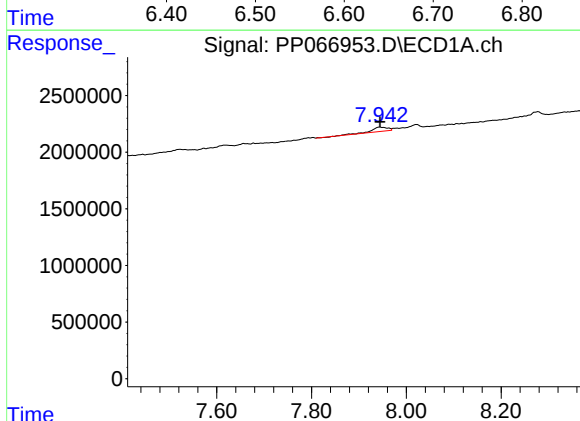


#30 AR-1254-5

R.T.: 7.944 min
Delta R.T.: -0.001 min
Response: 854365
Conc: 16.26 ng/ml

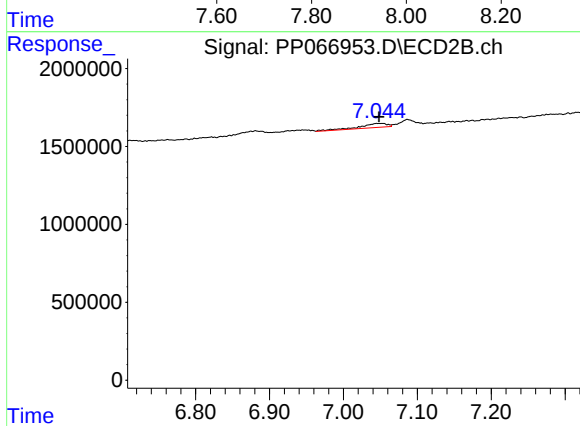

#30 AR-1254-5


R.T.: 7.045 min
Delta R.T.: -0.003 min
Response: 690893
Conc: 10.98 ng/ml

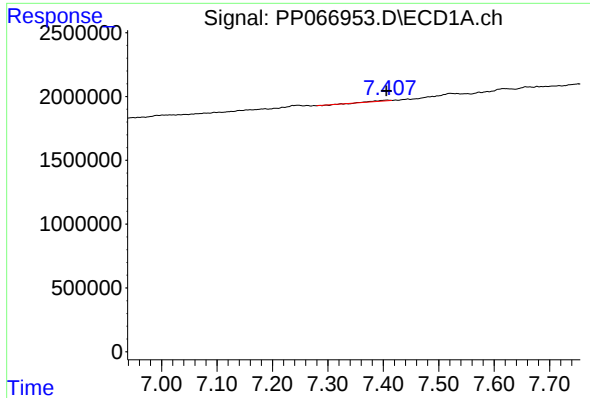

#31 AR-1260-1


R.T.: 7.407 min
Delta R.T.: 0.001 min
Response: 91891
Conc: 1.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

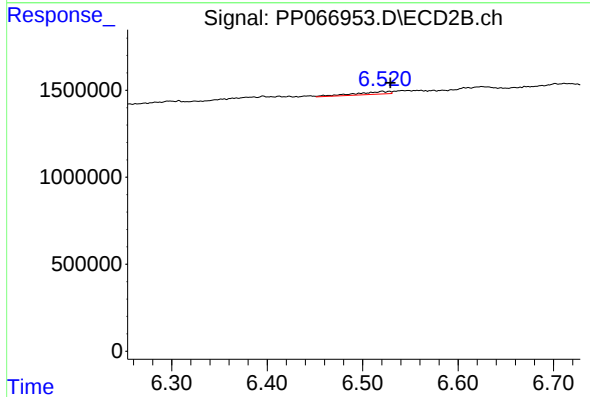


#31 AR-1260-1

R.T.: 6.520 min
Delta R.T.: -0.009 min
Response: 384281
Conc: 6.07 ng/ml

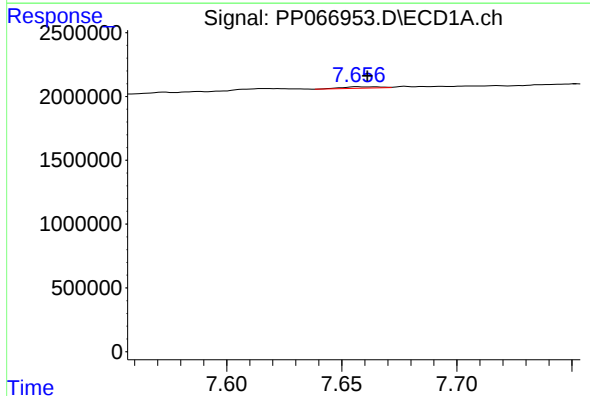


#32 AR-1260-2

R.T.: 7.658 min
Delta R.T.: -0.003 min
Response: 127435
Conc: 1.98 ng/ml

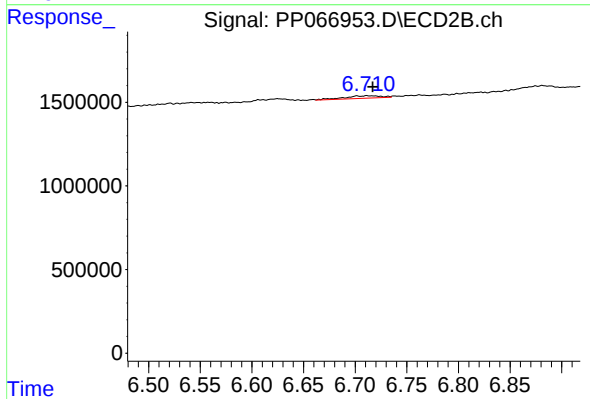

#32 AR-1260-2


R.T.: 6.711 min
Delta R.T.: -0.005 min
Response: 381077
Conc: 5.64 ng/ml

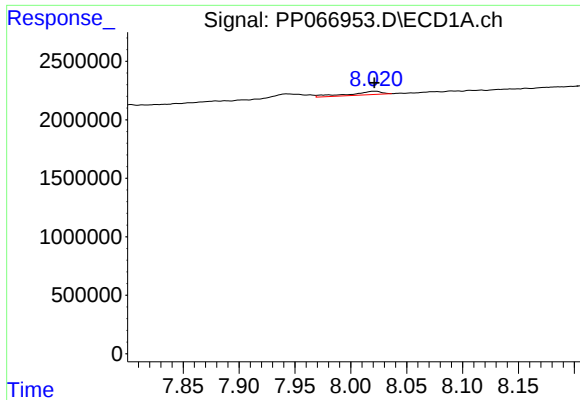

#33 AR-1260-3


R.T.: 8.021 min
Delta R.T.: 0.000 min
Response: 569909
Conc: 12.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

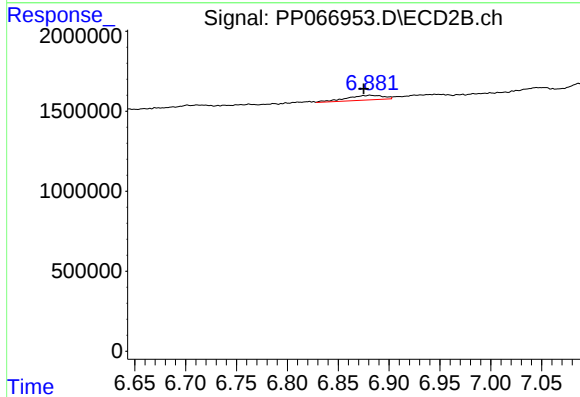


#33 AR-1260-3

R.T.: 6.881 min
Delta R.T.: 0.007 min
Response: 743939
Conc: 11.17 ng/ml

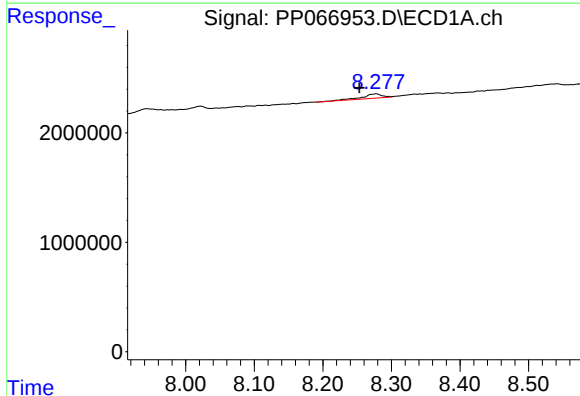


#34 AR-1260-4

R.T.: 8.277 min
Delta R.T.: 0.024 min
Response: 824971
Conc: 16.47 ng/ml

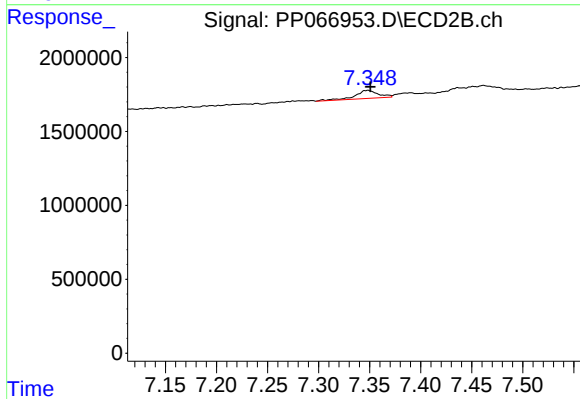

#34 AR-1260-4


R.T.: 7.348 min
Delta R.T.: -0.003 min
Response: 882052
Conc: 20.13 ng/ml

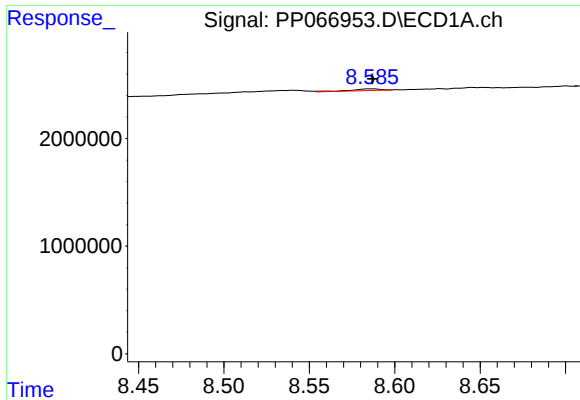

#35 AR-1260-5


R.T.: 8.586 min
Delta R.T.: 0.000 min
Response: 194539
Conc: 2.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

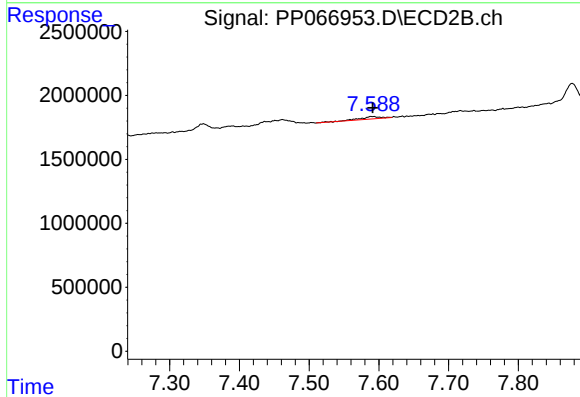


#35 AR-1260-5

R.T.: 7.589 min
Delta R.T.: -0.002 min
Response: 396341
Conc: 4.44 ng/ml

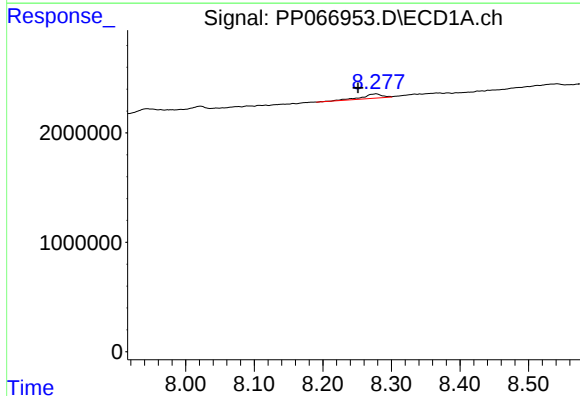


#36 AR-1262-1

R.T.: 8.277 min
Delta R.T.: 0.026 min
Response: 824971
Conc: 12.61 ng/ml

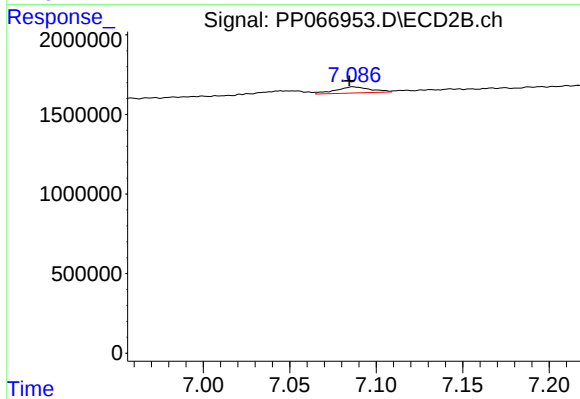

#36 AR-1262-1


R.T.: 7.087 min
Delta R.T.: 0.002 min
Response: 542219
Conc: 7.51 ng/ml

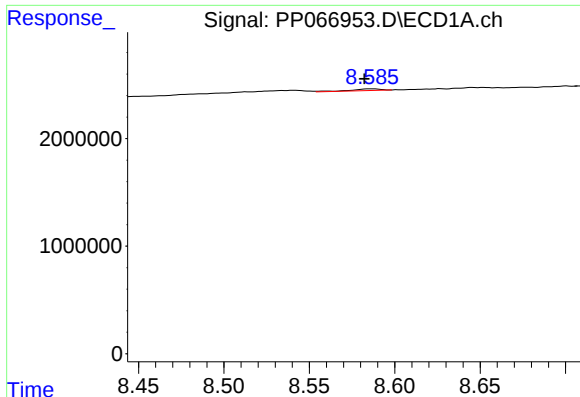

#37 AR-1262-2


R.T.: 8.586 min
Delta R.T.: 0.004 min
Response: 194539
Conc: 1.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

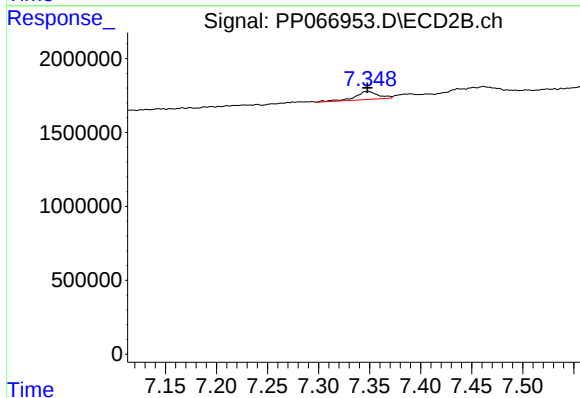


#37 AR-1262-2

R.T.: 7.348 min
Delta R.T.: 0.000 min
Response: 882052
Conc: 14.33 ng/ml

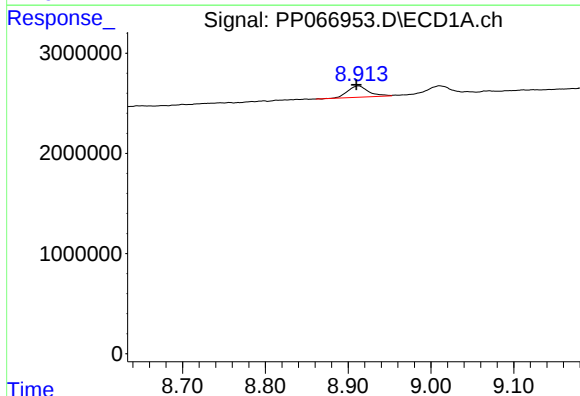


#38 AR-1262-3

R.T.: 8.912 min
Delta R.T.: 0.003 min
Response: 1964351
Conc: 27.50 ng/ml

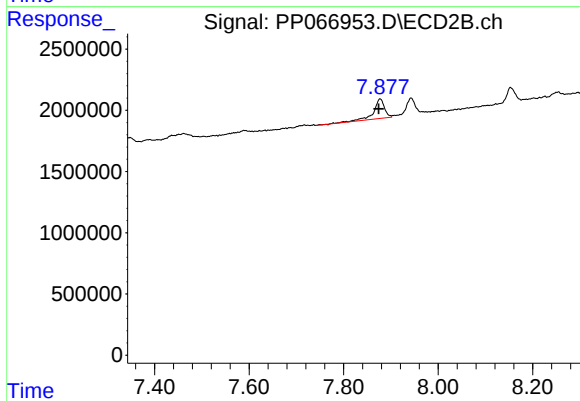

#38 AR-1262-3


R.T.: 7.877 min
Delta R.T.: 0.003 min
Response: 2555964
Conc: 60.76 ng/ml

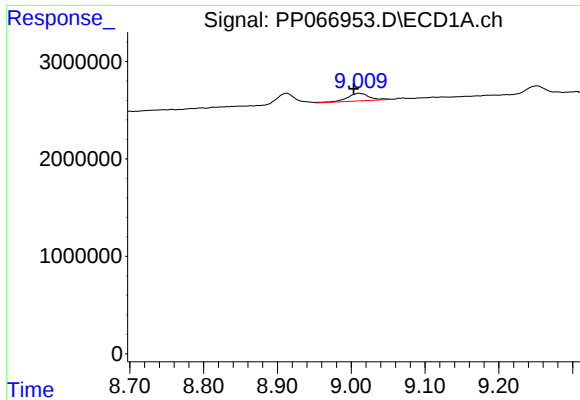

#39 AR-1262-4


R.T.: 9.011 min
Delta R.T.: 0.007 min
Response: 1652861
Conc: 28.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

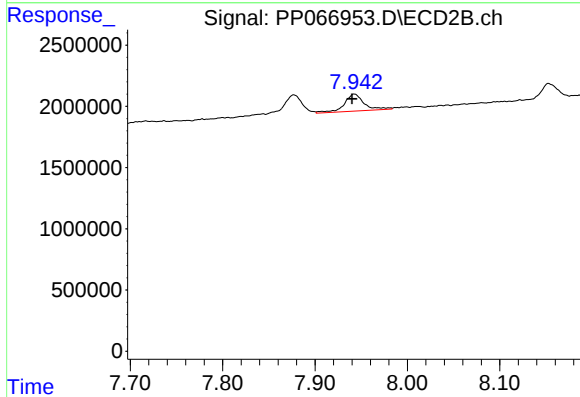


#39 AR-1262-4

R.T.: 7.943 min
Delta R.T.: 0.003 min
Response: 2072124
Conc: 26.71 ng/ml

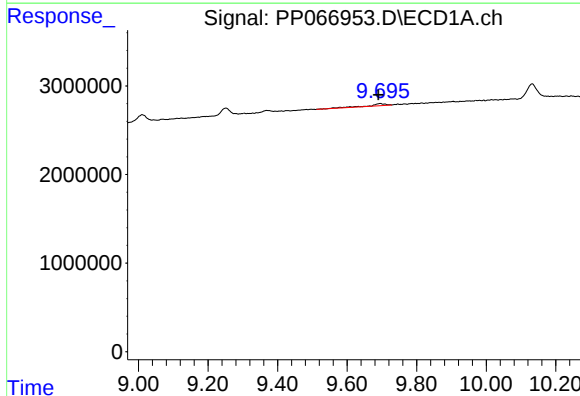


#40 AR-1262-5

R.T.: 9.695 min
Delta R.T.: 0.005 min
Response: 778398
Conc: 28.29 ng/ml

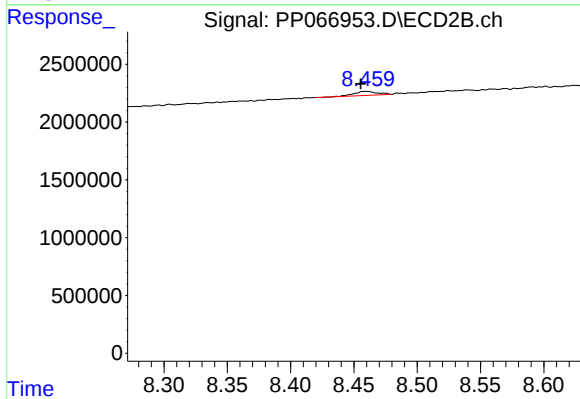

#40 AR-1262-5


R.T.: 8.459 min
Delta R.T.: 0.004 min
Response: 466162
Conc: 17.65 ng/ml

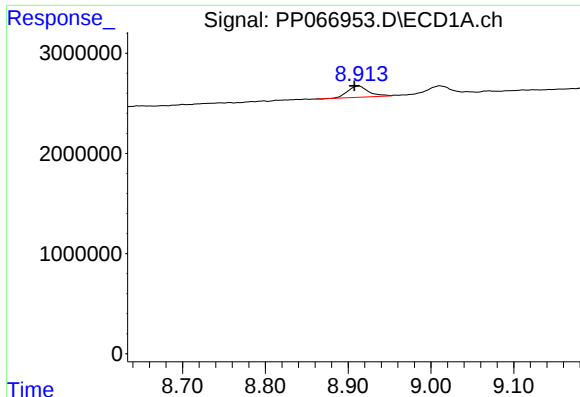

#41 AR-1268-1


R.T.: 8.912 min
Delta R.T.: 0.005 min
Response: 1964351
Conc: 15.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

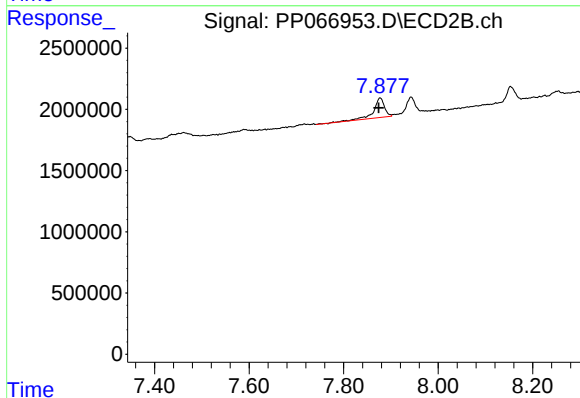


#41 AR-1268-1

R.T.: 7.877 min
Delta R.T.: 0.003 min
Response: 2555964
Conc: 20.43 ng/ml

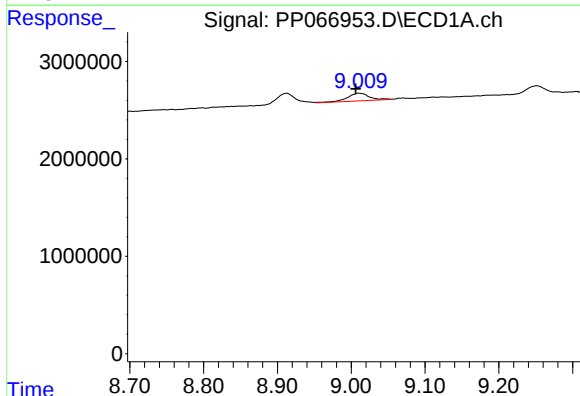


#42 AR-1268-2

R.T.: 9.011 min
Delta R.T.: 0.005 min
Response: 1652861
Conc: 14.12 ng/ml

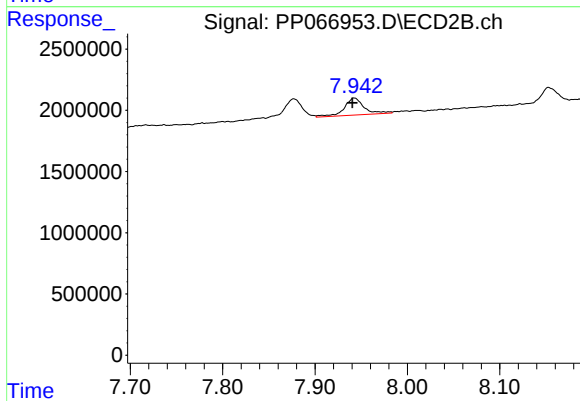

#42 AR-1268-2


R.T.: 7.943 min
Delta R.T.: 0.002 min
Response: 2072124
Conc: 18.54 ng/ml

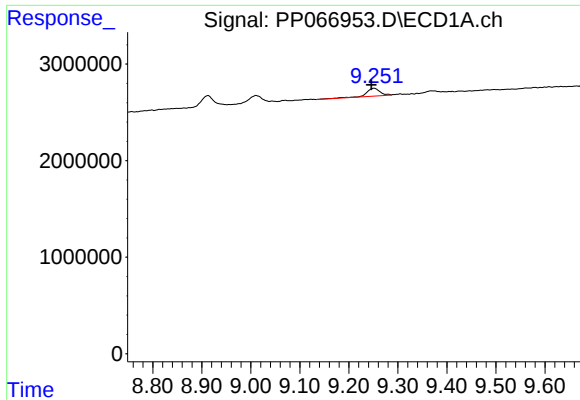

#43 AR-1268-3


R.T.: 9.251 min
Delta R.T.: 0.005 min
Response: 1570696
Conc: 15.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

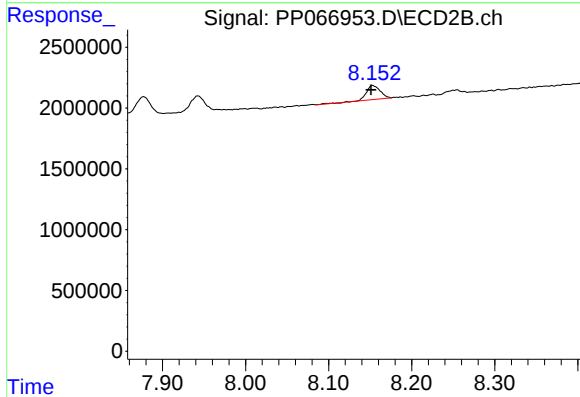


#43 AR-1268-3

R.T.: 8.153 min
Delta R.T.: 0.002 min
Response: 1327006
Conc: 12.98 ng/ml

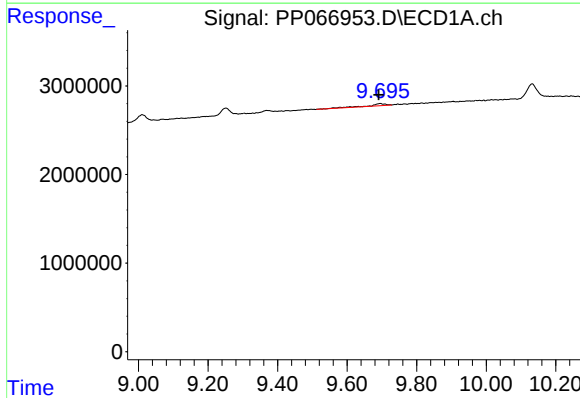


#44 AR-1268-4

R.T.: 9.695 min
Delta R.T.: 0.004 min
Response: 778398
Conc: 26.00 ng/ml

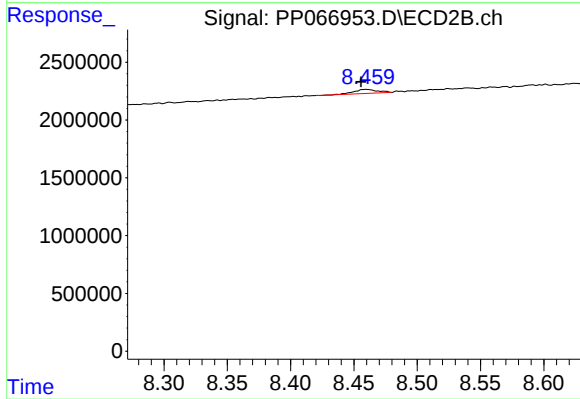

#44 AR-1268-4


R.T.: 8.459 min
Delta R.T.: 0.004 min
Response: 466162
Conc: 16.42 ng/ml

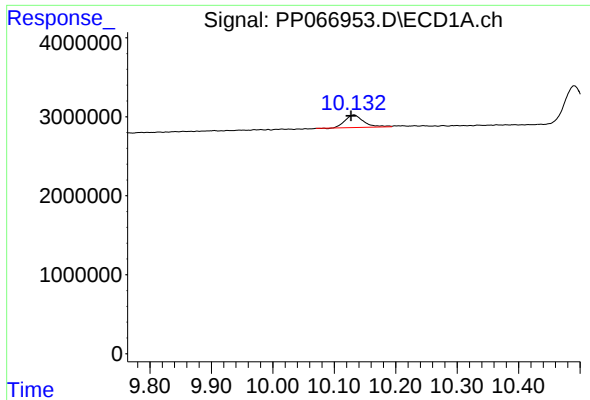

#45 AR-1268-5

R.T.: 10.132 min
Delta R.T.: 0.005 min
Response: 3332639
Conc: 11.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

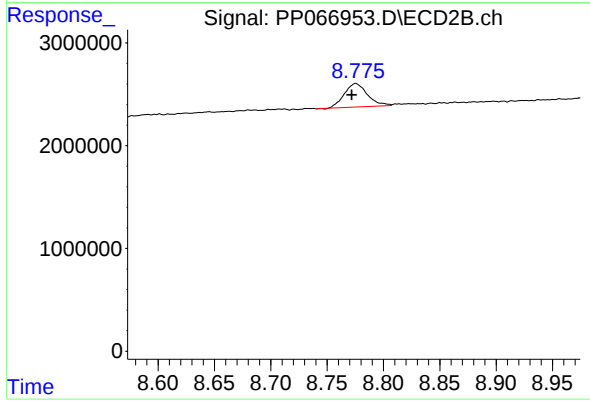

#45 AR-1268-5

R.T.: 8.775 min
Delta R.T.: 0.004 min
Response: 3249813
Conc: 13.25 ng/ml