

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
 Data File : PP066935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2024 09:43
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 04:27:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 09:05:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.623	3.910	34248137	27343036	20.347	19.075
2) SA Decachlor...	10.483	9.049	16309790	15448902	19.451	20.627

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
Data File : PP066935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2024 09:43
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 04:27:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 09:05:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

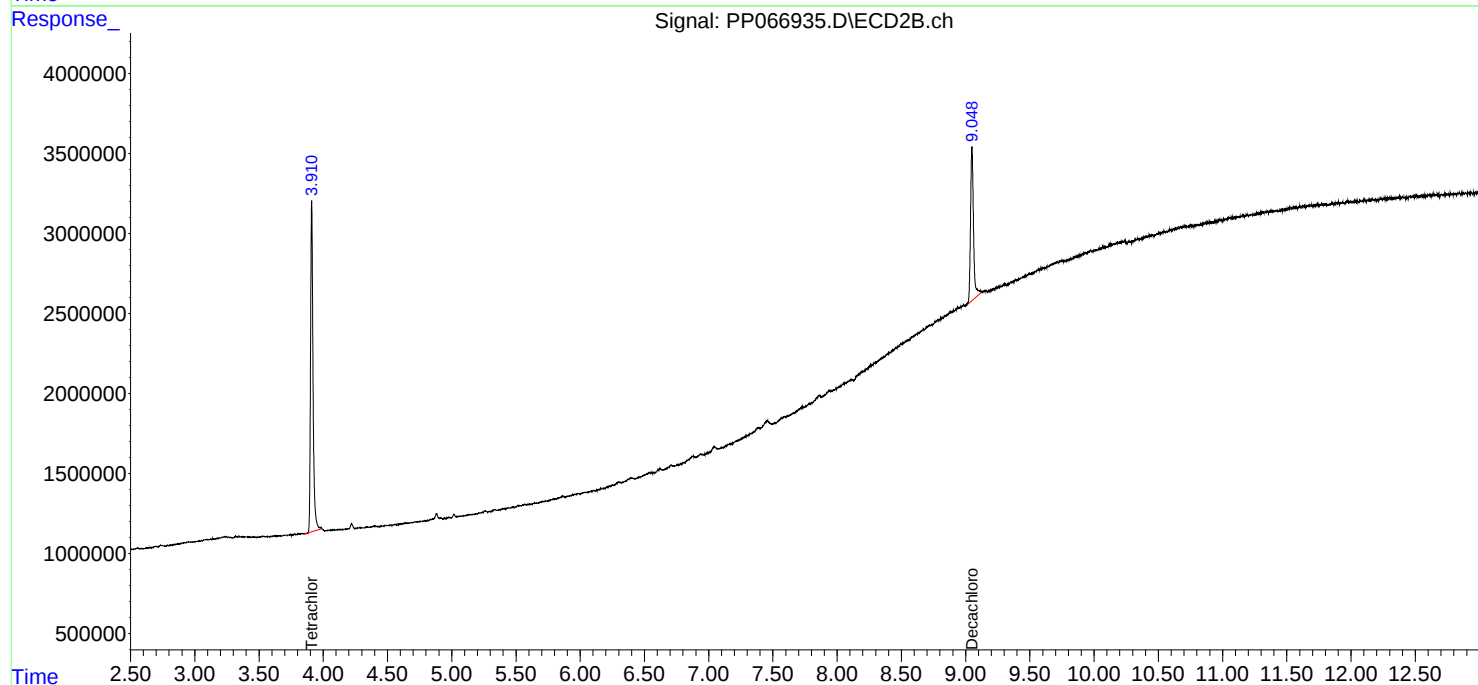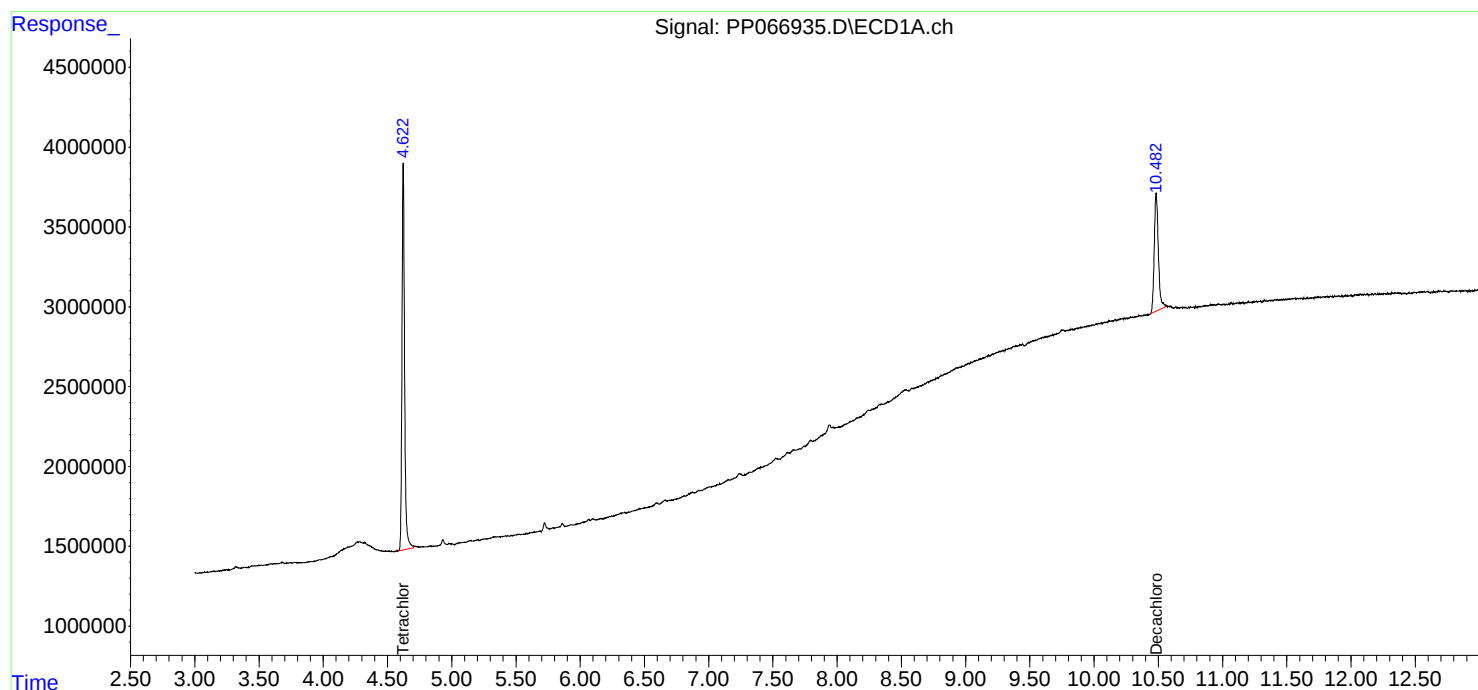


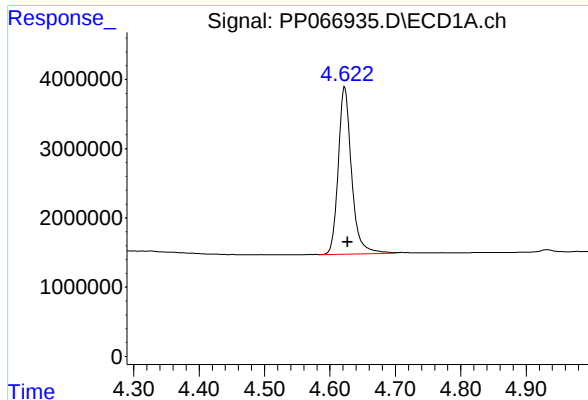

#1 Tetrachloro-m-xylene


R.T.: 4.623 min
Delta R.T.: -0.004 min
Response: 34248137
Conc: 20.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

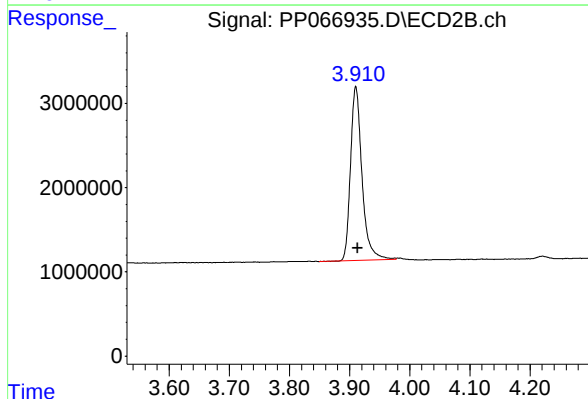


#1 Tetrachloro-m-xylene

R.T.: 3.910 min
Delta R.T.: -0.003 min
Response: 27343036
Conc: 19.08 ng/ml

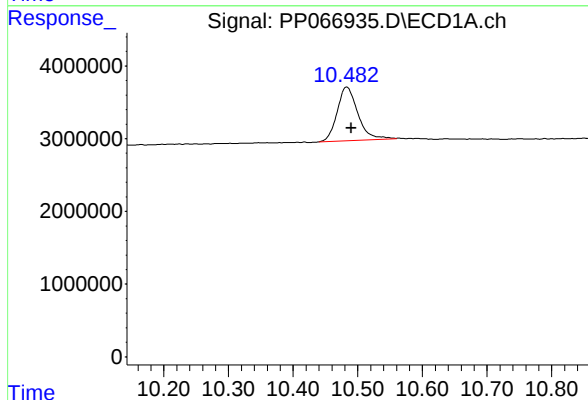

#2 Decachlorobiphenyl

R.T.: 10.483 min
Delta R.T.: -0.007 min
Response: 16309790
Conc: 19.45 ng/ml

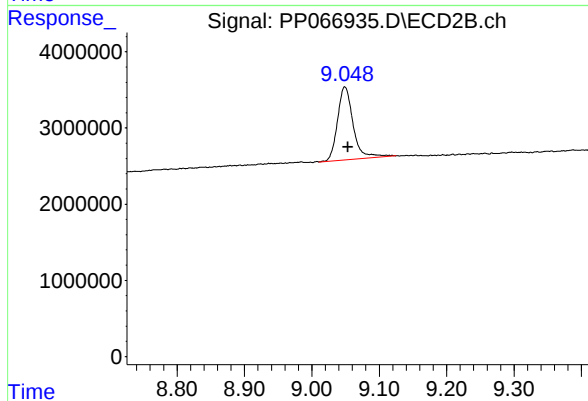

#2 Decachlorobiphenyl

R.T.: 9.049 min
Delta R.T.: -0.005 min
Response: 15448902
Conc: 20.63 ng/ml