

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
 Data File : PP066949.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2024 14:33
 Operator : YP\AJ
 Sample : P3390-09
 Misc : AR1242 MDL 25 PPB
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 04:36:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 09:05:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.627	3.914	30957553	25018544	18.392	17.454
2) SA Decachlor...	10.488	9.052	12763054	11725042	15.221	15.655
Target Compounds						
16) L4 AR-1242-1	5.802	5.022	856922	808192	24.912	26.016
17) L4 AR-1242-2	5.824	5.042	1445496	1162995	27.213	26.057
18) L4 AR-1242-3	5.885	5.223	965924	678755	28.167	28.137
19) L4 AR-1242-4	5.986	5.306	556995	723429	21.465	27.034 #
20) L4 AR-1242-5	6.722	5.837	599486	682153	25.800	24.441



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
Data File : PP066949.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2024 14:33
Operator : YP\AJ
Sample : P3390-09
Misc : AR1242 MDL 25 PPB
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 04:36:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 09:05:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

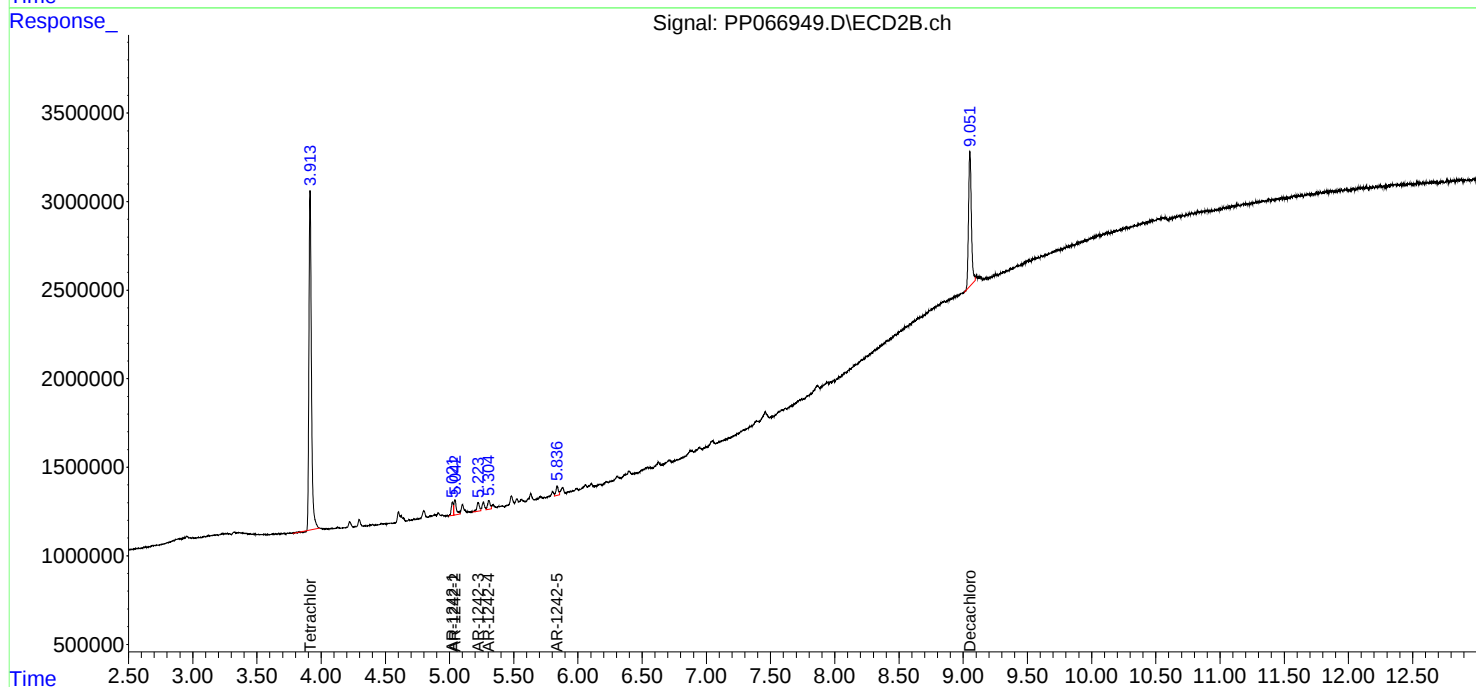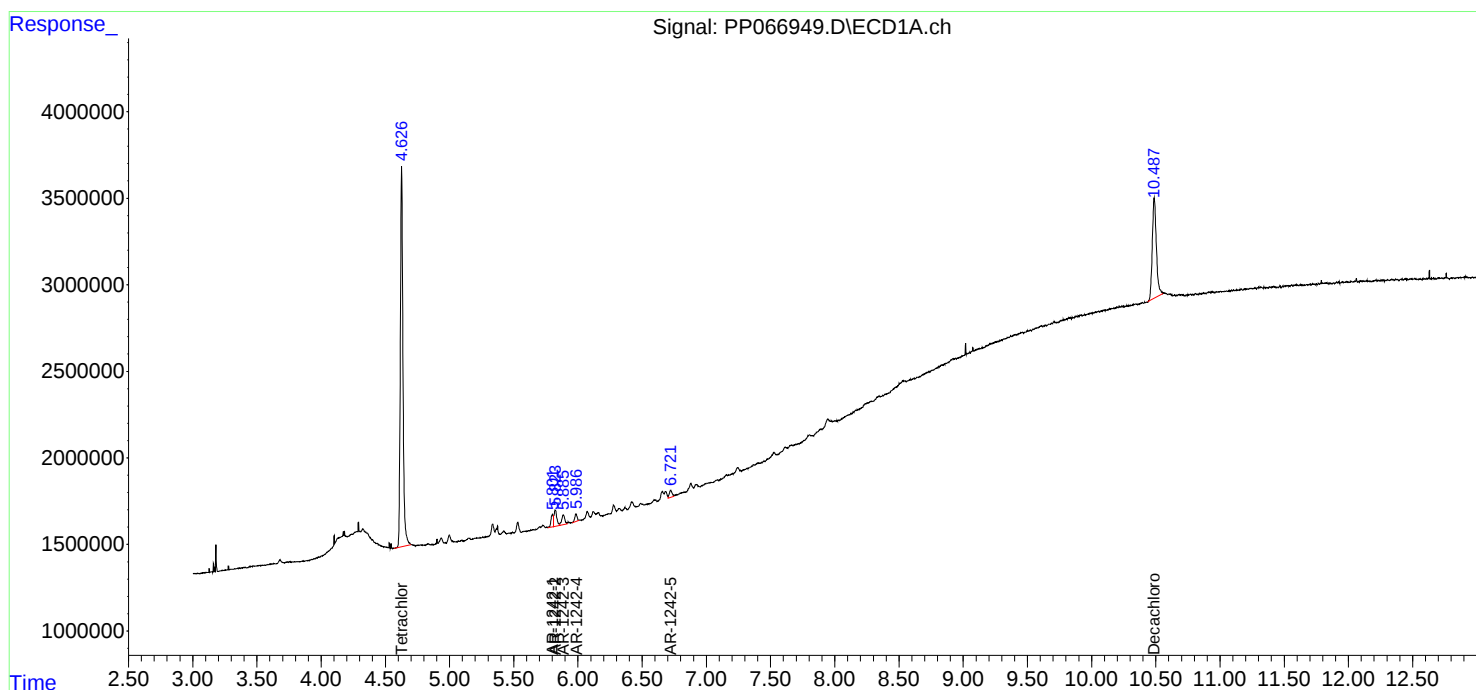


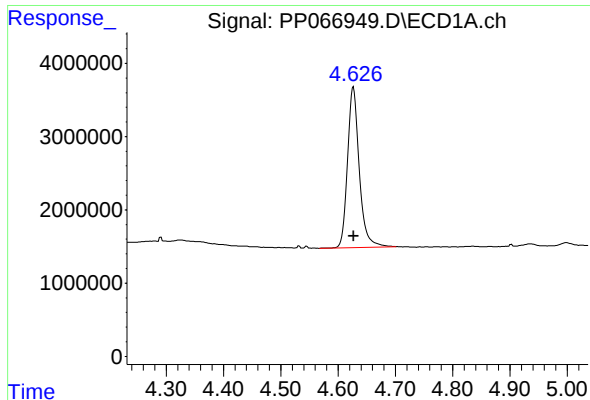

#1 Tetrachloro-m-xylene


R.T.: 4.627 min
Delta R.T.: 0.000 min
Response: 30957553
Conc: 18.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

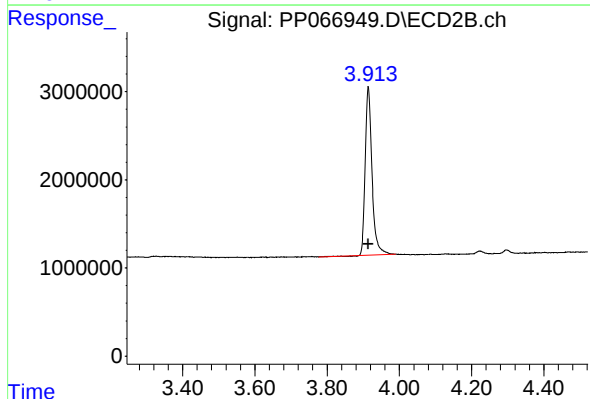


#1 Tetrachloro-m-xylene

R.T.: 3.914 min
Delta R.T.: 0.000 min
Response: 25018544
Conc: 17.45 ng/ml

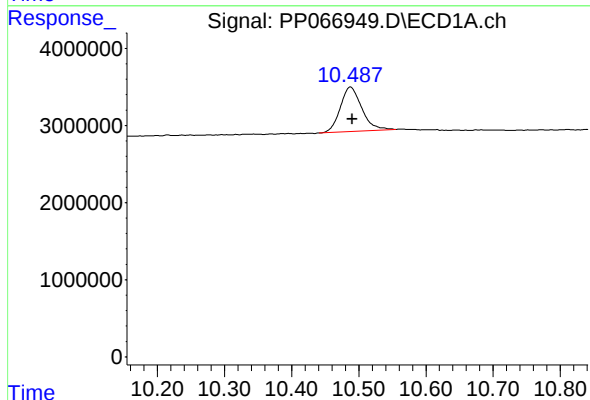


#2 Decachlorobiphenyl

R.T.: 10.488 min
Delta R.T.: -0.003 min
Response: 12763054
Conc: 15.22 ng/ml

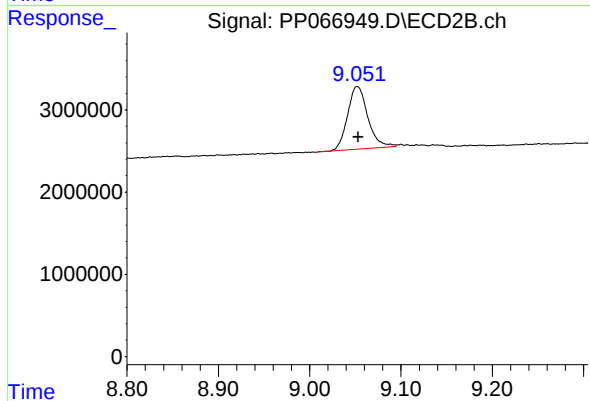

#2 Decachlorobiphenyl


R.T.: 9.052 min
Delta R.T.: -0.001 min
Response: 11725042
Conc: 15.65 ng/ml

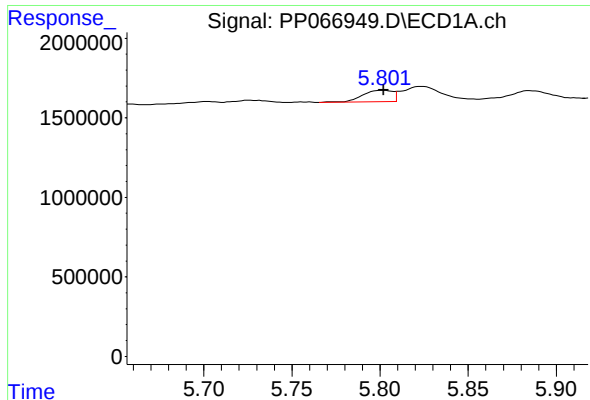

#16 AR-1242-1


R.T.: 5.802 min
Delta R.T.: 0.000 min
Response: 856922
Conc: 24.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

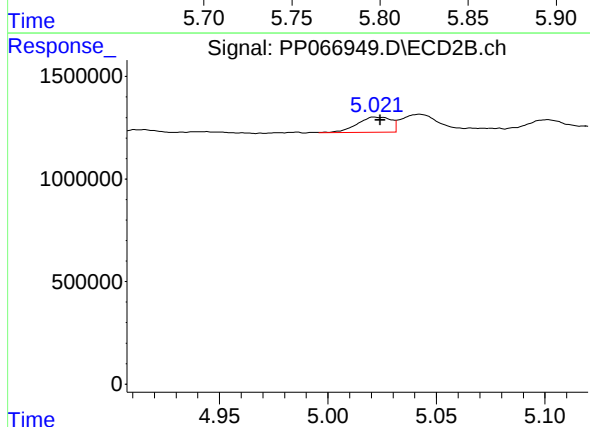


#16 AR-1242-1

R.T.: 5.022 min
Delta R.T.: -0.002 min
Response: 808192
Conc: 26.02 ng/ml

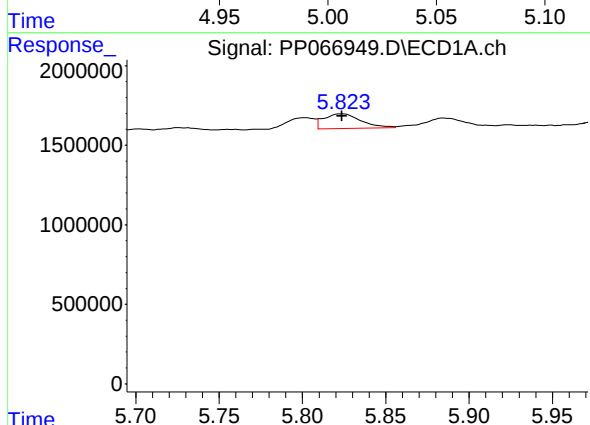


#17 AR-1242-2

R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 1445496
Conc: 27.21 ng/ml

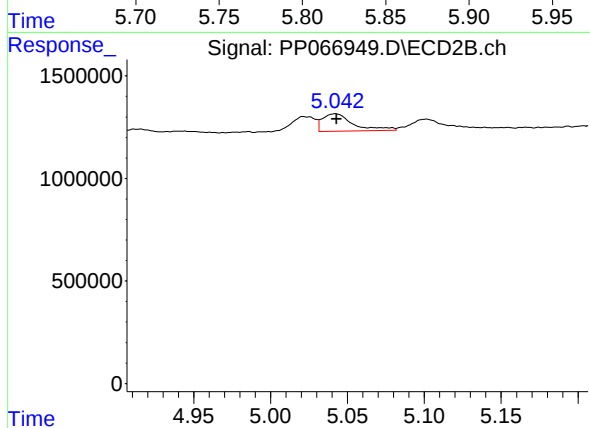

#17 AR-1242-2


R.T.: 5.042 min
Delta R.T.: 0.000 min
Response: 1162995
Conc: 26.06 ng/ml

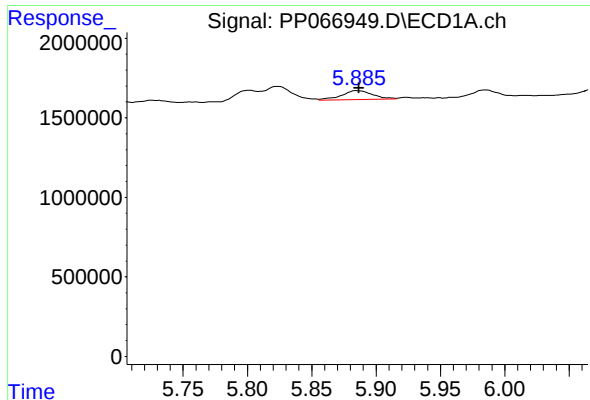

#18 AR-1242-3


R.T.: 5.885 min
Delta R.T.: -0.002 min
Response: 965924
Conc: 28.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

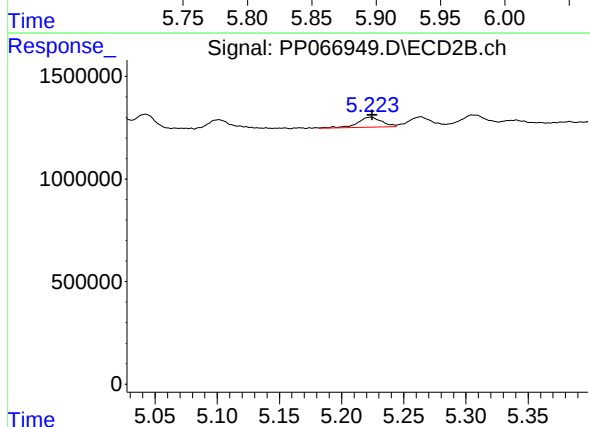


#18 AR-1242-3

R.T.: 5.223 min
Delta R.T.: -0.001 min
Response: 678755
Conc: 28.14 ng/ml

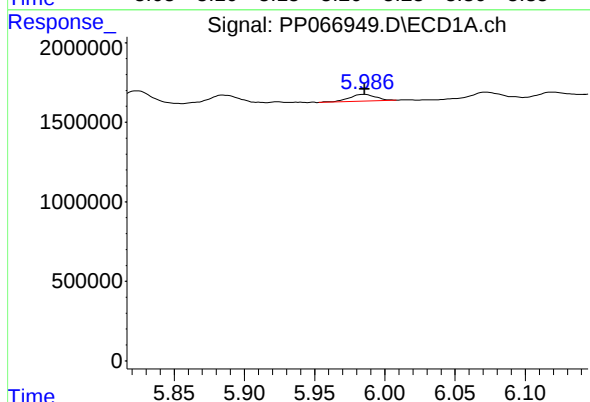


#19 AR-1242-4

R.T.: 5.986 min
Delta R.T.: 0.000 min
Response: 556995
Conc: 21.46 ng/ml

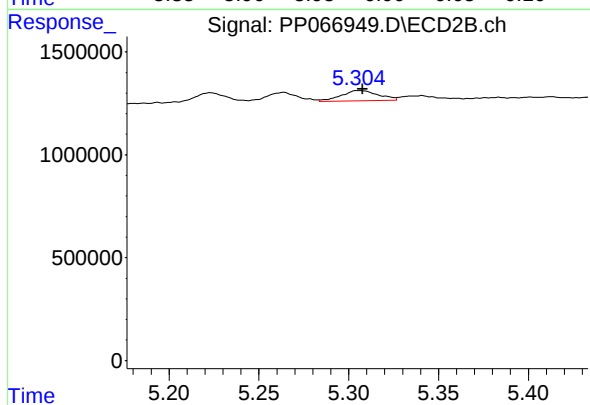

#19 AR-1242-4


R.T.: 5.306 min
Delta R.T.: -0.002 min
Response: 723429
Conc: 27.03 ng/ml

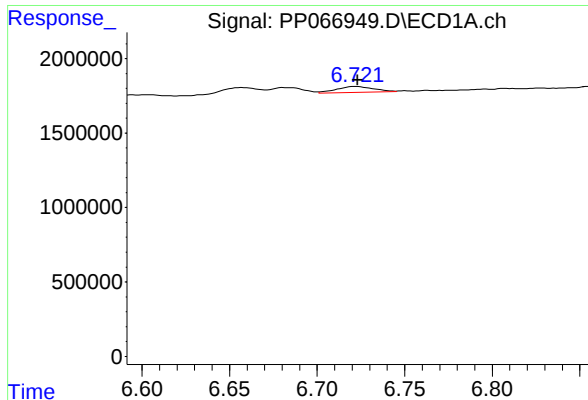

#20 AR-1242-5

R.T.: 6.722 min
Delta R.T.: 0.000 min
Response: 599486
Conc: 25.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2024

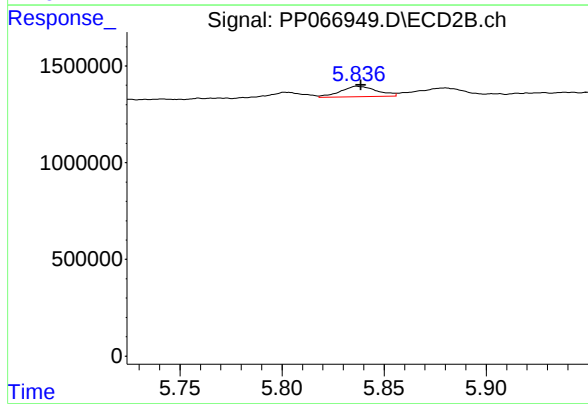

#20 AR-1242-5

R.T.: 5.837 min
Delta R.T.: -0.002 min
Response: 682153
Conc: 24.44 ng/ml