

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP082724\  
 Data File : PP067006.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 28 Aug 2024 10:26  
 Operator : YP\AJ  
 Sample : P3761-20  
 Misc :  
 ALS Vial : 54 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 PIPE-20

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 08/28/2024  
 Supervised By :Ankita Jodhani 08/28/2024

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Aug 28 14:35:32 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP082624.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Aug 27 09:05:47 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml     | ng/ml    |
|-----------------------------|--------|-------|----------|----------|-----------|----------|
| -----                       |        |       |          |          |           |          |
| System Monitoring Compounds |        |       |          |          |           |          |
| 1) SA Tetrachlo...          | 4.625  | 3.912 | 30840809 | 26551480 | 18.323    | 18.523m  |
| 2) SA Decachlor...          | 10.482 | 9.049 | 19982609 | 17704186 | 23.831    | 23.638   |
|                             |        |       |          |          |           |          |
| Target Compounds            |        |       |          |          |           |          |
| 26) L6 AR-1254-1            | 6.657  | 5.837 | 5697824  | 7087442  | 114.511   | 119.432  |
| 27) L6 AR-1254-2            | 6.872  | 5.985 | 30803439 | 19125678 | 436.085   | 365.001  |
| 28) L6 AR-1254-3            | 7.240  | 6.397 | 48972655 | 50261138 | 718.761   | 658.840  |
| 29) L6 AR-1254-4            | 7.525  | 6.626 | 59704688 | 49904744 | 1425.849  | 1321.107 |
| 30) L6 AR-1254-5            | 7.943  | 7.048 | 62122223 | 62214963 | 1182.255m | 988.523  |
| -----                       |        |       |          |          |           |          |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP082724\  
Data File : PP067006.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 28 Aug 2024 10:26  
Operator : YP\AJ  
Sample : P3761-20  
Misc :  
ALS Vial : 54 Sample Multiplier: 1



Instrument :  
ECD\_P  
ClientSampleId :  
PIPE-20


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/28/2024  
Supervised By :Ankita Jodhani 08/28/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 28 14:35:32 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP082624.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Aug 27 09:05:47 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

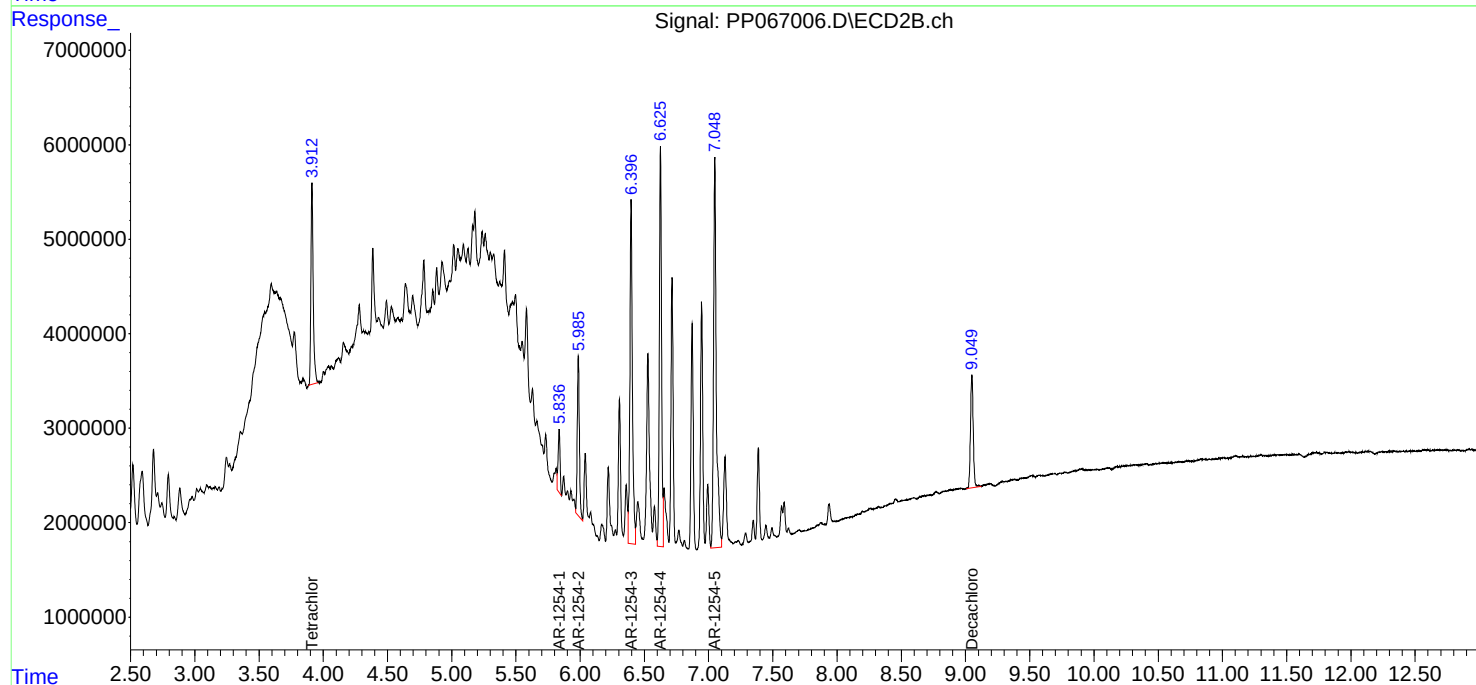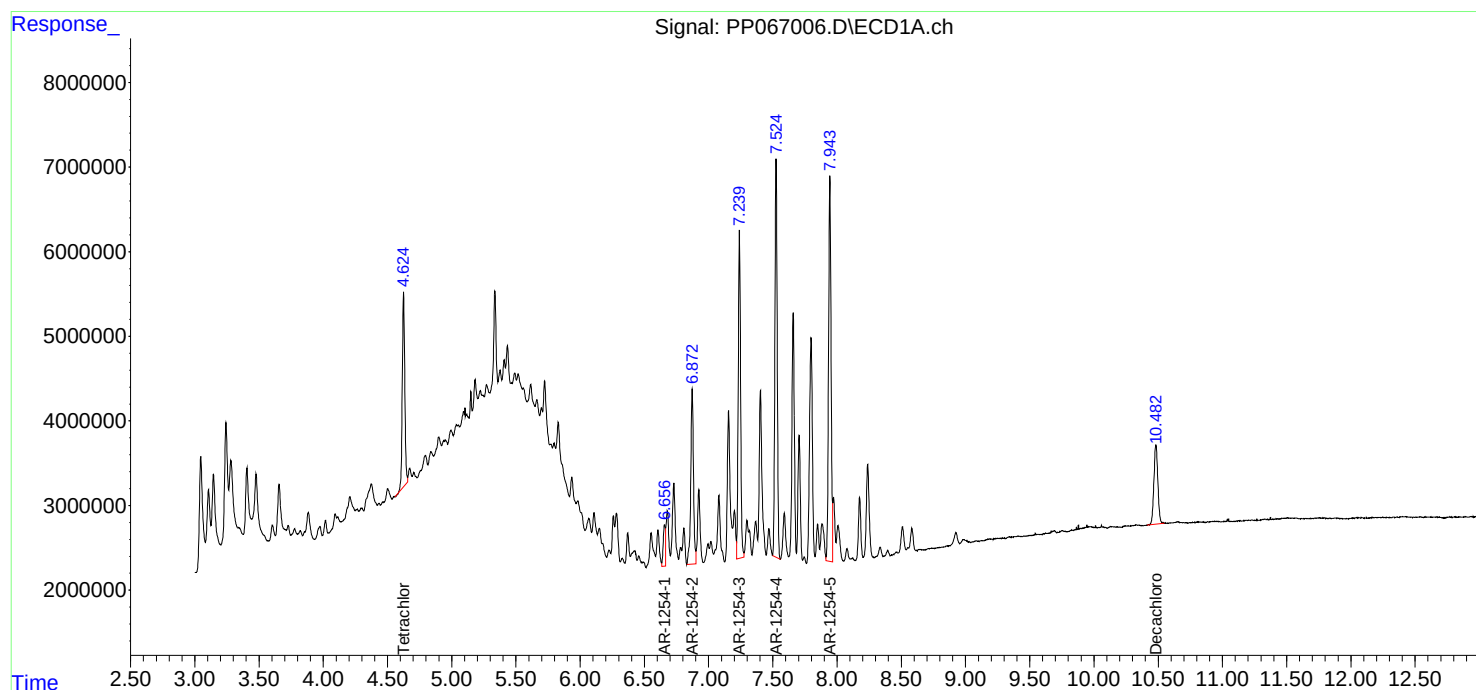

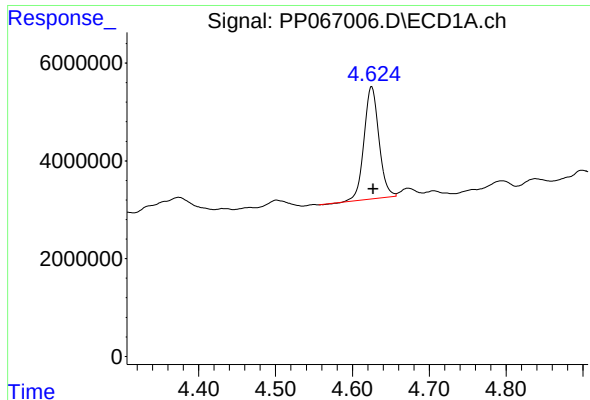


#1 Tetrachloro-m-xylene

R.T.: 4.625 min  
Delta R.T.: -0.002 min  
Response: 30840809  
Conc: 18.32 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PIPE-20


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/28/2024  
Supervised By :Ankita Jodhani 08/28/2024

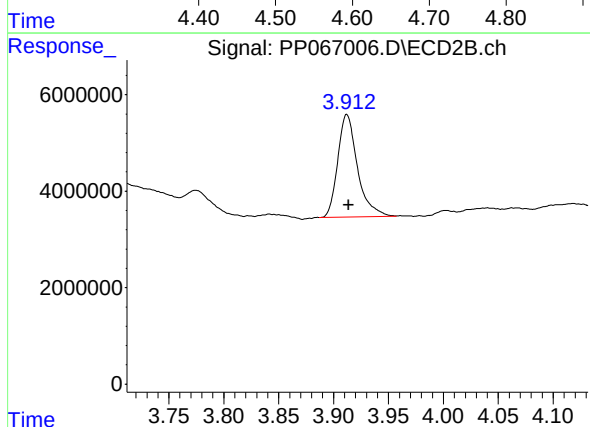


#1 Tetrachloro-m-xylene

R.T.: 3.912 min  
Delta R.T.: -0.002 min  
Response: 26551480  
Conc: 18.52 ng/ml

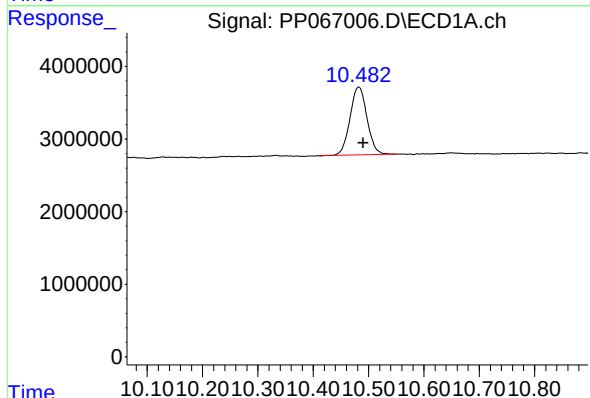


#2 Decachlorobiphenyl

R.T.: 10.482 min  
Delta R.T.: -0.008 min  
Response: 19982609  
Conc: 23.83 ng/ml

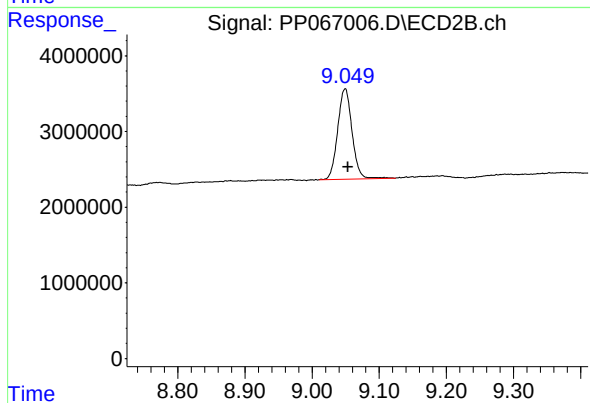

#2 Decachlorobiphenyl

R.T.: 9.049 min  
Delta R.T.: -0.004 min  
Response: 17704186  
Conc: 23.64 ng/ml

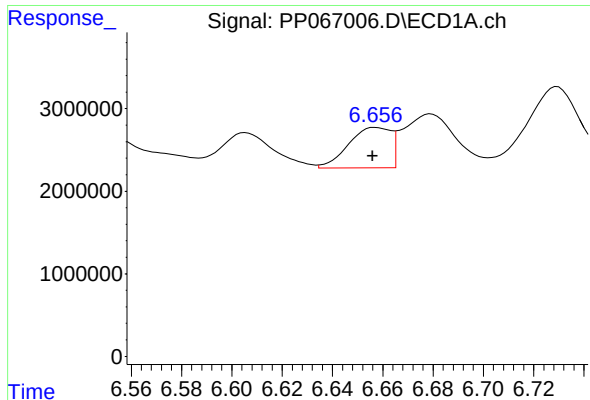


#26 AR-1254-1

R.T.: 6.657 min  
Delta R.T.: 0.001 min  
Response: 5697824  
Conc: 114.51 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PIPE-20


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/28/2024  
Supervised By :Ankita Jodhani 08/28/2024

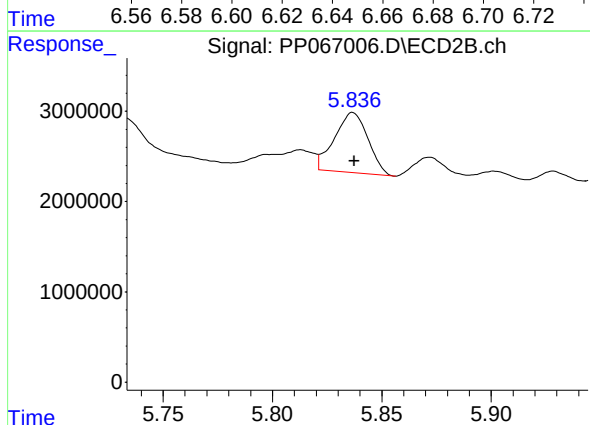


#26 AR-1254-1

R.T.: 5.837 min  
Delta R.T.: 0.000 min  
Response: 7087442  
Conc: 119.43 ng/ml

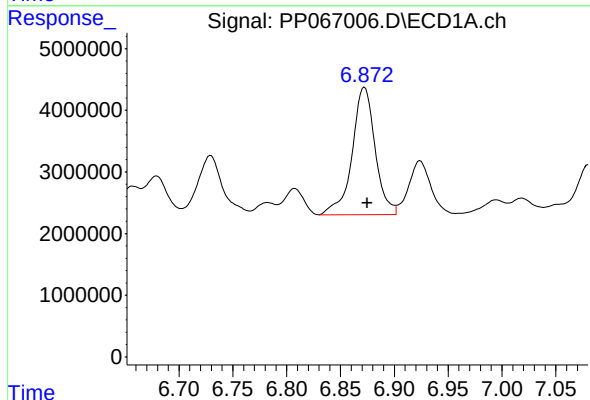


#27 AR-1254-2

R.T.: 6.872 min  
Delta R.T.: -0.003 min  
Response: 30803439  
Conc: 436.08 ng/ml

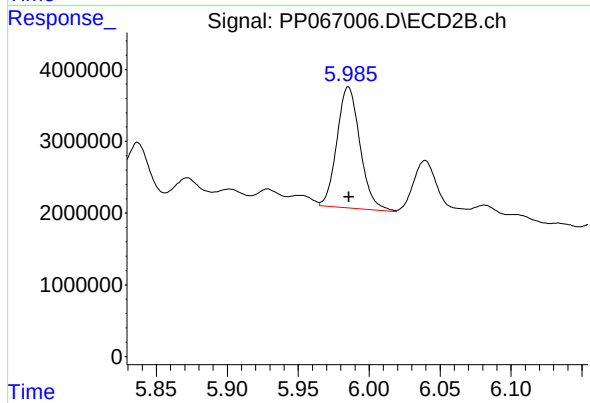

#27 AR-1254-2

R.T.: 5.985 min  
Delta R.T.: 0.000 min  
Response: 19125678  
Conc: 365.00 ng/ml

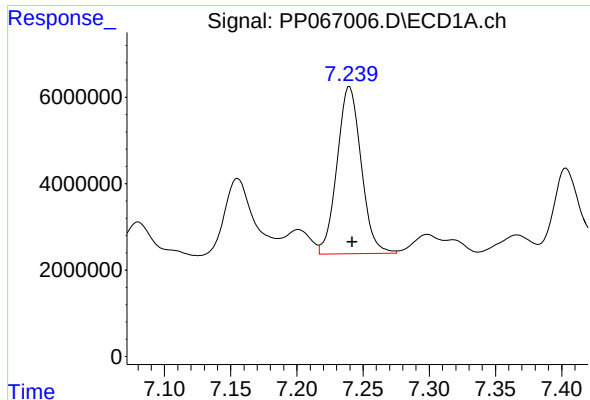


#28 AR-1254-3

R.T.: 7.240 min  
Delta R.T.: -0.002 min  
Response: 48972655  
Conc: 718.76 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PIPE-20


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/28/2024  
Supervised By :Ankita Jodhani 08/28/2024

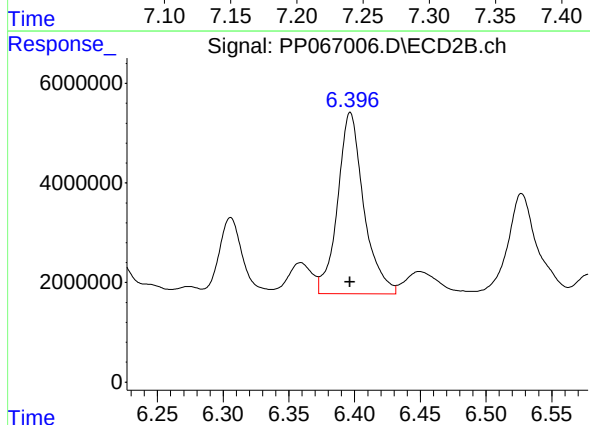


#28 AR-1254-3

R.T.: 6.397 min  
Delta R.T.: 0.000 min  
Response: 50261138  
Conc: 658.84 ng/ml

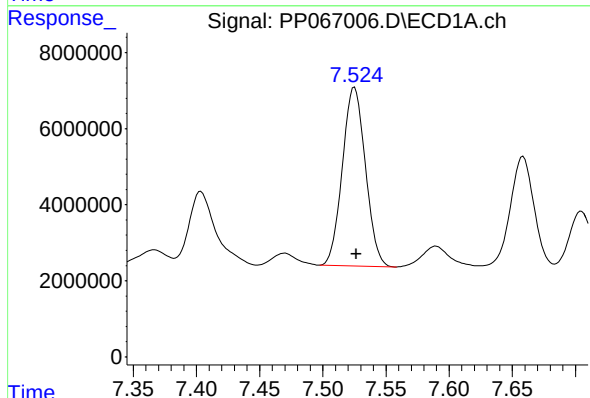


#29 AR-1254-4

R.T.: 7.525 min  
Delta R.T.: -0.001 min  
Response: 59704688  
Conc: 1425.85 ng/ml

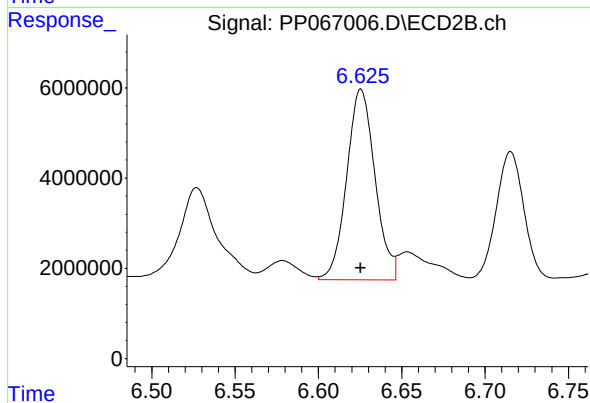

#29 AR-1254-4

R.T.: 6.626 min  
Delta R.T.: 0.000 min  
Response: 49904744  
Conc: 1321.11 ng/ml

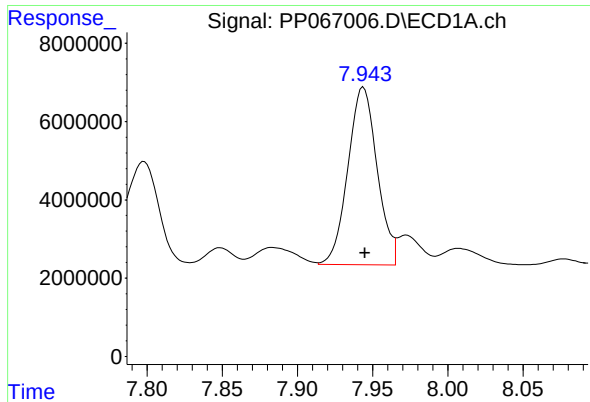


#30 AR-1254-5

R.T.: 7.943 min  
Delta R.T.: -0.002 min  
Response: 62122223  
Conc: 1182.25 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PIPE-20

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/28/2024  
Supervised By :Ankita Jodhani 08/28/2024

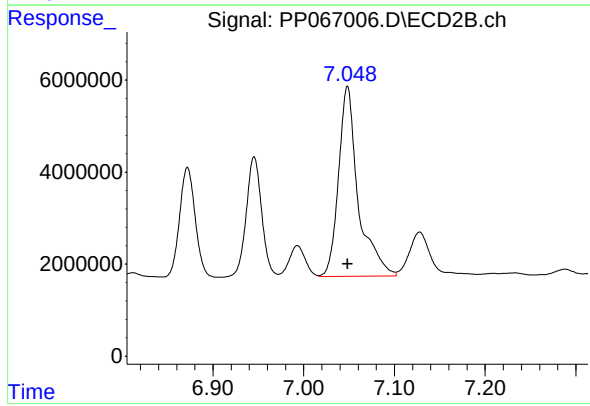

#30 AR-1254-5

R.T.: 7.048 min  
Delta R.T.: 0.000 min  
Response: 62214963  
Conc: 988.52 ng/ml