

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
 Data File : PP067007.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2024 10:42
 Operator : YP\AJ
 Sample : P3761-21
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PIPE-21

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/28/2024
 Supervised By :Ankita Jodhani 08/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 14:36:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 09:05:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.626	3.913	33684315	29210187	20.012	20.378
2) SA Decachlor...	10.485	9.050	19150395	17993792	22.838	24.024
Target Compounds						
26) L6 AR-1254-1	6.675	5.837	1998036	415442	40.155	7.001 #
27) L6 AR-1254-2	6.872	5.986	2591656	1551886	36.690m	29.617
28) L6 AR-1254-3	7.241	6.396	3627236	4394631	53.236	57.606
29) L6 AR-1254-4	7.526	6.626	4824800	4020807	115.224	106.441
30) L6 AR-1254-5	7.943	7.048	7966986	8882294	151.621m	141.129

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082724\
Data File : PP067007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2024 10:42
Operator : YP\AJ
Sample : P3761-21
Misc :
ALS Vial : 55 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PIPE-21


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/28/2024
Supervised By :Ankita Jodhani 08/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 14:36:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 09:05:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

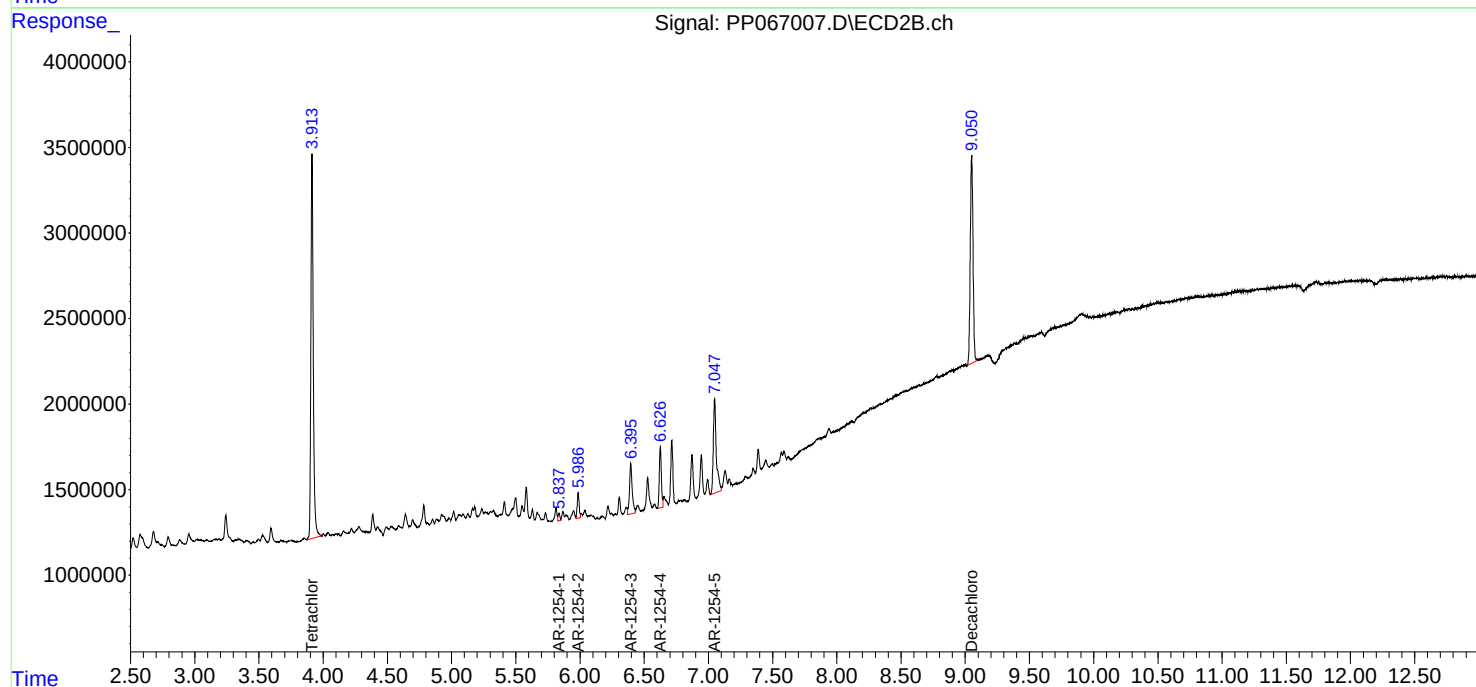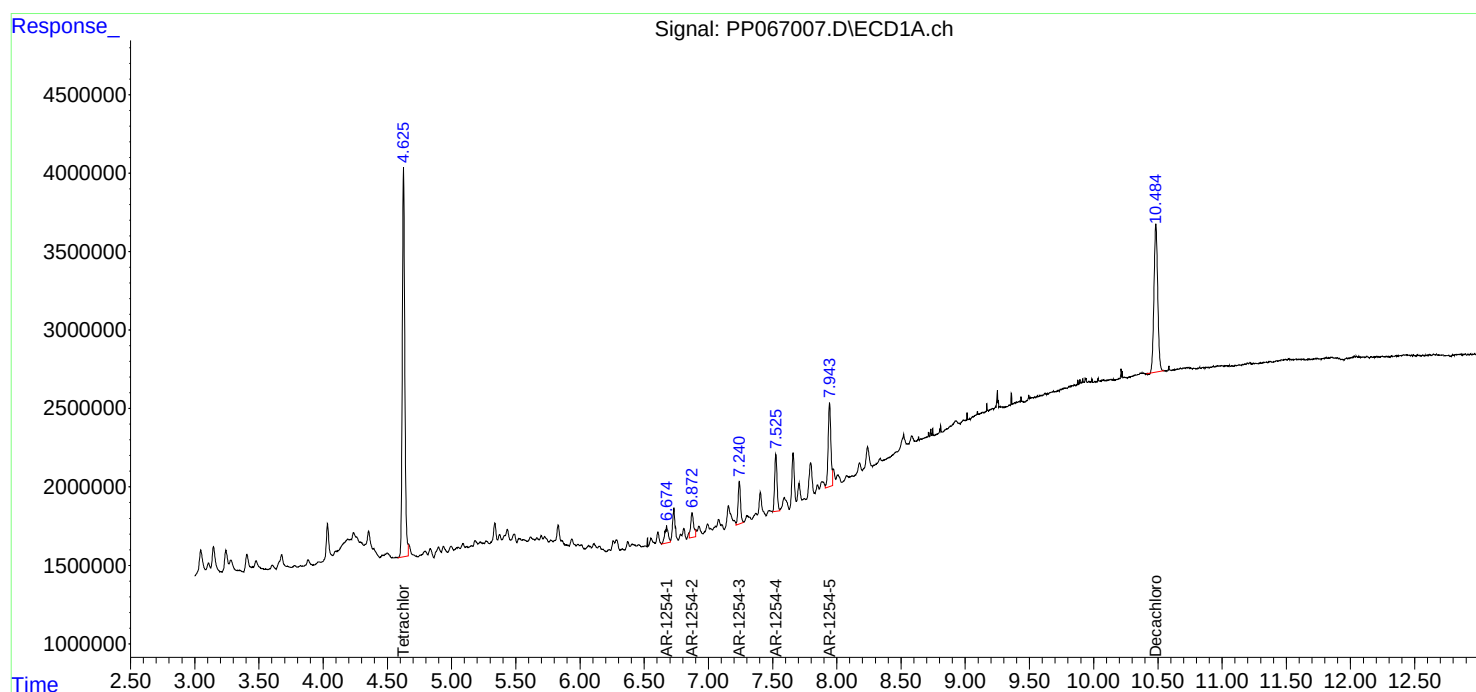

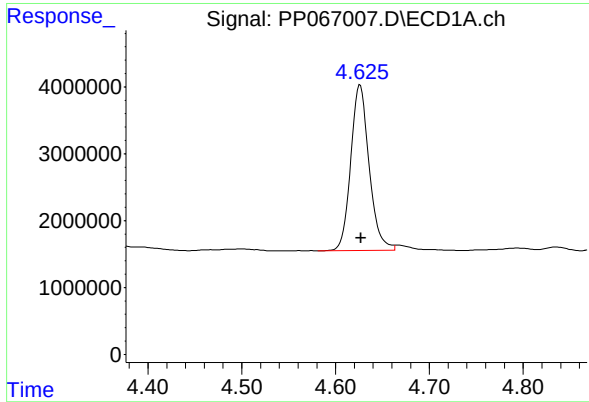


#1 Tetrachloro-m-xylene

R.T.: 4.626 min
Delta R.T.: 0.000 min
Response: 33684315
Conc: 20.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
PIPE-21


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/28/2024
Supervised By :Ankita Jodhani 08/28/2024

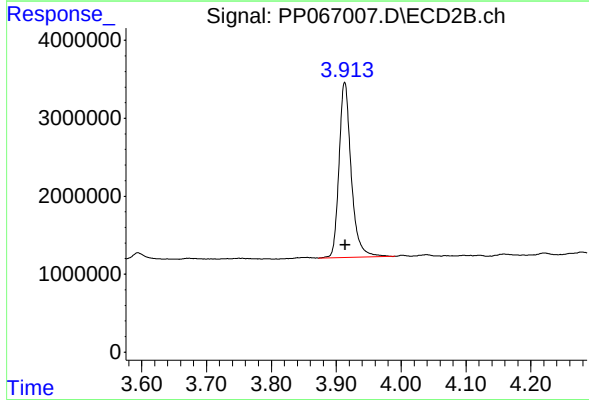


#1 Tetrachloro-m-xylene

R.T.: 3.913 min
Delta R.T.: 0.000 min
Response: 29210187
Conc: 20.38 ng/ml

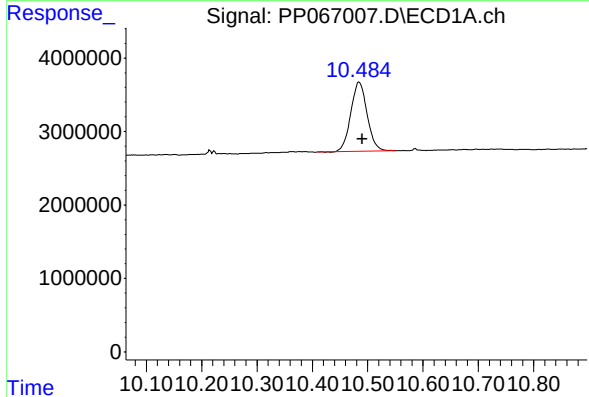


#2 Decachlorobiphenyl

R.T.: 10.485 min
Delta R.T.: -0.006 min
Response: 19150395
Conc: 22.84 ng/ml

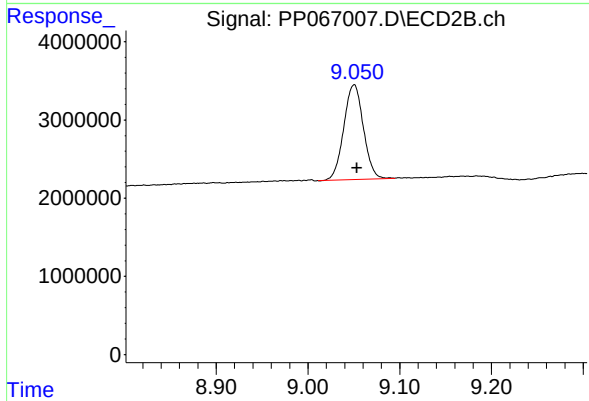

#2 Decachlorobiphenyl

R.T.: 9.050 min
Delta R.T.: -0.003 min
Response: 17993792
Conc: 24.02 ng/ml

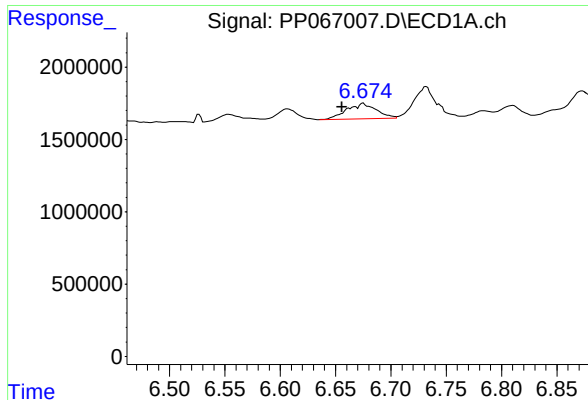


#26 AR-1254-1

R.T.: 6.675 min
Delta R.T.: 0.019 min
Response: 1998036
Conc: 40.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
PIPE-21


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/28/2024
Supervised By :Ankita Jodhani 08/28/2024

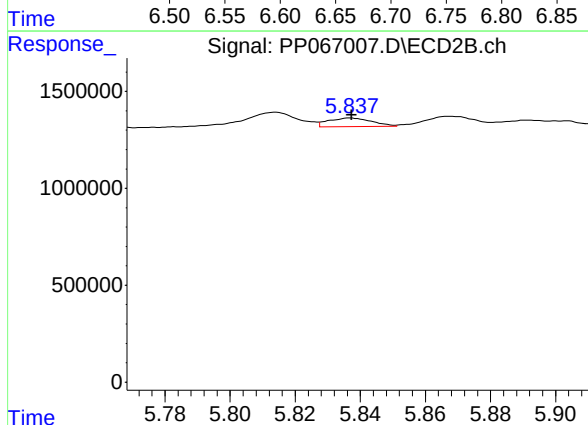


#26 AR-1254-1

R.T.: 5.837 min
Delta R.T.: 0.000 min
Response: 415442
Conc: 7.00 ng/ml

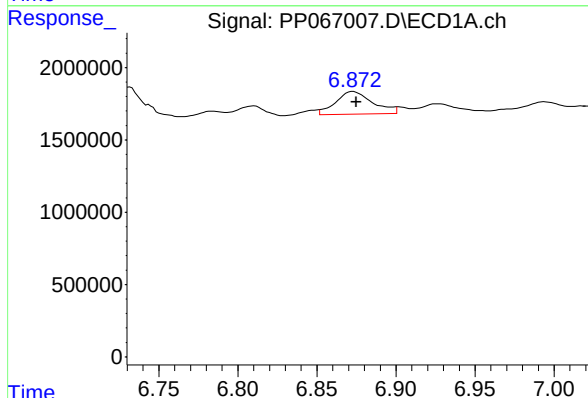


#27 AR-1254-2

R.T.: 6.872 min
Delta R.T.: -0.003 min
Response: 2591656
Conc: 36.69 ng/ml m

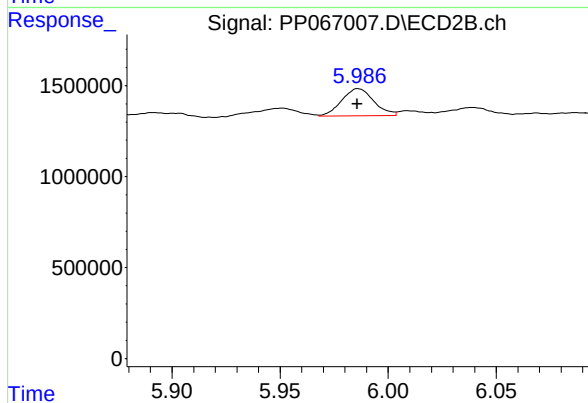

#27 AR-1254-2

R.T.: 5.986 min
Delta R.T.: 0.000 min
Response: 1551886
Conc: 29.62 ng/ml

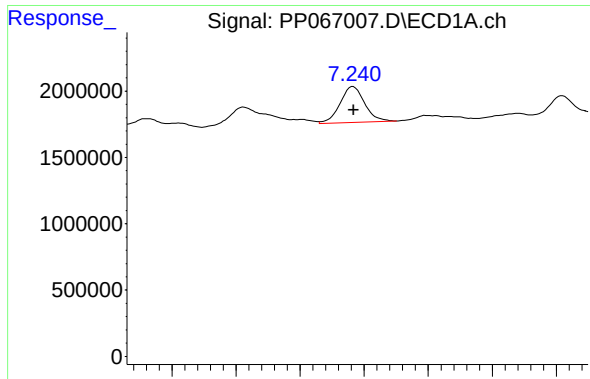


#28 AR-1254-3

R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 3627236
Conc: 53.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
PIPE-21


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/28/2024
Supervised By :Ankita Jodhani 08/28/2024

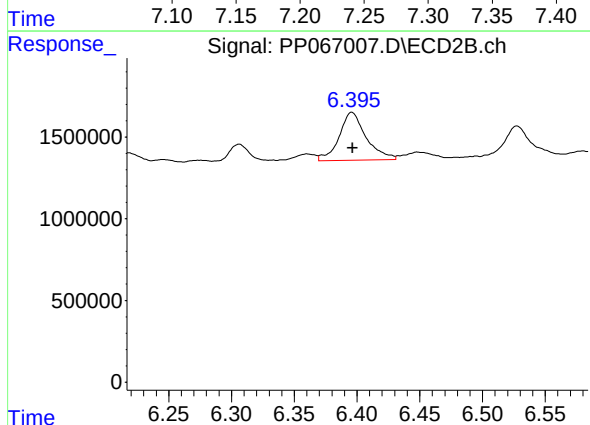


#28 AR-1254-3

R.T.: 6.396 min
Delta R.T.: 0.000 min
Response: 4394631
Conc: 57.61 ng/ml

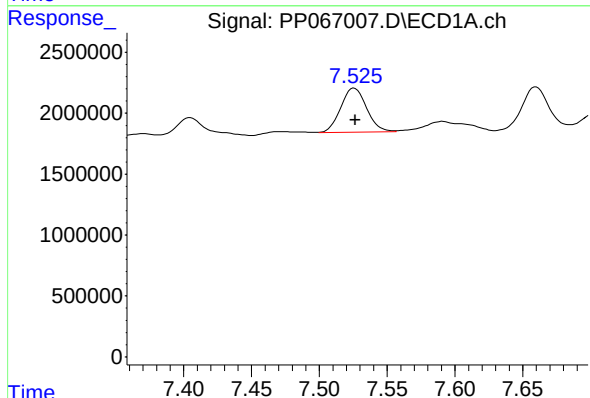


#29 AR-1254-4

R.T.: 7.526 min
Delta R.T.: 0.000 min
Response: 4824800
Conc: 115.22 ng/ml

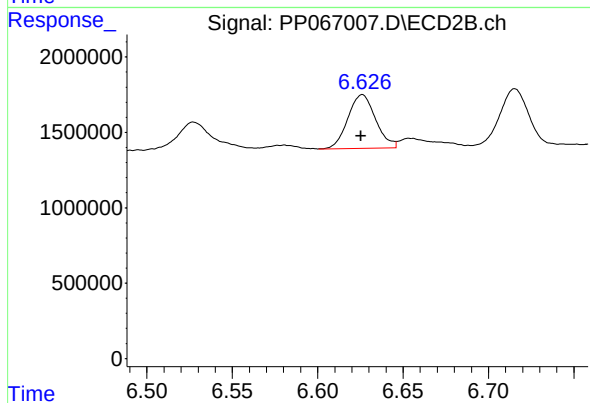

#29 AR-1254-4

R.T.: 6.626 min
Delta R.T.: 0.000 min
Response: 4020807
Conc: 106.44 ng/ml

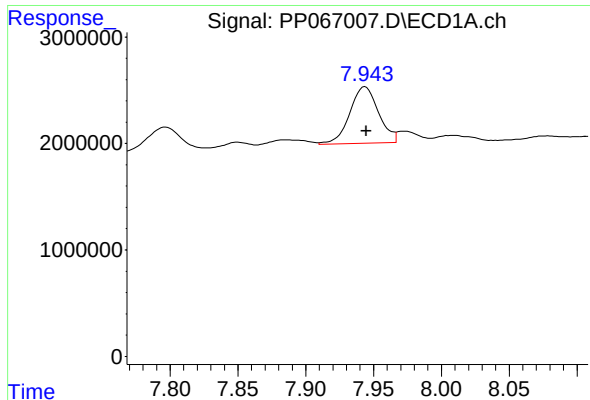


#30 AR-1254-5

R.T.: 7.943 min
Delta R.T.: -0.002 min
Response: 7966986
Conc: 151.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
PIPE-21

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/28/2024
Supervised By :Ankita Jodhani 08/28/2024

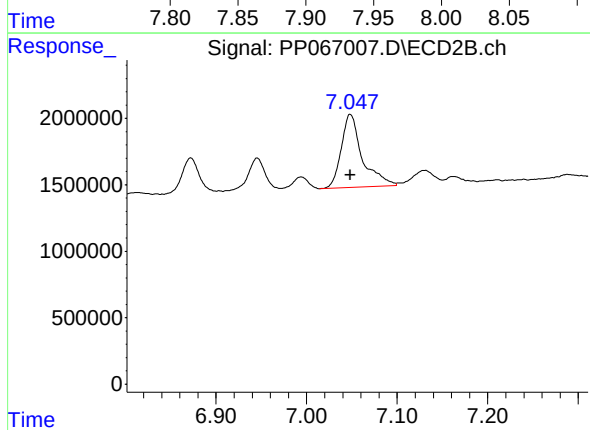

#30 AR-1254-5

R.T.: 7.048 min
Delta R.T.: 0.000 min
Response: 8882294
Conc: 141.13 ng/ml