

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082725\
 Data File : PP074668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2025 10:36
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 13:56:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.688f	3.804	336401	90801	0.275	0.019 #
2)	SA Decachlor...	0.000	8.812	0	809740	N.D.	0.108 #
Target Compounds							
3)	L1 AR-1016-1	5.786	4.898	94593	356553	2.146	0.700 #
4)	L1 AR-1016-2	5.786f	4.949	94593	924536	1.505	3.884 #
5)	L1 AR-1016-3	5.905	5.071	364491	778708	8.115	5.647 #
6)	L1 AR-1016-4	5.940f	5.133	411270	1961470	11.690	14.030
7)	L1 AR-1016-5	0.000	5.341	0	1779728	N.D.	10.716 #
8)	L2 AR-1221-1	4.898f	4.014	127654	297521	7.256	4.809 #
9)	L2 AR-1221-2	4.898f	4.094	127654	152660	9.557	3.377 #
10)	L2 AR-1221-3	5.059f	4.168	517875	85752	13.660	0.522 #
11)	L3 AR-1232-1	5.059f	4.168	517875	85752	17.050	0.669 #
12)	L3 AR-1232-2	5.603f	4.898	292372	356553	18.554	1.538 #
13)	L3 AR-1232-3	5.786f	5.071	94593	778708	3.097	12.966 #
14)	L3 AR-1232-4	5.940f	5.156	411270	1149148	23.815	15.591 #
15)	L3 AR-1232-5	6.110	5.341	555016	1779728	42.756	28.667 #
16)	L4 AR-1242-1	5.786	4.898	94593	356553	2.471	0.845 #
17)	L4 AR-1242-2	5.786f	4.949	94593	924536	1.675	4.616 #
18)	L4 AR-1242-3	5.905	5.071	364491	778708	8.977	6.583 #
19)	L4 AR-1242-4	5.940f	5.156	411270	1149148	12.957	6.714 #
20)	L4 AR-1242-5	6.724	5.675	380491	1208508	10.548	6.527 #
21)	L5 AR-1248-1	5.786	4.898	94593	356553	3.130	1.291 #
22)	L5 AR-1248-2	6.110	5.133	555016	1961470	12.879	11.097
23)	L5 AR-1248-3	6.347f	5.156	133641	1149148	2.861	5.058 #
24)	L5 AR-1248-4	6.654	5.341	3422620	1779728	62.229	8.163 #
25)	L5 AR-1248-5	6.724	5.703	380491	8040004	6.859	21.888 #
26)	L6 AR-1254-1	6.654	5.675	3422620	1208508	58.738	2.535 #
27)	L6 AR-1254-2	6.868	5.820	2009763	1059029	24.625	3.007 #
28)	L6 AR-1254-3	7.230	6.244	6293801	30806415	70.553	49.703 #
29)	L6 AR-1254-4	7.517	6.458	377623	2802068	5.729	5.979
30)	L6 AR-1254-5	7.952	6.874	513.3E6	3819.3E6	6177.792	7786.589 #
31)	L7 AR-1260-1	7.401	6.351	92500	3784498	1.600	10.086 #
32)	L7 AR-1260-2	7.637	6.518	564.2E6	17224559	8185.911	32.572 #
33)	L7 AR-1260-3	7.952f	6.771f	513.3E6	132225	9892.629	0.305 #
34)	L7 AR-1260-4	8.221	7.180	285086	173502	4.469	0.455 #
35)	L7 AR-1260-5	8.561	7.409	242889	539898	2.142	0.537 #
36)	L8 AR-1262-1	8.221	6.874f	285086	3819.3E6	3.702	5400.187 #
37)	L8 AR-1262-2	8.561	7.180	242889	173502	1.835	0.333 #
38)	L8 AR-1262-3	8.897	7.712	63238	60358966	0.651	129.443 #
39)	L8 AR-1262-4	0.000	7.712f	0	60358966	N.D.	73.442 #
40)	L8 AR-1262-5	9.647	8.256	94566	238842	1.551	0.667 #
41)	L9 AR-1268-1	8.897	7.712	63238	60358966	0.390	42.793 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082725\
 Data File : PP074668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2025 10:36
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 13:56:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.712f	0	60358966	N.D.	44.270 #
43) L9	AR-1268-3	9.156f	7.978	268668	733931	2.174	0.704 #
44) L9	AR-1268-4	9.647	8.256	94566	238842	1.406	0.623 #
45) L9	AR-1268-5	0.000	8.561	0	248071	N.D.	0.079 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082725\
Data File : PP074668.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2025 10:36
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 13:56:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

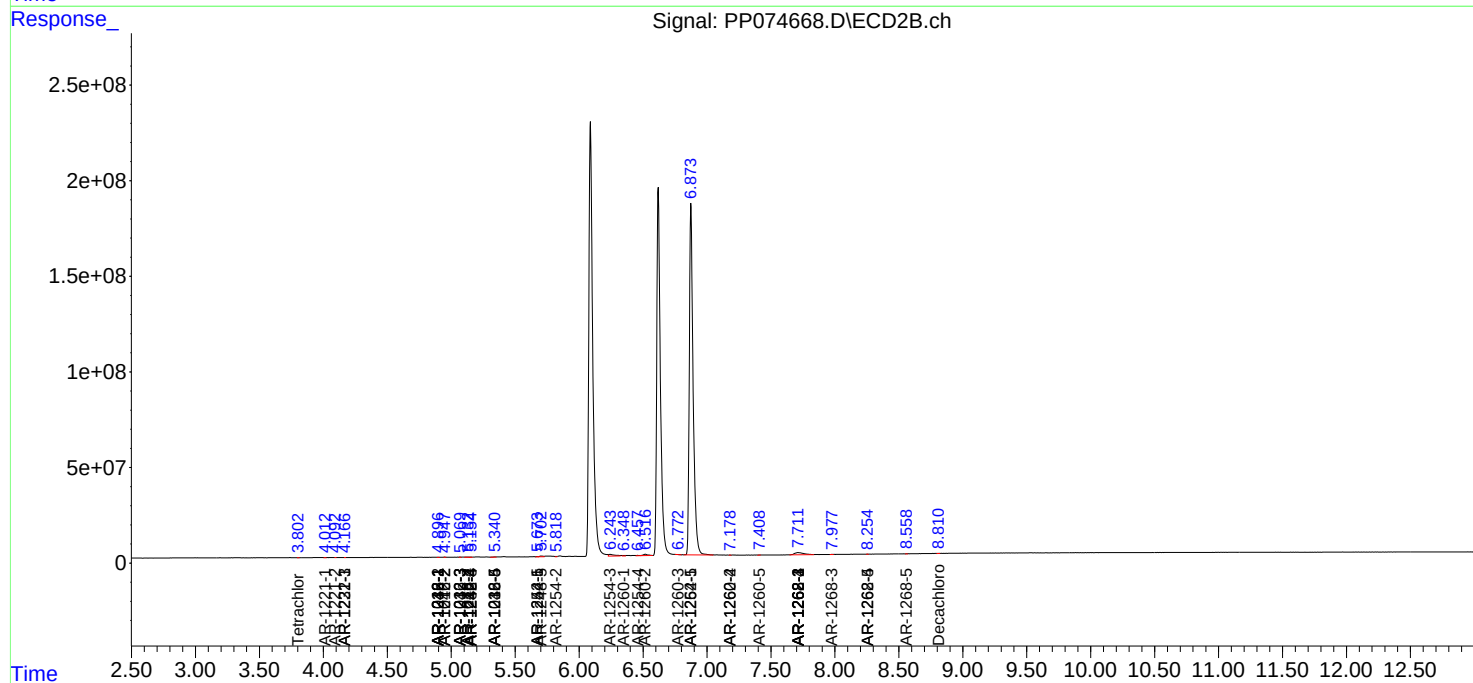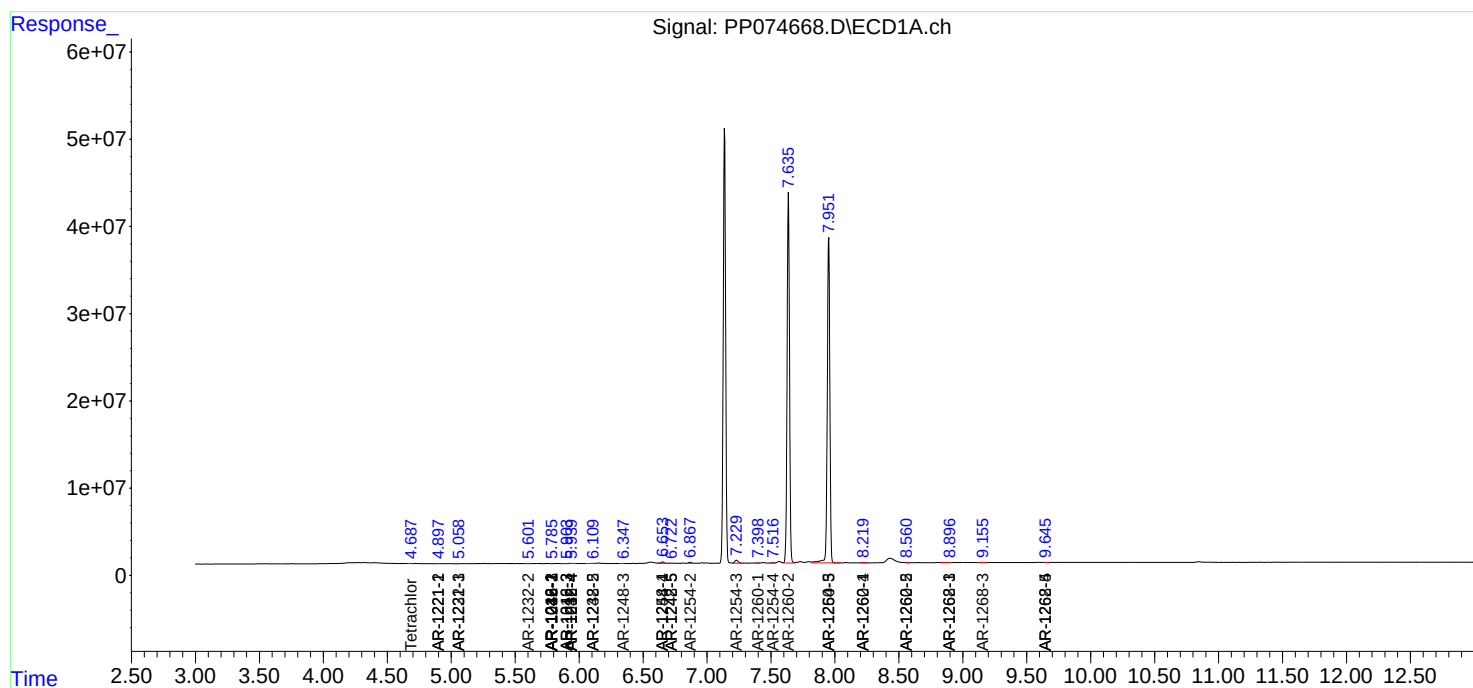


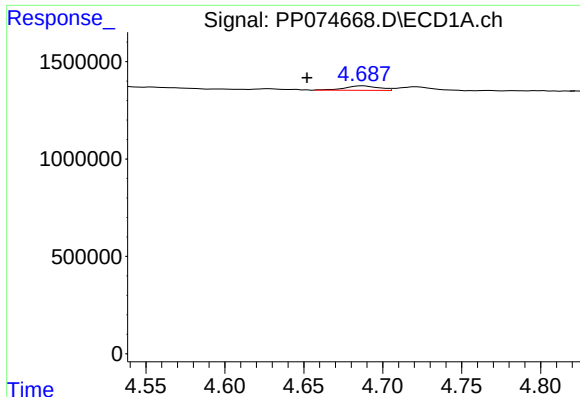

#1 Tetrachloro-m-xylene


R.T.: 4.688 min
Delta R.T.: 0.036 min
Response: 336401
Conc: 0.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

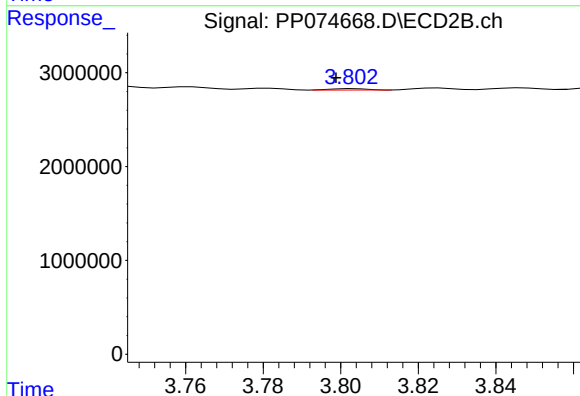


#1 Tetrachloro-m-xylene

R.T.: 3.804 min
Delta R.T.: 0.005 min
Response: 90801
Conc: 0.02 ng/ml

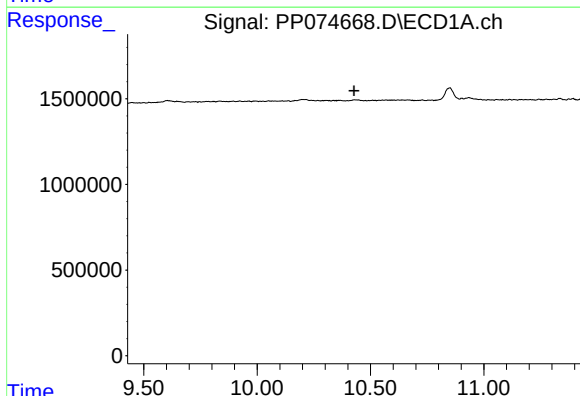


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.428 min
Response: 0
Conc: N.D.

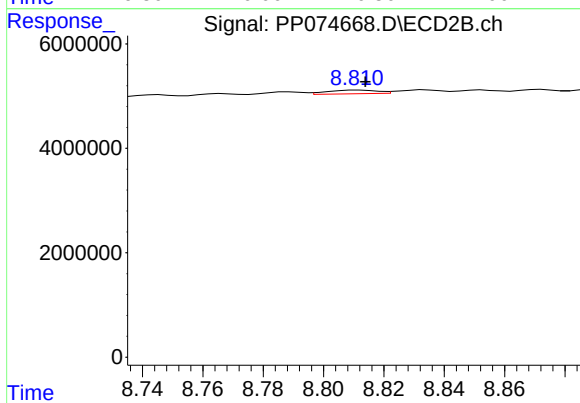

#2 Decachlorobiphenyl


R.T.: 8.812 min
Delta R.T.: -0.002 min
Response: 809740
Conc: 0.11 ng/ml

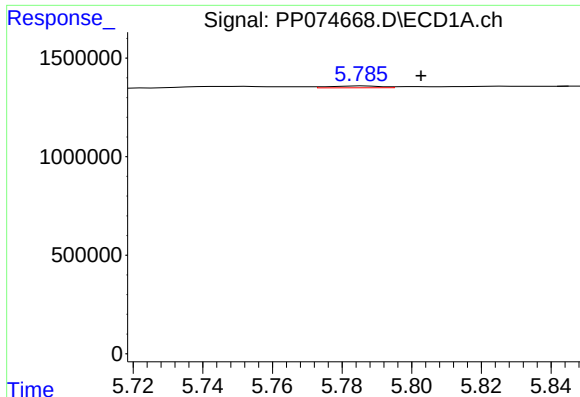

#3 AR-1016-1


R.T.: 5.786 min
Delta R.T.: -0.017 min
Response: 94593
Conc: 2.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

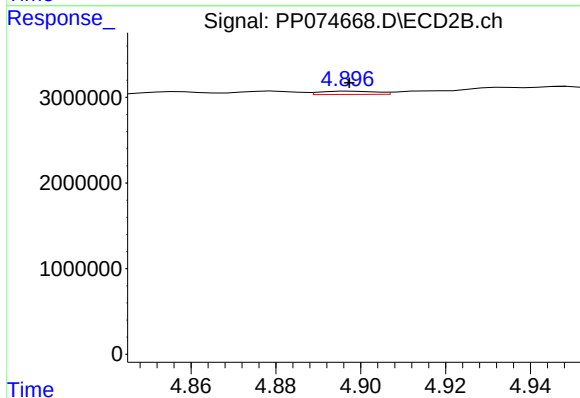


#3 AR-1016-1

R.T.: 4.898 min
Delta R.T.: 0.000 min
Response: 356553
Conc: 0.70 ng/ml

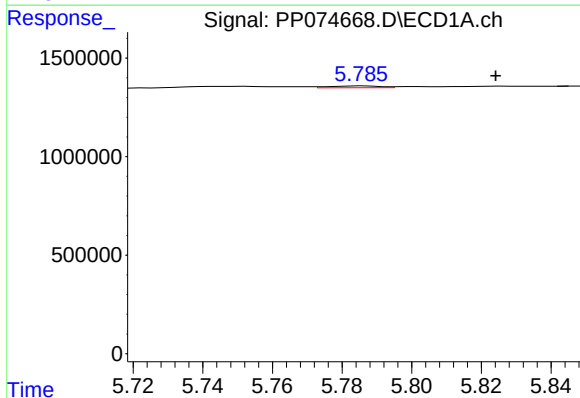


#4 AR-1016-2

R.T.: 5.786 min
Delta R.T.: -0.038 min
Response: 94593
Conc: 1.51 ng/ml

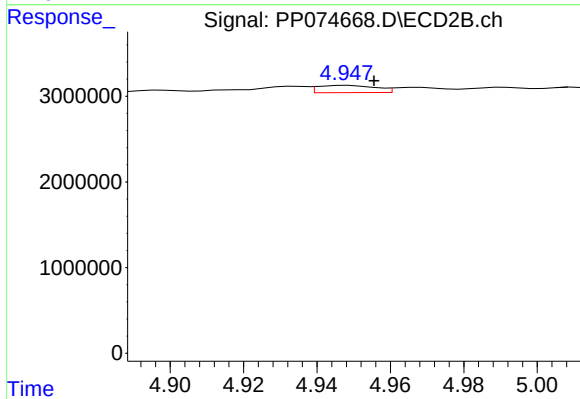

#4 AR-1016-2


R.T.: 4.949 min
Delta R.T.: -0.007 min
Response: 924536
Conc: 3.88 ng/ml

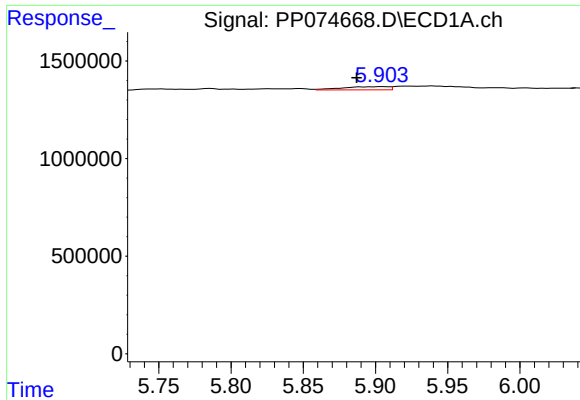

#5 AR-1016-3


R.T.: 5.905 min
Delta R.T.: 0.018 min
Response: 364491
Conc: 8.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

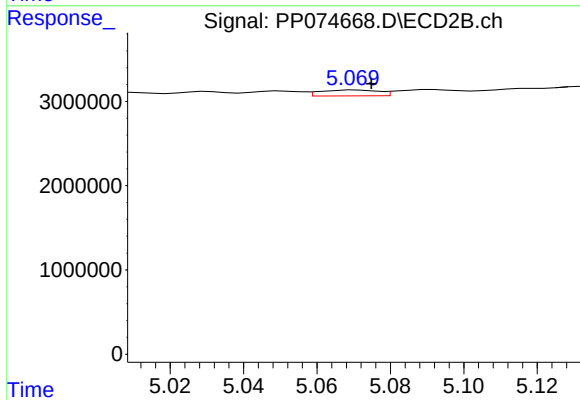


#5 AR-1016-3

R.T.: 5.071 min
Delta R.T.: -0.004 min
Response: 778708
Conc: 5.65 ng/ml

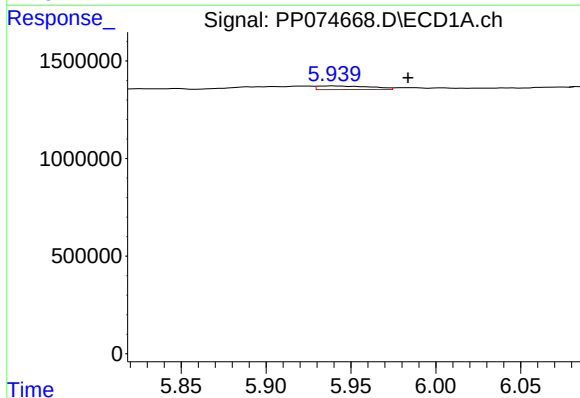


#6 AR-1016-4

R.T.: 5.940 min
Delta R.T.: -0.043 min
Response: 411270
Conc: 11.69 ng/ml

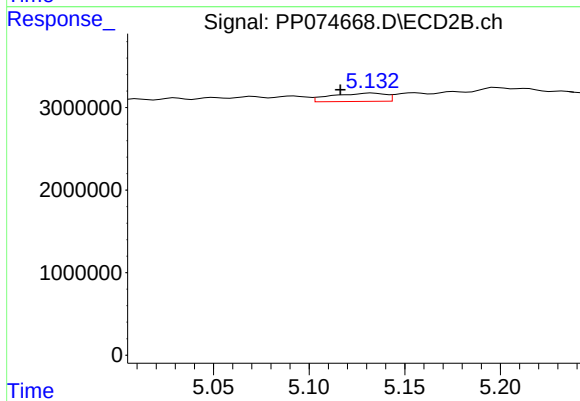

#6 AR-1016-4


R.T.: 5.133 min
Delta R.T.: 0.017 min
Response: 1961470
Conc: 14.03 ng/ml

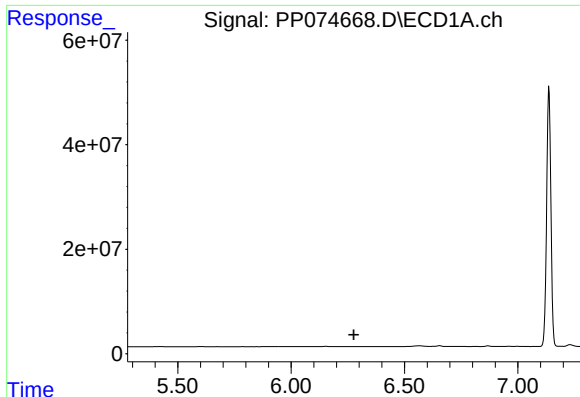

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

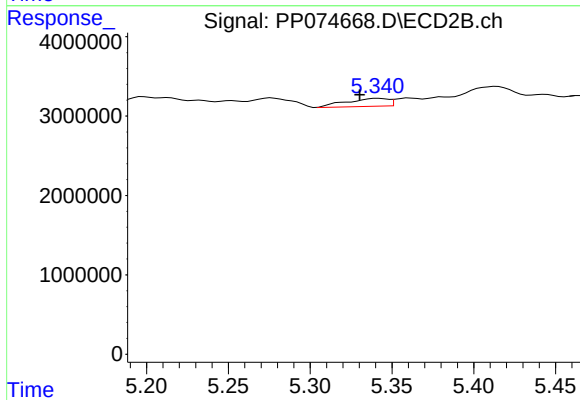


#7 AR-1016-5

R.T.: 5.341 min
Delta R.T.: 0.011 min
Response: 1779728
Conc: 10.72 ng/ml

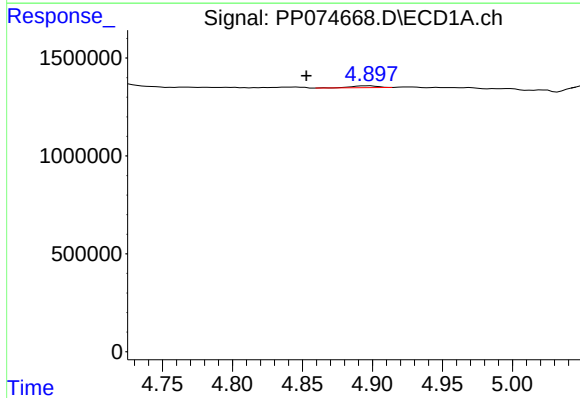


#8 AR-1221-1

R.T.: 4.898 min
Delta R.T.: 0.046 min
Response: 127654
Conc: 7.26 ng/ml

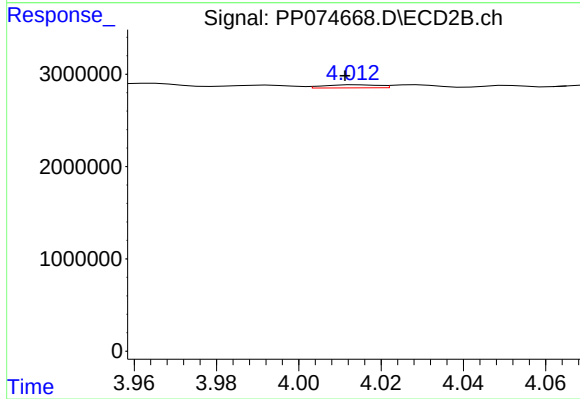

#8 AR-1221-1


R.T.: 4.014 min
Delta R.T.: 0.003 min
Response: 297521
Conc: 4.81 ng/ml

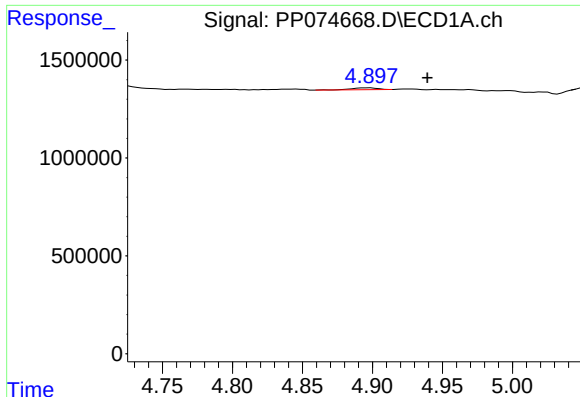

#9 AR-1221-2


R.T.: 4.898 min
Delta R.T.: -0.041 min
Response: 127654
Conc: 9.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

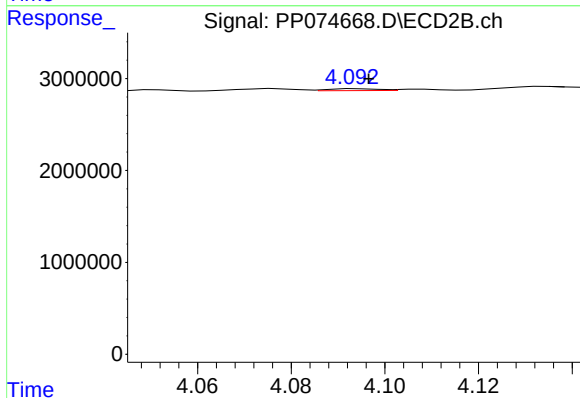


#9 AR-1221-2

R.T.: 4.094 min
Delta R.T.: -0.003 min
Response: 152660
Conc: 3.38 ng/ml

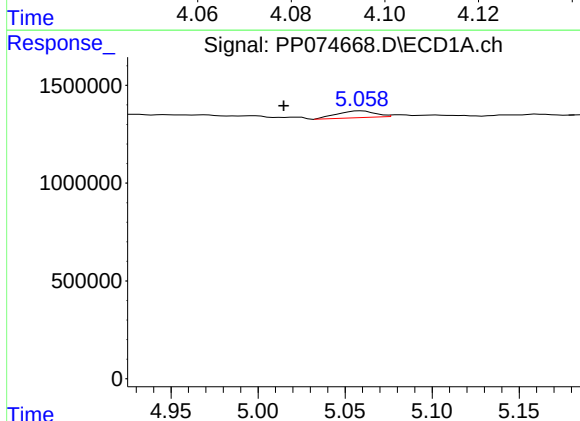


#10 AR-1221-3

R.T.: 5.059 min
Delta R.T.: 0.045 min
Response: 517875
Conc: 13.66 ng/ml

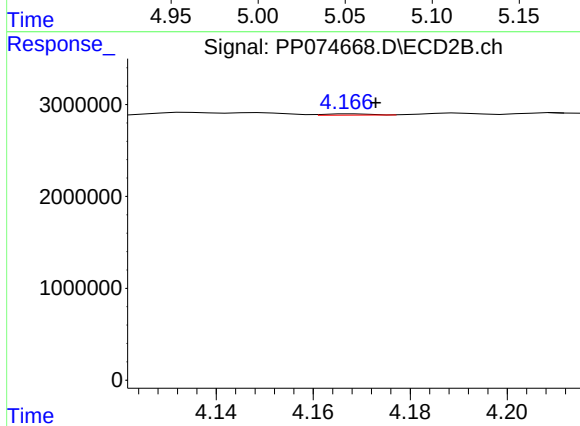

#10 AR-1221-3


R.T.: 4.168 min
Delta R.T.: -0.005 min
Response: 85752
Conc: 0.52 ng/ml

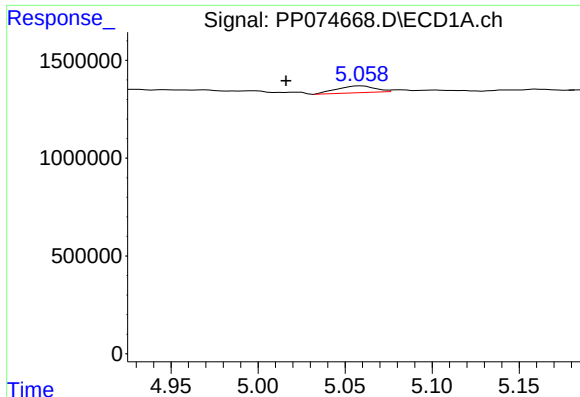

#11 AR-1232-1


R.T.: 5.059 min
Delta R.T.: 0.043 min
Response: 517875
Conc: 17.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

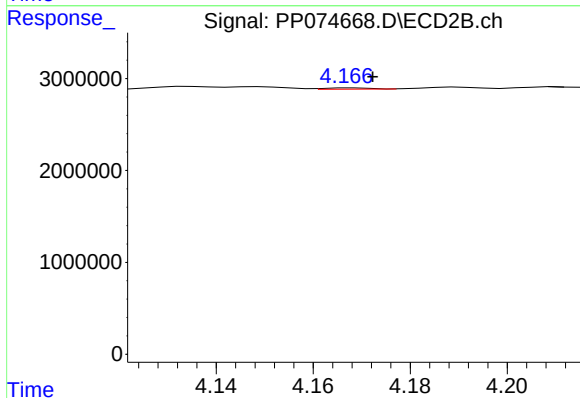


#11 AR-1232-1

R.T.: 4.168 min
Delta R.T.: -0.004 min
Response: 85752
Conc: 0.67 ng/ml

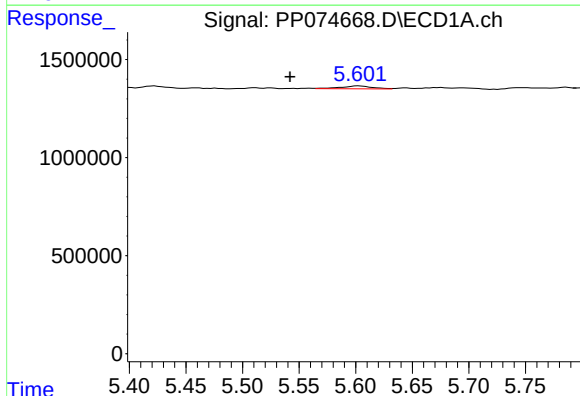


#12 AR-1232-2

R.T.: 5.603 min
Delta R.T.: 0.061 min
Response: 292372
Conc: 18.55 ng/ml

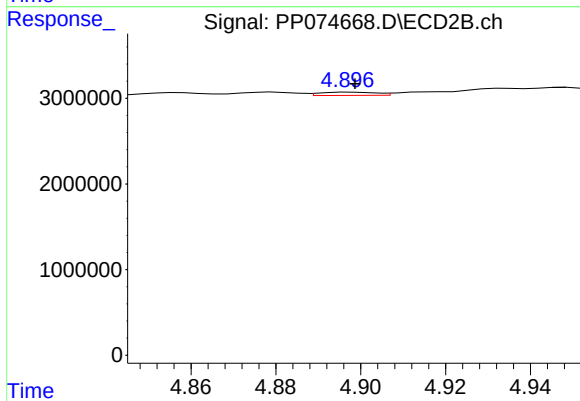

#12 AR-1232-2


R.T.: 4.898 min
Delta R.T.: 0.000 min
Response: 356553
Conc: 1.54 ng/ml

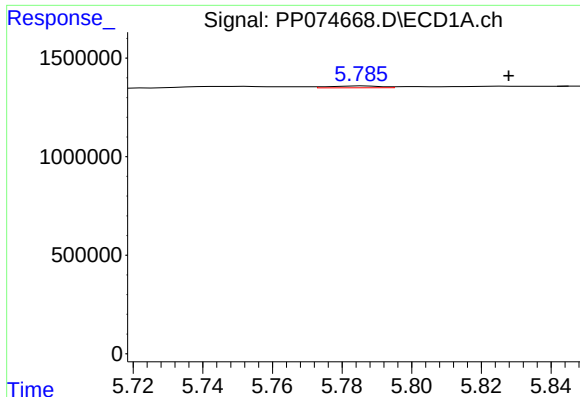

#13 AR-1232-3


R.T.: 5.786 min
Delta R.T.: -0.042 min
Response: 94593
Conc: 3.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

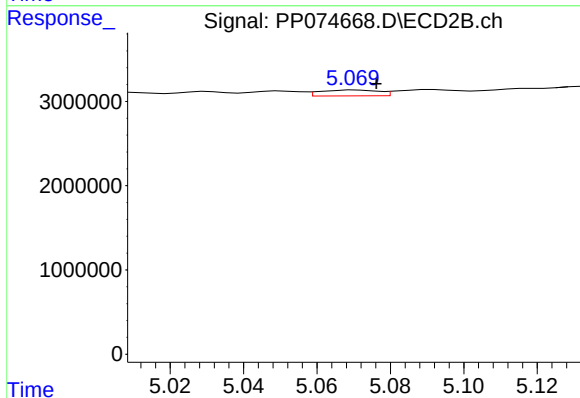


#13 AR-1232-3

R.T.: 5.071 min
Delta R.T.: -0.006 min
Response: 778708
Conc: 12.97 ng/ml

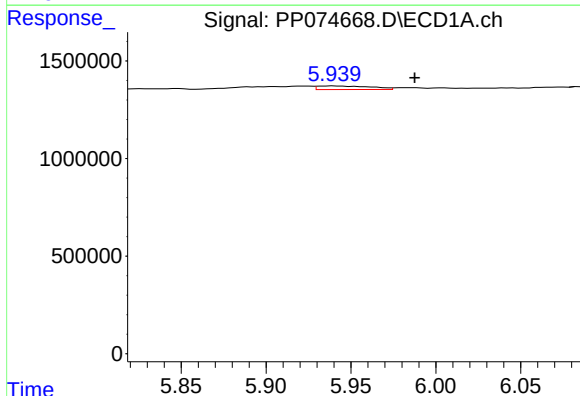


#14 AR-1232-4

R.T.: 5.940 min
Delta R.T.: -0.047 min
Response: 411270
Conc: 23.82 ng/ml

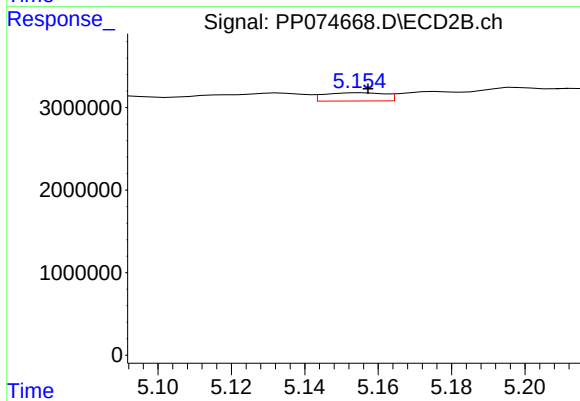

#14 AR-1232-4


R.T.: 5.156 min
Delta R.T.: -0.002 min
Response: 1149148
Conc: 15.59 ng/ml

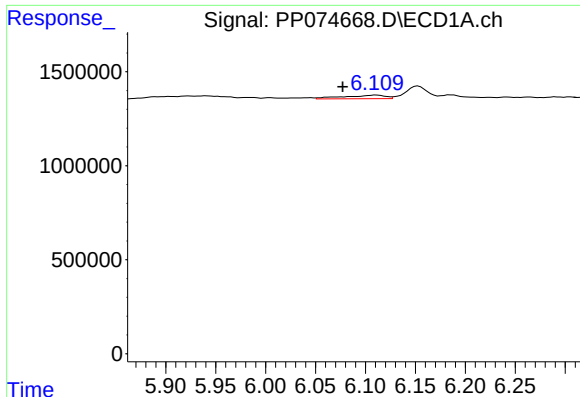

#15 AR-1232-5


R.T.: 6.110 min
Delta R.T.: 0.033 min
Response: 555016
Conc: 42.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

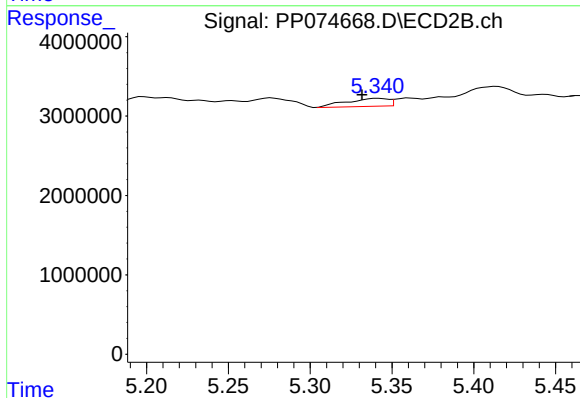


#15 AR-1232-5

R.T.: 5.341 min
Delta R.T.: 0.009 min
Response: 1779728
Conc: 28.67 ng/ml

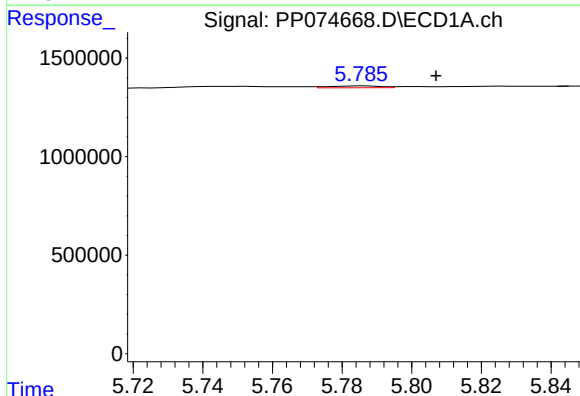


#16 AR-1242-1

R.T.: 5.786 min
Delta R.T.: -0.021 min
Response: 94593
Conc: 2.47 ng/ml

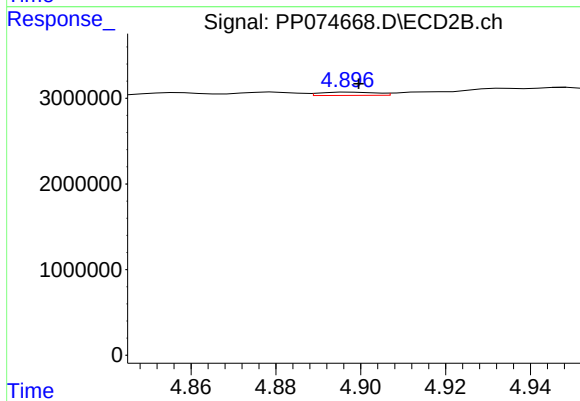

#16 AR-1242-1


R.T.: 4.898 min
Delta R.T.: -0.002 min
Response: 356553
Conc: 0.85 ng/ml

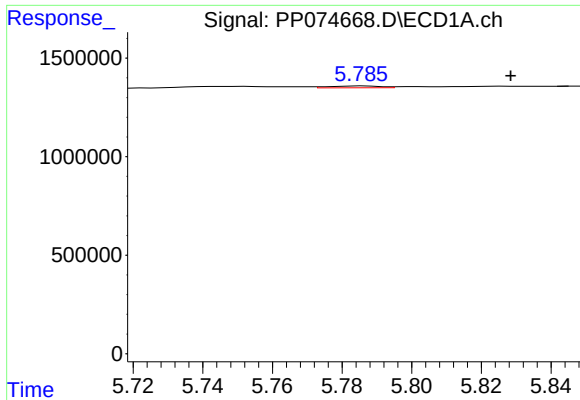

#17 AR-1242-2


R.T.: 5.786 min
Delta R.T.: -0.042 min
Response: 94593
Conc: 1.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

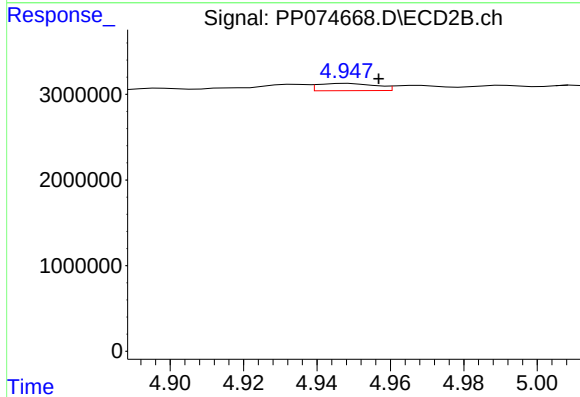


#17 AR-1242-2

R.T.: 4.949 min
Delta R.T.: -0.008 min
Response: 924536
Conc: 4.62 ng/ml

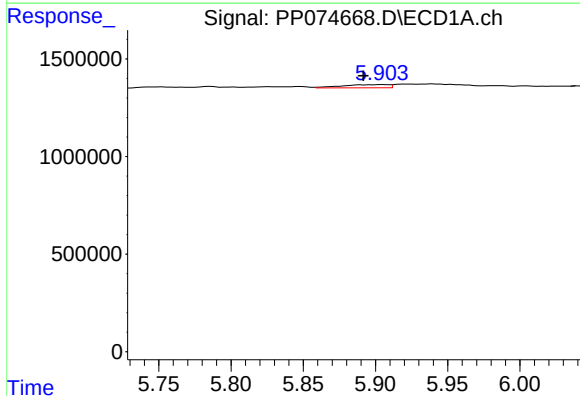


#18 AR-1242-3

R.T.: 5.905 min
Delta R.T.: 0.013 min
Response: 364491
Conc: 8.98 ng/ml

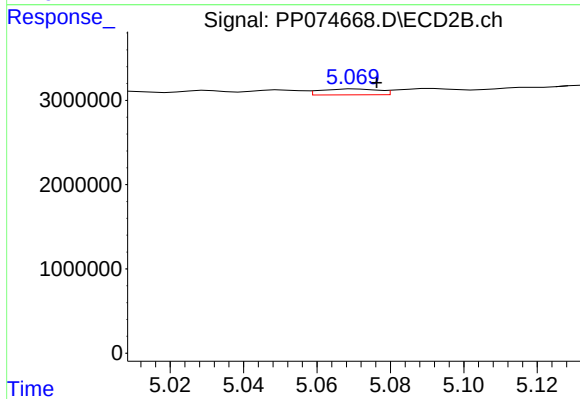

#18 AR-1242-3


R.T.: 5.071 min
Delta R.T.: -0.006 min
Response: 778708
Conc: 6.58 ng/ml

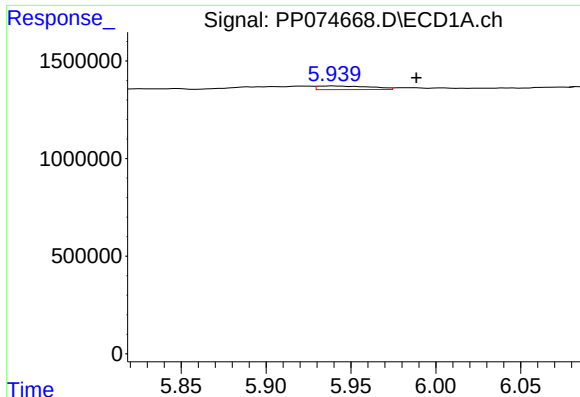

#19 AR-1242-4


R.T.: 5.940 min
Delta R.T.: -0.048 min
Response: 411270
Conc: 12.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

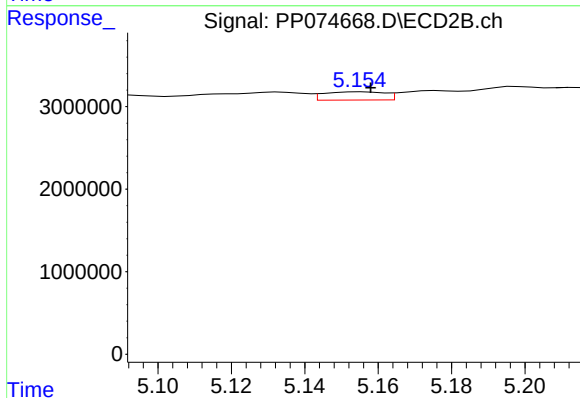


#19 AR-1242-4

R.T.: 5.156 min
Delta R.T.: -0.002 min
Response: 1149148
Conc: 6.71 ng/ml

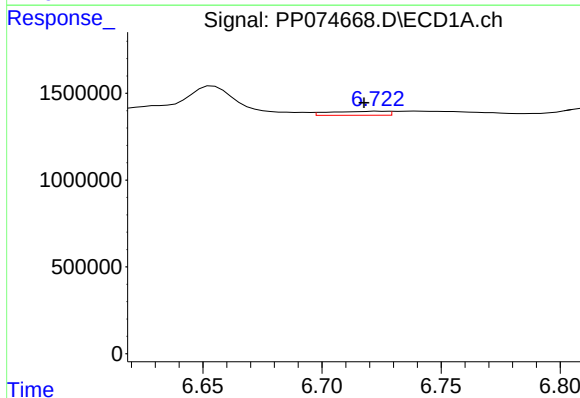


#20 AR-1242-5

R.T.: 6.724 min
Delta R.T.: 0.006 min
Response: 380491
Conc: 10.55 ng/ml

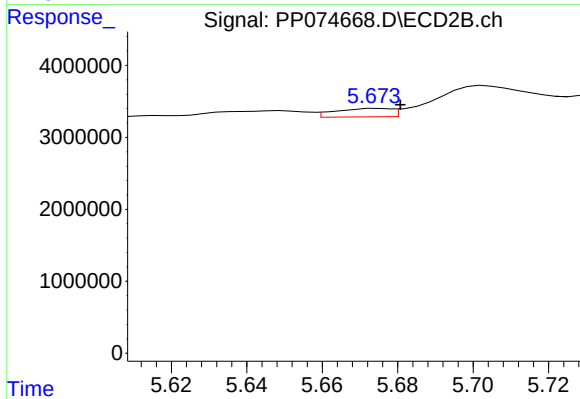

#20 AR-1242-5


R.T.: 5.675 min
Delta R.T.: -0.006 min
Response: 1208508
Conc: 6.53 ng/ml

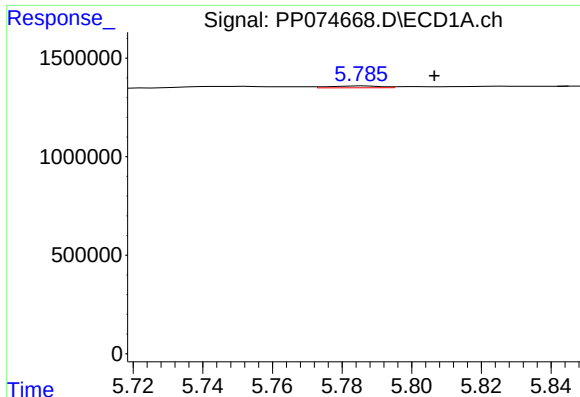

#21 AR-1248-1


R.T.: 5.786 min
Delta R.T.: -0.020 min
Response: 94593
Conc: 3.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

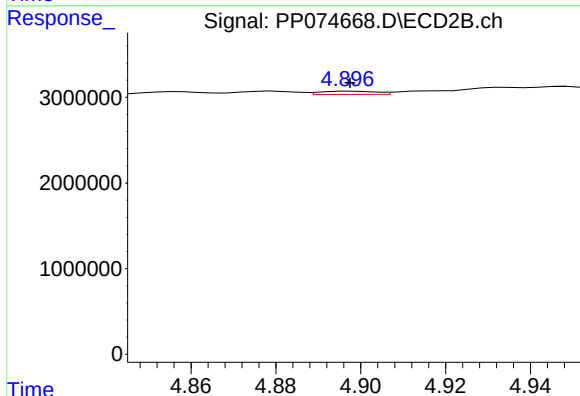


#21 AR-1248-1

R.T.: 4.898 min
Delta R.T.: 0.000 min
Response: 356553
Conc: 1.29 ng/ml

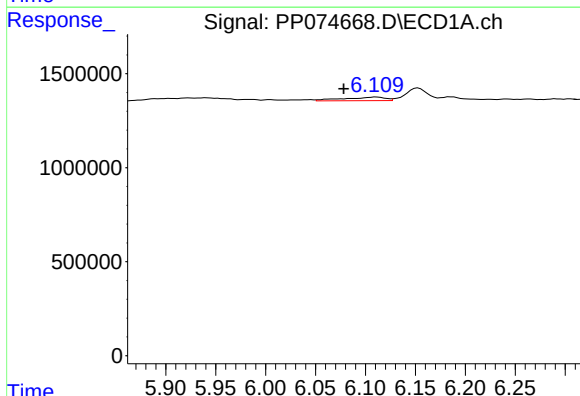


#22 AR-1248-2

R.T.: 6.110 min
Delta R.T.: 0.032 min
Response: 555016
Conc: 12.88 ng/ml

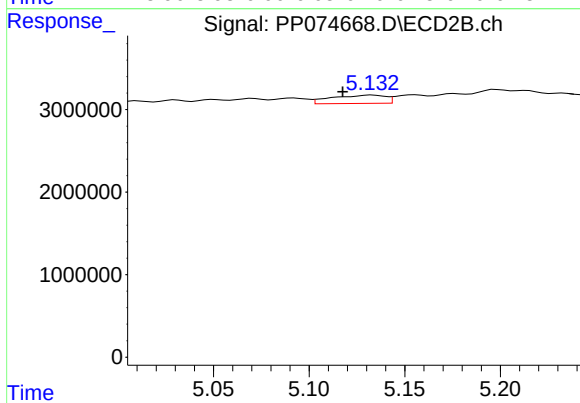

#22 AR-1248-2


R.T.: 5.133 min
Delta R.T.: 0.016 min
Response: 1961470
Conc: 11.10 ng/ml

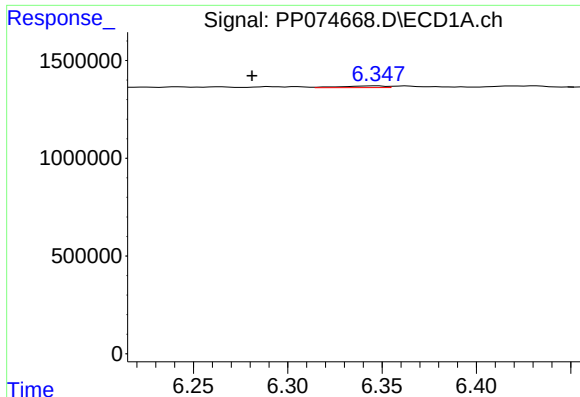

#23 AR-1248-3


R.T.: 6.347 min
Delta R.T.: 0.066 min
Response: 133641
Conc: 2.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

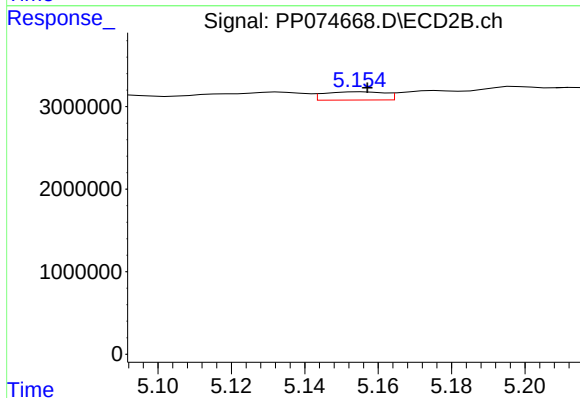


#23 AR-1248-3

R.T.: 5.156 min
Delta R.T.: -0.002 min
Response: 1149148
Conc: 5.06 ng/ml

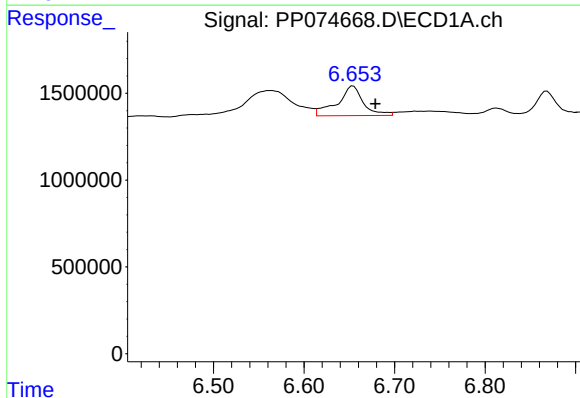


#24 AR-1248-4

R.T.: 6.654 min
Delta R.T.: -0.024 min
Response: 3422620
Conc: 62.23 ng/ml

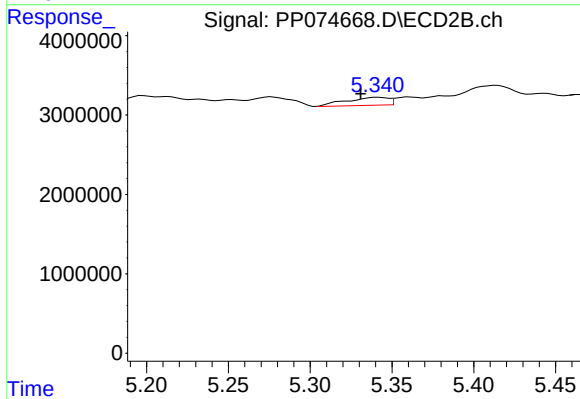

#24 AR-1248-4


R.T.: 5.341 min
Delta R.T.: 0.010 min
Response: 1779728
Conc: 8.16 ng/ml

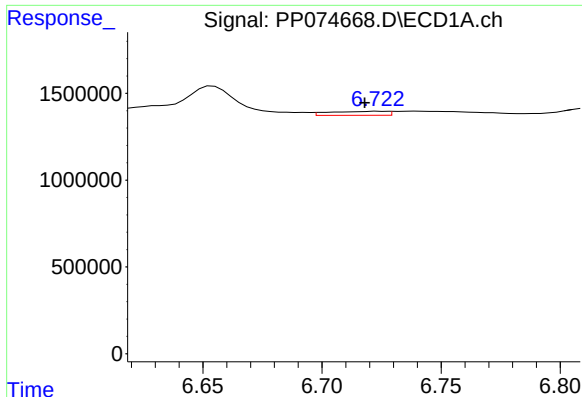

#25 AR-1248-5


R.T.: 6.724 min
Delta R.T.: 0.006 min
Response: 380491
Conc: 6.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

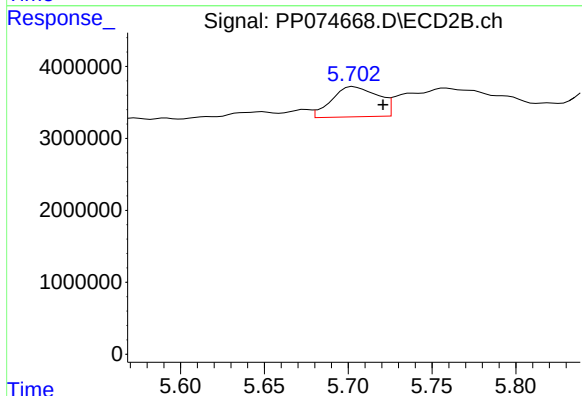


#25 AR-1248-5

R.T.: 5.703 min
Delta R.T.: -0.018 min
Response: 8040004
Conc: 21.89 ng/ml

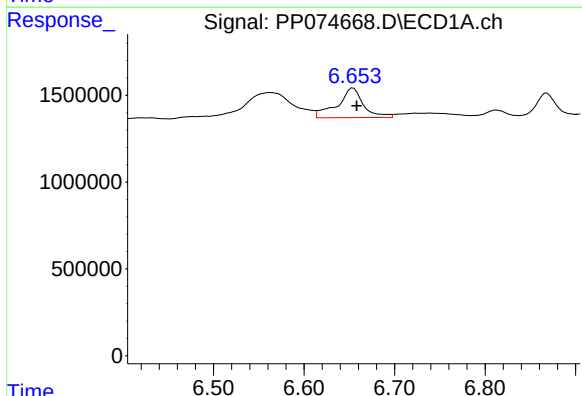


#26 AR-1254-1

R.T.: 6.654 min
Delta R.T.: -0.004 min
Response: 3422620
Conc: 58.74 ng/ml

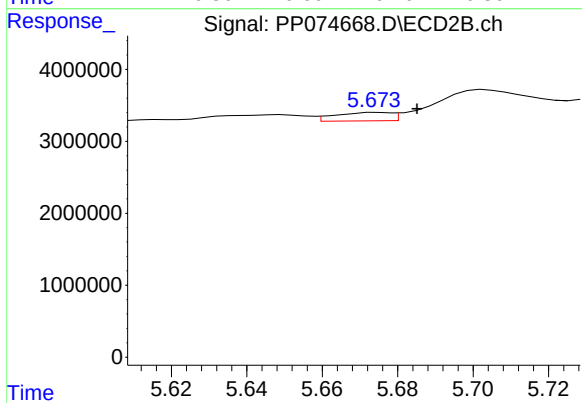

#26 AR-1254-1


R.T.: 5.675 min
Delta R.T.: -0.010 min
Response: 1208508
Conc: 2.54 ng/ml

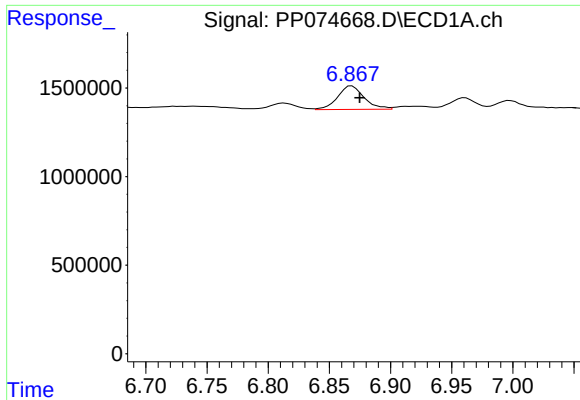

#27 AR-1254-2


R.T.: 6.868 min
Delta R.T.: -0.007 min
Response: 2009763
Conc: 24.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

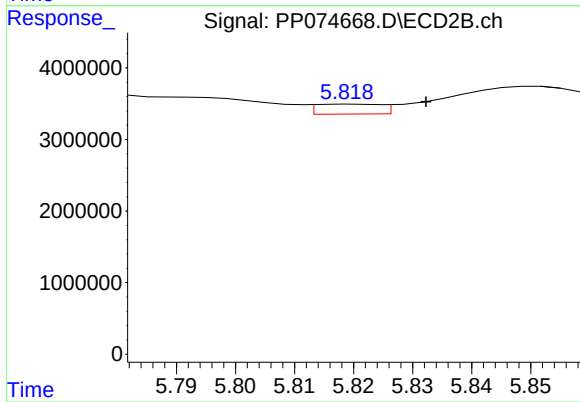


#27 AR-1254-2

R.T.: 5.820 min
Delta R.T.: -0.012 min
Response: 1059029
Conc: 3.01 ng/ml

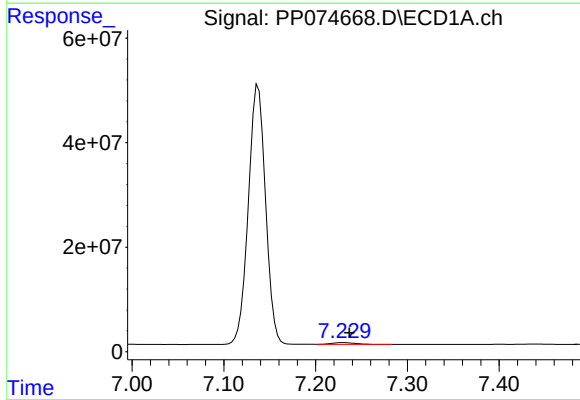


#28 AR-1254-3

R.T.: 7.230 min
Delta R.T.: -0.007 min
Response: 6293801
Conc: 70.55 ng/ml

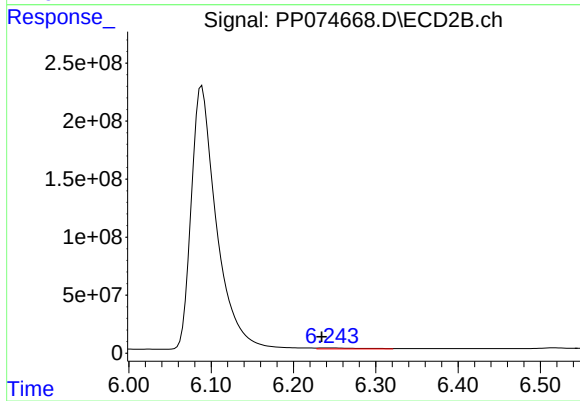

#28 AR-1254-3


R.T.: 6.244 min
Delta R.T.: 0.010 min
Response: 30806415
Conc: 49.70 ng/ml

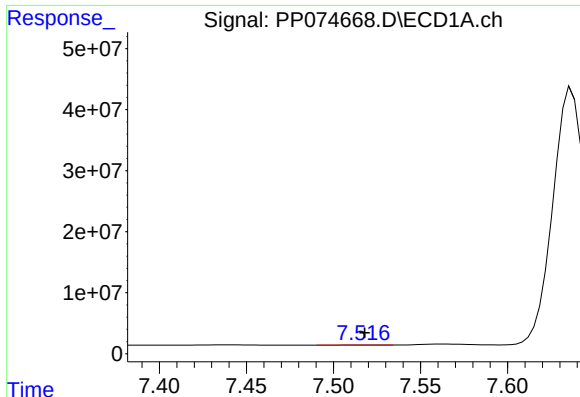

#29 AR-1254-4


R.T.: 7.517 min
Delta R.T.: 0.000 min
Response: 377623
Conc: 5.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

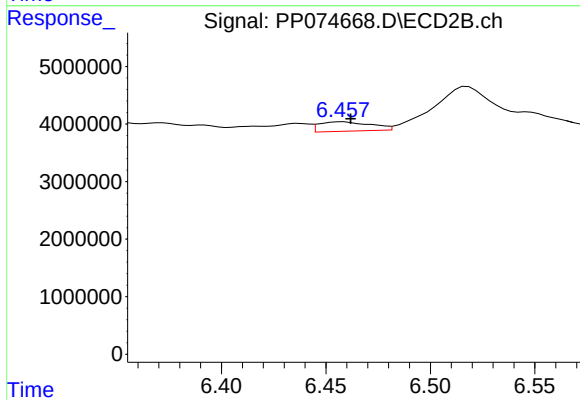


#29 AR-1254-4

R.T.: 6.458 min
Delta R.T.: -0.004 min
Response: 2802068
Conc: 5.98 ng/ml

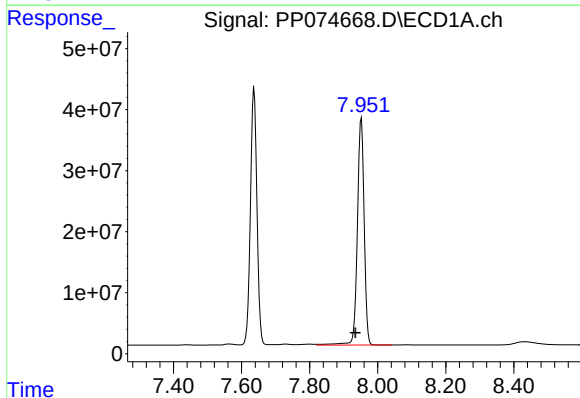


#30 AR-1254-5

R.T.: 7.952 min
Delta R.T.: 0.017 min
Response: 513281877
Conc: 6177.79 ng/ml

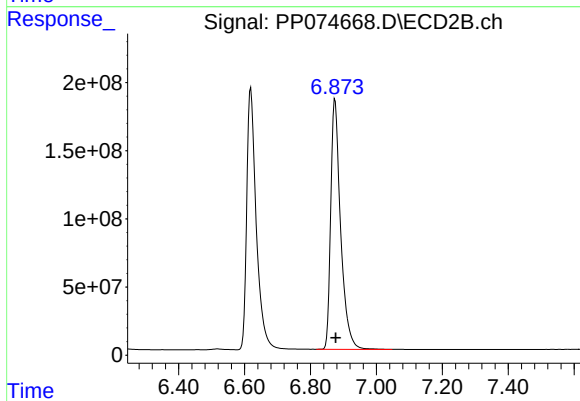

#30 AR-1254-5


R.T.: 6.874 min
Delta R.T.: -0.003 min
Response: 3819331178
Conc: 7786.59 ng/ml

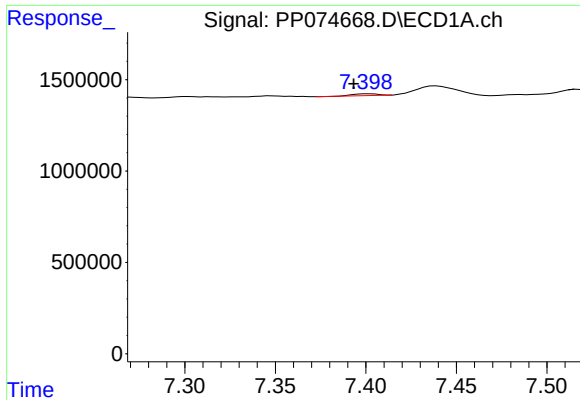

#31 AR-1260-1


R.T.: 7.401 min
Delta R.T.: 0.008 min
Response: 92500
Conc: 1.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

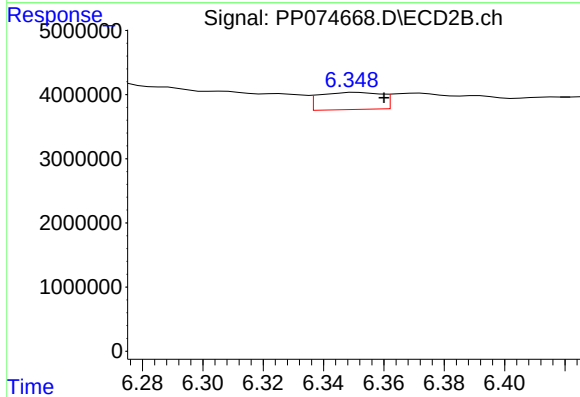


#31 AR-1260-1

R.T.: 6.351 min
Delta R.T.: -0.009 min
Response: 3784498
Conc: 10.09 ng/ml

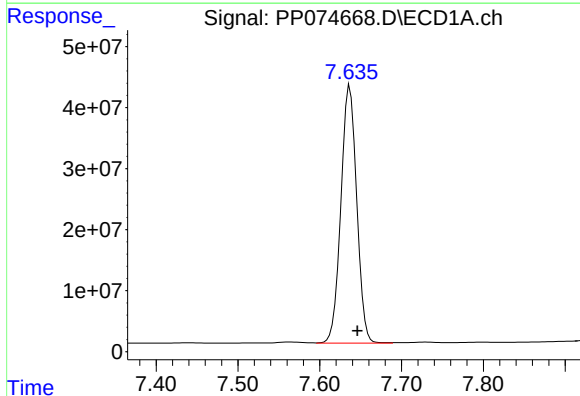


#32 AR-1260-2

R.T.: 7.637 min
Delta R.T.: -0.009 min
Response: 564152321
Conc: 8185.91 ng/ml

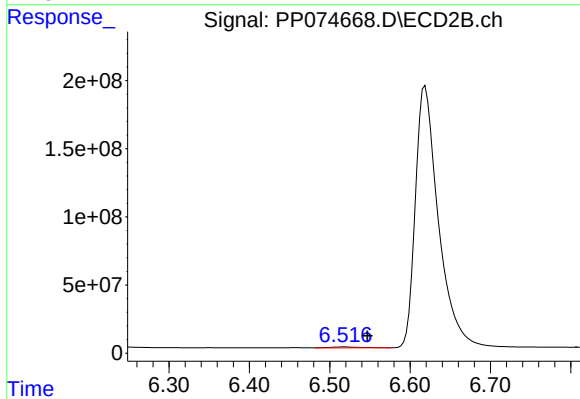

#32 AR-1260-2


R.T.: 6.518 min
Delta R.T.: -0.029 min
Response: 17224559
Conc: 32.57 ng/ml

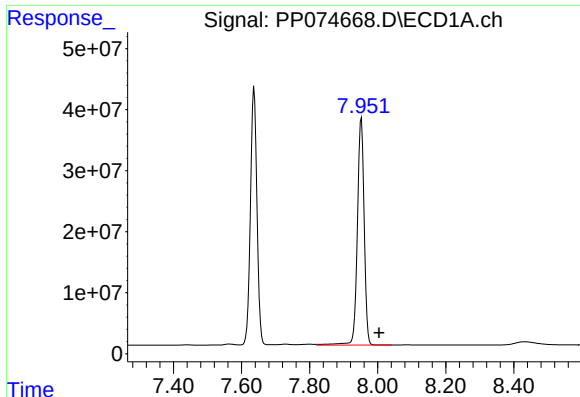

#33 AR-1260-3


R.T.: 7.952 min
Delta R.T.: -0.053 min
Response: 513281877
Conc: 9892.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

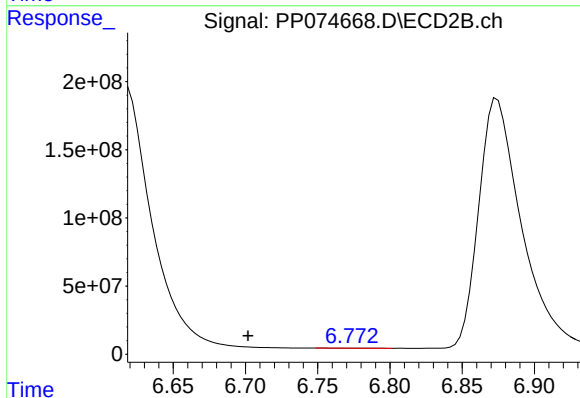


#33 AR-1260-3

R.T.: 6.771 min
Delta R.T.: 0.070 min
Response: 132225
Conc: 0.31 ng/ml

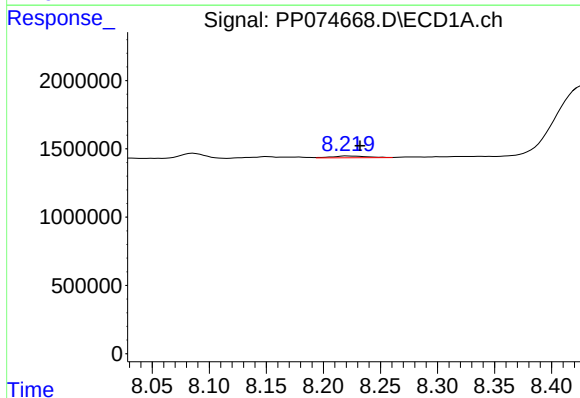


#34 AR-1260-4

R.T.: 8.221 min
Delta R.T.: -0.011 min
Response: 285086
Conc: 4.47 ng/ml

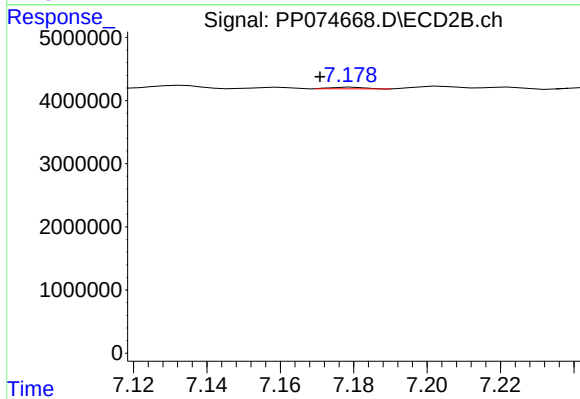

#34 AR-1260-4


R.T.: 7.180 min
Delta R.T.: 0.009 min
Response: 173502
Conc: 0.45 ng/ml

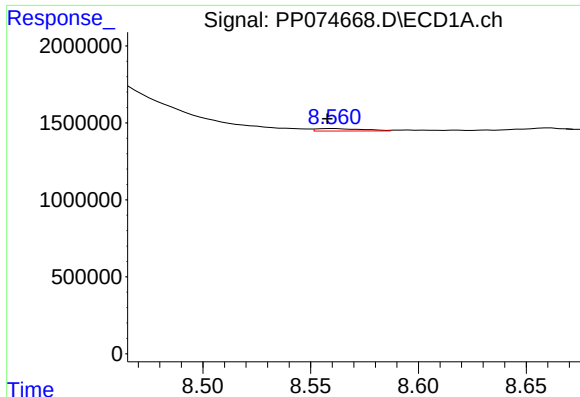

#35 AR-1260-5


R.T.: 8.561 min
Delta R.T.: 0.003 min
Response: 242889
Conc: 2.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

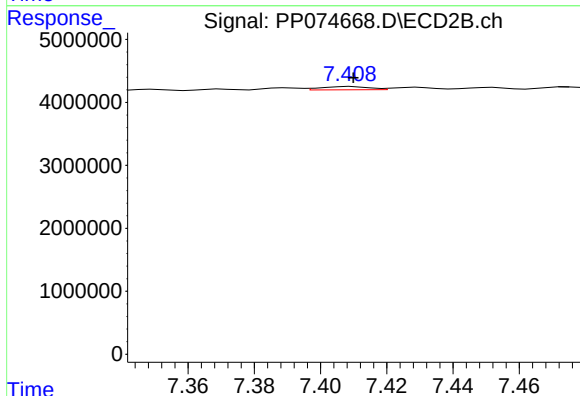


#35 AR-1260-5

R.T.: 7.409 min
Delta R.T.: 0.000 min
Response: 539898
Conc: 0.54 ng/ml

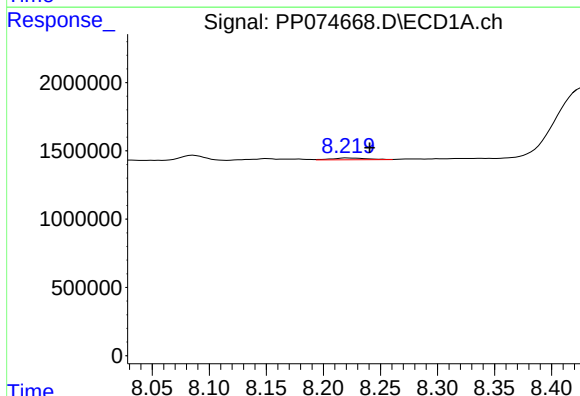


#36 AR-1262-1

R.T.: 8.221 min
Delta R.T.: -0.020 min
Response: 285086
Conc: 3.70 ng/ml

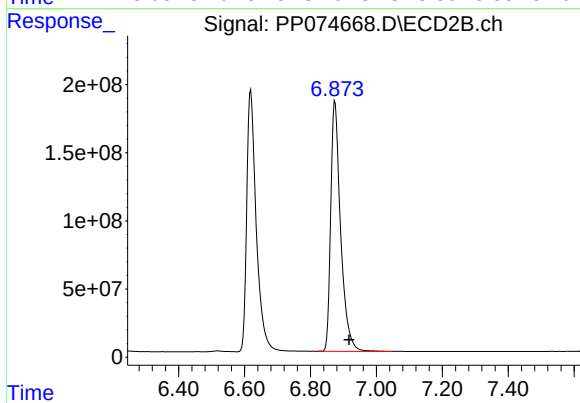

#36 AR-1262-1


R.T.: 6.874 min
Delta R.T.: -0.043 min
Response: 3819331178
Conc: 5400.19 ng/ml

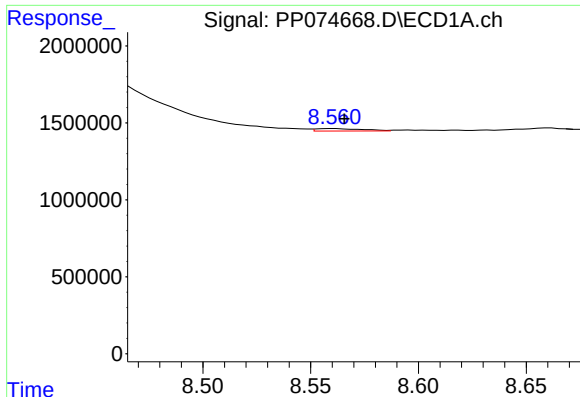

#37 AR-1262-2


R.T.: 8.561 min
Delta R.T.: -0.005 min
Response: 242889
Conc: 1.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

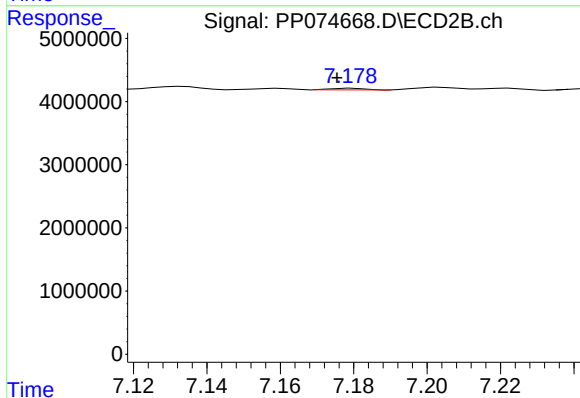


#37 AR-1262-2

R.T.: 7.180 min
Delta R.T.: 0.004 min
Response: 173502
Conc: 0.33 ng/ml

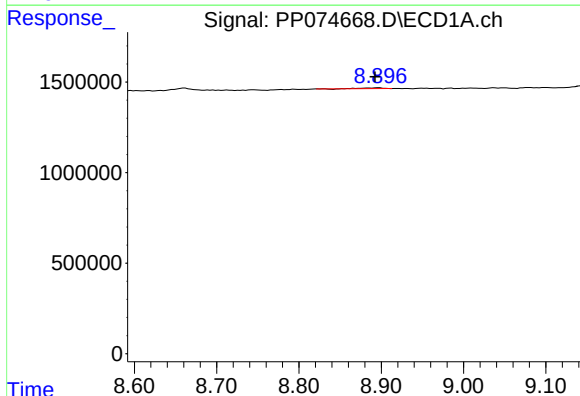


#38 AR-1262-3

R.T.: 8.897 min
Delta R.T.: 0.005 min
Response: 63238
Conc: 0.65 ng/ml

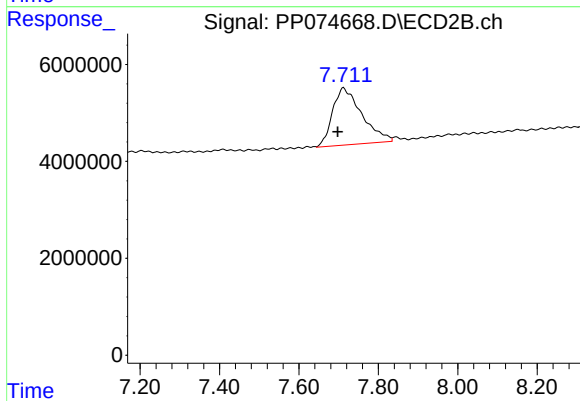

#38 AR-1262-3


R.T.: 7.712 min
Delta R.T.: 0.015 min
Response: 60358966
Conc: 129.44 ng/ml

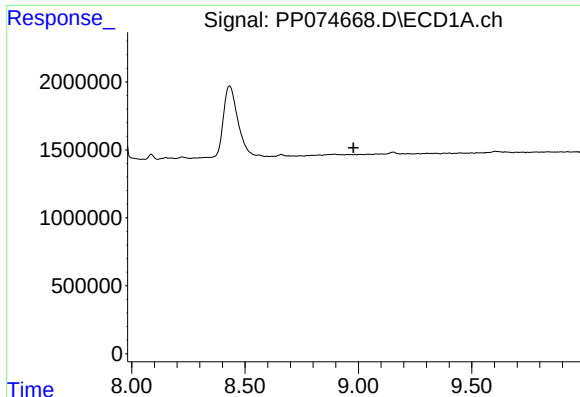

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

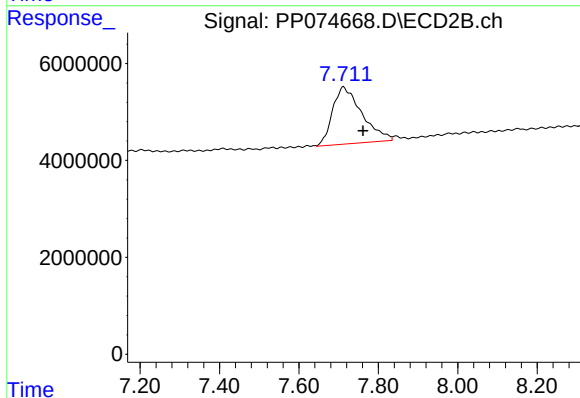


#39 AR-1262-4

R.T.: 7.712 min
Delta R.T.: -0.049 min
Response: 60358966
Conc: 73.44 ng/ml

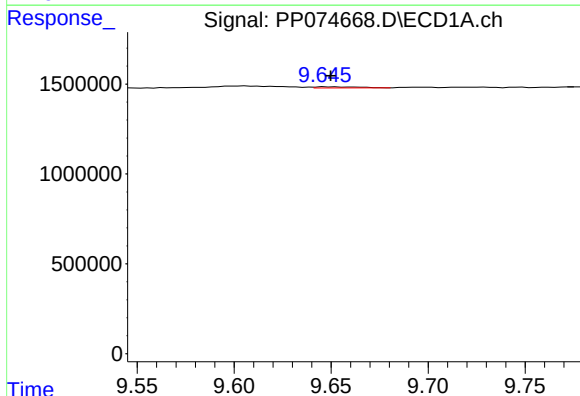


#40 AR-1262-5

R.T.: 9.647 min
Delta R.T.: -0.003 min
Response: 94566
Conc: 1.55 ng/ml

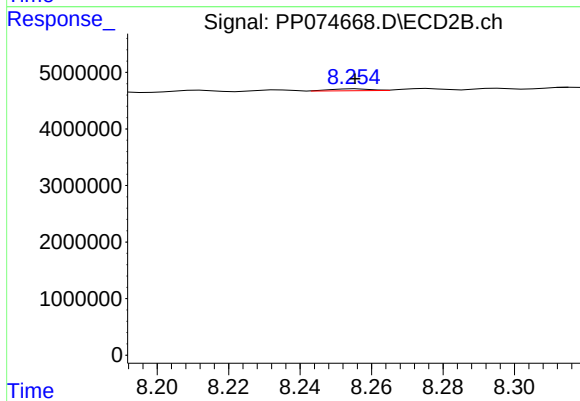

#40 AR-1262-5


R.T.: 8.256 min
Delta R.T.: 0.000 min
Response: 238842
Conc: 0.67 ng/ml

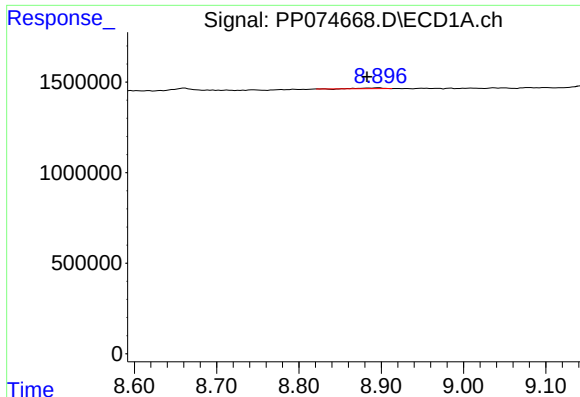

#41 AR-1268-1


R.T.: 8.897 min
Delta R.T.: 0.014 min
Response: 63238
Conc: 0.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

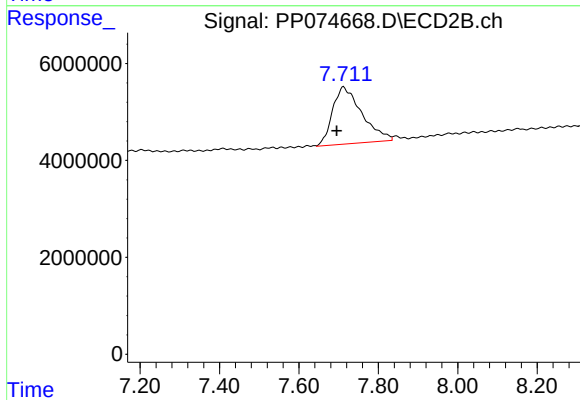


#41 AR-1268-1

R.T.: 7.712 min
Delta R.T.: 0.017 min
Response: 60358966
Conc: 42.79 ng/ml

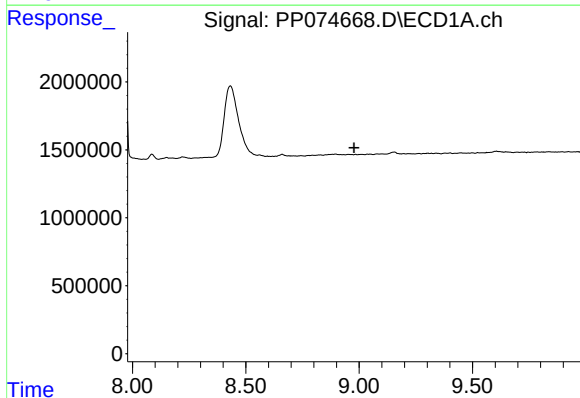


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.978 min
Response: 0
Conc: N.D.

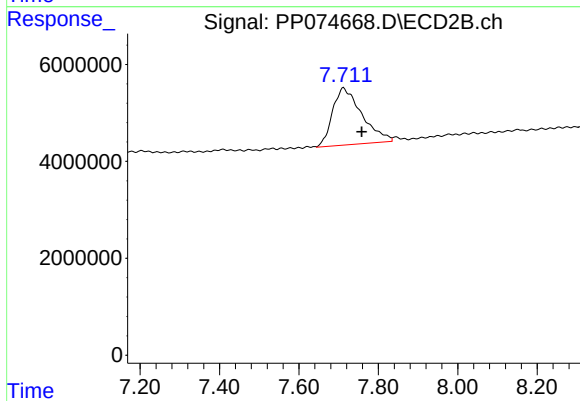

#42 AR-1268-2


R.T.: 7.712 min
Delta R.T.: -0.046 min
Response: 60358966
Conc: 44.27 ng/ml

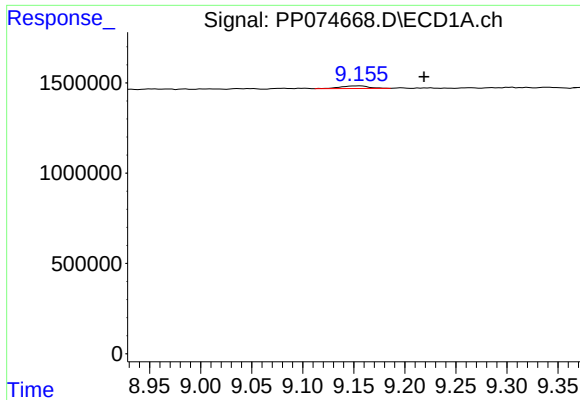

#43 AR-1268-3


R.T.: 9.156 min
Delta R.T.: -0.063 min
Response: 268668
Conc: 2.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

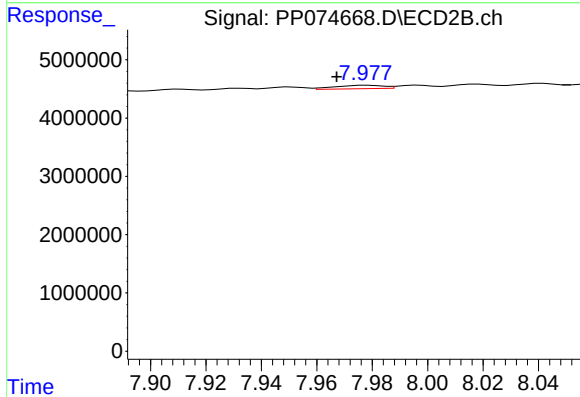


#43 AR-1268-3

R.T.: 7.978 min
Delta R.T.: 0.011 min
Response: 733931
Conc: 0.70 ng/ml

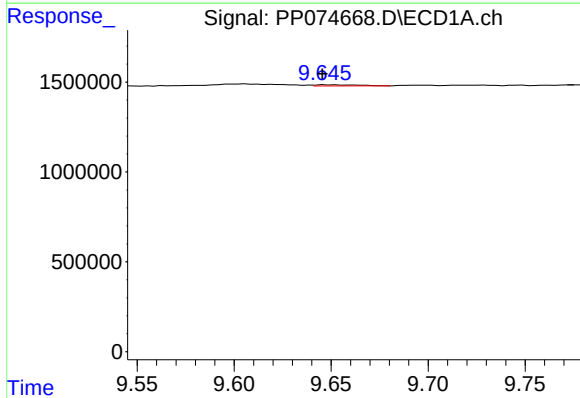


#44 AR-1268-4

R.T.: 9.647 min
Delta R.T.: 0.002 min
Response: 94566
Conc: 1.41 ng/ml

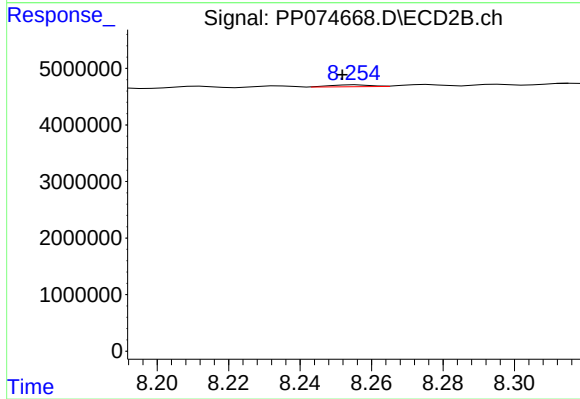

#44 AR-1268-4


R.T.: 8.256 min
Delta R.T.: 0.004 min
Response: 238842
Conc: 0.62 ng/ml

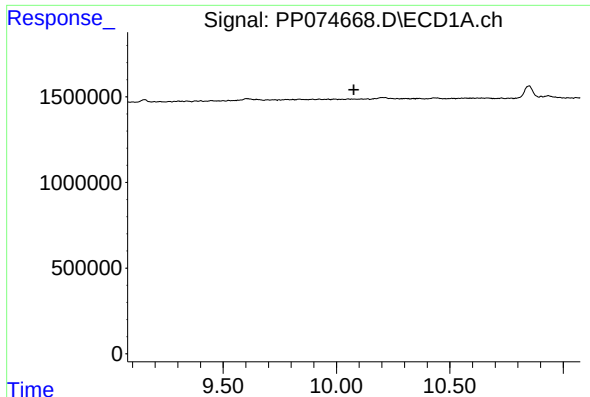

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

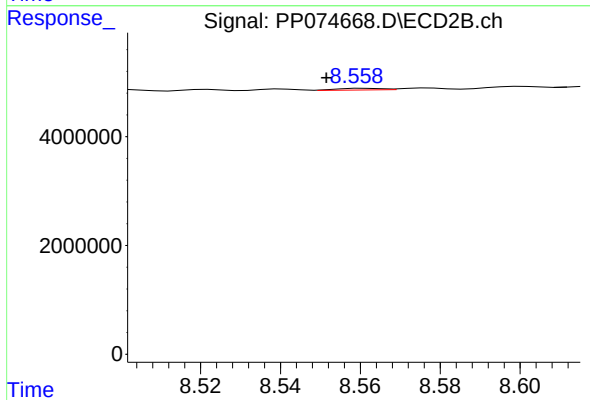

#45 AR-1268-5

R.T.: 8.561 min
Delta R.T.: 0.009 min
Response: 248071
Conc: 0.08 ng/ml