

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082823\
 Data File : PP059625.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2023 11:00
 Operator : YP\AJ
 Sample : 04160-01DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CHRT-24449DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/29/2023
 Supervised By :Ankita Jodhani 08/29/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 22:50:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 24 01:16:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.410	3.638	3639656	5299614	3.079m	2.743
2) SA Decachlor...	10.193	8.661	6926851	10264955	8.859	7.437
Target Compounds						
31) L7 AR-1260-1	7.197	6.214	26490643	39366189	473.394	407.031
32) L7 AR-1260-2	7.455	6.404	34385372	53967660	590.476	487.965
33) L7 AR-1260-3	7.815	6.556	19140885	44173866	486.976	416.730
34) L7 AR-1260-4	8.041	7.029	25650090	33229716	592.477	396.501 #
35) L7 AR-1260-5	8.362	7.274	46184166	88075503	617.298	504.061

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082823\
Data File : PP059625.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2023 11:00
Operator : YP\AJ
Sample : 04160-01DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CHRT-24449DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/29/2023
Supervised By :Ankita Jodhani 08/29/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 22:50:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082323.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 24 01:16:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

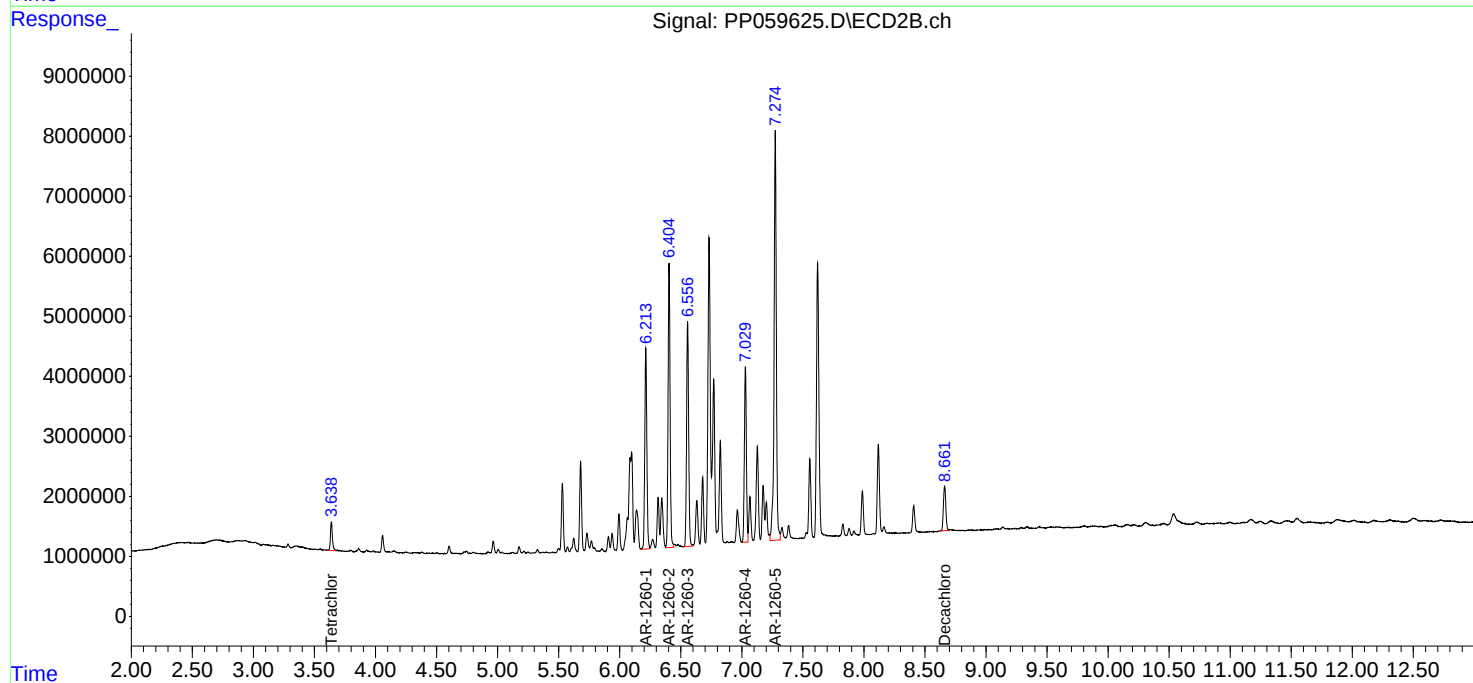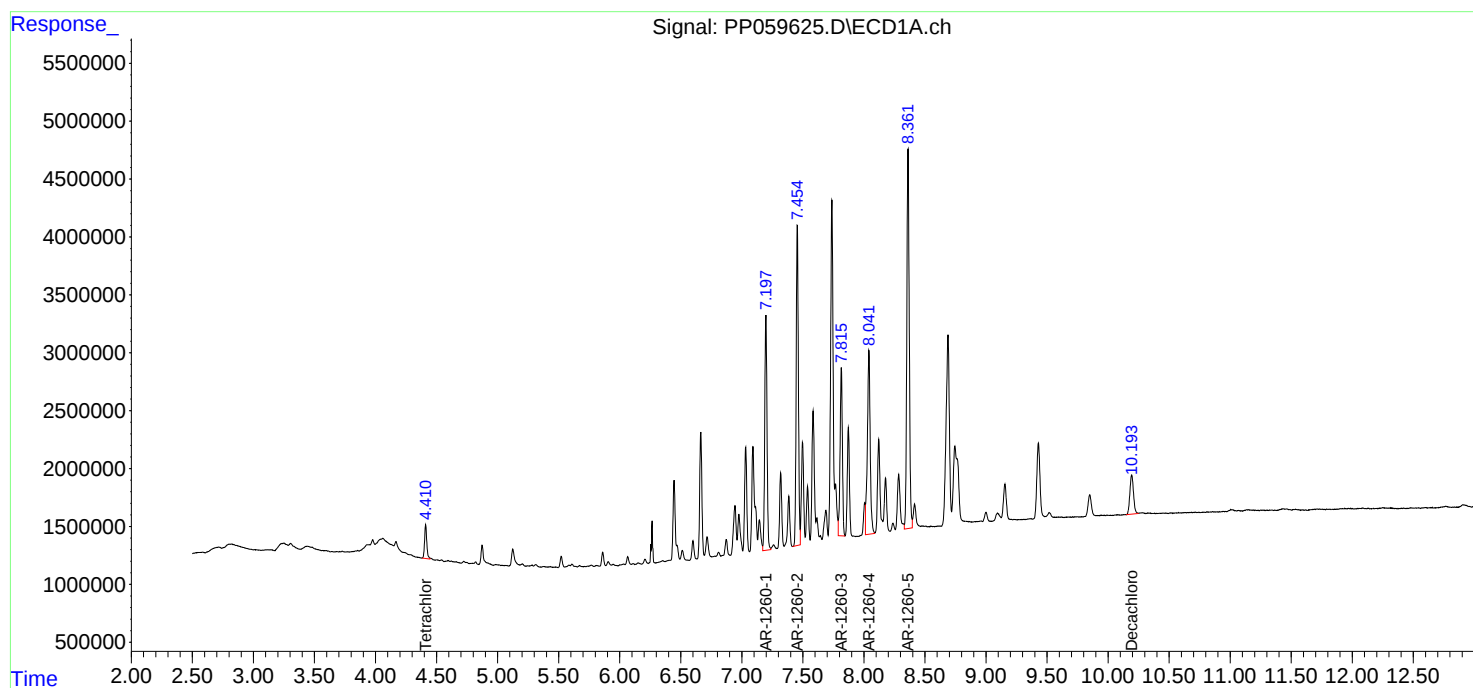

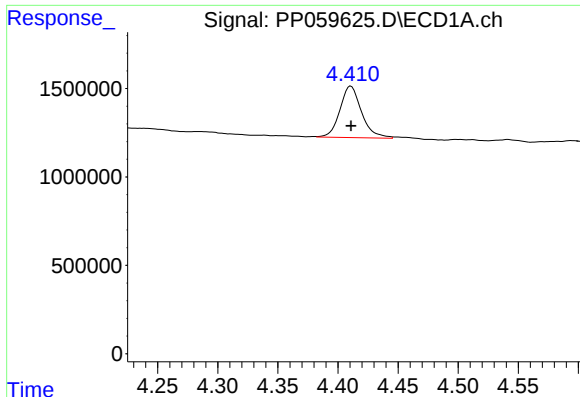


#1 Tetrachloro-m-xylene

R.T.: 4.410 min
Delta R.T.: 0.000 min
Response: 3639656
Conc: 3.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-24449DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/29/2023
Supervised By :Ankita Jodhani 08/29/2023

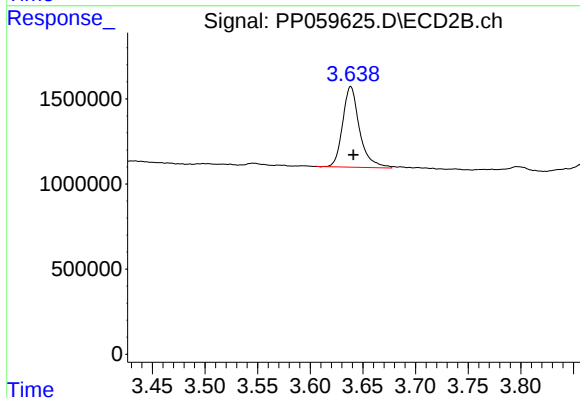


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: -0.003 min
Response: 5299614
Conc: 2.74 ng/ml

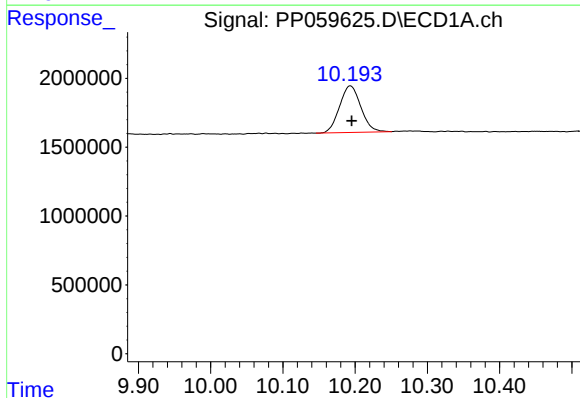


#2 Decachlorobiphenyl

R.T.: 10.193 min
Delta R.T.: -0.002 min
Response: 6926851
Conc: 8.86 ng/ml

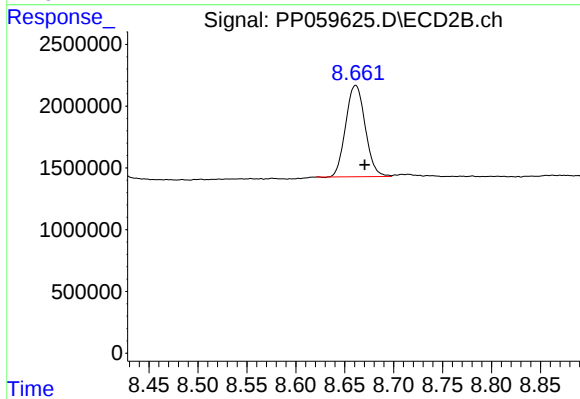

#2 Decachlorobiphenyl

R.T.: 8.661 min
Delta R.T.: -0.009 min
Response: 10264955
Conc: 7.44 ng/ml

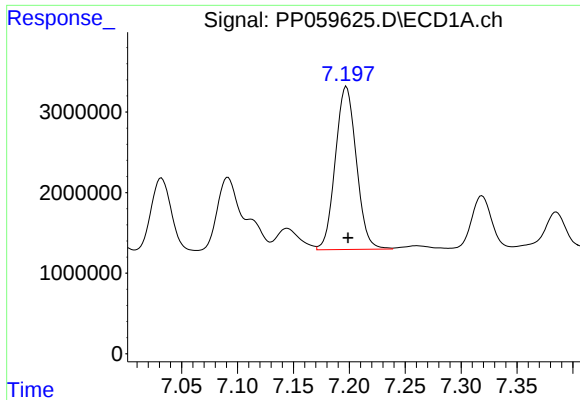


#31 AR-1260-1

R.T.: 7.197 min
Delta R.T.: -0.001 min
Response: 26490643
Conc: 473.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-24449DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/29/2023
Supervised By :Ankita Jodhani 08/29/2023

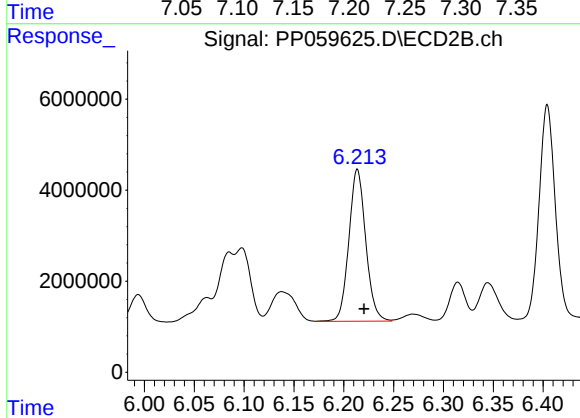


#31 AR-1260-1

R.T.: 6.214 min
Delta R.T.: -0.007 min
Response: 39366189
Conc: 407.03 ng/ml

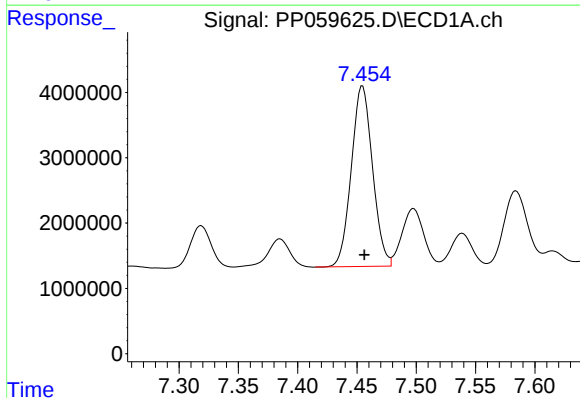


#32 AR-1260-2

R.T.: 7.455 min
Delta R.T.: -0.002 min
Response: 34385372
Conc: 590.48 ng/ml

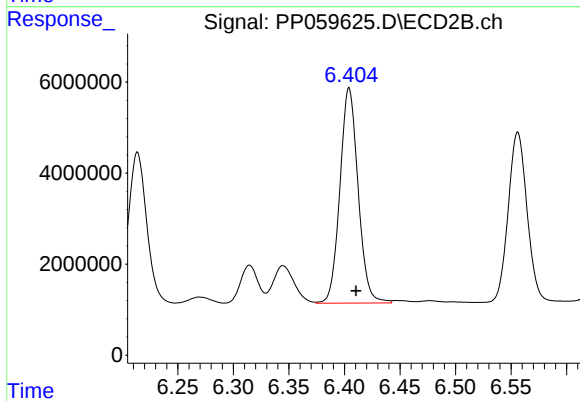

#32 AR-1260-2

R.T.: 6.404 min
Delta R.T.: -0.006 min
Response: 53967660
Conc: 487.96 ng/ml

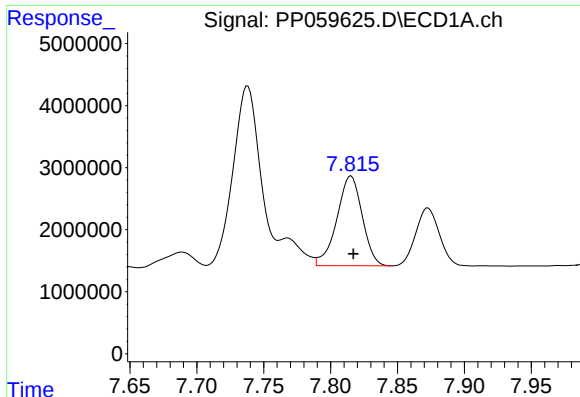


#33 AR-1260-3

R.T.: 7.815 min
Delta R.T.: -0.002 min
Response: 19140885
Conc: 486.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-24449DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/29/2023
Supervised By :Ankita Jodhani 08/29/2023

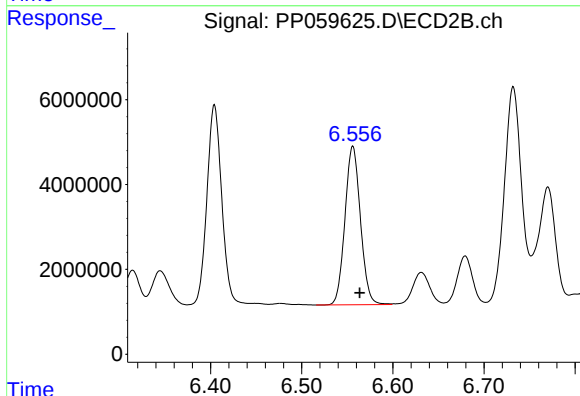


#33 AR-1260-3

R.T.: 6.556 min
Delta R.T.: -0.008 min
Response: 44173866
Conc: 416.73 ng/ml

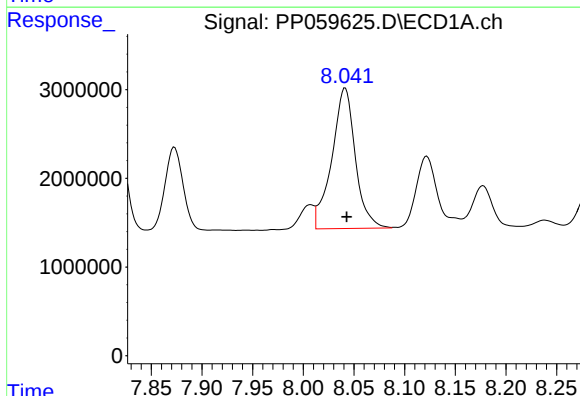


#34 AR-1260-4

R.T.: 8.041 min
Delta R.T.: -0.002 min
Response: 25650090
Conc: 592.48 ng/ml

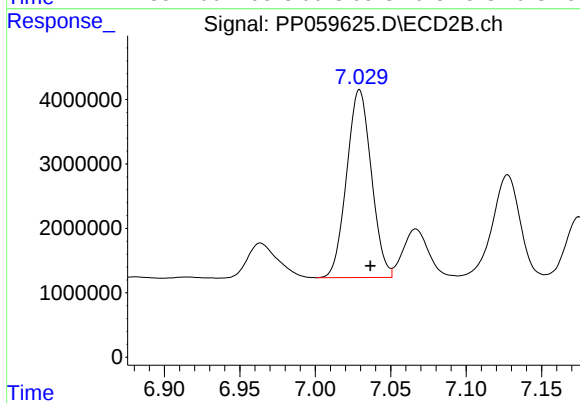

#34 AR-1260-4

R.T.: 7.029 min
Delta R.T.: -0.007 min
Response: 33229716
Conc: 396.50 ng/ml

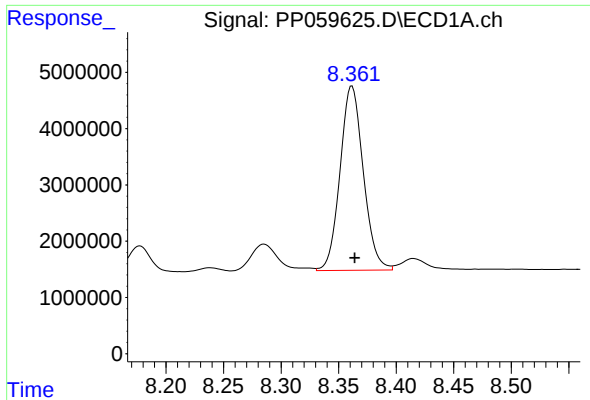


#35 AR-1260-5

R.T.: 8.362 min
Delta R.T.: -0.003 min
Response: 46184166
Conc: 617.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-24449DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/29/2023
Supervised By :Ankita Jodhani 08/29/2023

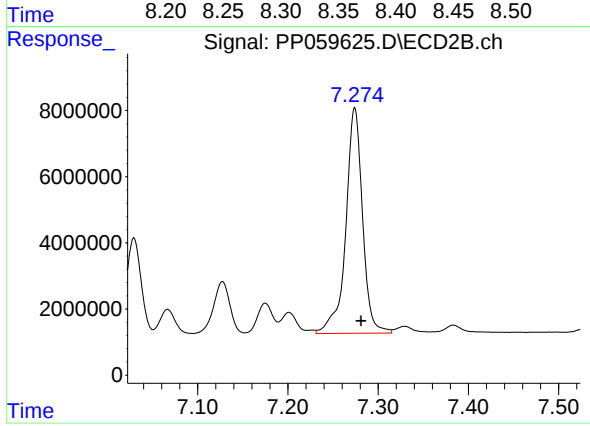

#35 AR-1260-5

R.T.: 7.274 min
Delta R.T.: -0.007 min
Response: 88075503
Conc: 504.06 ng/ml