

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082825\
 Data File : PP074703.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2025 11:40
 Operator : YP\AJ
 Sample : Q2968-02 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC271315LOZ-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/29/2025
 Supervised By :mohammad ahmed 09/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 12:08:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.656	3.795	2653980	6667388	2.169	1.379m#
2) SA Decachlor...	10.438	8.809	2162872	10311722	2.190	1.375m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082825\
Data File : PP074703.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2025 11:40
Operator : YP\AJ
Sample : Q2968-02 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC271315LOZ-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/29/2025
Supervised By :mohammad ahmed 09/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 12:08:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

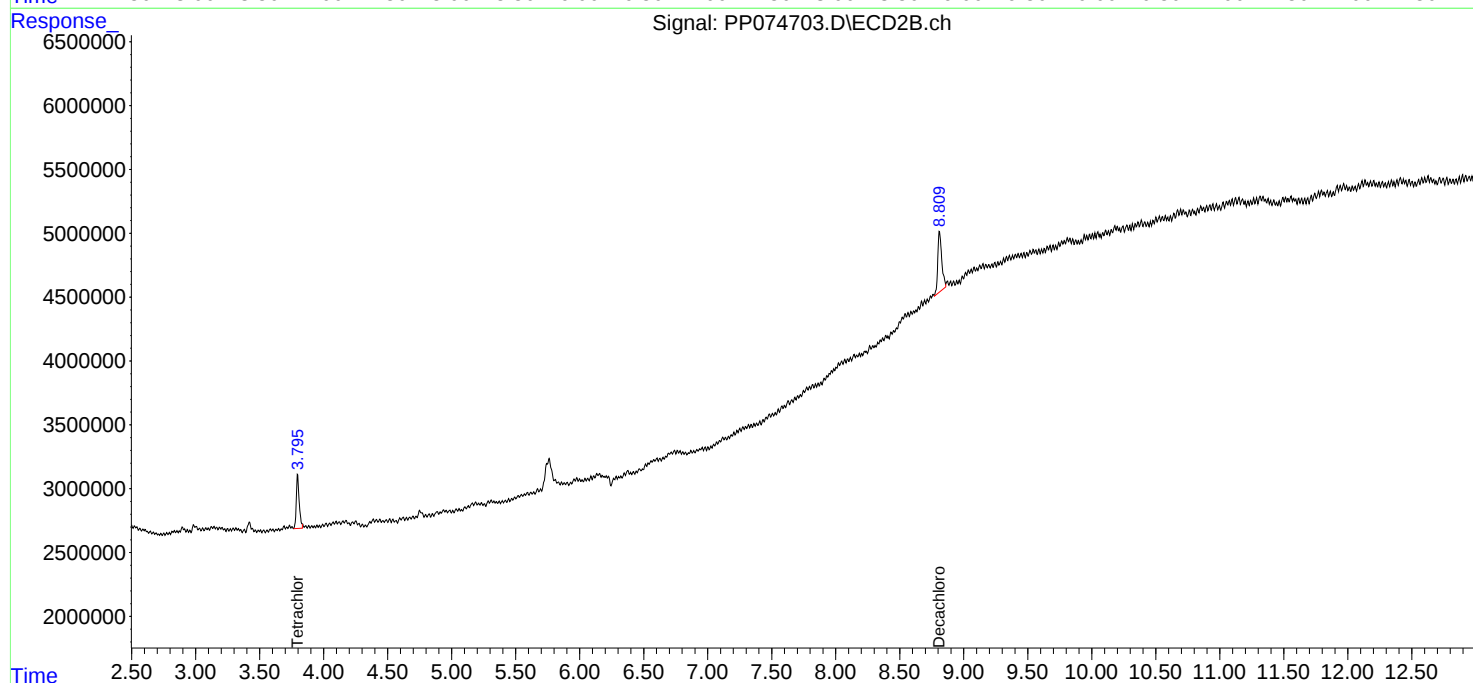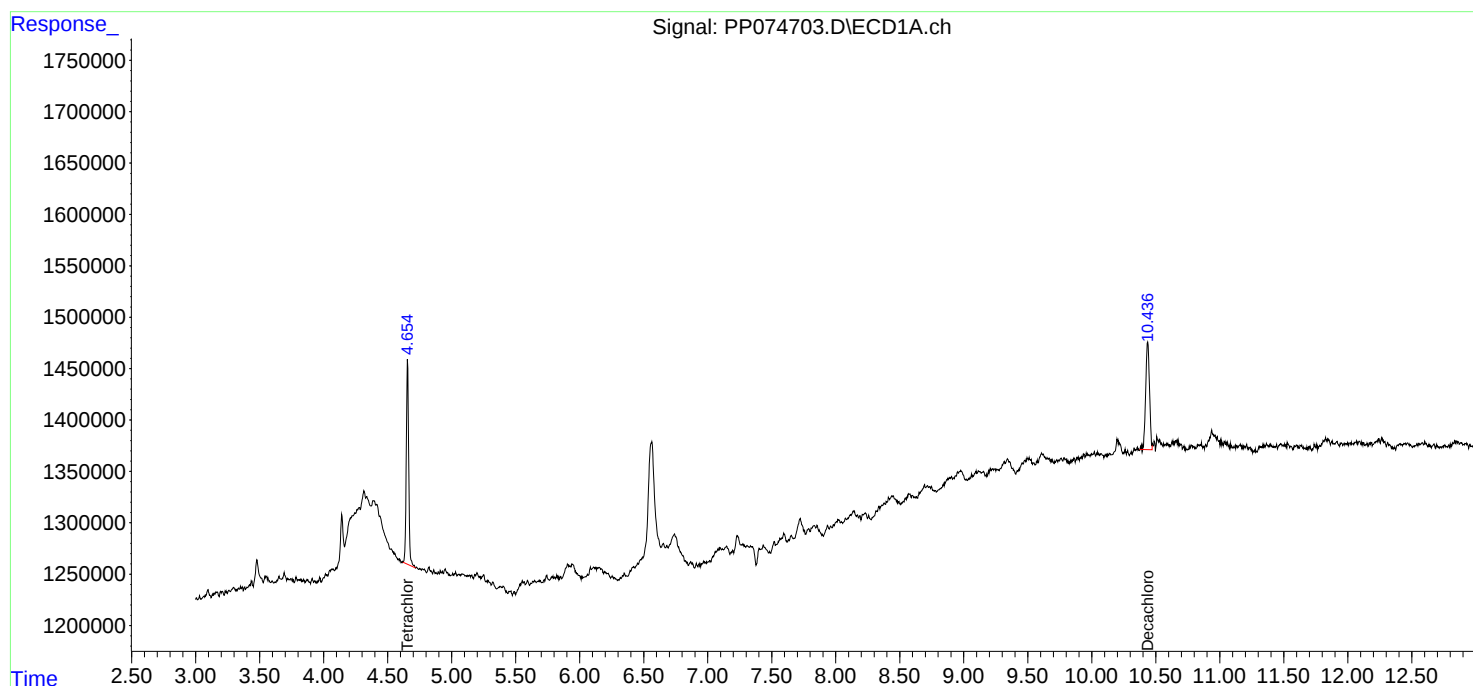

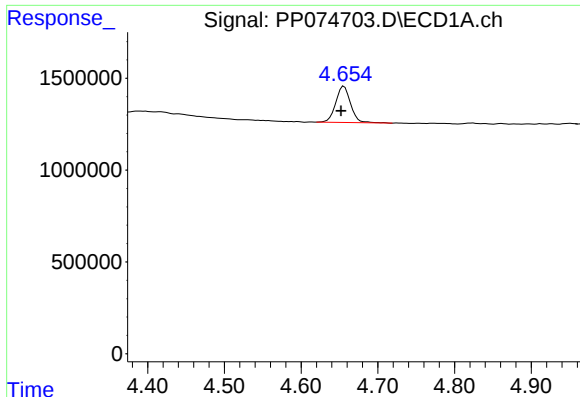


#1 Tetrachloro-m-xylene

R.T.: 4.656 min
Delta R.T.: 0.004 min
Response: 2653980
Conc: 2.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC271315LOZ-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/29/2025
Supervised By :mohammad ahmed 09/04/2025

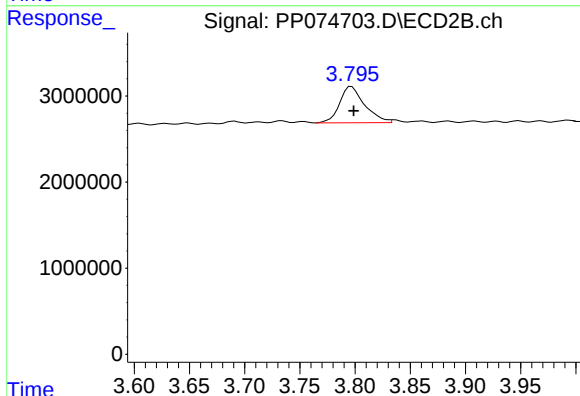


#1 Tetrachloro-m-xylene

R.T.: 3.795 min
Delta R.T.: -0.003 min
Response: 6667388
Conc: 1.38 ng/ml m

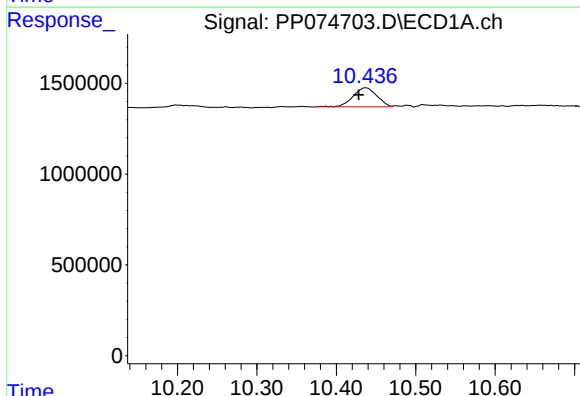

#2 Decachlorobiphenyl

R.T.: 10.438 min
Delta R.T.: 0.010 min
Response: 2162872
Conc: 2.19 ng/ml

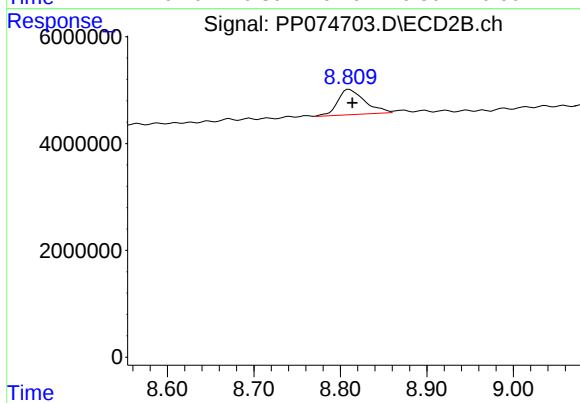

#2 Decachlorobiphenyl

R.T.: 8.809 min
Delta R.T.: -0.005 min
Response: 10311722
Conc: 1.38 ng/ml m