

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082925\
 Data File : PP074760.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2025 18:58
 Operator : YP\AJ
 Sample : Q2961-01 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 4075

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/04/2025
 Supervised By :mohammad ahmed 09/05/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 04:27:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.656	3.818	1668960	19152073	1.364	3.961m#
2) SA Decachlor...	10.436	8.809	1201362	5696072	1.217	0.760 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082925\
Data File : PP074760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2025 18:58
Operator : YP\AJ
Sample : Q2961-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
4075


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/04/2025
Supervised By :mohammad ahmed 09/05/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 04:27:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

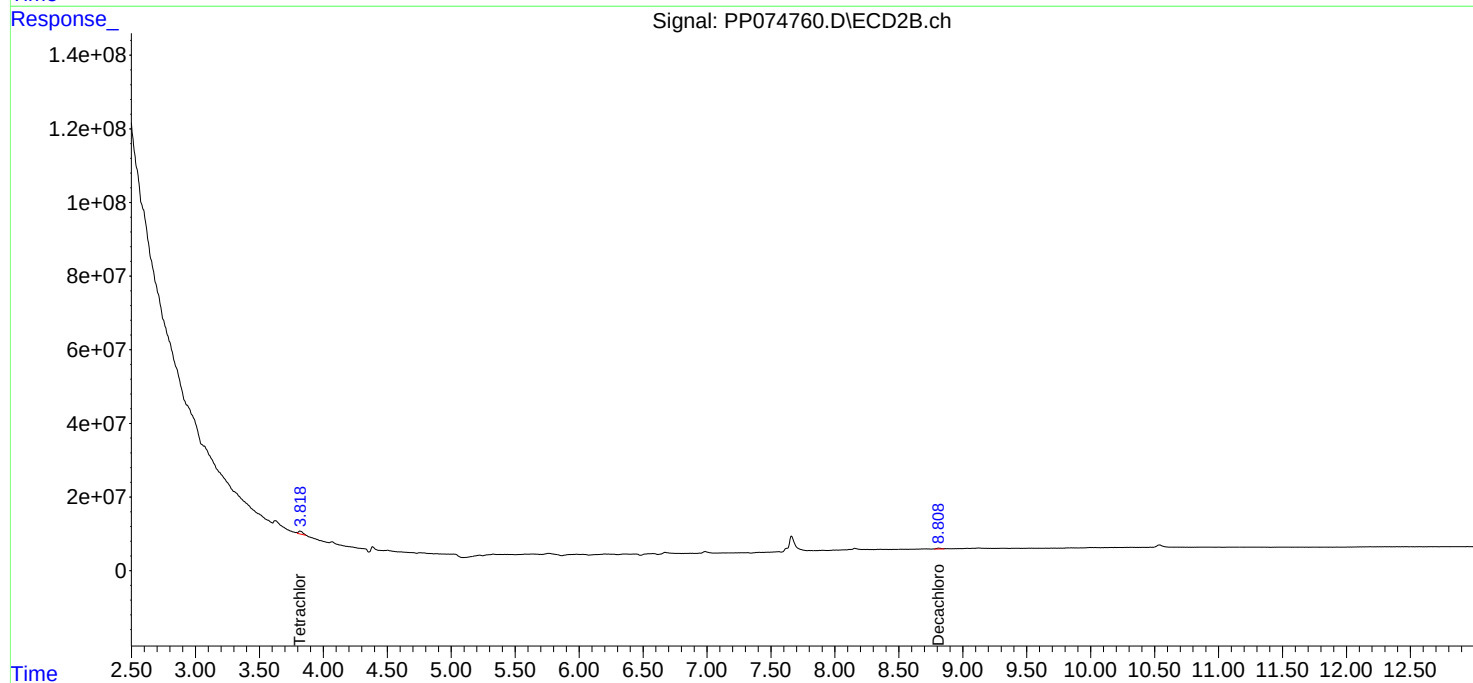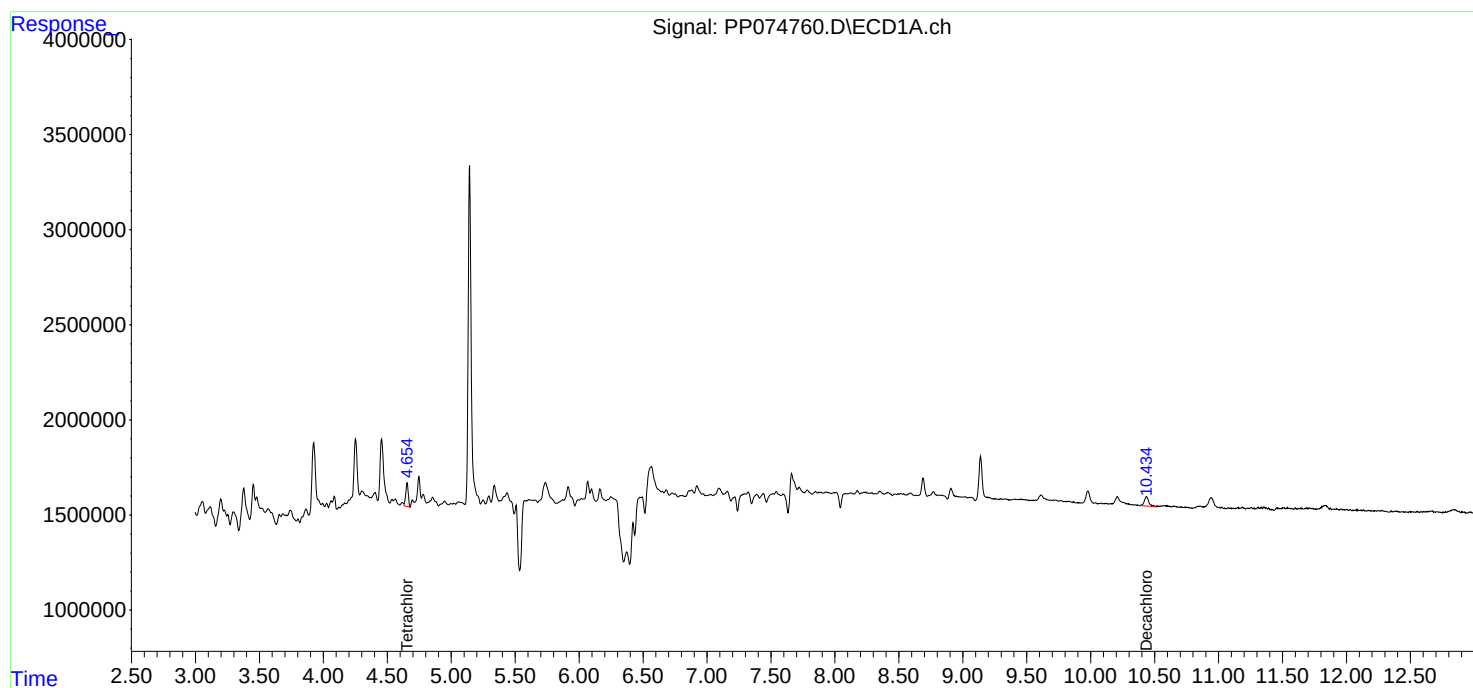

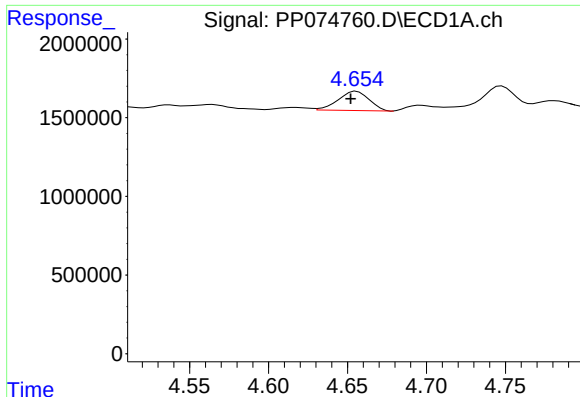


#1 Tetrachloro-m-xylene

R.T.: 4.656 min
Delta R.T.: 0.004 min
Response: 1668960
Conc: 1.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
4075


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/04/2025
Supervised By :mohammad ahmed 09/05/2025

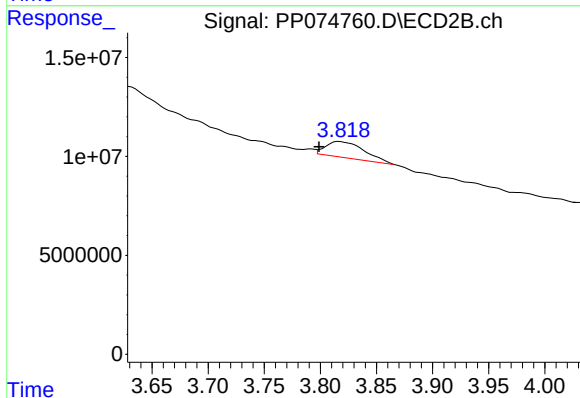


#1 Tetrachloro-m-xylene

R.T.: 3.818 min
Delta R.T.: 0.019 min
Response: 19152073
Conc: 3.96 ng/ml m

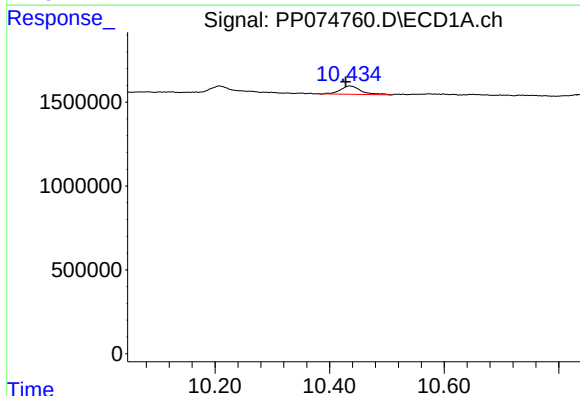

#2 Decachlorobiphenyl

R.T.: 10.436 min
Delta R.T.: 0.008 min
Response: 1201362
Conc: 1.22 ng/ml

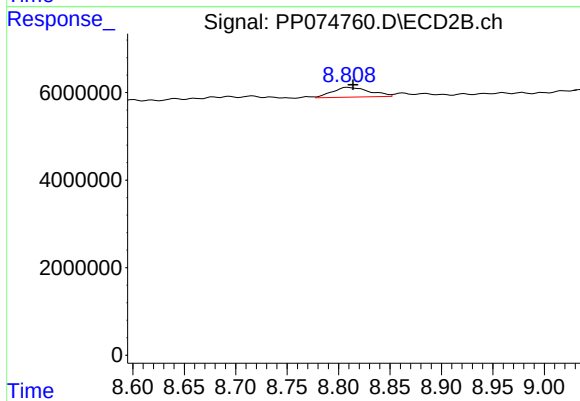

#2 Decachlorobiphenyl

R.T.: 8.809 min
Delta R.T.: -0.005 min
Response: 5696072
Conc: 0.76 ng/ml