

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083021\
 Data File : PP039022.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Aug 2021 10:42
 Operator : AJ\MA
 Sample : M2940-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 02:51:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 26 09:31:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.875	3.860	685490	447717	17.958	18.578
2)	SA Decachlor...	10.854	9.116	440303	432862	18.287	19.143
Target Compounds							
9)	L2 AR-1221-2	5.224	4.211	18748	10753	56.281	53.730
10)	L2 AR-1221-3	5.311	4.299	39694	16106	39.711	24.479 #
11)	L3 AR-1232-1	5.311	4.299	39694	16106	43.427	26.981 #
28)	L6 AR-1254-3	7.737f	6.573f	16457	10500	10.682	6.044 #
33)	L7 AR-1260-3	8.536f	0.000	1208	0	1.370	N.D. #
34)	L7 AR-1260-4	8.760	0.000	7352	0	7.264	N.D. #
36)	L8 AR-1262-1	8.536f	0.000	1208	0	0.905	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083021\
Data File : PP039022.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2021 10:42
Operator : AJ\MA
Sample : M2940-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 02:51:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 26 09:31:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

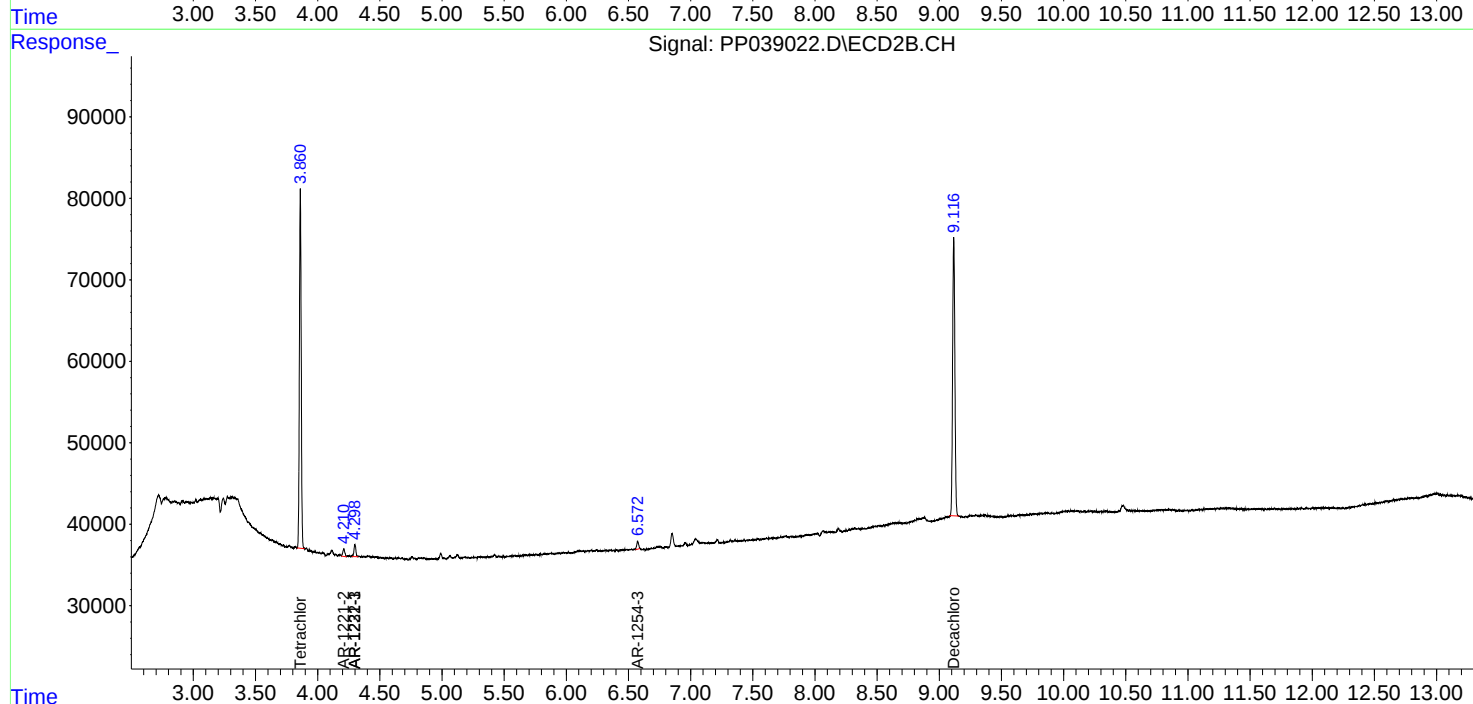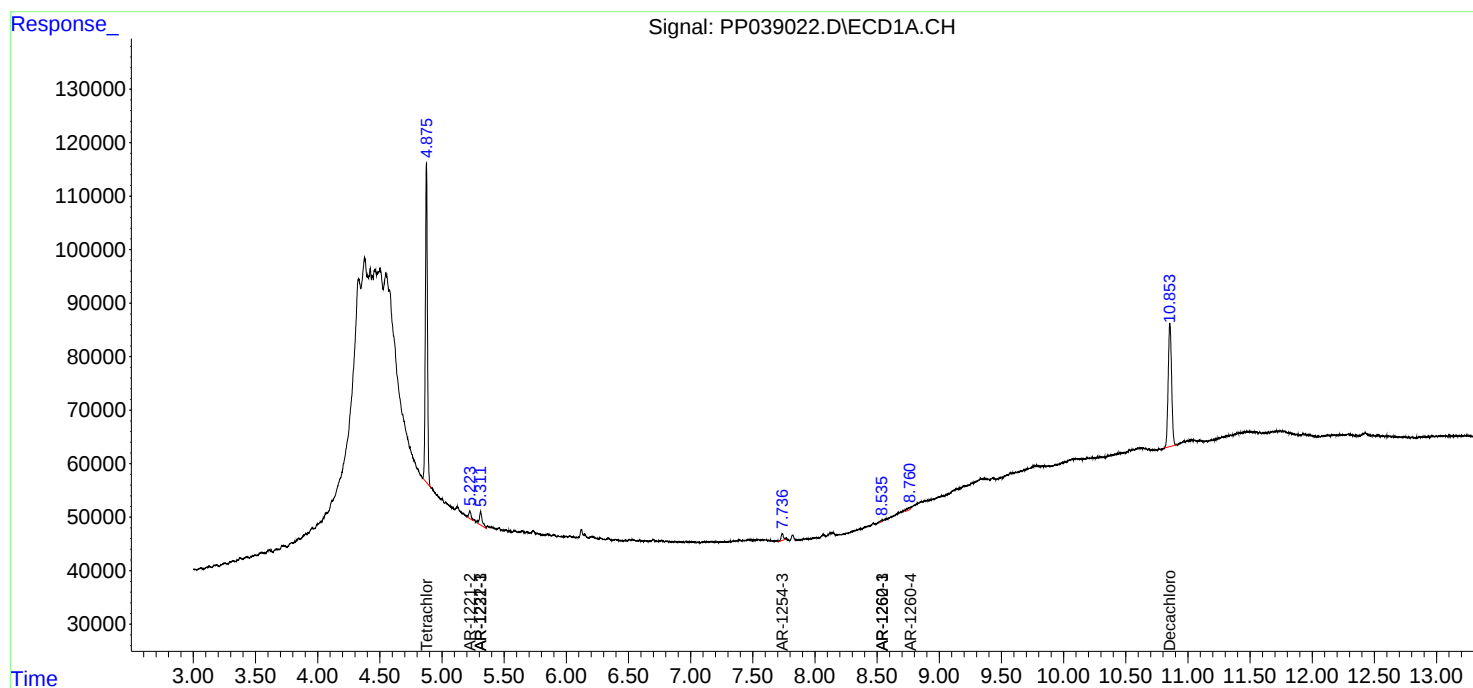


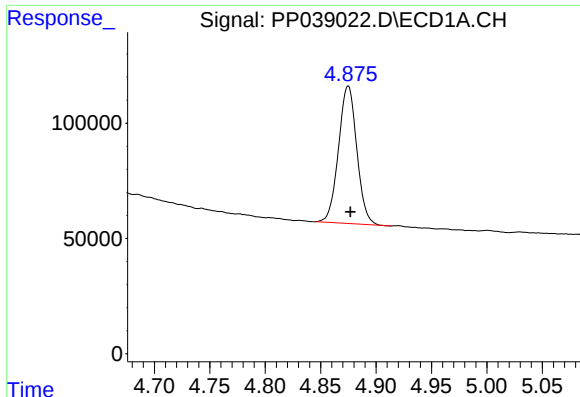

#1 Tetrachloro-m-xylene


R.T.: 4.875 min
Delta R.T.: -0.002 min
Response: 685490
Conc: 17.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

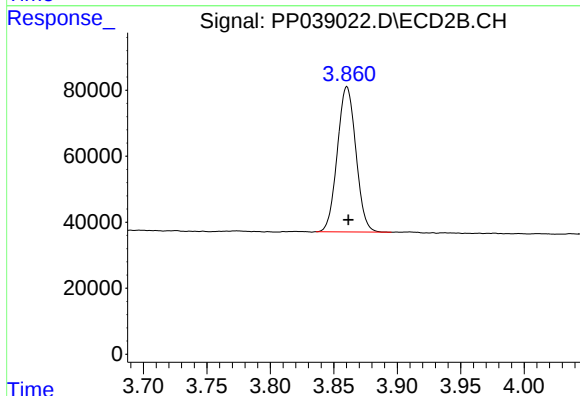


#1 Tetrachloro-m-xylene

R.T.: 3.860 min
Delta R.T.: -0.001 min
Response: 447717
Conc: 18.58 ng/ml

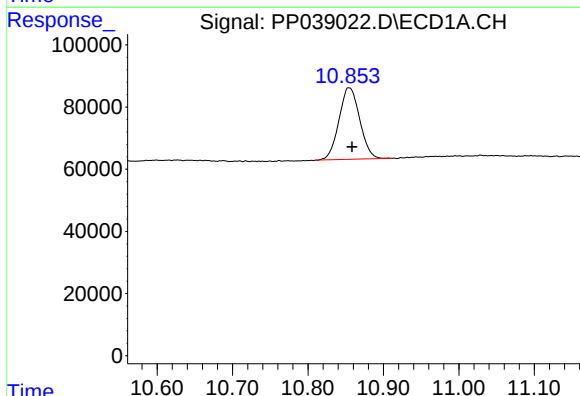


#2 Decachlorobiphenyl

R.T.: 10.854 min
Delta R.T.: -0.005 min
Response: 440303
Conc: 18.29 ng/ml

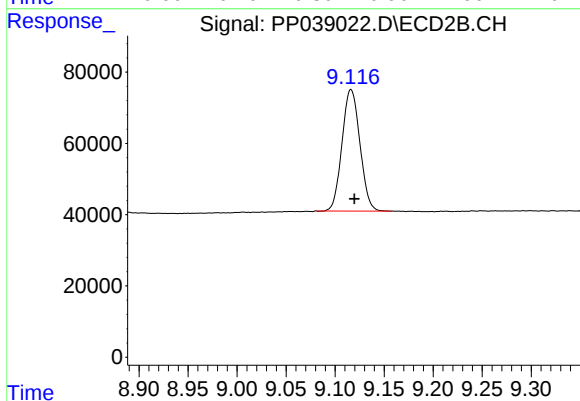

#2 Decachlorobiphenyl


R.T.: 9.116 min
Delta R.T.: -0.004 min
Response: 432862
Conc: 19.14 ng/ml

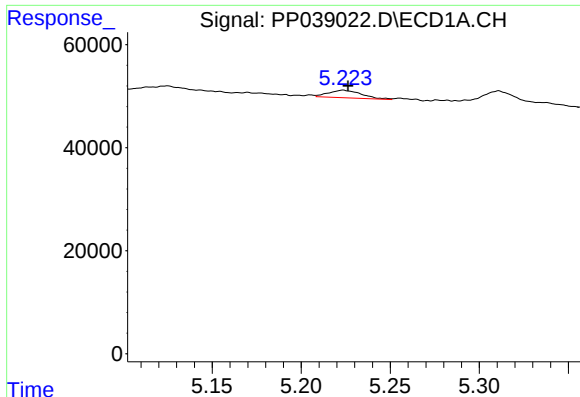

#9 AR-1221-2


R.T.: 5.224 min
Delta R.T.: -0.003 min
Response: 18748
Conc: 56.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

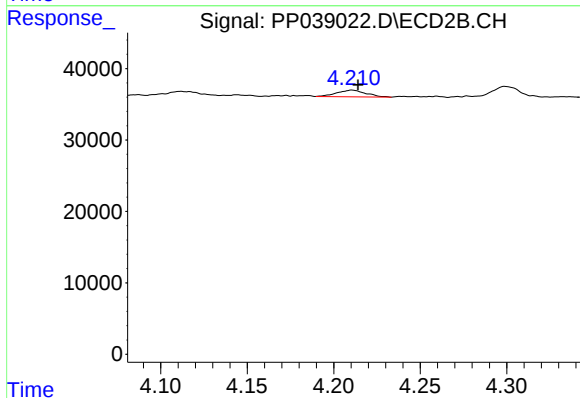


#9 AR-1221-2

R.T.: 4.211 min
Delta R.T.: -0.003 min
Response: 10753
Conc: 53.73 ng/ml

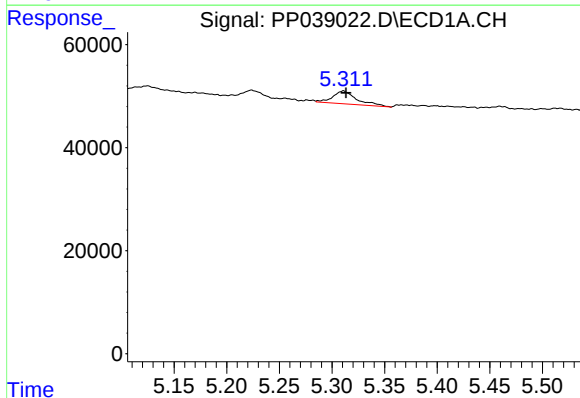


#10 AR-1221-3

R.T.: 5.311 min
Delta R.T.: -0.002 min
Response: 39694
Conc: 39.71 ng/ml

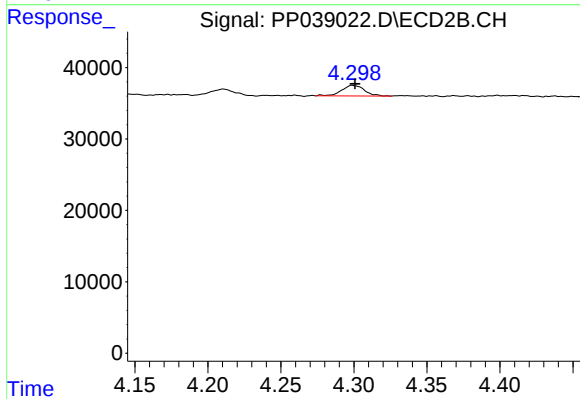

#10 AR-1221-3


R.T.: 4.299 min
Delta R.T.: -0.002 min
Response: 16106
Conc: 24.48 ng/ml

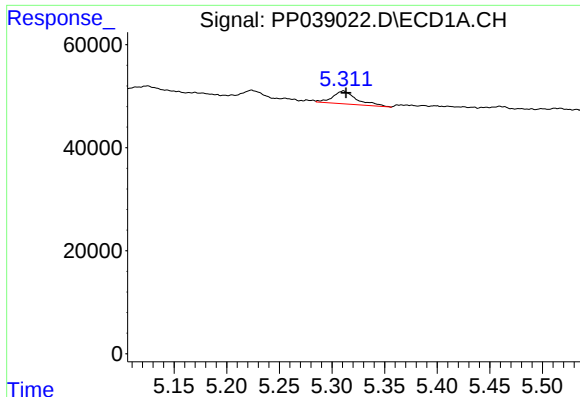

#11 AR-1232-1


R.T.: 5.311 min
Delta R.T.: -0.002 min
Response: 39694
Conc: 43.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

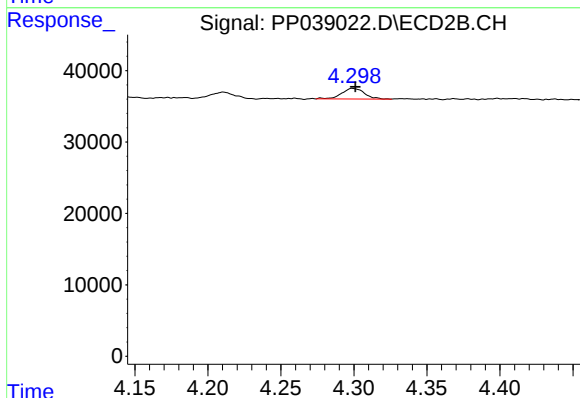


#11 AR-1232-1

R.T.: 4.299 min
Delta R.T.: -0.002 min
Response: 16106
Conc: 26.98 ng/ml

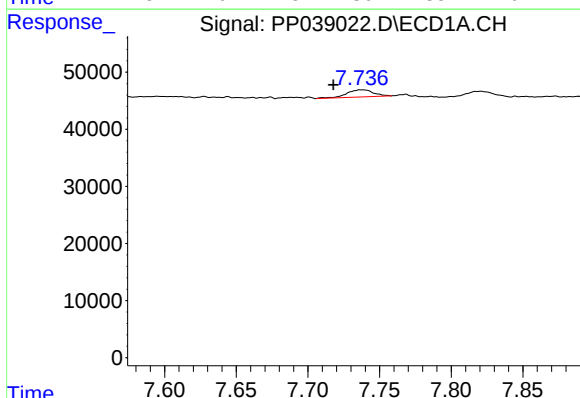


#28 AR-1254-3

R.T.: 7.737 min
Delta R.T.: 0.019 min
Response: 16457
Conc: 10.68 ng/ml

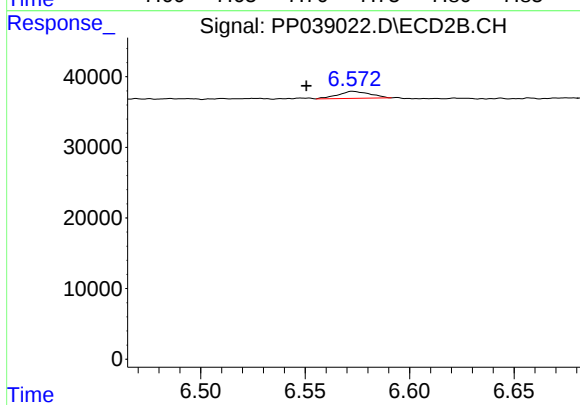

#28 AR-1254-3


R.T.: 6.573 min
Delta R.T.: 0.022 min
Response: 10500
Conc: 6.04 ng/ml

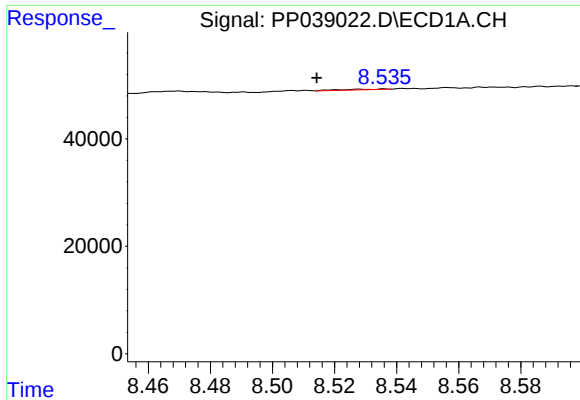

#33 AR-1260-3


R.T.: 8.536 min
Delta R.T.: 0.022 min
Response: 1208
Conc: 1.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

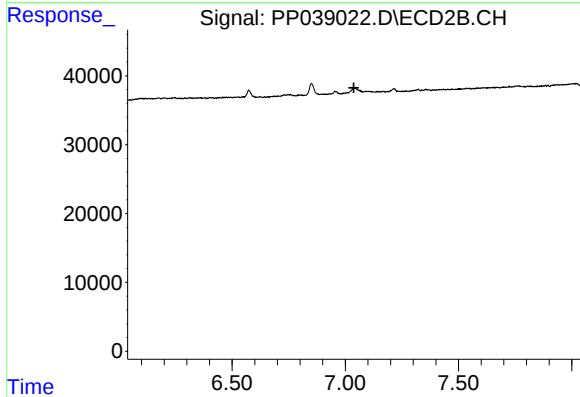


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.038 min
Response: 0
Conc: N.D.

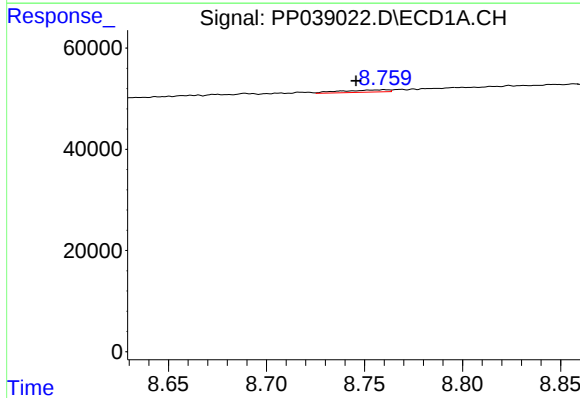


#34 AR-1260-4

R.T.: 8.760 min
Delta R.T.: 0.015 min
Response: 7352
Conc: 7.26 ng/ml

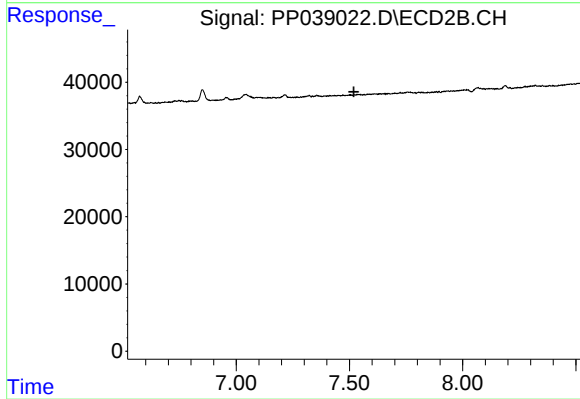

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.520 min
Response: 0
Conc: N.D.

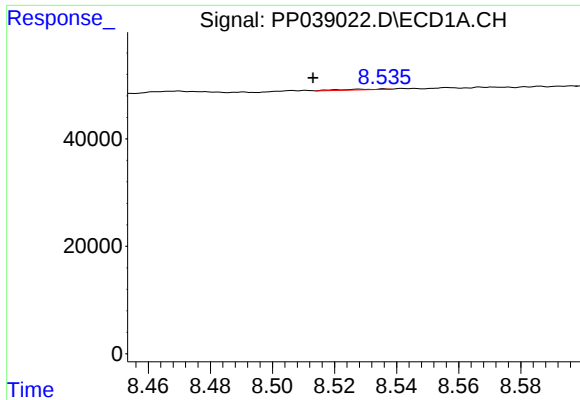

#36 AR-1262-1

R.T.: 8.536 min
Delta R.T.: 0.023 min
Response: 1208
Conc: 0.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

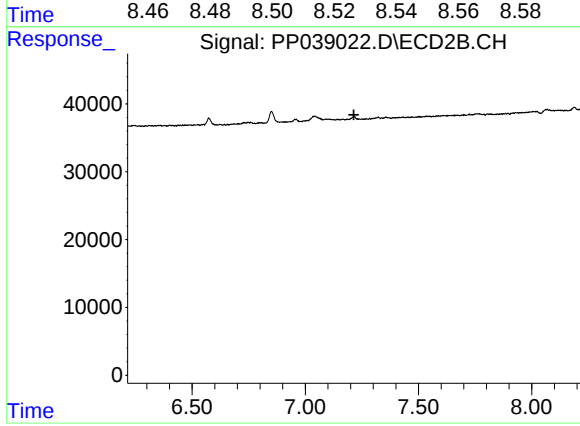

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.215 min
Response: 0
Conc: N.D.