

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083021\
 Data File : PP039042.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Aug 2021 17:29
 Operator : AJ\MA
 Sample : M3561-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DUPLICATE-082521

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 02:58:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 26 09:31:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.875	3.861	826529	532899	21.653	22.112
2)	SA Decachlor...	10.856	9.117	395917	402426	16.444	17.797
Target Compounds							
8)	L2 AR-1221-1	5.127	0.000	28350	0	62.940	N.D. #
9)	L2 AR-1221-2	5.230	0.000	10864	0	32.613	N.D. #
24)	L5 AR-1248-4	7.131	0.000	8760	0	8.336	N.D. #
26)	L6 AR-1254-1	7.131f	0.000	8760	0	8.396	N.D. #
28)	L6 AR-1254-3	7.736f	0.000	5378	0	3.491	N.D. #
33)	L7 AR-1260-3	8.504	7.051	3682	17149	4.176	12.410 #
34)	L7 AR-1260-4	8.747	0.000	7808	0	7.715	N.D. #
36)	L8 AR-1262-1	8.504	0.000	3682	0	2.757	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083021\
Data File : PP039042.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2021 17:29
Operator : AJ\MA
Sample : M3561-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DUPLICATE-082521

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 02:58:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 26 09:31:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

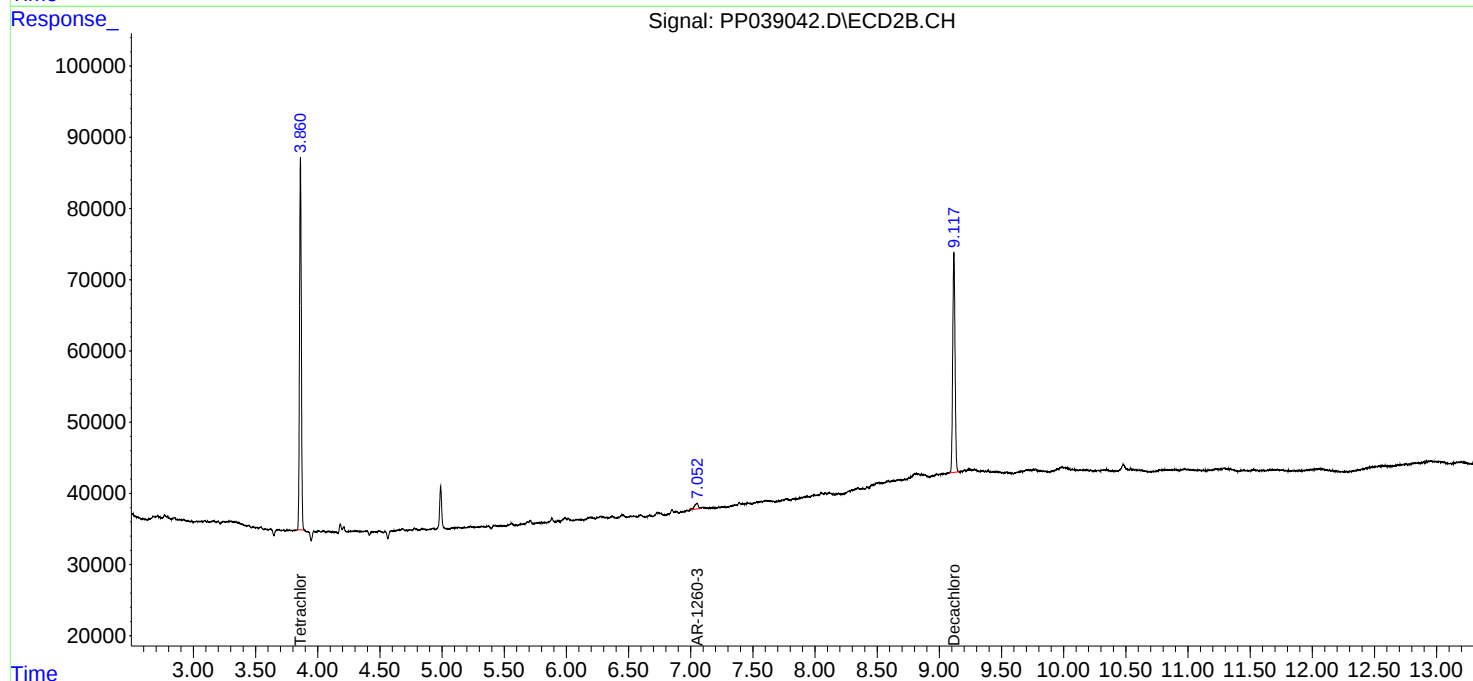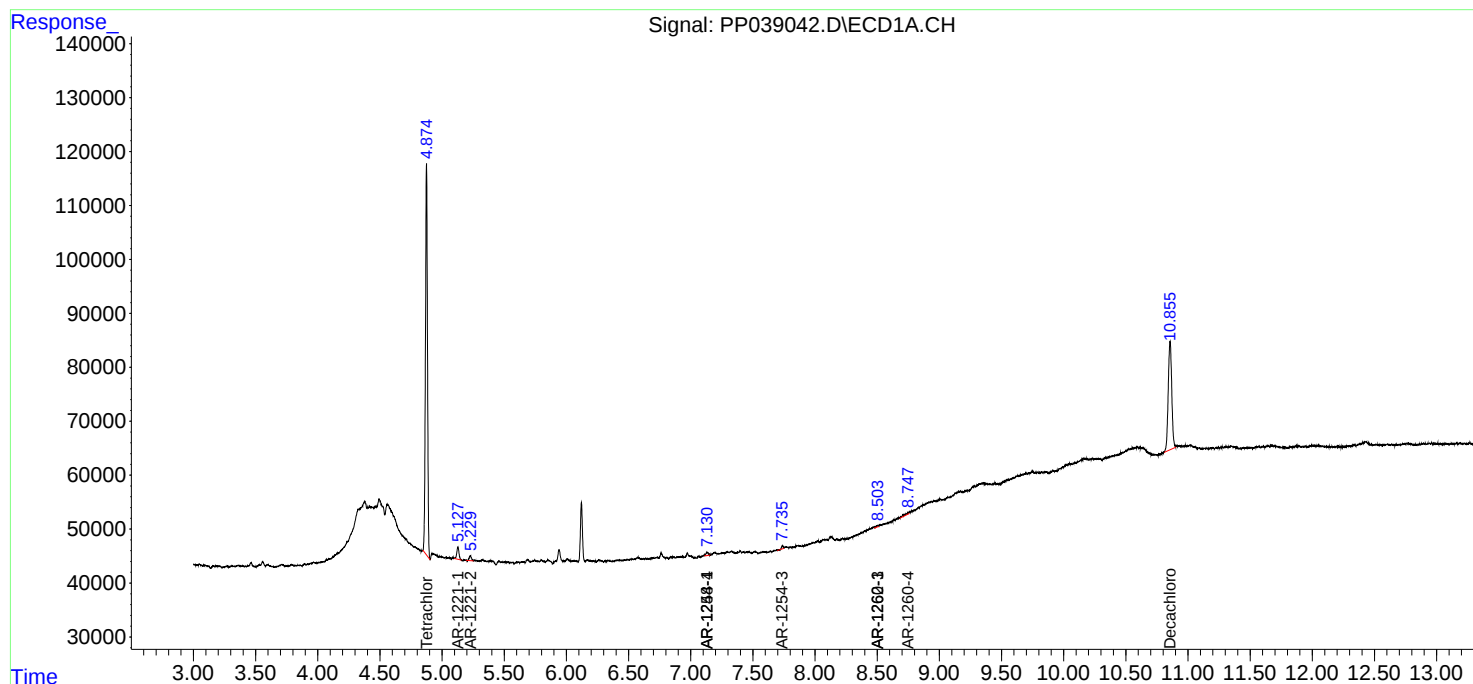


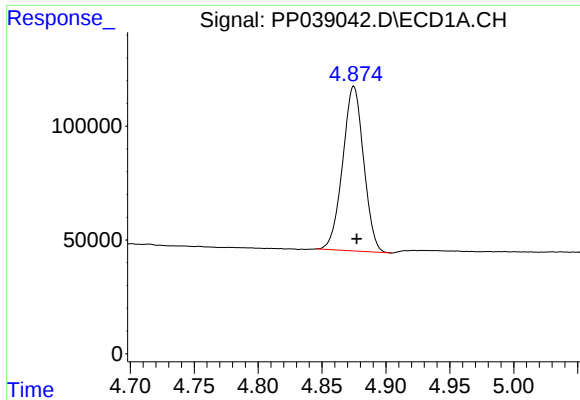

#1 Tetrachloro-m-xylene


R.T.: 4.875 min
Delta R.T.: -0.002 min
Response: 826529
Conc: 21.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
DUPLICATE-082521

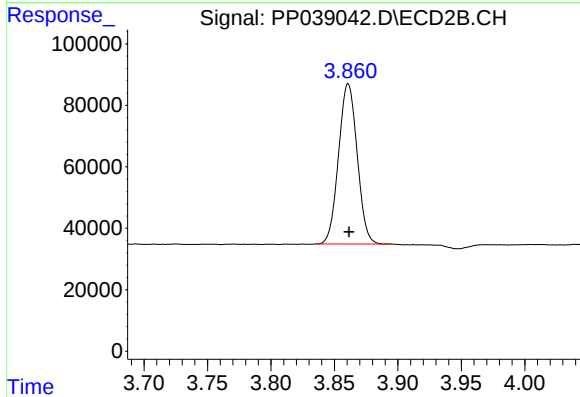


#1 Tetrachloro-m-xylene

R.T.: 3.861 min
Delta R.T.: 0.000 min
Response: 532899
Conc: 22.11 ng/ml

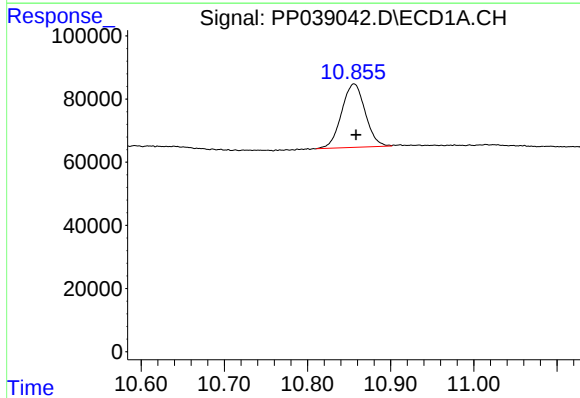


#2 Decachlorobiphenyl

R.T.: 10.856 min
Delta R.T.: -0.003 min
Response: 395917
Conc: 16.44 ng/ml

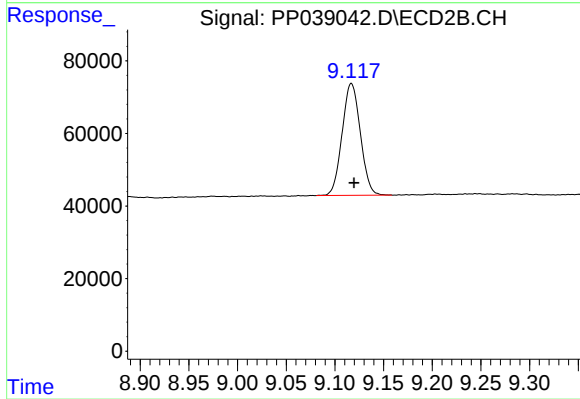

#2 Decachlorobiphenyl


R.T.: 9.117 min
Delta R.T.: -0.003 min
Response: 402426
Conc: 17.80 ng/ml

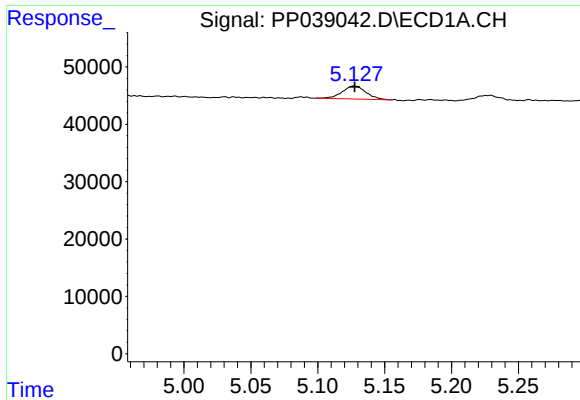

#8 AR-1221-1


R.T.: 5.127 min
Delta R.T.: 0.000 min
Response: 28350
Conc: 62.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
DUPLICATE-082521

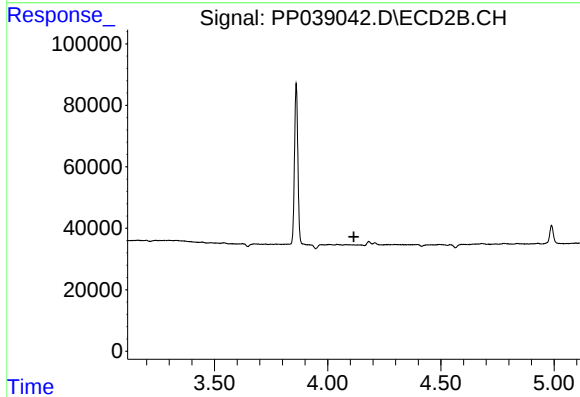


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.116 min
Response: 0
Conc: N.D.

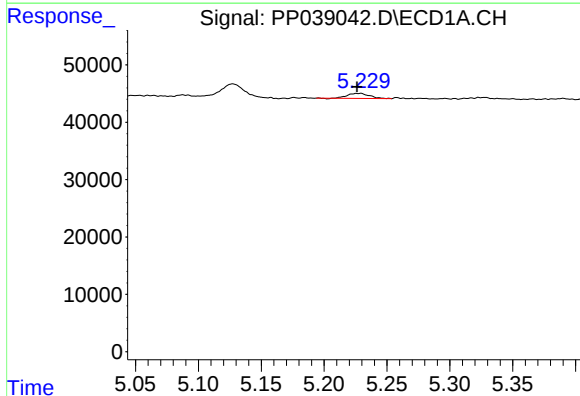


#9 AR-1221-2

R.T.: 5.230 min
Delta R.T.: 0.003 min
Response: 10864
Conc: 32.61 ng/ml

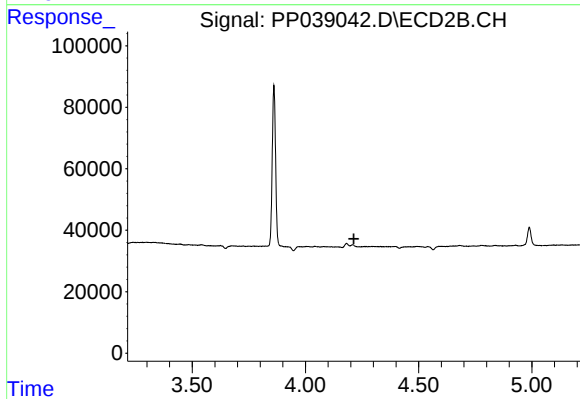

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.214 min
Response: 0
Conc: N.D.

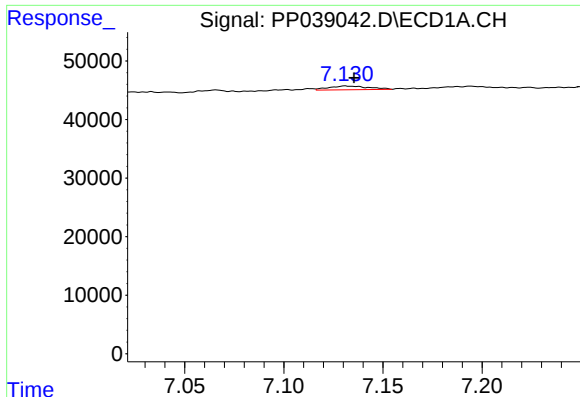

#24 AR-1248-4


R.T.: 7.131 min
Delta R.T.: -0.005 min
Response: 8760
Conc: 8.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
DUPLICATE-082521

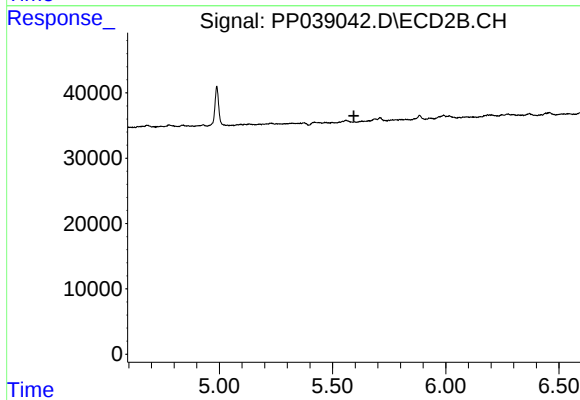


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.594 min
Response: 0
Conc: N.D.

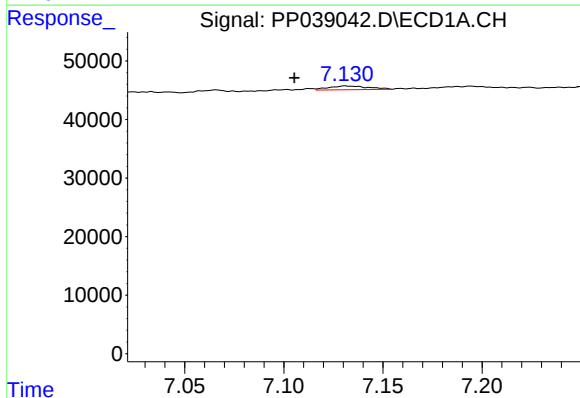


#26 AR-1254-1

R.T.: 7.131 min
Delta R.T.: 0.025 min
Response: 8760
Conc: 8.40 ng/ml

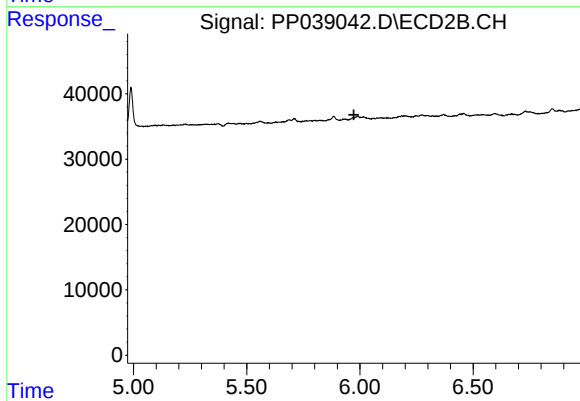

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.973 min
Response: 0
Conc: N.D.

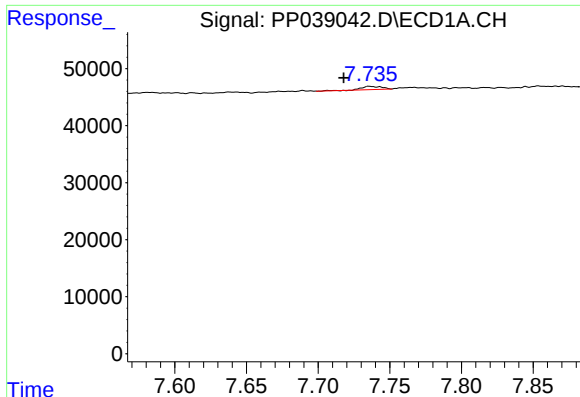

#28 AR-1254-3


R.T.: 7.736 min
Delta R.T.: 0.018 min
Response: 5378
Conc: 3.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
DUPLICATE-082521

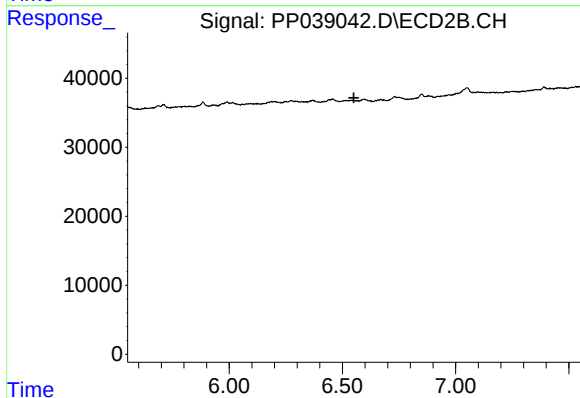


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.551 min
Response: 0
Conc: N.D.

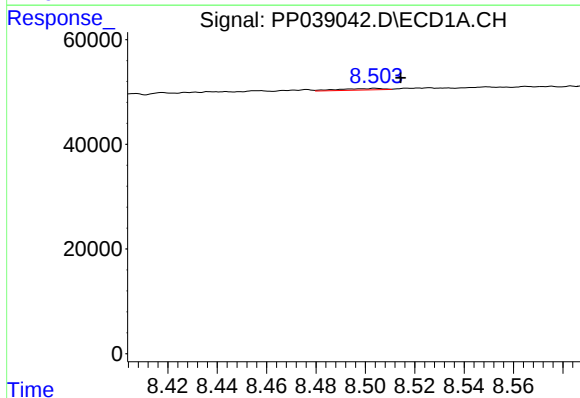


#33 AR-1260-3

R.T.: 8.504 min
Delta R.T.: -0.010 min
Response: 3682
Conc: 4.18 ng/ml

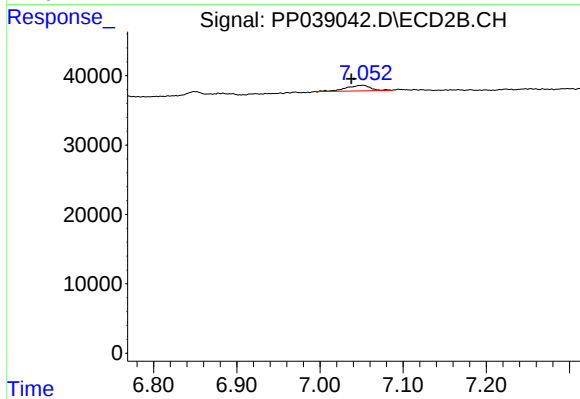

#33 AR-1260-3


R.T.: 7.051 min
Delta R.T.: 0.013 min
Response: 17149
Conc: 12.41 ng/ml

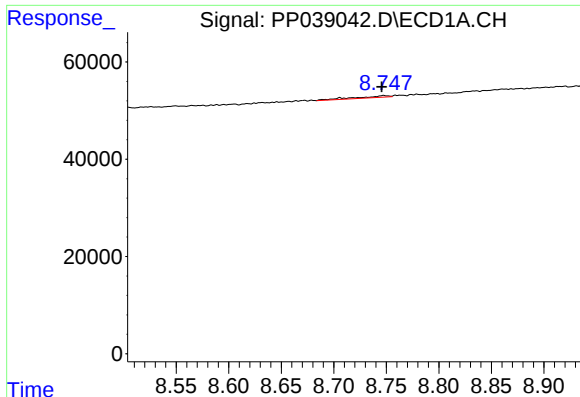

#34 AR-1260-4


R.T.: 8.747 min
Delta R.T.: 0.002 min
Response: 7808
Conc: 7.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
DUPLICATE-082521

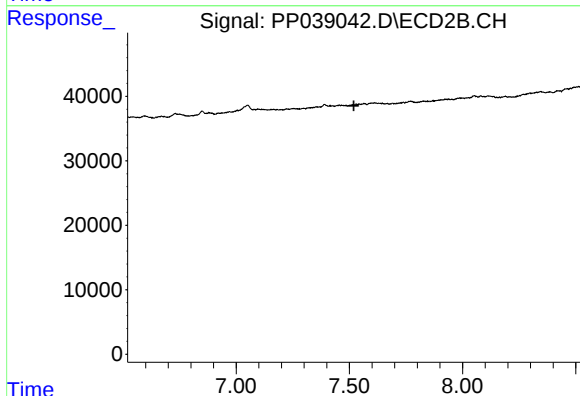


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.520 min
Response: 0
Conc: N.D.

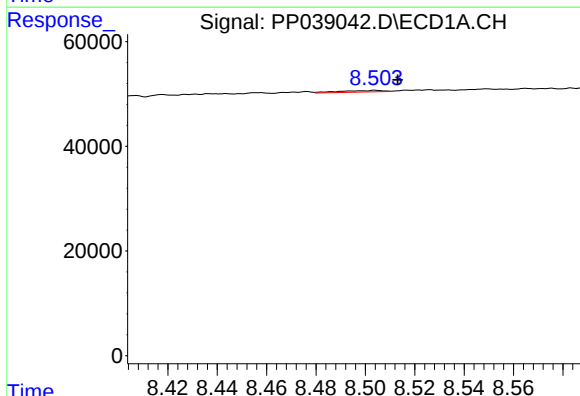

#36 AR-1262-1

R.T.: 8.504 min
Delta R.T.: -0.009 min
Response: 3682
Conc: 2.76 ng/ml

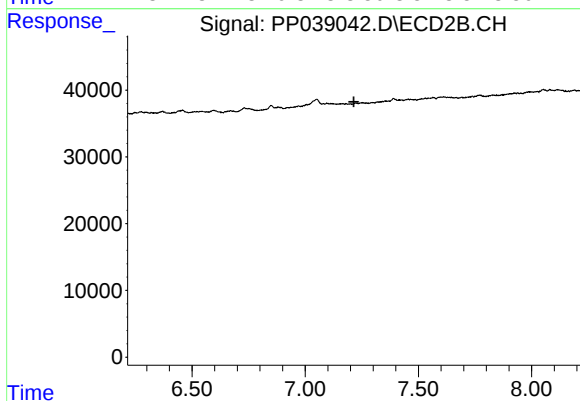

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.215 min
Response: 0
Conc: N.D.