

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083021\
 Data File : PP039054.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Aug 2021 21:26
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 03:02:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 26 09:31:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.874	3.860	916048	571148	23.998	23.700
2)	SA Decachlor...	10.853	9.116	572990	581440	23.798	25.714
Target Compounds							
9)	L2 AR-1221-2	5.225	0.000	9806	0	29.439	N.D. #
28)	L6 AR-1254-3	7.738f	0.000	10241	0	6.647	N.D. #
30)	L6 AR-1254-5	8.454	0.000	2905	0	2.573	N.D. #
32)	L7 AR-1260-2	8.123f	0.000	10625	0	8.821	N.D. #
33)	L7 AR-1260-3	8.502	0.000	2047	0	2.322	N.D. #
34)	L7 AR-1260-4	8.758	0.000	5943	0	5.872	N.D. #
36)	L8 AR-1262-1	8.502	0.000	2047	0	1.533	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083021\
Data File : PP039054.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2021 21:26
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 03:02:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 26 09:31:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

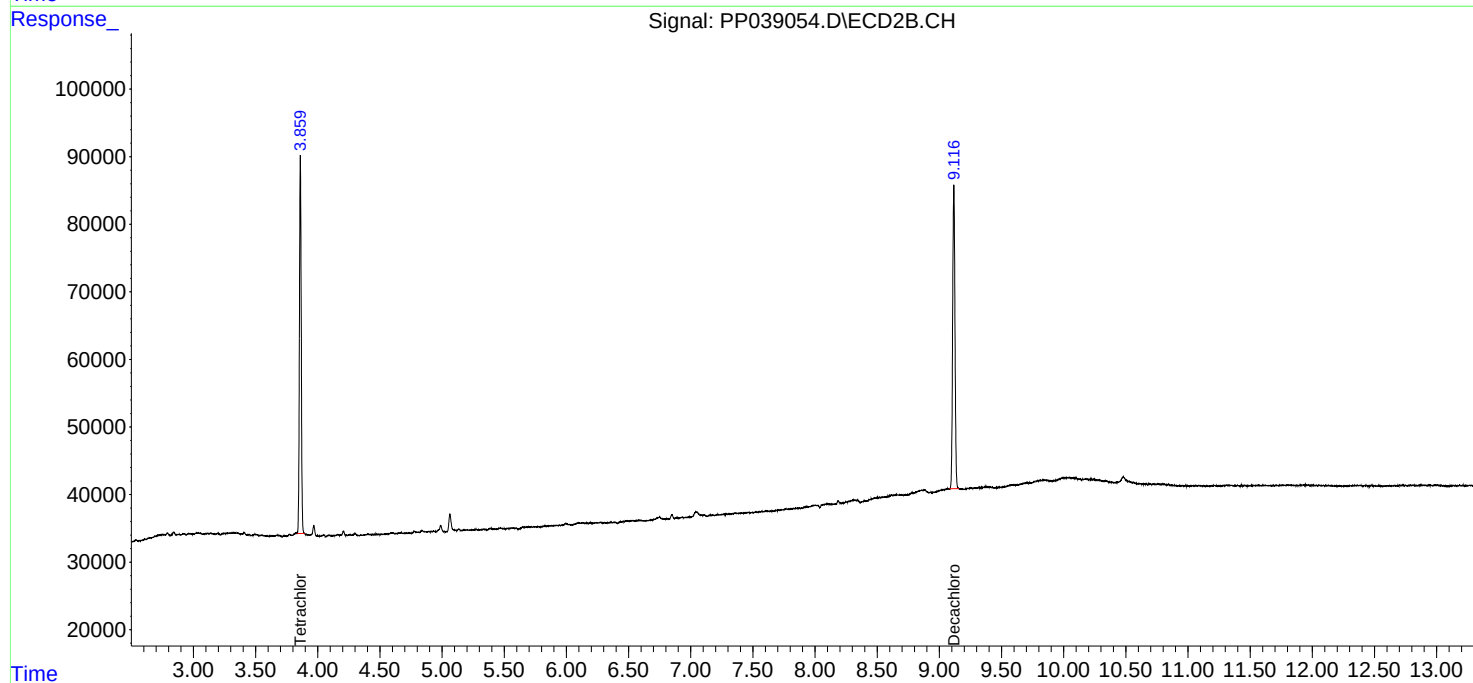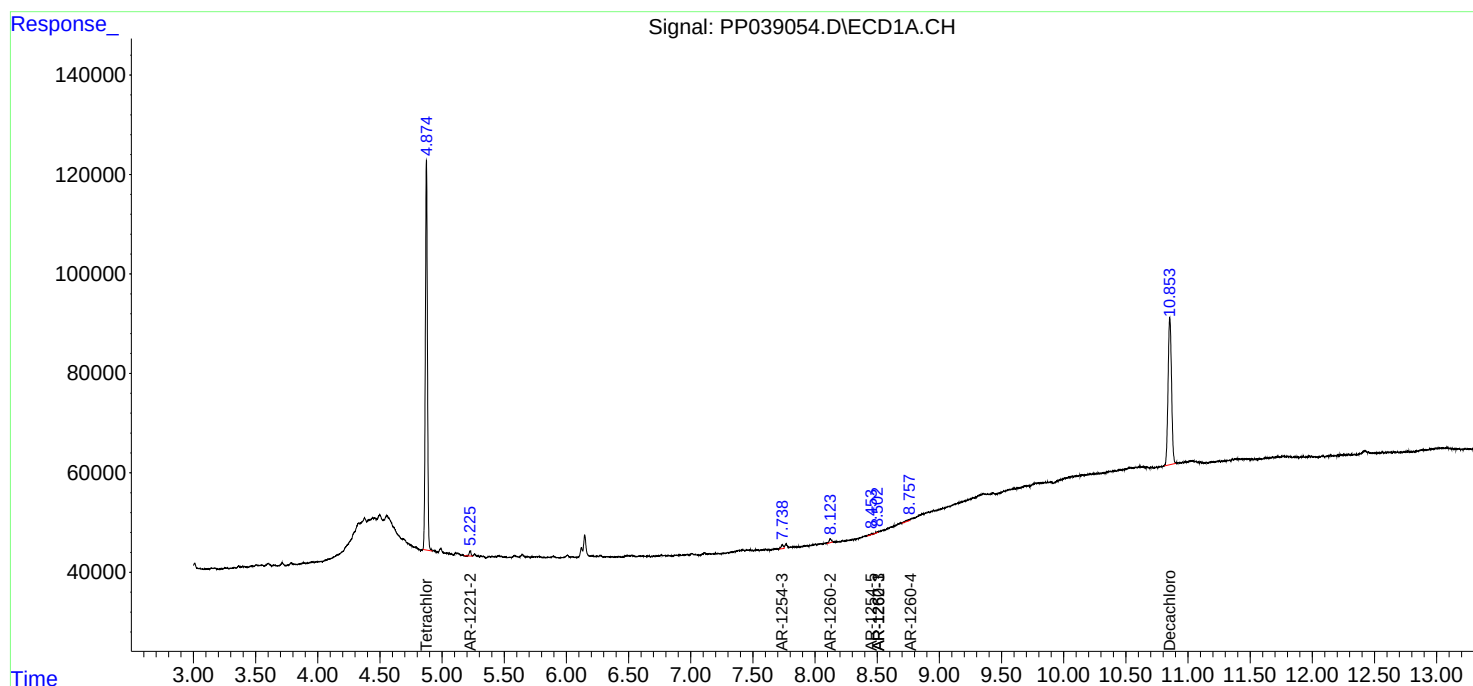


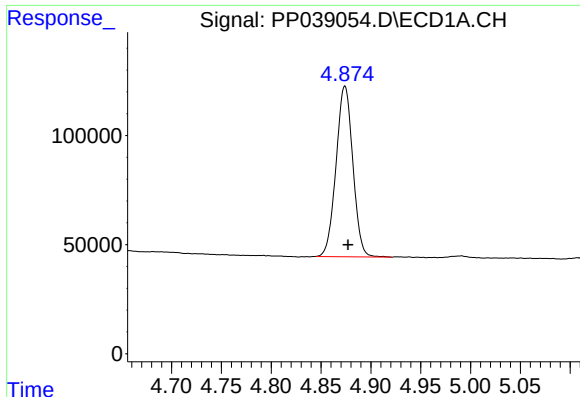

#1 Tetrachloro-m-xylene


R.T.: 4.874 min
Delta R.T.: -0.003 min
Response: 916048
Conc: 24.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

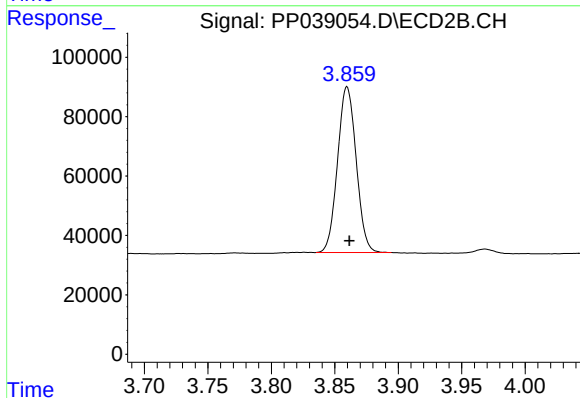


#1 Tetrachloro-m-xylene

R.T.: 3.860 min
Delta R.T.: -0.002 min
Response: 571148
Conc: 23.70 ng/ml

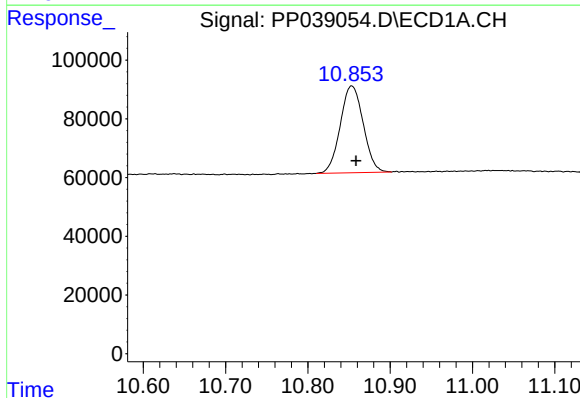


#2 Decachlorobiphenyl

R.T.: 10.853 min
Delta R.T.: -0.005 min
Response: 572990
Conc: 23.80 ng/ml

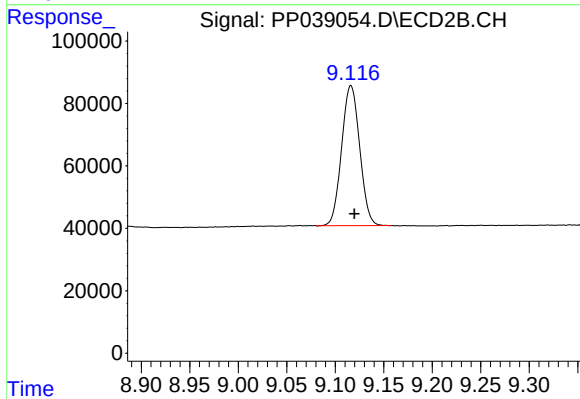

#2 Decachlorobiphenyl


R.T.: 9.116 min
Delta R.T.: -0.004 min
Response: 581440
Conc: 25.71 ng/ml

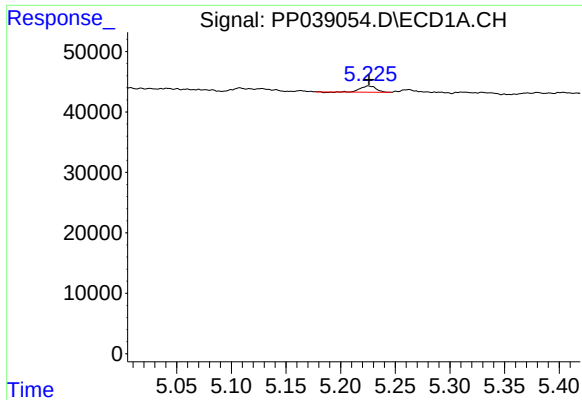

#9 AR-1221-2


R.T.: 5.225 min
Delta R.T.: 0.000 min
Response: 9806
Conc: 29.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

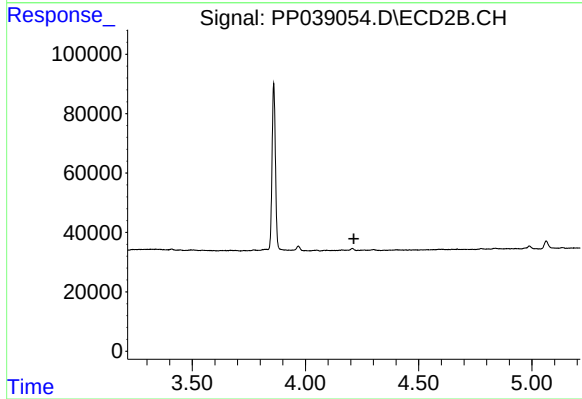


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.214 min
Response: 0
Conc: N.D.

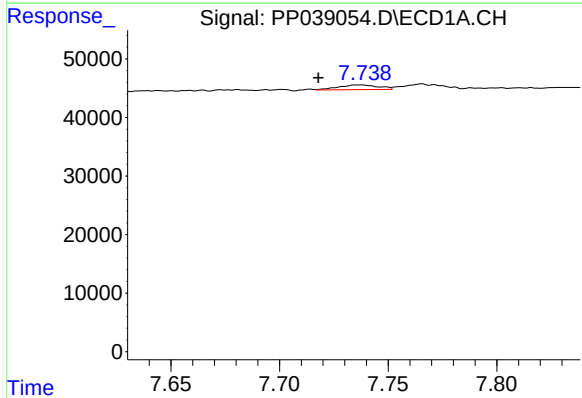


#28 AR-1254-3

R.T.: 7.738 min
Delta R.T.: 0.020 min
Response: 10241
Conc: 6.65 ng/ml

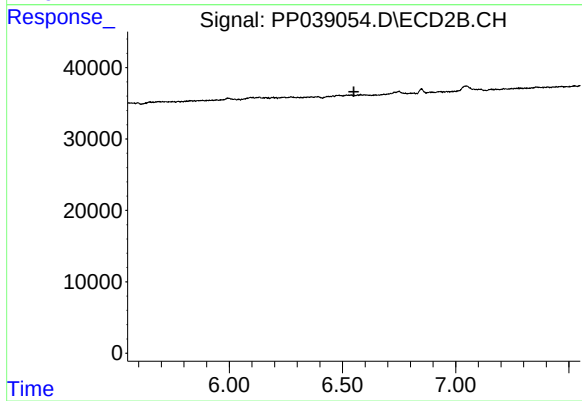

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.551 min
Response: 0
Conc: N.D.

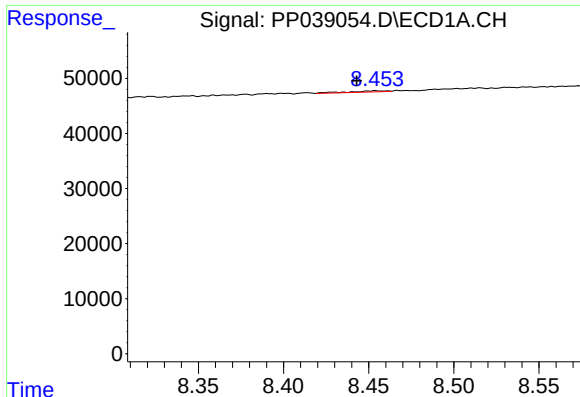

#30 AR-1254-5


R.T.: 8.454 min
Delta R.T.: 0.011 min
Response: 2905
Conc: 2.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

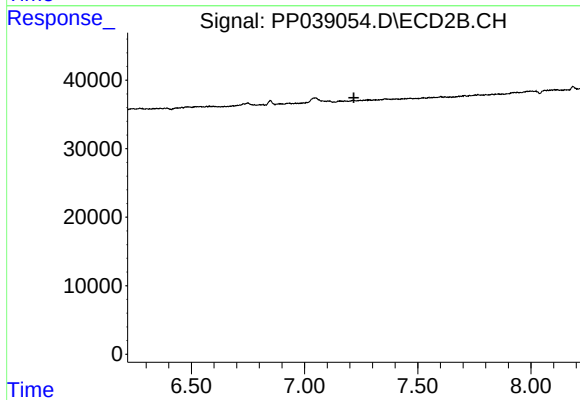


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.218 min
Response: 0
Conc: N.D.

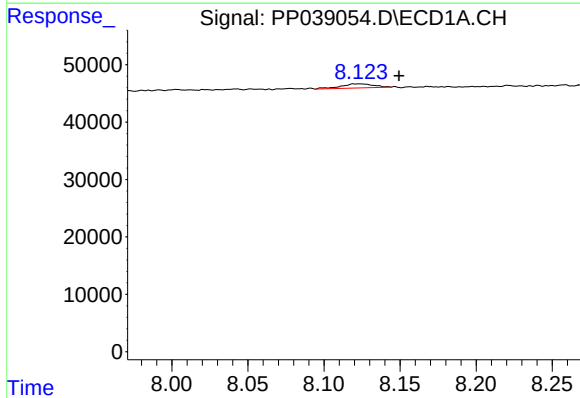


#32 AR-1260-2

R.T.: 8.123 min
Delta R.T.: -0.026 min
Response: 10625
Conc: 8.82 ng/ml

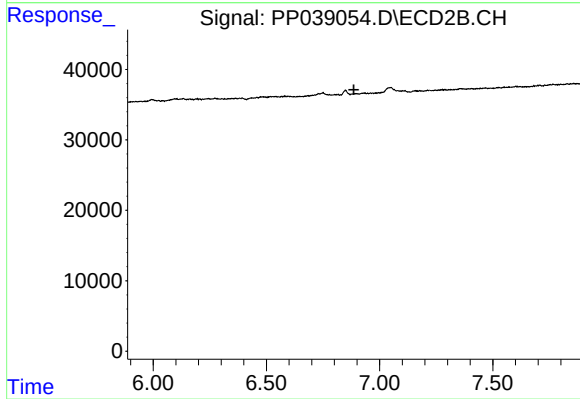

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.886 min
Response: 0
Conc: N.D.

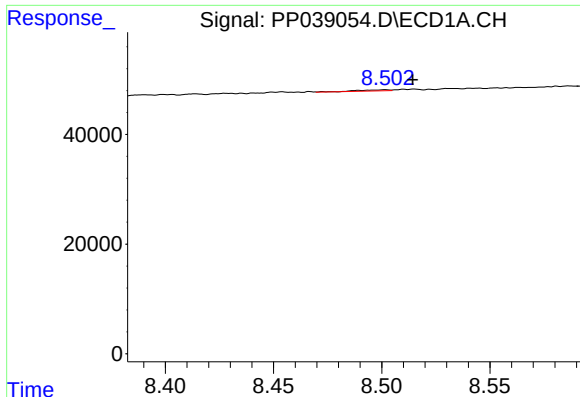

#33 AR-1260-3


R.T.: 8.502 min
Delta R.T.: -0.012 min
Response: 2047
Conc: 2.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

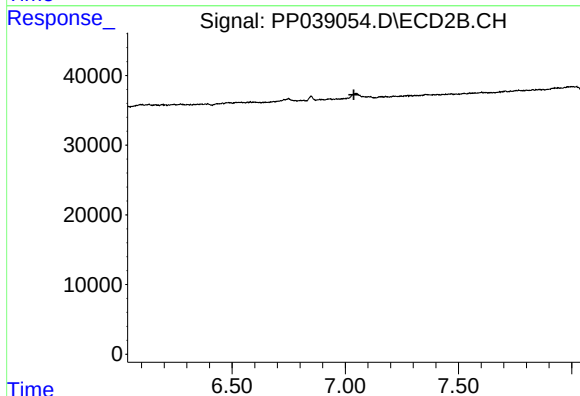


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.038 min
Response: 0
Conc: N.D.

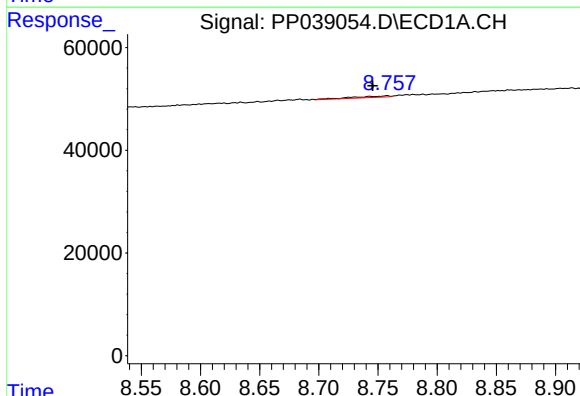


#34 AR-1260-4

R.T.: 8.758 min
Delta R.T.: 0.012 min
Response: 5943
Conc: 5.87 ng/ml

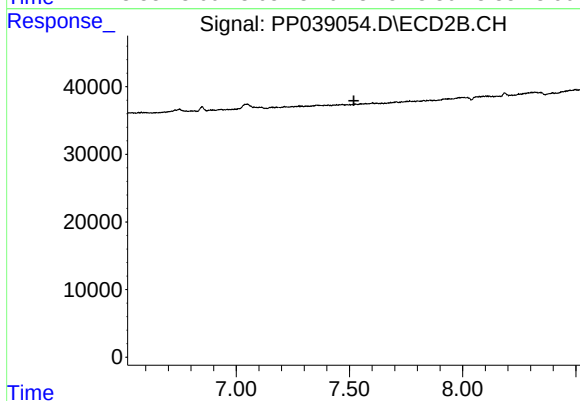

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.520 min
Response: 0
Conc: N.D.

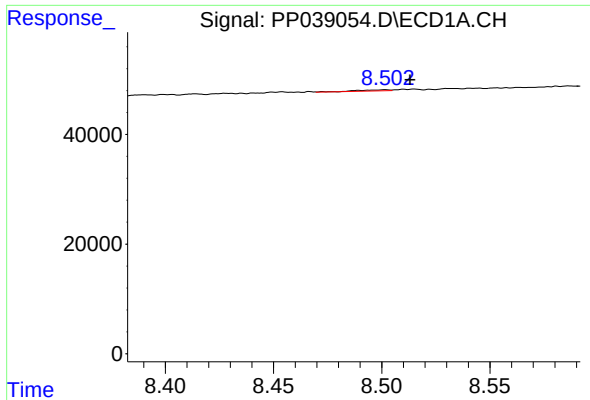

#36 AR-1262-1

R.T.: 8.502 min
Delta R.T.: -0.011 min
Response: 2047
Conc: 1.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

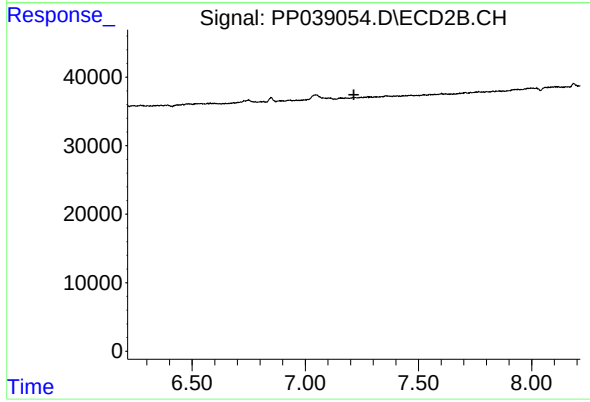

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.215 min
Response: 0
Conc: N.D.