

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083021\
 Data File : PP039059.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Aug 2021 23:39
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 03:03:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 26 09:31:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.874	3.859	915084	573478	23.973	23.796
2)	SA Decachlor...	10.855	9.116	553419	559787	22.985	24.757
Target Compounds							
9)	L2 AR-1221-2	5.225	0.000	10825	0	32.495	N.D. #
24)	L5 AR-1248-4	7.110f	0.000	13523	0	12.869	N.D. #
26)	L6 AR-1254-1	7.110	0.000	13523	0	12.961	N.D. #
28)	L6 AR-1254-3	7.735f	0.000	7347	0	4.769	N.D. #
32)	L7 AR-1260-2	8.124f	0.000	9352	0	7.764	N.D. #
33)	L7 AR-1260-3	8.507	7.036	1096	337	1.243	0.244 #
36)	L8 AR-1262-1	8.507	0.000	1096	0	0.821	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083021\
Data File : PP039059.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2021 23:39
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 03:03:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 26 09:31:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

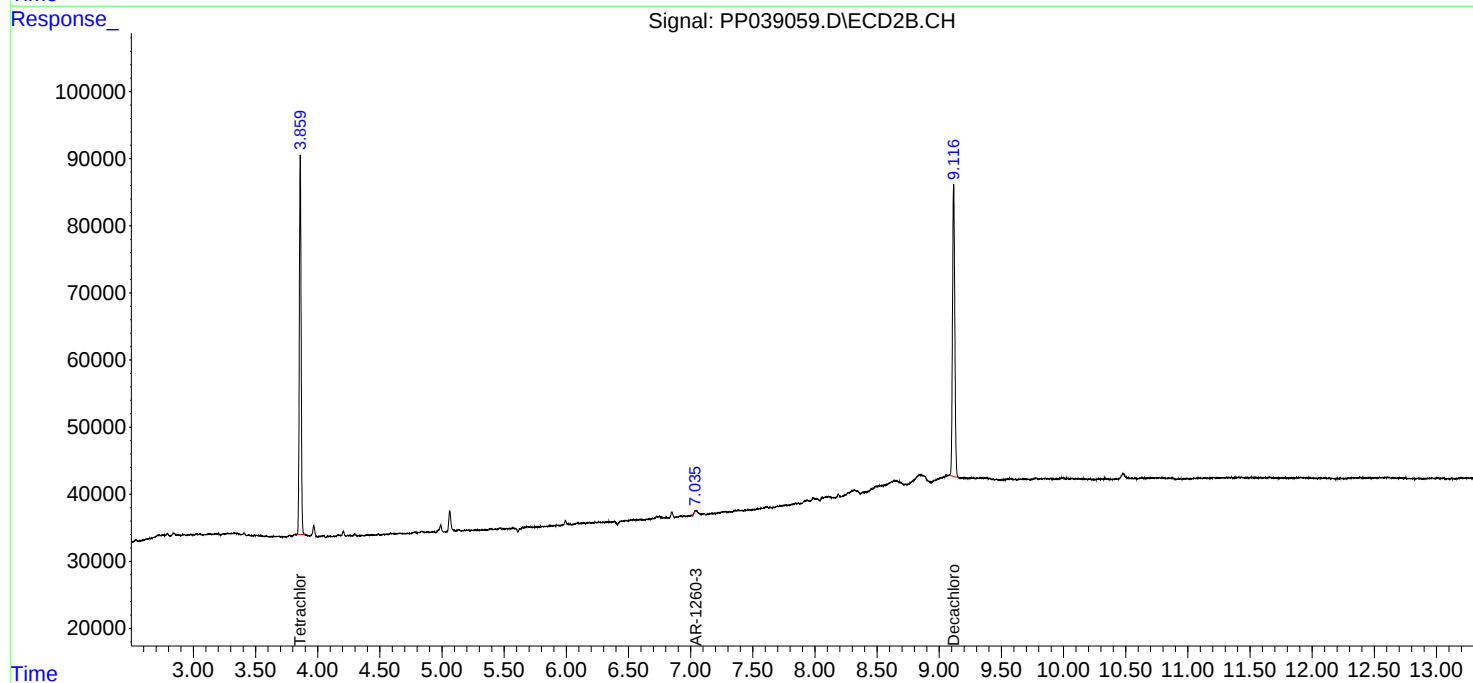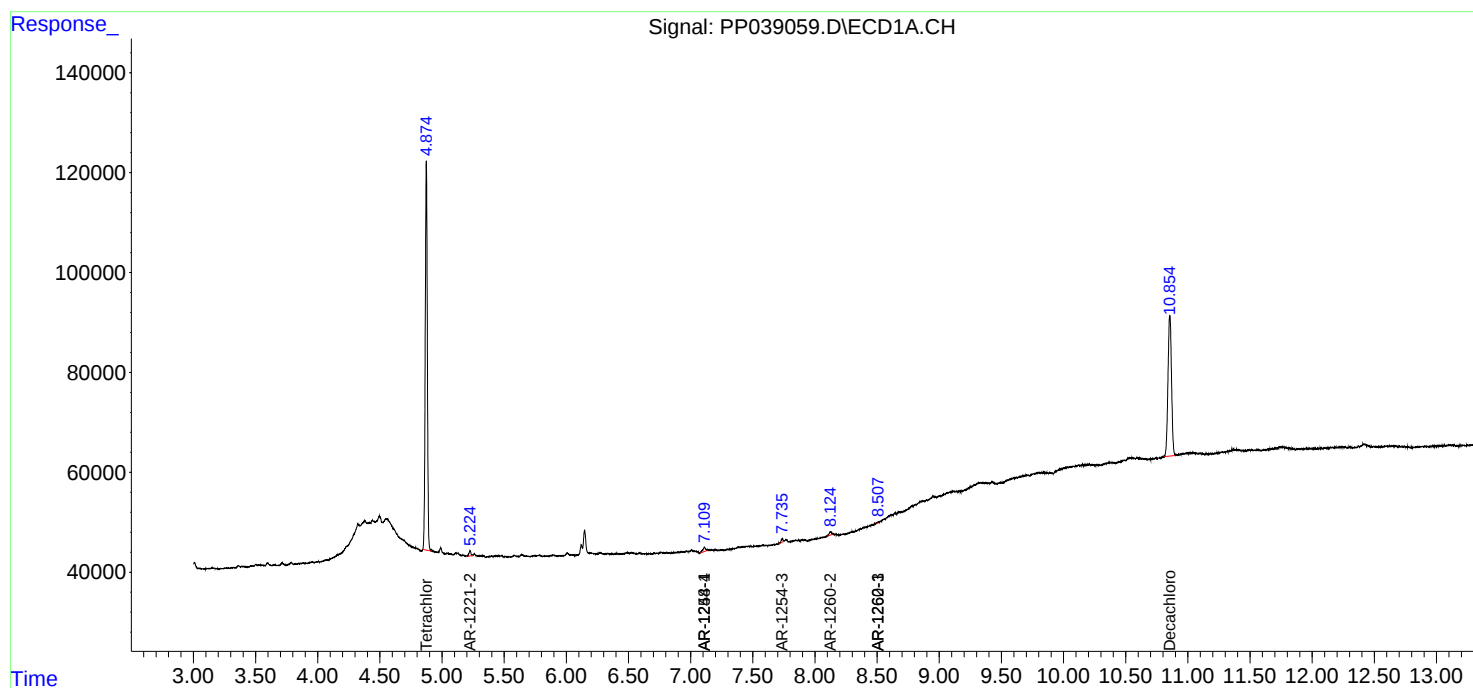


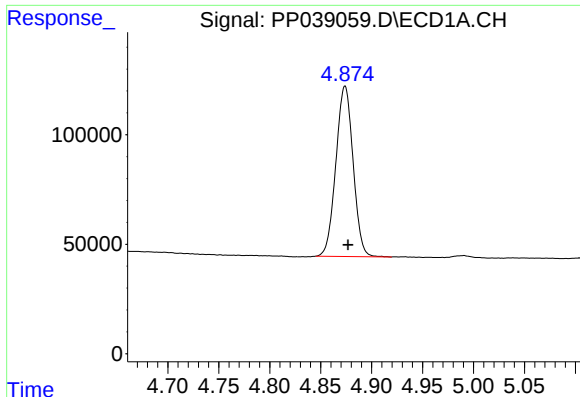

#1 Tetrachloro-m-xylene


R.T.: 4.874 min
Delta R.T.: -0.003 min
Response: 915084
Conc: 23.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

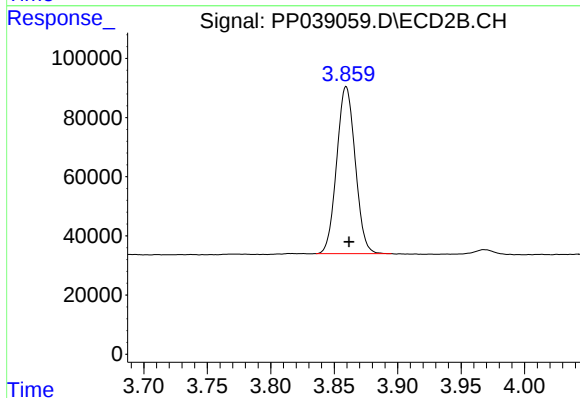


#1 Tetrachloro-m-xylene

R.T.: 3.859 min
Delta R.T.: -0.002 min
Response: 573478
Conc: 23.80 ng/ml

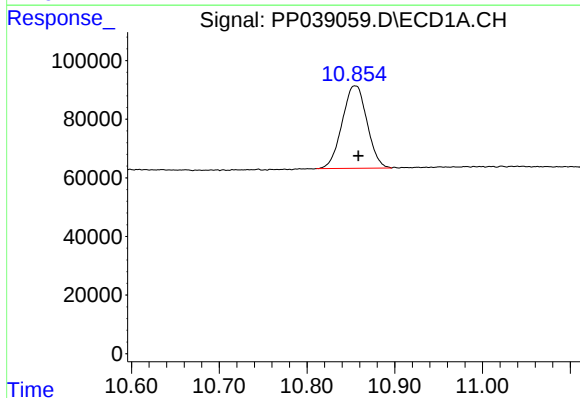


#2 Decachlorobiphenyl

R.T.: 10.855 min
Delta R.T.: -0.004 min
Response: 553419
Conc: 22.99 ng/ml

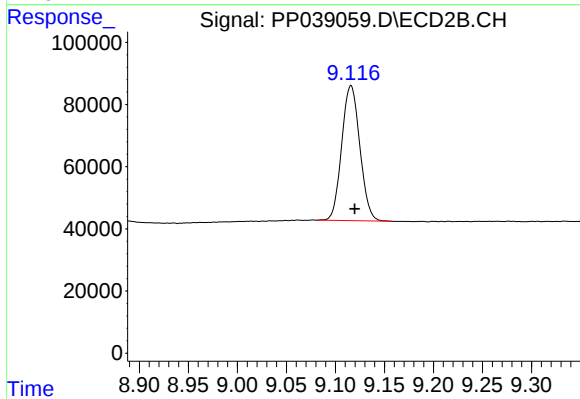

#2 Decachlorobiphenyl


R.T.: 9.116 min
Delta R.T.: -0.004 min
Response: 559787
Conc: 24.76 ng/ml

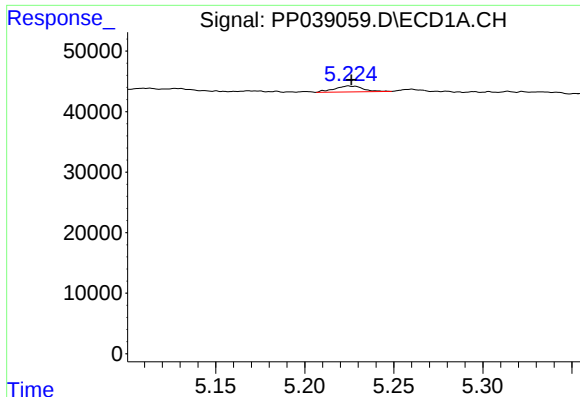

#9 AR-1221-2


R.T.: 5.225 min
Delta R.T.: -0.002 min
Response: 10825
Conc: 32.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

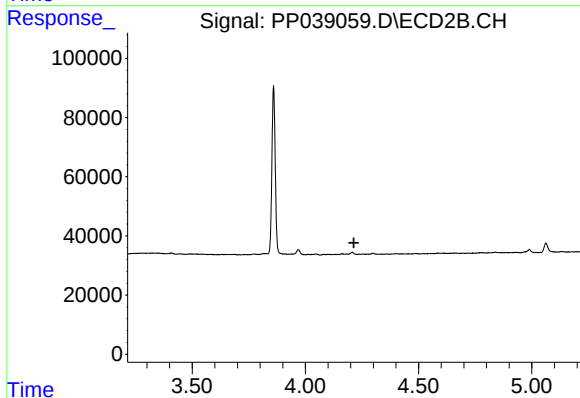


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.214 min
Response: 0
Conc: N.D.

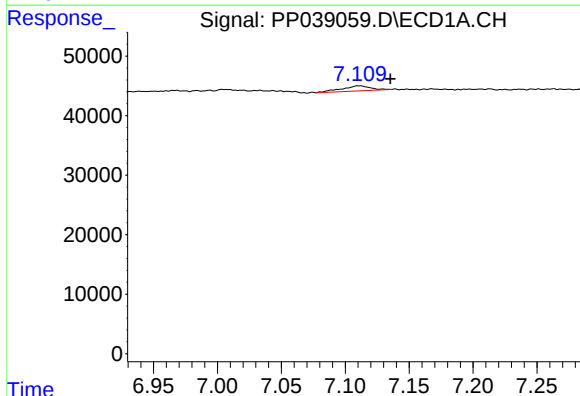


#24 AR-1248-4

R.T.: 7.110 min
Delta R.T.: -0.026 min
Response: 13523
Conc: 12.87 ng/ml

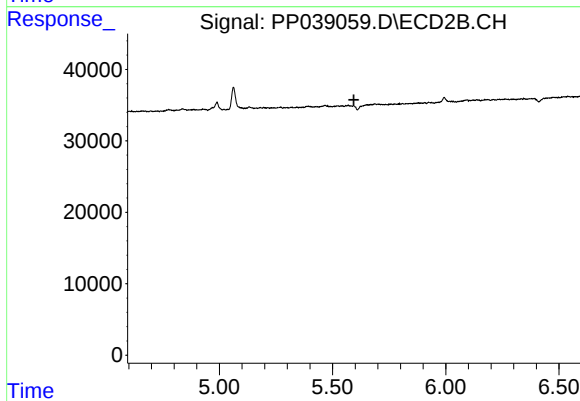

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.594 min
Response: 0
Conc: N.D.

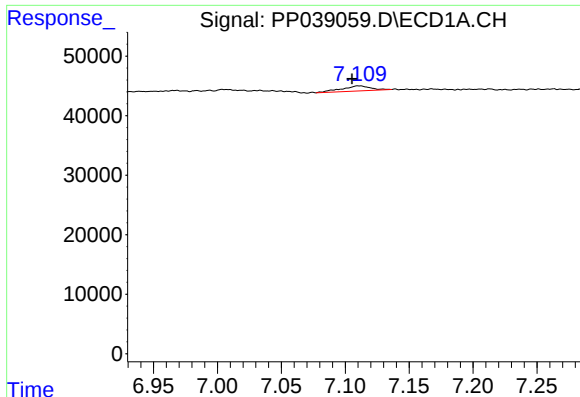

#26 AR-1254-1


R.T.: 7.110 min
Delta R.T.: 0.004 min
Response: 13523
Conc: 12.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

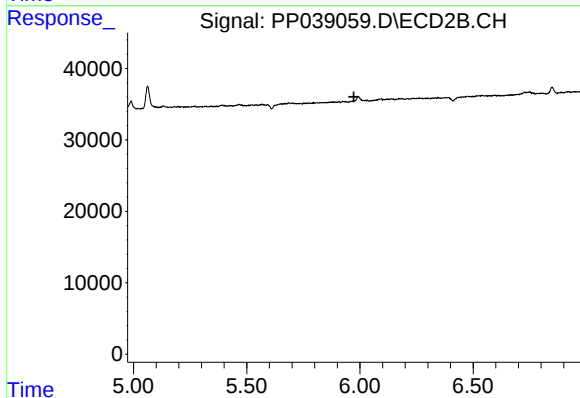


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.973 min
Response: 0
Conc: N.D.

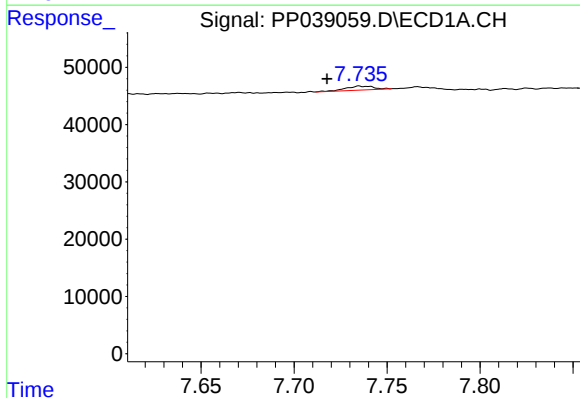


#28 AR-1254-3

R.T.: 7.735 min
Delta R.T.: 0.017 min
Response: 7347
Conc: 4.77 ng/ml

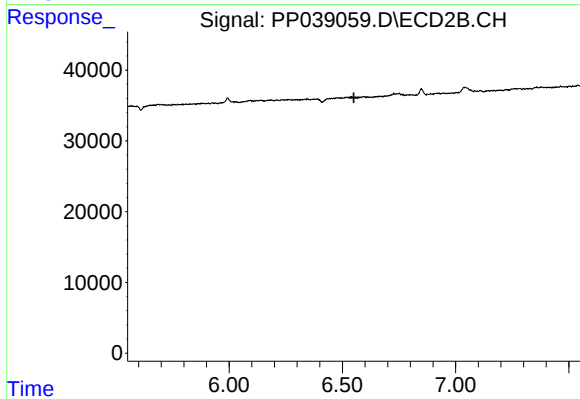

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.551 min
Response: 0
Conc: N.D.

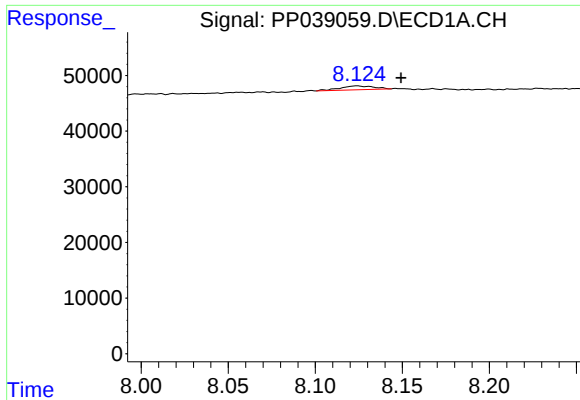

#32 AR-1260-2


R.T.: 8.124 min
Delta R.T.: -0.025 min
Response: 9352
Conc: 7.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

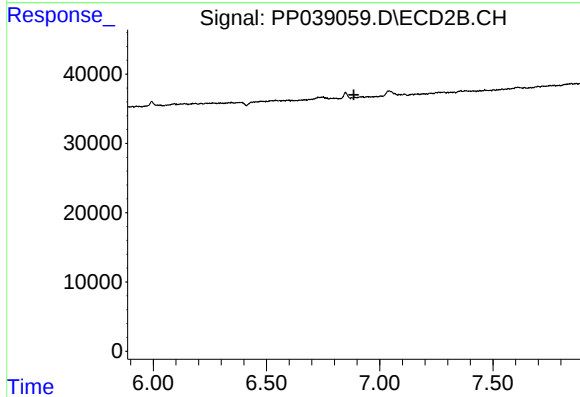


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.886 min
Response: 0
Conc: N.D.

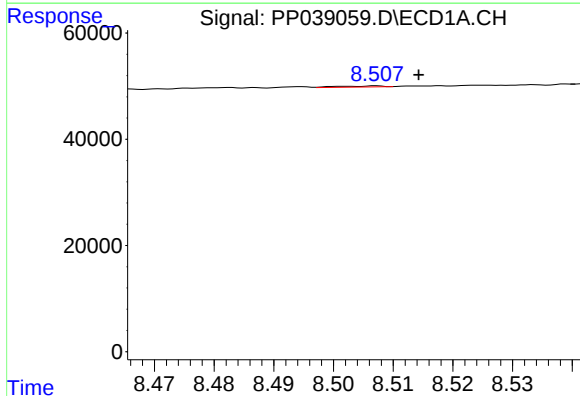


#33 AR-1260-3

R.T.: 8.507 min
Delta R.T.: -0.007 min
Response: 1096
Conc: 1.24 ng/ml

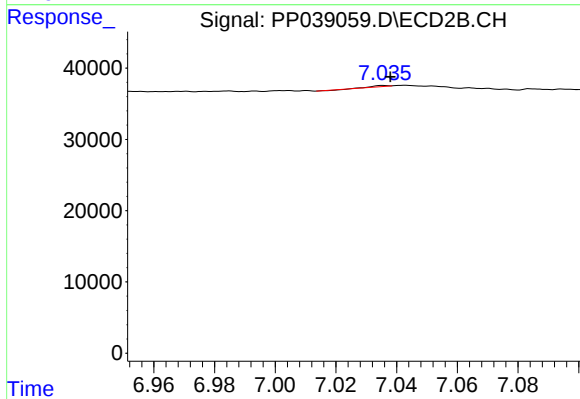

#33 AR-1260-3


R.T.: 7.036 min
Delta R.T.: -0.002 min
Response: 337
Conc: 0.24 ng/ml

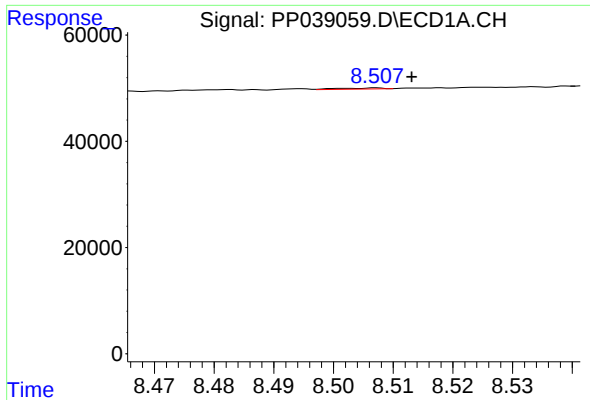

#36 AR-1262-1

R.T.: 8.507 min
Delta R.T.: -0.006 min
Response: 1096
Conc: 0.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

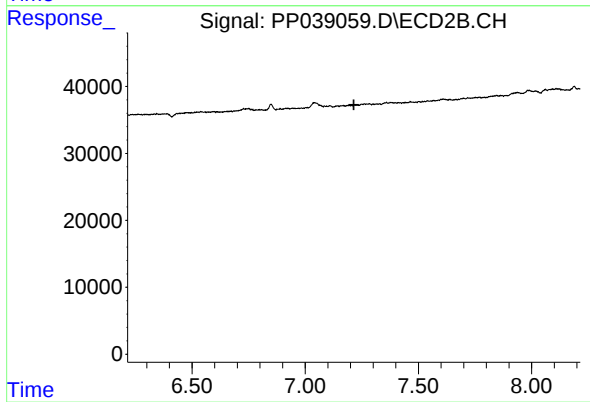

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.215 min
Response: 0
Conc: N.D.