

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083021\
 Data File : PP039047.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Aug 2021 18:54
 Operator : AJ\MA
 Sample : M3561-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VE4-9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 02:59:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 26 09:31:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.874	3.860	745551	474354	19.532	19.683
2) SA Decachlor...	10.854	9.116	346983	349293	14.411	15.447

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083021\
Data File : PP039047.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2021 18:54
Operator : AJ\MA
Sample : M3561-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
VE4-9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 02:59:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 26 09:31:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

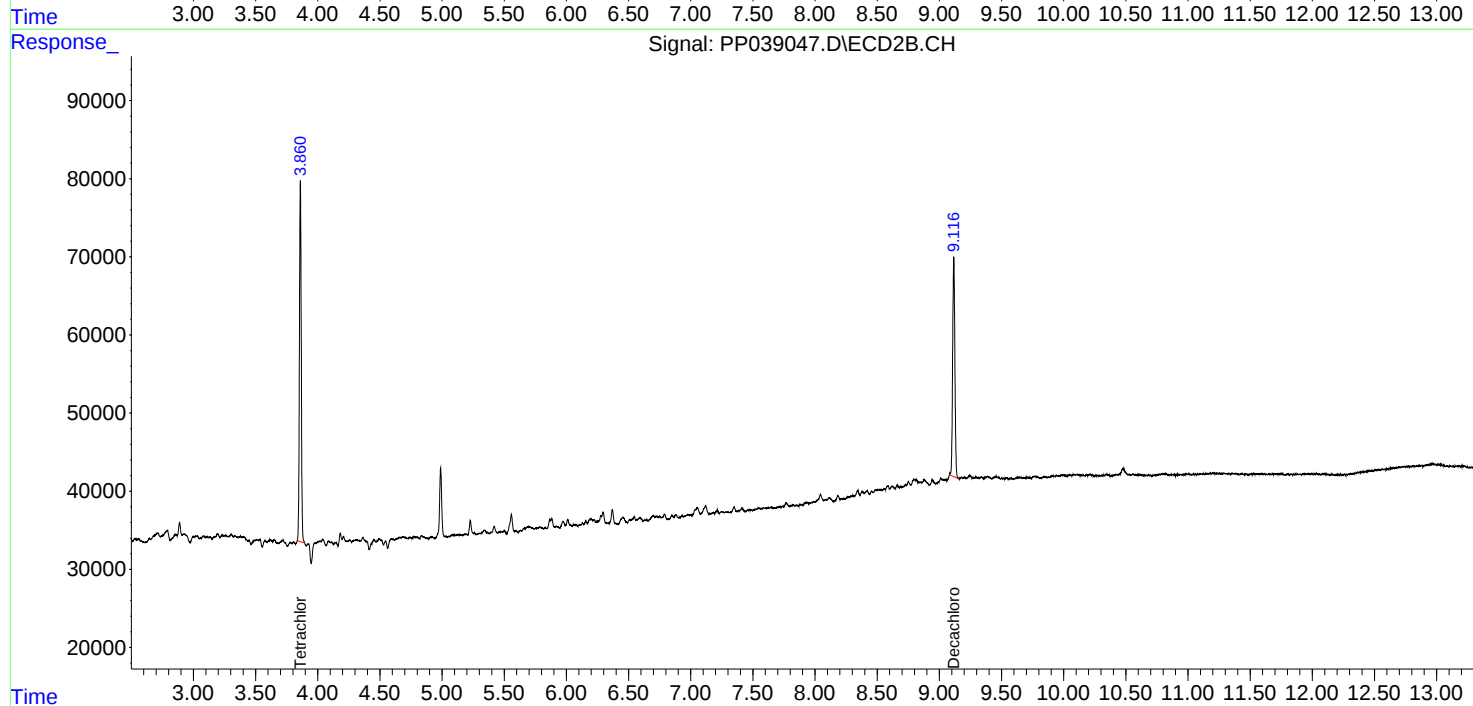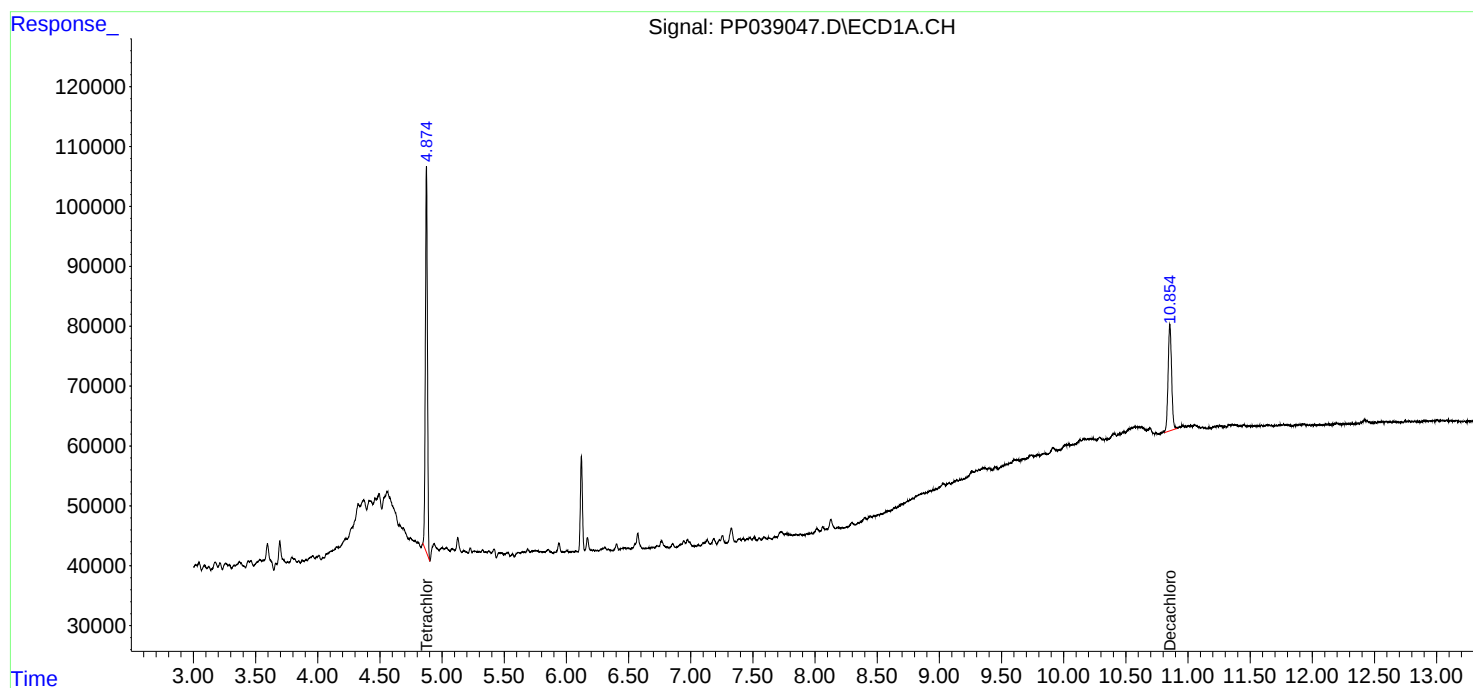


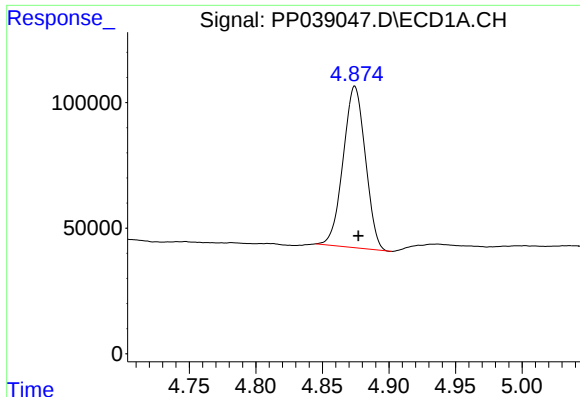

#1 Tetrachloro-m-xylene


R.T.: 4.874 min
Delta R.T.: -0.003 min
Response: 745551
Conc: 19.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
VE4-9

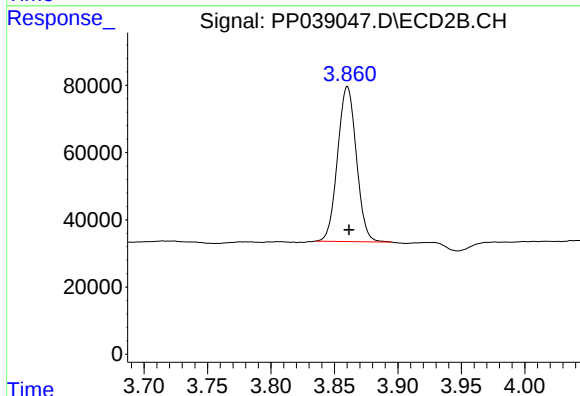


#1 Tetrachloro-m-xylene

R.T.: 3.860 min
Delta R.T.: -0.001 min
Response: 474354
Conc: 19.68 ng/ml

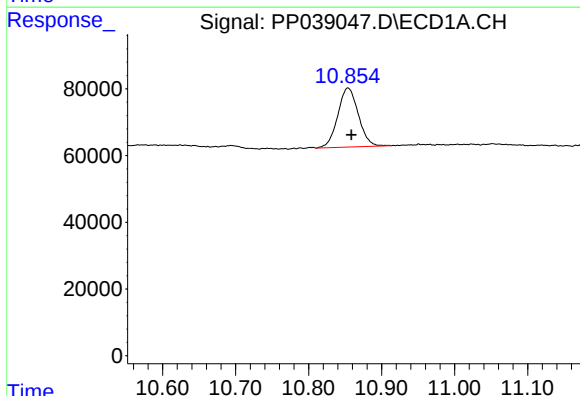

#2 Decachlorobiphenyl

R.T.: 10.854 min
Delta R.T.: -0.005 min
Response: 346983
Conc: 14.41 ng/ml

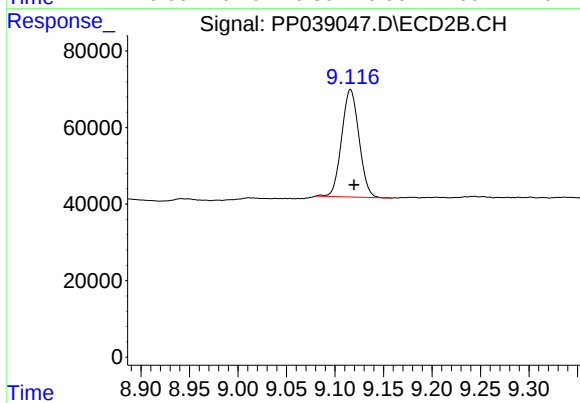

#2 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: -0.004 min
Response: 349293
Conc: 15.45 ng/ml