

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083021\
 Data File : PP039048.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Aug 2021 19:11
 Operator : AJ\MA
 Sample : M3561-17
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DAY-1

Manual Integrations
 APPROVED

mohammad
 8/31/2021 12:51:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 02:59:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 26 09:31:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.875	3.861	717576	467203	18.799	19.386
2) SA Decachlor...	10.856	9.116	380043	419787	15.784	18.565m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083021\
Data File : PP039048.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2021 19:11
Operator : AJ\MA
Sample : M3561-17
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
DAY-1


Manual Integrations
APPROVED

mohammad
8/31/2021 12:51:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 02:59:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 26 09:31:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

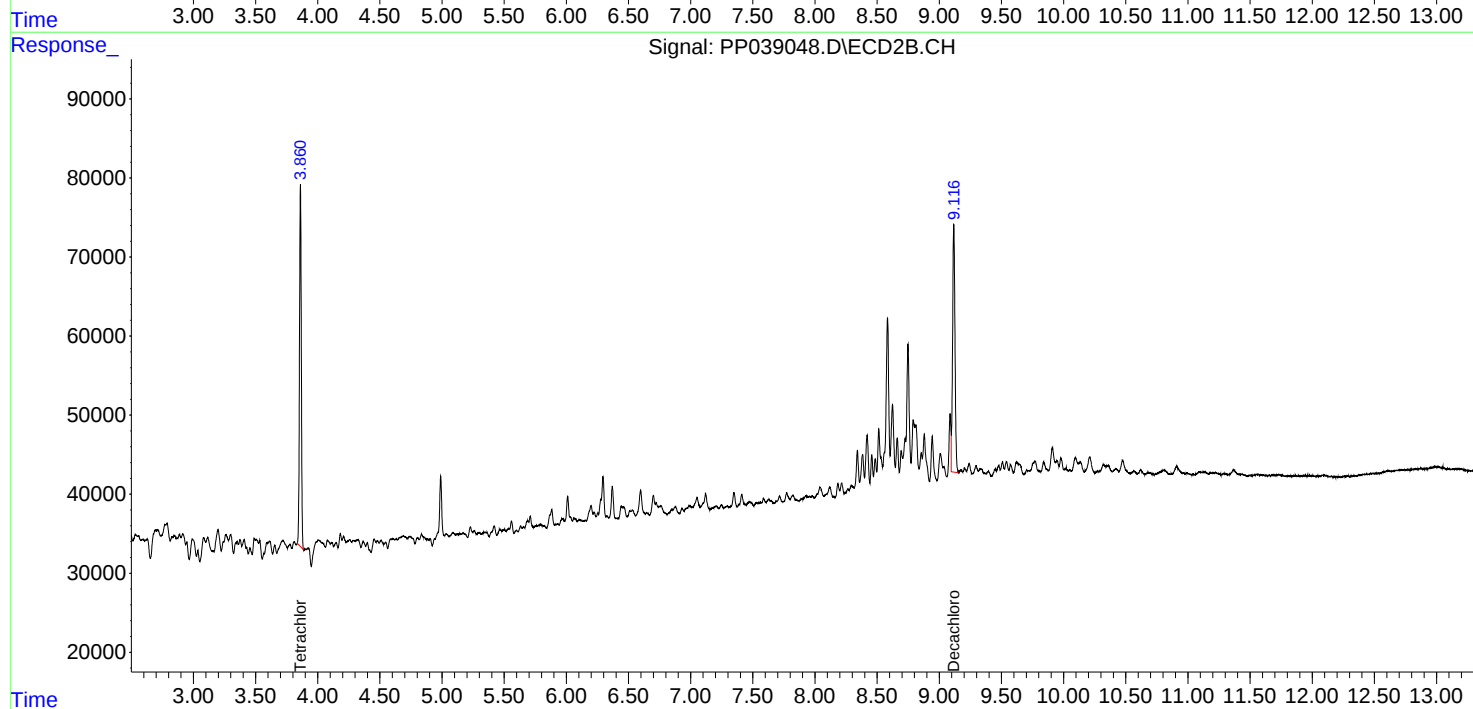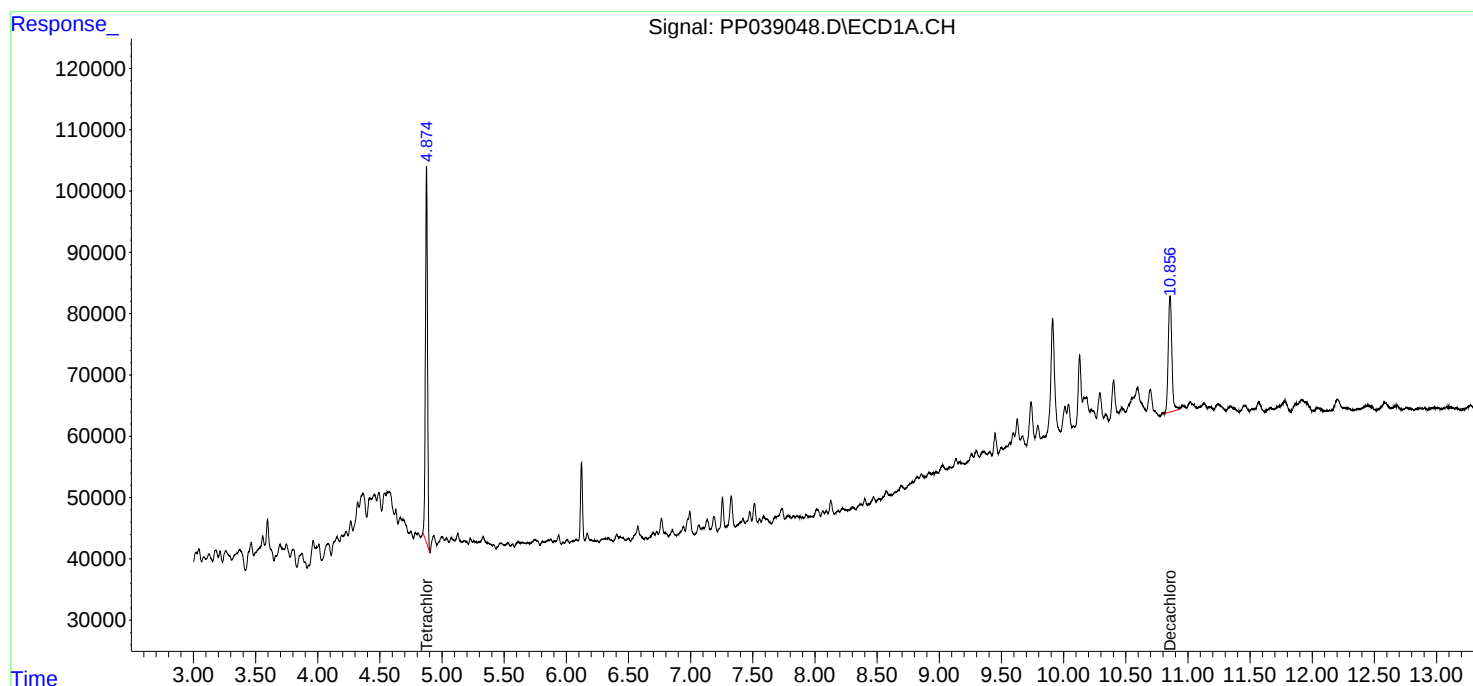

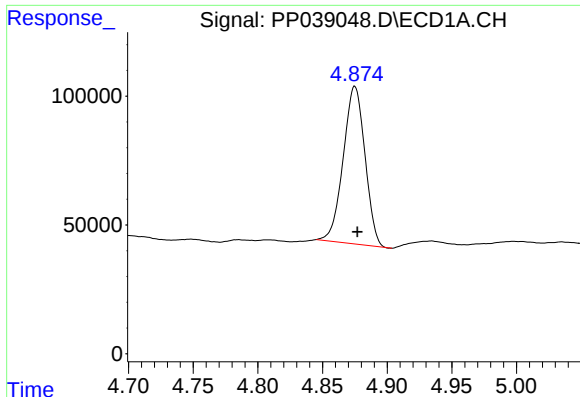


#1 Tetrachloro-m-xylene

R.T.: 4.875 min
Delta R.T.: -0.002 min
Response: 717576
Conc: 18.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
DAY-1


Manual Integrations
APPROVED

mohammad
8/31/2021 12:51:23 PM

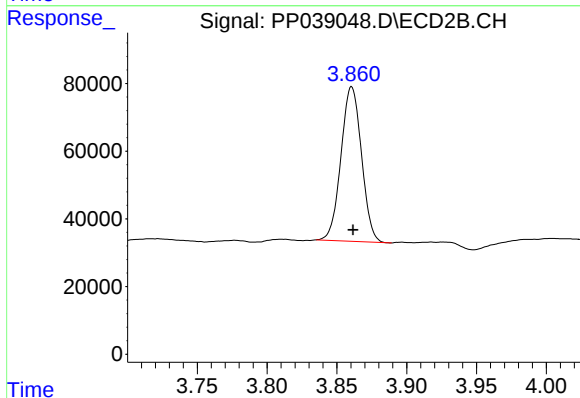


#1 Tetrachloro-m-xylene

R.T.: 3.861 min
Delta R.T.: -0.001 min
Response: 467203
Conc: 19.39 ng/ml

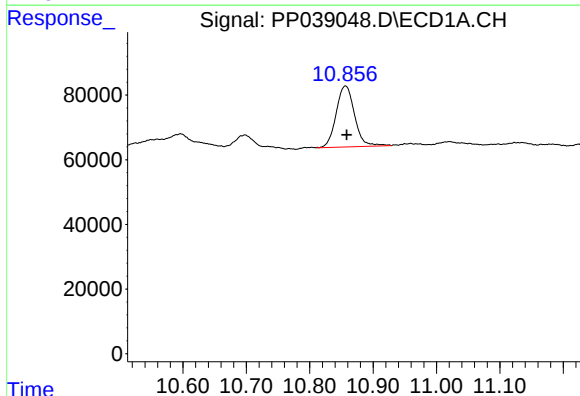

#2 Decachlorobiphenyl

R.T.: 10.856 min
Delta R.T.: -0.002 min
Response: 380043
Conc: 15.78 ng/ml

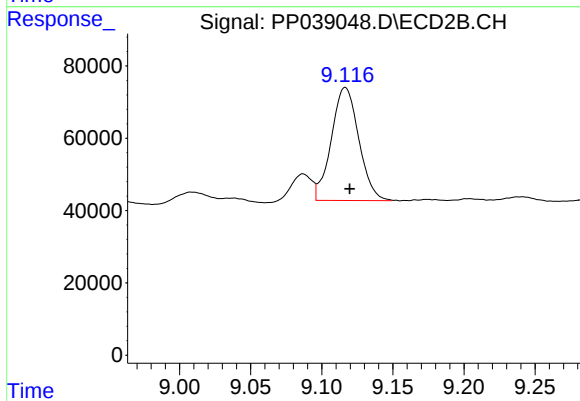

#2 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: -0.004 min
Response: 419787
Conc: 18.57 ng/ml m