

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083121\
 Data File : PP039091.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Aug 2021 18:42
 Operator : AJ\MA
 Sample : M3607-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20211021-SITE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:13:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 26 09:31:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.874	3.860	813170	515296	21.303	21.382
2) SA Decachlor...	10.854	9.114	454828	470538	18.890	20.810
Target Compounds						
8) L2 AR-1221-1	5.128	0.000	46080	0	102.305	N.D. #
9) L2 AR-1221-2	5.228	0.000	3760	0	11.288	N.D. #
30) L6 AR-1254-5	8.437	0.000	13837	0	12.256	N.D. #
31) L7 AR-1260-1	7.883	0.000	18337	0	19.237	N.D. #
32) L7 AR-1260-2	8.148	0.000	24192	0	20.085	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083121\
Data File : PP039091.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Aug 2021 18:42
Operator : AJ\MA
Sample : M3607-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20211021-SITE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:13:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 26 09:31:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

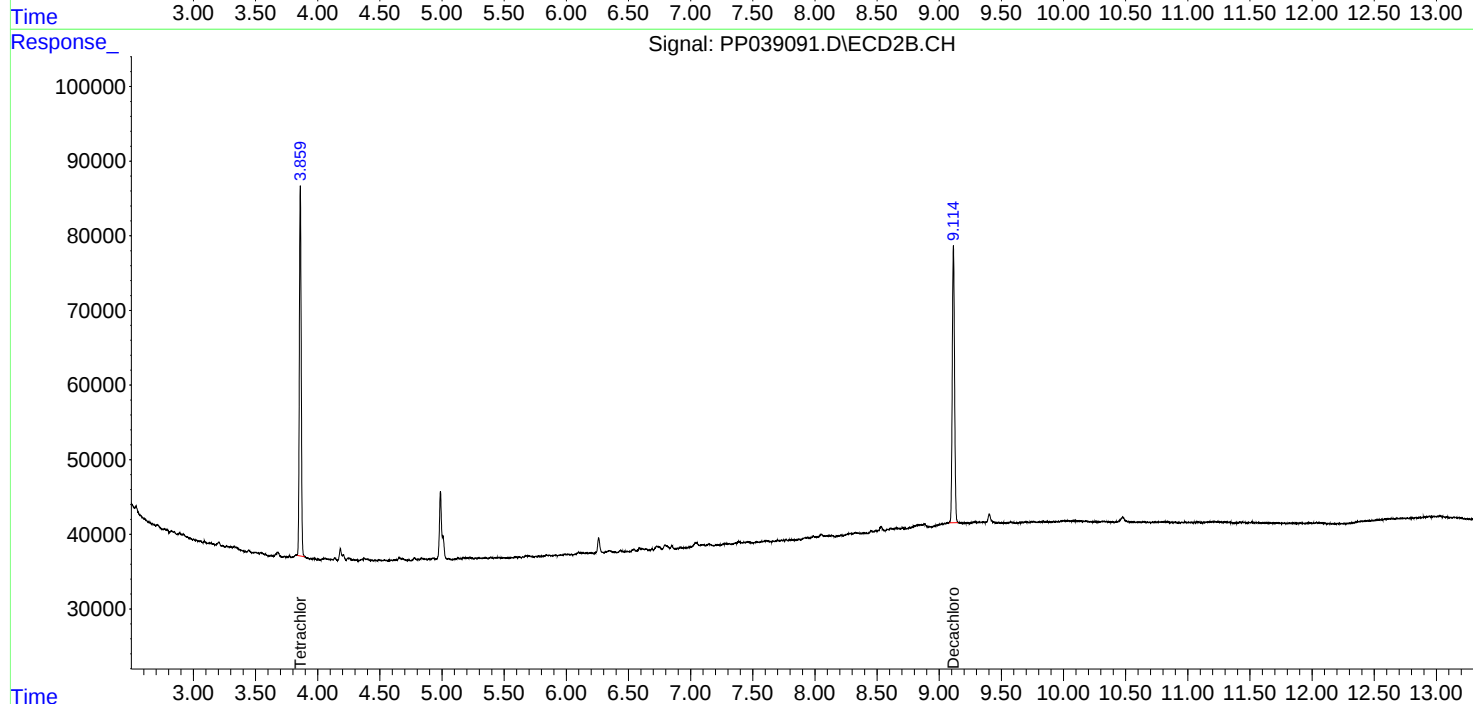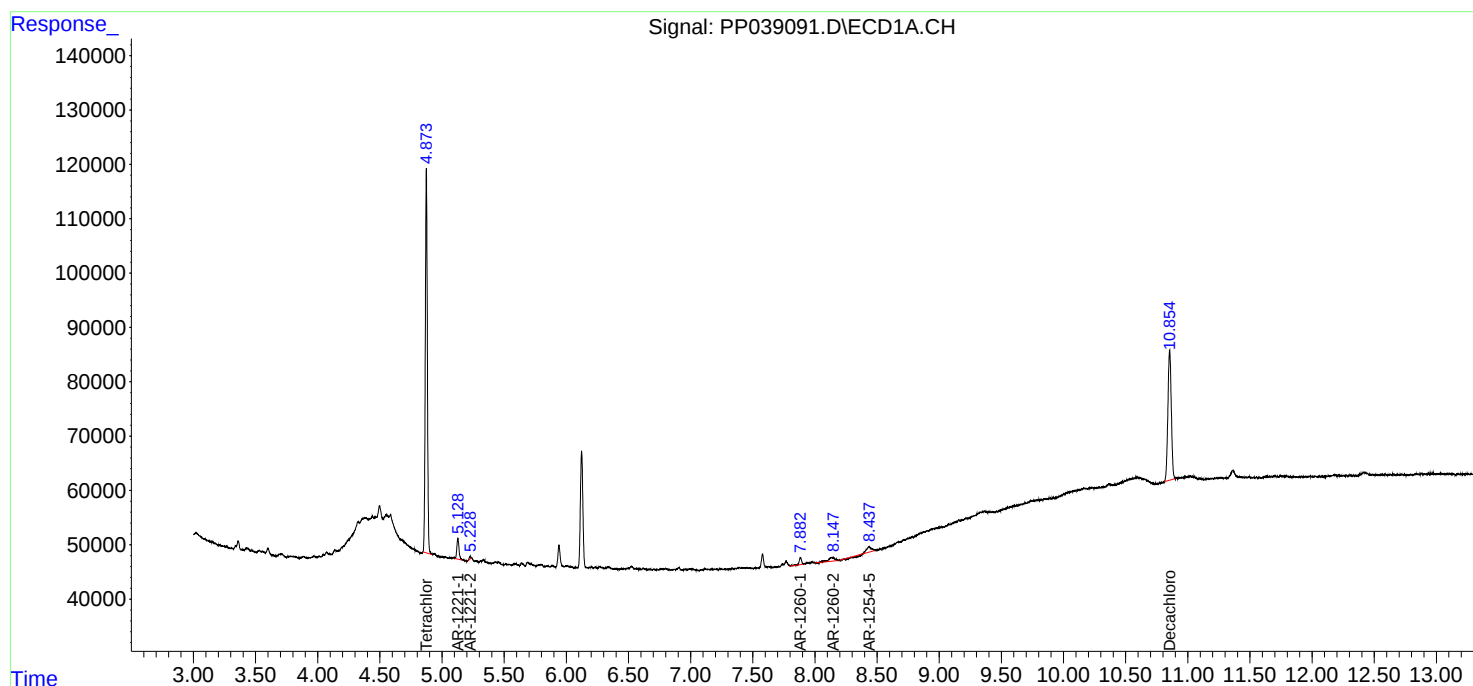


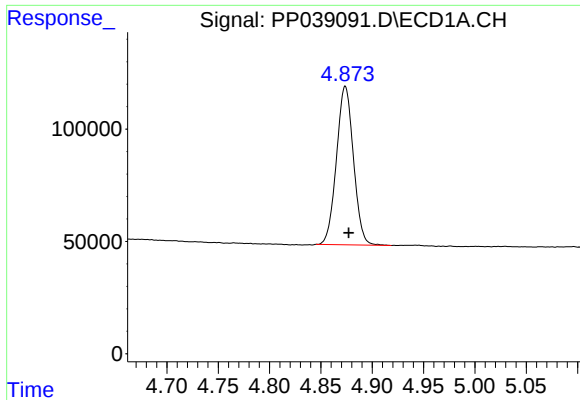

#1 Tetrachloro-m-xylene


R.T.: 4.874 min
Delta R.T.: -0.003 min
Response: 813170
Conc: 21.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
20211021-SITE-WATER

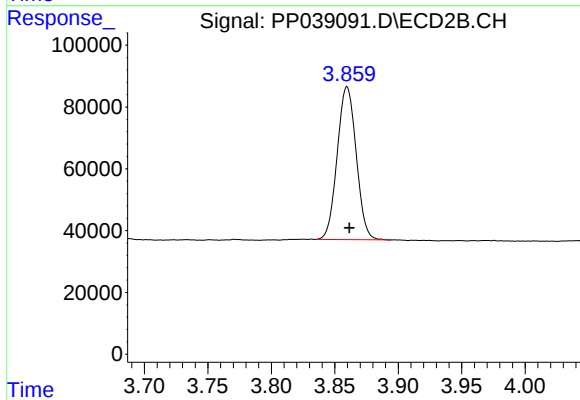


#1 Tetrachloro-m-xylene

R.T.: 3.860 min
Delta R.T.: -0.002 min
Response: 515296
Conc: 21.38 ng/ml

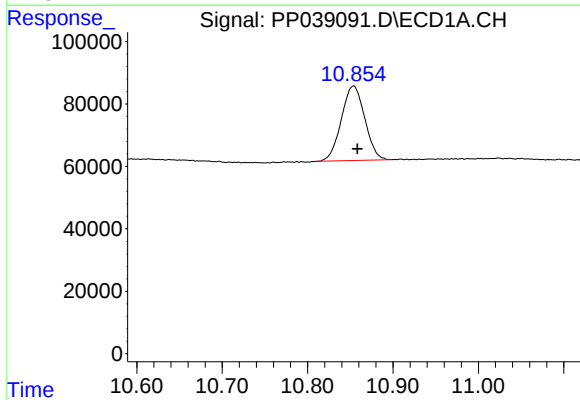


#2 Decachlorobiphenyl

R.T.: 10.854 min
Delta R.T.: -0.005 min
Response: 454828
Conc: 18.89 ng/ml

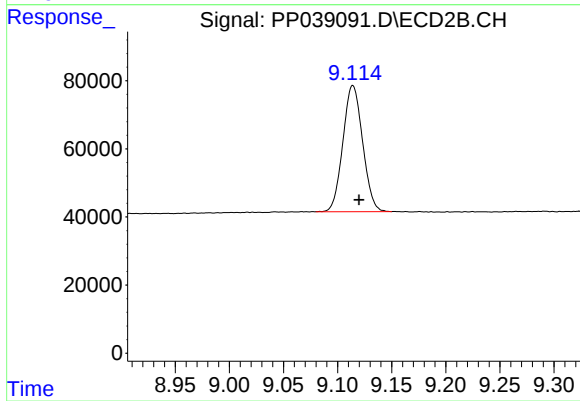

#2 Decachlorobiphenyl


R.T.: 9.114 min
Delta R.T.: -0.006 min
Response: 470538
Conc: 20.81 ng/ml

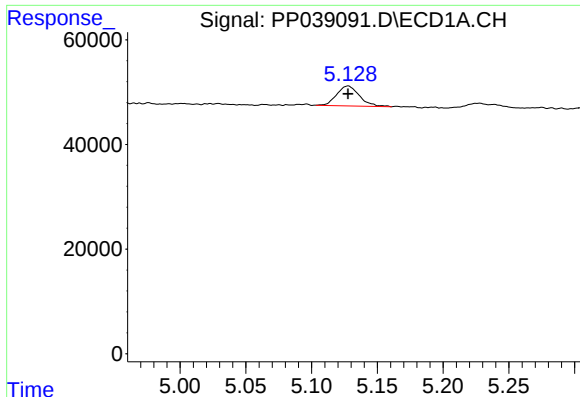

#8 AR-1221-1


R.T.: 5.128 min
Delta R.T.: 0.000 min
Response: 46080
Conc: 102.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
20211021-SITE-WATER

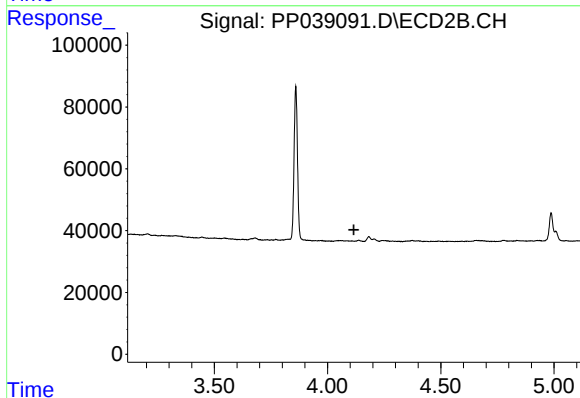


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.116 min
Response: 0
Conc: N.D.

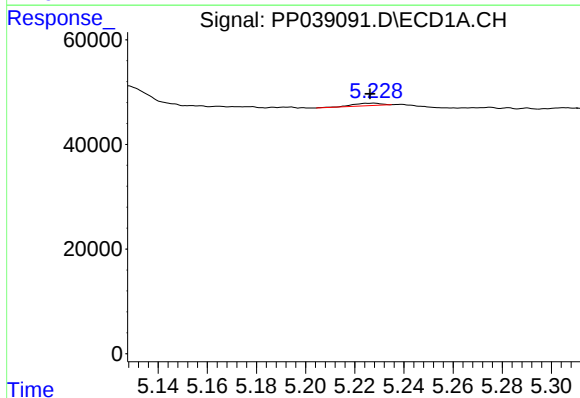


#9 AR-1221-2

R.T.: 5.228 min
Delta R.T.: 0.002 min
Response: 3760
Conc: 11.29 ng/ml

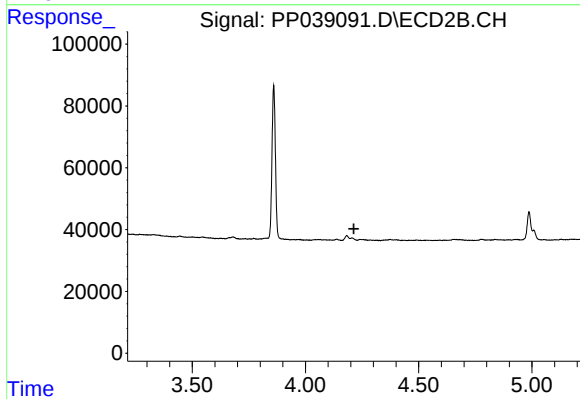

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.214 min
Response: 0
Conc: N.D.

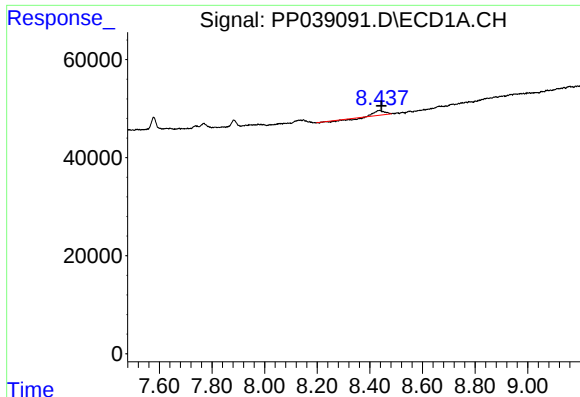

#30 AR-1254-5


R.T.: 8.437 min
Delta R.T.: -0.006 min
Response: 13837
Conc: 12.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
20211021-SITE-WATER

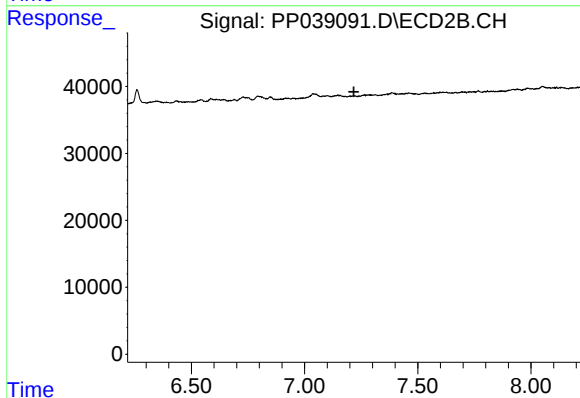


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.218 min
Response: 0
Conc: N.D.

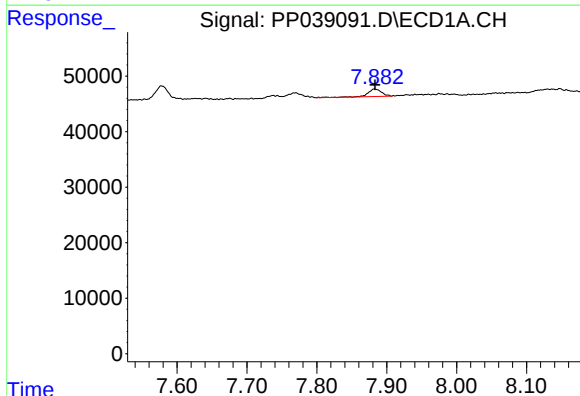


#31 AR-1260-1

R.T.: 7.883 min
Delta R.T.: 0.000 min
Response: 18337
Conc: 19.24 ng/ml

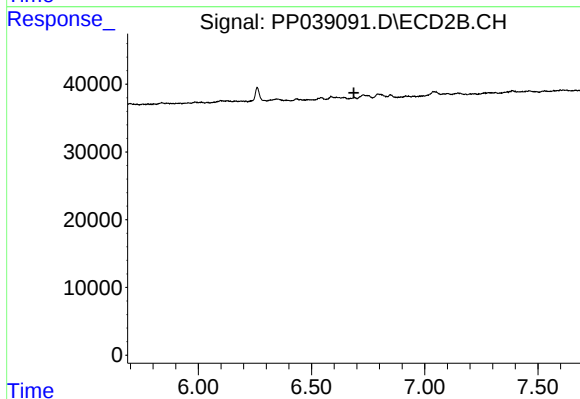

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.687 min
Response: 0
Conc: N.D.

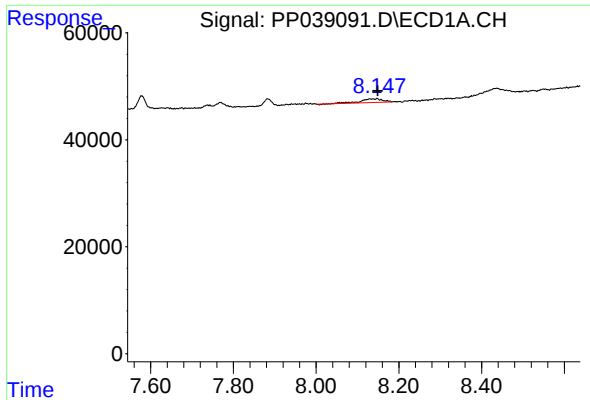

#32 AR-1260-2

R.T.: 8.148 min
Delta R.T.: -0.002 min
Response: 24192
Conc: 20.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
20211021-SITE-WATER

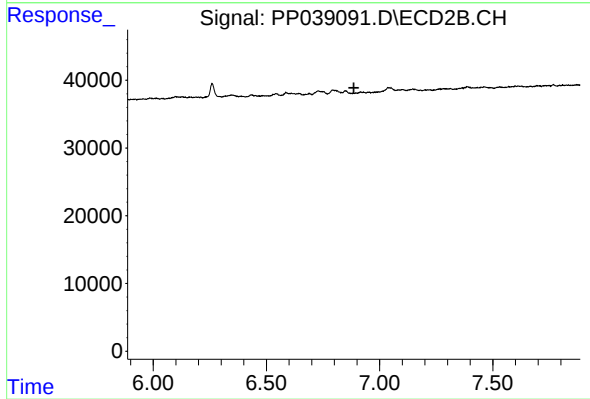

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.886 min
Response: 0
Conc: N.D.