

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083121\
 Data File : PP039092.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Aug 2021 18:59
 Operator : AJ\MA
 Sample : M3607-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20211022-FIELD-BLANK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:13:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 26 09:31:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.874	3.860	768404	485561	20.130	20.148
2) SA Decachlor...	10.855	9.115	262505	276967	10.903	12.249

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083121\
Data File : PP039092.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Aug 2021 18:59
Operator : AJ\MA
Sample : M3607-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20211022-FIELD-BLANK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:13:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 26 09:31:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

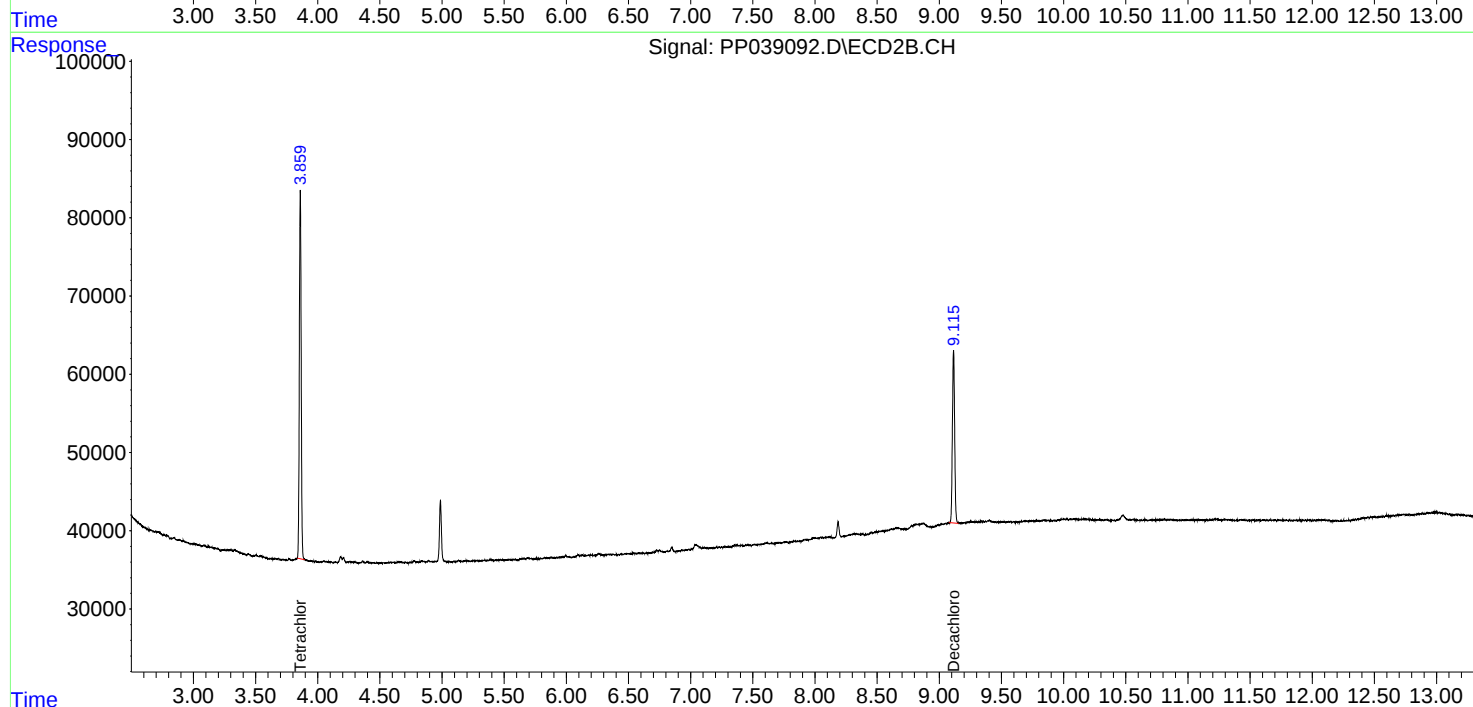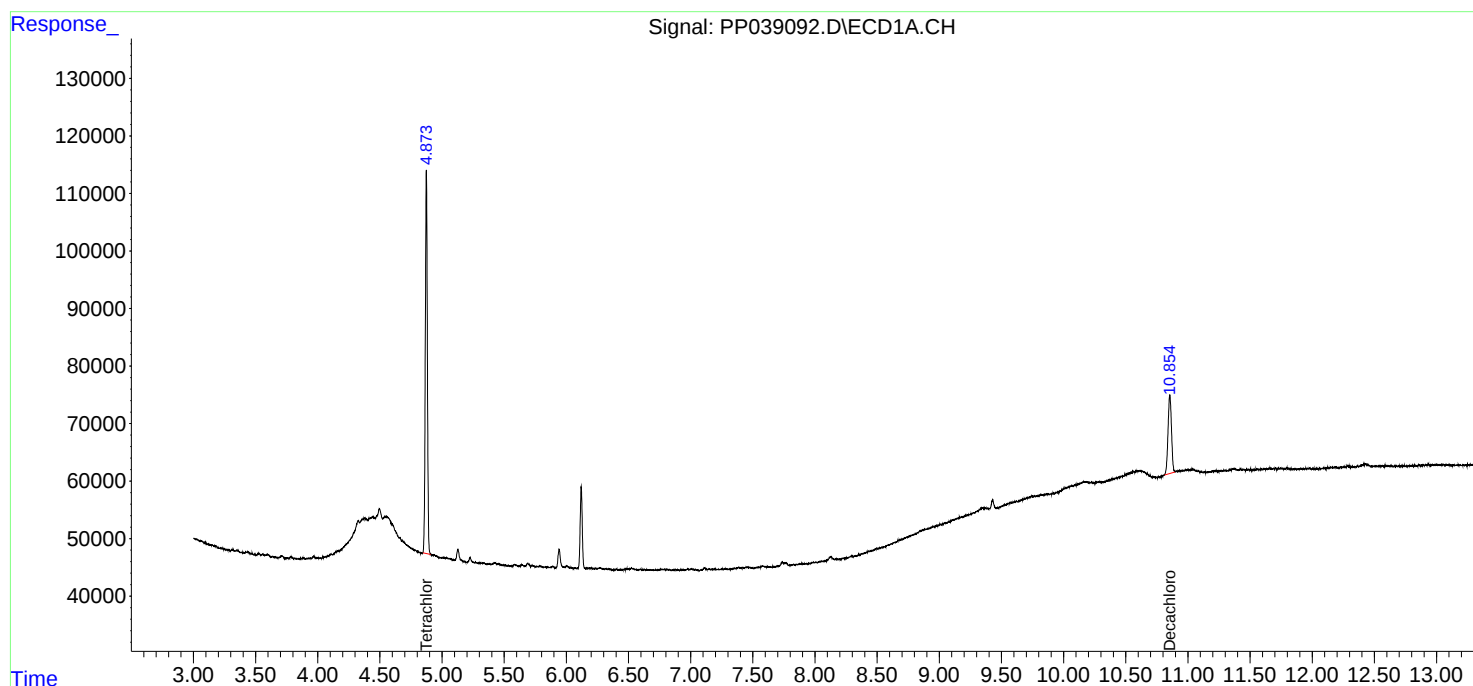


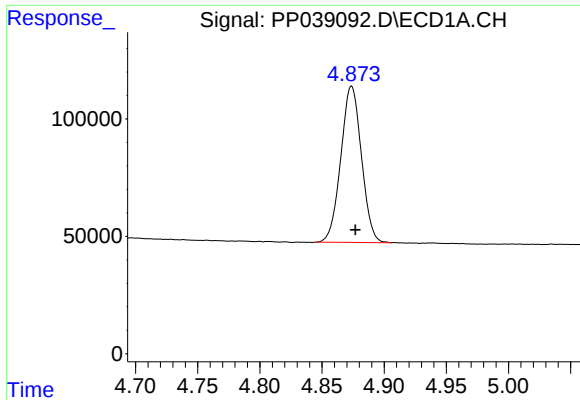

#1 Tetrachloro-m-xylene


R.T.: 4.874 min
Delta R.T.: -0.003 min
Response: 768404
Conc: 20.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
20211022-FIELD-BLANK

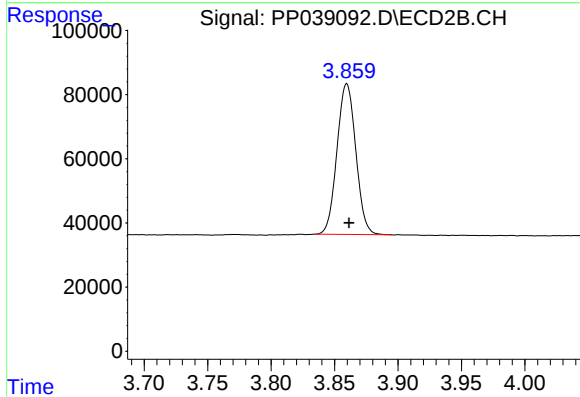


#1 Tetrachloro-m-xylene

R.T.: 3.860 min
Delta R.T.: -0.002 min
Response: 485561
Conc: 20.15 ng/ml

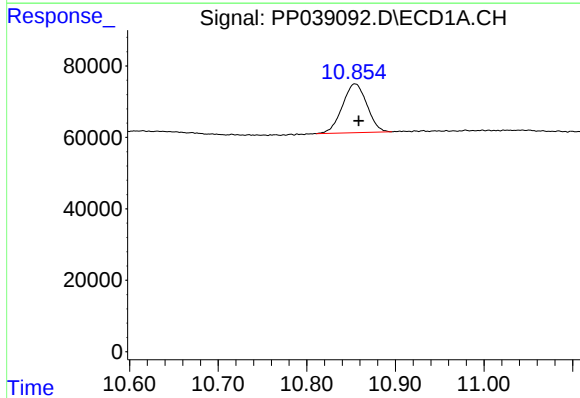

#2 Decachlorobiphenyl

R.T.: 10.855 min
Delta R.T.: -0.004 min
Response: 262505
Conc: 10.90 ng/ml

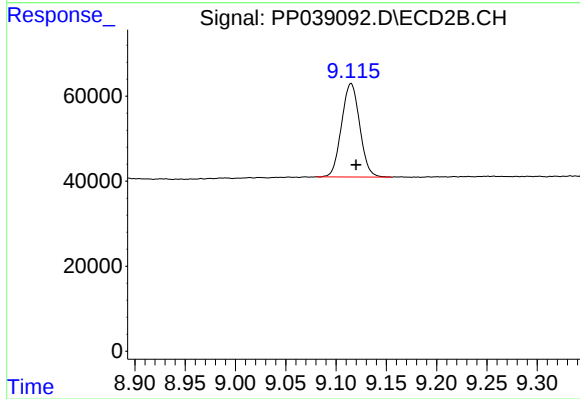

#2 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: -0.005 min
Response: 276967
Conc: 12.25 ng/ml