

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083123\
 Data File : PP059660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2023 15:26
 Operator : YP\AJ
 Sample : 04246-01 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC226599LOZ-END-1-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:20:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 24 01:16:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.410	3.638	1840775	2440017	1.557	1.263
2)	SA Decachlor...	10.195	8.661	1720201	2562601	2.200	1.857

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083123\
Data File : PP059660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2023 15:26
Operator : YP\AJ
Sample : 04246-01 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BC226599LOZ-END-1-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:20:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082323.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 24 01:16:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

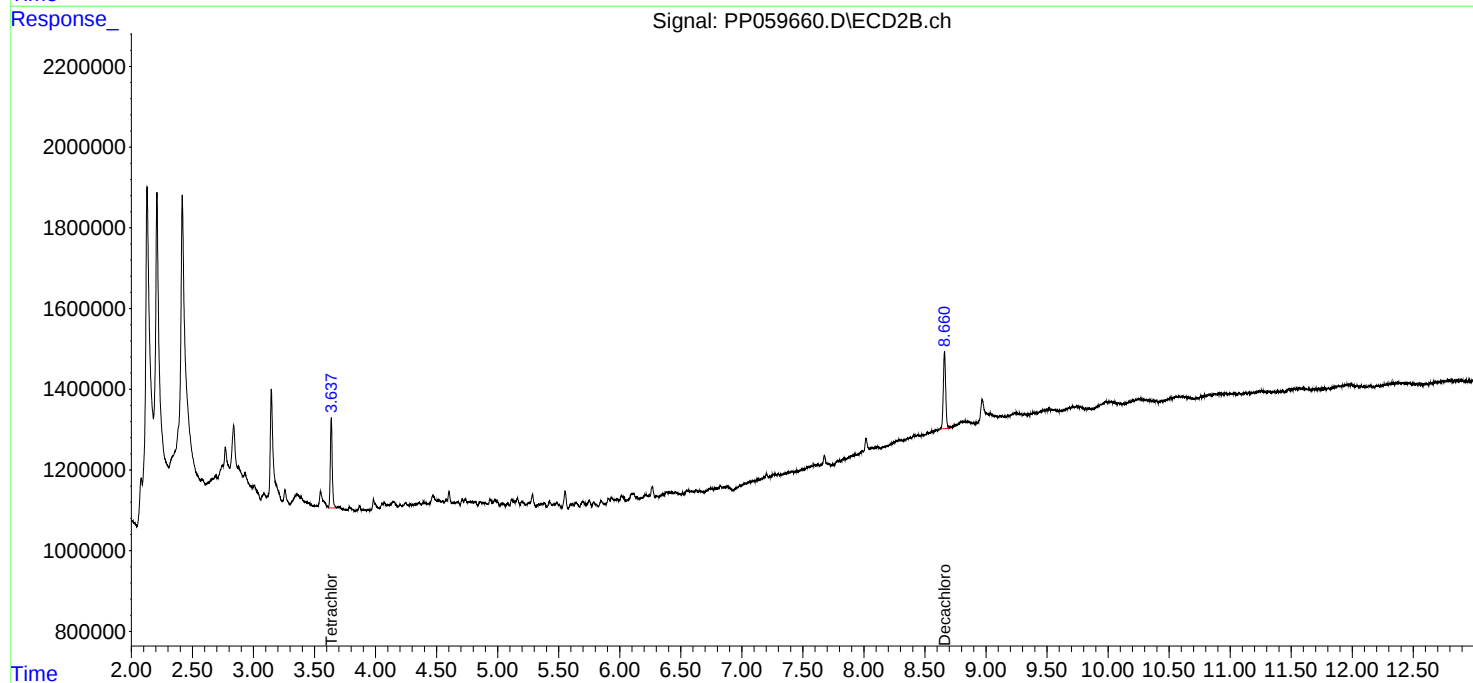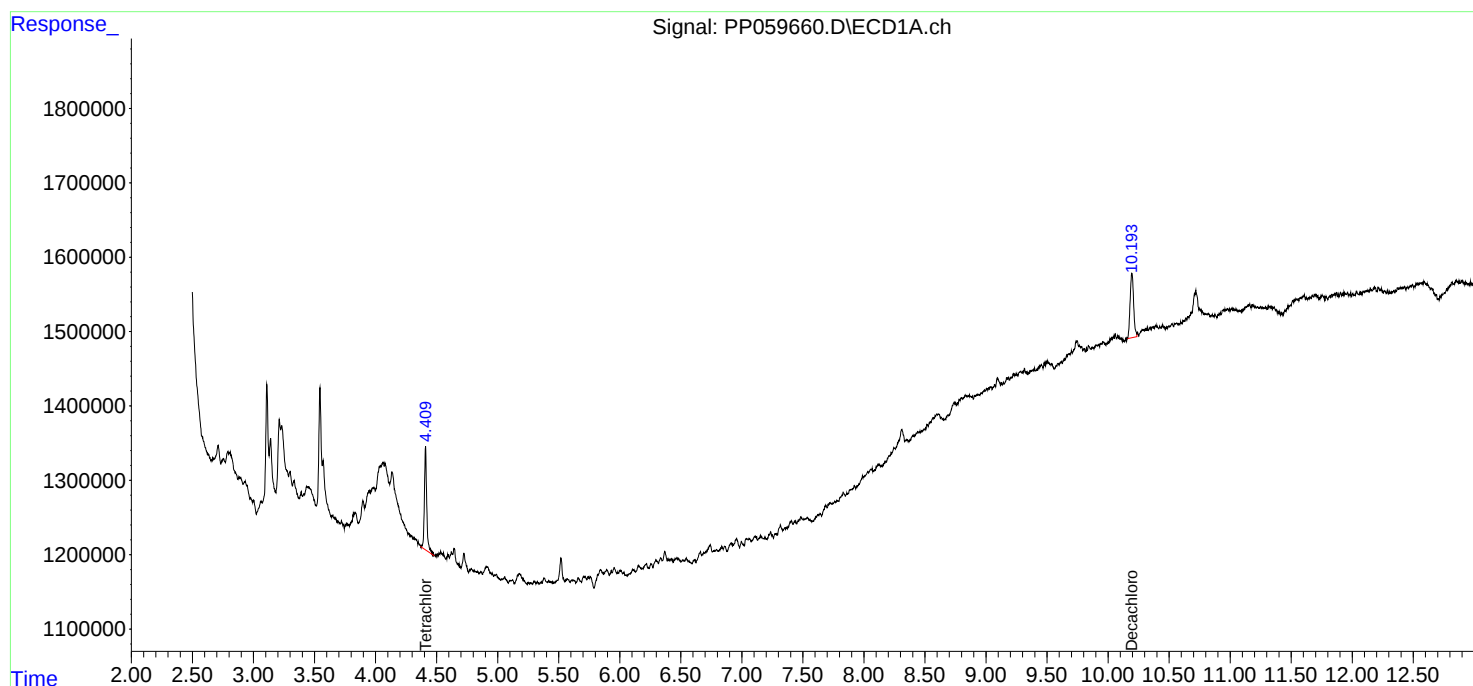


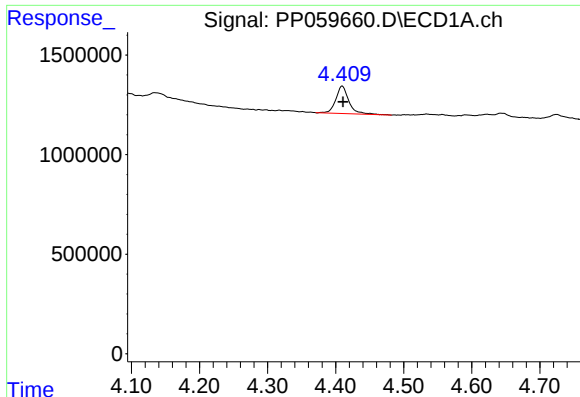

#1 Tetrachloro-m-xylene


R.T.: 4.410 min
Delta R.T.: -0.001 min
Response: 1840775
Conc: 1.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC226599LOZ-END-1-1

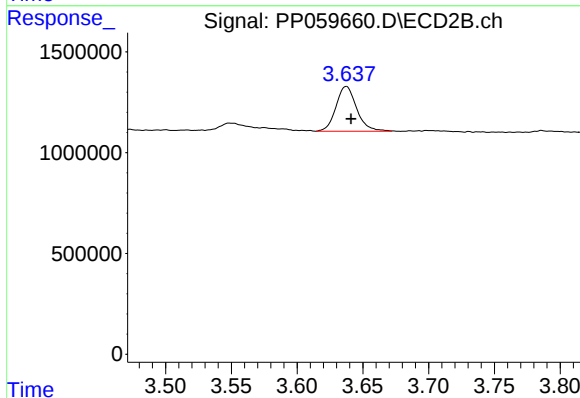


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: -0.003 min
Response: 2440017
Conc: 1.26 ng/ml

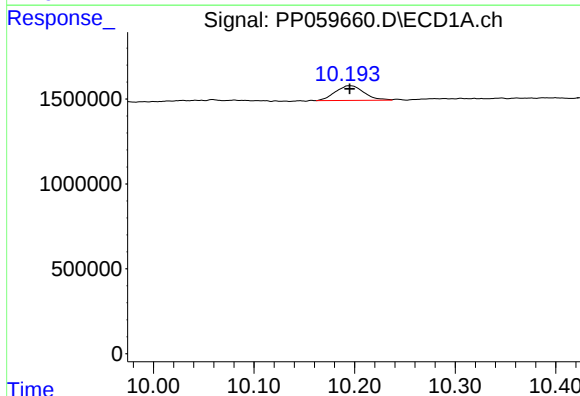

#2 Decachlorobiphenyl

R.T.: 10.195 min
Delta R.T.: 0.000 min
Response: 1720201
Conc: 2.20 ng/ml

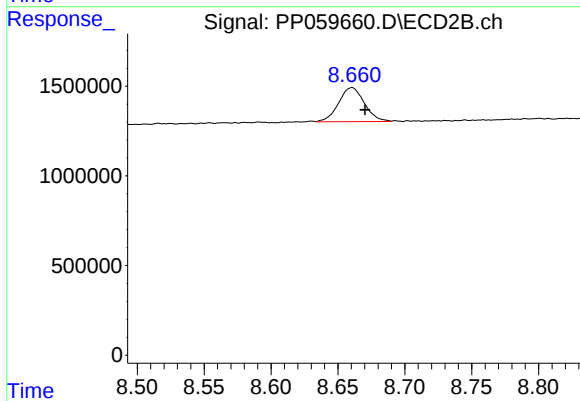

#2 Decachlorobiphenyl

R.T.: 8.661 min
Delta R.T.: -0.010 min
Response: 2562601
Conc: 1.86 ng/ml