

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083123\
 Data File : PP059662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2023 15:58
 Operator : YP\AJ
 Sample : 04246-03 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC280325LLZ-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/05/2023
 Supervised By :Ankita Jodhani 09/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:22:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 24 01:16:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.410	3.637	1773224	2982878	1.500	1.544
2) SA Decachlor...	10.195	8.660	1835348	2718969	2.347	1.970

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083123\
Data File : PP059662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2023 15:58
Operator : YP\AJ
Sample : 04246-03 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC280325LLZ-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/05/2023
Supervised By :Ankita Jodhani 09/05/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:22:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082323.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 24 01:16:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

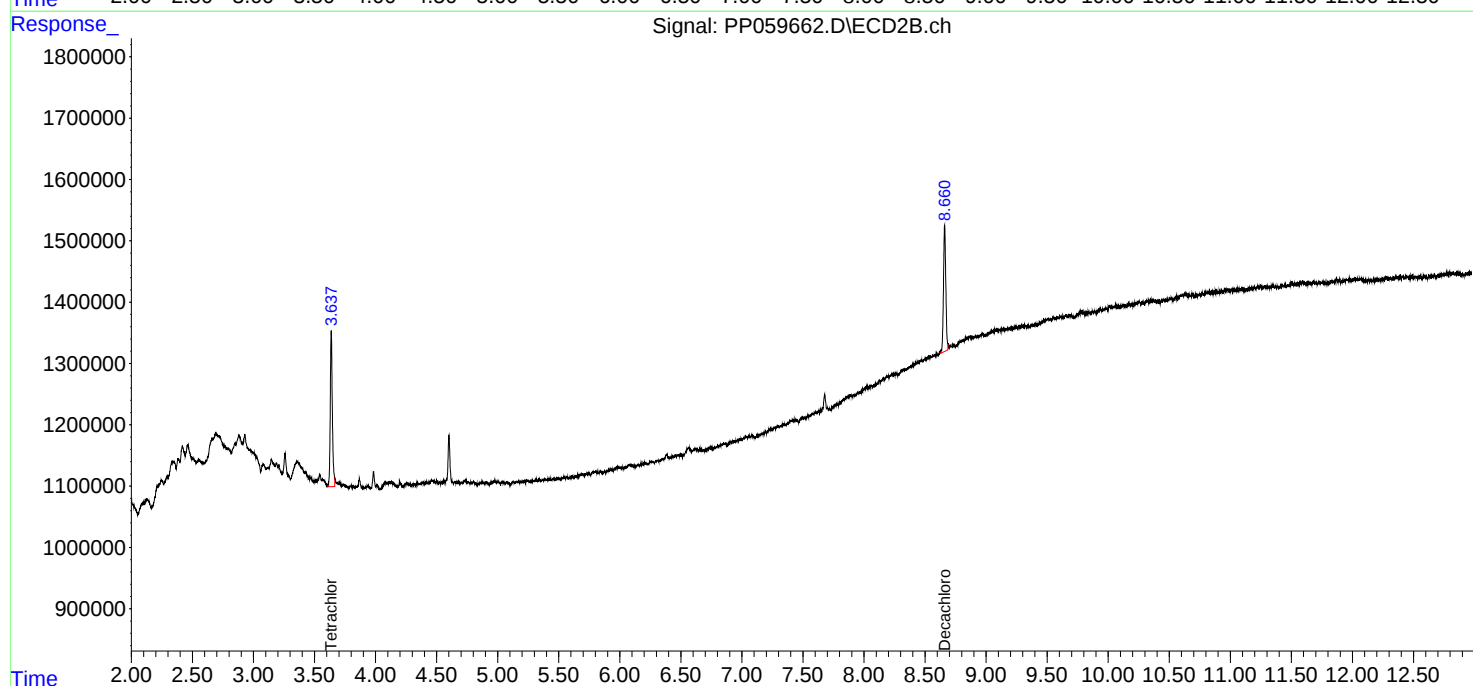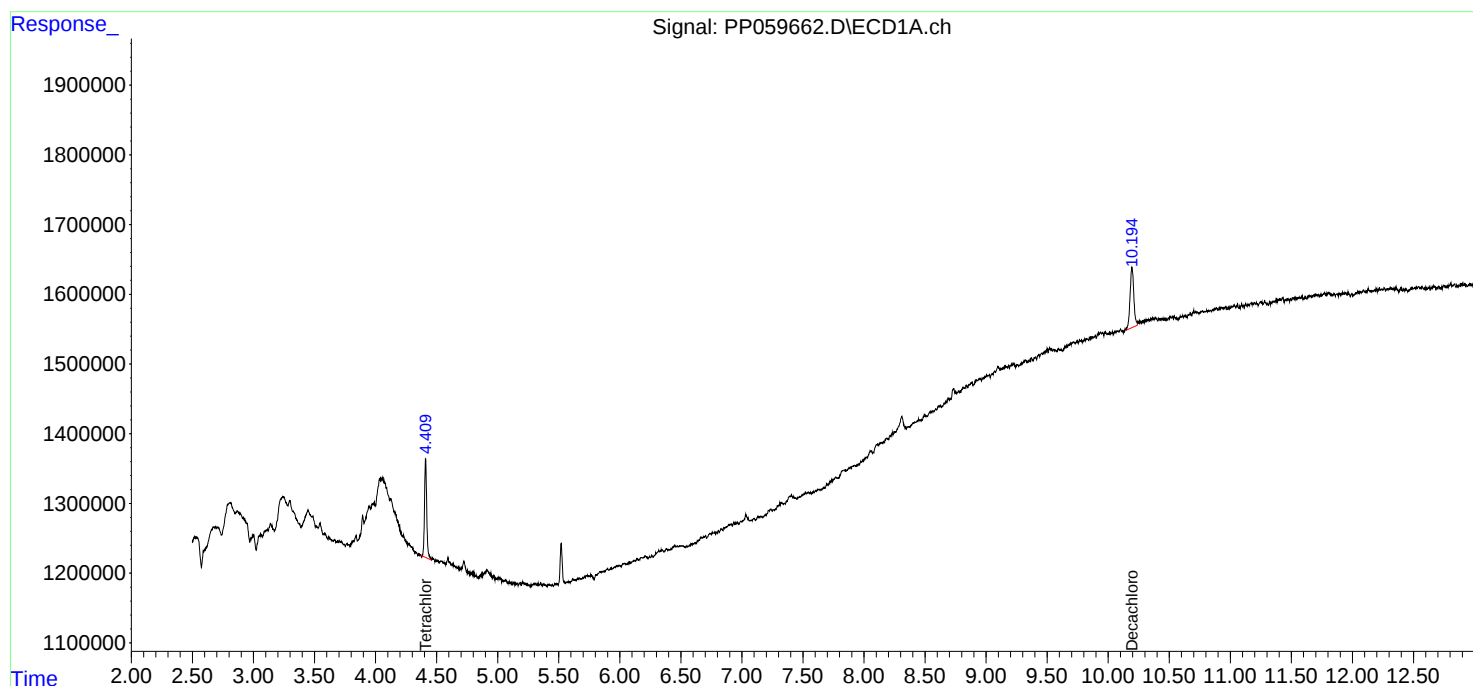

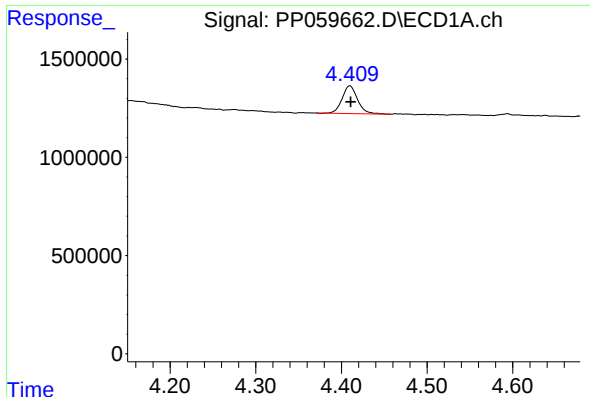


#1 Tetrachloro-m-xylene

R.T.: 4.410 min
Delta R.T.: 0.000 min
Response: 1773224
Conc: 1.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC280325LLZ-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/05/2023
Supervised By :Ankita Jodhani 09/05/2023

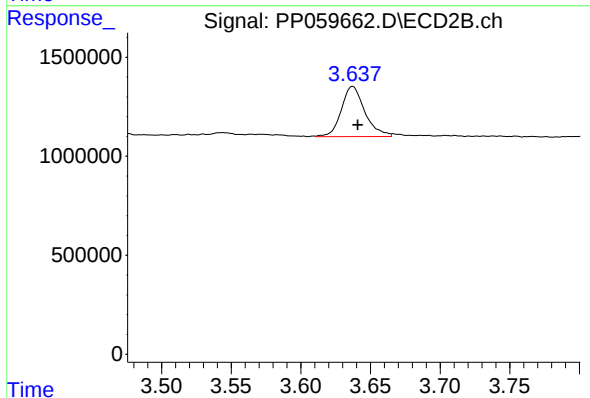


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.004 min
Response: 2982878
Conc: 1.54 ng/ml

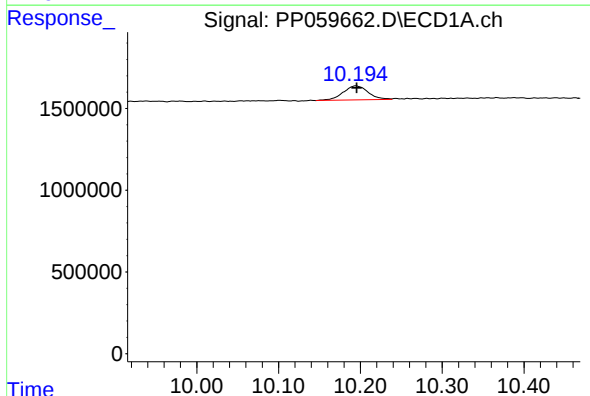

#2 Decachlorobiphenyl

R.T.: 10.195 min
Delta R.T.: 0.000 min
Response: 1835348
Conc: 2.35 ng/ml

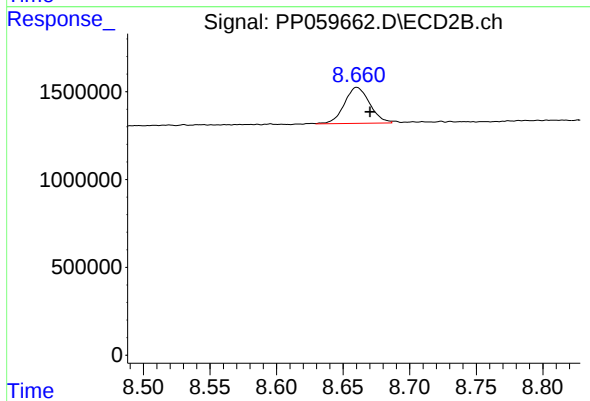

#2 Decachlorobiphenyl

R.T.: 8.660 min
Delta R.T.: -0.010 min
Response: 2718969
Conc: 1.97 ng/ml